Quantitative Analysis Results Summary Rep

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PENTA(LG NJ 3.26)\QuantResults\PENTA.batch.bin				
Analysis Time	2026-03-30 오후 3:37:36	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-30 오후 3:37:36	**Analyze Quant Version**	10.2	**Report Quant Version**	10.2

Pentachlorophenol

Data File	Type	RT	Resp.	ISTD Resp	Final Conc.
PENTA ST-01.D	Cal	8.523	1496	123821	0.0014
PENTA ST-02.D	Cal	8.523	3088	102747	0.0021
PENTA ST-03.D	Cal	8.523	5106	112152	0.0027
PENTA ST-04.D	Cal	8.523	7776	107855	0.0037
PENTA ST-05.D	Cal	8.523	10965	110762	0.0048
PENTA ST-06.D	Cal	8.523	12207	94456	0.0059
PENTA ST-07.D	Cal	8.523	17486	90816	0.0084
BK-.D	Blank			93024	ND
FBK(LG NJ 26-03-26).D	Blank			86994	ND
LG NJ-01.D	Sample	8.523	0	176958	ND
LG NJ-02.D	Sample			137897	ND
LG NJ-03.D	Sample			148553	ND
LG NJ-04.D	Sample			161491	ND
LG NJ-05.D	Sample			194787	ND
LG NJ-06.D	Sample			157770	ND
MBK.D	Blank			180375	ND
CCV-.D	QC	8.523	10838	189359	0.0032

Pentachlorophenol

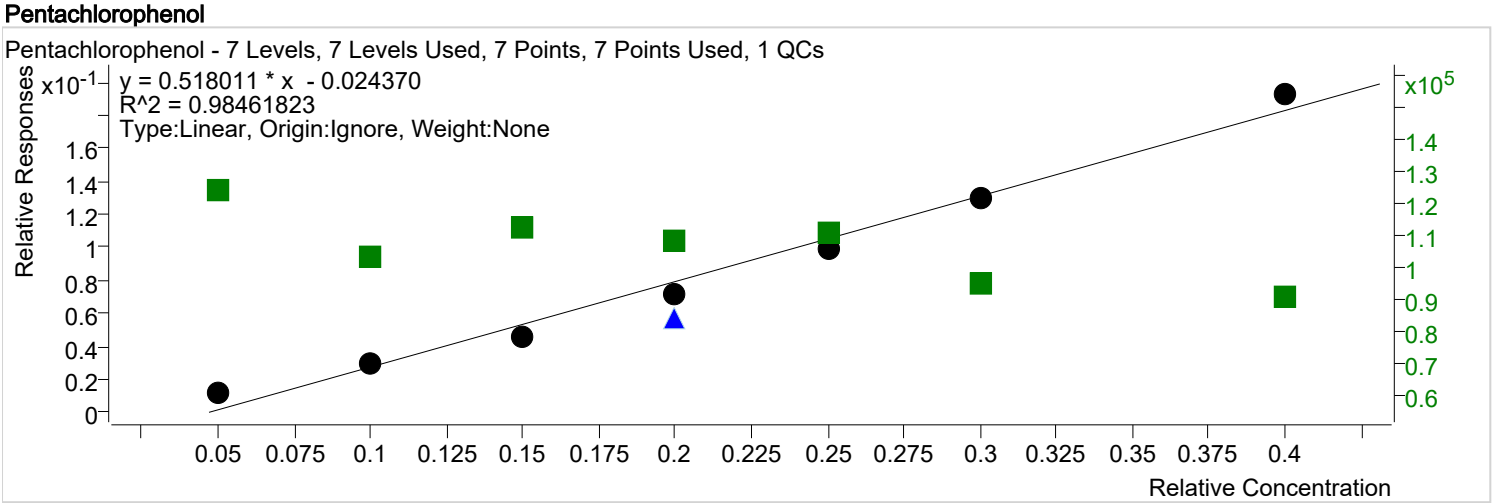

Cal. Path	Type	Level	Enable	Conc.	Response
\\192.168.254.121\data\2026\3. 2026-03\PENTA(LG NJ 3.26)\PENTA ST-01.D	Calibration	1	x	0.500	1496
\\192.168.254.121\data\2026\3. 2026-03\PENTA(LG NJ 3.26)\PENTA ST-02.D	Calibration	2	x	1.000	3088
\\192.168.254.121\data\2026\3. 2026-03\PENTA(LG NJ 3.26)\PENTA ST-03.D	Calibration	3	x	1.500	5106
\\192.168.254.121\data\2026\3. 2026-03\PENTA(LG NJ 3.26)\PENTA ST-04.D	Calibration	4	x	2.000	7776
\\192.168.254.121\data\2026\3. 2026-03\PENTA(LG NJ 3.26)\CCV-.D	QC	4	x	2.000	10838
\\192.168.254.121\data\2026\3. 2026-03\PENTA(LG NJ 3.26)\PENTA ST-05.D	Calibration	5	x	2.500	10965
\\192.168.254.121\data\2026\3. 2026-03\PENTA(LG NJ 3.26)\PENTA ST-06.D	Calibration	6	x	3.000	12207
\\192.168.254.121\data\2026\3. 2026-03\PENTA(LG NJ 3.26)\PENTA ST-07.D	Calibration	7	x	4.000	17486

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PENTA(LG NJ 3.26)\QuantResults\PENTA.batch.bin		
Analysis Time	2026-03-30 오후 3:37:36	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:43:03	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-30 오후 3:37:36	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-30 오전 10:56:45	**Data File**	PENTA ST-01.D
Type	Cal	**Name**	PENTA ST-01
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

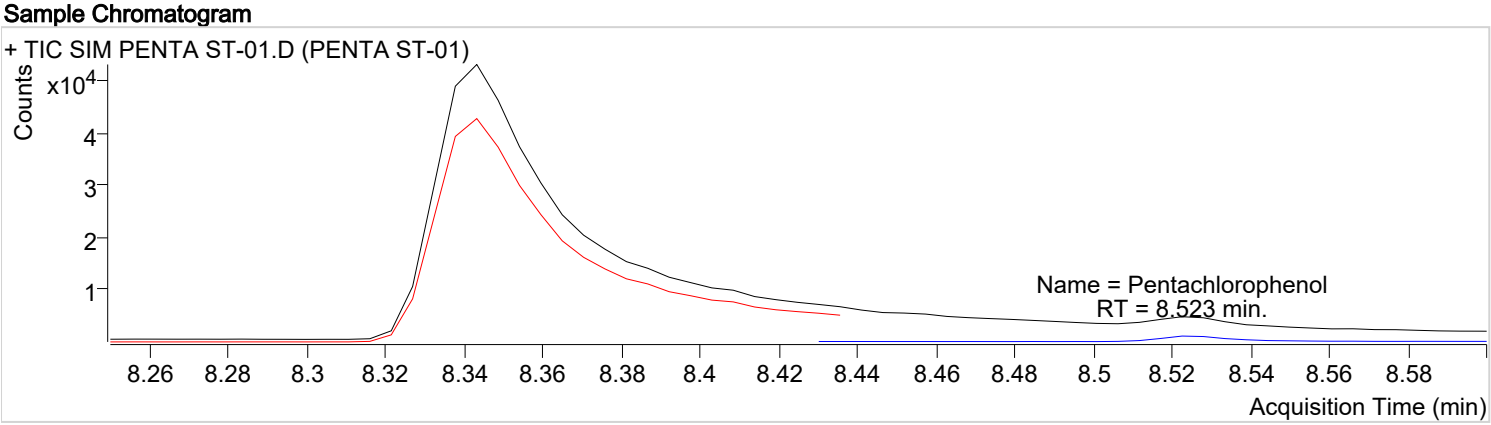

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol	8.523	1496	123821	0.0014 mg/L

Pentachlorophenol





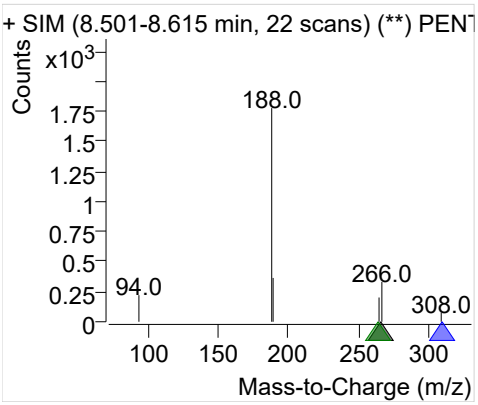

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PENTA(LG NJ 3.26)\QuantResults\PENTA.batch.bin		
Analysis Time	2026-03-30 오후 3:37:36	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:43:03	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-30 오후 3:37:36	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-30 오전 11:10:08	**Data File**	PENTA ST-02.D
Type	Cal	**Name**	PENTA ST-02
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

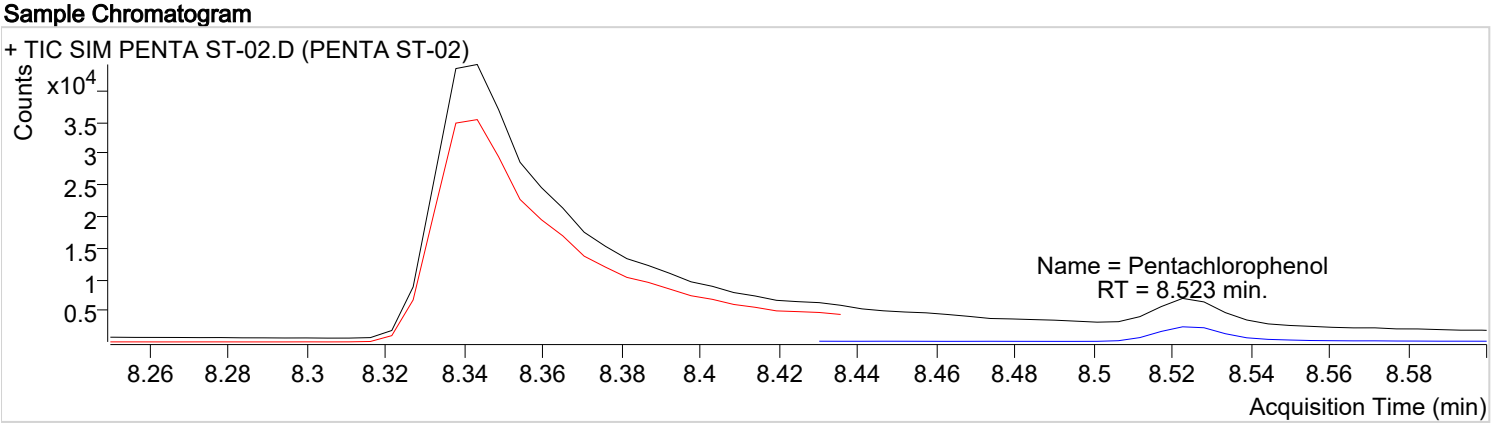

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol	8.523	3088	102747	0.0021 mg/L

Pentachlorophenol





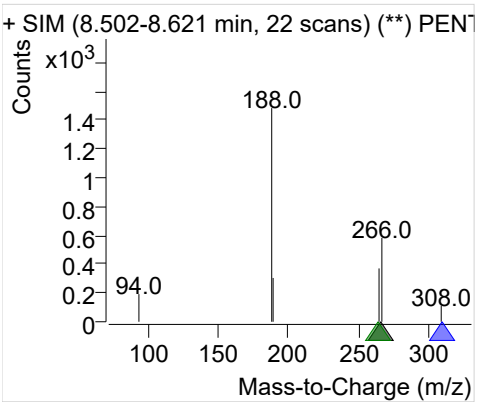

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PENTA(LG NJ 3.26)\QuantResults\PENTA.batch.bin		
Analysis Time	2026-03-30 오후 3:37:36	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:43:03	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-30 오후 3:37:36	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-30 오전 11:23:32	**Data File**	PENTA ST-03.D
Type	Cal	**Name**	PENTA ST-03
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

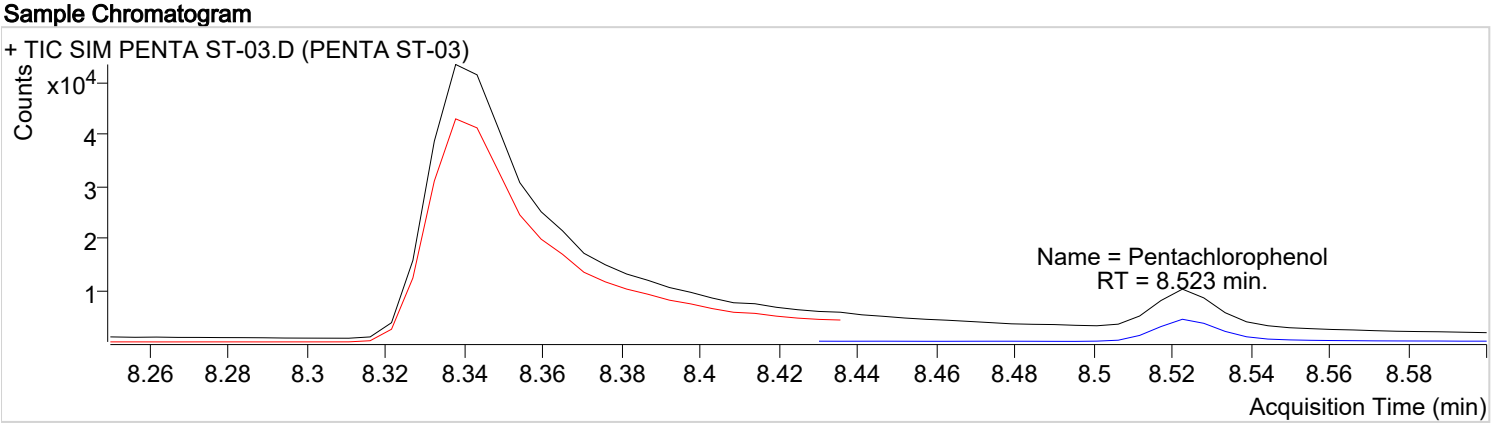

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol	8.523	5106	112152	0.0027 mg/L

Pentachlorophenol





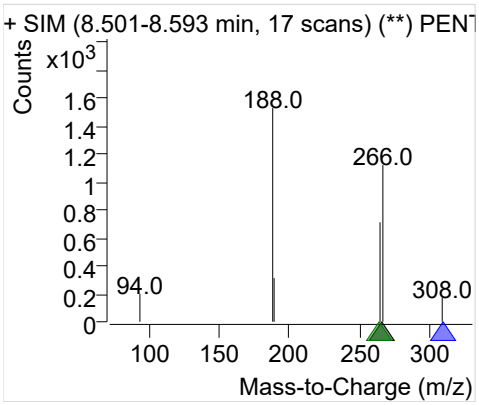

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PENTA(LG NJ 3.26)\QuantResults\PENTA.batch.bin		
Analysis Time	2026-03-30 오후 3:37:36	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:43:03	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-30 오후 3:37:36	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-30 오전 11:36:54	**Data File**	PENTA ST-04.D
Type	Cal	**Name**	PENTA ST-04
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

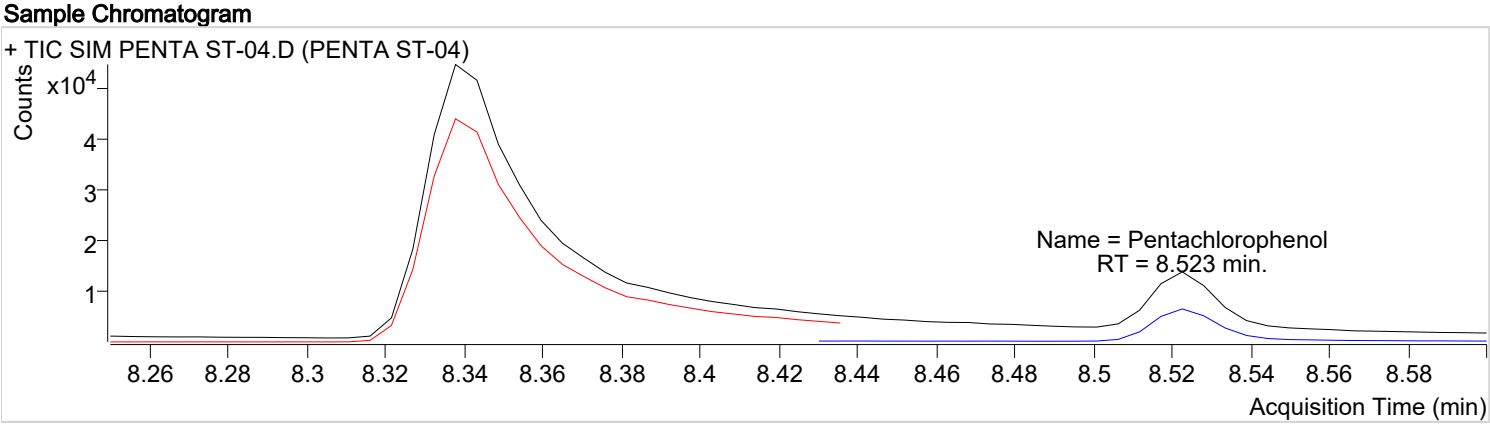

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol	8.523	7776	107855	0.0037 mg/L

Pentachlorophenol

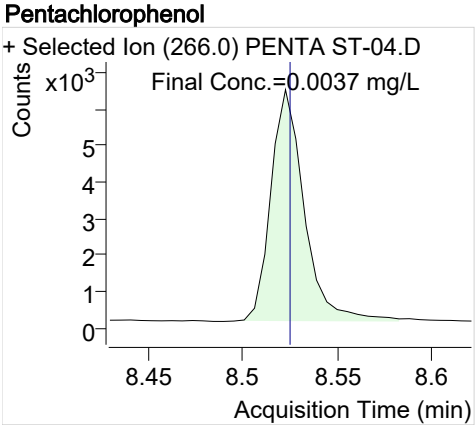



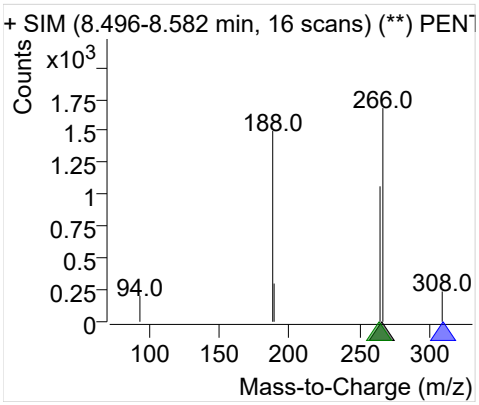

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PENTA(LG NJ 3.26)\QuantResults\PENTA.batch.bin		
Analysis Time	2026-03-30 오후 3:37:36	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:43:03	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-30 오후 3:37:36	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-30 오전 11:50:17	**Data File**	PENTA ST-05.D
Type	Cal	**Name**	PENTA ST-05
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

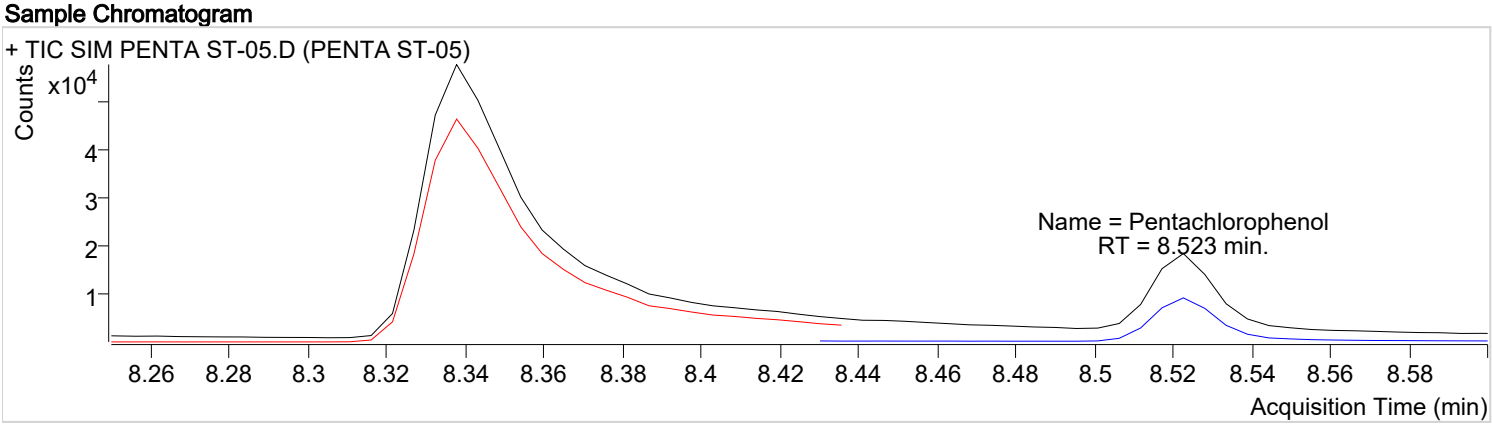

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol	8.523	10965	110762	0.0048 mg/L

Pentachlorophenol





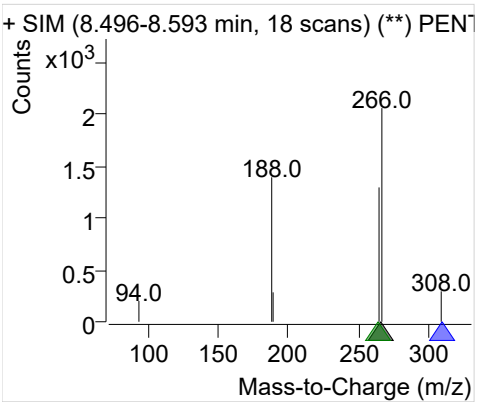

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PENTA(LG NJ 3.26)\QuantResults\PENTA.batch.bin		
Analysis Time	2026-03-30 오후 3:37:36	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:43:03	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-30 오후 3:37:36	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-30 오후 12:03:40	**Data File**	PENTA ST-06.D
Type	Cal	**Name**	PENTA ST-06
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

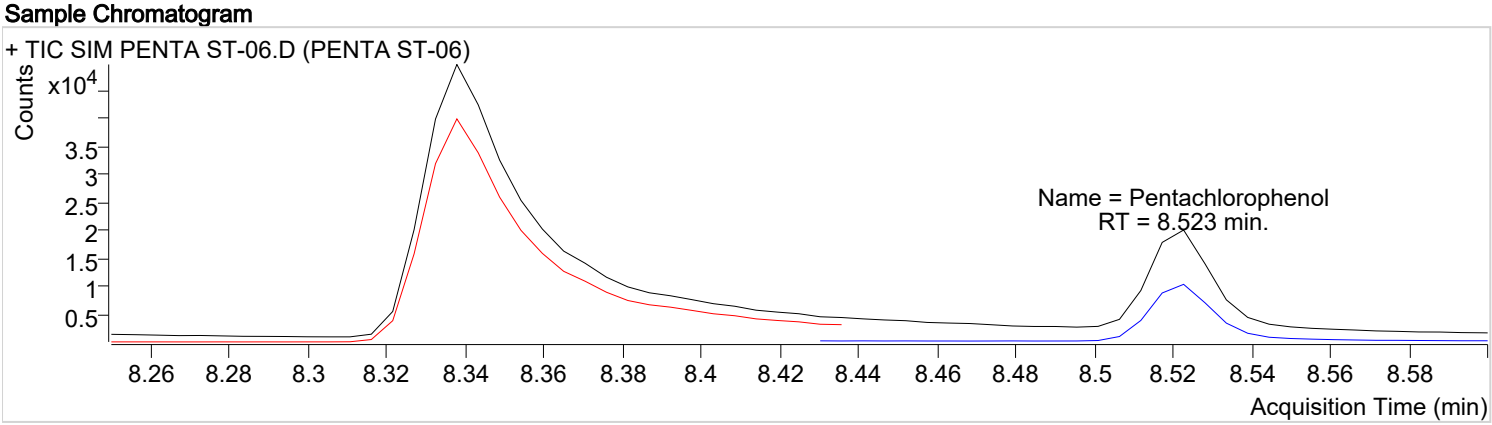

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol	8.523	12207	94456	0.0059 mg/L

Pentachlorophenol





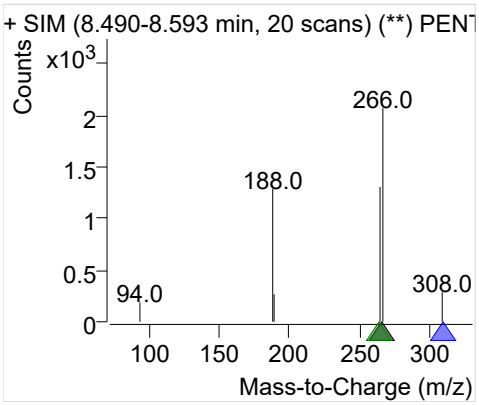

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PENTA(LG NJ 3.26)\QuantResults\PENTA.batch.bin		
Analysis Time	2026-03-30 오후 3:37:36	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:43:03	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-30 오후 3:37:36	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-30 오후 12:17:04	**Data File**	PENTA ST-07.D
Type	Cal	**Name**	PENTA ST-07
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

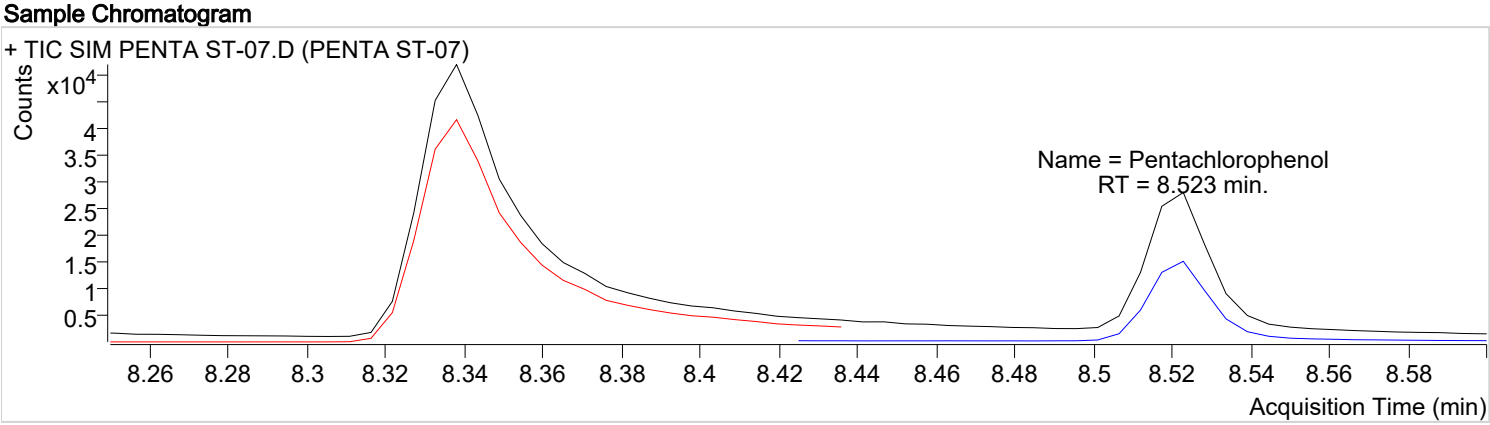

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol	8.523	17486	90816	0.0084 mg/L

Pentachlorophenol





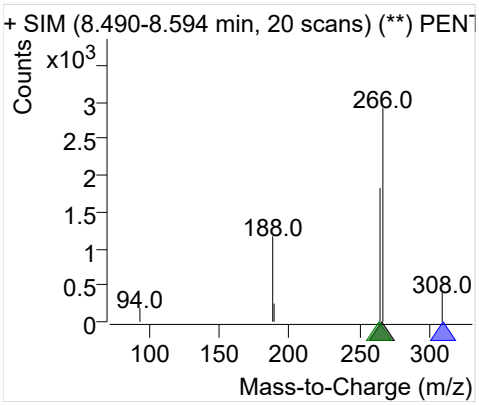

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PENTA(LG NJ 3.26)\QuantResults\PENTA.batch.bin		
Analysis Time	2026-03-30 오후 3:37:36	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:43:03	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-30 오후 3:37:36	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-30 오후 12:43:51	**Data File**	BK-.D
Type	Blank	**Name**	BK-
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

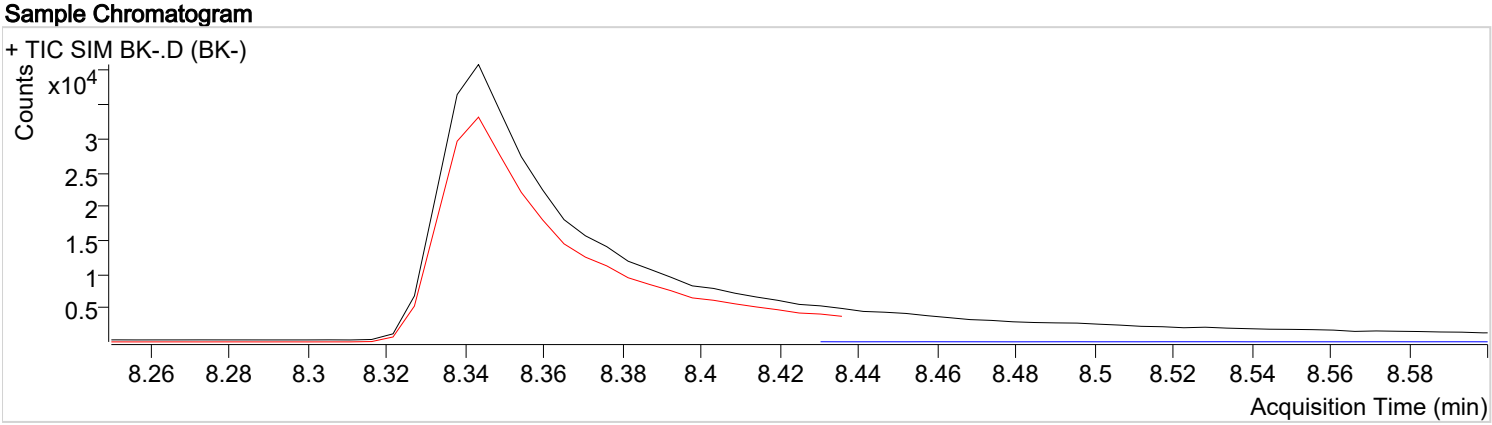

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol			93024	ND mg/L

Pentachlorophenol





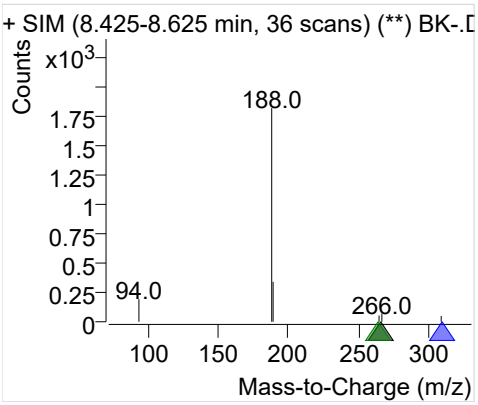

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PENTA(LG NJ 3.26)\QuantResults\PENTA.batch.bin		
Analysis Time	2026-03-30 오후 3:37:36	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:43:03	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-30 오후 3:37:36	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-30 오후 12:57:16	**Data File**	FBK(LG NJ 26-03-26).D
Type	Blank	**Name**	FBK(LG NJ 26-03-26)
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

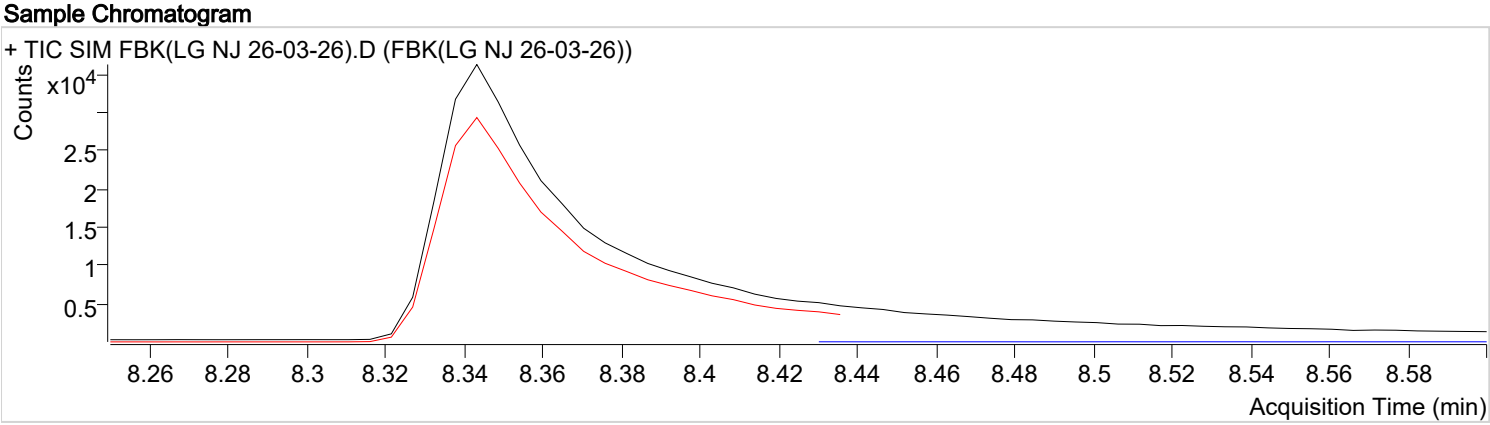

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol			86994	ND mg/L

Pentachlorophenol

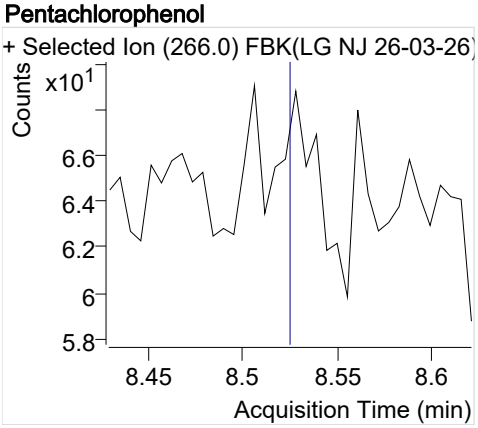

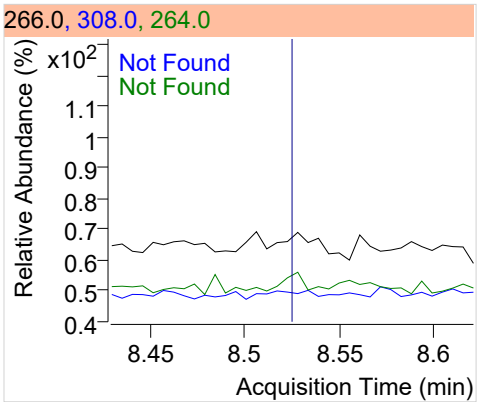

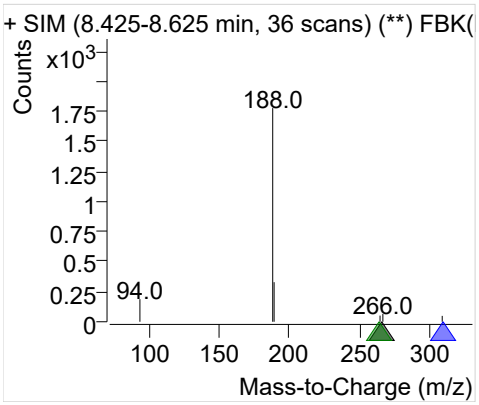

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PENTA(LG NJ 3.26)\QuantResults\PENTA.batch.bin		
Analysis Time	2026-03-30 오후 3:37:36	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:43:03	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-30 오후 3:37:36	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-30 오후 1:10:40	**Data File**	LG NJ-01.D
Type	Sample	**Name**	LG NJ-01
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

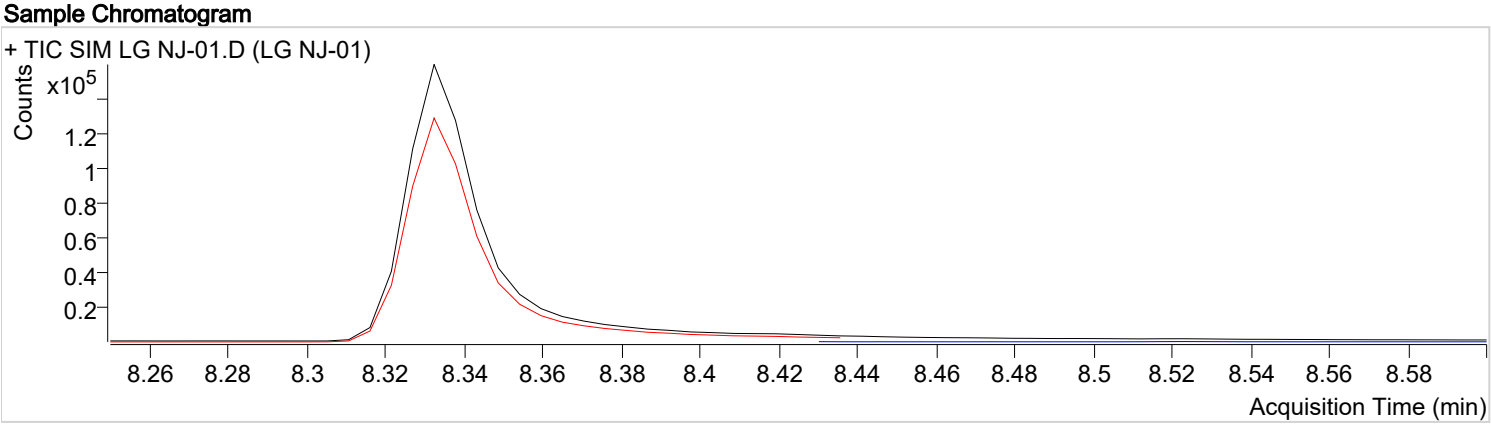

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol	8.523	0	176958	ND mg/L

Pentachlorophenol





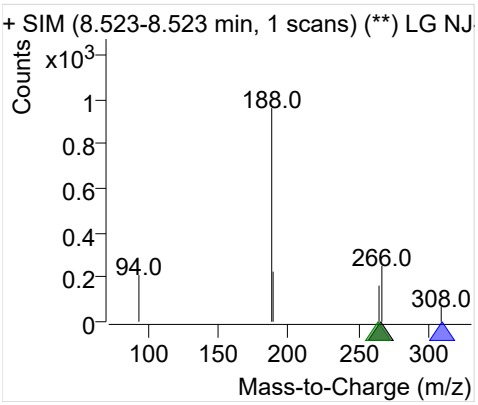

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PENTA(LG NJ 3.26)\QuantResults\PENTA.batch.bin		
Analysis Time	2026-03-30 오후 3:37:36	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:43:03	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-30 오후 3:37:36	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-30 오후 1:24:04	**Data File**	LG NJ-02.D
Type	Sample	**Name**	LG NJ-02
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

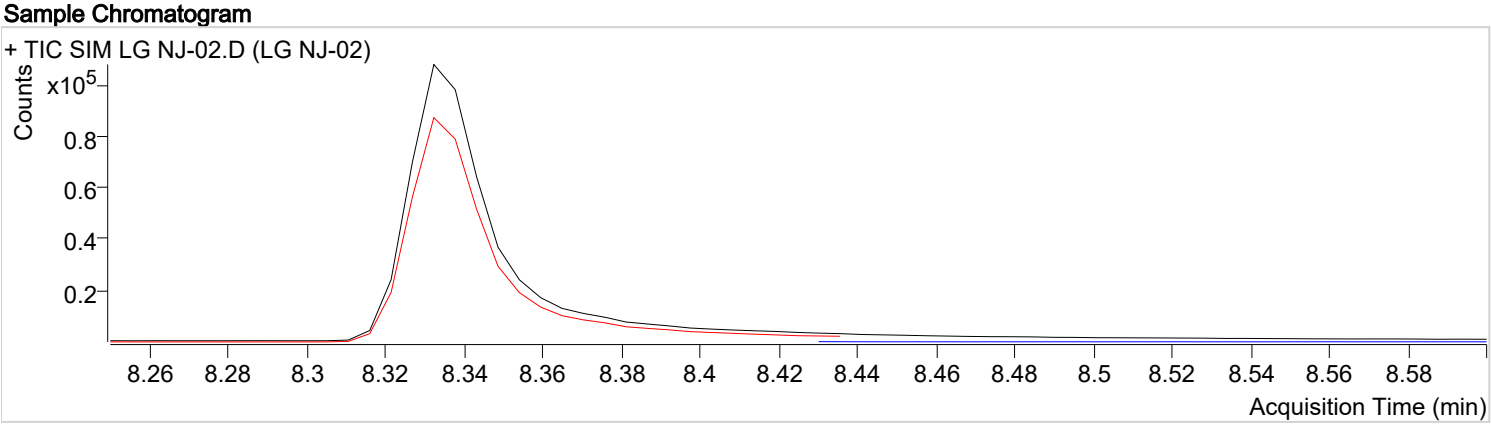

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol			137897	ND mg/L

Pentachlorophenol





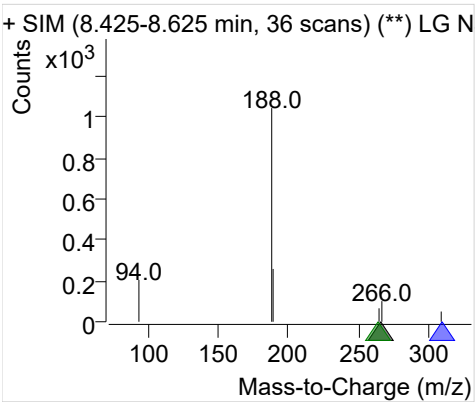

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PENTA(LG NJ 3.26)\QuantResults\PENTA.batch.bin		
Analysis Time	2026-03-30 오후 3:37:36	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:43:03	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-30 오후 3:37:36	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-30 오후 1:37:27	**Data File**	LG NJ-03.D
Type	Sample	**Name**	LG NJ-03
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

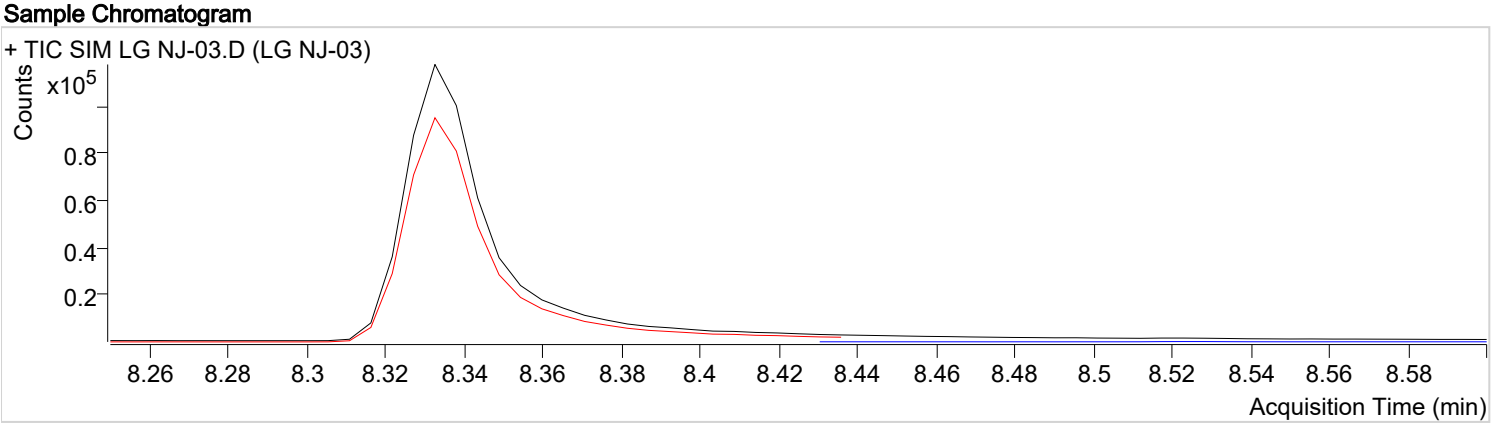

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol			148553	ND mg/L

Pentachlorophenol





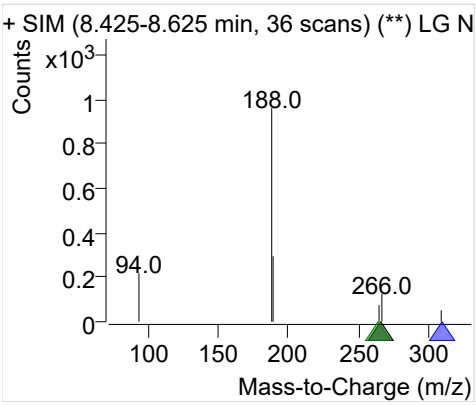

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PENTA(LG NJ 3.26)\QuantResults\PENTA.batch.bin		
Analysis Time	2026-03-30 오후 3:37:36	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:43:03	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-30 오후 3:37:36	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-30 오후 1:50:50	**Data File**	LG NJ-04.D
Type	Sample	**Name**	LG NJ-04
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

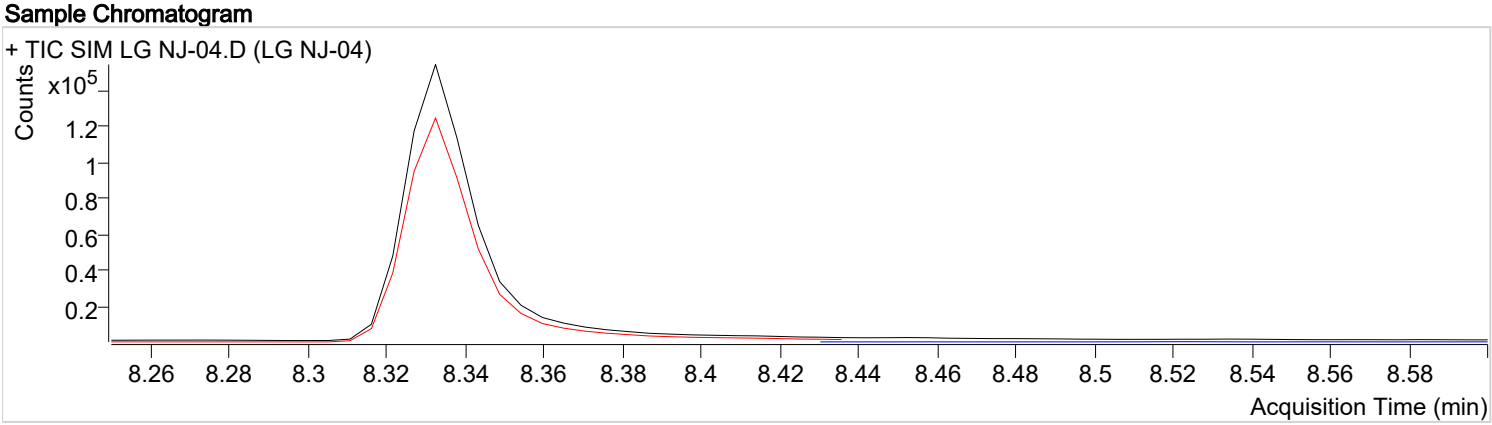

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol			161491	ND mg/L

Pentachlorophenol





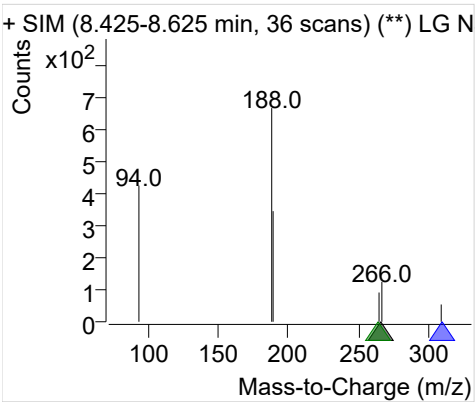

Quant Sample Report

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PENTA(LG NJ 3.26)\QuantResults\PENTA.batch.bin		
Analysis Time	2026-03-30 오후 3:37:36	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:43:03	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-30 오후 3:37:36	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-30 오후 2:04:16	**Data File**	LG NJ-05.D
Type	Sample	**Name**	LG NJ-05
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

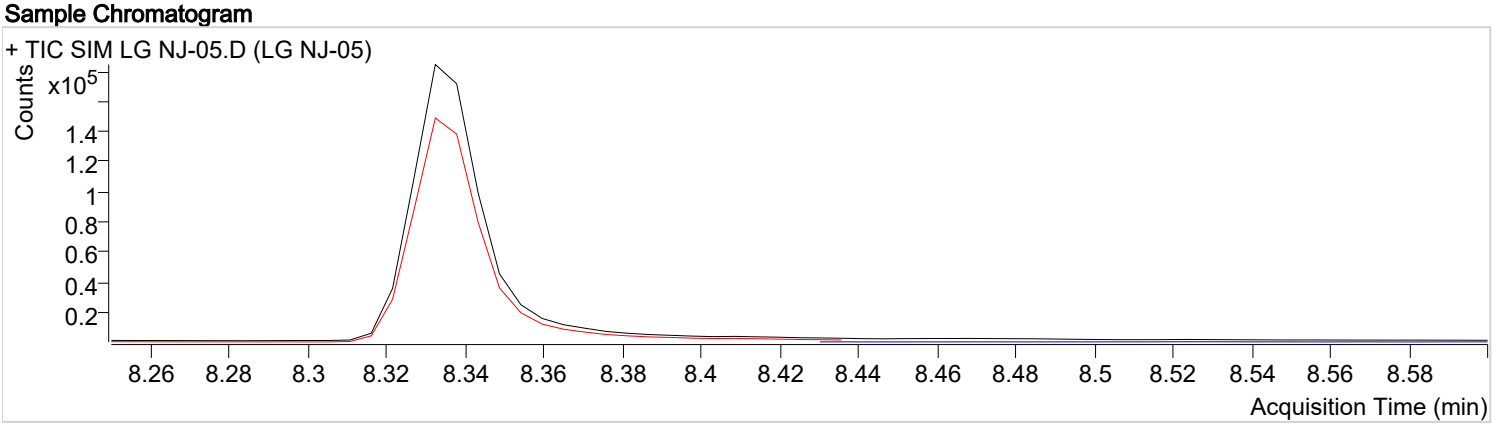

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol			194787	ND mg/L

Pentachlorophenol





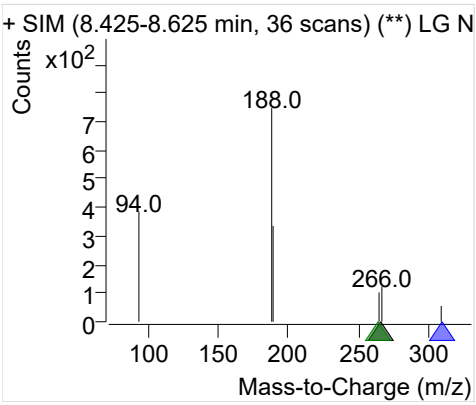

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PENTA(LG NJ 3.26)\QuantResults\PENTA.batch.bin		
Analysis Time	2026-03-30 오후 3:37:36	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:43:03	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-30 오후 3:37:36	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-30 오후 2:17:39	**Data File**	LG NJ-06.D
Type	Sample	**Name**	LG NJ-06
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

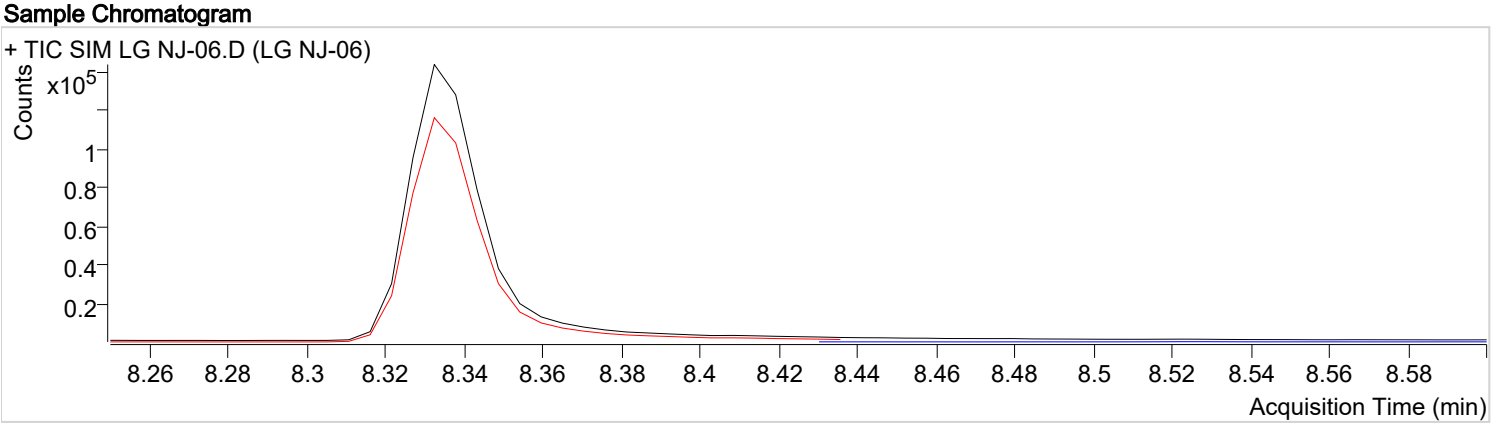

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol			157770	ND mg/L

Pentachlorophenol



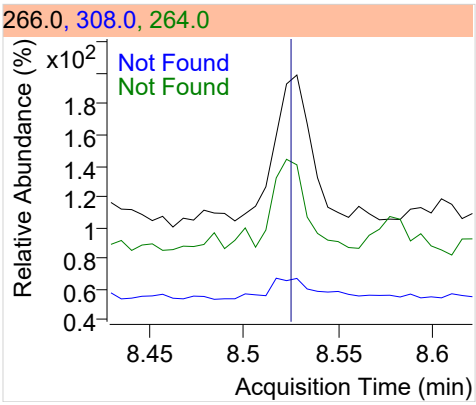

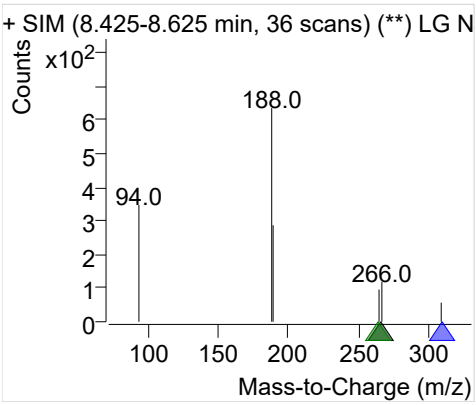

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PENTA(LG NJ 3.26)\QuantResults\PENTA.batch.bin		
Analysis Time	2026-03-30 오후 3:37:36	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:43:03	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-30 오후 3:37:36	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-30 오후 2:31:03	**Data File**	MBK.D
Type	Blank	**Name**	MBK
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

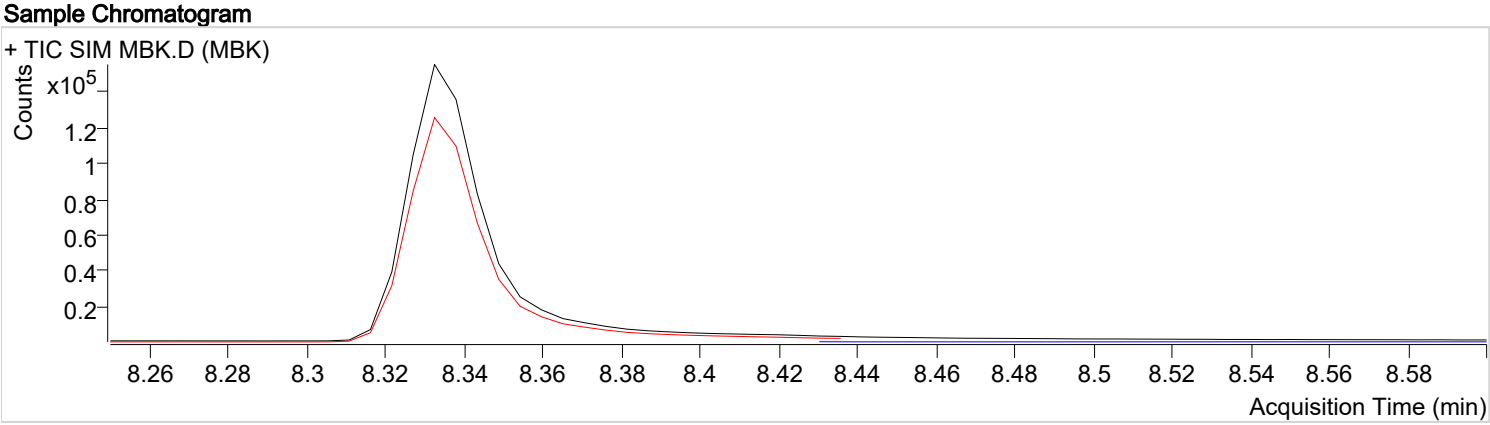

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol			180375	ND mg/L

Pentachlorophenol

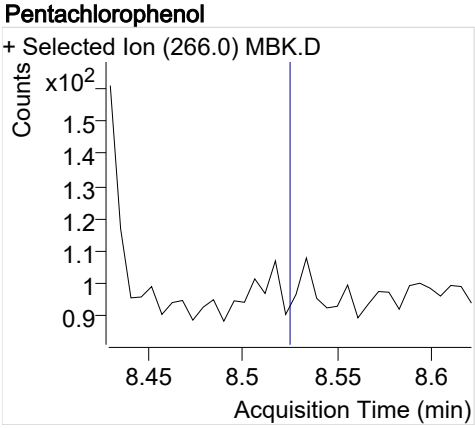

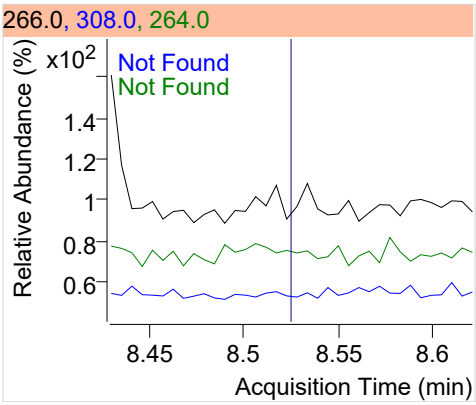

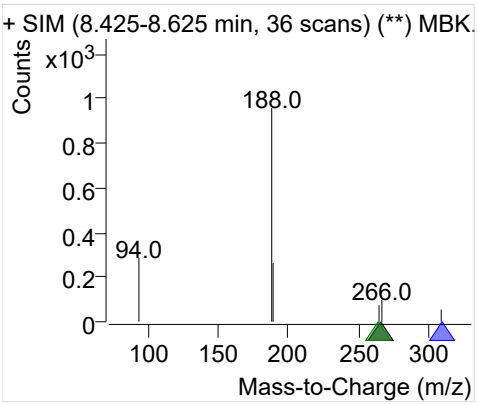

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	\\192.168.254.121\data\2026\3. 2026-03\PENTA(LG NJ 3.26)\QuantResults\PENTA.batch.bin		
Analysis Time	2026-03-30 오후 3:37:36	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:43:03	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-30 오후 3:37:36	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-30 오후 2:44:26	**Data File**	CCV-.D
Type	QC	**Name**	CCV-
Dil.	0.002	**Acq. Method File**	VOCS(Pentacl-Phenol)

Sample Chromatogram

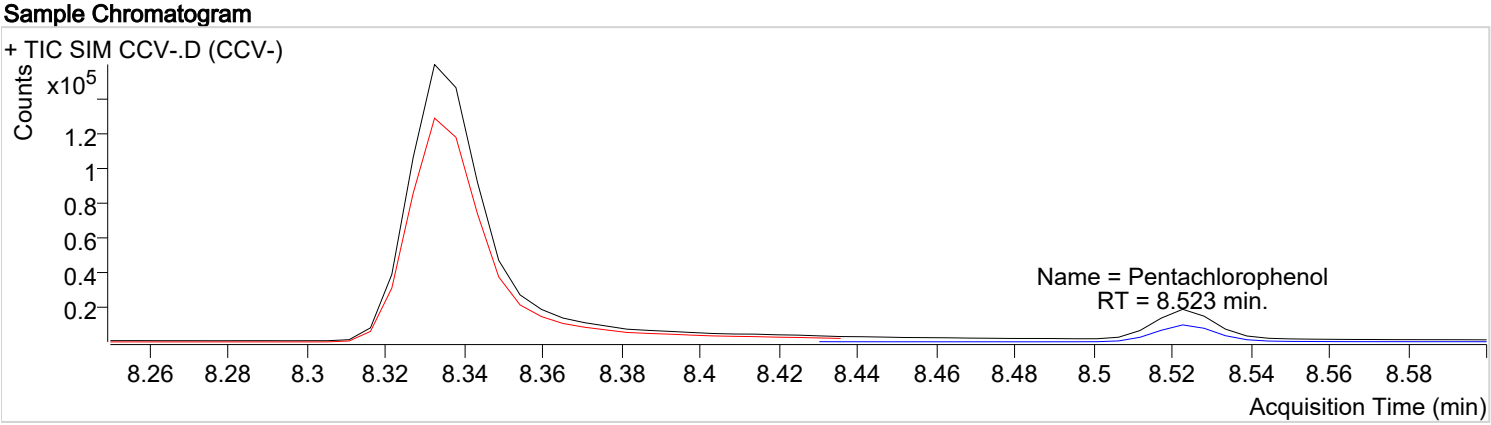

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol	8.523	10838	189359	0.0032 mg/L
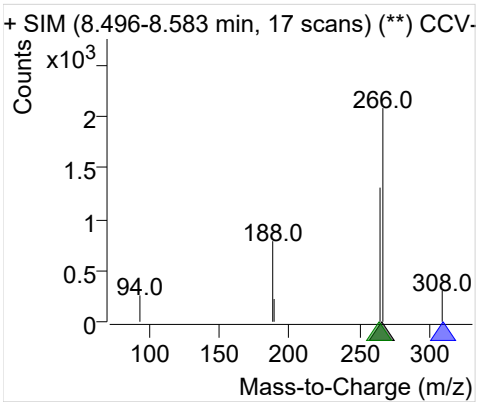
Pentachlorophenol