Quantitative Analysis Results Summary Rep

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-02\PENTA(GS 2.10 KH 2.10)\QuantResults\PHENTA.batch.bin				
Analysis Time	2026-02-19 오후 5:32:08	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-19 오후 5:32:08	**Analyze Quant Version**	10.2	**Report Quant Version**	10.2

Pentachlorophenol

Data File	Type	RT	Resp.	ISTD Resp	Final Conc.
PENTA ST-01.d	Cal	4.391	3870	114798	0.0014
PENTA ST-02.d	Cal	4.386	8987	100093	0.0021
PENTA ST-03.d	Cal	4.386	15662	110258	0.0027
PENTA ST-04.d	Cal	4.386	26321	112996	0.0038
PENTA ST-05.d	Cal	4.391	35415	113747	0.0047
PENTA ST-06.d	Cal	4.386	44778	107266	0.0060
PENTA ST-07.d	Cal	4.386	73121	119689	0.0083
BK-.d	Sample			97936	ND
FBK(GS 26-02-10).d	Sample			108574	ND
KH 26-02-10.d	Sample			108763	ND
GS-01.d	Sample			108264	ND
GS-02.d	Sample			113890	ND
GS-03.d	Sample			122490	ND
GS-04.d	Sample			116053	ND
GS-05.d	Sample			114526	ND
GS-06.d	Sample			121436	ND
GS-11.d	Sample			118540	ND
MBK.d	Blank			129279	ND
-C-C-V-.d	QC	4.386	35933	146998	0.0039

Pentachlorophenol

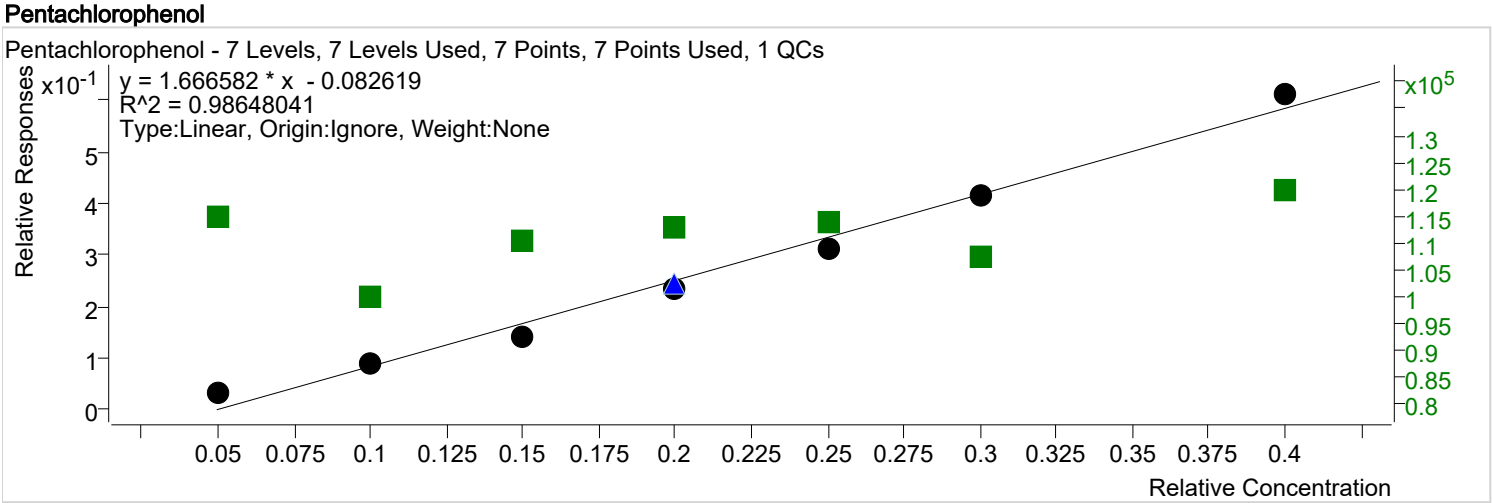

Cal. Path	Type	Level	Enable	Conc.	Response
V:\2026\2026-02\PENTA(GS 2.10 KH 2.10)\PENTA ST-01.d	Calibration	1	x	0.500	3870
V:\2026\2026-02\PENTA(GS 2.10 KH 2.10)\PENTA ST-02.d	Calibration	2	x	1.000	8987
V:\2026\2026-02\PENTA(GS 2.10 KH 2.10)\PENTA ST-03.d	Calibration	3	x	1.500	15662
V:\2026\2026-02\PENTA(GS 2.10 KH 2.10)\PENTA ST-04.d	Calibration	4	x	2.000	26321
V:\2026\2026-02\PENTA(GS 2.10 KH 2.10)\-C-C-V-.d	QC	4	x	2.000	35933
V:\2026\2026-02\PENTA(GS 2.10 KH 2.10)\PENTA ST-05.d	Calibration	5	x	2.500	35415
V:\2026\2026-02\PENTA(GS 2.10 KH 2.10)\PENTA ST-06.d	Calibration	6	x	3.000	44778
V:\2026\2026-02\PENTA(GS 2.10 KH 2.10)\PENTA ST-07.d	Calibration	7	x	4.000	73121

Quant Sample Report

Batch Data Path	V:\2026\2026-02\PENTA(GS 2.10 KH 2.10)\QuantResults\PHENTA.batch.bin		
Analysis Time	2026-02-19 오후 5:32:08	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:46:59	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-19 오후 5:32:08	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-19 오전 10:01:16	**Data File**	PENTA ST-01.d
Type	Cal	**Name**	PENTA ST-01
Dil.	0.002	**Acq. Method File**	VOCs(Penta-phenol)

Sample Chromatogram

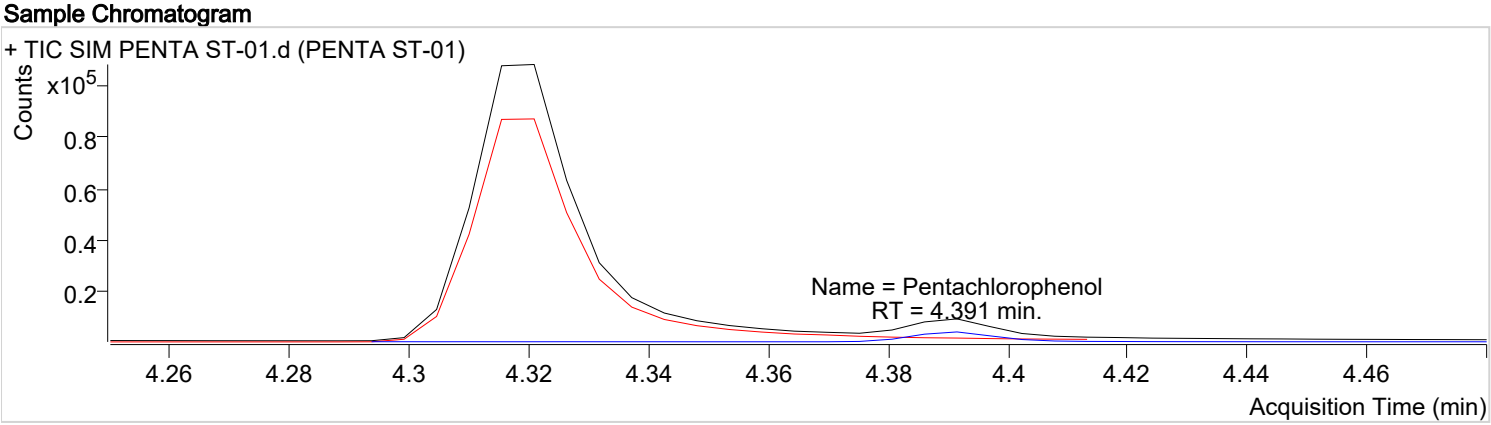

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol	4.391	3870	114798	0.0014 mg/L

Pentachlorophenol

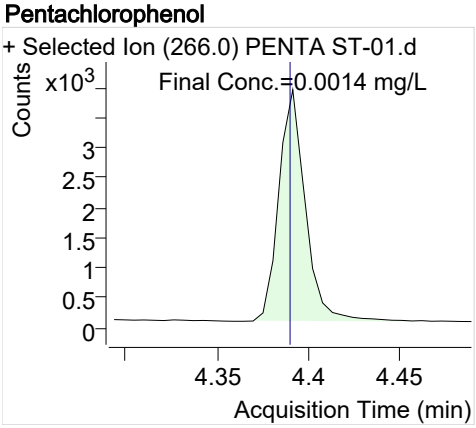



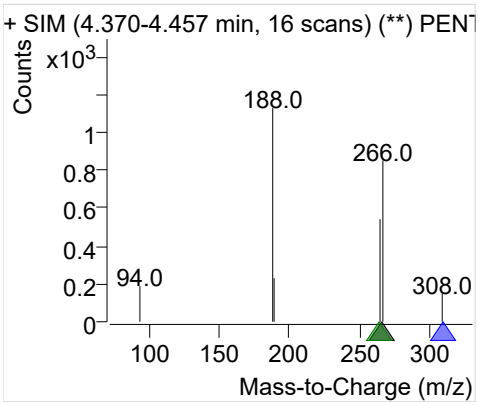

Quant Sample Report

Batch Data Path	V:\2026\2026-02\PENTA(GS 2.10 KH 2.10)\QuantResults\PHENTA.batch.bin		
Analysis Time	2026-02-19 오후 5:32:08	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:46:59	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-19 오후 5:32:08	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-19 오전 10:09:02	**Data File**	PENTA ST-02.d
Type	Cal	**Name**	PENTA ST-02
Dil.	0.002	**Acq. Method File**	VOCs(Penta-phenol)

Sample Chromatogram

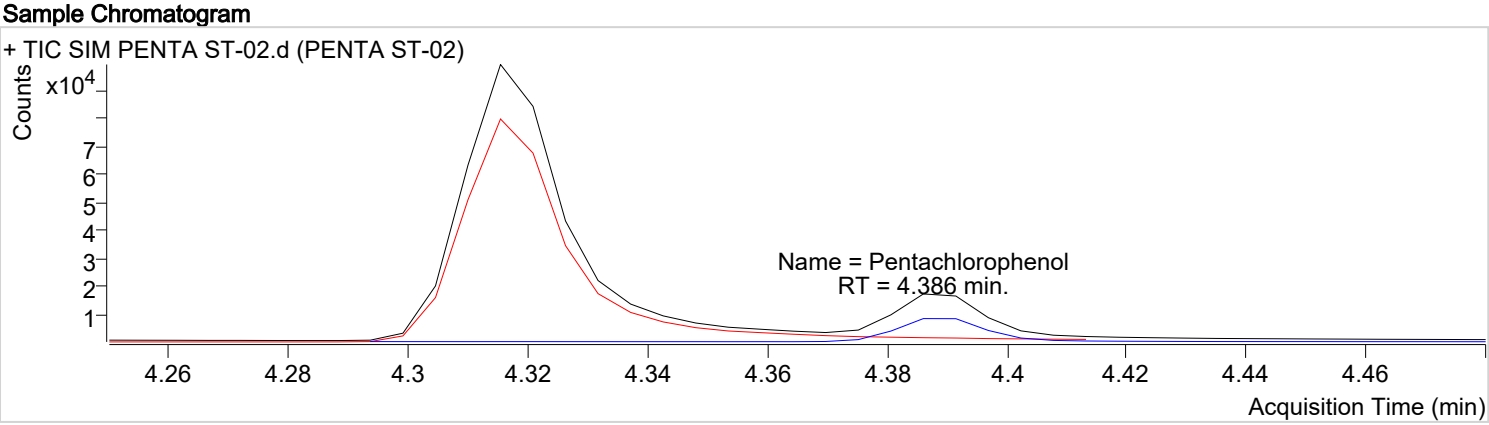

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol	4.386	8987	100093	0.0021 mg/L

Pentachlorophenol

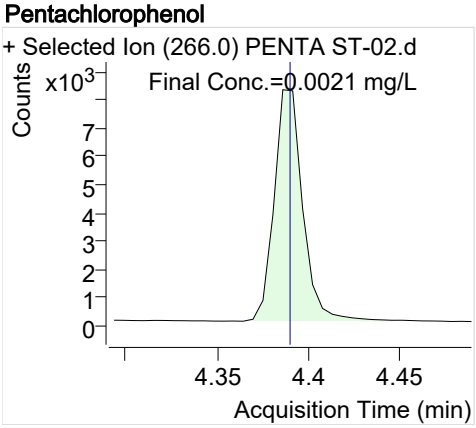



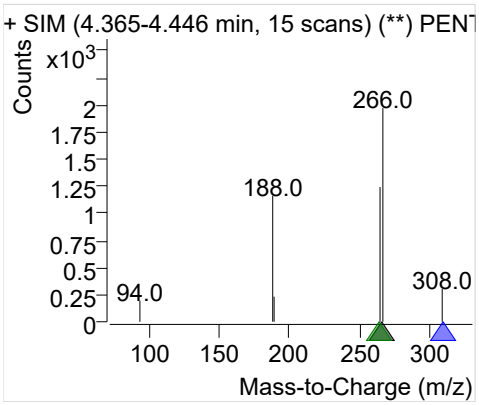

Quant Sample Report

Batch Data Path	V:\2026\2026-02\PENTA(GS 2.10 KH 2.10)\QuantResults\PHENTA.batch.bin		
Analysis Time	2026-02-19 오후 5:32:08	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:46:59	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-19 오후 5:32:08	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-19 오전 10:16:51	**Data File**	PENTA ST-03.d
Type	Cal	**Name**	PENTA ST-03
Dil.	0.002	**Acq. Method File**	VOCs(Penta-phenol)

Sample Chromatogram

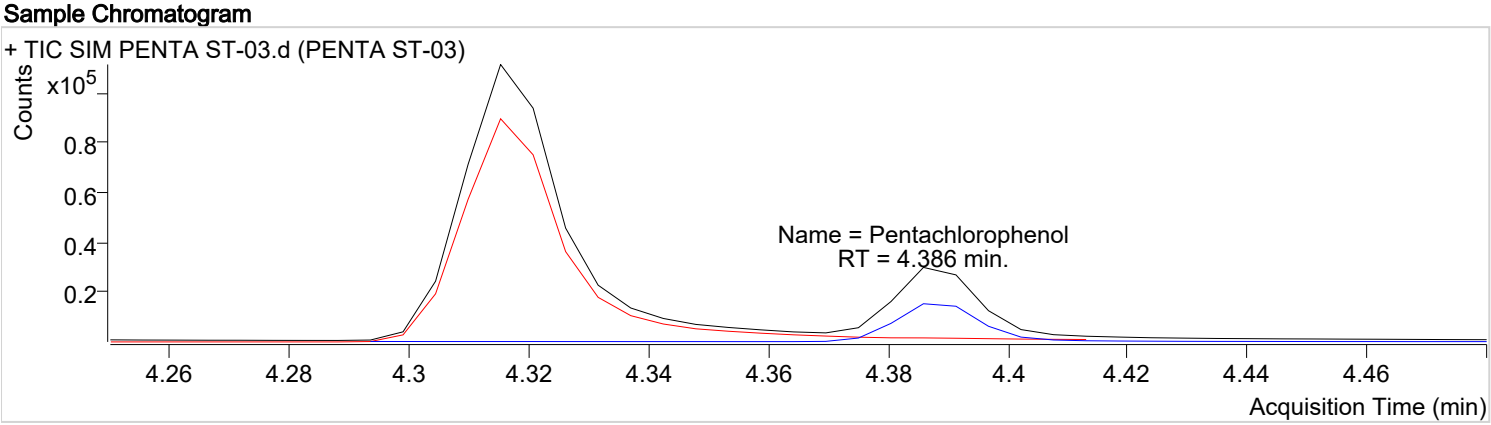

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol	4.386	15662	110258	0.0027 mg/L

Pentachlorophenol

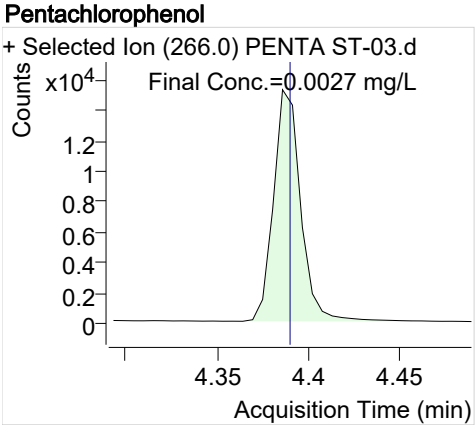



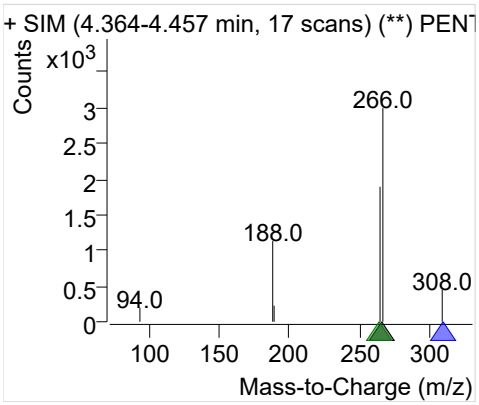

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-02\PENTA(GS 2.10 KH 2.10)\QuantResults\PHENTA.batch.bin		
Analysis Time	2026-02-19 오후 5:32:08	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:46:59	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-19 오후 5:32:08	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-19 오전 10:24:41	**Data File**	PENTA ST-04.d
Type	Cal	**Name**	PENTA ST-04
Dil.	0.002	**Acq. Method File**	VOCs(Penta-phenol)

Sample Chromatogram

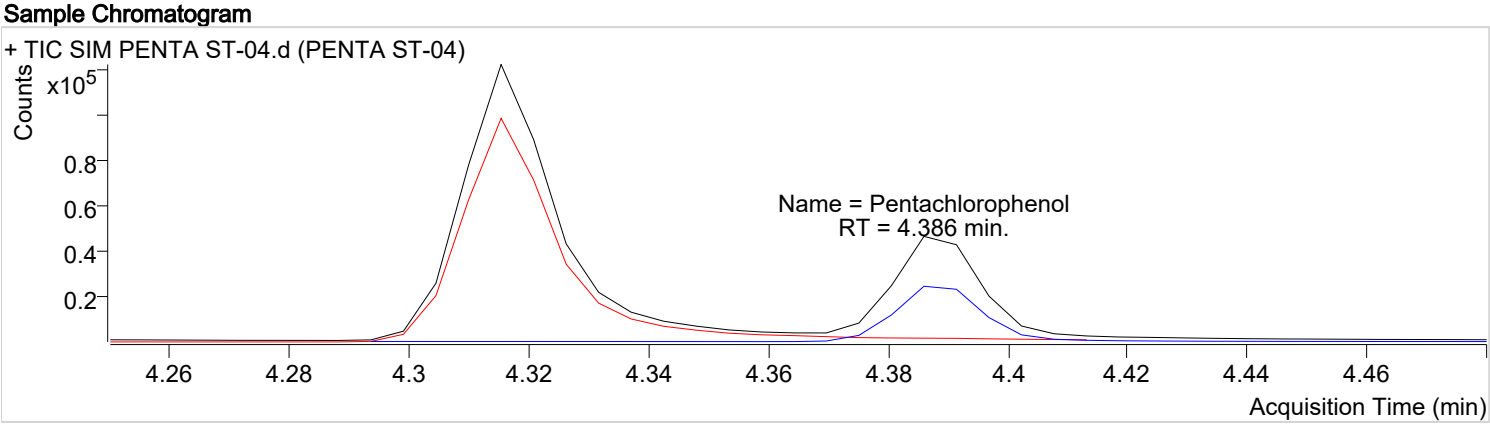

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol	4.386	26321	112996	0.0038 mg/L

Pentachlorophenol





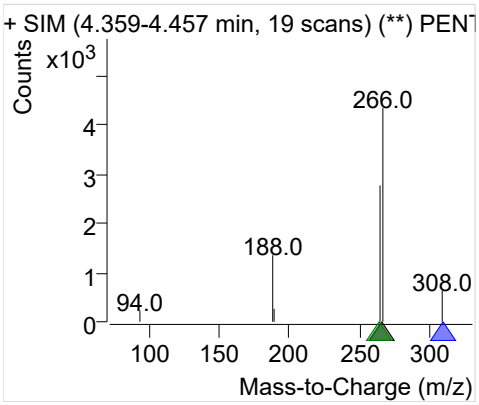

Quant Sample Report

Batch Data Path	V:\2026\2026-02\PENTA(GS 2.10 KH 2.10)\QuantResults\PHENTA.batch.bin		
Analysis Time	2026-02-19 오후 5:32:08	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:46:59	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-19 오후 5:32:08	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-19 오전 10:32:33	**Data File**	PENTA ST-05.d
Type	Cal	**Name**	PENTA ST-05
Dil.	0.002	**Acq. Method File**	VOCs(Penta-phenol)

Sample Chromatogram

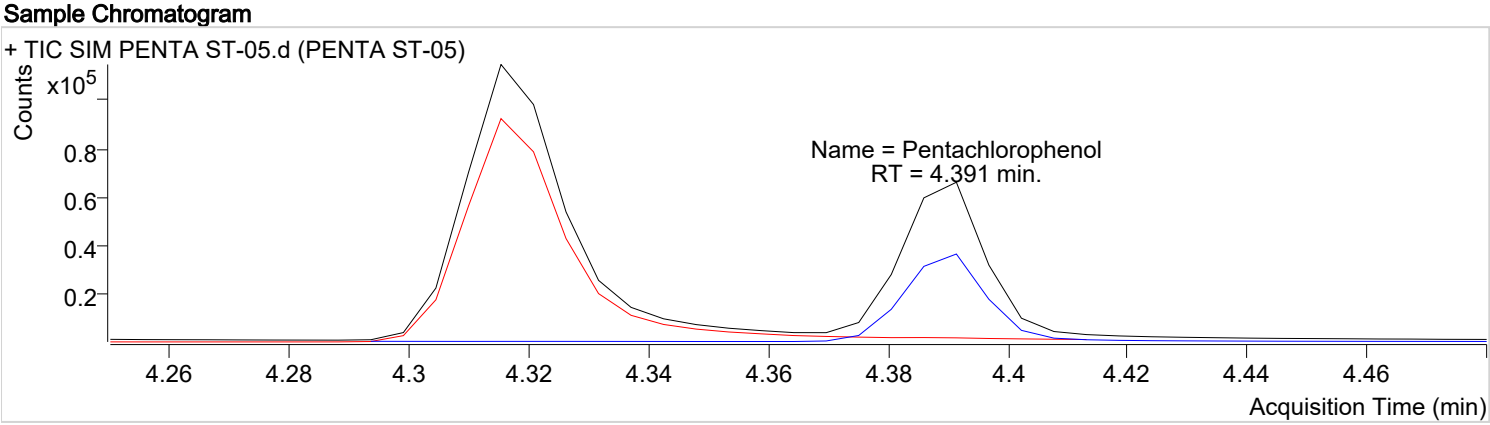

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol	4.391	35415	113747	0.0047 mg/L

Pentachlorophenol





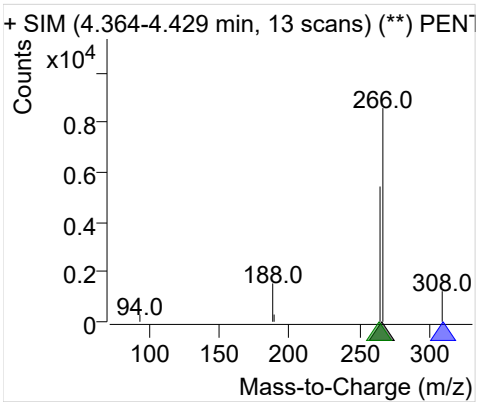

Quant Sample Report

Batch Data Path	V:\2026\2026-02\PENTA(GS 2.10 KH 2.10)\QuantResults\PHENTA.batch.bin		
Analysis Time	2026-02-19 오후 5:32:08	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:46:59	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-19 오후 5:32:08	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-19 오전 10:40:24	**Data File**	PENTA ST-06.d
Type	Cal	**Name**	PENTA ST-06
Dil.	0.002	**Acq. Method File**	VOCs(Penta-phenol)

Sample Chromatogram

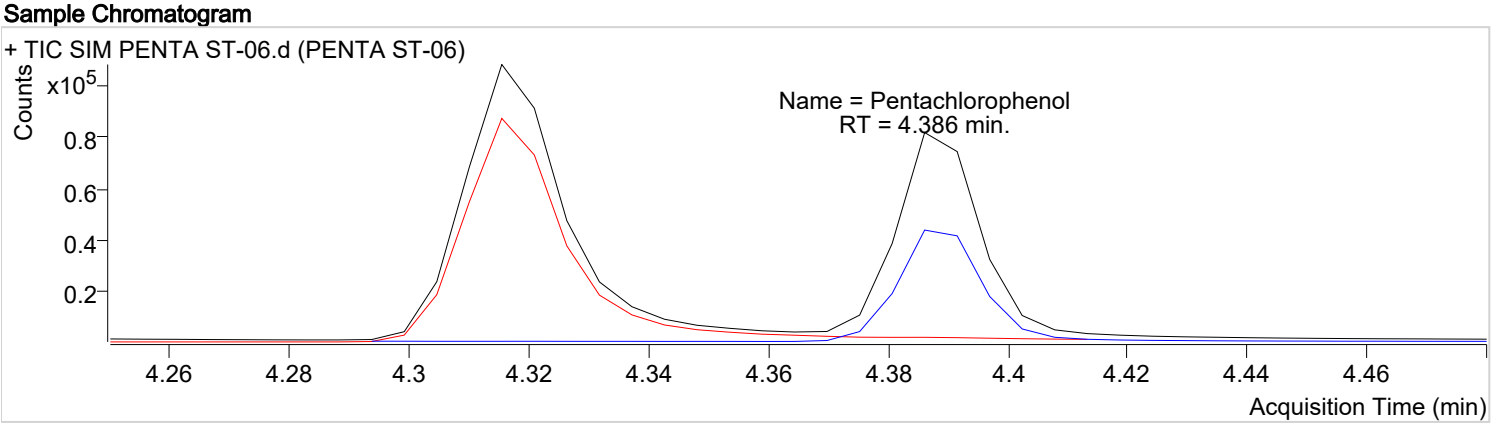

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol	4.386	44778	107266	0.0060 mg/L

Pentachlorophenol

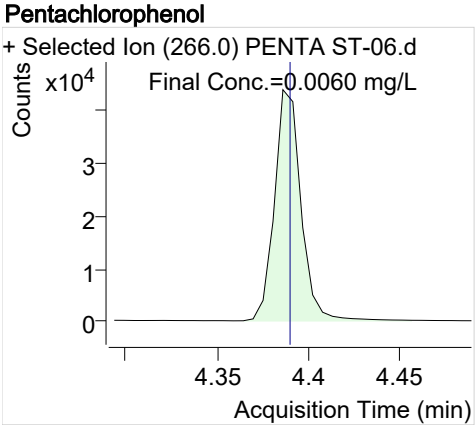



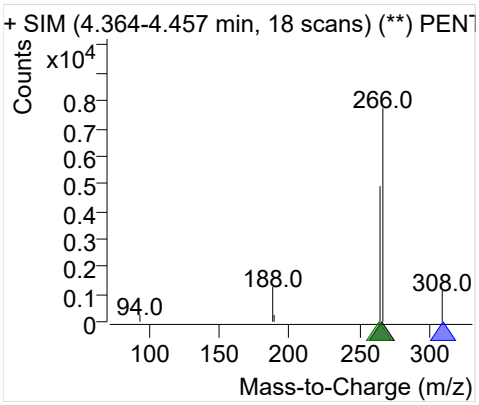

Quant Sample Report

Batch Data Path	V:\2026\2026-02\PENTA(GS 2.10 KH 2.10)\QuantResults\PHENTA.batch.bin		
Analysis Time	2026-02-19 오후 5:32:08	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:46:59	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-19 오후 5:32:08	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-19 오전 10:48:14	**Data File**	PENTA ST-07.d
Type	Cal	**Name**	PENTA ST-07
Dil.	0.002	**Acq. Method File**	VOCs(Penta-phenol)

Sample Chromatogram

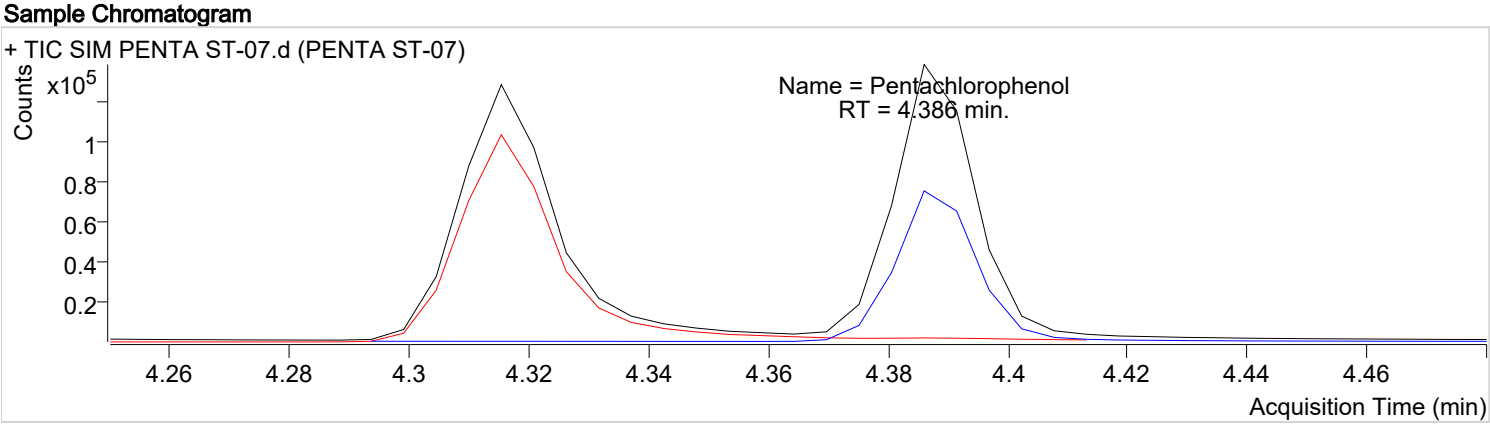

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol	4.386	73121	119689	0.0083 mg/L

Pentachlorophenol

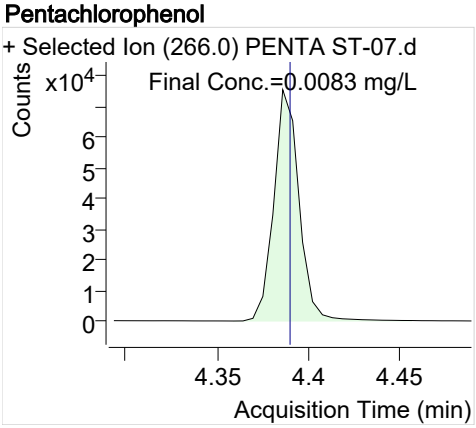



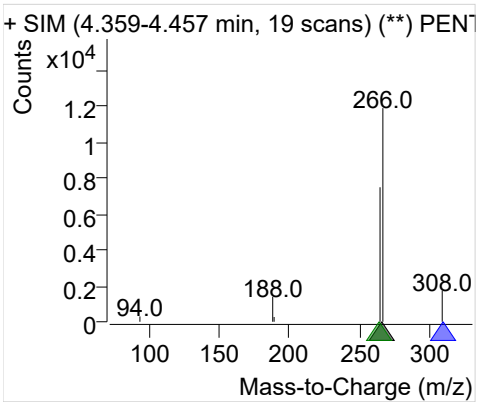

Quant Sample Report

Batch Data Path	V:\2026\2026-02\PENTA(GS 2.10 KH 2.10)\QuantResults\PHENTA.batch.bin		
Analysis Time	2026-02-19 오후 5:32:08	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:46:59	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-19 오후 5:32:08	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-19 오전 11:03:56	**Data File**	BK-.d
Type	Sample	**Name**	BK-
Dil.	0.002	**Acq. Method File**	VOCs(Penta-phenol)

Sample Chromatogram

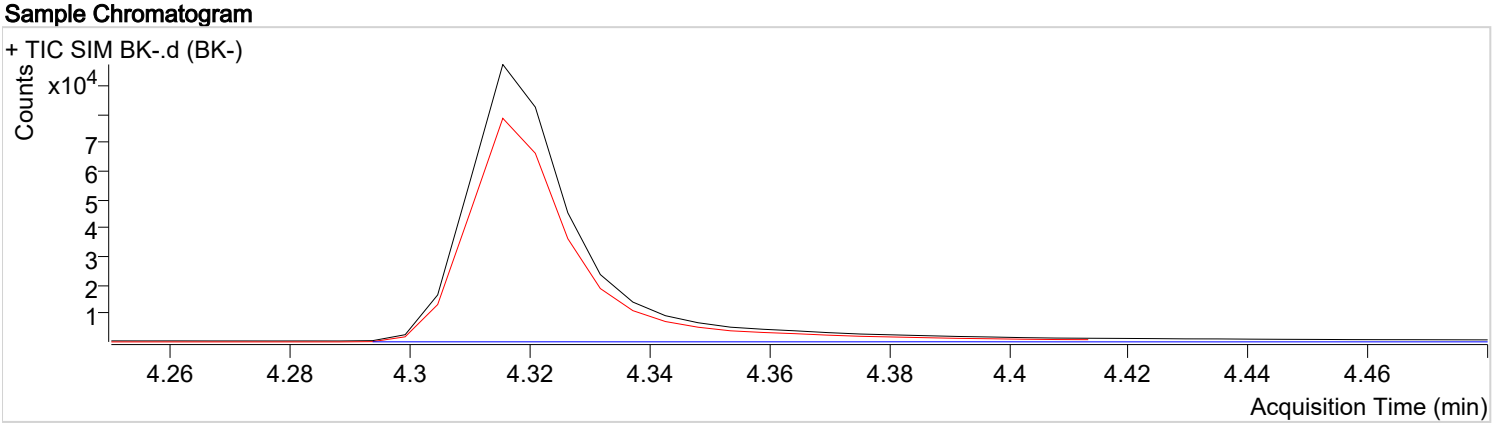

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol			97936	ND mg/L

Pentachlorophenol





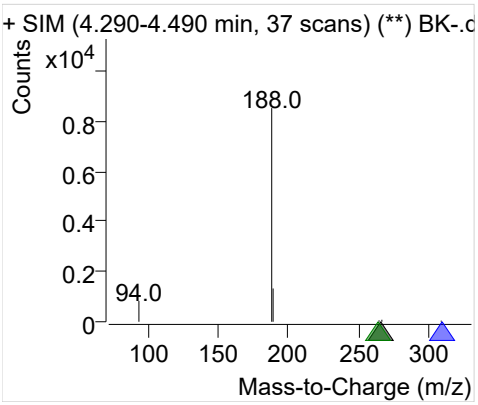

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-02\PENTA(GS 2.10 KH 2.10)\QuantResults\PHENTA.batch.bin		
Analysis Time	2026-02-19 오후 5:32:08	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:46:59	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-19 오후 5:32:08	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-19 오전 11:11:47	**Data File**	FBK(GS 26-02-10).d
Type	Sample	**Name**	FBK(GS 26-02-10)
Dil.	0.002	**Acq. Method File**	VOCs(Penta-phenol)

Sample Chromatogram

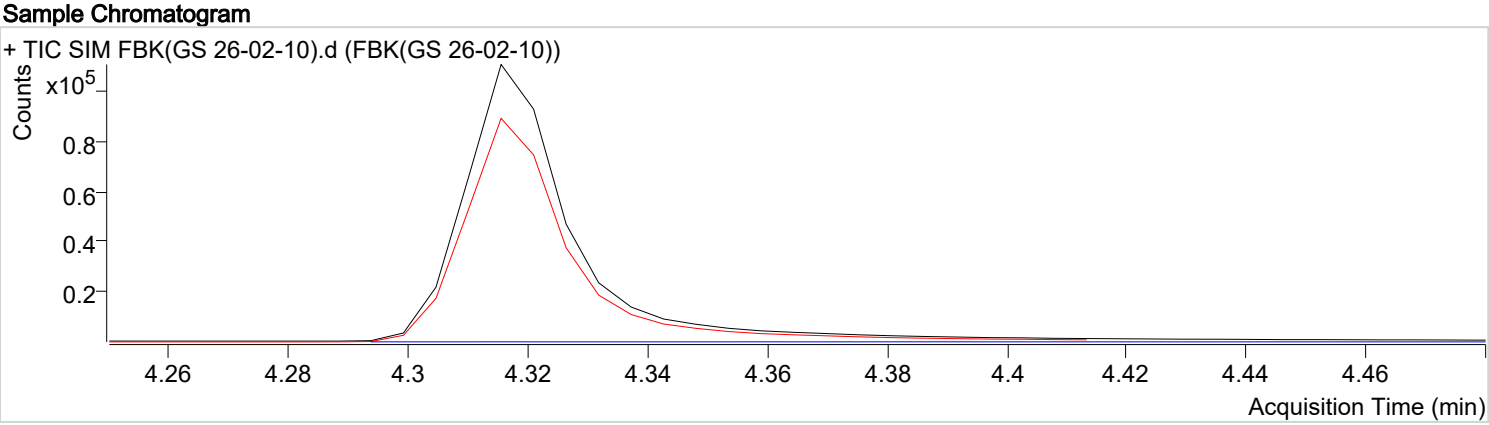

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol			108574	ND mg/L

Pentachlorophenol

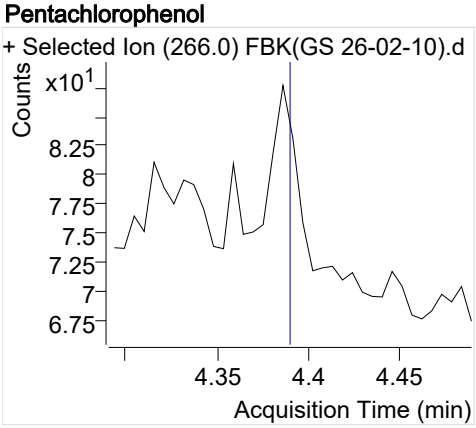



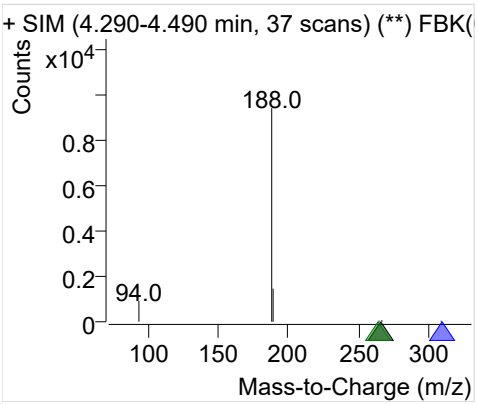

Quant Sample Report

Batch Data Path	V:\2026\2026-02\PENTA(GS 2.10 KH 2.10)\QuantResults\PHENTA.batch.bin		
Analysis Time	2026-02-19 오후 5:32:08	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:46:59	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-19 오후 5:32:08	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-19 오전 11:19:39	**Data File**	KH 26-02-10.d
Type	Sample	**Name**	KH 26-02-10
Dil.	0.002	**Acq. Method File**	VOCs(Penta-phenol)

Sample Chromatogram

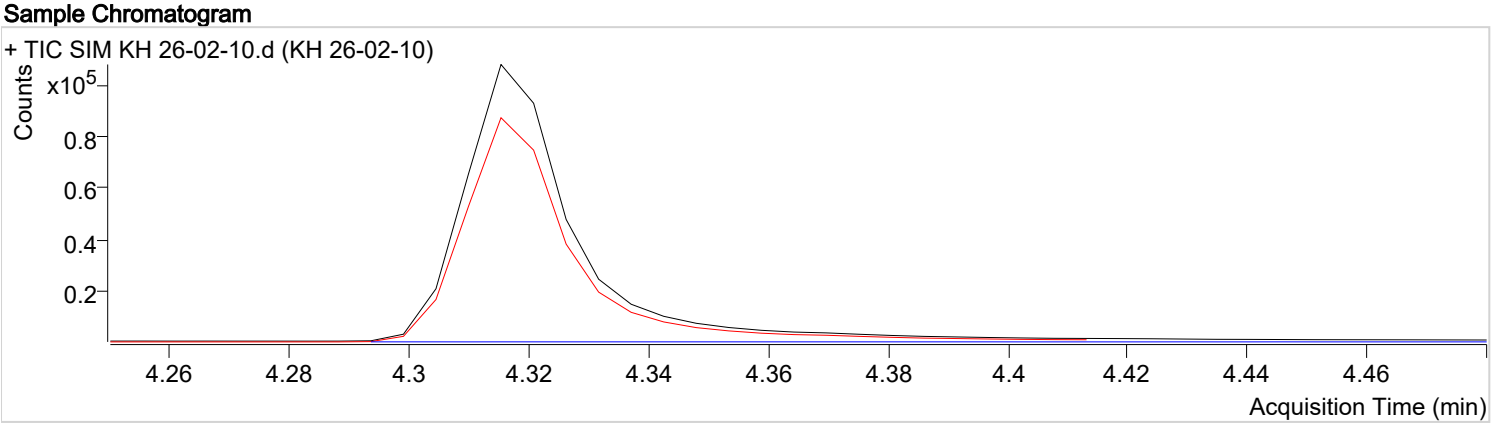

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol			108763	ND mg/L

Pentachlorophenol





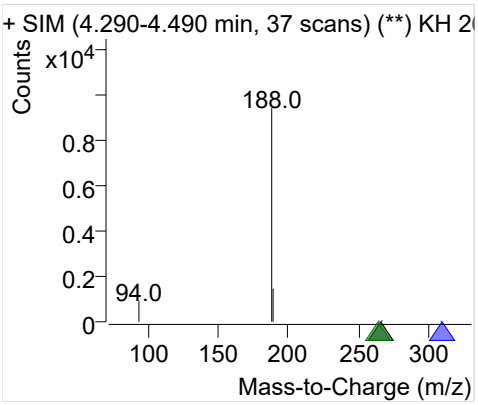

Quant Sample Report

Batch Data Path	V:\2026\2026-02\PENTA(GS 2.10 KH 2.10)\QuantResults\PHENTA.batch.bin		
Analysis Time	2026-02-19 오후 5:32:08	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:46:59	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-19 오후 5:32:08	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-19 오전 11:27:30	**Data File**	GS-01.d
Type	Sample	**Name**	GS-01
Dil.	0.002	**Acq. Method File**	VOCs(Penta-phenol)

Sample Chromatogram

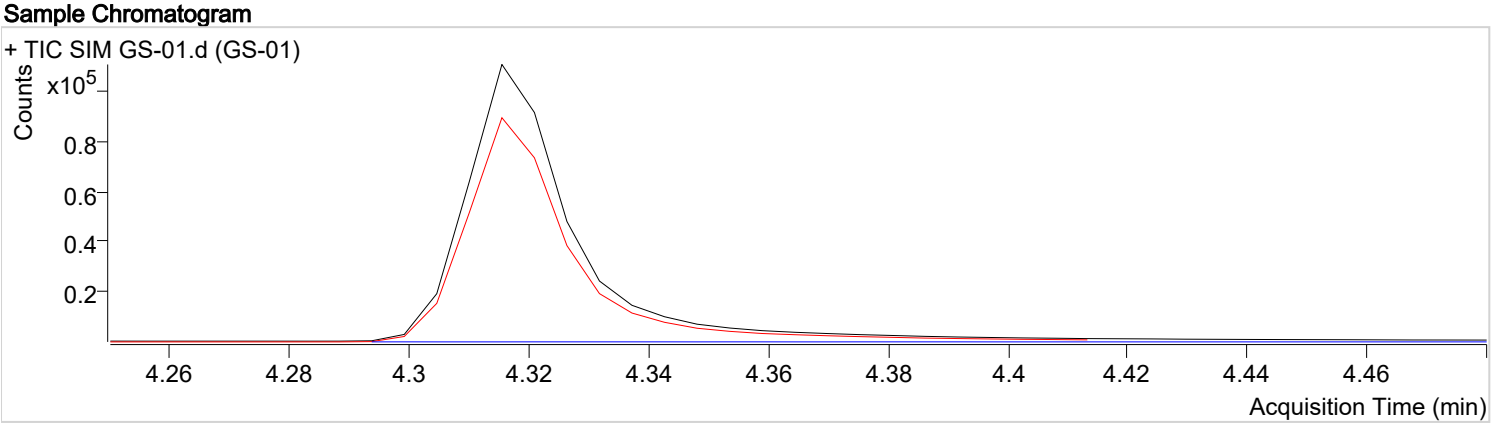

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol			108264	ND mg/L

Pentachlorophenol







Quant Sample Report

Batch Data Path	V:\2026\2026-02\PENTA(GS 2.10 KH 2.10)\QuantResults\PHENTA.batch.bin		
Analysis Time	2026-02-19 오후 5:32:08	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:46:59	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-19 오후 5:32:08	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-19 오전 11:35:21	**Data File**	GS-02.d
Type	Sample	**Name**	GS-02
Dil.	0.002	**Acq. Method File**	VOCs(Penta-phenol)

Sample Chromatogram

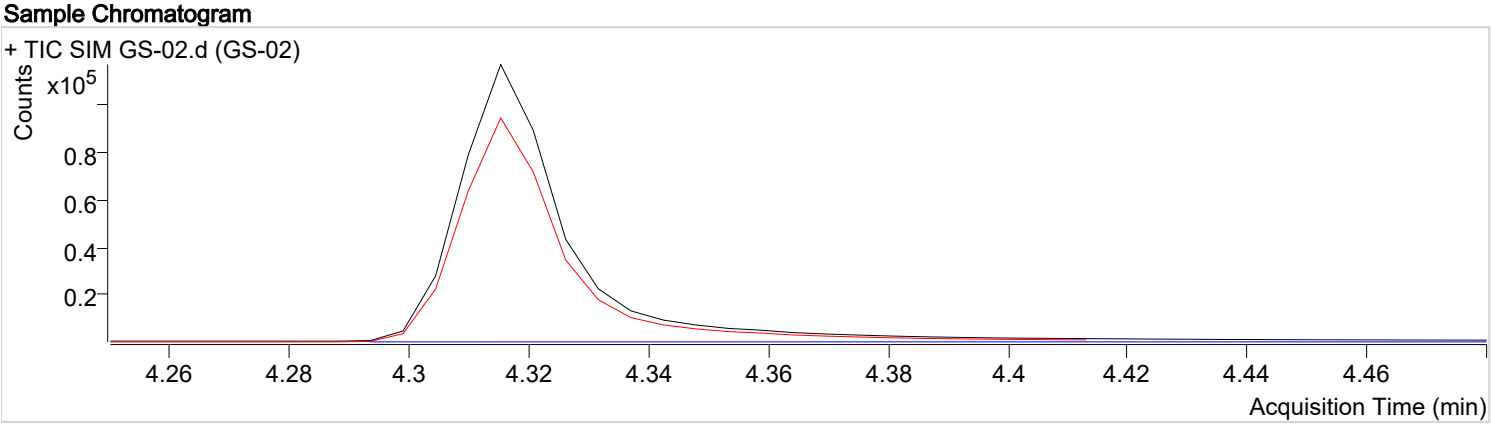

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol			113890	ND mg/L

Pentachlorophenol







Quant Sample Report

Batch Data Path	V:\2026\2026-02\PENTA(GS 2.10 KH 2.10)\QuantResults\PHENTA.batch.bin		
Analysis Time	2026-02-19 오후 5:32:08	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:46:59	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-19 오후 5:32:08	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-19 오전 11:43:13	**Data File**	GS-03.d
Type	Sample	**Name**	GS-03
Dil.	0.002	**Acq. Method File**	VOCs(Penta-phenol)

Sample Chromatogram

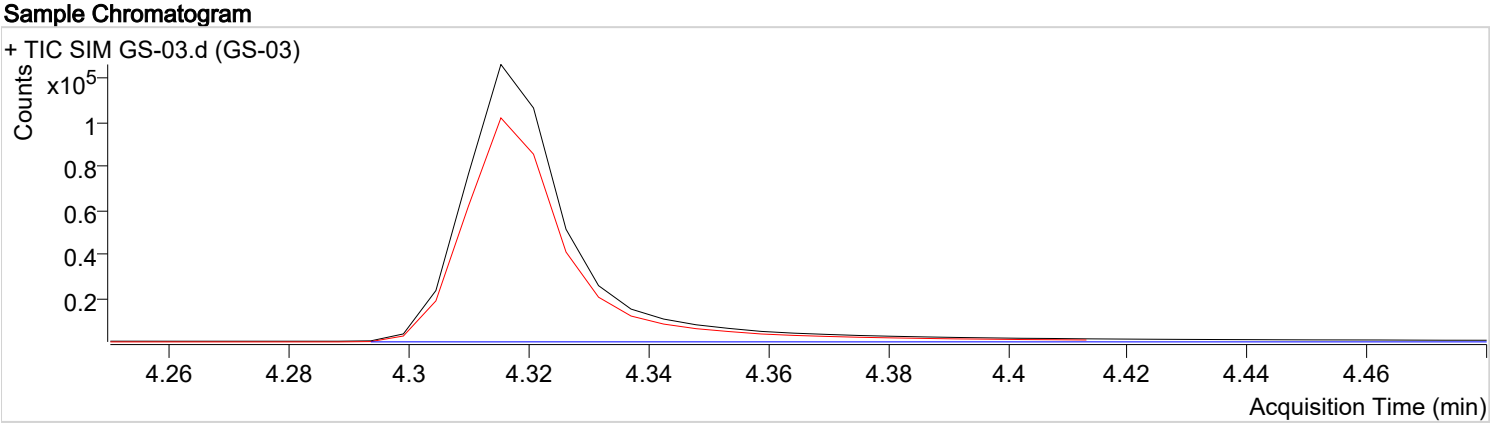

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol			122490	ND mg/L

Pentachlorophenol







Quant Sample Report

Batch Data Path	V:\2026\2026-02\PENTA(GS 2.10 KH 2.10)\QuantResults\PHENTA.batch.bin		
Analysis Time	2026-02-19 오후 5:32:08	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:46:59	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-19 오후 5:32:08	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-19 오전 11:51:05	**Data File**	GS-04.d
Type	Sample	**Name**	GS-04
Dil.	0.002	**Acq. Method File**	VOCs(Penta-phenol)

Sample Chromatogram

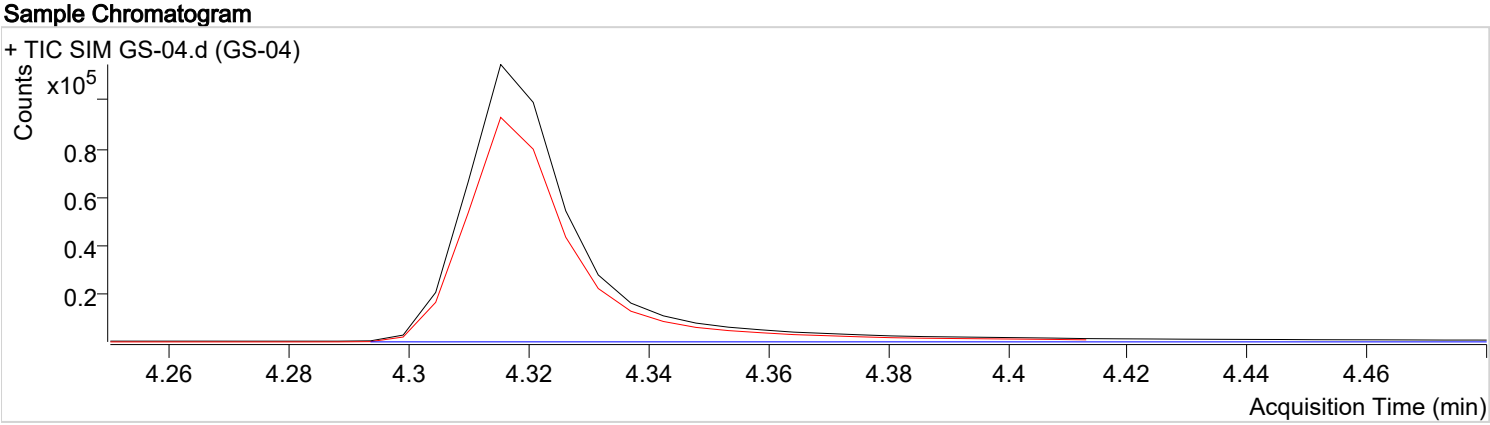

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol			116053	ND mg/L

Pentachlorophenol





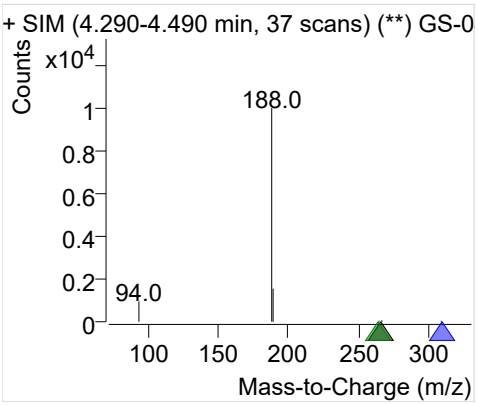

Quant Sample Report

Batch Data Path	V:\2026\2026-02\PENTA(GS 2.10 KH 2.10)\QuantResults\PHENTA.batch.bin		
Analysis Time	2026-02-19 오후 5:32:08	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:46:59	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-19 오후 5:32:08	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-19 오전 11:59:01	**Data File**	GS-05.d
Type	Sample	**Name**	GS-05
Dil.	0.002	**Acq. Method File**	VOCs(Penta-phenol)

Sample Chromatogram

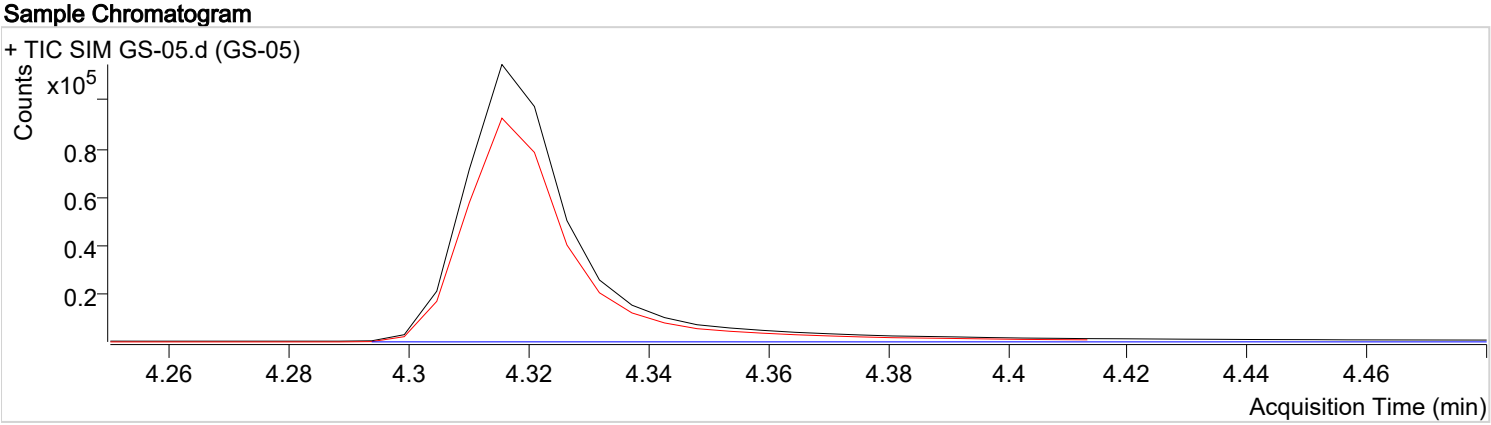

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol			114526	ND mg/L

Pentachlorophenol







Quant Sample Report

Batch Data Path	V:\2026\2026-02\PENTA(GS 2.10 KH 2.10)\QuantResults\PHENTA.batch.bin		
Analysis Time	2026-02-19 오후 5:32:08	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:46:59	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-19 오후 5:32:08	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-19 오후 12:06:53	**Data File**	GS-06.d
Type	Sample	**Name**	GS-06
Dil.	0.002	**Acq. Method File**	VOCs(Penta-phenol)

Sample Chromatogram

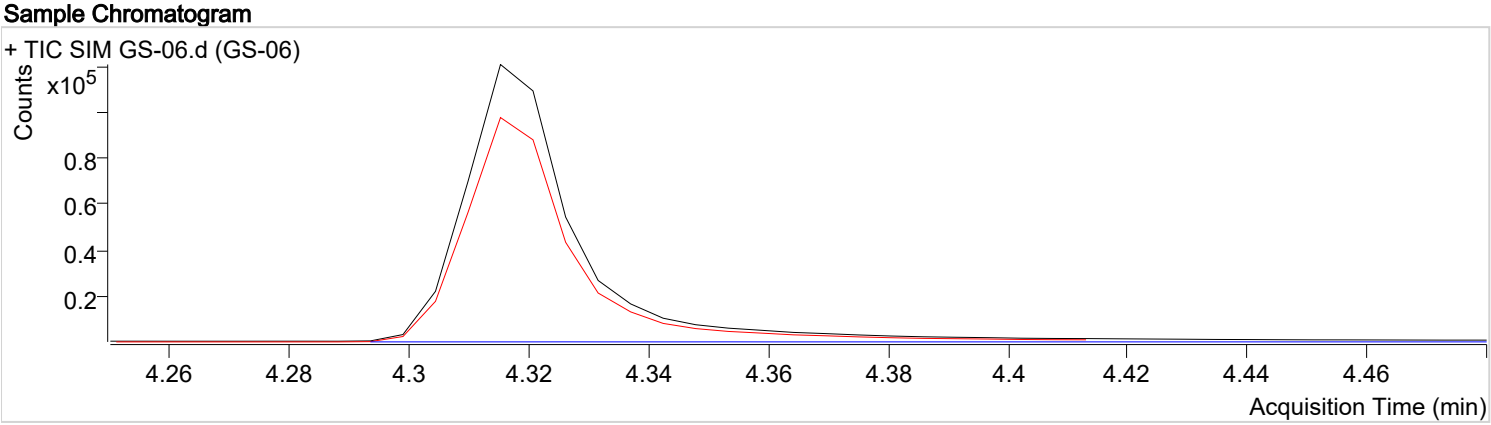

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol			121436	ND mg/L

Pentachlorophenol







Quant Sample Report

Batch Data Path	V:\2026\2026-02\PENTA(GS 2.10 KH 2.10)\QuantResults\PHENTA.batch.bin		
Analysis Time	2026-02-19 오후 5:32:08	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:46:59	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-19 오후 5:32:08	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-19 오후 12:14:46	**Data File**	GS-11.d
Type	Sample	**Name**	GS-11
Dil.	0.002	**Acq. Method File**	VOCs(Penta-phenol)

Sample Chromatogram

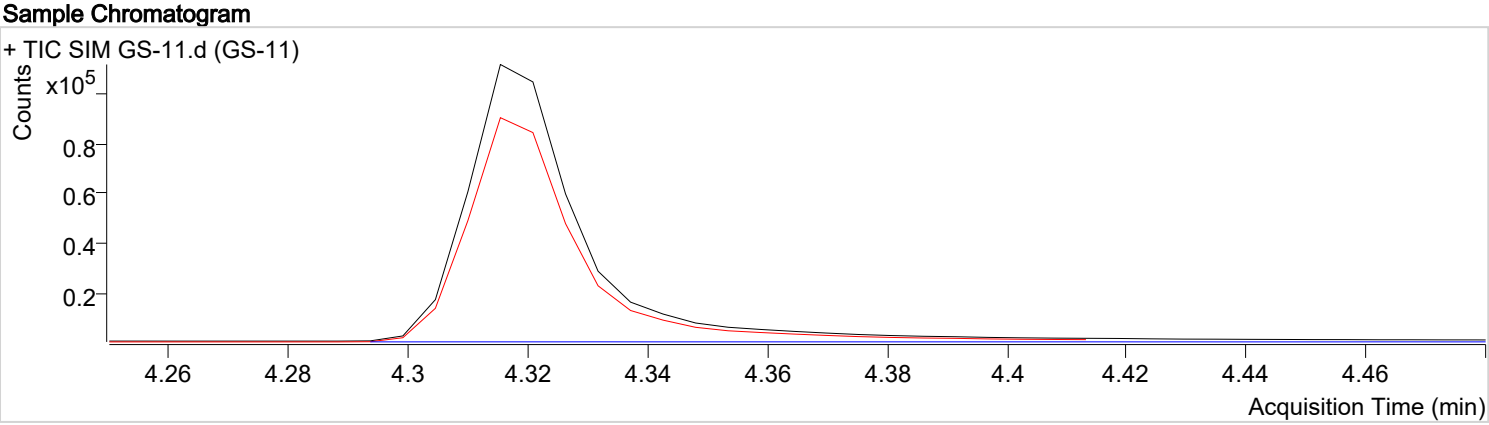

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol			118540	ND mg/L

Pentachlorophenol







Quant Sample Report

Batch Data Path	V:\2026\2026-02\PENTA(GS 2.10 KH 2.10)\QuantResults\PHENTA.batch.bin		
Analysis Time	2026-02-19 오후 5:32:08	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:46:59	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-19 오후 5:32:08	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-19 오후 12:22:36	**Data File**	MBK.d
Type	Blank	**Name**	MBK
Dil.	0.002	**Acq. Method File**	VOCs(Penta-phenol)

Sample Chromatogram

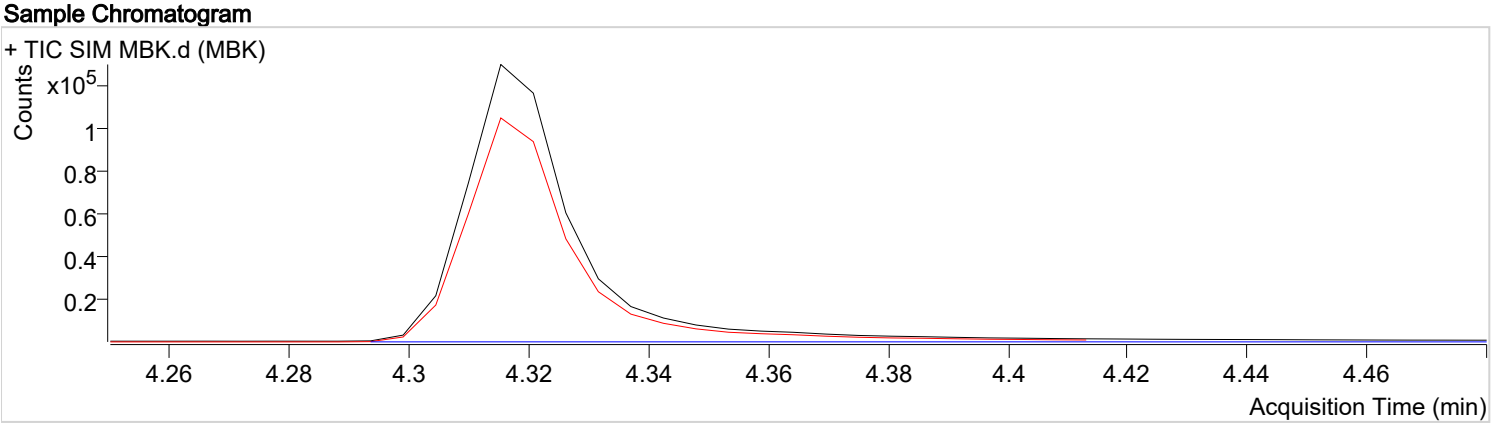

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol			129279	ND mg/L

Pentachlorophenol





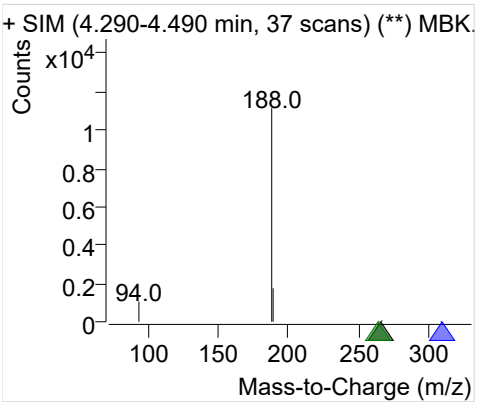

Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-02\PENTA(GS 2.10 KH 2.10)\QuantResults\PHENTA.batch.bin		
Analysis Time	2026-02-19 오후 5:32:08	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오후 1:46:59	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-02-19 오후 5:32:08	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-02-19 오후 12:46:11	**Data File**	-C-C-V-.d
Type	QC	**Name**	-C-C-V-
Dil.	0.002	**Acq. Method File**	VOCs(Penta-phenol)

Sample Chromatogram

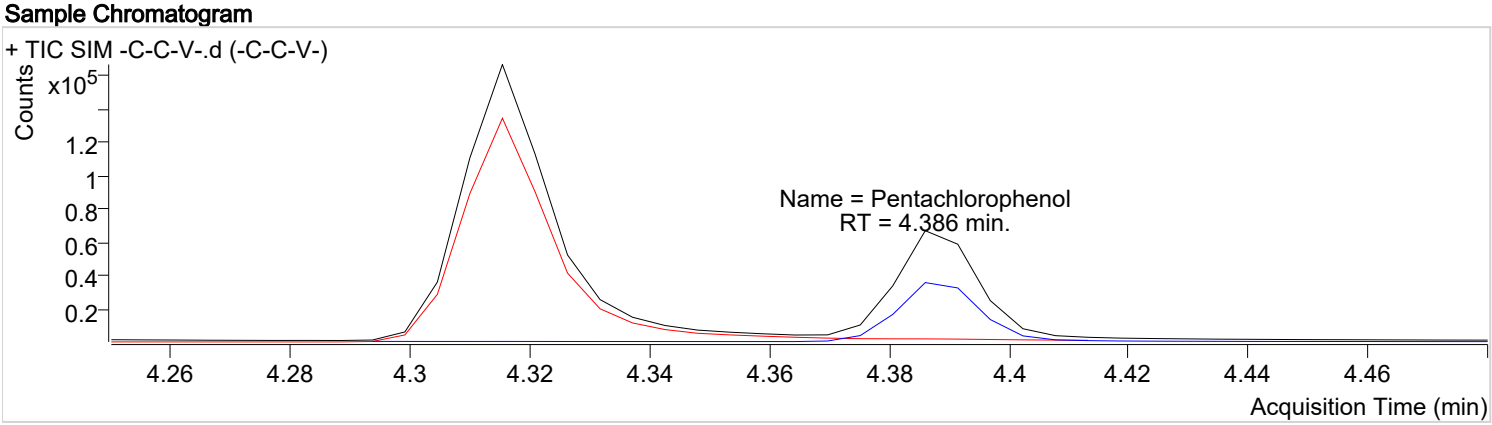

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Pentachlorophenol	4.386	35933	146998	0.0039 mg/L

Pentachlorophenol

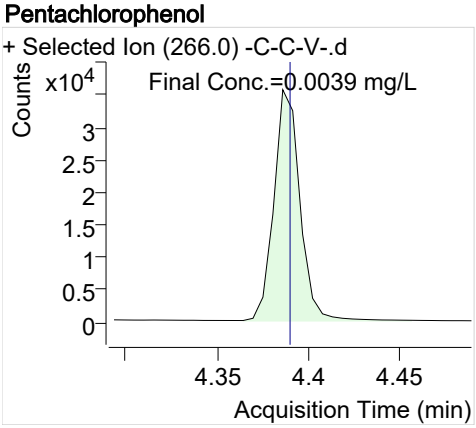



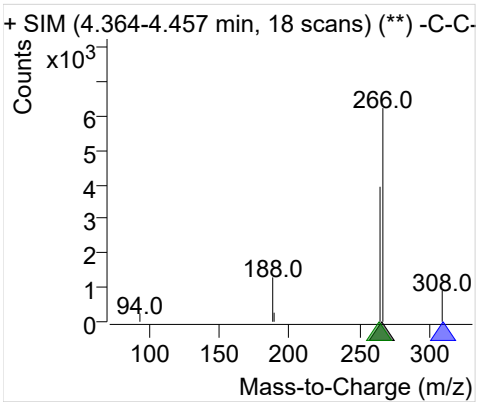

Generated at 오후 1:46 on 2026-04-10