Quantitative Analysis Results Summary Rep

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\FORM(RE 3.4, KD 3.4)\QuantResults\FORM.batch.bin				
Analysis Time	2026-03-06 오후 3:05:55	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-06 오후 3:05:55	**Analyze Quant Version**	10.2	**Report Quant Version**	10.2

Formaldehyde

Data File	Type	RT	Resp.	ISTD Resp	Final Conc.
FORM ST-01.d	Cal	5.023	84752	22309	0.000
FORM ST-02.d	Cal	5.020	933108	29225	0.038
FORM ST-03.d	Cal	5.019	1831032	25702	0.095
FORM ST-04.d	Cal	5.020	3779036	19738	0.269
FORM ST-05.d	Cal	5.016	7296148	19690	0.528
FORM ST-06.d	Cal	5.018	11256027	16429	0.983
BK-.d	Blank	5.023	53465	23786	0.000
FBK(RE 26-03-04).d	Blank	5.023	44779	23924	0.000
FBK(KD 26-03-04).d	Blank	5.023	33841	24025	0.000
RE-01.d	Sample	5.016	5915421	24430	0.342
RE-02.d	Sample	5.020	266140	23405	0.008
RE-03.d	Sample	5.018	7124933	25778	0.392
RE-04.d	Sample	5.020	718437	21257	0.041
RE-09.d	Sample	5.020	14076019	23341	0.864
RE-10.d	Sample	5.016	8407233	25599	0.467
RE-11.d	Sample	5.020	1294905	21657	0.078
RE-12.d	Sample	5.023	151746	18715	0.004
KD-01.d	Sample	5.020	9699438	30970	0.445
KD-02.d	Sample	5.018	15166355	24069	0.903
KD-03.d	Sample	5.019	2864302	22485	0.176
MBK.d	Blank	5.020	30582	29226	0.000
CCV.d	QC	5.016	6939813	17096	0.579

Formaldehyde

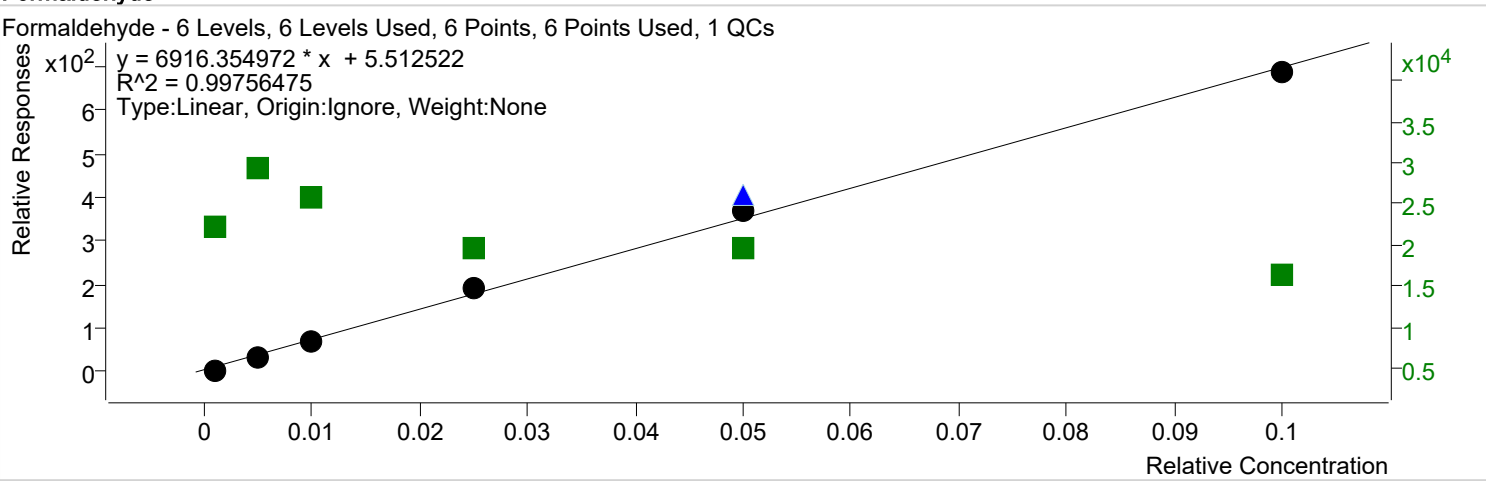

Cal. Path	Type	Level	Enable	Conc.	Response
V:\2026\2026-03\FORM(RE 3.4, KD 3.4)\FORM ST-01.d	Calibration	1	x	0.010	84752
V:\2026\2026-03\FORM(RE 3.4, KD 3.4)\FORM ST-02.d	Calibration	2	x	0.050	933108
V:\2026\2026-03\FORM(RE 3.4, KD 3.4)\FORM ST-03.d	Calibration	3	x	0.100	1831032
V:\2026\2026-03\FORM(RE 3.4, KD 3.4)\FORM ST-04.d	Calibration	4	x	0.250	3779036
V:\2026\2026-03\FORM(RE 3.4, KD 3.4)\FORM ST-05.d	Calibration	5	x	0.500	7296148
V:\2026\2026-03\FORM(RE 3.4, KD 3.4)\CCV.d	QC	5	x	0.500	6939813
V:\2026\2026-03\FORM(RE 3.4, KD 3.4)\FORM ST-06.d	Calibration	6	x	1.000	11256027

Quant Sample Report

Batch Data Path	V:\2026\2026-03\FORM(RE 3.4, KD 3.4)\QuantResults\FORM.batch.bin		
Analysis Time	2026-03-06 오후 3:05:55	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:41:14	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-06 오후 3:05:55	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-05 오전 11:44:29	**Data File**	FORM ST-01.d
Type	Cal	**Name**	FORM ST-01
Dil.	1	**Acq. Method File**	VOCs(Form)

Sample Chromatogram

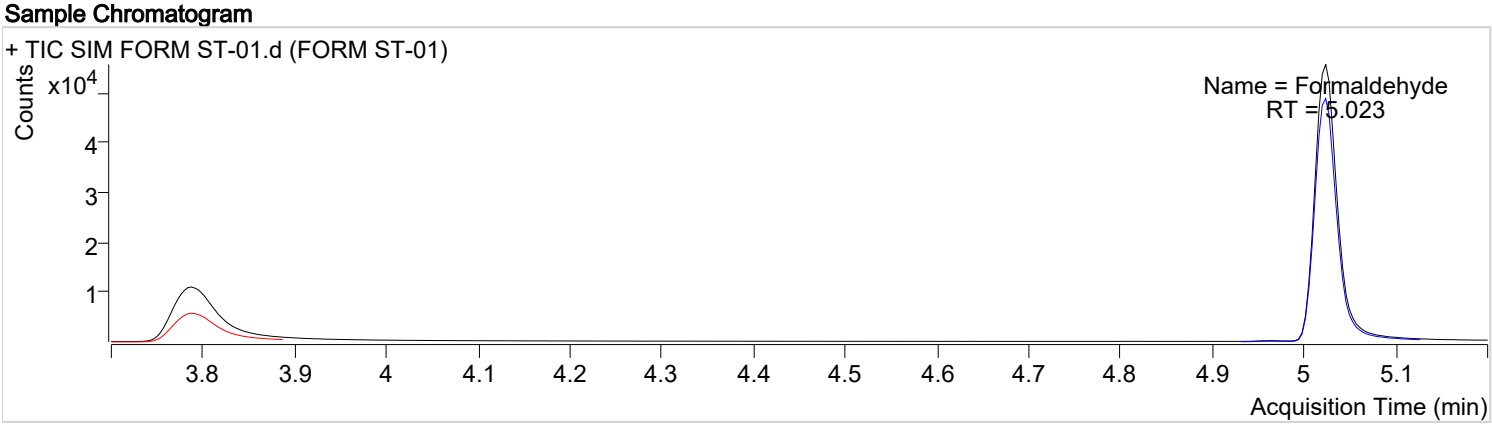

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Formaldehyde	5.023	84752	22309	0.000 mg/L

Formaldehyde

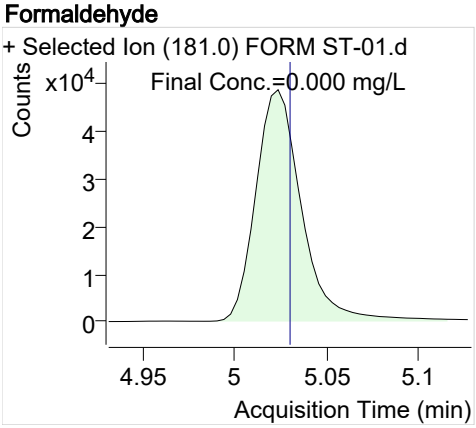





Quant Sample Report

Batch Data Path	V:\2026\2026-03\FORM(RE 3.4, KD 3.4)\QuantResults\FORM.batch.bin		
Analysis Time	2026-03-06 오후 3:05:55	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:41:14	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-06 오후 3:05:55	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-05 오후 12:03:28	**Data File**	FORM ST-02.d
Type	Cal	**Name**	FORM ST-02
Dil.	1	**Acq. Method File**	VOCs(Form)

Sample Chromatogram

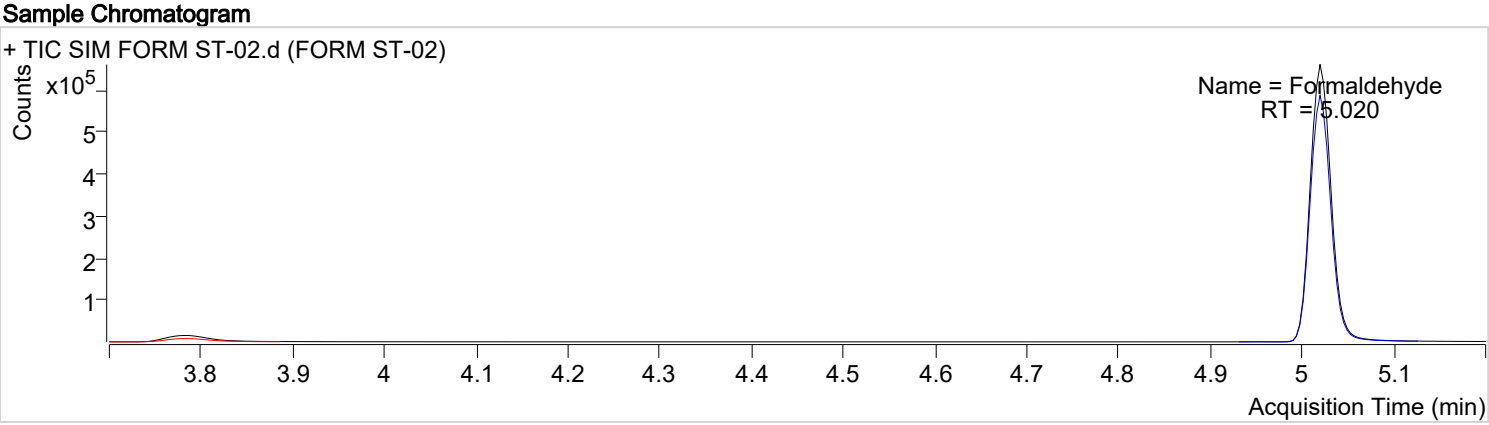

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Formaldehyde	5.020	933108	29225	0.038 mg/L

Formaldehyde

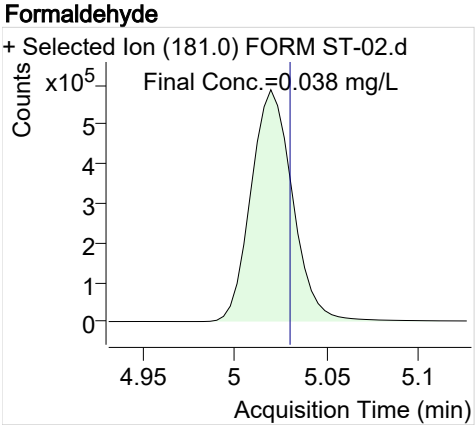





Quant Sample Report

Batch Data Path	V:\2026\2026-03\FORM(RE 3.4, KD 3.4)\QuantResults\FORM.batch.bin		
Analysis Time	2026-03-06 오후 3:05:55	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:41:14	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-06 오후 3:05:55	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-05 오후 12:17:17	**Data File**	FORM ST-03.d
Type	Cal	**Name**	FORM ST-03
Dil.	1	**Acq. Method File**	VOCs(Form)

Sample Chromatogram

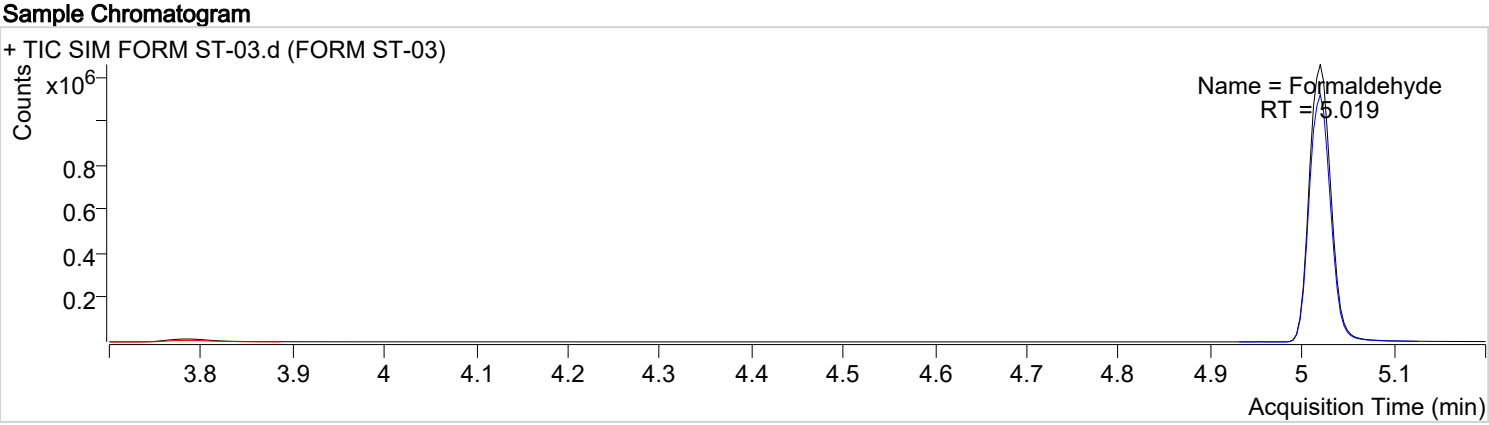

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Formaldehyde	5.019	1831032	25702	0.095 mg/L

Formaldehyde





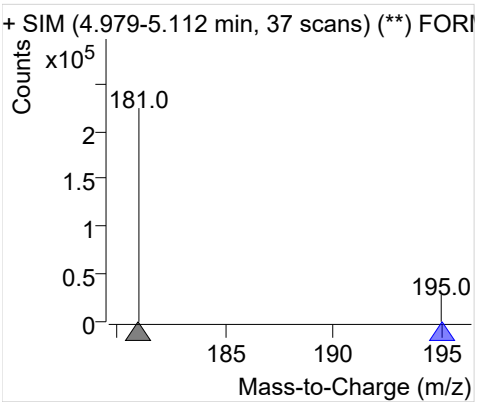

Quant Sample Report

Batch Data Path	V:\2026\2026-03\FORM(RE 3.4, KD 3.4)\QuantResults\FORM.batch.bin		
Analysis Time	2026-03-06 오후 3:05:55	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:41:14	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-06 오후 3:05:55	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-05 오후 12:31:10	**Data File**	FORM ST-04.d
Type	Cal	**Name**	FORM ST-04
Dil.	1	**Acq. Method File**	VOCs(Form)

Sample Chromatogram

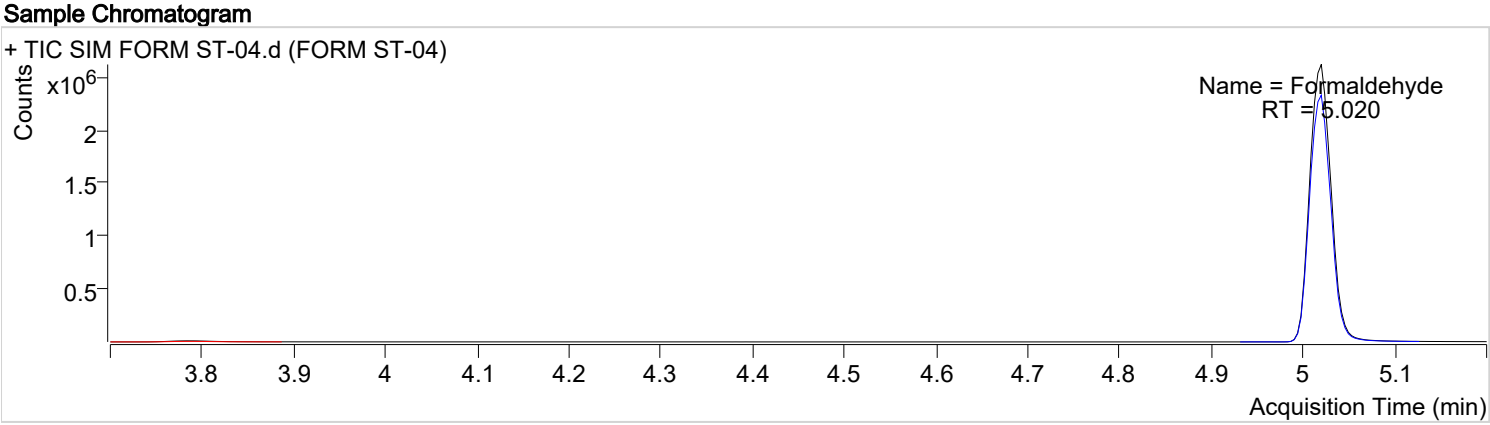

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Formaldehyde	5.020	3779036	19738	0.269 mg/L

Formaldehyde







Quant Sample Report

Batch Data Path	V:\2026\2026-03\FORM(RE 3.4, KD 3.4)\QuantResults\FORM.batch.bin		
Analysis Time	2026-03-06 오후 3:05:55	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:41:14	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-06 오후 3:05:55	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-05 오후 12:48:30	**Data File**	FORM ST-05.d
Type	Cal	**Name**	FORM ST-05
Dil.	1	**Acq. Method File**	VOCs(Form)

Sample Chromatogram

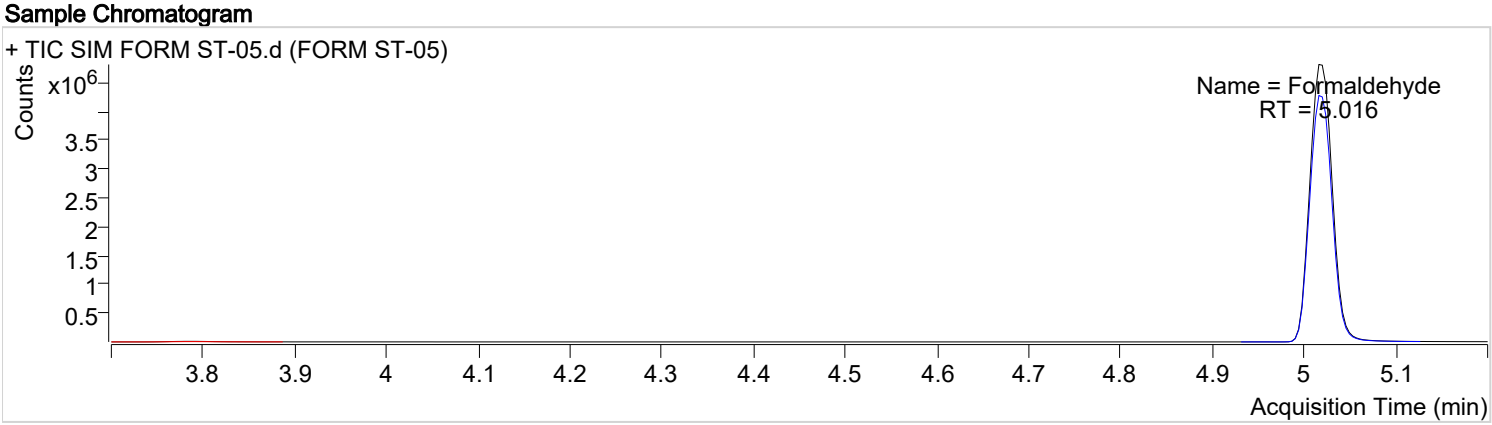

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Formaldehyde	5.016	7296148	19690	0.528 mg/L

Formaldehyde

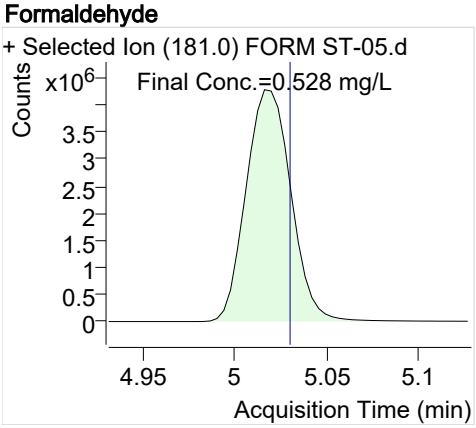





Quant Sample Report

Batch Data Path	V:\2026\2026-03\FORM(RE 3.4, KD 3.4)\QuantResults\FORM.batch.bin		
Analysis Time	2026-03-06 오후 3:05:55	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:41:14	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-06 오후 3:05:55	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-05 오후 1:02:19	**Data File**	FORM ST-06.d
Type	Cal	**Name**	FORM ST-06
Dil.	1	**Acq. Method File**	VOCs(Form)

Sample Chromatogram

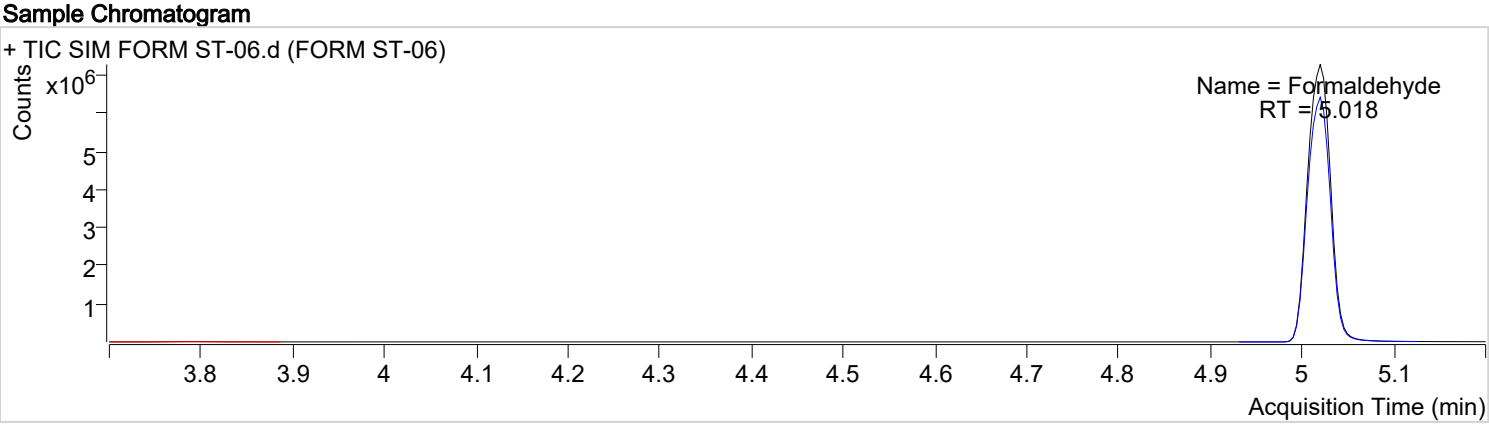

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Formaldehyde	5.018	11256027	16429	0.983 mg/L

Formaldehyde

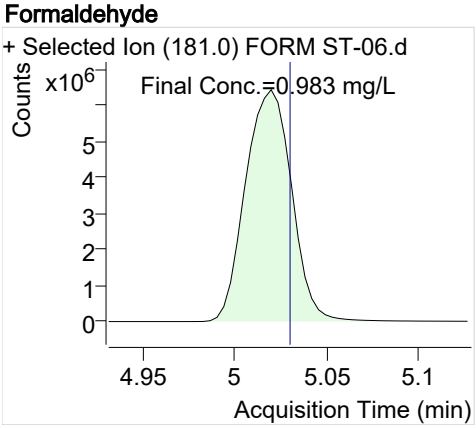





Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\FORM(RE 3.4, KD 3.4)\QuantResults\FORM.batch.bin		
Analysis Time	2026-03-06 오후 3:05:55	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:41:14	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-06 오후 3:05:55	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-05 오후 1:33:33	**Data File**	BK-.d
Type	Blank	**Name**	BK-
Dil.	1	**Acq. Method File**	VOCs(Form)

Sample Chromatogram

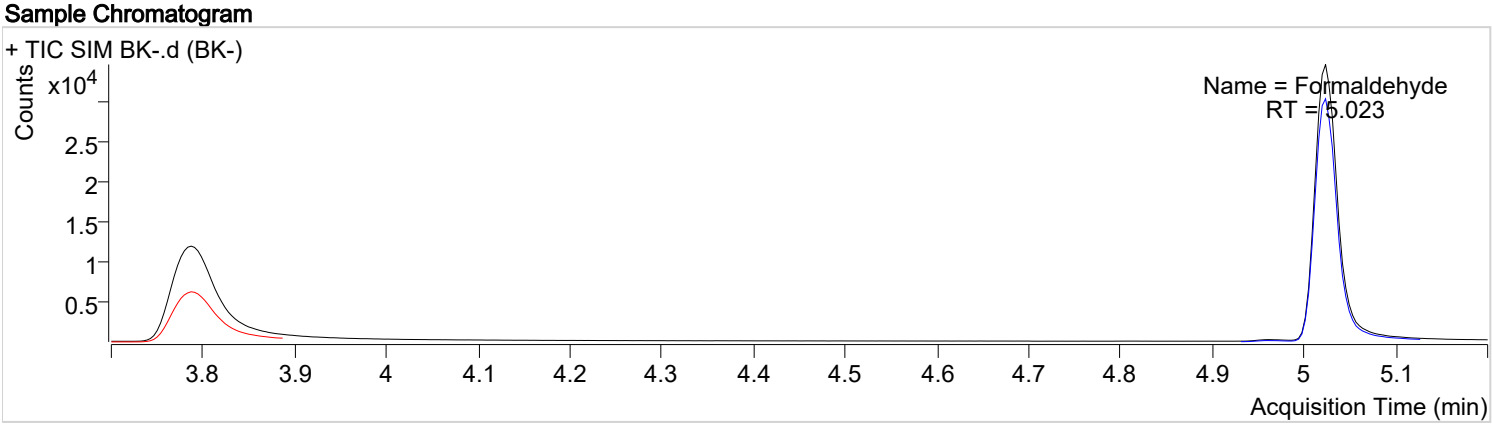

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Formaldehyde	5.023	53465	23786	0.000 mg/L

Formaldehyde

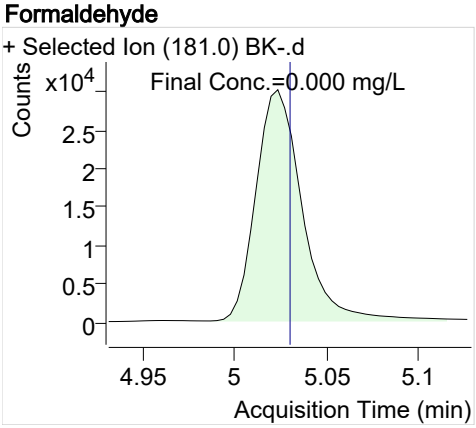





Quant Sample Report

Batch Data Path	V:\2026\2026-03\FORM(RE 3.4, KD 3.4)\QuantResults\FORM.batch.bin		
Analysis Time	2026-03-06 오후 3:05:55	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:41:14	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-06 오후 3:05:55	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-05 오후 1:47:20	**Data File**	FBK(RE 26-03-04).d
Type	Blank	**Name**	FBK(RE 26-03-04)
Dil.	1	**Acq. Method File**	VOCs(Form)

Sample Chromatogram

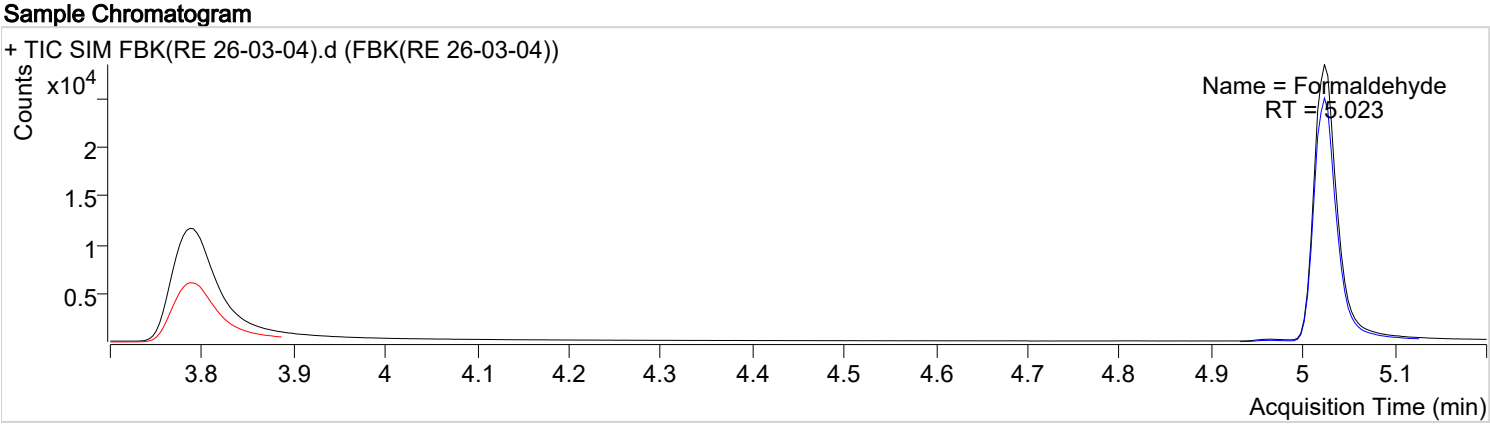

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Formaldehyde	5.023	44779	23924	0.000 mg/L

Formaldehyde







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\FORM(RE 3.4, KD 3.4)\QuantResults\FORM.batch.bin		
Analysis Time	2026-03-06 오후 3:05:55	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:41:14	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-06 오후 3:05:55	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-05 오후 2:01:11	**Data File**	FBK(KD 26-03-04).d
Type	Blank	**Name**	FBK(KD 26-03-04)
Dil.	1	**Acq. Method File**	VOCs(Form)

Sample Chromatogram

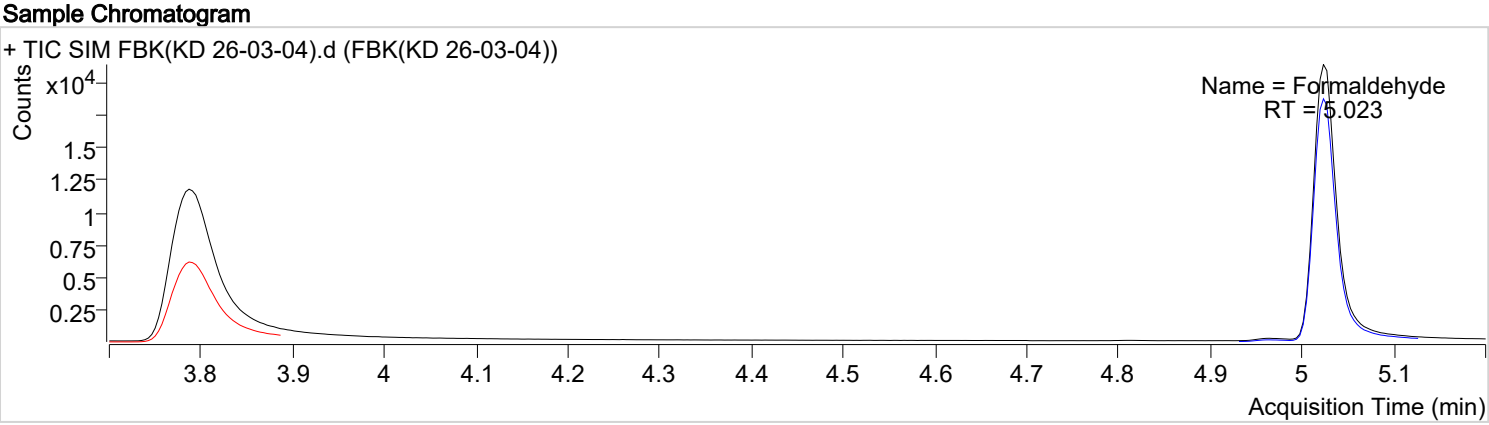

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Formaldehyde	5.023	33841	24025	0.000 mg/L

Formaldehyde

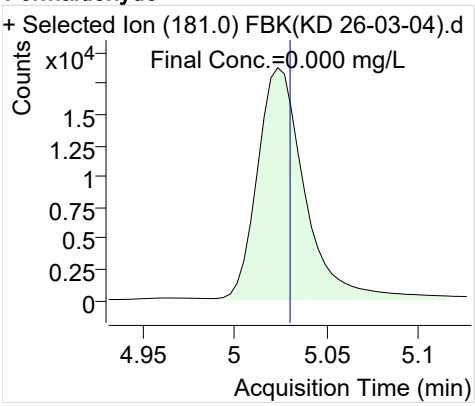

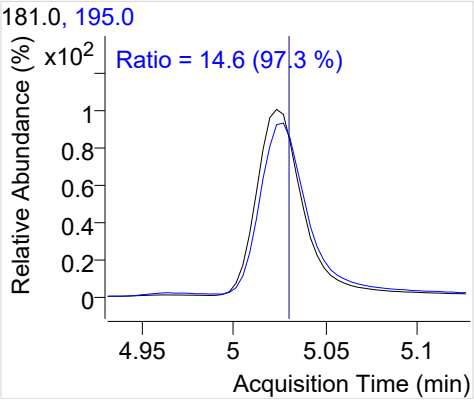

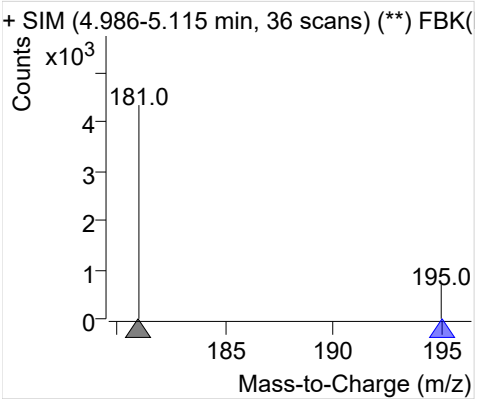

Quant Sample Report

Batch Data Path	V:\2026\2026-03\FORM(RE 3.4, KD 3.4)\QuantResults\FORM.batch.bin		
Analysis Time	2026-03-06 오후 3:05:55	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:41:14	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-06 오후 3:05:55	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-05 오후 2:18:36	**Data File**	RE-01.d
Type	Sample	**Name**	RE-01
Dil.	1	**Acq. Method File**	VOCs(Form)

Sample Chromatogram

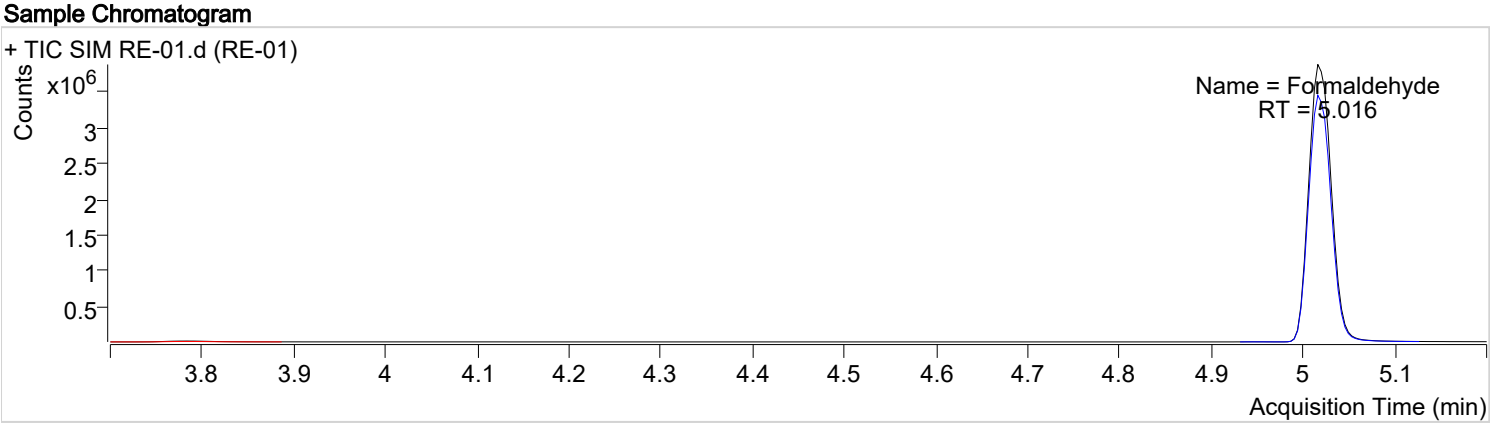

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Formaldehyde	5.016	5915421	24430	0.342 mg/L

Formaldehyde







Quant Sample Report

Batch Data Path	V:\2026\2026-03\FORM(RE 3.4, KD 3.4)\QuantResults\FORM.batch.bin		
Analysis Time	2026-03-06 오후 3:05:55	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:41:14	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-06 오후 3:05:55	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-05 오후 2:32:20	**Data File**	RE-02.d
Type	Sample	**Name**	RE-02
Dil.	1	**Acq. Method File**	VOCs(Form)

Sample Chromatogram

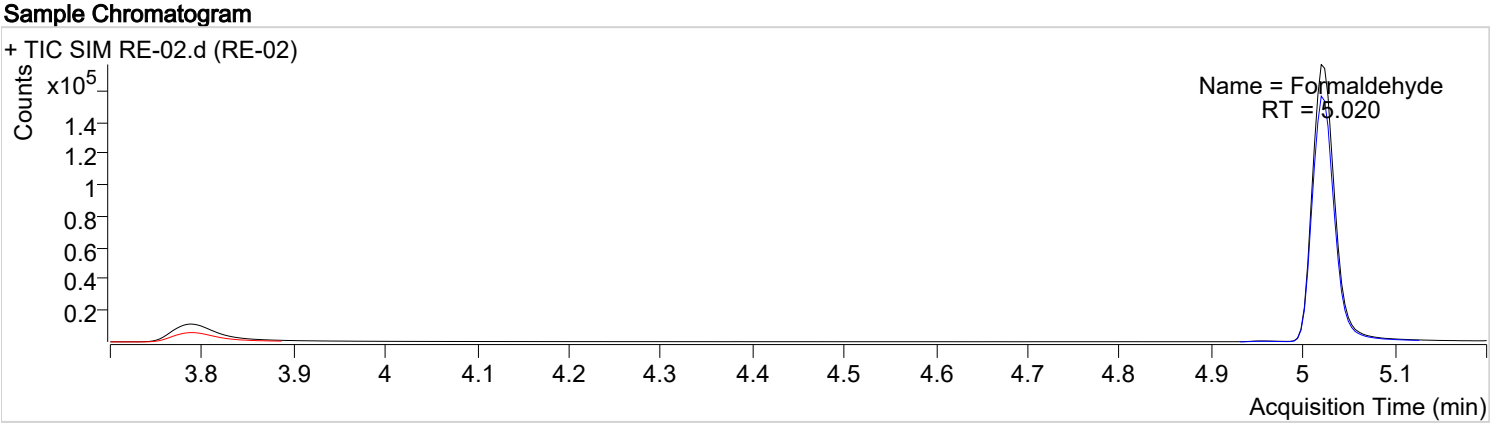

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Formaldehyde	5.020	266140	23405	0.008 mg/L

Formaldehyde







Quant Sample Report

Batch Data Path	V:\2026\2026-03\FORM(RE 3.4, KD 3.4)\QuantResults\FORM.batch.bin		
Analysis Time	2026-03-06 오후 3:05:55	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:41:14	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-06 오후 3:05:55	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-05 오후 2:46:22	**Data File**	RE-03.d
Type	Sample	**Name**	RE-03
Dil.	1	**Acq. Method File**	VOCs(Form)

Sample Chromatogram

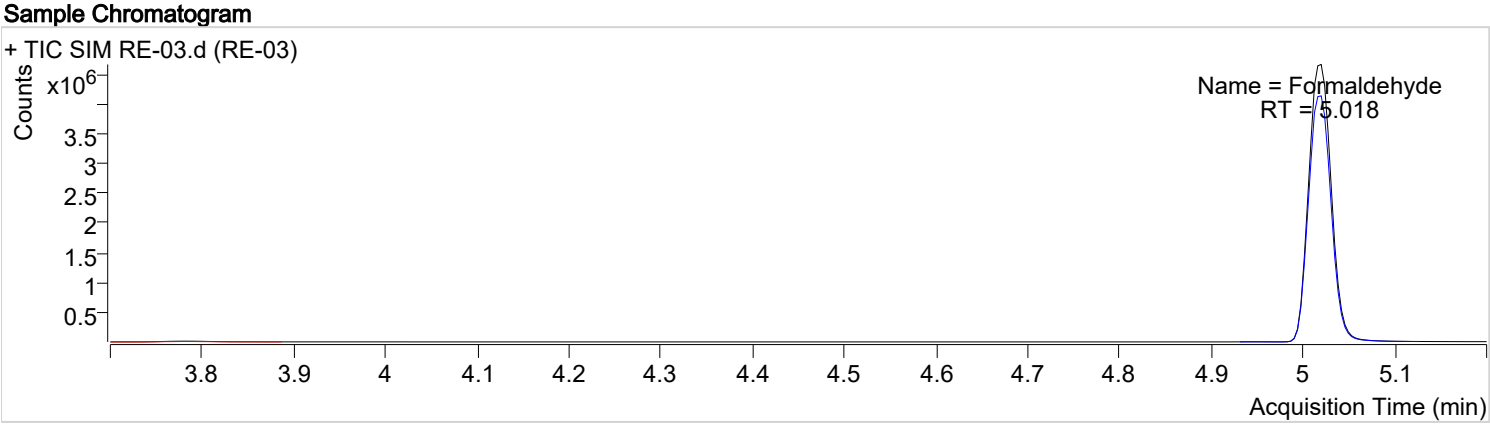

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Formaldehyde	5.018	7124933	25778	0.392 mg/L

Formaldehyde







Quant Sample Report

Batch Data Path	V:\2026\2026-03\FORM(RE 3.4, KD 3.4)\QuantResults\FORM.batch.bin		
Analysis Time	2026-03-06 오후 3:05:55	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:41:14	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-06 오후 3:05:55	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-05 오후 3:03:36	**Data File**	RE-04.d
Type	Sample	**Name**	RE-04
Dil.	1	**Acq. Method File**	VOCs(Form)

Sample Chromatogram

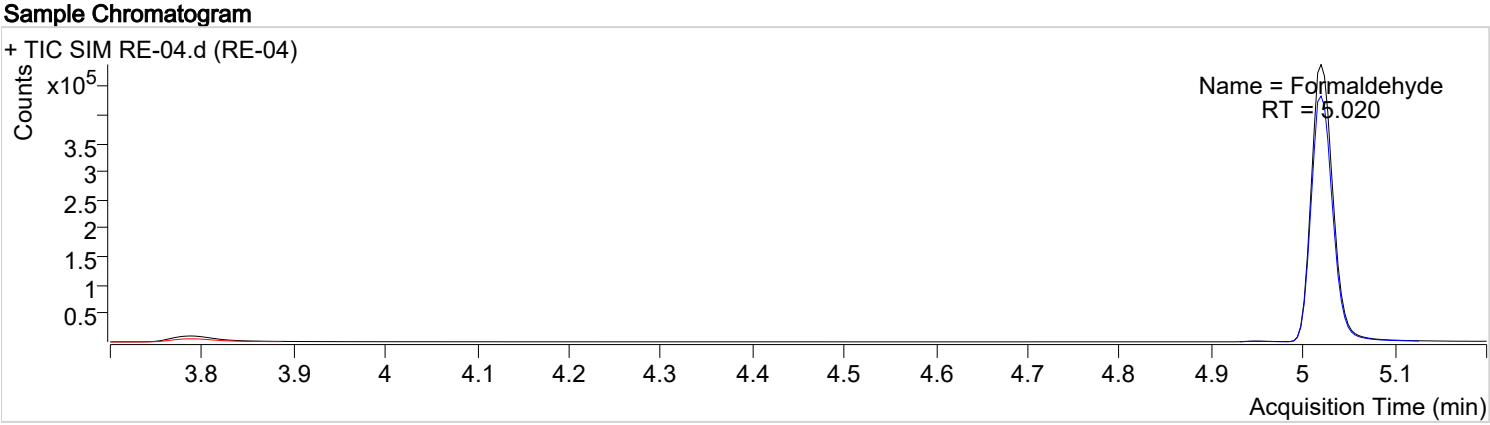

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Formaldehyde	5.020	718437	21257	0.041 mg/L

Formaldehyde







Quant Sample Report

Batch Data Path	V:\2026\2026-03\FORM(RE 3.4, KD 3.4)\QuantResults\FORM.batch.bin		
Analysis Time	2026-03-06 오후 3:05:55	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:41:14	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-06 오후 3:05:55	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-05 오후 3:17:31	**Data File**	RE-09.d
Type	Sample	**Name**	RE-09
Dil.	1	**Acq. Method File**	VOCs(Form)

Sample Chromatogram

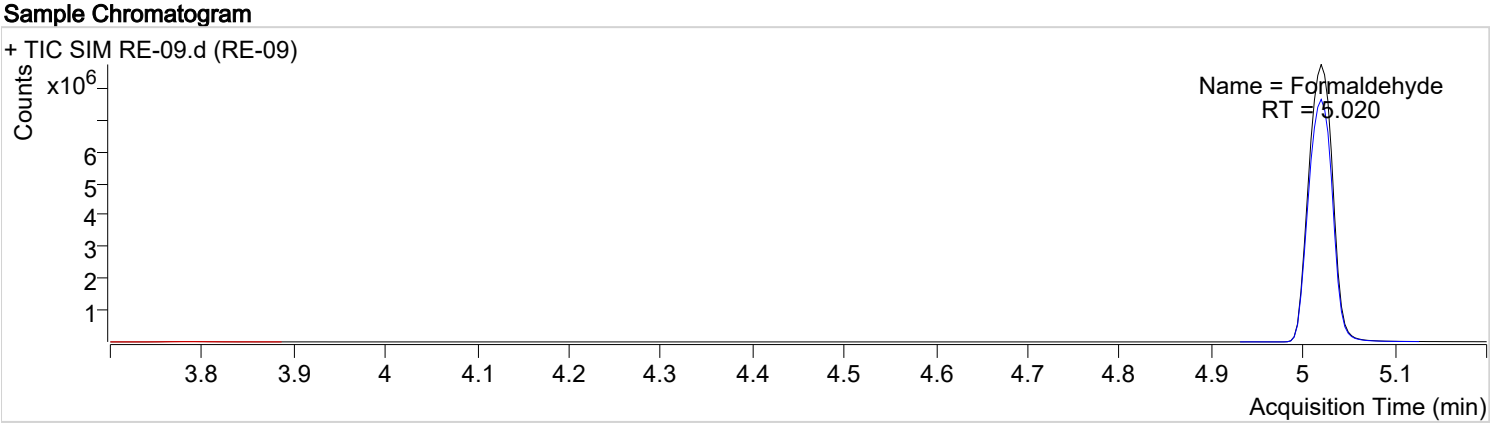

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Formaldehyde	5.020	14076019	23341	0.864 mg/L

Formaldehyde







Quant Sample Report

Batch Data Path	V:\2026\2026-03\FORM(RE 3.4, KD 3.4)\QuantResults\FORM.batch.bin		
Analysis Time	2026-03-06 오후 3:05:55	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:41:14	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-06 오후 3:05:55	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-05 오후 3:31:24	**Data File**	RE-10.d
Type	Sample	**Name**	RE-10
Dil.	1	**Acq. Method File**	VOCs(Form)

Sample Chromatogram

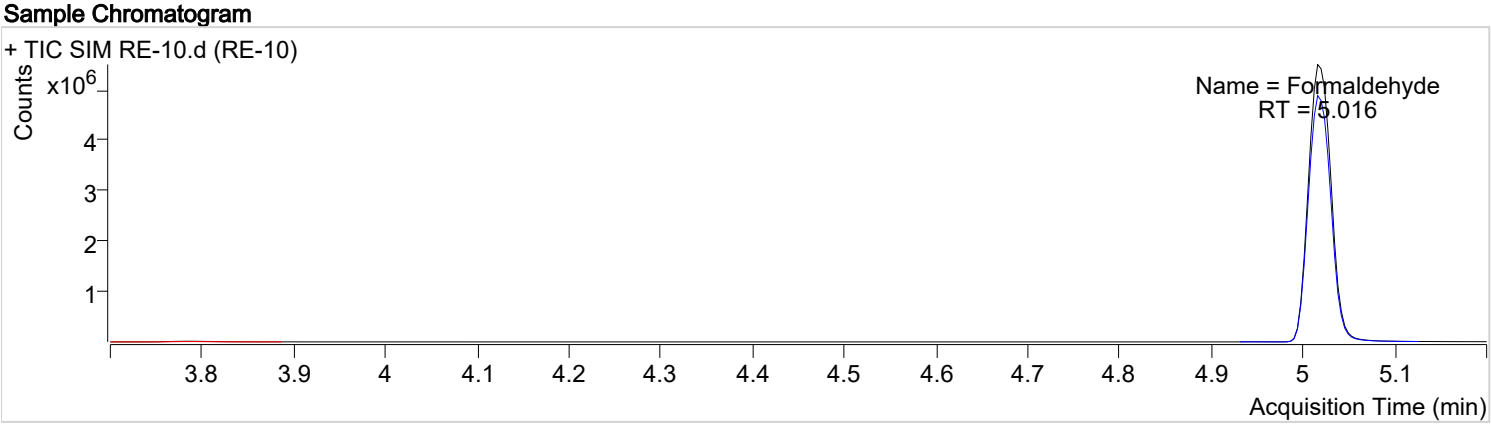

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Formaldehyde	5.016	8407233	25599	0.467 mg/L

Formaldehyde

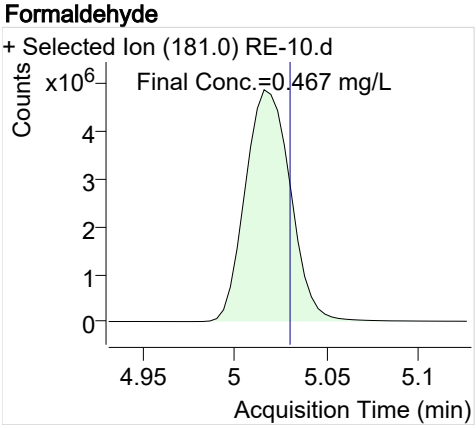





Quant Sample Report

Batch Data Path	V:\2026\2026-03\FORM(RE 3.4, KD 3.4)\QuantResults\FORM.batch.bin		
Analysis Time	2026-03-06 오후 3:05:55	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:41:14	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-06 오후 3:05:55	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-05 오후 3:48:42	**Data File**	RE-11.d
Type	Sample	**Name**	RE-11
Dil.	1	**Acq. Method File**	VOCs(Form)

Sample Chromatogram

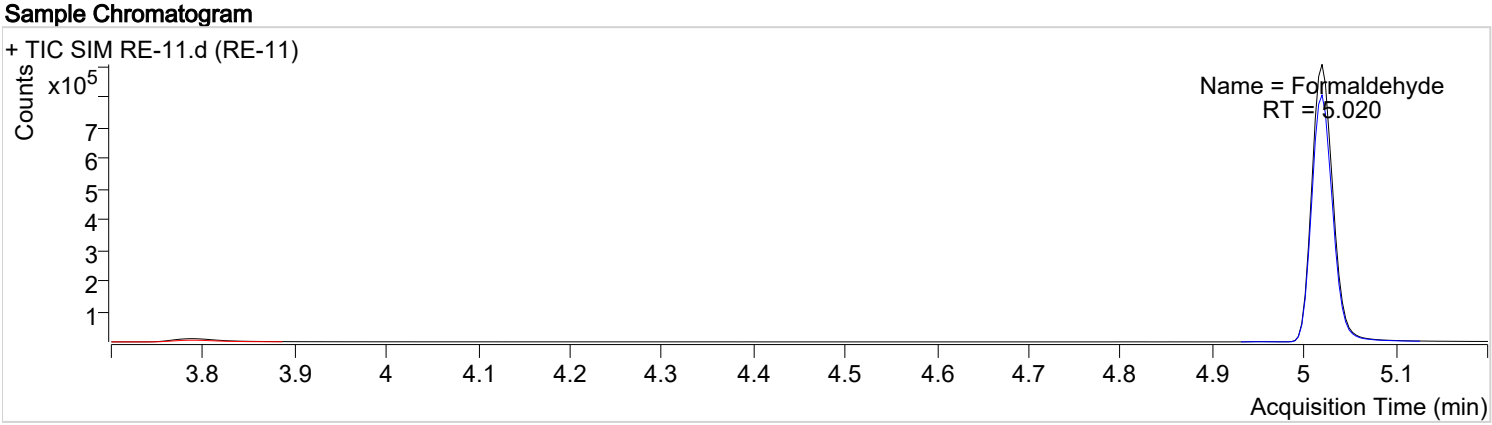

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Formaldehyde	5.020	1294905	21657	0.078 mg/L

Formaldehyde







Quant Sample Report

Batch Data Path	V:\2026\2026-03\FORM(RE 3.4, KD 3.4)\QuantResults\FORM.batch.bin		
Analysis Time	2026-03-06 오후 3:05:55	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:41:14	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-06 오후 3:05:55	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-05 오후 4:02:35	**Data File**	RE-12.d
Type	Sample	**Name**	RE-12
Dil.	1	**Acq. Method File**	VOCs(Form)

Sample Chromatogram

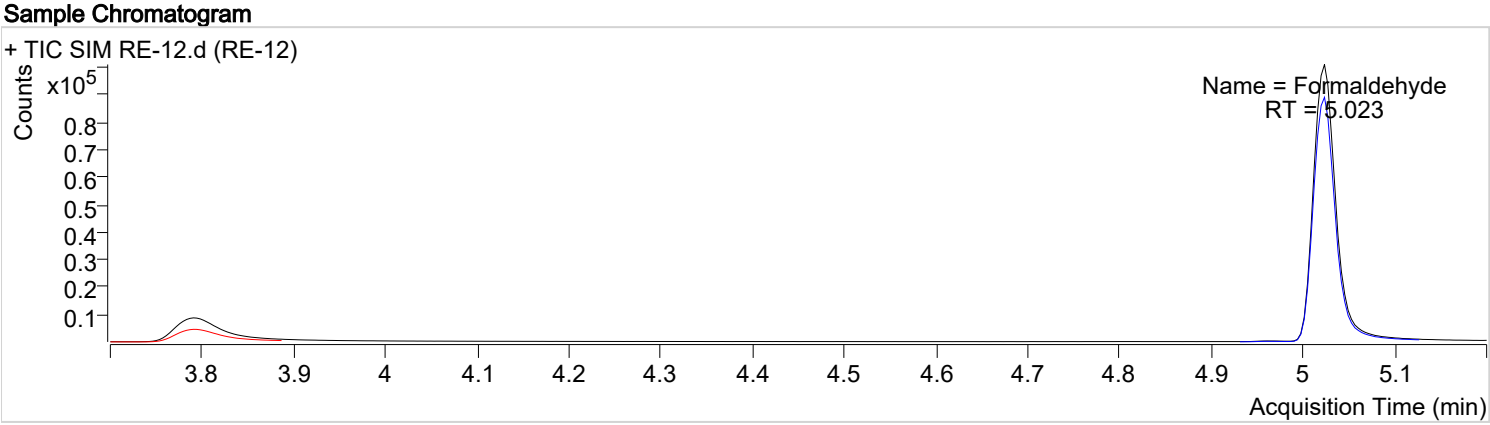

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Formaldehyde	5.023	151746	18715	0.004 mg/L

Formaldehyde



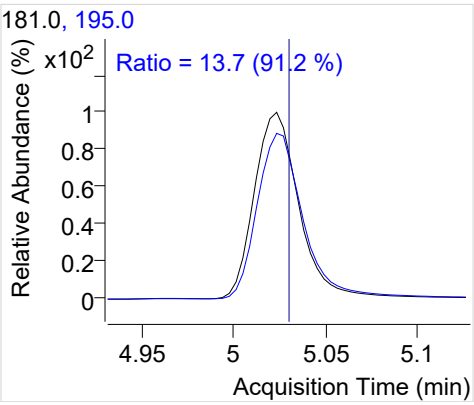

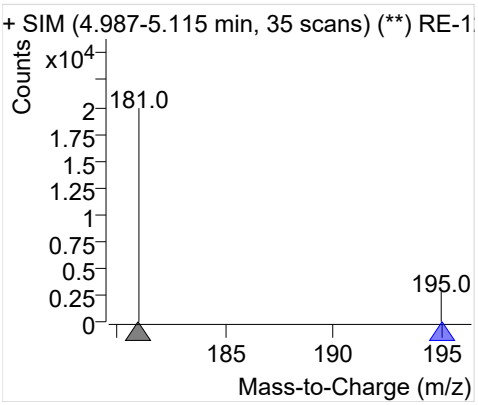

Quant Sample Report

Batch Data Path	V:\2026\2026-03\FORM(RE 3.4, KD 3.4)\QuantResults\FORM.batch.bin		
Analysis Time	2026-03-06 오후 3:05:55	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:41:14	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-06 오후 3:05:55	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-05 오후 4:16:26	**Data File**	KD-01.d
Type	Sample	**Name**	KD-01
Dil.	1	**Acq. Method File**	VOCs(Form)

Sample Chromatogram

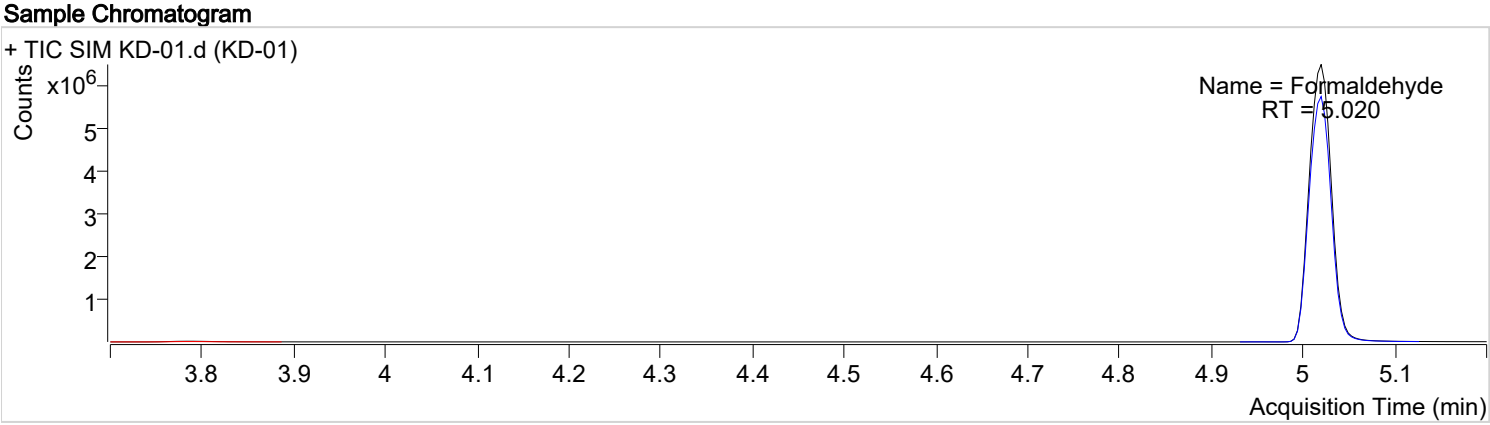

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Formaldehyde	5.020	9699438	30970	0.445 mg/L

Formaldehyde







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\FORM(RE 3.4, KD 3.4)\QuantResults\FORM.batch.bin		
Analysis Time	2026-03-06 오후 3:05:55	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:41:14	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-06 오후 3:05:55	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-05 오후 4:33:42	**Data File**	KD-02.d
Type	Sample	**Name**	KD-02
Dil.	1	**Acq. Method File**	VOCs(Form)

Sample Chromatogram

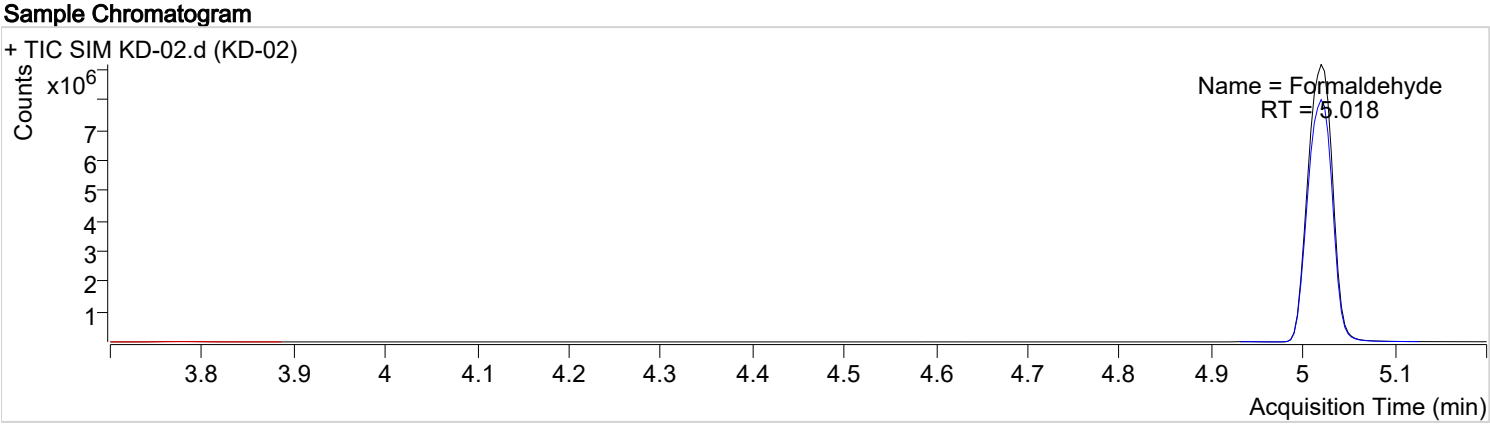

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Formaldehyde	5.018	15166355	24069	0.903 mg/L

Formaldehyde







Quant Sample Report

Agilent | Trusted Answers

Batch Data Path	V:\2026\2026-03\FORM(RE 3.4, KD 3.4)\QuantResults\FORM.batch.bin		
Analysis Time	2026-03-06 오후 3:05:55	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:41:14	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-06 오후 3:05:55	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-05 오후 4:47:36	**Data File**	KD-03.d
Type	Sample	**Name**	KD-03
Dil.	1	**Acq. Method File**	VOCs(Form)

Sample Chromatogram

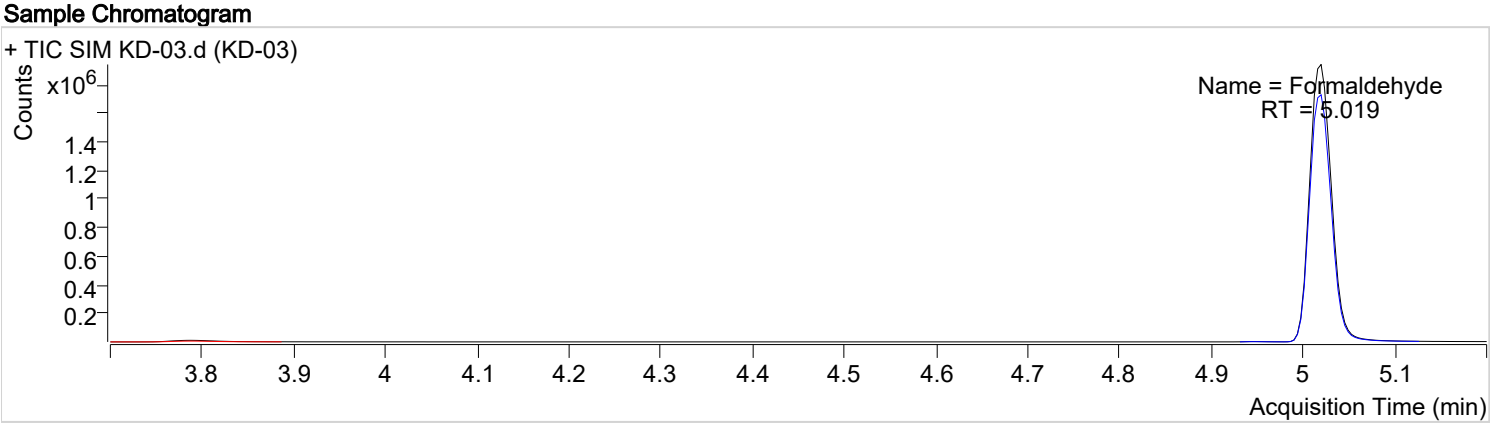

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Formaldehyde	5.019	2864302	22485	0.176 mg/L

Formaldehyde







Quant Sample Report

Batch Data Path	V:\2026\2026-03\FORM(RE 3.4, KD 3.4)\QuantResults\FORM.batch.bin		
Analysis Time	2026-03-06 오후 3:05:55	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:41:14	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-06 오후 3:05:55	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-05 오후 7:11:47	**Data File**	MBK.d
Type	Blank	**Name**	MBK
Dil.	1	**Acq. Method File**	VOCs(Form)

Sample Chromatogram

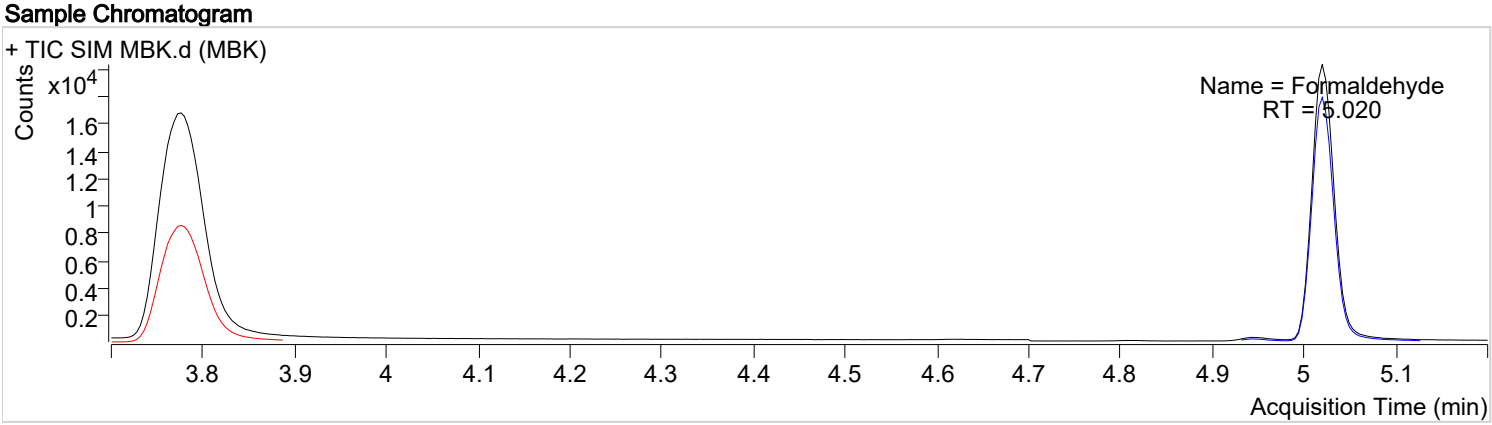

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Formaldehyde	5.020	30582	29226	0.000 mg/L

Formaldehyde







Quant Sample Report

Batch Data Path	V:\2026\2026-03\FORM(RE 3.4, KD 3.4)\QuantResults\FORM.batch.bin		
Analysis Time	2026-03-06 오후 3:05:55	**Analyst Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Report Generation Time	2026-04-10 오전 10:41:14	**Report Generator Name**	DESKTOP-N82KMQD\수질분석센터 GC2
Calibration Last Update	2026-03-06 오후 3:05:55	**Batch State**	Processed
Analyze Quant Version	10.2	**Report Quant Version**	10.2

Acq. Date-Time	2026-03-05 오후 7:30:44	**Data File**	CCV.d
Type	QC	**Name**	CCV
Dil.	1	**Acq. Method File**	VOCs(Form)

Sample Chromatogram

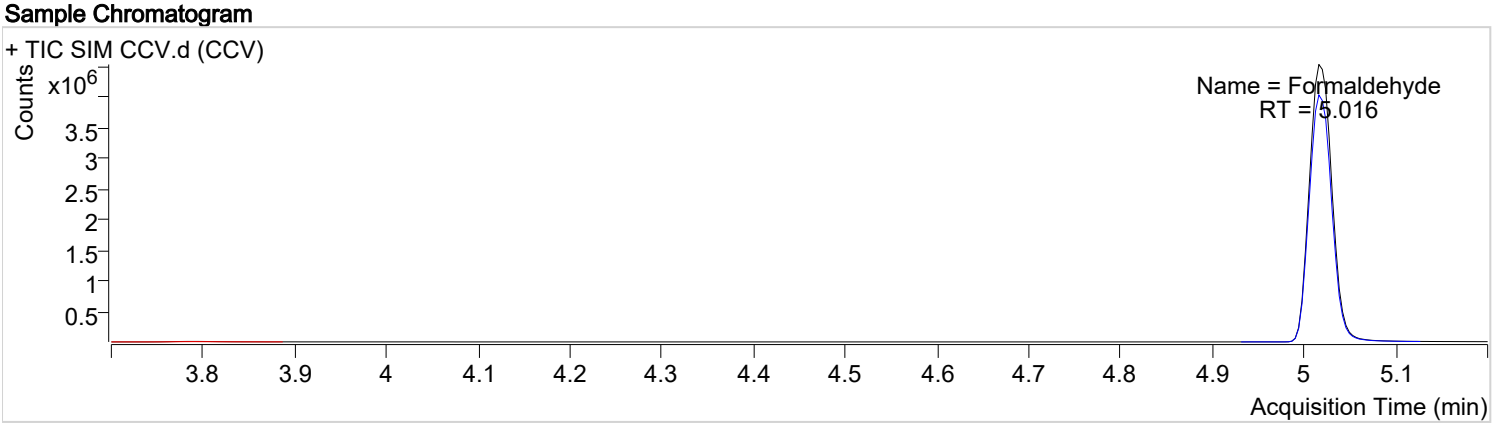

Name	RT	Resp.	ISTD Resp	Final Units Conc.
Formaldehyde	5.016	6939813	17096	0.579 mg/L
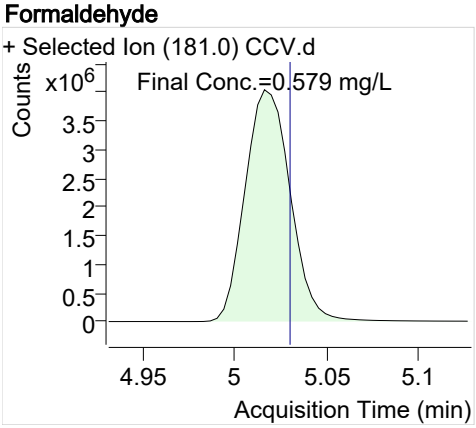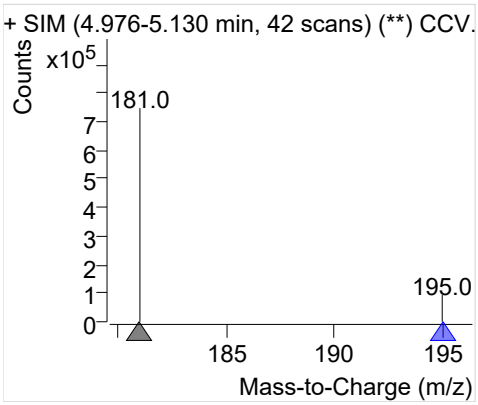
Formaldehyde