


(a) Real Measured Precision Degradation (Δ PPL)



(b) DACP Advantage over InShrinkerator (Real V100 Measurements)

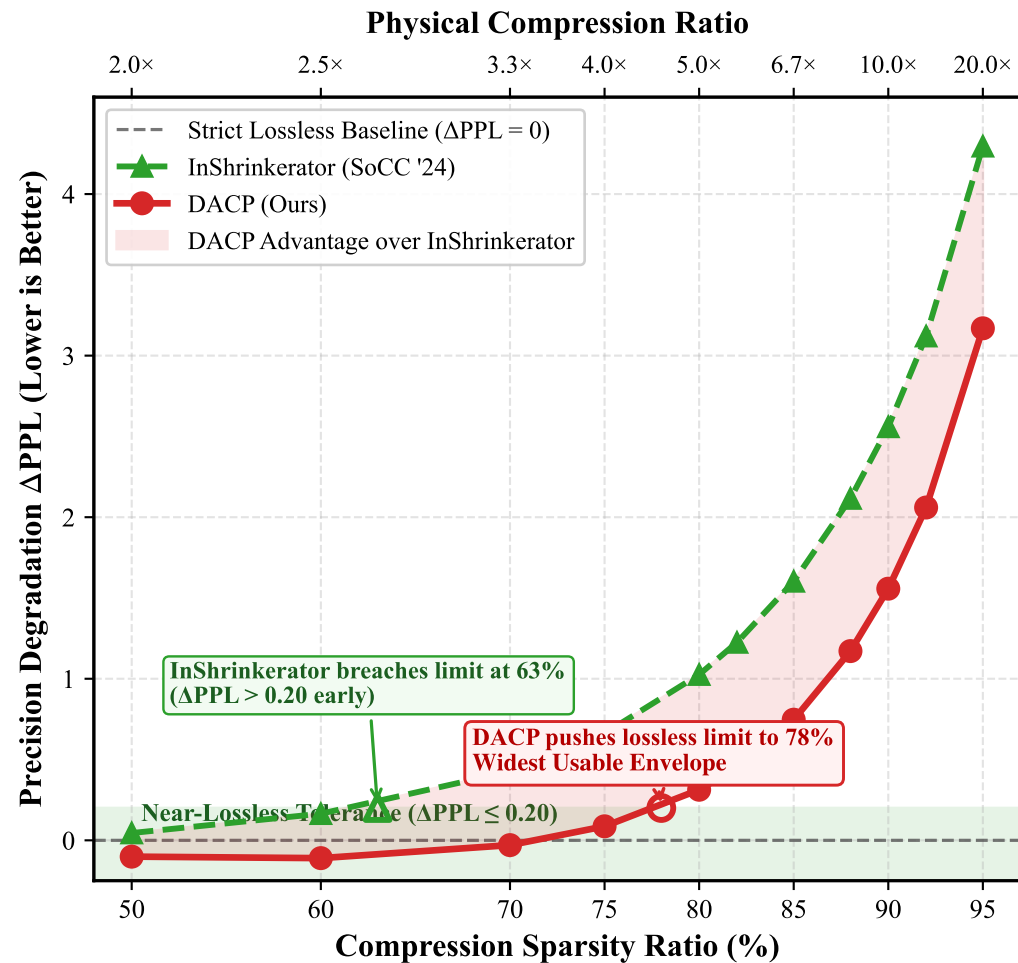