

Intake, Assessment, and Complaint Determination

Work Instruction

027-WI185

Revision R

Page 1 of 33

Medtronic

Overview

Purpose	This document describes the requirements for performing intake for potential complaints, making complaint determinations and documenting event details in complaint records.
Scope	This document applies to functions that perform complaint intake, complaint determination and completion of the complaint record.
Roles	Formally Designated Complaint Handling Unit - Operating Unit (OU) Complaint Unit - Region Complaint Unit

Table of Contents

Terms and Definitions	2
Process Overview	7
Process Detail.....	8
1. Create Record.....	8
2. Complaint Determination.....	10
3. Complete Event Details	12
4. Assign Event Coding	14
5. Event Reassessment.....	15
References.....	16
Quality Records.....	16
Appendix A – Complaint Assessment Decision Tree	17
Appendix B – Reassessment of FER Decisions for Brazil, China, Korea, and Japan	18
Appendix C – Literature Review Guidance.....	19
Section 1: Record Creation	19
Section 2: Translation Requirements.....	19
Appendix D – Non-complaint Details	19
Appendix E – Event Details for Complaint Records.....	20
Appendix F – Information for Service and Repair Events.....	22
Appendix G – Regional Privacy Laws	24
Appendix H – OEM Regulatory Reporting Responsibility Matrix	32

Terms and Definitions

Term	Definition	Source
Adverse Experience (for Drugs/Biologics)	Any adverse event associated with the use of a drug or biological (product) in humans, whether or not considered related, including the following: An adverse event occurring in the course of the use of a product in professional practice; an adverse event occurring from overdose of the product whether accidental or intentional; an adverse event occurring from abuse of the product; an adverse event occurring from withdrawal of the product; and any failure of expected pharmacological action.	Medtronic
Authorized	Authorized means having received regulatory approval for product(s) within the applicable geography for being placed on the market (e.g. released for distribution). NOTE: For events within Canada: A medical device is considered authorized when having a Medical Device Active License, a Pre- or Post-Market Investigational Testing Authorization (ITA) or approval under the Special Access Program (SAP).	Medtronic
Aware Date	The date that a Medtronic Employee/Agent acquires information that reasonably suggests that a reportable event has occurred. Aware Date may or may not be the same date as Notify Date (see definition of Notify Date below). NOTE: See 054-P044, <i>Medical Device Reporting Appendix A</i> for additional detail and examples of Aware Date vs. Notify Date.	Medtronic
Complaint	Any written, electronic, or verbal communication that alleges deficiencies related to the identity, quality, durability, reliability, safety, effectiveness, usability or performance of a product, or related to a service that affects the performance of such product*. This definition is applicable to authorized products manufactured, imported, or distributed by Medtronic. *Includes all Medical devices & accessories, cells/tissues/organs (CTO) product, HTP (Human Tissue	Medtronic

Intake, Assessment, and Complaint Determination

027-WI185

Revision R Page 3 of 33

Work Instruction

Medtronic

Term	Definition	Source
	Product), Drug, Biopharma, Combination (device and drug), in-vitro diagnostic medical devices.	
Constituent Part	Constituent part is a drug, device, or biological product that is part of a combination product.	21 CFR 4
Constituent Part Applicant	The applicant for a constituent part of a combination product the constituent parts of which are marketed under applications held by different applicants.	21 CFR 4
Cross-labeled Combination Product	A drug, device, or biological product packaged separately that according to its investigational plan or proposed labeling, is intended for use only with an approved, individually specified drug, device, or biological product where both are required to achieve the intended use, indication, or effect and, where upon approval of the proposed product, the labeling of the approved product would need to be changed or, any investigational drug, device, or biological product packaged separately that, according to its proposed labeling, is for use only with another individually specified investigational drug, device, or biological product where both are required to achieve the intended use, indication, or effect.	21 CFR 3.2(e)
Cybersecurity Signal	Any information that indicates the potential for, or confirmation of, a cybersecurity vulnerability or exploit that affects or could affect a medical device.	Medtronic
Distributor	Any person, other than the manufacturer or importer, who furthers the marketing of a device from the original place of manufacture to the person who makes final delivery or sale to the ultimate user.	21 CFR 803.3
Event Date	The date when an event occurred or was observed or identified by the user, patient, or initial reporter.	Medtronic
External Contact	A non-Medtronic source of information other than the initial reporter (or <i>complainant</i>), such as the distributor or another Medtronic agent.	Medtronic
FDA Patient Problem (FDP)	An FDA code that describes actual adverse effects on the patient that may be related to the device problem that is observed during a reported event. This code may be represented by IMDRF Annex E and/or Annex F codes.	Medtronic

Intake, Assessment, and Complaint Determination

027-WI185

Revision R

Page 4 of 33

Work Instruction

Medtronic

Term	Definition	Source
Foreign Experience Report (FER)	Report that may be required when the complaint event did not occur in a specific country, but because the product in question is registered there, that country's Regulatory Body may require a report notifying them of the complaint.	Medtronic
Harm	Physical injury or damage to the health of people, or damage to property or the environment, or breach of data or system security.	MEDDEV 2.12-1
Hazard	Potential source of harm.	ISO14971
Importer	Natural or legal person in the supply chain who is the first in a supply chain to make a medical device, manufactured in another country or jurisdiction, available in the country or jurisdiction where it is to be marketed.	ISO 13485
Initial Reporter	Any individual who initially reports the event to Medtronic, the distributor, or another Medtronic Contractor/Agent. If a Medtronic employee is the individual who first identifies the event, they would be the initial reporter.	Medtronic
Internal Contact	A Medtronic employee who provides details of the event.	Medtronic
International Medical Device Regulators Forum (IMDRF) Code	Adverse event terminology intended to facilitate the reporting of observations at the level of the medical device, its constituting components including accessories, observations of the patient (concerning patient or user health), and investigations into possible causes relating to malfunctioning of the device as well as causal links between use of the device and adverse event.	IMDRF
IMDRF Annex A – Medical Device Problem	Terms/codes for describing problems (malfunction, deterioration of function, failure) of medical devices that have occurred in pre- or post-market contexts (e.g., clinical studies, clinical evaluation, or post-market surveillance)	IMDRF

Intake, Assessment, and Complaint Determination

Work Instruction

027-WI185

Revision R

Page 5 of 33

Medtronic

Term	Definition	Source
IMDRF Annex B – Cause Investigation/ Type of Investigation	Terms/codes for describing what was investigated and what kind of investigation was conducted to specify the root cause of the adverse event.	IMDRF
IMDRF Annex C – Cause Investigation/ Investigation Findings	Terms/codes for describing the findings in the specific investigation that are the keys to identifying the root cause.	IMDRF
IMDRF Annex D – Cause Investigation/ Investigation Conclusion	Terms/codes for describing the conclusion of the device involved in the reported event.	IMDRF
IMDRF Annex E – Health Effects – Clinical Signs and Symptoms or Conditions	Terms/codes for describing the clinical signs and symptoms or conditions of the affected person appearing as a result of the medical device adverse event/incident.	IMDRF
IMDRF Annex F – Health Effects – Health Impact	Terms/codes for describing the consequences of the medical device adverse event/incident on the person affected.	IMDRF
IMDRF Annex G – Component	Terms/codes for describing the parts and components which were involved in, or affected by, the medical device adverse event/incident.	IMDRF
Medtronic Agent	An individual or entity that works on behalf of Medtronic pursuant to a contract, including distributors, independent sales or field agents, resellers, or any other forms of third-party sales or distribution representatives in both developed and emerging markets.	Medtronic
Notify Date	The date when a Medtronic Employee/Agent was initially informed of a potential complaint. Notify Date may or may not be the same as Aware Date (see Aware Date definition above). NOTE: See 054-P044, <i>Medical Device Reporting Appendix A</i> for additional detail and examples of Aware Date vs. Notify Date. NOTE: Distributors and Medtronic Agents are not considered Medtronic employees except for tissue or drug product in Europe. In those cases, distributors and	Medtronic

Intake, Assessment, and Complaint Determination

027-WI185

Revision R Page 6 of 33

Work Instruction

Medtronic

Term	Definition	Source
	Medtronic Agents are considered Medtronic employees per local and regional regulations. NOTE: This definition is synonymous with the Canada "Awareness Date".	
Original Equipment Manufacturer (OEM) Product	An external supplier of a finished device, drug, biologic, human tissue or combination product which: ▪ Owns the design and manufacture; ▪ Is designated as the Legal Manufacturer; and ▪ Owns primary regulatory responsibility. Medtronic may perform certain other regulatory actions / responsibilities (e.g., product registration and listing) in specific geographies.	Medtronic
Reason for Report (RFR)	A code that documents the product allegation, resulting in record creation.	Medtronic
Serious Injury	An injury or illness that: ▪ Is life threatening, even if temporary in nature, ▪ Results in permanent impairment of a body function or permanent damage to a body structure, or ▪ Necessitates medical or surgical intervention to preclude permanent impairment of a body function or permanent damage to a body structure. NOTE: Some regions have unique definitions of Serious Injury for reporting purposes; please refer to those definitions when making reporting decisions.	Medtronic
Service	"Service" as it relates to complaints, means activities performed by Medtronic in relation to a device which may have an effect on the identity, quality, durability, reliability, safety, effectiveness, usability or performance of a product (e.g. a device returned from service delivering out of specification).	Medtronic
Target Record	The earliest created record of a complaint event that all potential duplicate records will be merged into. Also referred to as Primary Record	Medtronic
Unique Device Identifier (UDI)	Unique Device Identifier (UDI) #: This number can be found on the device, its label, or accompanying packaging and is located below the barcode. FDA defines the UDI: UDI is composed of two parts:	Medtronic

Intake, Assessment, and Complaint Determination

027-WI185

Revision R


Page 7 of 33

Work Instruction

Medtronic

Term	Definition	Source
	- Device Identifier (DI) = GTIN - Product Identifier(s) (PI) that can include the following: - Lot Number - Serial number - Expiration Date - Date of Manufacture - Internal Product Variant (Product version number) EXAMPLE UDI: (01) 12345678901234 (17) 140102 (11) 100102 (10) A1234 (21) 1234	

Process Overview



- Potential Complaints

- Record Creation
- Complaint Processing

The Formally Designated Complaint Handling Unit is responsible for intake, assessment, and complaint determination, as defined below.

Complaint Unit	Responsibilities
Formally Designated Complaint Handling Unit	- Make the complaint determination. - Complete the event narrative and coding. - Perform a review for minimum information/event details. - For information entered into the complaint handling system through an automated interface, perform initial source review. - Determine the correct number of complaint records to be created per event. For instances when complaints do not interface directly to the complaint handling system, ensure sources are monitored routinely to ensure timely intake of potential complaint information.
Region Complaint Unit	Ensure translation of record information as necessary per regulatory requirements. For information received through a manual source (e.g., phone call, letter or e-mail), perform initial source document review and ensure timely creation of the complaint record in the complaint handling system to document the potential complaint.

Intake, Assessment, and Complaint Determination

027-WI185

Revision R Page 8 of 33

Work Instruction

Medtronic

NOTE: If the Region does not have access to the complaint handling system, then the Region will forward the complaint immediately to the Complaint Unit for complaint record creation.

Process Detail

1. Create Record

Step	Role	Action
1.	Formally Designated Complaint Handling Unit	Review to ensure the complaint has been assigned to the correct Complaint Handling Unit (Operating Unit). If it was incorrectly assigned, escalate to the correct team by utilizing D01111998, <i>Complaint Contact List</i> to identify the appropriate complaint handling unit team contact.
2.		Review to determine if there is an existing record for the event. ▪ If a record already exists for the event, merge the new information into the existing record, as applicable. When unable to merge, ensure that the oldest record is maintained where possible, with relevant cross-references and associated records closed per local processes. – The existing record becomes the Target Record, and its associated creation dates are unchanged. The Notified Date should reflect the earliest date of the associated records. – If the additional information includes details that warrant creation of a new and separate event in addition to merging into the Target Record, create a new record. – Refer to 054-P044, <i>Medical Device Reporting and Appendix B Reassessment of FER Decisions for Brazil, China, Korea and Japan</i>, for requirements on reassessing new details for reportability including evaluating the Aware Date. ▪ If a record does not already exist, create record(s). – Record(s) should be created for each unique event noted in the potential complaint. All products involved in that event should be included in that record. NOTE: If additional related information is received belonging to an existing record, but occurred in a different country,

Intake, Assessment, and Complaint Determination

Work Instruction

027-WI185

Revision R

Page 9 of 33

Medtronic

		capture the new information in the same record with a reportability decision specific to the new country. – If there was patient involvement, a unique record should be created for each patient involved and for each event, e.g., if a potential complaint notes several patients individually to have unique events, each patient would warrant a separate record. – For Literature, see Appendix C <i>Literature Review Guidance</i>. – If the information does not include enough detail regarding individual patients, e.g., “several patients experienced this”, a single record may suffice. ▪ If it is unclear whether a potential complaint is a duplicate or if the event should be split into multiple records, the complaint record(s) should be created based on information available, and initiate follow up communication to obtain required information per 027-WI188, <i>Customer Communication</i>.
3.		Document each product that is involved in a potential complaint to allow for individual complaint determination, regulatory decision documentation, and/or investigation determination. ▪ For cross-labeled combination product, continue to step 4. ▪ Identify and document any Original Equipment Manufacturer (OEM) products. For OEM products identified, continue to step 5. – OEM products may be identified by referring to master data. – For events occurring in Mainland China, refer to D01506786 <i>China OEM Product List (License Holder is Not MDT but MDT China is Agent)</i>. – For all other products, skip to next section.
4.		For cross-labeled combination products only: ▪ Document details about the drug that is associated with the event. ▪ Determine whether information needs to be sent to a Constituent Part Applicant and document the decision. Information needs to be sent to a Constituent Part Applicant if both of the following items are true: – The event is associated with the Constituent Part Applicant’s product.

Intake, Assessment, and Complaint Determination

Work Instruction

027-WI185

Revision R Page 10 of 33

Medtronic

		– Either the event involves a death or Serious Injury related to the device or the event involves an Adverse Experience (regardless of relatedness to the device). ▪ Send the information, when required, to the Constituent Part Applicant within 5 calendar days of the notify date in accordance with 027-WI188.
5.		For OEM products: ▪ Identify complaint handling responsibilities assigned to Medtronic. Contact Supplier Quality if assistance is needed with this determination. ▪ Refer to Appendix H - <i>OEM Regulatory Reporting Responsibility Matrix</i> to determine if regulatory reporting of OEM product complaints is applicable to Medtronic. Consult Regulatory Affairs and Supplier Quality as needed to determine whether Medtronic holds a role listed in the Appendix. – If Medtronic reporting responsibility is applicable per Appendix H, proceed to Section 2 to make the complaint determination. – If reporting is not applicable per Appendix H, and Medtronic has no complaint handling responsibilities per the Supplier Quality Agreement, the record may be closed after notifying the OEM of the event per Section 2 Step 5 below.

2. Complaint Determination

Step	Role	Action
1.	Formally Designated Complaint Handling Unit	Evaluate each potential complaint using the complaint-assessment decision tree in Appendix A, or per an existing quality agreement that contains complaint-handling responsibilities. ▪ If information is needed to make the complaint determination (e.g., the manufacturer is unknown, initial information is vague/contradictory, reason for product return is unclear or product is returned with no allegation) initiate follow-up in accordance with 027-WI188. ▪ If an issue is identified prior to distributing the product or component, (e.g., issue identified at a Medtronic distribution or technical service center during Pre-Delivery

Intake, Assessment, and Complaint Determination

Work Instruction

027-WI185

Revision R

Page 11 of 33

Medtronic

Step	Role	Action
		Inspection), the information does not meet the definition of a complaint. ▪ If the potential complaint was received from China's National Medical Device Adverse Events Monitoring Information System and the external complaint source is Regulatory Body, it is understood that the Chinese Regulatory Authority deemed the issue as an adverse event requiring investigation. Document the event as a complaint.
2.		Review the event to determine if the report received concerns a Medtronic Single Use Device (SUD). If event information suggests the SUD has been reprocessed or re-sterilized and reused with a patient: • Create an additional event record. • Request any additional information needed to confirm the report, including if a third party performed the re-processing or re-sterilization of the SUD in order to reuse with a patient. • If the complaint received on the SUD is confirmed to be re-sterilized or reprocessed by a third party for use in humans, the device is then considered a non-Medtronic device. Follow process in 027-WI188 <i>Customer Communications</i> for communicating non-Medtronic complaints.
3.		Review the event to determine if additional actions are needed or if escalation is required. Potential examples include, but are not limited to: – Potential Serious Public Health Threat (SPHT): If a complaint indicates a potential threat to public health, escalate immediately to management via e-mail to dl.CQExtendedLeaders@medtronic.com. Reference 027-P428, <i>Submitting Potential Complaints</i> for examples of complaints that may potentially indicate a SPHT. – Cybersecurity: If the complaint indicates a potential Cybersecurity Signal, evaluate need for a cybersecurity assessment per 027-WI186, <i>Complaint Investigation</i> – Patient Death: If a patient death is reported, ensure timely reportability decisions are made per 054-P044 and any technical assessments required per 027-WI186 are initiated.

Intake, Assessment, and Complaint Determination

027-WI185

Revision R

Page 12 of 33

Work Instruction

Medtronic

Step	Role	Action
		– Potential Manufacturing Issue: If the complaint indicates a potential manufacturing issue, initiate technical assessments per 027-WI186. – Non-Medtronic Device: If the information indicates a potential complaint regarding a device Medtronic did <i>not</i> manufacture, and the information was received in error, refer to 027-WI188 for notification requirements. – 5-day Reporting: Escalate immediately to management. – Potential Field Alert Reports: Escalate immediately to management. Reference D00788855 Field Alert Report (FAR) for specific examples.
4.		Document the complaint determination. ▪ If the information is determined to not meet the definition of a complaint: – Populate or confirm that information is present in the complaint-handling system in accordance with Appendix D, <i>Non-complaint Details</i>. – Close the record.
5		Notify other parties as needed about the complaint. Notification is required in the following situations: ▪ If Medtronic is the Manufacturer of the product, but is not the Distributor of the product, notify the Distributor of the complaint. ▪ If Medtronic is <i>not</i> the manufacturer but has an agreement with the OEM, notify the OEM per 027-WI188.

3. Complete Event Details

Step	Role	Action
1.	Formally Designated Complaint Handling Unit	If the event is a complaint, review pre-populated basic event information as defined in Appendix E, <i>Event Details for Complaint Records</i> and complete as necessary.
2.		Ensure the Device Problem or Failure Mode, as well as any impact to the patient, is understood and reflected in the complaint record. This information may be critical to ensuring a timely regulatory reporting decision. If this information is unknown, escalate for follow-up in accordance with 027-WI188.
3.		Review to ensure that in each complaint record, the Event Narrative, or Description Summary:

Intake, Assessment, and Complaint Determination

Work Instruction

027-WI185

Revision R

Page 13 of 33

Medtronic

Step	Role	Action
		- Summarizes the reporter's allegation, in their own words - Contains a chronological description of the event - Includes objective information and allegations from the report source or information obtained during follow-up. The narrative does not include Medtronic speculations about the event. - Does not contain duplicative text (e.g., when additional information is received, ensure that previously reported information is not repeated). NOTES: - Event Narrative information may be pre-populated, but when applicable, information should be manually entered to include all relevant details. - For additional information about Event Narratives, refer to Appendix E, <i>Event Details for Complaint Records</i> and Appendix F, <i>Information for Service and Repair Events</i>.
4.		Include relevant medical history and relevant tests/laboratory data as available. Refer to Appendix E for further guidance about what information may be considered relevant information to include. NOTE: When available, applicable supporting materials (medical records, films, etc.) should be attached to the complaint record.
5.		Confirm that the UDI field in each complaint record contains the Unique Device Identifier (UDI) from all involved devices. If the UDI is not pre-populated in the field, check that the SN/Lot is valid. If the SN/Lot is not available, follow the instructions in Appendix E and 027-WI188 to determine follow-up required. For Global Complaint Handling system users: once the SN/Lot is confirmed valid then copy and delete SN/Lot, save twice, re-enter SN/Lot and save.
6.		Populate or confirm that information is present in the complaint handling system in accordance with Appendix E. Request any additional information needed per 027-WI188.
7.		Review the event to determine if additional actions are needed. Potential examples include, but are not limited to: Service & Repair Event: If the complaint refers to a Service & Repair event, initiate the follow-up based on Appendix F. Clinical Study: If a complaint record originates from a Clinical Study and requests for additional information are

Intake, Assessment, and Complaint Determination

027-WI185

Revision R

Page 14 of 33

Work Instruction

Medtronic

Step	Role	Action
		being facilitated through the Clinical Study Team, refer to 027-WI188 for additional information on Good Faith Effort (GFE). ▪ Legal: If the complaint relates to an event involved in litigation or other type of legal proceeding, or includes mention of a lawyer being involved, document that information in the complaint record and forward the information to the Medtronic Legal Team for awareness.

4. Assign Event Coding

NOTE: For specifics related to code application, refer to local coding tools/documents.

Step	Role	Action
1.	Formally Designated Complaint Handling Unit	Add the Reason for Report (RFR) code(s) to each product as reported by the complainant NOTE: ▪ The codes are assigned on an as-reported basis. Confirm any pre-populated codes to ensure they match the reported complaint(s). ▪ Subsequent results of analysis do not change the assignment of RFR codes. ▪ If no product allegation is reported, the RFR code field still must be populated. If there is no applicable RFR code, follow the process outlined in D01045331, <i>Complaint Codes Governance and Maintenance</i>. If the cause has not yet been determined, select the primary code based on the initiating factor of the event.
2.		Add the FDA Patient Problem (FDP) code or Harm code to each complaint record. These code(s) may be represented by IMDRF Annex E and/or Annex F codes. NOTE: Select the primary code based on most severe harm.
3.		Add the International Medical Device Regulators Forum (IMDRF) codes, when applicable, using the most detailed code that is possible within each IMDRF code type (e.g., Annex A code, Annex B code). NOTE: When more than one code per type is available, select a primary code for each code type.

Intake, Assessment, and Complaint Determination

Work Instruction

027-WI185

Revision R Page 15 of 33

Medtronic

4.		If applicable, add Hazard codes. NOTE: Multiple hazard codes may be needed if multiple hazardous situations occurred.
5.		If applicable, add any additional code types required per local processes.

5. Event Reassessment

Step	Role	Action
1.	Formally Designated Complaint Handling Unit	Upon receipt of any new information, including completed analysis/investigation, review and update record as needed. If changes are required document the changes accordingly in the complaint file. Potential updates may include but are not limited to: ▪ Reassessing complaint decisions ▪ Updating the event description ▪ Updating coding ▪ Updating product information ▪ Reassessing reportability decision(s) or need for an additional regulatory report – Refer to 054-P044 for information on reassessing new details for reportability, including evaluating the aware date. ▪ Re-opening the investigation. ▪ Re-opening previously completed technical assessment tasks (if needed) per 027-WI186.
2.		After a region has completed their initial reporting decision (RD) as per 054-P044, if there are changes in the complaint information that may influence the RD or regulatory report (RR), ensure the regions with a completed initial RD are notified in a timely manner. This also applies to Foreign Experience Reporting (FER) RDs/RRs, see notes below. Complaint information that may require notification to the region includes but is not limited to: ▪ Patient outcome or patient involvement ▪ Device/supplier analysis (if region is not automatically notified) ▪ Product involvement, or a change to which products are involved

Intake, Assessment, and Complaint Determination

027-WI185

Revision R

Page 16 of 33

Work Instruction

Medtronic

Step	Role	Action
		▪ Forgery information (Brazil only) NOTES: ▪ Refer to Appendix B for additional information on reassessing FER decisions. ▪ Region notifications may require manual notification to ensure that re-assessment is completed when complaint details are changed (e.g., if information is received via the communication task in the complaint system, a manual reassess task for the region may be required). ▪ Update the FER or notify the region when the need for the update/notification is identified, even if the complaint investigation has not been re-closed.


References

Number	Title
027-P428	Submitting Potential Complaints
027-WI186	Complaint Investigation
027-WI188	Customer Communication
054-P044	Medical Device Reporting
054-WI198	Medical Device Reporting Decision and Regulatory Reporting - United States
D01045331	Complaint Codes Governance and Maintenance
D01111998	Complaint Contact List
D00788855	Field Alert Report (FAR)
D01506786	China OEM Product List


Quality Records

Quality Record	Required Approvals
Complaint Record	None

Appendix A – Complaint Assessment Decision Tree

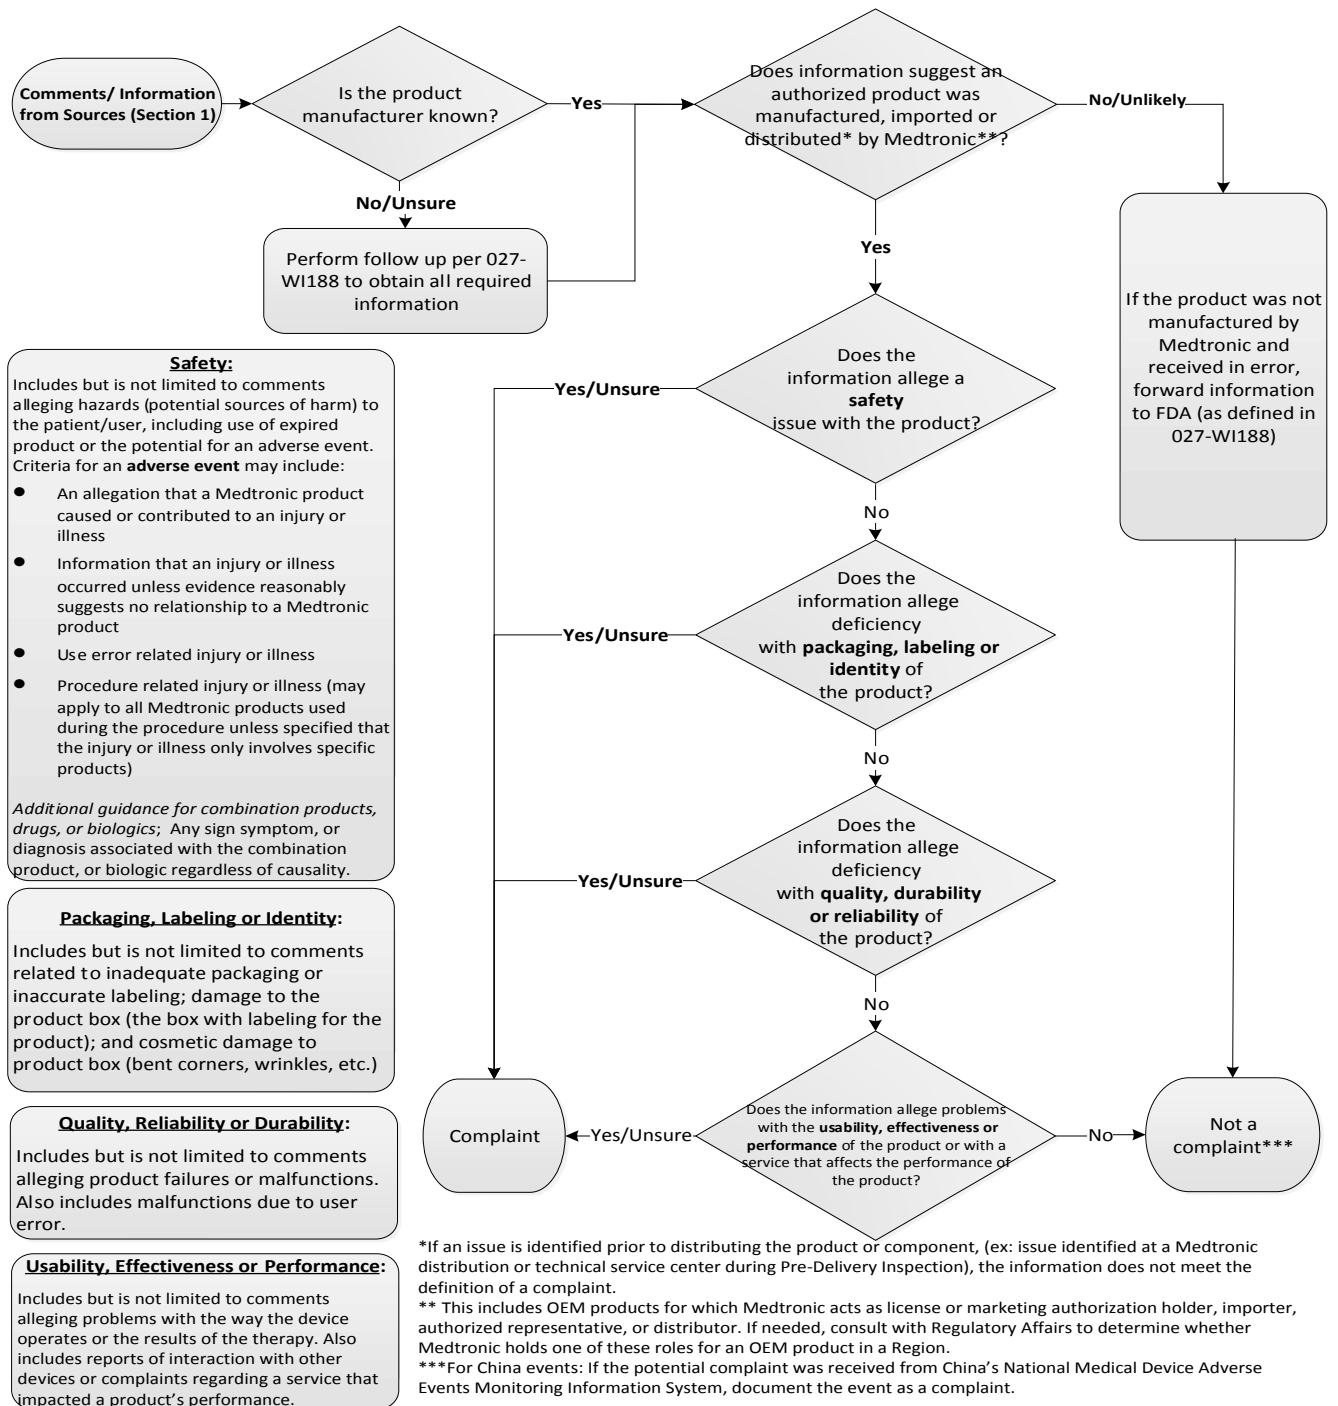

Appendix B – Reassessment of FER Decisions for Brazil, China, Korea, and Japan

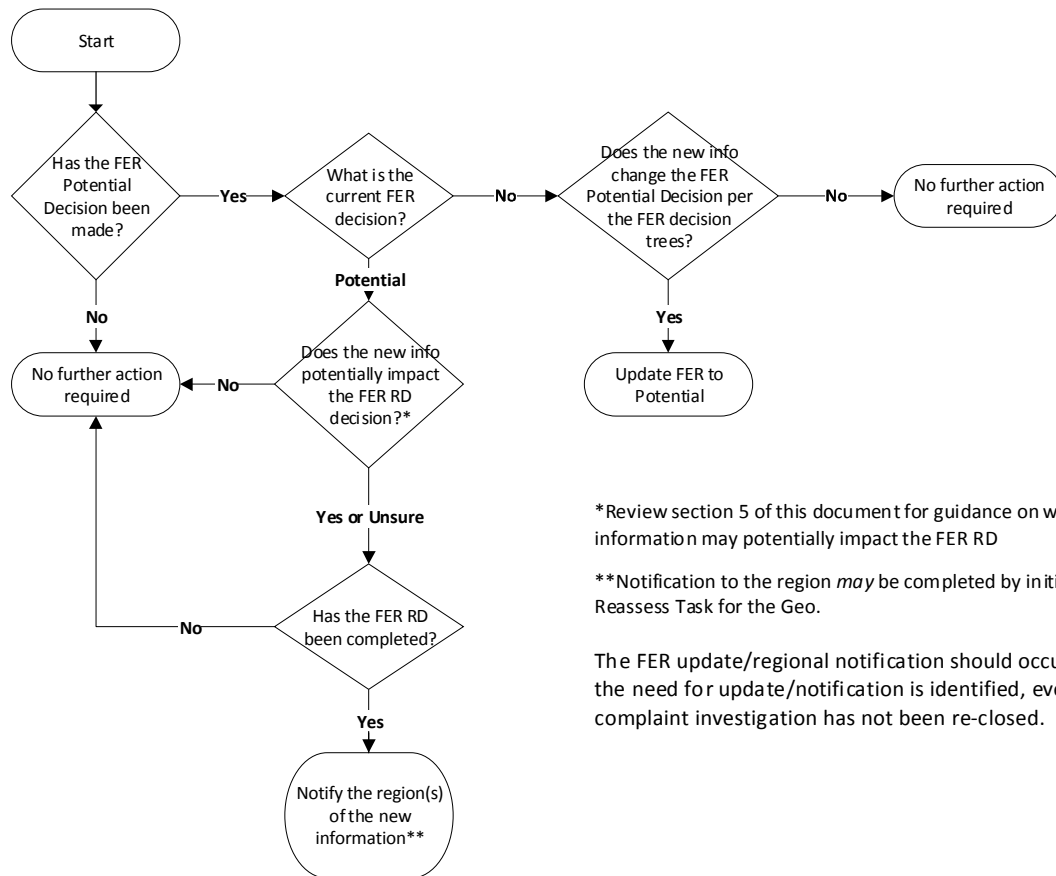

Appendix C – Literature Review Guidance

Section 1: Record Creation

For each patient/device mentioned, determine whether the patient/device is uniquely identified:

- Unique patient or device identifiers include but are not limited to name, initials, date of birth, clinical ID, serial number.
- Non-unique patient or device identifiers include but are not limited to age, weight, gender, lot number, model number, and device type.

Create the necessary number of records and/or reports according to the following rules:

- Non-unique patient or device identifiers: Create one record. Contact the author of the literature source, and request information as needed per 027-WI188 to obtain unique identifiers. If unique identifiers are provided, then continue to the unique identifier section below.
 - Create a line item in the event for each device or product family.
 - Create a line item for each event type to make the appropriate RD for each type of event reported. Potential event types include but are not limited to: death, serious injury or serious deterioration in the state of health or serious adverse event, malfunction, non-serious injury/illness.
- Unique patient or device identifiers: Create a new record for each uniquely identified patient or device with an associated allegation.

Section 2: Translation Requirements

Follow these rules for literature articles in languages other than English:

- If the literature article is noted as a listing in a search or in a bibliography:
 - Translation is not required if both the article and abstract are not in English, complaint determination should be made with information available at time of review; however
 - If the article is not in English, but the abstract is in English, then the abstract is evaluated for complaint information. If a potential complaint exists, then the article must be translated for evaluation, or the event is based solely on the abstract.
- If the Complaint Handling Unit receives literature submitted by a Medtronic employee in a language other than English (partly or entirely), the literature should be translated into English and assessed for a complaint. If a complaint is found, the literature should be routed for regulatory reporting review.

Appendix D – Non-complaint Details

The following information must be documented in the non-complaint record.

Non-complaint Details

- **Country:** Country where the event occurred.
- **Notified Date**
- **Brief Description – (if provided)**

- **Product Identifiers:** If the serial or lot number is unavailable, then enter the product, model, or catalog number, if known.
- **Non-complaint Rationale**
- **Is a Customer Response requested?**

Appendix E – Event Details for Complaint Records

As allowed by data-privacy regulations (refer to Appendix G, *Regional Privacy Laws*), document the following information in the complaint record when it is available to Medtronic. If information is marked with an * below and it is not in the complaint record, perform Good Faith Effort activities per 027-WI188.

NOTE: Refer to the applicable regional Work Instruction to complete the reporting decision and to determine if additional information is required for the event (based on specific regional requirements).

Example: Complaints that are reportable to the US FDA require additional information as defined in 054-WI198, *Medical Device Reporting Decision and Regulatory Reporting - United States*.

Information for Complaint Record

- **Product Identifiers*:**
 - Unique Device Identifier (UDI) and Serial or Lot Number
 - If the serial or lot number is not available, then enter the product, model, or catalog number, if known.
- **Software Version (*required when the version is potentially relevant to the reported event)**
- **Country*:** Country where the event occurred
- **Event Date***
- **Notified Date***
- **Initial Reporter*:** Name, address, and phone number (as allowed by data-privacy regulations)
- **Product Return Status*:**
 - Is there intent to return product?
 - Provide rationale for no return of product
 - If received, record the date that product was received by Medtronic Analysis Site
- **Customer Response:** Was a response requested by the Initial Reporter?
- **Relevant Patient Information:** Collect relevant patient information at intake as allowed by privacy laws.

Information Regarding Event

- **Event Narrative:** May include, but is not limited to:
 - Medical status prior to the event
 - Event context/when the issued occurred* (ex: prior to use, during use, post procedure)
 - Type of procedure
 - If the device was used for treatment or diagnosis

Intake, Assessment, and Complaint Determination

Work Instruction

027-WI185

Revision R

Page 21 of 33

Medtronic

- The alleged issue (patient and/or product problem) *
- Clinical signs and/or symptoms
- Differential diagnosis for the event
- Clinical course and treatment (including imaging involved, device revision/ replacement/ reprogramming, hospitalization, medication, resolution of event)
- Impact to the patient and/or user*
- Patient outcome due to the event*
- Potential contributing factors to the event
- Product use or patient specific information that may have caused or contributed to the reported or alleged event
- **Relevant Tests/Laboratory Data:** May include:
 - Clinical and laboratory tests and their results, and laboratory data used to investigate/diagnose the event or to determine device relationship to the reported event.
 - Potential examples of relevant laboratory tests and exams and their results: cultures and dates collected, blood counts and dates collected, blood glucose results, or echocardiograms, etc.
- **Relevant History:**
 - Relevant medical history including current and pre-existing conditions that may be related to the event or need for medical device.
 - Potential examples of relevant history:
 - hypertension, diabetes, renal/hepatic dysfunction, recent infection, allergies, pregnancy history, smoking/alcohol use, drug abuse, etc.

NOTE: If tests, lab data, or relevant history are embedded in the event narrative it is not required to repeat that information in other separate sections of the file. However, raw data or extensive lists should be placed in separate designated sections of the file (where available).

Adverse Drug Experience:

All complaint records that involve either co-packaged or single-entity combination products or a product that is approved as a drug must be assessed for the presence of the following information, if death and/or symptoms are reported. If any of the information is not in the complaint record, perform Good Faith Effort activities per 027-WI188.

- Name(s) of Drug(s) at the time of the event
- Concentration
- Dose
- Frequency
- Route
- Therapy Dates: Start and/or stop dates
- Diagnosis for use
- Concomitant other drugs

- Relevant medical history (see Appendix E)

Source-Specific Required Information

All complaint records that involve one or more of the sources identified below must include each item listed per source, if available.

- **Literature**
 - Literature Author(s)
 - Title of Article
 - Journal Name
 - Issue Number
 - Year Published
 - Citation or Reference (ex: WEBSITE.PMID#.PAGES.)
- **Service and Repair** (see Appendix F)
- **Social Media / News**
 - Name of Media Source
 - Author Name or User Identification
 - Date Posted
- **Clinical:** Applicable to clinical studies involving any products or components that are market approved anywhere in the world.
 - Study Name
 - Device, Procedure, and Drug Relatedness (if applicable)
 - Patient Clinical ID

Appendix F – Information for Service and Repair Events

For a complaint that is initiated from service and repair events, include the information below. If the information below is not available, perform Good Faith Effort activities per 027-WI188.

- **Event Narrative:** Provide information regarding the event with as much detail as is known at the time of the report. For example: What occurred; what is the reason for the call and/or device return; was the service or repair performed as a part of routine service or was it in response to a service call?
- **Alleged Issue:** Why is the product alleged to be defective or returned? Document information about what is not working or what alerted the user that it was not working as expected. For example, when was the issue found (during use at customer site, during use [including demo or training], during routine service, or during predelivery inspection)?
- **Additional Product information:** Serial, lot, model, or catalog number, quantity of products impacted, and prioritization of record (if applicable). If serial or lot number is not available, then enter the model or catalog number, if known. This includes any additional products (whether reportable or not) that may have contributed to the event.
- **Service Record Number**
- **Country**

Intake, Assessment, and Complaint Determination

027-WI185

Revision R

Page 23 of 33

Work Instruction

Medtronic

- **Event Date:** If unknown, use the date the service or repair was requested.
- **Device Return or Replacement Status:**
 - Has the device been returned? If not, will it be returned? Include tracking information, if applicable.
 - Has the device been replaced? If so, provide replacement device information.
 - NOTE: If the technician already completed all testing on a device during servicing that would be completed at the analysis center, then Good Faith Effort (GFE) for device return is not needed. See 027-WI188.
- **Initial Reporter**
- **Patient Impact:**
 - When did the event occur (e.g., during planned maintenance, device check, prior to use on a patient)? If unknown, explain the situation or when or how it was triggered for service (for example, premature failure).
 - Were there any patient complications or issues as a result of the event?
 - If yes, what was the patient outcome?
 - What action or mitigation step was taken (e.g., device replaced, same device was used to complete the case, worked fine after long boot)?
- **Customer Response:** Is a response requested by the customer? (The service record provided to the customer at the time of the repair may serve as the customer response.)
- **External Contact (if applicable)**
- **Internal Contact (if applicable)**

Document the following items in the complaint record upon receipt of the product:

- Any additional information that is received with returned product (including documents).
- Date of product receipt

Appendix G – Regional Privacy Laws

The tables below represent how data in our complaint handling system can be processed in accordance with regional privacy laws. This is not a comprehensive list, and the complaint handling specialist should consult with the Global Data Privacy Office regarding a specific region's privacy laws if there is a question on data.

EMEA (Europe, Midde East and Africa):

EMEA/Israel				
Field (patient info)	Can be documented in Complaint System?	Follow-up for missing information allowed?	Include in any regulatory reports?	Supporting Regulation
Name	No**	No**	No	EMEA ■ Articles 109 and 110 of the EU MDR 201/745 ■ Article 110 of MDR Directive 95/46/EC ■ Regulation (EC) No 45/2001 ■ GDPR 2016/679 Israel ■ Israel Privacy Protection Law, 5571-1981 ■ Israel Patient's Rights Law, 5756-1996 ■ MOH General Director Circular No. 1/2018 - Secondary uses of health information
Initials	No**	No**	No	
Date of Birth	No	No	No	
Age (in years)	Yes	Yes	Yes	
Gender/Sex	Yes	Yes	Yes	
Weight	Yes	Yes	Yes	
Medical History	Yes*	Yes*	Yes*	
Contact Info (phone/address)	No**	No**	No	
Ethnicity & Race	No	No	No	N/A

*To the extent that the individual is not identifiable, unless the individual is the initial reporter.

** The initial reporter's contact information shall be documented within the system, and follow-up for additional information is permissible.

Intake, Assessment, and Complaint Determination

027-WI185

Revision R

Page 25 of 33

Work Instruction

Medtronic

Canada:

Canada				
Field (patient info)	Can be documented in Complaint System?	Follow-up for missing information allowed?	Include in any regulatory reports?	Supporting Regulation
Name	No	No	No	Personal Information Protection and Electronic Documents Act PIPEDA s.7(3) (c.1)
Initials	No	No	No	
Date of Birth	No	No	No	
Age (in years)	No	No	No	
Gender/Sex	No	No	No	
Weight	No	No	No	
Medical History	Yes *	Yes *	Yes *	
Contact Info (phone/address)	No	No	No	
Ethnicity & Race	No	No	No	

**To the extent that an individual is not identifiable.*

Greater China:

Mainland China				
Field (patient info)	Can be documented in Complaint System?	Follow-up for missing information allowed?	Include in any regulatory reports?	Supporting Regulation
Name	No	No	No	Personal Information Protection Law
Initials	No	No	No	
Date of Birth	No	No	No	
Age (in years)	Yes	Yes	Yes	
Gender/Sex	Yes	Yes	Yes	
Weight	Yes	Yes	Yes	

Intake, Assessment, and Complaint Determination

027-WI185

Revision R

Page 26 of 33

Work Instruction

Medtronic

Mainland China

Field (patient info)	Can be documented in Complaint System?	Follow-up for missing information allowed?	Include in any regulatory reports?	Supporting Regulation
Medical History	Yes	Yes	Yes	
Contact Info (phone/address)	No	No	No	
Ethnicity & Race	No	No	No	

Hong Kong

Field (patient info)	Can be documented in Complaint System?	Follow-up for missing information allowed?	Include in any regulatory reports?	Supporting Regulation
Name	Yes	Yes	Yes	Personal Data (Privacy) Ordinance CAP 486 Guidance Notes for Adverse Event Reporting by Local Responsible Persons GN-03
Initials	Yes	Yes	Yes	
Date of Birth	Yes	Yes	Yes	
Age (in years)	Yes	Yes	Yes	
Gender/Sex	Yes	Yes	Yes	
Weight	Yes	Yes	Yes	
Medical History	Yes	Yes	Yes	
Contact Info (phone/address)	No	No	No	
Ethnicity & Race	Yes	Yes	Yes	

Taiwan

Field (patient info)	Can be documented in Complaint System?	Follow-up for missing information allowed?	Include in any regulatory reports?	Supporting Regulation
Name	Yes	Yes	Yes	

Intake, Assessment, and Complaint Determination

027-WI185

Revision R

Page 27 of 33

Work Instruction

Medtronic

Taiwan				
Field (patient info)	Can be documented in Complaint System?	Follow-up for missing information allowed?	Include in any regulatory reports?	Supporting Regulation
Initials	Yes	Yes	Yes	- Personal Data Protection Act - Regulations for Reporting Serious Adverse Events of Medical Device - Regulations for Management of Medical Device Safety Surveillance
Date of Birth	Yes	Yes	Yes	
Age (in years)	Yes	Yes	Yes	
Gender/Sex	Yes	Yes	Yes	
Weight	Yes	Yes	Yes	
Medical History	Yes	Yes	Yes	
Contact Info (phone/address)	No	No	No	
Ethnicity & Race	Yes	Yes	Yes	

APAC Region:

Australia and New Zealand				
Field (patient info)	Can be documented in Complaint System?	Follow-up for missing information allowed?	Include in any regulatory reports?	Supporting Regulation
Name	No	No	No	Australia - Australian Privacy Principle 6 - Section 16B(2)(a) of the Privacy Act 1988 (Cth) New Zealand - Information Privacy Principle 3 - Information Privacy Principle 10 - Information Privacy Principle 11
Initials	No	No	No	
Date of Birth	No	No	No	
Age (in years)	No	No	No	
Gender/Sex	Yes	Yes	Yes	
Weight	Yes	Yes	Yes	
Medical History	No	No	No	

Intake, Assessment, and Complaint Determination

027-WI185

Revision R

Page 28 of 33

Work Instruction

Medtronic

Australia and New Zealand

Contact Info (phone/address)	No	No	No	- Information Privacy Principle 12 - Privacy Act 2020 (NZ)
Ethnicity & Race	Yes	Yes	Yes	

Japan

Field (patient info)	Can be documented in Complaint System?	Follow-up for missing information allowed?	Include in any regulatory reports?	Supporting Regulation
Name	No	No	No	Act on the Protection of Personal Information Law number: Act No. 57 of 2003
Initials	Yes	No	No^	
Date of Birth	No	No	No	
Age (in years)	Yes	No	No^	
Gender/Sex	Yes	No	No^	
Weight	Yes	No	No^	
Medical History	Yes	Yes*	Yes*	
Contact Info (phone/address)	No	No	No	
Ethnicity & Race	No	No	No	

^Information is only permitted in Japan regulatory reports.

*To the extent that an individual is not identifiable.

South Korea

Field (patient info)	Can be documented in Complaint System?	Follow-up for missing information allowed?	Include in any regulatory reports?	Supporting Regulation
Name	Yes	Yes	Yes	
Initials	Yes	Yes	Yes	

Intake, Assessment, and Complaint Determination

027-WI185

Revision R

Page 29 of 33

Work Instruction

Medtronic

South Korea				
Field (patient info)	Can be documented in Complaint System?	Follow-up for missing information allowed?	Include in any regulatory reports?	Supporting Regulation
Date of Birth	Yes	Yes	Yes	PERSONAL INFORMATION PROTECTION ACT [Act No.16930, 04. Feb, 2020]
Age (in years)	Yes	Yes	Yes	
Gender/Sex	Yes	Yes	Yes	
Weight	No	No	No	
Medical History	Yes	Yes	Yes	
Contact Info (phone/address)	No	No	No	
Ethnicity & Race	No	No	No	

India				
Field (patient info)	Can be documented in Complaint System?	Follow-up for missing information allowed?	Include in any regulatory reports?	Supporting Regulation
Name	No**	No**	No**	Information Technology Act 2000 The Information Technology Act 2000 and Information Technology (Reasonable security practices and procedures and sensitive personal data or information) Rules, 2011 CERT-In Cyber Security Guidelines 2022.
Initials	No**	No**	No**	
Date of Birth	No**	No**	No**	
Age (in years)	Yes	Yes	Yes	
Gender/Sex	Yes	Yes	Yes	
Weight	Yes	Yes	Yes	
Medical History	No**	No**	No**	
Contact Info (phone/address)	No**	No**	No**	
Ethnicity & Race	No**	No**	No**	

Intake, Assessment, and Complaint Determination

027-WI185

Revision R

Page 30 of 33

Work Instruction

Medtronic

***Restricted unless patient consent is received.*

Singapore, Malaysia, Thailand, Vietnam, Indonesia, the Philippines, Brunei, Myanmar, Cambodia, and Laos				
Field (patient info)	Can be documented in Complaint System?	Follow-up for missing information allowed?	Include in any regulatory reports?	Supporting Regulation
Name	No^^	No^^	No^^	Singapore: Personal Data Protection Act 2012 Malaysia: Personal Data Protection Act 2010 Thailand: Personal Data Protection Act 2019 Vietnam: The data protection provisions can be found across laws such as the LCIS, Cybersecurity Law, and Law No. 59/2010QH12 of 17 November 2010 on Protection of Consumers' Rights. Indonesia: Law No. 11 of 2008 on Electronic Information and Transactions, as amended by Law No. 19 of 2016 on the Amendment to Law No. 11 of 2008 on Electronic Information and Transactions provides certain data privacy rights. Philippines: The Data Privacy Act of 2012 Brunei/Myanmar/Cambodia: No specific data protection legislation has been adopted Laos: The Electronic Data Protection Act 2017
Initials	No^^	No^^	No^^	
Date of Birth	No^^	No^^	No^^	
Age (in years)	Yes	Yes	Yes	
Gender/Sex	Yes	Yes	Yes	
Weight	Yes	Yes	Yes	
Medical History	No^^	No^^	No^^	
Contact Info (phone/address)	No^^	No^^	No^^	
Ethnicity & Race	No^^	No^^	No^^	

^^Restricted unless patient consent is received. As per local data minimization principle, only record patient identifiable information where necessary to perform complaint handling functions.

Intake, Assessment, and Complaint Determination

Work Instruction

027-WI185

Revision R

Page 31 of 33

Medtronic

LATAM Region:

LATAM (Latin America)				
Field (patient info)	Can be documented in Complaint System?	Follow-up for missing information allowed?	Include in any regulatory reports?	Supporting Regulation
Name	Yes	No	No	Peru. Law NO.29733 personal data protection Law Chile. Law No. 19628 private life data protection law Mex. Personal Data Protection on Individuals hands Law Argentina. Law No. 25326 Public information access supplemented by decree 1558/01 Uruguay. Law No. 18331 Public Information Access Panama. Law 68 Data Privacy Law Colombia. Decree 1377 published on 2013 law 1581 published on 2012 Brazil. Law 13709 Personal Data disposition
Initials	Yes	Yes	Yes	
Date of Birth	Yes	No***	No***	
Age (in years)	Yes	Yes	Yes	
Gender/Sex	Yes	Yes	Yes	
Weight	Yes	Yes	Yes	
Medical History	Yes	No***	No***	
Contact Info (phone/address)	Yes	No***	No***	
Ethnicity & Race	Yes	No***	No***	

***Restricted unless patient consent is received. If patient consent is received manually populate in the RR.

Appendix H – OEM Regulatory Reporting Responsibility Matrix

This appendix contains a list of countries and the roles responsible for regulatory reporting of complaints in those countries. If Medtronic holds one of these roles for an OEM product in these countries, Medtronic will have regulatory reporting responsibility. Consult Regulatory Affairs and Supplier Quality as needed to determine whether Medtronic holds these roles for a given OEM product in the countries listed.

Countries	Roles				
	Authorized / Legal Representative	Distributor	Importer	License Holder / Marketing Authorization Holder (MAH)	Sponsor
Argentina				Responsible	
Australia				Responsible	Responsible
Brazil				Responsible	
Canada			Responsible		
China			Responsible	Responsible	
Columbia				Responsible	
Costa Rica		Responsible		Responsible	
Ecuador				Responsible	
Egypt	Responsible				
El Salvador				Responsible	
Honduras			Responsible	Responsible	
Hong Kong	Responsible*				
India			Responsible	Responsible	
Indonesia				Responsible	
Israel				Responsible	
Japan				Responsible	
Kazakhstan	Responsible				
Malaysia	Responsible				
Mexico				Responsible	
New Zealand				Responsible	Responsible
Peru				Responsible	
Philippines				Responsible	
Russia	Responsible				
Saudi Arabia	Responsible				
Serbia	Responsible			Responsible	
Singapore		Responsible	Responsible	Responsible	
South Africa		Responsible		Responsible***	
South Korea			Responsible	Responsible	

Intake, Assessment, and Complaint Determination

027-WI185

Revision R

Page 33 of 33

Work Instruction

Medtronic

Taiwan				Responsible	
Thailand			Responsible	Responsible	
Uruguay				Responsible	
United States			Responsible**		
Vietnam				Responsible	

* This role for Hong Kong may be referred to as the Local Responsible Person (LRP).

** If Medtronic is the Importer of an OEM product in the US, reporting to FDA is applicable for events resulting in Death or Serious Injury.

*** This would also apply if Medtronic is the Certificate of Registration Holder (HCR).