


The Biovarase User Manual

Contents

Introduction.....	2
Logical organization of the Biovarase program.....	3
Start application.....	4
Log into application.....	4
Change password.....	5
Manage Tests.....	6
How create a test.....	6
Create a Test Method.....	7
Assign a Test Method to a sections.....	9
Assign the test to the workstation.....	10
Manage Workstations.....	11
Create an equipment.....	11
Create a workstation.....	12
Manage controls.....	13
Create a control.....	13
Create a batch.....	14
Manage results.....	16
Manage Users.....	17
Manage Sites.....	18
Create sites.....	19
Create wards.....	20
Create sections.....	21
Plots.....	23
Levey Jennings plots.....	23
Youden plots.....	23
TEA plots.....	23
Export data.....	24
Analytical Goals.....	24
Quick data analysis.....	24
Counts.....	24
Controls list.....	24
Database operations.....	24

The Biovarase User Manual

Introduction

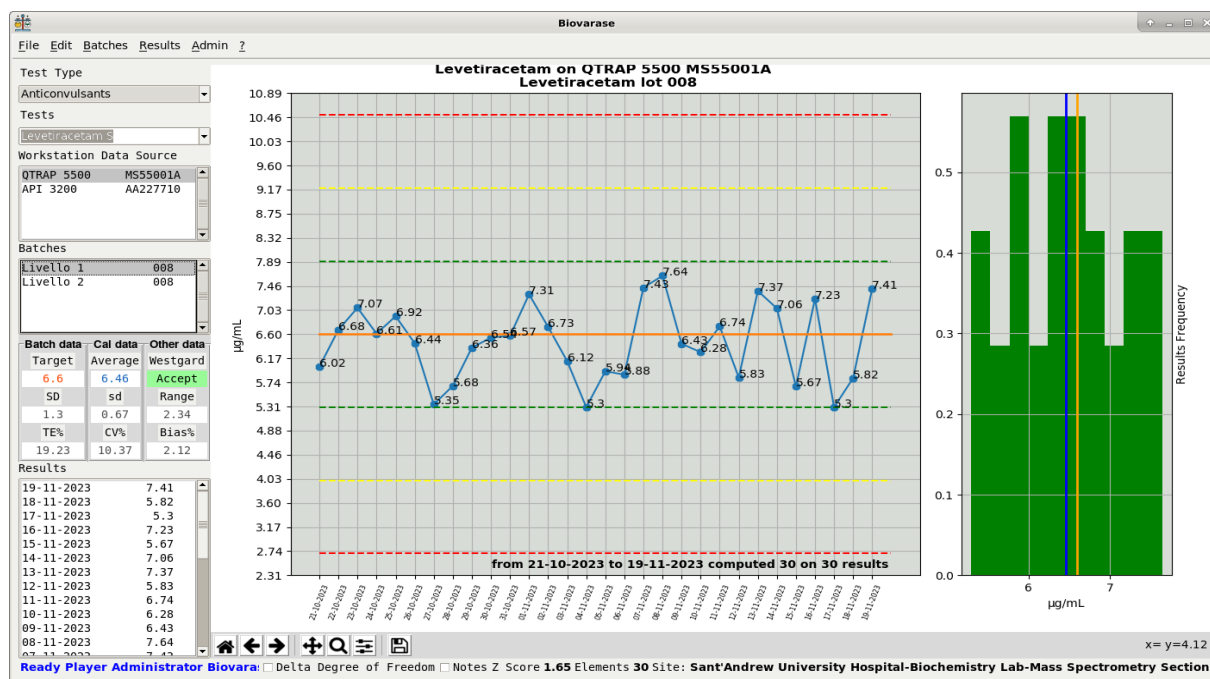

Biovarase is an application for managing the internal quality control of an clinical laboratory.

This program allows the monitoring of IQC through the calculation of the following parameters:

- (a) standard deviation, sd
- (b) coefficient of variation cv%
- (c) range
- (d) bias
- (e) Westgard's rules
- (f) Levey-Jennings graphs
- (g) Youdent's test

The Biovarase User Manual

In addition, based on the use of data reported by the article

"Current Databases on biologic variation: pros, cons and progress."

Scand J Clin Lab Invest 1999;59:491-500 (updated version 2014)

the program is able to calculate the TEa (total allowable error), and the critical difference (Dcr), of some analytes, allowing to define the laboratory's analytical goals.

Logical organization of the Biovarase program.

In Biovarase each test must be associated with an analytical method, and this is because a test could be performed with different analytical methods.

In addition, each test must be assigned to an analytical section and a workstation on which it is run.

A workstation is defined as the physical instrument where the test is performed.

To use a test for quality control, you must first create it, then assign it a method; a test can have from 1 to n associated methods. Then you have to associate the test-method with the section that runs it and also with the workstation where it is dosed.

You also have to create a control and its batches and assign these batches to the workstations and its tests.

Analytical sections are created from the sites. Site means the facility, usually a hospital within which there are departments, laboratories, in which there are specialized sections, for example, Hematology or Mass Spectrometry that perform tests to which quality control is submitted.

The samples used for quality control are associated with various batches normally supplied by firms outside the laboratory that certify the values for the target and standard deviation, which are to be calculated from the maximum and minimum values given on the control package inserts.

The Biovarase User Manual

Start application

Biovarase is developed on Debian 10 with Python 3.7.3

Biovarase use Tkinter patch level 8.6.9 as gui.

Biovarase use Sqlite3 as database.

Before launching the program make sure you have installed the following libraries

- matplotlib
- xlwt
- numpy

To launch the application, you must locate the file named biovarase.py in the folder where the Biovarase files reside and run it. On windows systems it will be enough to invoke it from the command line. You could also compile the program using Pyinstaller.


On linux systems you will need to make the file executable by typing the command "chmod +x filename" basically do something like this

- bc@hal9000:~\$ cd Documents/Biovarase-master/
- bc@hal9000:~/Documents/Biovarase-master\$ chmod +x biovarase.py
- bc@hal9000:~/Documents/Biovarase-master\$./biovarase.py

Log into application

Once the application is launched, the login mask will open.


To log in you can use the credentials "adm" as the user and "adm" as the password.

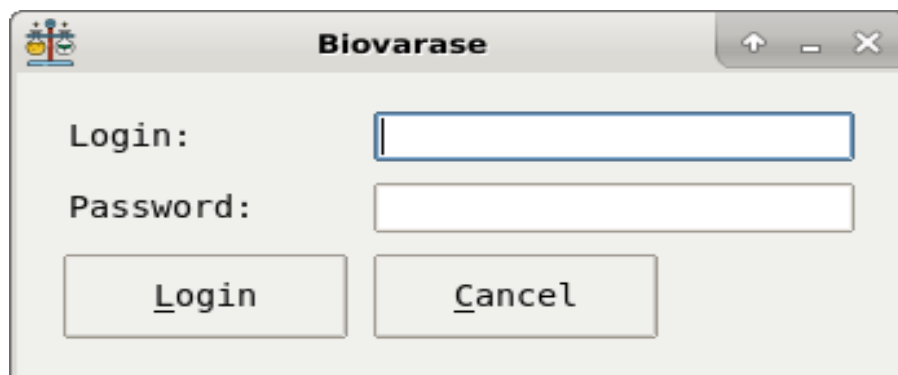

The Biovarase User Manual

Change password

Per cambiare la password bisogna andare dalla barra del menu sulla voce File e poi in basso cliccare sulla voce Change Password. RIempire tutti i campi e salvare i dati. Alla prossima apertra dell'applicazione potrete utilizzare la nuova passwod.

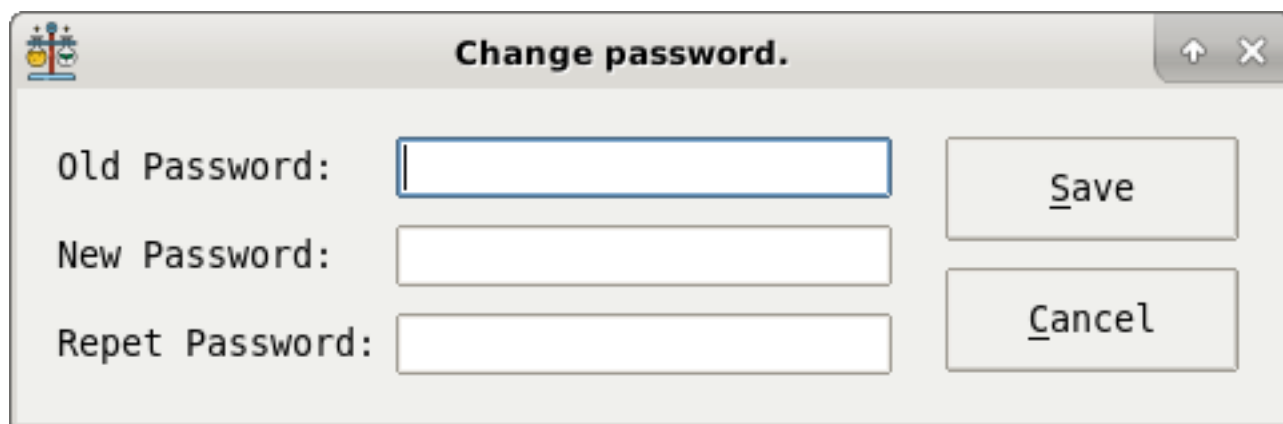

The screenshot shows a standard Windows-style dialog box titled "Change password.". On the left side, there are three labels with corresponding text input fields: "Old Password:", "New Password:", and "Repet Password:". The "Old Password:" field is currently selected with a blue border. To the right of these fields are two buttons: "Save" and "Cancel". The "Save" button has the letter "S" underlined, and the "Cancel" button has the letter "C" underlined. The dialog box has a title bar with a small icon on the left and standard window controls (minimize, maximize, close) on the right.


Se l'utente loggato ha impostato le credenziali di amministratore può resettare la password di un altro utente dalla maschera di gestione degli utenti, vedi il capitolo apposito.

The Biovarase User Manual


Manage Tests

How create a test.

From the menu bar, select the Edit item and then the Tests item.

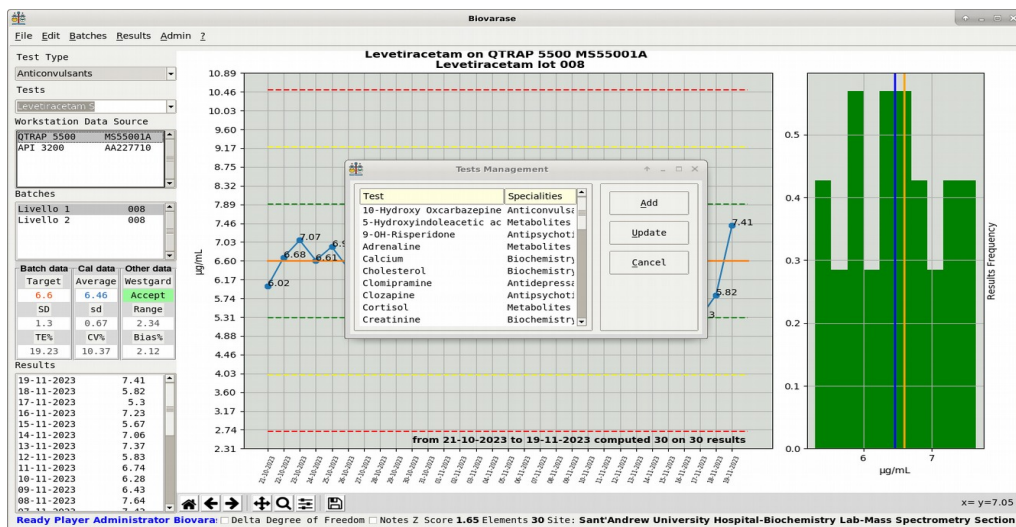

In the window that opens press the Add button and in the mask that opens fill in the two fields assigning a specialty and a name to the test.

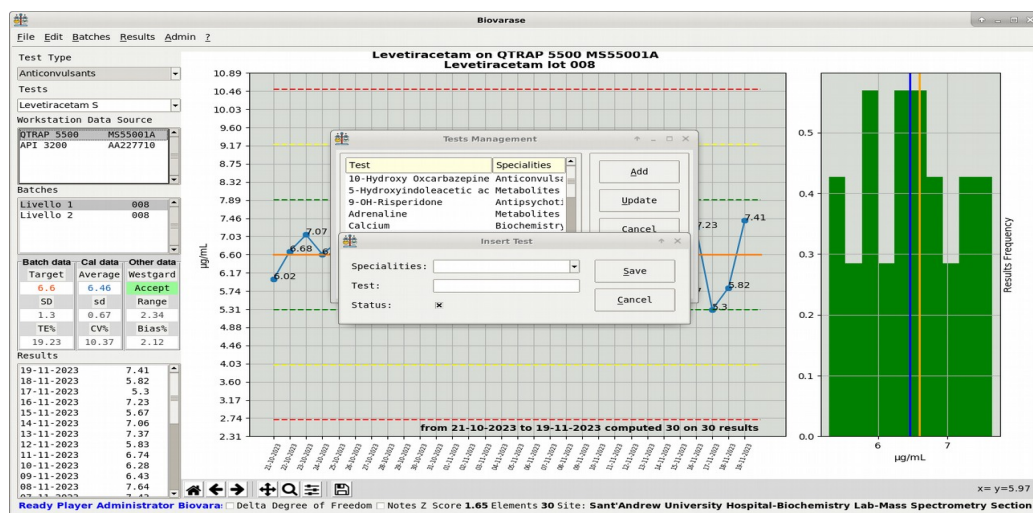


The Biovarase User Manual

Create a Test Method


To use a test, it is not enough to create it but you will need to associate with it a method.

From the menu bar select the Edit item and then the Tests Methods item.

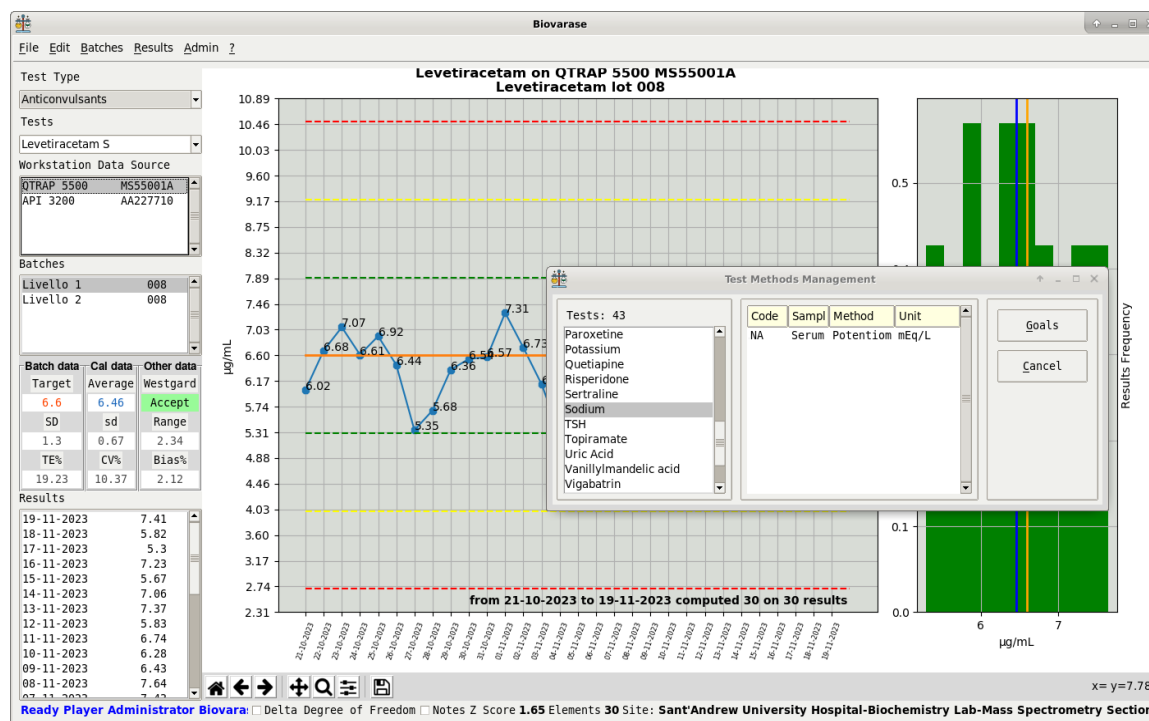

The Biovarase User Manual


In the window that opens locate on the left list the test you entered. Click on it twice. In the mask that opens fill in all fields and save. Remember that the code field must be unique.

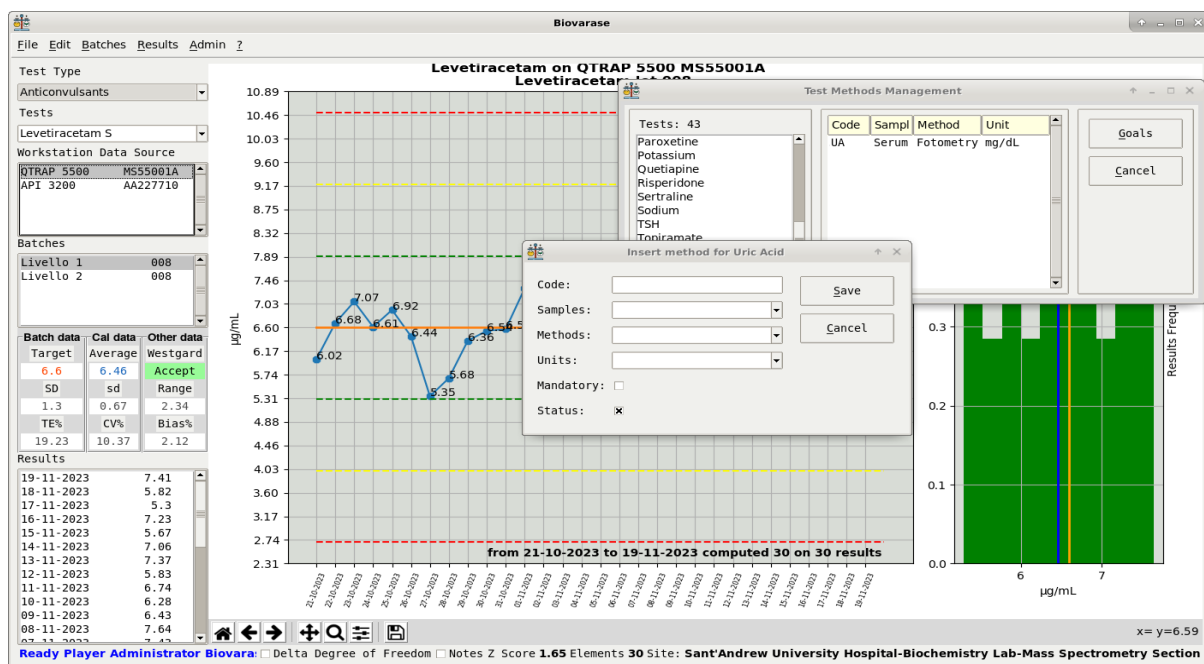


The Biovarase User Manual

Assign a Test Method to a sections

Now assign the test to the section(s) running it by opening the Tests Sections mask from the edit item on the menu bar. When you open the Tests Sections mask open the tree list on the left until you locate the section to which you want to assign the test.

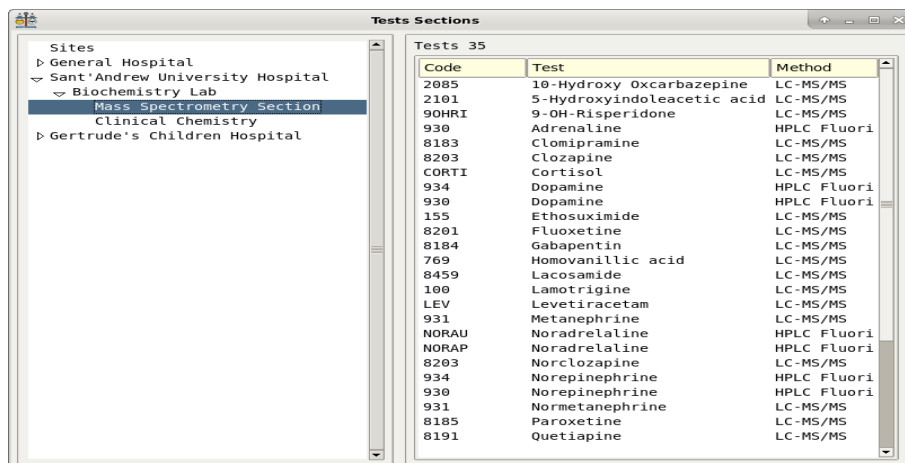

Double-click on it, locate on the list that opens the test you want to assign and double-click on it to assign it to the section, the assignment can be seen because the test appears in the list on the right that represents the executed tests of the section.

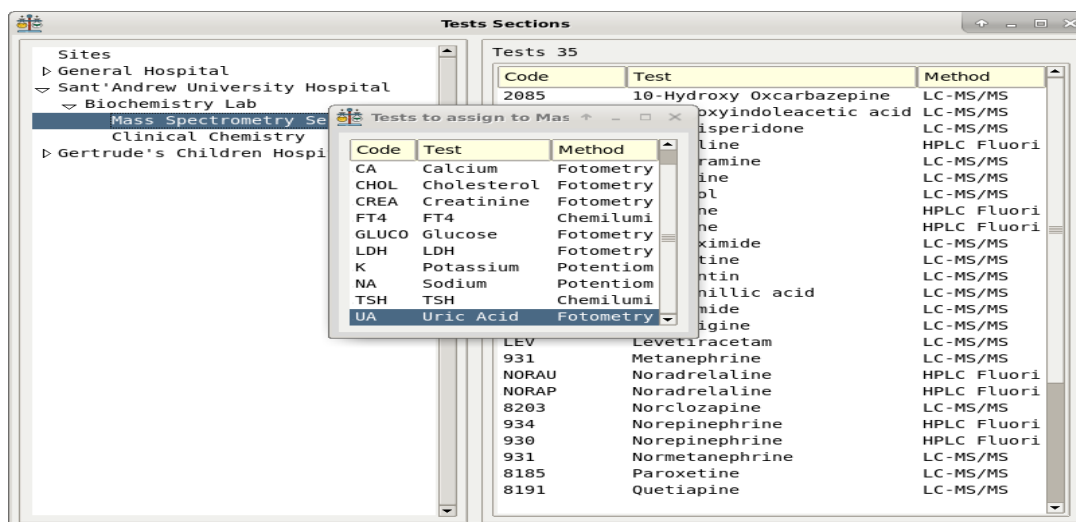


The Biovarase User Manual

Assign the test to the workstation.


Tests have to be assigned both to the sections that run them but also to the workstations on which they are run. To do this you must first create the workstations, see the dedicated chapter to understand how to do this.

Opening the Workstation Tests Methods window from the edit item on the menu bar.

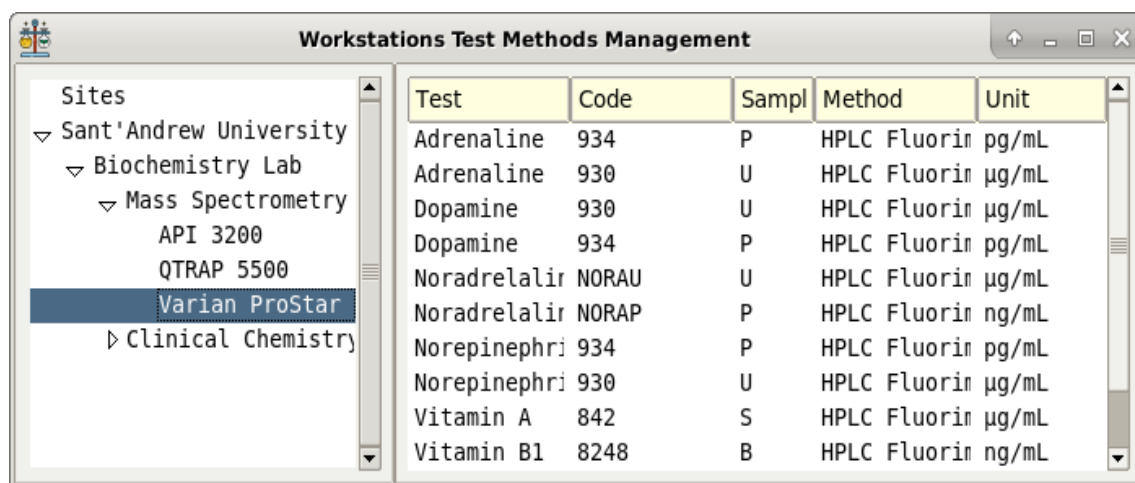

Locate from the left list the workstation to be assigned a test and click on it twice. Select the test on the window that opens and double-click on it to assign it to the workstation.

The test will appear in the right-hand list and disappear from the left-hand list.

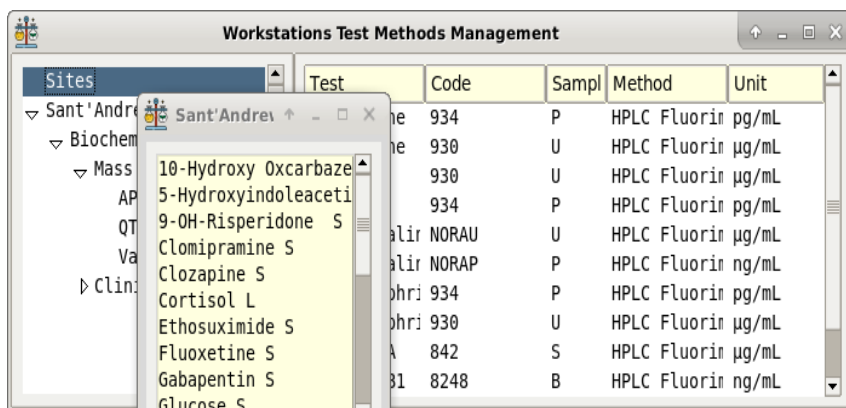

The Biovarase User Manual

Manage Workstations


A workstation physically represents , an equipment model, on which tests are run. So we may have more than one workstations of the same type i.e. of the same model. For example we may have more than one Advia 1800 that is a Siemens equipment on which we run the cholesterol test.

So to create a workstation we must first create the equipment that is the model and then the actual workstation that will be assigned to a given section. This workstation will be characterized by its serial number and device id which is a parameter that uniquely identifies it and will soon be used to interface Biovarase to the various workstations in a laboratory.

Create an equipment.

Opening the Equipments window from the Edit item on the menu bar.


Uses left buttons to add or update an equipment. Remember that an equipment is a general model of a workstation.

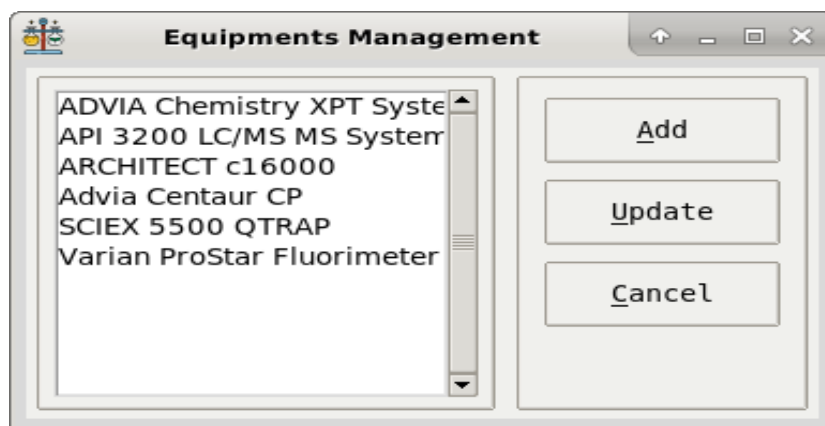

The Biovarase User Manual

Create a workstation

Opening the Workstations window from the Edit item on the menu bar.

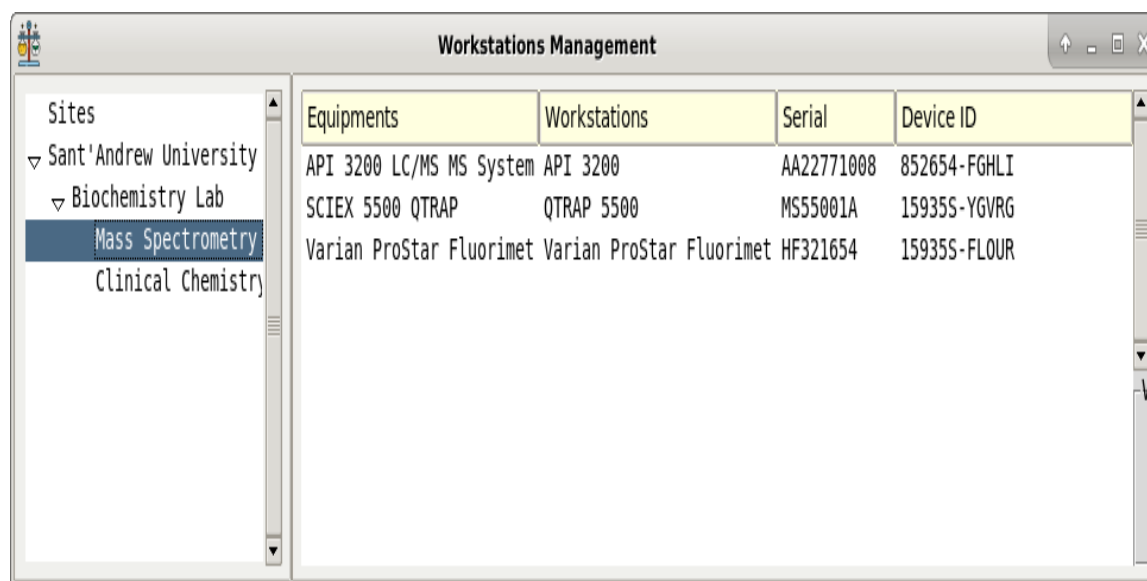

Select a section from the left-hand list and double-click on it to open the mask for creating a new workstation.

The screenshot shows the 'Insert workstation' dialog box. It contains the following fields and controls:

- Equipments: A dropdown menu.
- Device id: A text input field.
- Description: A text input field.
- Serial: A text input field.
- Sections: A dropdown menu with 'Mass Spectrometry Section' selected.
- Ranck: A text input field containing '0'.
- Status: A checkbox that is checked.
- Buttons: 'Save' and 'Cancel' buttons.

The Biovarase User Manual

Fill in all fields and save. Remember that the device id field must be unique from other entries.


The rank field represents the order in which the workstation is displayed in the main window.

Manage Controls

This type of functionality is accessible only to users who have set the level to a value other than 2.

Create a control

To insert a control locate the Controls mask found on the menu bar under Edit. Open it and enter from the Add button the data for the new control.

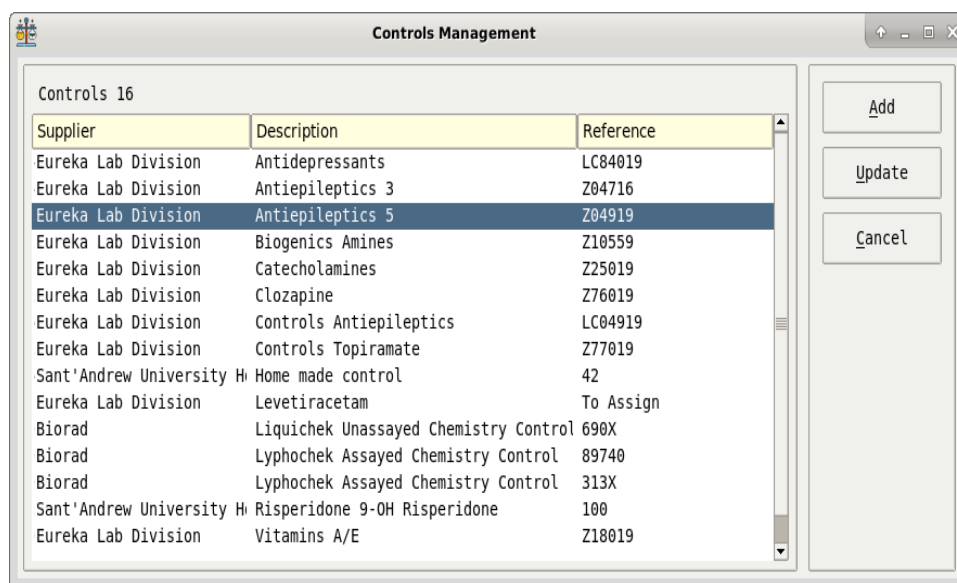


The Biovarase User Manual

Create a batch

A batch represents a production of a control with its expiration date and the values, target, maximum and minimum values, associated with the tests that can be performed with that specific batch.

Enter the batches of the controls.


From the menu bar locate the Edit item and then Data. Click on Data to open the corresponding form.

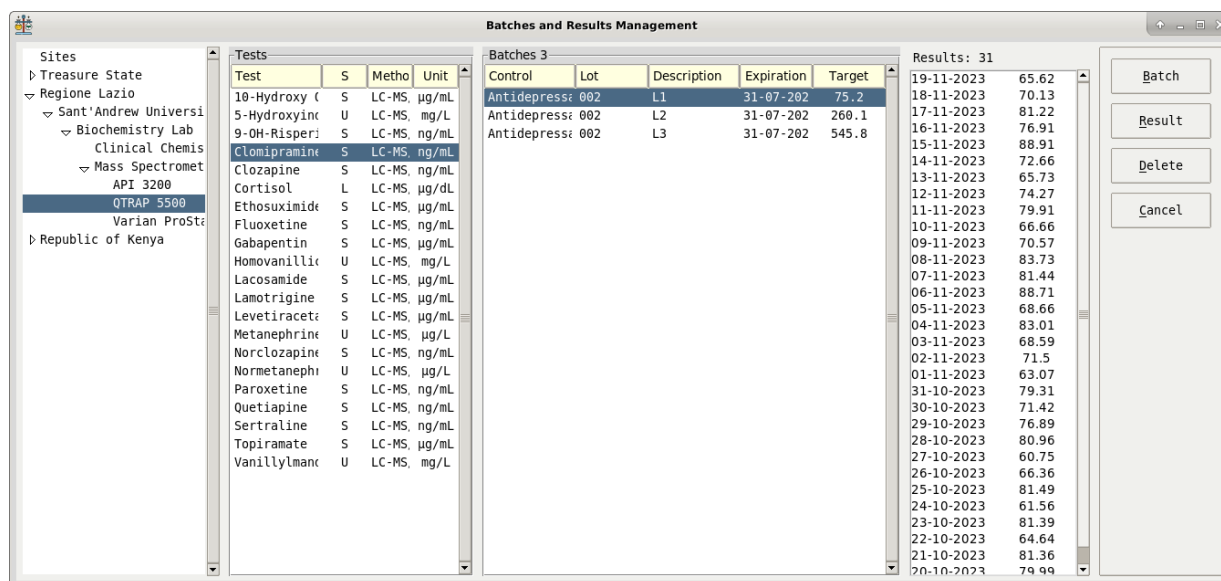

Locate on the left list the workstation on which you are running the test and select it. In the list next to it appears the list of tests you are running on the selected workstation. Double-click on the test to which you want to assign a control batch.

The Biovarase User Manual

In the window that opens fill in all the fields assigning a control, the batch, a description, usually it is Level 1 or Level 2, the due date, and the target.

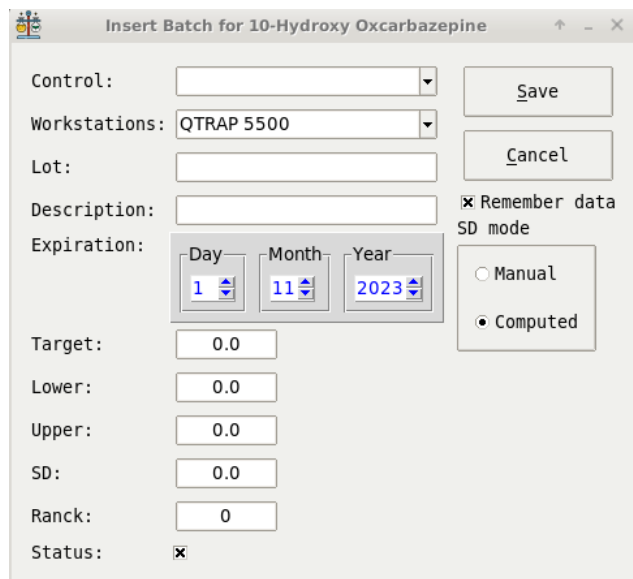

The screenshot shows a dialog box titled "Insert Batch for 10-Hydroxy Oxcarbazepine". It contains several input fields and buttons. The "Control:" field is a dropdown menu. The "Workstations:" field is a dropdown menu showing "QTRAP 5500". The "Lot:" field is a text box. The "Description:" field is a text box. The "Expiration:" field is a date picker with "Day" (1), "Month" (11), and "Year" (2023) components. The "Target:" field is a text box with "0.0". The "Lower:" field is a text box with "0.0". The "Upper:" field is a text box with "0.0". The "SD:" field is a text box with "0.0". The "Ranck:" field is a text box with "0". The "Status:" field has a checked checkbox. There are "Save" and "Cancel" buttons. A checkbox labeled "Remember data" is checked. Below it, "SD mode" is indicated with "Manual" and "Computed" radio buttons, where "Computed" is selected.

If you enter the minimum and maximum value the program will calculate the standard deviation if computed is selected in the "SD mode" options otherwise if manual is selected you can enter the data without any calculation being done.


Note that each batch must be assigned a control and a workstation.

The ranck field represents the order in which the batch is displayed in the main window.

The Biovarase User Manual

Manage Results

Control results can be entered in two ways. If the user has a level other than 2 from the Data window while for any level from the main program window.

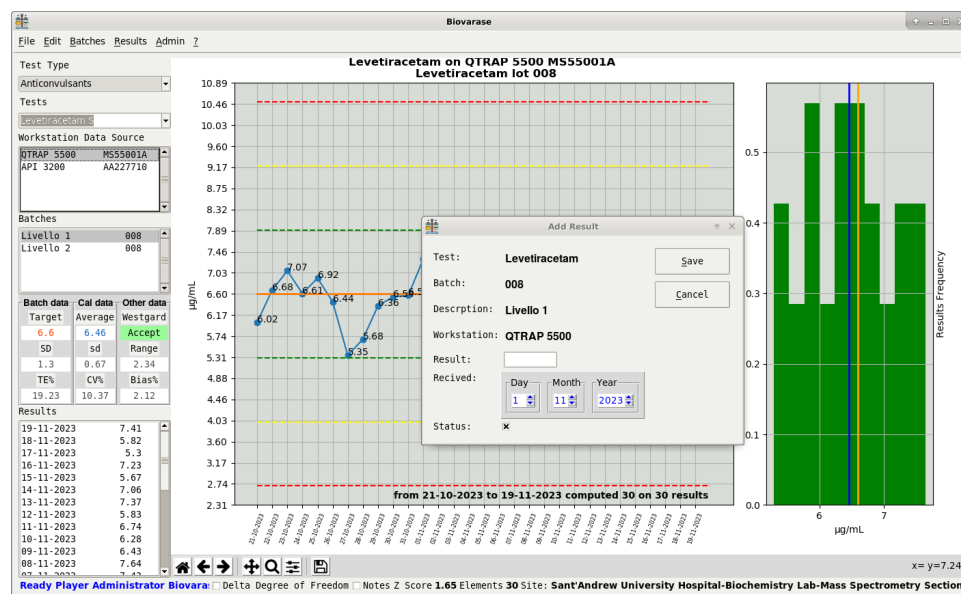

To enter a result referring to a given test, for a given batch run on a given workstation on the main window you must first select the test type from the combo at the top left, then select the test in the combo just below.

By selecting the test you will see in the list under "Workstation data source" appear the list of workstations associated with the selected test.

Selecting the workstation on which the test was run will cause the list of batches associated with the selected test and workstation to appear in the list below.

Selecting a batch further will cause the results entered previously for the selected batch to appear, if any, and the related levey jennings graph will be drawn.

To enter a new result locate on the menu bar the Results item and then Add Results. Enter the result in the window that opens.

The value will be loaded into the database and consequently onto the graphs.

The Biovarase User Manual

On entering a new result, the current day's date is proposed. If you want to edit a result you can double-click on it. It will open the same window used in the insertion phase but with the fields filled. If the user has a level equal to two he can edit the data and also make the result inactive by removing the check on the "Status" control which will cause the result not to be used for the calculation of quality control data or even to make the related graphs. If the user has a level greater than 2 he will also be able to delete the result, the "Delete" button will appear.

Manage Users

Users are managed from the Users mask found from the menu bar by clicking on the Adm item and then the Users item.

Only an enabled user can access this window, which means that the user must have set the "level" value to zero.

Once this mask is open, users can be added or modified. You can also reset a user's password by selecting it from the list and then pressing the "Reset" button.

By doing so, the password will be set as "pass".

Assigning the value 0 to a user's rule entry is equivalent to making him or her an administrator and thus giving him or her access to all program features.

Assigning the value 1 means allowing him to edit all menu voices except for the administrator voices.

Assigning the value 2 means allowing him to enter only the results, edit them but not delete them.

The Biovarase User Manual

Manage Sites


The management of the sites is reserved to the users with preset level to 0 that is that of administrator.

Biovarase is a multi-site application that is able to manage data from different workstations in different clinical laboratories.

For example, it is able to manage the results associated with a particular batch for the cholesterol test coming from different laboratories located in different places and involving different hospitals

To do this you must first of all create references to sites. For example, a hospital will be headed by a private company or a government agency, at least here in Italy it is.


So to create the site "Sant'Andrew University Hospital" we should include in the window Suppliers that is locate under Admin voices of the menu bar a voice with "Sant'Andrew University Hospital" and another as "Lazio Region" as this hospital is a public hospital and depends on the Lazio region

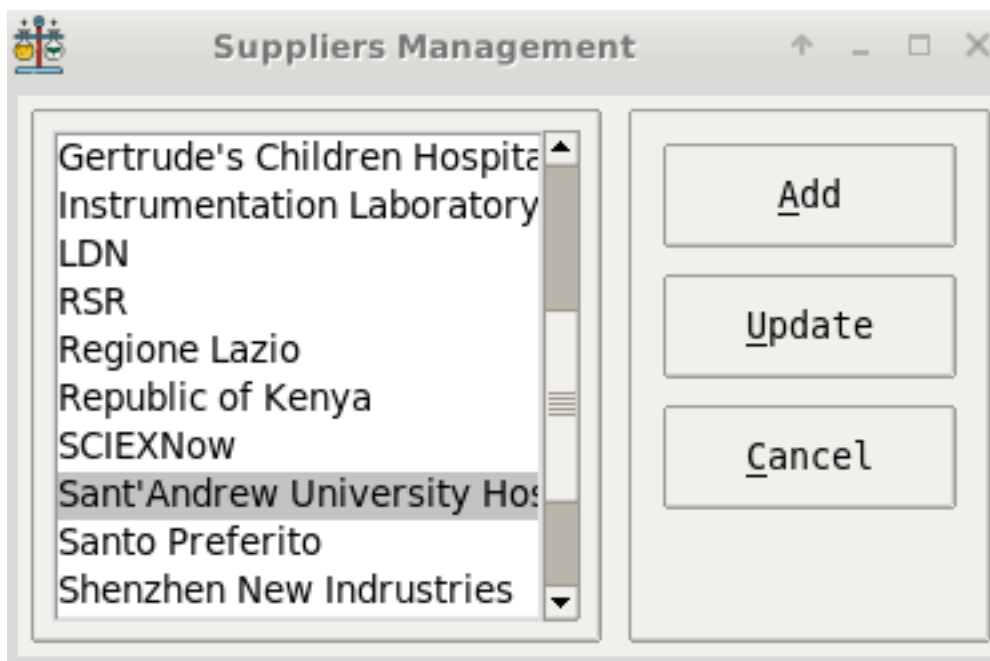

The Biovarase User Manual

Create sites


Then open the window "Sites" always under Admin and pressing the Add key will open the following window

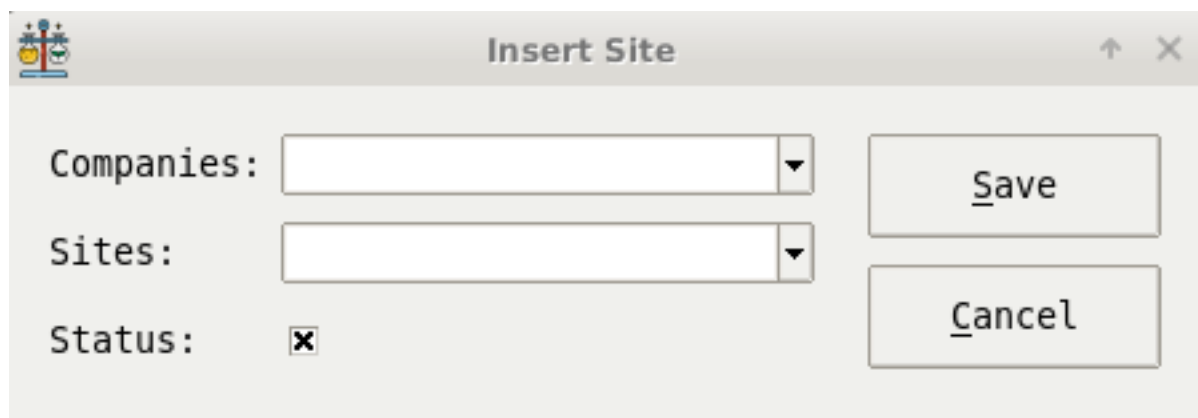

The "Insert Site" dialog box contains three input fields on the left and two buttons on the right. The first field is labeled "Companies:" and is a dropdown menu. The second field is labeled "Sites:" and is also a dropdown menu. The third field is labeled "Status:" and contains a checked checkbox. The buttons are labeled "Save" and "Cancel".

Companies:	<input type="text"/>	<input type="button" value="Save"/>
Sites:	<input type="text"/>	
Status:	<input checked="" type="checkbox"/>	

The first field "Company" represents the parent company while the second "Site" the daughter company. We can thus add to the same mother other daughter companies

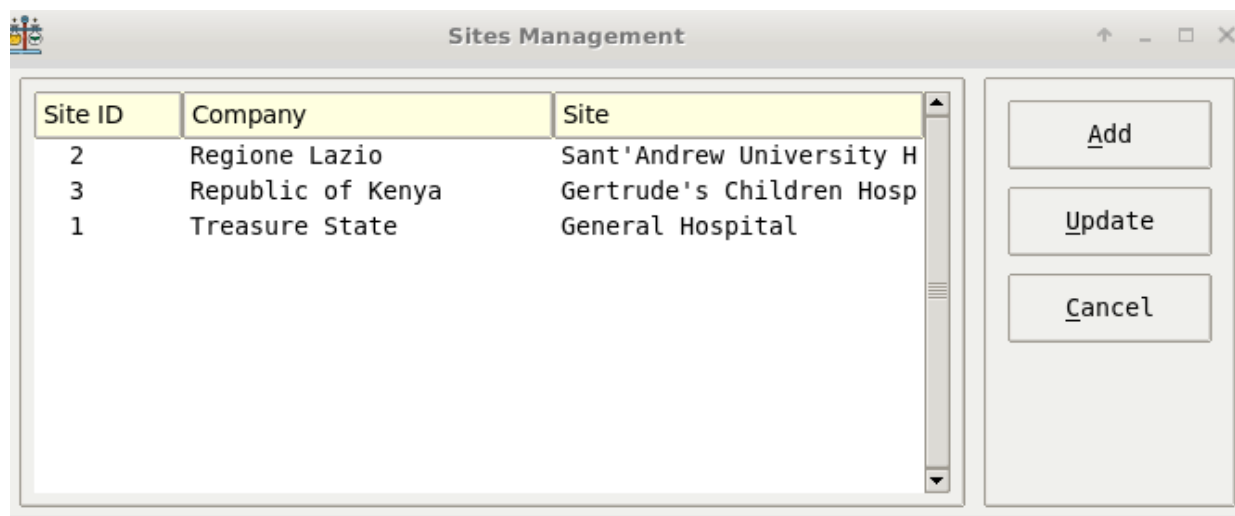

The "Sites Management" window displays a table with three columns: Site ID, Company, and Site. The table contains three rows of data. To the right of the table are three buttons: Add, Update, and Cancel.


Site ID	Company	Site
2	Regione Lazio	Sant'Andrew University H
3	Republic of Kenya	Gertrude's Children Hosp
1	Treasure State	General Hospital

The Biovarase User Manual

Create wards

Once we have created the site we have to create the departments, that is, the laboratories of the site.

To do this we open from Admin the window "Wards"

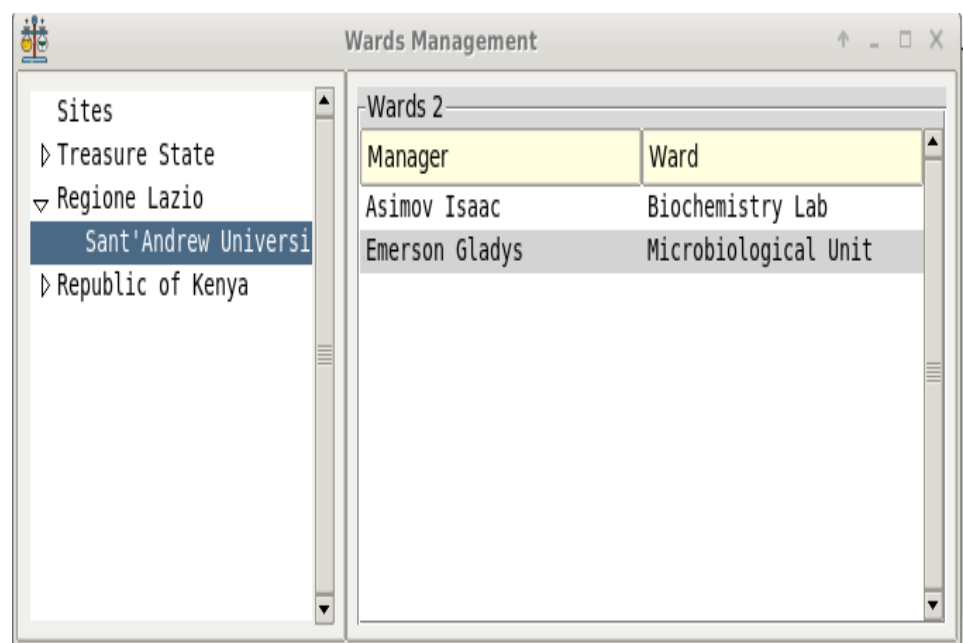

From the list on the left we want to add a section by clicking on it twice and fill in the fields in the window that opens.

To update a ward make double click on it row on the right list.


Once created the wards can not be deleted but only disabled by setting the value of "Status".

The Biovarase User Manual

Create sections


Once we have created the wards we have to create the sections, that is, the laboratory section such as Biochemistry or Ematology or Mass Spectrometry etc etc where workstation stay.

To do this we open from Admin the window "Sections"

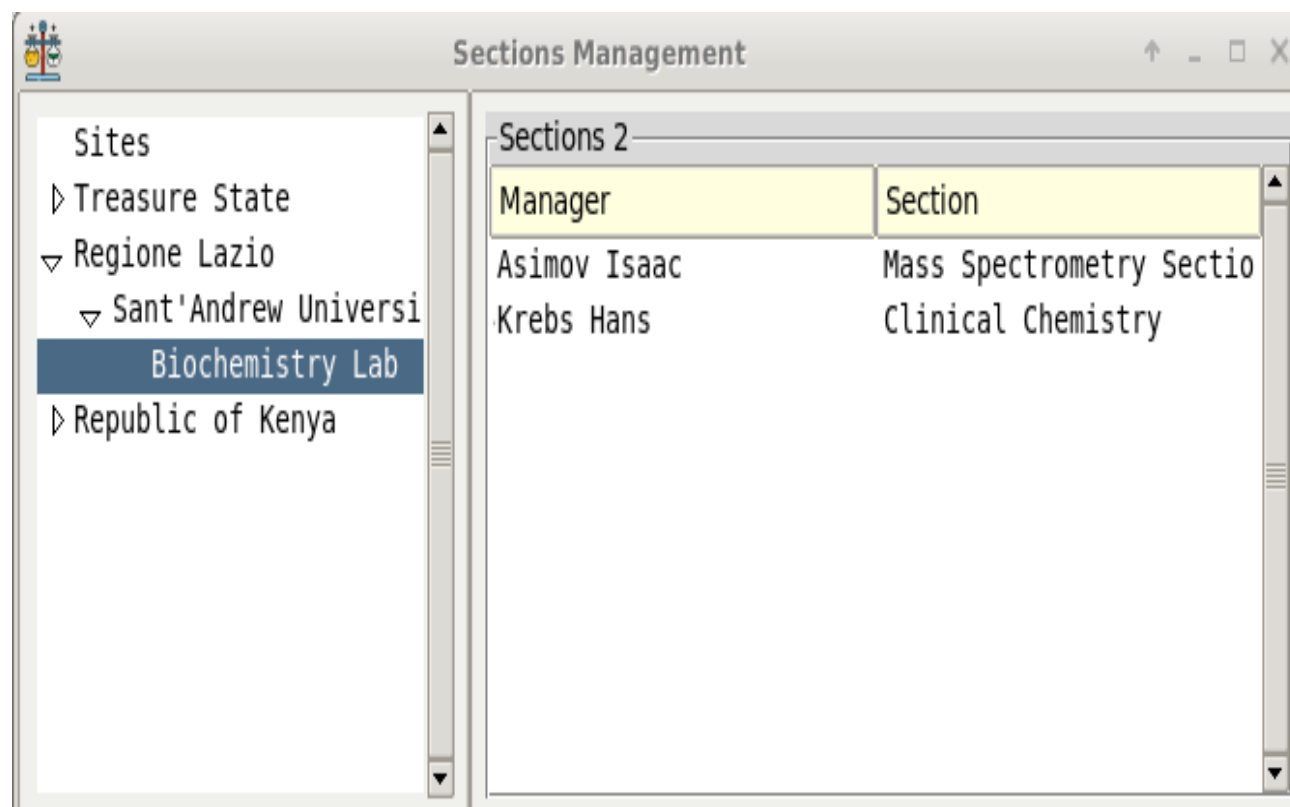

The Biovarase User Manual

Locate on the left list the ward previously created and where you want to create a section and click on it twice to open the data entry window

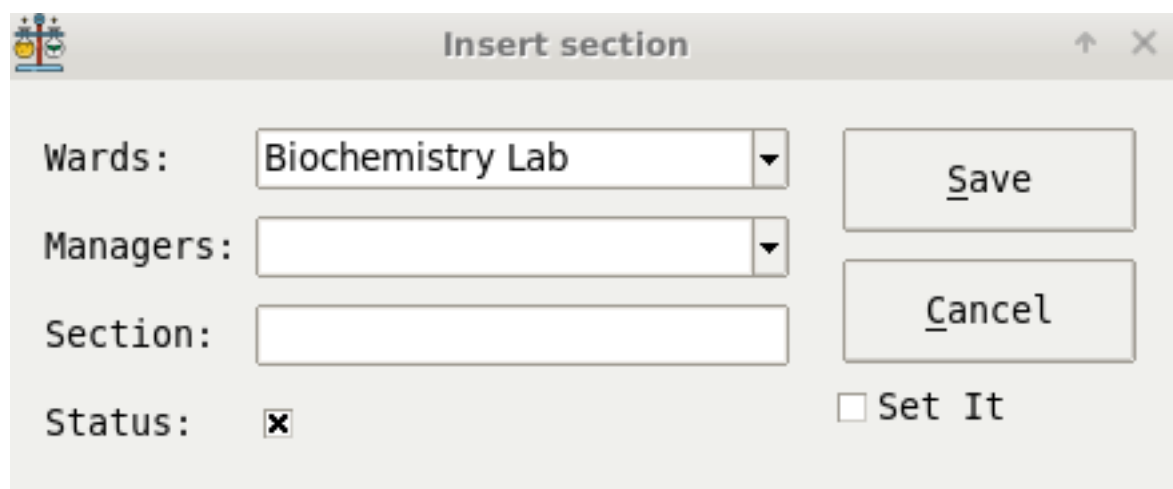

The screenshot shows a dialog box titled "Insert section" with a standard Windows icon in the top-left corner and maximize, minimize, and close buttons in the top-right corner. The dialog contains four input fields on the left and two buttons on the right. The "Wards:" field is a dropdown menu with "Biochemistry Lab" selected. The "Managers:" field is an empty dropdown menu. The "Section:" field is an empty text box. The "Status:" field has a checked checkbox with an 'x' inside. To the right of the "Status:" field is an unchecked checkbox labeled "Set It". The "Save" button is located below the "Wards:" and "Managers:" fields, and the "Cancel" button is below the "Section:" field.

Wards:	Biochemistry Lab	Save
Managers:		
Section:		Cancel
Status:	<input checked="" type="checkbox"/>	<input type="checkbox"/> Set It

Fill in all fields and save.

The field "Set It" if activated will cause the program will point to the data in this section.

In the program directory there is a file called section_id where the section id set with "Set It" is written.

To update a section make double click on it row on the right list.

Once created the sections can not be deleted but only disabled by setting the value of "Status".

The Biovarase User Manual

Plots

Biovarase can generate the following graphs

Levey Jennings plots

The Levey Jennings chart that is always shown in the main window but can be generated separately, after selecting a workstation on the main window and then clicking on the item in the menu bar under File and then Plots.

This generates a chart summarizing the active plots for the selected workstation,

Youden plots

The Youden graph can be generated only if you select two batches of the same test and an eworkstation provided that the two batches have the same number of results.

After selecting a workstation on the main window and then

two batches clicking on the item in the menu bar under File and then Youden is generated this type of chart.

TEA plots

This type of graph can only be generated if the selected test is adsorbed to the data for the analytical goals.

Export data

Biovarase can export the results data in excel format. From the menu bar select the Export item on the File item. Choose an item and click on it.

Analytical Goals

To manage analytical goals, we need to assign values, if any, of CVw, CVb, Imp%, Bias%, TEa% to a test on the mask for assigning methods to tests. To do this, once a method has been assigned to the test from the Test Methods Management mask, press the Goals button and fill in the fields with the required data.

Enable the export of the test by enabling the check field named "To export"

The Biovarase User Manual

Quick data analysis

Selecting this item opens a window that asks for the date of the data to be exported. By default the current date is set. Clicking on Export vngono exported all the quality control data performed on the selected day referable to the section set on the program.

Counts

Export the number of checks performed for tests

Controls list

Shows the list of controls used with expiration dates and supplier

Database operations

From the menu bar select the Database item on the File voices.

Now you can execute a vacuum of the Sqlite 3 or a dump of the database. Dumping the database generate a text file in the application directory named as `yyyymmddhhmmss.sql`, something like `20231101133155.sql`