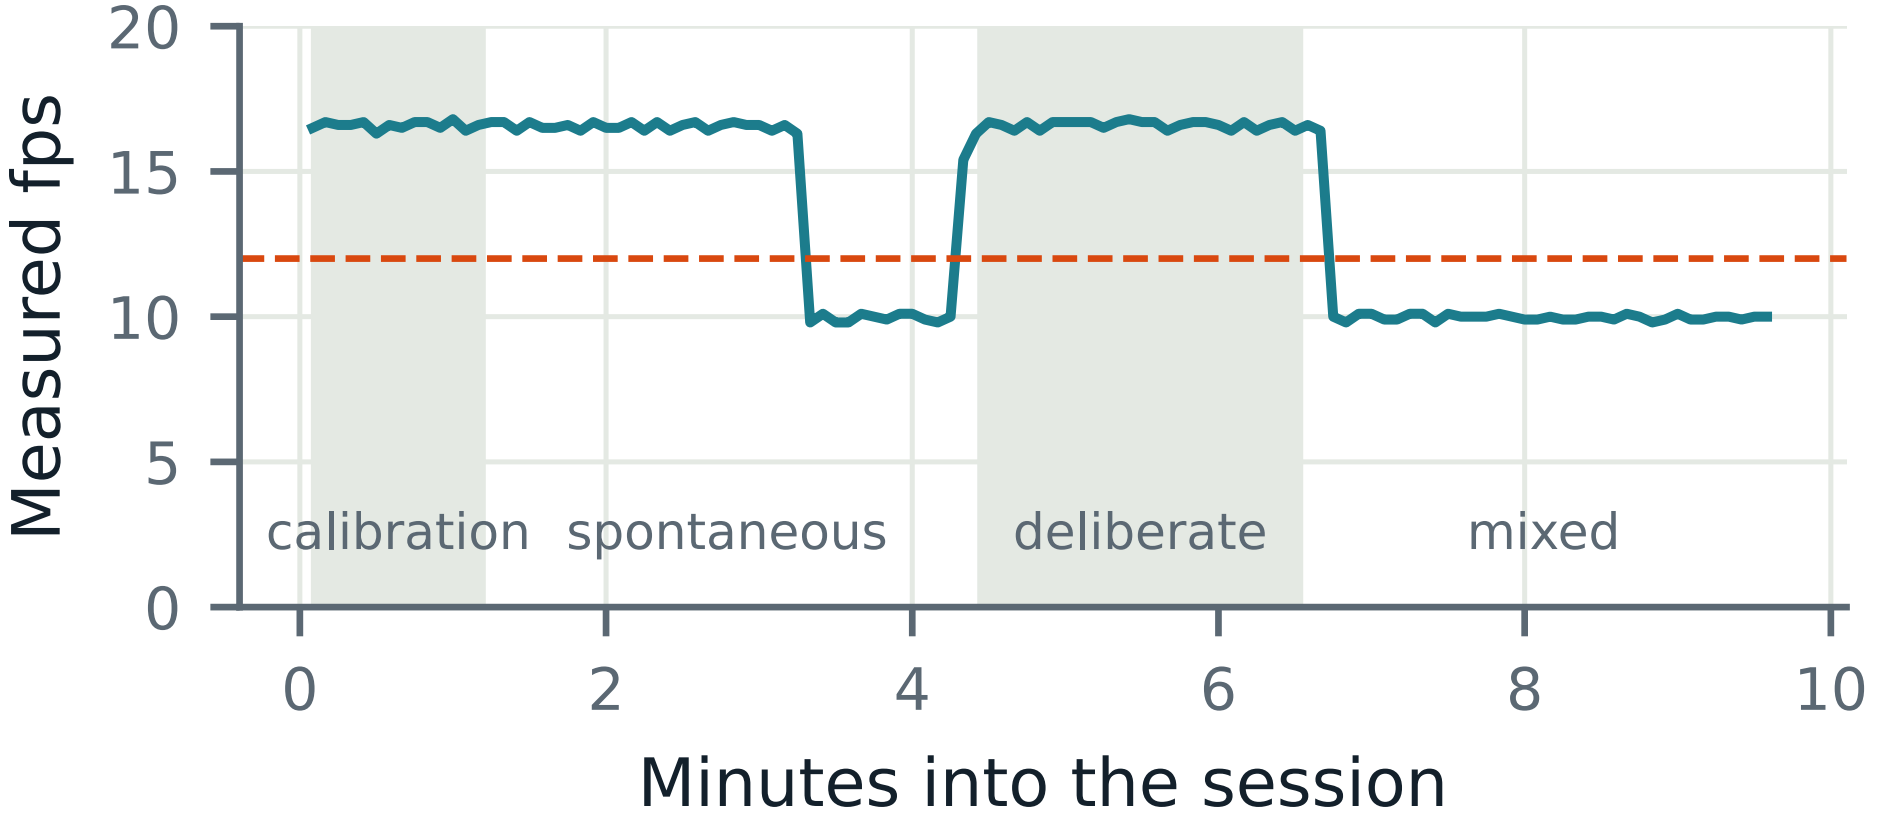
Measured fps
20
15
10
5
0
calibration
spontaneous
deliberate
mixed
0
2
4
6
8
10
Minutes into the session