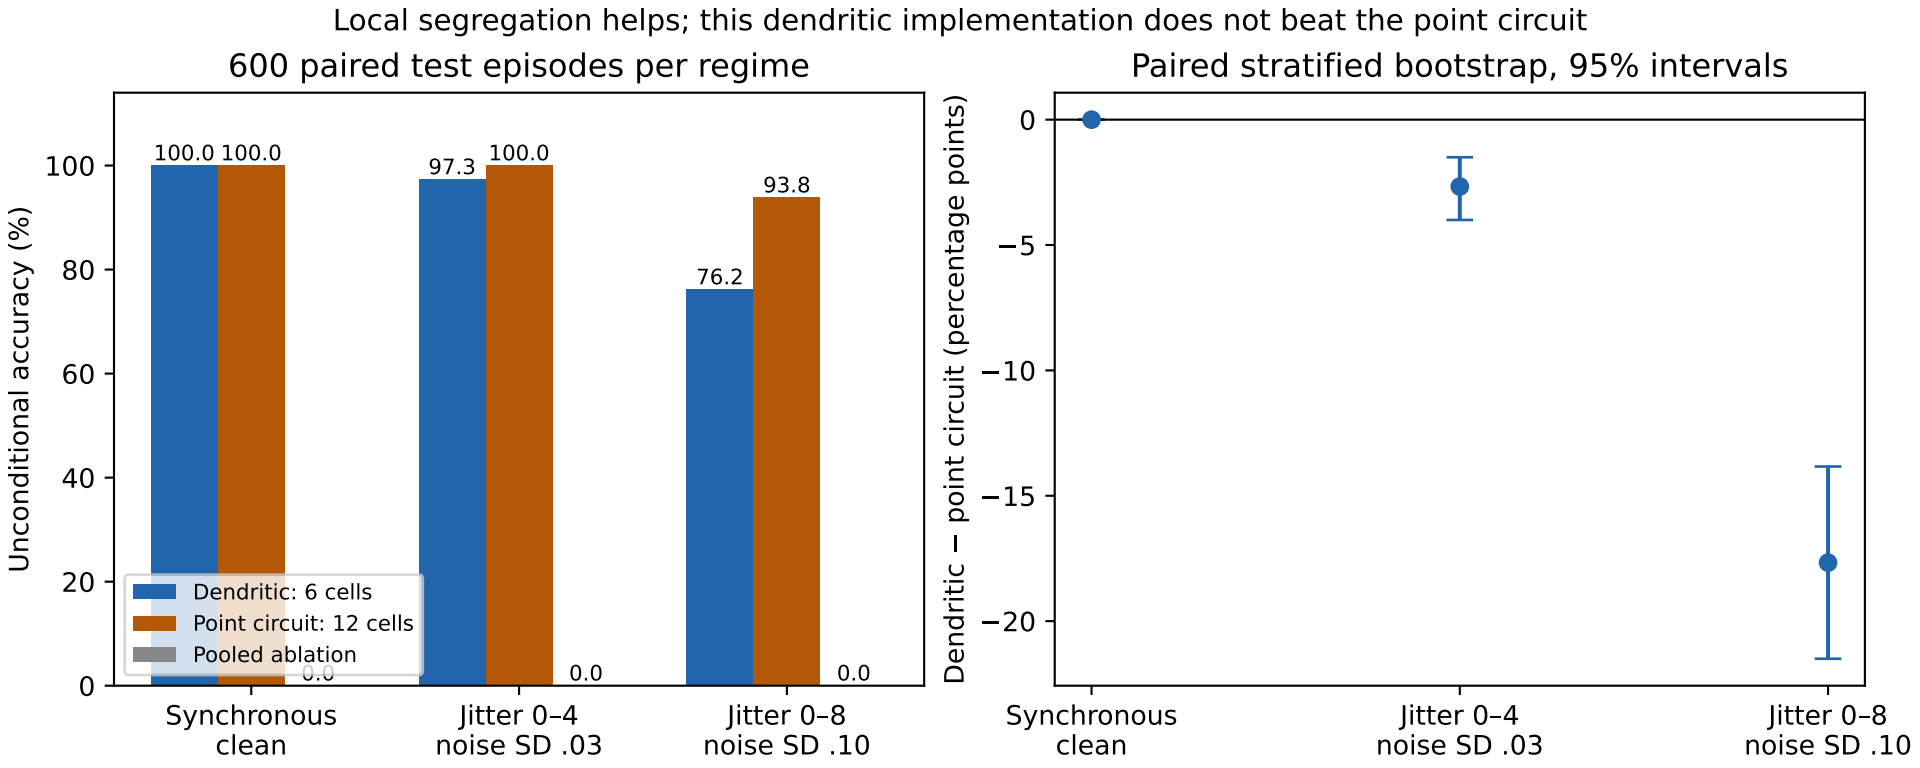
Local segregation helps; this dendritic implementation does not beat the point circuit
600 paired test episodes per regime
Unconditional accuracy (%)
100.0
100.0
97.3
100.0
76.2
93.8
0.0
0.0
0.0
Dendritic: 6 cells
Point circuit: 12 cells
Pooled ablation
Synchronous clean
Jitter 0–4 noise SD .03
Jitter 0–8 noise SD .10
Paired stratified bootstrap, 95% intervals
Dendritic − point circuit (percentage points)
0
−5
−10
−15
−20
Synchronous clean
Jitter 0–4 noise SD .03
Jitter 0–8 noise SD .10