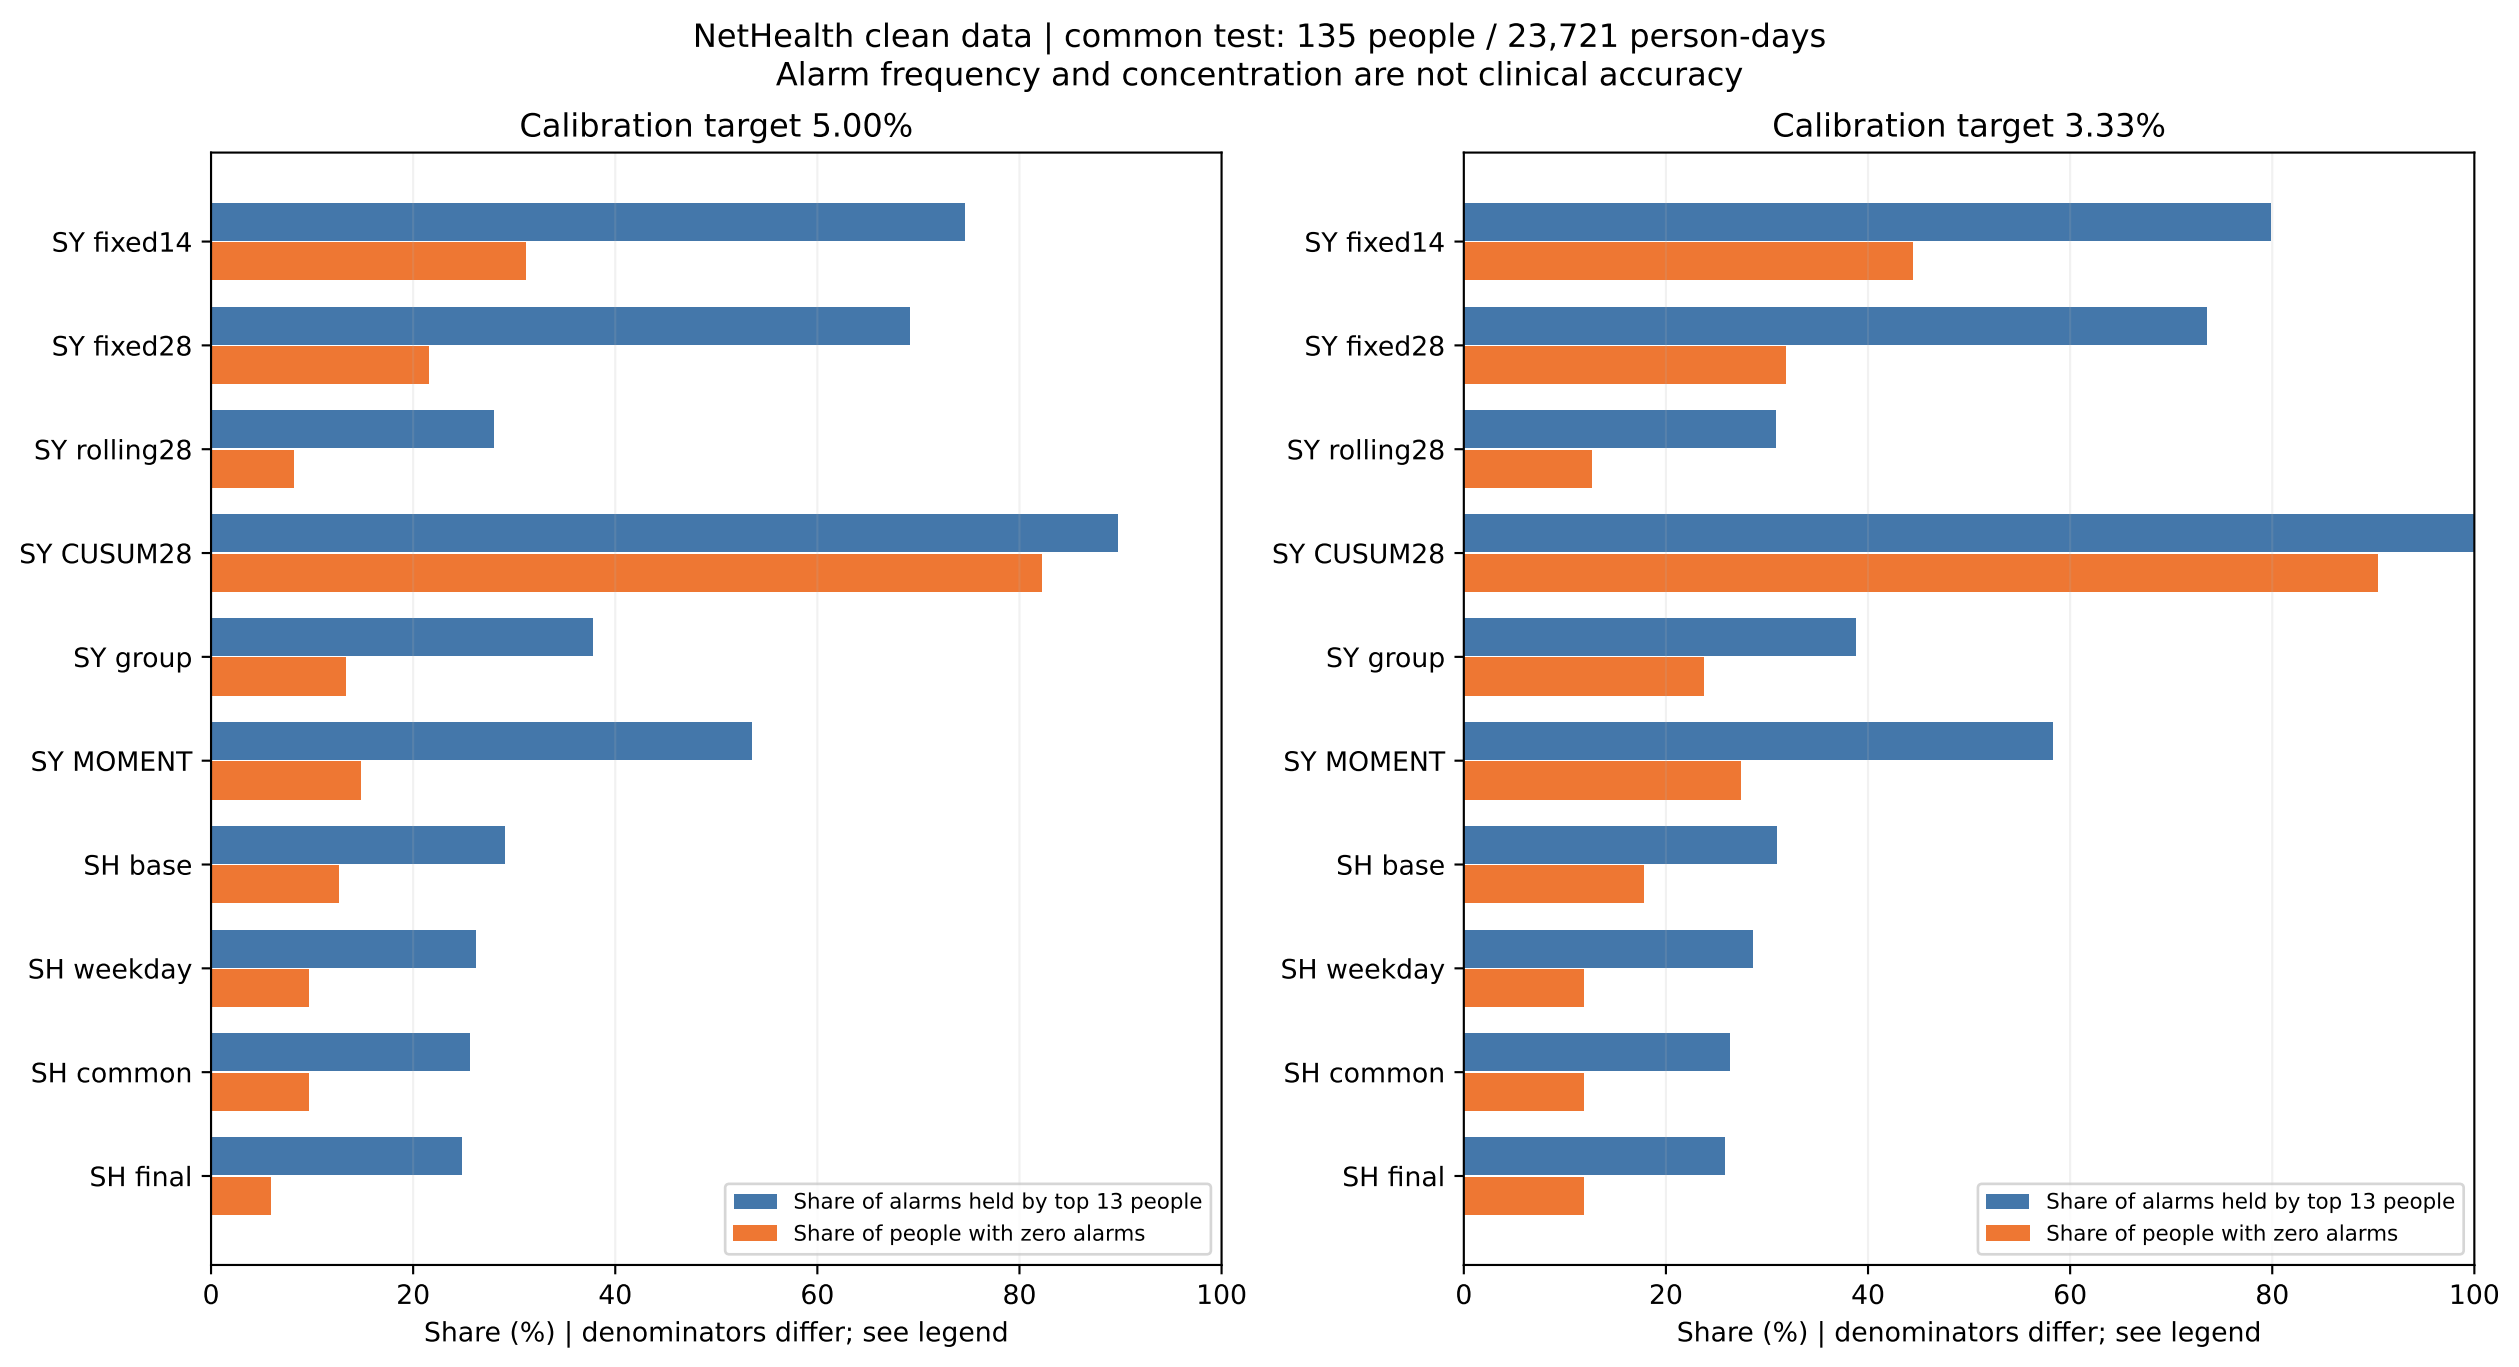
NetHealth clean data | common test: 135 people / 23,721 person-days
Alarm frequency and concentration are not clinical accuracy
Calibration target 5.00%
Calibration target 3.33%
SY fixed14
SY fixed28
SY rolling28
SY CUSUM28
SY group
SY MOMENT
SH base
SH weekday
SH common
SH final
Share of alarms held by top 13 people
Share of people with zero alarms
0
20
40
60
80
100
Share (%) | denominators differ; see legend