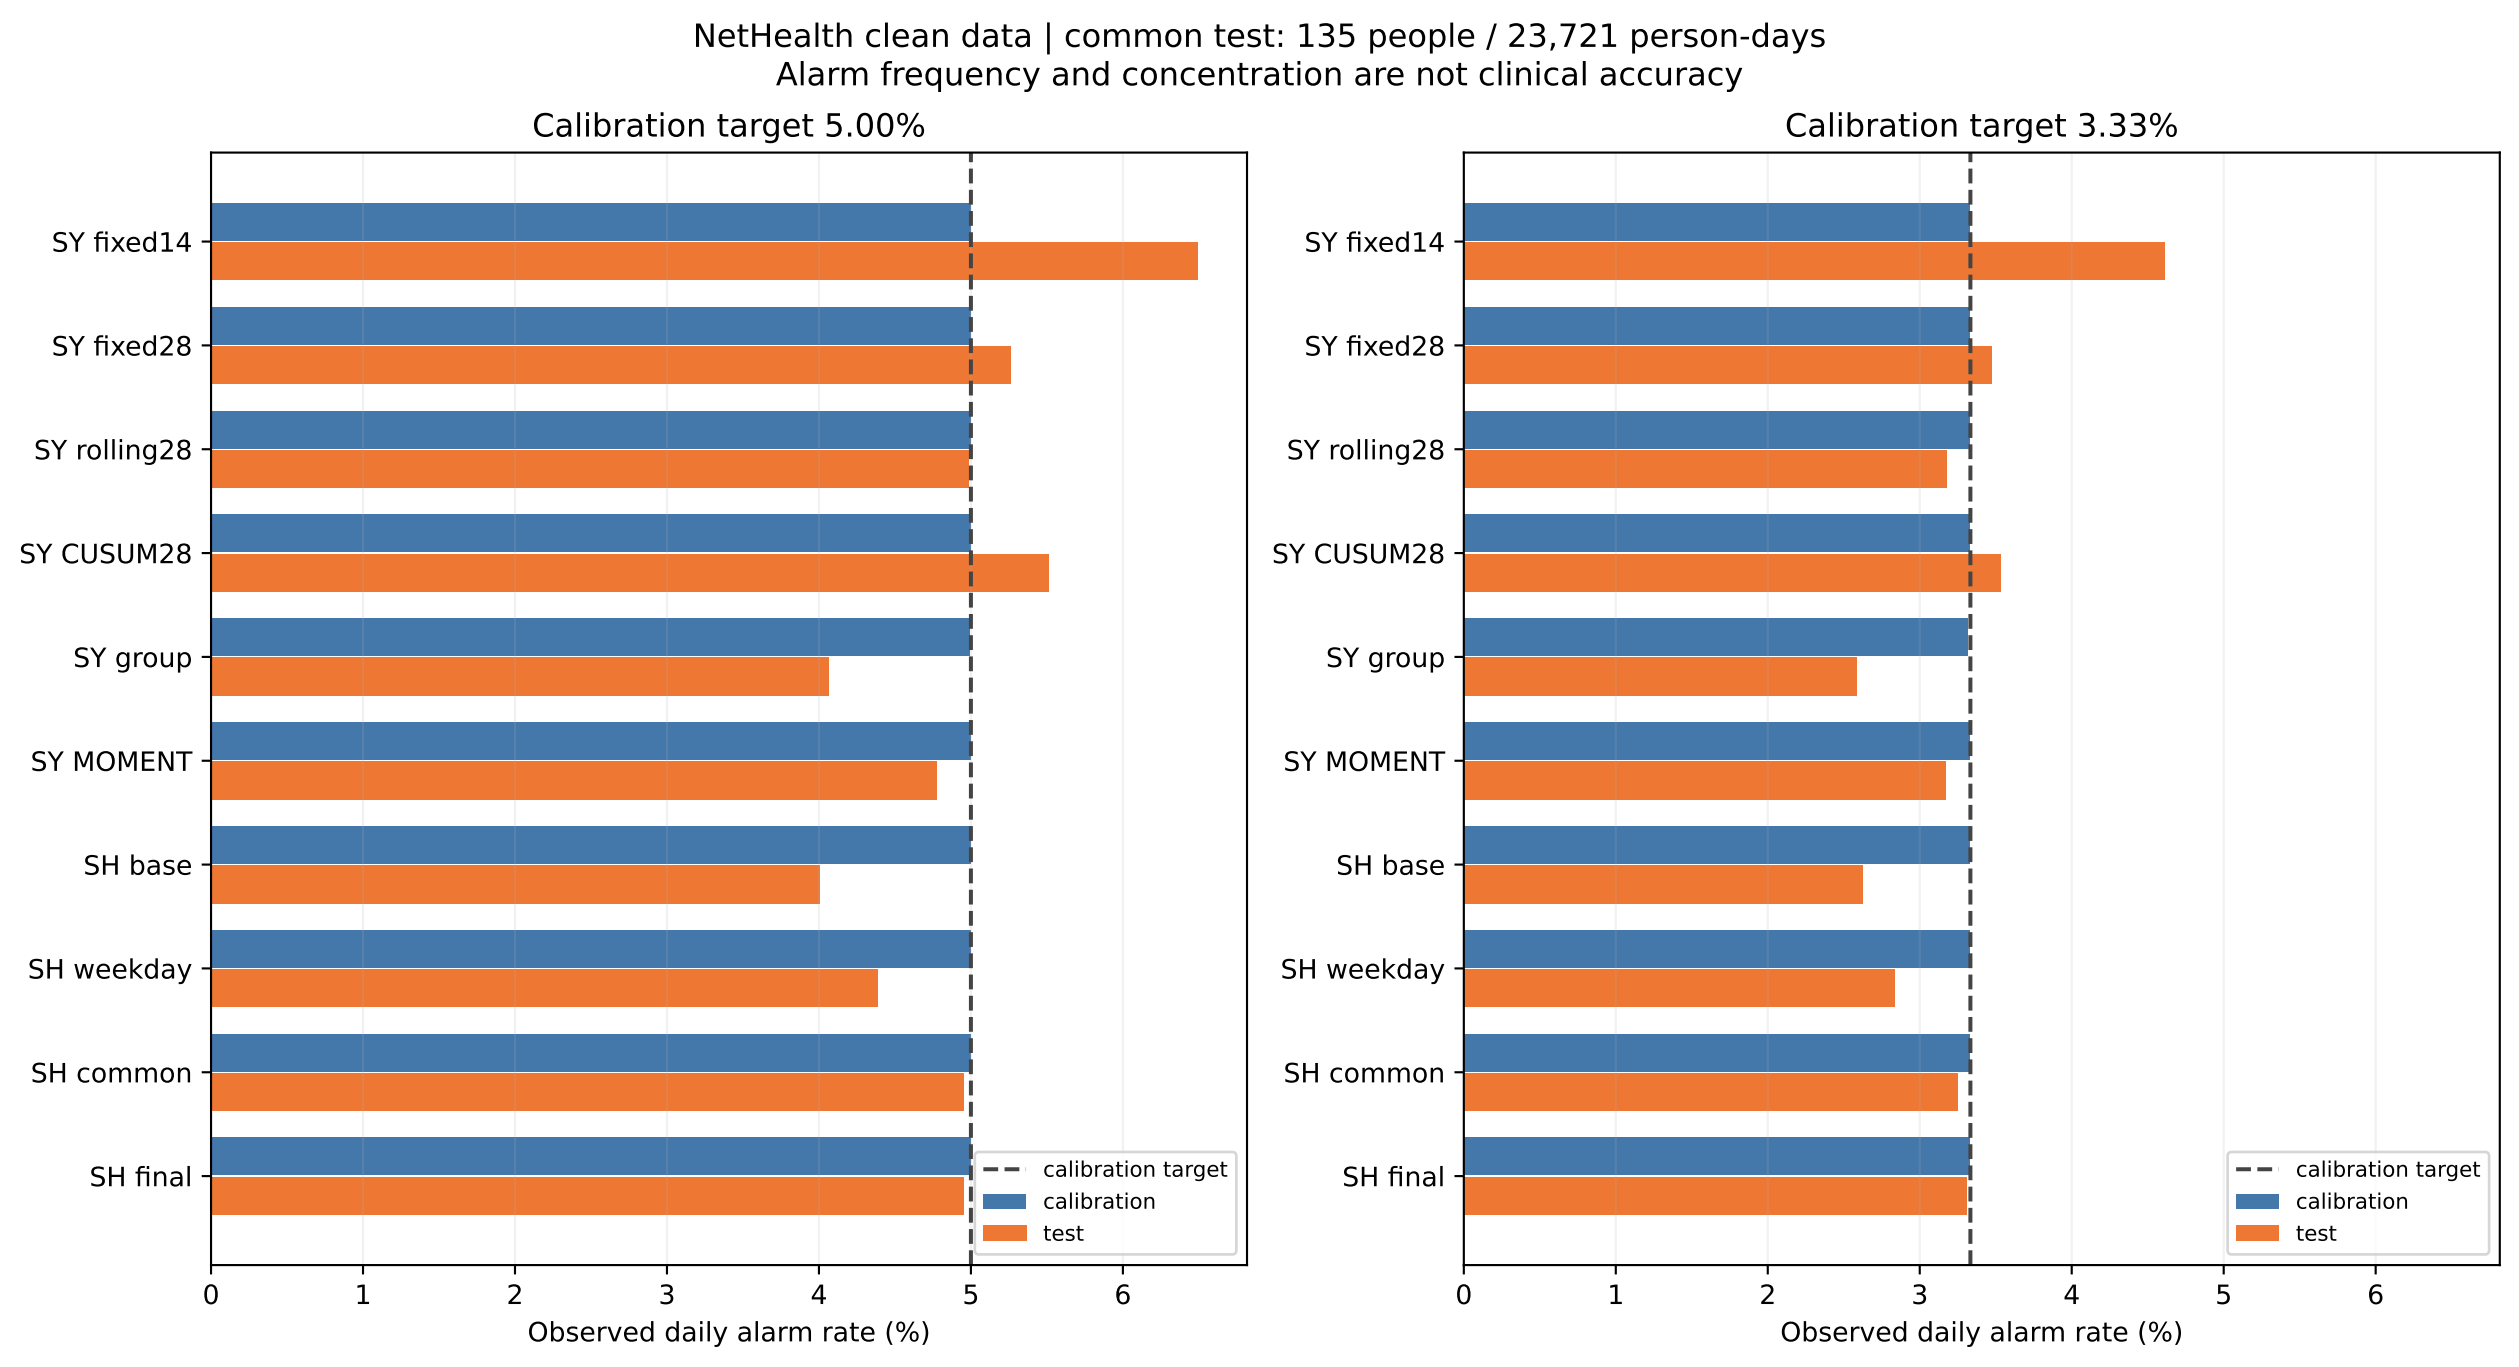
NetHealth clean data | common test: 135 people / 23,721 person-days
Alarm frequency and concentration are not clinical accuracy
Calibration target 5.00%
Calibration target 3.33%
SY fixed14
SY fixed28
SY rolling28
SY CUSUM28
SY group
SY MOMENT
SH base
SH weekday
SH common
SH final
calibration target
calibration
test
0
1
2
3
4
5
6
Observed daily alarm rate (%)