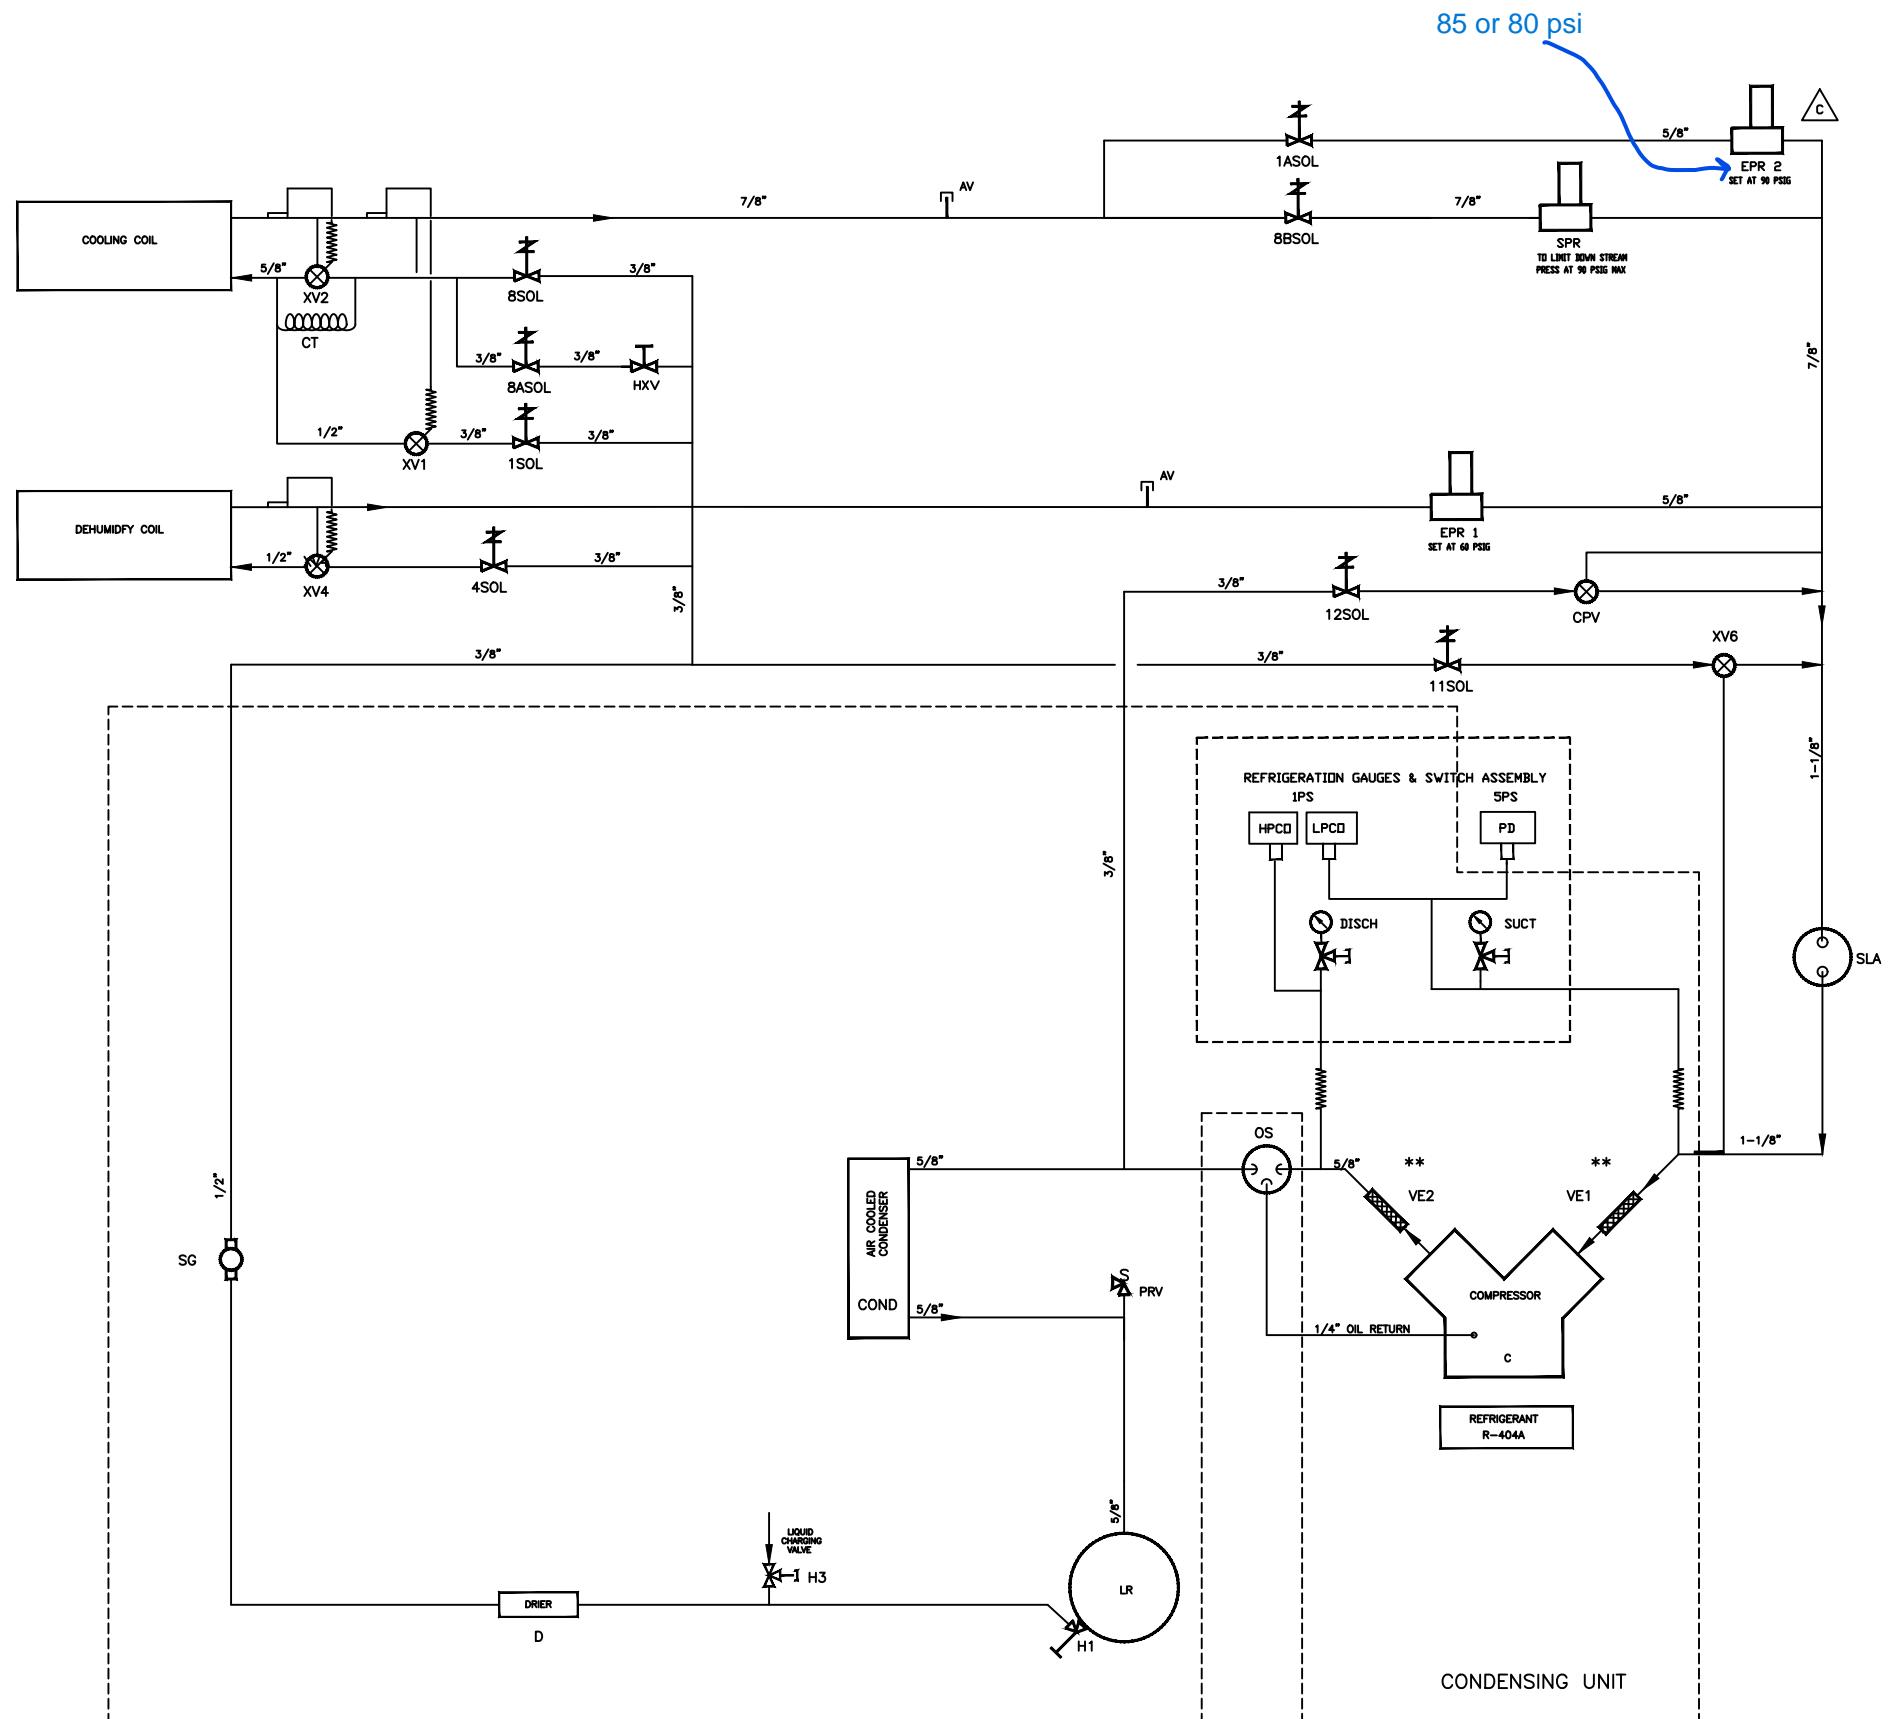


ITEM	QTY	DESCRIPTION	PART NO
--	--	--	--


**NOTES:**

1. REFER TO TAG SHEETS FOR COMPONENTS PART NUMBER.
2. ALL LINE SIZES ARE O.D. COPPER TUBE.
3. SOL'S VAL'S SHALL BE INSTALLED IN HORIZONTAL LINES ONLY.
4. CONDENSING UNIT RECEIVER PUMP DOWN: 14 LBS, R404A

C	REMOVED H6, ADDED EPR2	ACW	6/17/2024
B	ADDED PRV	CZT	6/08/10
A	CHANGED CU SCOPE TO REFLECT ACTUAL	CZT	3/30/10
TOLERANCE: +/- .25"	REV	DESCRIPTION	BY DATE

TPS Thermal Product Solutions  
GRUENBERG • LUNAIRE • TENNEY • BLUE M • LINDBERG

NOTICE: THIS DRAWING IS THE PROPERTY OF THERMAL PRODUCT SOLUTIONS AND IS LOANED SUBJECT TO THE CONDITION THAT IT SHALL NOT BE REPRODUCED, COPIED, OR SUBMITTED TO OUTSIDE BUSINESS FOR EXAMINATION WITHOUT OUR CONSENT.

CUSTOMER: GENERAL ELECTRIC

P.O. NO. 3029393 R4 SHEET 1 REV 1  
QUOTE NO. 10255 Dwg No. D660 C  
DATE 4/13/2010 Model WTR32185D  
APP DATE 70410 Job No. 70410