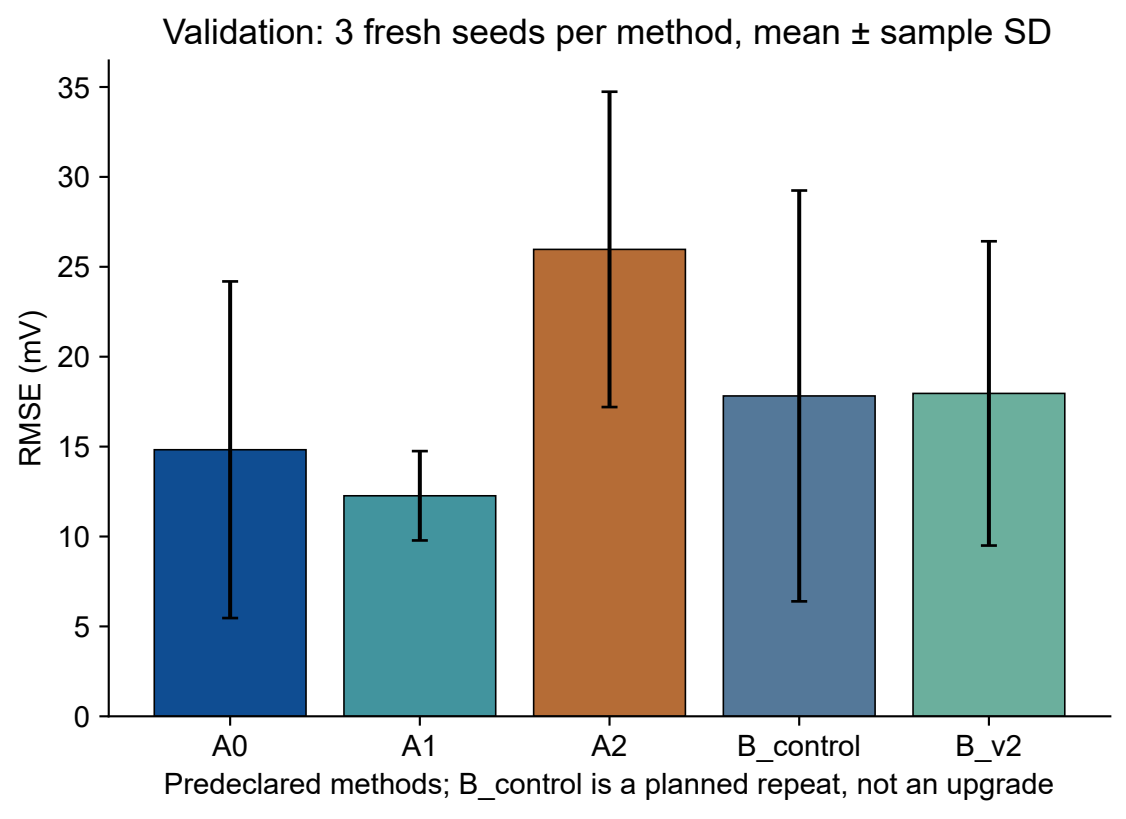
Validation: 3 fresh seeds per method, mean ± sample SD
RMSE (mV)
0
5
10
15
20
25
30
35
A0
A1
A2
B_control
B_v2
Predeclared methods; B_control is a planned repeat, not an upgrade

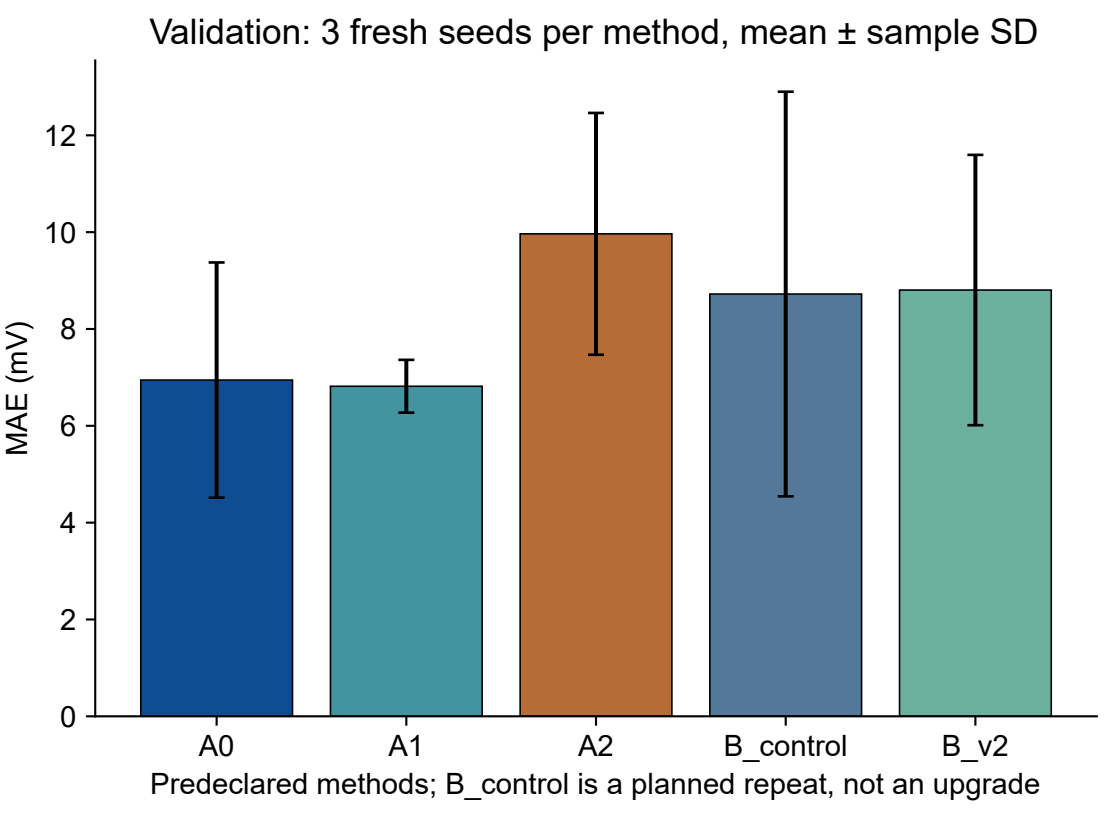
Validation: 3 fresh seeds per method, mean ± sample SD
MAE (mV)
0
2
4
6
8
10
12
A0
A1
A2
B_control
B_v2
Predeclared methods; B_control is a planned repeat, not an upgrade