

Polarized neutron diffraction with *ex-situ* ^3He neutron spin filter and two-dimensional detector for noncollinear incommensurate magnetic order

Shingo Takahashi,^{1,2} Yuta Osawa,¹ Ryuju Kobayashi,² Takashi Ino,³ Hiraku Saito,¹
Takuro Kawasaki,² Takayuki Oku,² Tatsuya Nakamura,² Yoichi Ikeda,⁴ Masaki Fujita,⁴
Daisuke Koto,⁵ Yusuke Tokunaga,⁵ Taka-hisa Arima,^{5,6} and Taro Nakajima^{1,3,6}

¹*Institute for Solid State Physics, The University of Tokyo, Kashiwa, Chiba 277-8581, Japan*

²*J-PARC Center, Japan Atomic Energy Agency, Tokai, Ibaraki 319-1195, Japan*

³*Institute of Materials Structure Science, High Energy Accelerator Research Organization, Tsukuba, Ibaraki 305-0801, Japan*

⁴*Institute for Materials Research, Tohoku University, Sendai, Miyagi 980-8577, Japan*

⁵*Department of Advanced Materials Science, The University of Tokyo, Kashiwa, Chiba 277-8561, Japan*

⁶*RIKEN Center for Emergent Matter Science, Wako, Saitama 351-0198, Japan*

Polarized neutron scattering has been widely used for studying magnetic orders in condensed matter. A typical setup for this technique is a triple-axis spectrometer with a ferromagnetic single-crystal monochromator and analyzer, which is suited for point-by-point measurements within the horizontal scattering plane. However, this setup cannot fully meet the demands of recent studies on complex magnetic orders with emergent cross-correlated phenomena. For instance, multiferroics, magnetic skyrmions, and other topologically nontrivial magnetic orders tend to have incommensurate magnetic modulation vectors running along various directions in reciprocal space, which cannot be captured by measurements restricted to the horizontal scattering plane. To overcome these limitations, we have developed an experimental setup combining a ^3He neutron spin filter (^3He -NSF) and a two-dimensional (2D) detector, which enables us to analyze the polarization of neutrons scattered away from the horizontal plane. We also establish a data reduction procedure to convert the 2D intensity maps into three-dimensional intensity distributions in reciprocal space, correcting for the effect of imperfect ^3He polarization. This method is applied to single-crystal diffraction measurements on the multiferroic material Mn_3WO_6 , which exhibits complex incommensurate magnetic orders. We have successfully observed polarization-dependent intensities of out-of-plane incommensurate magnetic reflections, demonstrating the effectiveness of the present method for analyzing complex magnetic structures.

I. INTRODUCTION

Polarized neutron scattering is a powerful technique for investigating magnetic order and excitations in condensed matter. This capability arises from the magnetic moment of neutron, which directly interacts with magnetic moments of electrons in the material through the magnetic dipole-dipole interaction. By analyzing the spin states of neutrons before and after scattering, one can separate magnetic scattering from nuclear scattering and determine the directions of magnetic moments in the sample. To perform these measurements, devices for controlling and probing the neutron polarization are required. To date, three techniques have been widely used for polarized neutron scattering. The first is a single crystal of ferromagnetic material, such as a Cu_2MnAl Heusler compound. By exploiting the nuclear-magnetic interference effect, which gives rise to different Bragg reflectivities for two neutron spin states, a polarized monochromatic neutron beam can be obtained [1]. The second is a polarizing supermirror, which utilizes the difference in critical angle between neutrons with different spin states [2]. The third is a polarizing filter, utilizing the strong spin dependence of the neutron absorption cross section of ^3He nuclei (^3He neutron spin filter, ^3He -NSF) [3]. Among these techniques, the ferromagnetic single-crystal monochromators are often used to polarize incident neutrons and analyze scattered neutrons in triple-axis spec-

trometers [4–8], as shown in Fig. 1(a). While this type of instrument has been widely used for studying magnetic structures, accessible reflections are often restricted to the horizontal scattering plane.

In recent years, increasing attention has been paid to materials hosting complex incommensurate magnetic orders, such as spin-driven multiferroics, magnetic skyrmions and related topological magnetic orders [9–13]. In these systems, the magnetic moments are often arranged in noncollinear or noncoplanar configurations, which can give rise to emergent cross-correlated phenomena. To study these systems, it is necessary to measure magnetic satellite reflections corresponding to magnetic modulation wavevectors (q -vectors), which often run along various directions in reciprocal space. Consequently, three-dimensional exploration of the reciprocal space with a two-dimensional (2D) detector is of great importance. To realize polarization analysis in the measurements with a 2D detector, polarization devices with a large solid-angle coverage, such as ^3He -NSF, are required.

The combination of a ^3He -NSF and a 2D detector has been implemented in several small-angle neutron scattering (SANS) instruments and applied to studies of complex magnetic structures [14, 15]. However, their accessible reciprocal space region is generally limited to relatively low- Q . To extend the accessible Q range for polarization analysis to middle- Q and high- Q regions, it would be necessary to place a ^3He -NSF and a 2D detector at

various scattering angles, as illustrated in Fig. 1(b). Related instrumental concepts have already been reported at several neutron facilities, including POLI at MLZ [16] and WOMBAT at ANSTO [17]. Nevertheless, quantitative experimental demonstrations of polarization analysis using this type of setup remain limited. The ^3He -NSF has also been used in the two-axis diffractometer D1B at ILL [18]. This instrument has a one-dimensional (1D) array of detectors, which can cover a wide range of the scattering angle in a horizontal plane, and is dedicated to powder diffraction measurements. As for inelastic scattering instruments, the ^3He -NSFs have been used in MACS at NIST [19–21] and LET at ISIS [22, 23]; the former and latter have 1D and 2D detectors, respectively. It should be mentioned that another neutron inelastic spectrometer HYSPEC in ORNL also has polarization analysis capability using not ^3He -NSF but radial supermirror analyzers and 2D detectors [24]. These extensive developments of polarized neutron instruments indicate a growing demand for polarized neutron measurements in condensed matter physics.

In the present study, we performed polarized neutron diffraction measurements combining a ^3He -NSF and a 2D detector on the 5G beamport at JRR-3. This paper mainly describes the experimental setup, the measurement procedures, and corrections for the effects of imperfect neutron polarization. We also performed polarized neutron diffraction on a single crystal of Mn_3WO_6 , which exhibits incommensurate magnetic orders. This compound has a crystal structure belonging to the space group $R\bar{3}$ and displays two magnetically ordered phases at low temperatures [25]. As we describe in the following sections, we focus on the data measured at 23 K, which corresponds to the higher-temperature magnetic phase. We performed polarization analysis for magnetic reflections that were slightly shifted from the horizontal plane. The details of the magnetic structure will be reported elsewhere [26].

II. EXPERIMENTAL DETAILS

A. Setup

The 5G beamport at JRR-3 is normally operated as the Polarized Neutron Triple-Axis spectrometer (PONTA), which has a longitudinal polarization analysis option with a conventional Heusler polarizing monochromator and analyzer [8]. In the present experiment, the Heusler analyzer and the point detector were replaced with a ^3He -NSF and a 2D detector. The Heusler polarizing monochromator provided a polarized incident neutron beam with an energy of 14.7 meV. The higher-order reflections from the monochromator were suppressed by a pyrolytic graphite filter placed between the monochromator and the sample.

Figure 2 shows an overview of the experimental setup between the sample and the detector. Scattered neu-

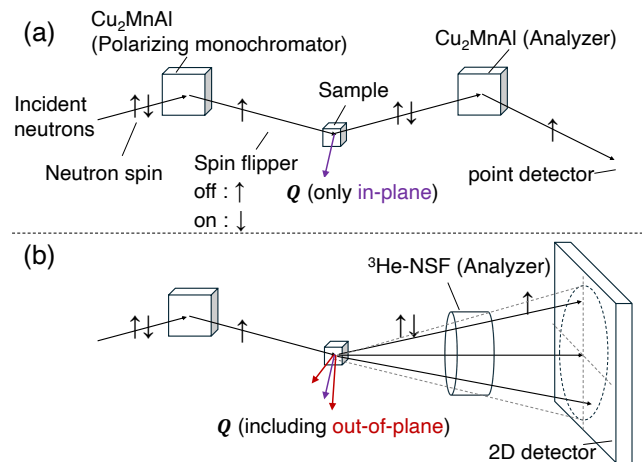


FIG. 1. Schematic illustrations comparing neutron polarization analysis techniques. (a) Conventional setup using Heusler crystals for both the polarizer and the analyzer, where only in-plane scattered neutrons are detected by a point detector. (b) Polarization analysis setup combining a ^3He -NSF and a 2D detector, enabling detection of both in-plane and out-of-plane scattered neutrons.

trons were detected using a scintillation-type 2D detector employing wavelength-shifting fiber readout [27, 28]. The active area was $256 \times 256 \text{ mm}^2$, consisting of 64×64 channels with a channel pitch of 4 mm. To access the target reflections, the detector was positioned at an angle of 32° from the incident direction throughout the experiment. The sample-to-detector distance was 915 mm. A ^3He -NSF was installed 430 mm downstream of the sample. The cylindrical ^3He cell provided an angular acceptance of $\pm 4.0^\circ$, which corresponded to a circular region with a radius of 76 mm (approximately 19 channels) centered on the detector. Polarization analysis of the scattered neutrons was possible only within this region. To reduce the background, a B_4C -shielded neutron guide tube was installed between the ^3He -NSF and the detector, and B_4C shielding was also attached around the ^3He -NSF coil. The non-spin-flip and spin-flip intensities of the scattered neutrons were obtained by flipping the ^3He polarization using an adiabatic fast passage nuclear magnetic resonance (AFP NMR). Therefore, the neutron spin flipper for the incident beam was not used. A Helmholtz coil was used to maintain the neutron spin polarization along the neutron flight path by applying a vertical magnetic field. The magnetic field in the ^3He -NSF was oriented parallel to the beam axis, and the spins of neutrons scattered from the sample adiabatically followed the field direction, as illustrated in Fig. 2. The magnetic field strength generated by both the ^3He -NSF coil and the Helmholtz coil was approximately 1 mT.

A single-crystal sample of Mn_3WO_6 with a volume of 8 mm^3 was mounted on an aluminum holder and installed in a ^4He closed-cycle refrigerator. This compound has

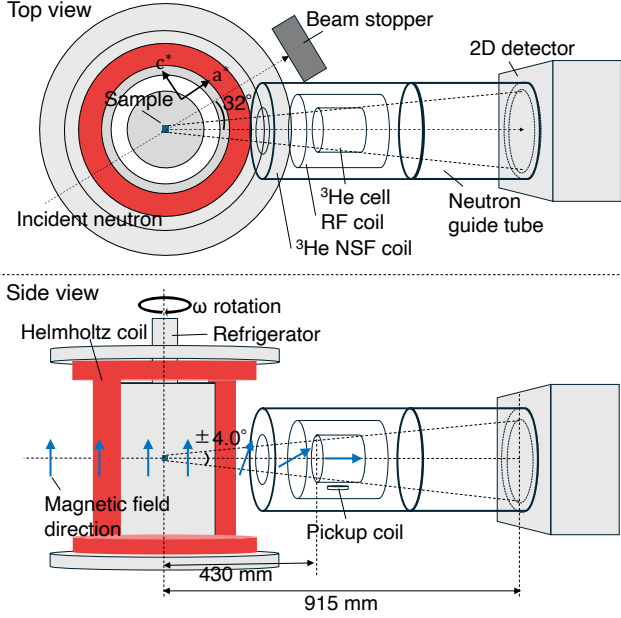


FIG. 2. Schematic illustration of the experimental setup on the 5G beamport. Scattered neutrons from the sample pass through the ^3He -NSF coil and the neutron guide tube before reaching the 2D detector. The sample is mounted in a cryostat whose rotation angle is denoted by ω . The magnetic field direction induced by the Helmholtz coil is vertical, whereas the field within the ^3He -NSF is oriented along the beam axis. The neutron spins are adiabatically rotated to follow the field direction. A radio-frequency (RF) coil is used to flip the ^3He polarization, and an NMR pickup coil monitors the ^3He polarization after each spin flip.

a rhombohedral crystal structure belonging to the space group of $R\bar{3}$. The lattice constants were reported to be $a = 8.8905(6)$ Å and $c = 10.4734(8)$ Å in the hexagonal setting [25]. The $(H, 0, L)$ plane was aligned with the horizontal scattering plane. The sample rotation angle ω about the vertical axis was adjusted for each target reflection to satisfy the corresponding Bragg condition.

B. ^3He neutron spin filter

In this section, we describe the ^3He -NSF employed in the present experiment in detail. Neutrons with spins antiparallel to the ^3He nuclear spins are strongly absorbed, while those with spins parallel to the ^3He nuclear spins are transmitted. Thus, neutrons are polarized by passing through the polarized ^3He gas, and neutron polarization and transmission depend on the ^3He polarization. The two major methods for polarizing ^3He nuclei are spin-exchange optical pumping (SEOP) [29] and metastability-exchange optical pumping (MEOP) [30]. In the present study, we employed the SEOP method. In the SEOP method, generally, a glass cell is filled with ^3He , N_2 , and a small amount of alkali metal. The cell

is irradiated with circularly polarized light resonant with an optical transition of the alkali metal. The alkali-metal electrons undergo repeated excitation and de-excitation, with N_2 serving as a quenching gas to suppress radiative decay, resulting in electron spin polarization. The polarization of the alkali metal is then transferred to the ^3He nuclei via spin-exchange collisions, thereby achieving ^3He nuclear polarization. The SEOP system used in this study was a modified version of the system developed for the polarized neutron spectrometer POLANO, installed at BL23 in MLF of J-PARC [31]. Both the ^3He -NSF coil used for polarization analysis shown in Fig. 2 and the SEOP system were equipped with an AFP NMR system [32]. The AFP NMR system consisted of a radio-frequency (RF) coil for flipping the ^3He polarization and a pickup coil located at the bottom of the ^3He cell for monitoring the ^3He polarization. Two cylindrical ^3He glass cells, named Kenji and Shimpachi, made of aluminosilicate glass (GE180) with nearly identical dimensions, were used in this experiment. Both cells were filled with ^3He , N_2 , and a mixture of Rb and K for hybrid SEOP, which provided a higher pumping efficiency than Rb-only SEOP [33, 34]. The details of the cell specifications are described in Table I. A darkroom to house the SEOP laser system, where the ^3He gas was polarized, was constructed in the 5G beamport experimental area. After the ^3He polarization reached saturation, only the ^3He cell was transported to the ^3He -NSF coil on the beamline. Neutron measurements were performed during the relaxation of the ^3He polarization, with the neutron polarization and transmission decreasing. This technique is known as the *ex-situ* ^3He -NSF method. Since the ^3He polarization decreased with time, two cells were used alternately for the experiment. While one cell was used for the polarized neutron experiment, the other was polarized in the SEOP system. The cells were exchanged every two or three days.

III. DATA REDUCTION PROCEDURE INCLUDING POLARIZATION CORRECTION

Figure 3 shows the procedure for data acquisition, reduction, and polarization correction in the present study. At a sample rotation angle of $\omega = \omega_n$, we measured a pair of 2D intensity maps corresponding to non-spin-flip and spin-flip scattering by flipping the ^3He polarization. We refer to the observed intensities measured with the ^3He nuclear polarization parallel or antiparallel to the neutron polarization produced by the Heusler polarizer as I_{obs}^{++} and I_{obs}^{+-} , respectively. All intensity maps were normalized by the measurement time. In general, a full polarization analysis experiment, one would measure four scattering intensities, I^{++} , I^{+-} , I^{-+} , and I^{--} , corresponding to the four possible combinations of the polarizer and analyzer spin state [35]. These comprise two non-spin-flip channels, I^{++} and I^{--} , and two spin-flip channels, I^{+-} and I^{-+} . In the present experiment,

TABLE I. Specifications of ^3He cells.

Name	$D \times L$ (mm)	Volume (cm^3)	^3He density (amg)	N_2 pressure (Torr)	K/Rb (mol)
Kenji	72×67	140	3.2	97	26
Shimpachi	72×65	146	3.1	100	37

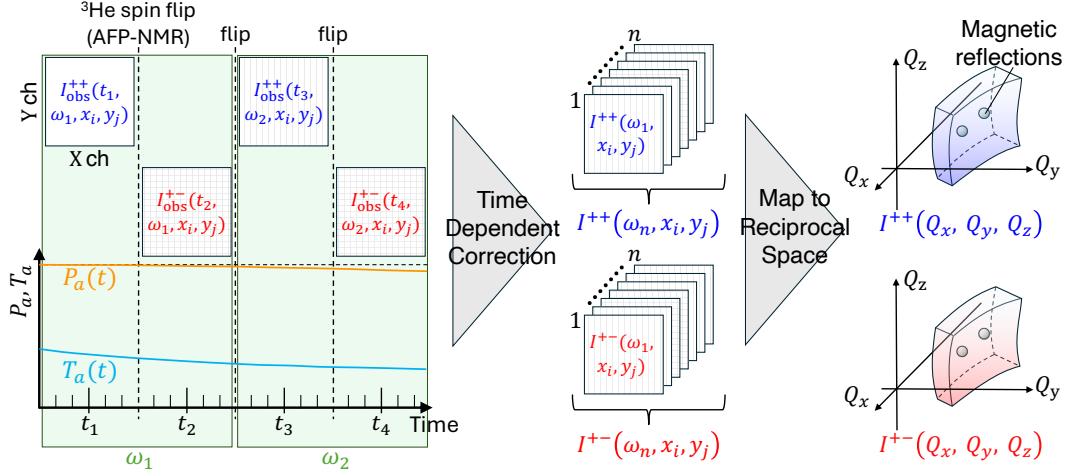


FIG. 3. Schematic diagram of the data-reduction procedure for polarization analysis using an *ex-situ* ^3He -NSF and a 2D detector. Raw 2D detector data measured at different sample rotation angles ω and times t are corrected for the time-dependent neutron polarization $P_a(t)$ and transmission $T_a(t)$ of the ^3He -NSF. The detector coordinates (X,Y) and sample rotation angle ω are converted to Q_x, Q_y, Q_z , and then transformed to H, K, L using the UB matrix. The corrected three-dimensional reciprocal-space data can then be sliced along an arbitrary plane.

the nuclear and magnetic reflections were spatially separated, and chiral magnetic scattering was negligible because the neutron polarization and the scattering vector were nearly perpendicular to each other [36]. We therefore assumed $I^{++} = I^{--}$ and $I^{+-} = I^{-+}$, allowing the polarization analysis to be performed using only the two measured channels. The corresponding treatment of imperfect polarization is described in Appendix A. Each intensity map was measured for 20 min, which was suf-

ficiently short compared with the relaxation time of the ^3He polarization. The transmission and neutron polarization of the ^3He -NSF during each measurement were therefore approximated by their values at the midpoint of the measurement. As shown in the left panel of Fig. 3, the midpoint times of two successive measurements at $\omega = \omega_n$ are denoted by t_{2n-1} and t_{2n} . Using this notation, the observed intensities at detector pixel (x_i, y_j) are expressed as

$$I_{\text{obs}}^{++}(\omega_n, t_{2n-1}, x_i, y_j) = T_p T_a(t_{2n-1}) \left[(1 + P_p P_a(t_{2n-1})) I^{++}(\omega_n, x_i, y_j) + (1 - P_p P_a(t_{2n-1})) I^{+-}(\omega_n, x_i, y_j) \right] + \text{BG}(x_i, y_j), \quad (1)$$

$$I_{\text{obs}}^{+-}(\omega_n, t_{2n}, x_i, y_j) = T_p T_a(t_{2n}) \left[(1 - P_p P_a(t_{2n})) I^{++}(\omega_n, x_i, y_j) + (1 + P_p P_a(t_{2n})) I^{+-}(\omega_n, x_i, y_j) \right] + \text{BG}(x_i, y_j), \quad (2)$$

where $I^{++}(\omega_n, x_i, y_j)$ and $I^{+-}(\omega_n, x_i, y_j)$ are the ideal non-spin-flip and spin-flip scattering intensities, respectively. T_p and $T_a(t)$ denote the neutron reflectance of the

Heusler polarizer and the transmission of the ^3He -NSF, respectively. P_p and $P_a(t)$ are the neutron polarizations produced by the Heusler polarizer and ^3He -NSF, respec-

tively. Note that the transmission and the polarization are defined for an incident unpolarized neutron beam. For the Heusler polarizer, T_p is defined as the ratio of the Bragg-reflected intensity to the incident unpolarized neutron intensity. Although $P_a(t)$ is generally defined as a signed quantity ranging from -1 to $+1$, we define it as its magnitude, $0 \leq P_a(t) \leq 1$. Instead, the parallel and antiparallel orientations of the ^3He polarization relative to the incident neutron polarization is represented by the sign in the factor $1 \pm P_p P_a(t)$ in Eqs. 1 and 2. The quantities T_p and P_p were treated as time-independent, whereas $T_a(t)$ and $P_a(t)$ were time-dependent because of the re-

laxation of the ^3He nuclear polarization. $\text{BG}(x_i, y_j)$ is the background intensity at the detector pixel (x_i, y_j) . In the present experiment, the background signals were mainly due to imperfect shielding of the detector and the neutron flight path. Thus, we assumed that the background signals were independent of time, ^3He polarization, and the sample rotation angle ω . We measured the $\text{BG}(x_i, y_j)$ by setting the ω angle away from any Bragg reflections from the sample. We repeated the measurements of I_{obs}^{++} and I_{obs}^{+-} while varying the sample rotation angle ω .

By solving Eqs. 1 and 2 for I^{++} and I^{+-} , we obtain the equations of the polarization correction for the dataset measured at $\omega = \omega_n$ as follows:

$$I^{++}(\omega_n, x_i, y_j) = \frac{1 + P_p P_a(t_{2n})}{2T_p T_a(t_{2n-1}) P_p [P_a(t_{2n-1}) + P_a(t_{2n})]} [I_{\text{obs}}^{++}(\omega_n, t_{2n-1}, x_i, y_j) - \text{BG}(x_i, y_j)] - \frac{1 - P_p P_a(t_{2n-1})}{2T_p T_a(t_{2n}) P_p [P_a(t_{2n-1}) + P_a(t_{2n})]} [I_{\text{obs}}^{+-}(\omega_n, t_{2n}, x_i, y_j) - \text{BG}(x_i, y_j)], \quad (3)$$

$$I^{+-}(\omega_n, x_i, y_j) = -\frac{1 - P_p P_a(t_{2n})}{2T_p T_a(t_{2n-1}) P_p [P_a(t_{2n-1}) + P_a(t_{2n})]} [I_{\text{obs}}^{++}(\omega_n, t_{2n-1}, x_i, y_j) - \text{BG}(x_i, y_j)] + \frac{1 + P_p P_a(t_{2n-1})}{2T_p T_a(t_{2n}) P_p [P_a(t_{2n-1}) + P_a(t_{2n})]} [I_{\text{obs}}^{+-}(\omega_n, t_{2n}, x_i, y_j) - \text{BG}(x_i, y_j)]. \quad (4)$$

As we show later, we also experimentally determined the neutron polarizations produced by the polarizer and the analyzer, P_p and $P_a(t)$, and the transmission of the analyzer, $T_a(t)$, including the temporal decay of the ^3He polarization. Since T_p is time-independent, it was instead treated as a constant scale factor. Substituting all the parameters into the equations above, we corrected the effect of imperfect polarization for all the pixels.

Finally, we converted the detector coordinates and sample rotation angle (x_i, y_j, ω_n) into reciprocal-space coordinates (Q_x, Q_y, Q_z) . The resulting data were further transformed into (H, K, L) coordinates using the UB matrix, allowing the intensity distribution to be sliced along an arbitrary plane in reciprocal space.

IV. RESULTS

A. Evaluation of ^3He neutron spin filter from nuclear scattering

The ^3He polarization was evaluated by measuring a nuclear Bragg peak. Specifically, we selected the $\bar{1}02$ reflection, which has a similar scattering angle to that of the magnetic reflections of interest. The neutron transmission $T_a(t)$, the neutron polarization $P_a(t)$, and the ^3He polarization $P_{\text{He}}(t)$ are given by the following equa-

tions [37]:

$$T_a(t) = T_{\text{cell}} \exp(-\mathcal{O}) \cosh(\mathcal{O} P_{\text{He}}(t)), \quad (5)$$

$$P_a(t) = \tanh(\mathcal{O} P_{\text{He}}(t)), \quad (6)$$

$$P_{\text{He}}(t) = P_{\text{He}}(0) \exp(-t/\tau). \quad (7)$$

Here, T_{cell} is the transmission of the glass walls of the ^3He cell. $\mathcal{O}$ is the opacity of the ^3He cell, defined as $\mathcal{O} = \rho d \sigma$. ρ is the number density of ^3He , and d is the neutron path length through the ^3He cell, which depends on the positions of the detector pixels. σ is the neutron absorption cross section of unpolarized ^3He , which depends on the incident neutron energy. According to the literature, σ for the incident neutron energy of 14.7 meV is 6997 barn [38]. $P_{\text{He}}(0)$ is the initial polarization at $t = 0$, and τ is the relaxation time.

First, the areal density ρd of each cell was determined as follows. Before polarizing ^3He by SEOP, we measured the nuclear peak through the unpolarized ^3He cell with ω fixed at the Bragg condition. From the intensity map, we extracted a box-integrated intensity near the peak. After subtracting the background signals, we obtained the integrated intensity of the Bragg reflection, $\mathcal{I}_{\text{obs}}^{\text{unpol}}$. By using Eqs. 1, 5, and 7, and assuming that the ^3He polarization is zero ($P_{\text{He}}(t) = 0$), $\mathcal{I}_{\text{obs}}^{\text{unpol}}$ is expressed as follows:

$$\mathcal{I}_{\text{obs}}^{\text{unpol}} = \sum_{(i,j) \in R} T_p T_{\text{cell}} \exp(-\mathcal{O}) I^{++}(x_i, y_j). \quad (8)$$

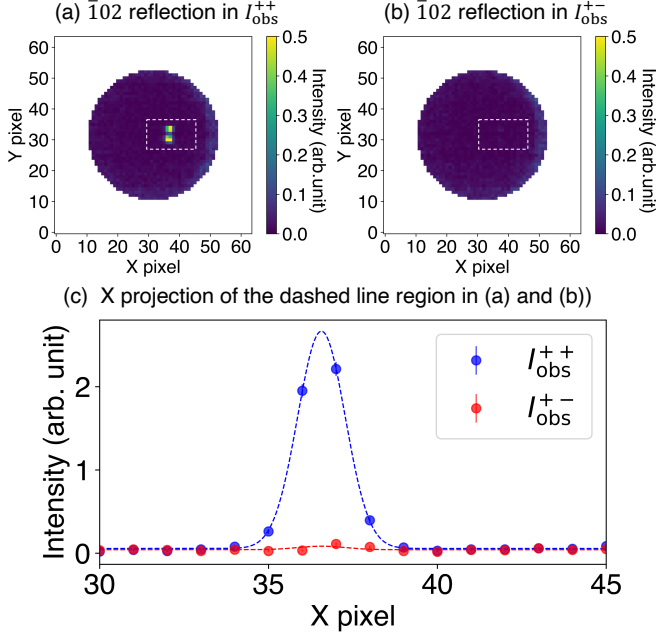


FIG. 4. (a) Observed non-spin-flip (I_{obs}^{++}) and (b) spin-flip (I_{obs}^{+-}) intensity maps, showing only the analyzing region. (c) Line profile along the X direction, obtained by integrating the intensity within the rectangular regions indicated by the dashed lines in (a) and (b).

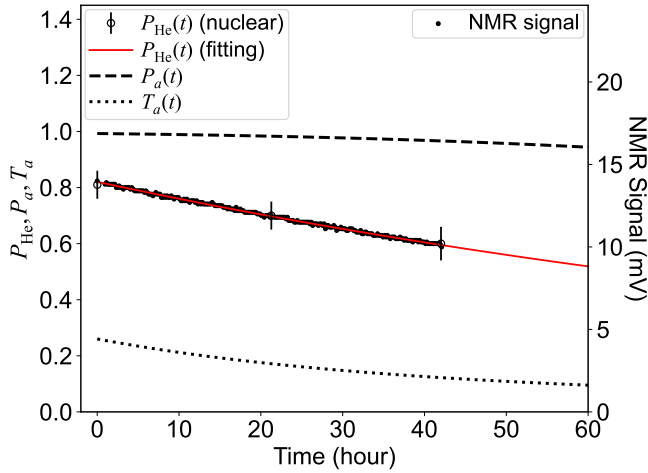


FIG. 5. Time dependence of the ^3He polarization, neutron polarization, and neutron transmission. The open circles show the ^3He polarization determined from the intensity of the $\bar{1}02$ nuclear reflection, while the closed circles show the NMR signal. The NMR signal was normalized to the initial ^3He polarization determined from the reflection. The red line represents the fitting result using Eq. 7. The dashed and dotted lines indicate the calculations for $P_a(t)$ and $T_a(t)$, respectively, obtained from $P_{\text{He}}(t)$.

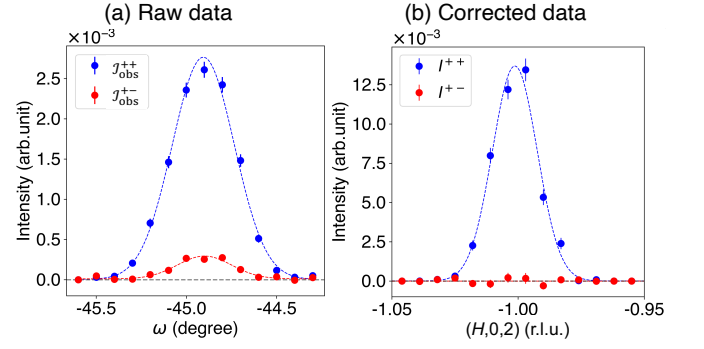


FIG. 6. (a) Raw non-spin-flip and spin-flip intensities, $\mathcal{I}_{\text{obs}}^{++}$ (red) and $\mathcal{I}_{\text{obs}}^{+-}$ (blue), obtained by integrating the peak intensity on the 2D detector while scanning the sample rotation angle ω . (b) Corrected non-spin-flip and spin-flip scattering intensities, $I^{++}(H, K, L)$ (red) and $I^{+-}(H, K, L)$ (blue) in reciprocal space. The data were obtained by slicing along the $(H, 0, 2)$ line in the three-dimensional reciprocal space and integrating over a thickness of ± 0.025 r.l.u. along the $(K/2, -K, 0)$ direction, which is perpendicular to the horizontal $(H0L)$ scattering plane, and over ± 0.03 r.l.u. along the L direction.

where R denotes the box-integrated region. Note that the nuclear Bragg reflection contains only the non-spin-flip scattering intensity, and thus we can impose $I^{+-} = 0$ in Eq. 1. The same measurement was performed using an empty cell with the same dimensions as the ^3He glass cell, yielding $\mathcal{I}_{\text{obs}}^{\text{empty}}$. Here, the transmission term $T_{\text{cell}} \exp(-\mathcal{O})$ is replaced by T_{cell} . Then, taking the ratio $\mathcal{I}_{\text{obs}}^{\text{unpol}}/\mathcal{I}_{\text{obs}}^{\text{empty}}$, the ρd values of the Kenji and Shim-pachi cells were determined to be 18.5 ± 0.5 amg cm and 18.8 ± 0.4 amg cm, respectively. Note that the amagat is a non-SI unit of the volumetric number density of an ideal gas at 0°C (273.15 K) and 1 atm (101.325 kPa), and one amagat is equivalent to $2.69 \times 10^{19}/\text{cm}^3$. The ρd values determined here correspond to the path lengths through the ^3He gas at the pixel positions of the detected nuclear peaks, and the path length d varies with pixel position. However, the solid angle covered by the cell was sufficiently small (up to 4°) that the variation in d could be neglected. Therefore, these ρd values were used for all pixels included in the present data analysis. T_{cell} was determined to be 0.91 ± 0.04 by comparing the nuclear peak intensities measured without the cell with the empty cell. This value was not directly used in the polarization analysis.

Second, we determined $P_{\text{He}}(0)$ in Eq. 7 by measuring the nuclear reflection with the polarized ^3He cell. Immediately after moving the ^3He cell from the SEOP system to the beamline, we measured the intensities of the reflection with the ^3He polarization parallel and antiparallel to the incident neutron polarization. The integrated intensities were obtained following the same procedure as that used for the measurement with the unpolarized ^3He cell. These are referred to as $\mathcal{I}_{\text{obs}}^{++}(t=0)$ and $\mathcal{I}_{\text{obs}}^{+-}(t=0)$,

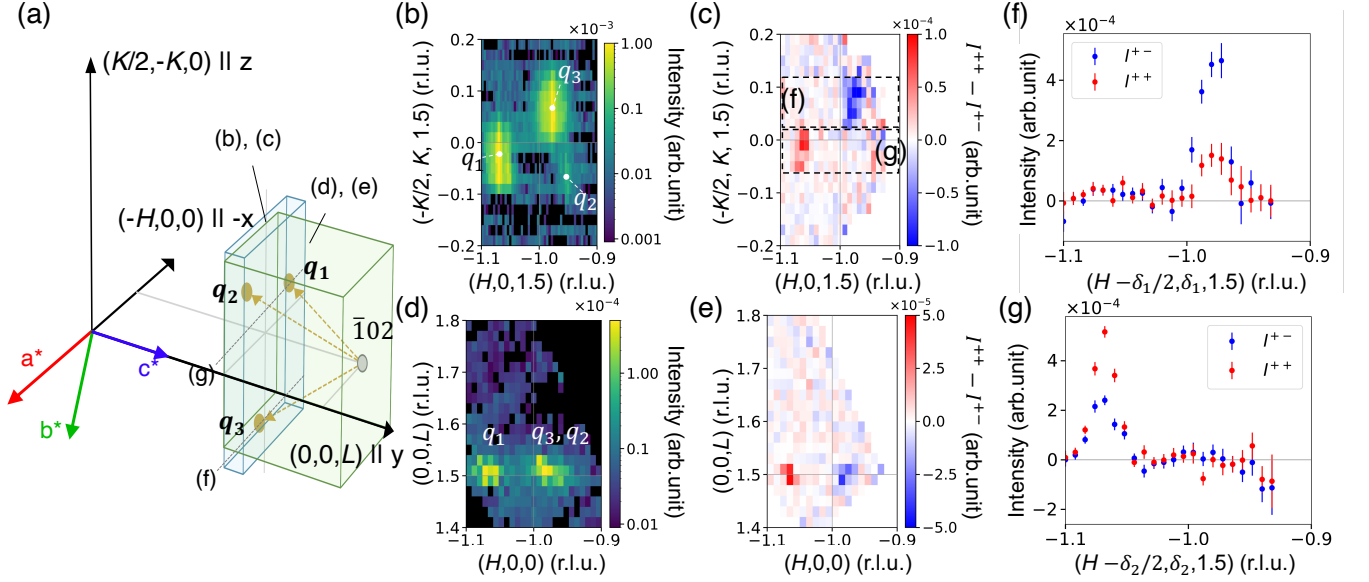


FIG. 7. (a) Schematic illustration of the reciprocal-space region measured in the present experiment. The translucent volumes labeled (b), (c) and (d), (e) indicate the regions integrated along the L direction and the $(-K/2, K, 0)$ direction, respectively. The dotted lines along the $-H$ direction through q_3 and q_1 indicate the line cuts shown in panels (f) and (g), respectively. (b), (d) Unpolarized neutron intensity maps in the $(H, K, 1.5)$ and $(H, 0, L)$ planes, respectively. (c), (e) Polarization-analysis maps obtained from the difference between the corrected non-spin-flip and corrected spin-flip intensities, $I^{++} - I^{+-}$. The intensity maps in the $(H, K, 1.5)$ plane shown in (b) and (c) were obtained from the three-dimensional reciprocal space data by integrating over $1.47 \leq L \leq 1.52$ r.l.u. Similarly, the intensity maps in the $(H, 0, L)$ plane shown in (d) and (e) were obtained by integrating along the $(-1/2, 1, 0)$ direction over the range of ± 0.1 r.l.u. (f), (g) Line profiles of I^{++} and I^{+-} through q_3 and q_1 , respectively, obtained by projecting the intensities within the dotted boxes in (c) onto the horizontal axis. Here, the coordinate along the $(-1/2, 1, 0)$ direction is parameterized by δ , such that the horizontal axis is given by $(H - \delta/2, \delta, 1.5)$. The projected ranges were $0.015 \leq \delta_1 \leq 0.095$ for (f) and $-0.07 \leq \delta_2 \leq 0.02$ for (g).

respectively. Since these measurement times were much shorter than the ^3He relaxation time, the ^3He polarizations for the two measurements were assumed to be equal. As shown in Fig. 4, we clearly observed the nuclear Bragg peak in the non-spin-flip channel, while the intensity in the spin-flip channel was extremely weak. Note that the peak in Fig. 4(a) shows a slight splitting due to the mosaicity of the single-crystal sample. From Eqs. 1, 2, 5, and 8, the ^3He polarization $P_{\text{He}}(t)$ at $t = 0$ satisfies the following relationship:

$$\frac{\mathcal{I}_{\text{obs}}^{++}(t=0) + \mathcal{I}_{\text{obs}}^{+-}(t=0)}{\mathcal{I}_{\text{obs}}^{\text{unpol}}} = 2 \cosh(OP_{\text{He}}(0)). \quad (9)$$

We measured the nuclear Bragg reflection to estimate $P_{\text{He}}(0)$ each time the cell was changed. For instance, the initial ^3He polarization of Shimpachi cell was determined to be $P_{\text{He}}(0) = 0.81 \pm 0.05$.

We then measured the relaxation of the ^3He polarization by tracking the NMR signal of the ^3He -NSF, which is proportional to the ^3He polarization. Throughout the neutron diffraction measurement, the NMR signal was recorded each time the ^3He polarization was flipped. Figure 5 shows the time dependence of the NMR signal of Shimpachi cell. By normalizing the NMR data to the $P_{\text{He}}(0)$ determined by the nuclear reflection, we obtained

the ^3He polarization as a function of time. We fitted Eq. 7 to the normalized NMR data and obtained P_{He} as shown by the red solid curve in Fig. 5. The relaxation times τ for Shimpachi and Kenji cells were determined to be $\tau = 131.1 \pm 0.7$ and $\tau = 128.4 \pm 0.3$ hours, respectively. We also measured the nuclear Bragg reflection several times during the experiment, confirming that the values of the ^3He polarization deduced from the measurements of the nuclear reflection and the NMR signal showed good agreement. The time evolutions of $T_a(t)$ and $P_a(t)$ were also obtained using Eqs. 5, 6, and 7, as shown in Fig. 5.

The neutron polarization produced by the Heusler polarizer, P_p , was also determined from the integrated intensities of the nuclear reflection. From Eqs. 1 and 2, the asymmetry between $\mathcal{I}_{\text{obs}}^{++}$ and $\mathcal{I}_{\text{obs}}^{+-}$ after subtracting the background $\text{BG}(x_i, y_j)$ from each is given by

$$\frac{\mathcal{I}_{\text{obs}}^{++} - \mathcal{I}_{\text{obs}}^{+-}}{\mathcal{I}_{\text{obs}}^{++} + \mathcal{I}_{\text{obs}}^{+-}} = P_p P_a(t). \quad (10)$$

Since $P_a(t)$ has already been determined from the ^3He polarization, P_p can be obtained from this equation. The values of P_p deduced from the measurements of the nuclear reflection were averaged, yielding $P_p = 0.86 \pm 0.06$. Note that P_p includes the effects of environmental back-

ground and neutron depolarization in the guide field.

To check the validity of the polarization correction, we measured the intensity distributions near the $\bar{1}02$ reflection while varying the ω angle. Figure 6(a) shows the observed box-integrated intensities, $\mathcal{I}_{\text{obs}}^{++}(\omega_n, t_{2n-1})$ and $\mathcal{I}_{\text{obs}}^{+-}(\omega_n, t_{2n})$. The polarization correction was not applied to these data. Non-zero I_{obs}^{+-} was observed owing to the imperfect neutron polarization of the polarizer and analyzer. Then, we applied the polarization correction to all the observed intensity maps and converted them into an intensity distribution in reciprocal space. Figure 6(b) shows the profiles of the corrected non-spin-flip and spin-flip intensities, I^{++} and I^{+-} , along the $(H, 0, 2)$ line, which were sliced from the three-dimensional data. This result indicates that the polarization correction was successfully performed. Details of the polarization correction are described in Appendix A.

B. Polarization analysis of magnetic scattering

We applied the polarization analysis with the ^3He -NSF and the 2D detector to the study of magnetic structures of Mn_3WO_6 . As mentioned in the introduction, this compound displays two antiferromagnetically ordered phases. In this paper, we focus on the high-temperature phase and show the data measured at 23 K. First, we determined the q -vector of the magnetic order by unpolarized neutron diffraction measurements with the 2D detector. The horizontal scattering plane was set to the $(H, 0, L)$ plane with the c axis perpendicular to the incident neutron beam. We measured intensity maps by scanning the ω angle from -52.9° to -46.0° in steps of 0.1° and converted the resulting data into reciprocal-space coordinates. Figure 7(d) shows the intensity distribution projected onto the $(H, 0, L)$ plane. We observed two incommensurate reflections near $(-1, 0, 1.5)$. To investigate the position of the reflections in more detail, we plotted the intensity distribution on the $(H, K, 1.5)$ plane, which is perpendicular to the horizontal plane, as shown in Fig. 7(b). This reveals three incommensurate peaks surrounding $(-1, 0, 1.5)$. One of the reflections (labeled q_1 in Fig. 7(b)) can be indexed using the q -vector $\mathbf{q}_1 = (0.059, 0.019, 0.5)$. The other two reflections can be indexed using $\mathbf{q}_2$ and $\mathbf{q}_3$, which are obtained by threefold rotations of $\mathbf{q}_1$ about the c^* axis. This relationship is consistent with the threefold rotational symmetry of the crystal structure about the c axis. Note that the unequal distribution of the magnetic intensities would be due to the orientations of the Fourier-transformed magnetic moments with respect to the direction of the scattering vector. We emphasize here that $\mathbf{q}_1$, $\mathbf{q}_2$, and $\mathbf{q}_3$ cannot lie within a single 2D plane passing through the reciprocal-space origin as shown in Fig. 7(a). This highlights the importance of three-dimensional reciprocal-space measurements for elucidating such complex incommensurate magnetic structures.

We thus measured the spin-flip and non-spin-flip in-

TABLE II. Measured and calculated asymmetries for the $(-1, 0, 2) - \mathbf{q}_1$ and $(-1, 0, 2) - \mathbf{q}_3$ reflections. The asymmetry is defined as $(I^{++} - I^{+-})/(I^{++} + I^{+-})$. The experimental values were obtained by integrating the line profiles shown in Figs. 7(f) and 7(g). The c -axis-parallel and oblique sinusoidal models of the magnetic moment $\mathbf{M}$ are illustrated in Figs. 8(a) and 8(b), respectively.

	$(-1, 0, 2) - \mathbf{q}_1$	$(-1, 0, 2) - \mathbf{q}_3$
Experiment values	0.30 ± 0.04	-0.49 ± 0.10
$\mathbf{M} \parallel c$ sinusoidal model ($\theta = 0^\circ$, $\phi = 0^\circ$)	-0.99	-0.99
Oblique sinusoidal model ($\theta = 49.5^\circ$, $\phi = 108.5^\circ$)	0.30	-0.50

tensity distributions around $(-1, 0, 1.5)$ using the ^3He -NSF. Figures 7(c) and 7(e) show the intensity difference $I^{++} - I^{+-}$ mapped onto the $(H, K, 1.5)$ and $(H, 0, L)$ planes, respectively. We clearly observed that the difference in intensity takes positive and negative values for the reflections $\mathbf{q}_1$ and $\mathbf{q}_3$, respectively. To compare the spin-dependent intensities more quantitatively, line profiles along the H direction were obtained by projecting the intensities within the dashed-box regions corresponding to $\mathbf{q}_3$ and $\mathbf{q}_1$ in Fig. 7(c). The resulting line profiles are shown in Figs. 7(f) and 7(g), respectively. At the reflection corresponding to $\mathbf{q}_3$, we found that the magnetic scattering intensity was dominated by spin-flip scattering, while at $\mathbf{q}_1$, the non-spin-flip scattering was more prominent. The asymmetry of the line profiles, defined as $(I^{++} - I^{+-})/(I^{++} + I^{+-})$, was calculated from the integrated intensities, and the results are summarized in Table II. Since the neutron polarization is parallel to the z axis defined in Fig. 7(a), the spin-flip scattering arises from the Fourier-transformed magnetization components in the xy plane, which contains the a and c axes. If the magnetic moments have only a c -axis component, as illustrated in Fig. 8(a), the calculated asymmetry is -0.99 for both reflections. In this case, both reflections would appear predominantly in the spin-flip channel, which is inconsistent with the experimental results. We therefore considered an oblique sinusoidal model, as illustrated in Fig. 8(b). The moment direction is specified by the polar angle θ , measured from the c axis, and the azimuthal angle ϕ , measured from the a axis. A least-squares analysis was performed to determine θ and ϕ , yielding $\theta = 49.5^\circ$ and $\phi = 108.5^\circ$. A more detailed structural analysis, including data from other regions of reciprocal space, will be reported elsewhere [26]. The present results demonstrated that polarized neutron scattering with a ^3He -NSF and a 2D detector is quite useful for solving complex incommensurate magnetic structures.

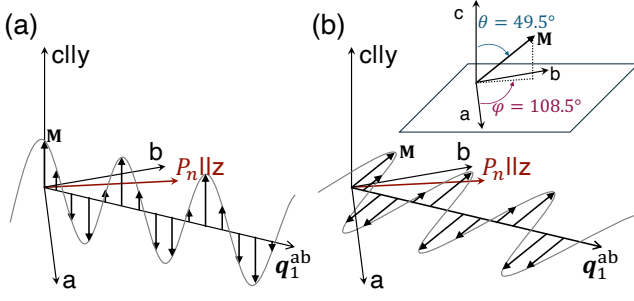


FIG. 8. Schematic illustrations of the sinusoidal magnetic structures. (a) the c -axis-parallel sinusoidal model and (b) the oblique sinusoidal model. The q_1^{ab} vector is the projection of the magnetic propagation vector q_1 onto the ab plane. The P_n vector is the neutron polarization direction, which is parallel to the z axis in Fig. 7(a). Inset of the panel (b) shows the definition of the polar angle θ and azimuthal angle ϕ . In the oblique sinusoidal model, the magnetic moment direction $\mathbf{M}$ is specified by $\theta = 49.5^\circ$ and $\phi = 108.5^\circ$.

V. SUMMARY AND OUTLOOK

In this work, we demonstrated polarized neutron diffraction measurements combining the ^3He -NSF and the 2D detector to explore three-dimensional reciprocal space. We established the correction procedure for the time-dependent neutron polarization and transmission using a nuclear Bragg reflection and the NMR signal, and confirmed its validity. The polarization analysis for the incommensurate magnetic reflections of Mn_3WO_6 was successfully performed, highlighting its importance for magnetic reflections outside the horizontal plane. Although the present *ex-situ* method requires time-dependent correction, it is possible to upgrade it to an *in-situ* SEOP method. In fact, a compact *in-situ* ^3He -NSF system has been recently developed at J-PARC [39]. This implementation is expected to maintain high neutron polarization and transmission throughout the experiment, thereby facilitating polarization analysis of complex magnetic structures over a wider region of reciprocal space and for a broader range of materials.

ACKNOWLEDGMENTS

We thank Mr. Manabu Ohkawara for his kind support in operating the SEOP laser system in the 5G beamport experimental area, and Dr. Takuya Okudaira and Dr. Shusuke Takada for their constructive discussions. We are also grateful to Dr. Earl Babcock and Dr. Jonathan White for their valuable comments on the manuscript. The polarized neutron scattering experiment on the 5G beamport at JRR-3 was carried out under Proposal No. 25401. This work was supported by JSPS KAKENHI Grant Number 25KJ0050. The construction of the NSF system was supported by JSPS KAKENHI Grant Num-

ber JP21H04987, with partial support from JP24K21682.

Appendix A: Polarization correction with an *ex-situ* ^3He neutron spin filter

In this section, the polarization correction in the present experimental setup is described. This correction is based on the polarization matrix reported by A. Wildes [40, 41]. A count obtained when both the polarizer and the analyzer are set to the spin-up state, I_{obs}^{++} , is expressed as the sum of the contributions from the four scattering channels:

$$\begin{aligned} I_{\text{obs}}^{++} = & N^+ 2T_p p_p I^{++} 2T_a p_a \\ & + N^+ 2T_p p_p I^{+-} 2T_a (1 - p_a) \\ & + N^- 2T_p (1 - p_p) I^{-+} 2T_a p_a \\ & + N^- 2T_p (1 - p_p) I^{--} 2T_a (1 - p_a). \end{aligned} \quad (\text{A1})$$

Here, N^+ and N^- denote the numbers of up and down neutrons incident on the polarizer from the neutron source, respectively. T_p and T_a are the unpolarized neutron reflectance and the transmissions of the polarizer and analyzer, respectively. The polarization efficiencies of the polarizer and analyzer are defined as $p_p = (1 + P_p)/2$ and $p_a = (1 + P_a)/2$, respectively, where P_p and P_a are the neutron polarization magnitudes produced by the polarizer and analyzer. These parameters take values in the ranges $0 \leq T_p, T_a, P_p, P_a \leq 1$, and $0.5 \leq p_p, p_a \leq 1$. I^{++} , I^{+-} , I^{-+} , and I^{--} are the scattering intensities for the corresponding spin states. The derivation of this equation is schematically illustrated in Fig. 9. In practice, this equation also includes a background term, which is ignored here for simplicity.

In the present experimental setup, only the I_{obs}^{++} and I_{obs}^{+-} configurations can be measured. If the ^3He -NSF analyzer is switched to the spin-down state, the factors for the up and down neutrons, $2T_a p_a$ and $2T_a (1 - p_a)$, are interchanged. Here, we define the total number of incident neutrons as $N_0 = N^+ + N^-$. Assuming an unpolarized incident beam coming from the neutron source, we have $N^+ = N^- = N_0/2$. N_0 is usually normalized by the counting time or monitor counts. As also noted in Sec. III, the sample is an antiferromagnet and its nuclear and magnetic reflections are separated from each other. Moreover, the chiral magnetic scattering, which depends on the sign of the incident neutron polarization direction, can be neglected because the neutron polarization is nearly perpendicular to the scattering vector. With these conditions, $I^{++} = I^{--}$ and $I^{+-} = I^{-+}$ hold, allowing Eq. A1 to be simplified into the following matrix form in terms of the non-spin-flip and spin-flip intensities:

$$\begin{bmatrix} I_{\text{obs}}^{++} \\ I_{\text{obs}}^{+-} \end{bmatrix} = 2T_p T_a \begin{bmatrix} p_p & 1 - p_p \\ 1 - p_p & p_p \end{bmatrix} \begin{bmatrix} p_a & 1 - p_a \\ 1 - p_a & p_a \end{bmatrix} \begin{bmatrix} I^{++} \\ I^{+-} \end{bmatrix}. \quad (\text{A2})$$

Since the ^3He polarization of the *ex-situ* ^3He -NSF analyzer decays over time, both the neutron polarization

efficiency p_a and the neutron transmission T_a become time-dependent. Accordingly, by treating Eq. A2 as a

time-dependent matrix equation and taking its inverse, the following expression is obtained:

$$\begin{bmatrix} I^{++} \\ I^{+-} \end{bmatrix} = \frac{1}{2T_p P_p (P_a(t_1) + P_a(t_2))} \begin{bmatrix} 1 + P_p P_a(t_2) & -1 + P_p P_a(t_1) \\ -1 + P_p P_a(t_2) & 1 + P_p P_a(t_1) \end{bmatrix} \begin{bmatrix} 1/T_a(t_1) & 0 \\ 0 & 1/T_a(t_2) \end{bmatrix} \begin{bmatrix} I_{\text{obs}}^{++}(t_1) \\ I_{\text{obs}}^{+-}(t_2) \end{bmatrix}, \quad (\text{A3})$$

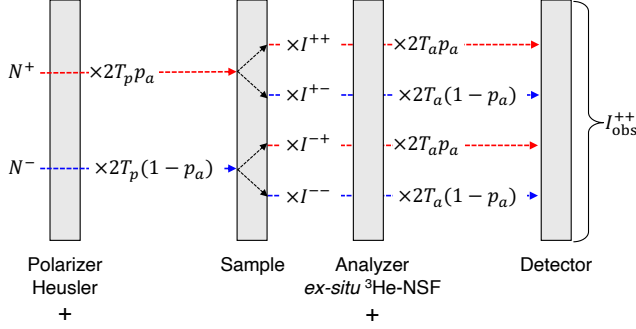


FIG. 9. Schematic diagram of the spin-dependent neutron intensities in the present experimental setup when the Heusler polarizer and the ^3He -NSF are both set to select up-spin (+) neutrons. The red and blue lines indicate the paths of the up neutrons (N^+) and down neutrons (N^-), respectively. The observed intensity, I_{obs}^{++} , is obtained as the sum of the contributions from the four spin-scattering channels.

where p_p and p_a are converted to P_p and P_a using the relations $P_p = 2p_p - 1$ and $P_a = 2p_a - 1$. $T_a(t)$, P_p , and $P_a(t)$ are determined experimentally, as described in Sec. IV A. In contrast, T_p of the Heusler polarizer does not depend on time and is treated as a single constant scale factor. This time-dependent correction was applied to each detector pixel, allowing data collected throughout the entire measurement period to be used for the polarization analysis.

- [1] G. L. Squires, *Introduction to the theory of thermal neutron scattering* (Courier Corporation, 1996).
- [2] F. Mezei, Commun. Phys.;(United Kingdom) **1** (1976).
- [3] T. R. Gentile, P. Nacher, B. Saam, and T. Walker, Reviews of modern physics **89**, 045004 (2017).
- [4] J. Kulda, J. Šaroun, P. Courtois, M. Enderle, M. Thomas, and P. Flores, Appl Phys A **74**, s246 (2002).
- [5] E. Faulhaber, A. Schneidewind, F. Tang, P. Link, D. Etzdorf, and M. Loewenhaupt, J. Phys.: Conf. Ser. **211**, 012031 (2010).
- [6] J. Fernandez-Baca, M. Lumsden, B. Winn, J. Zarestky, and A. Zheludev, Neutron News **19**, 18 (2008), eprint: <https://doi.org/10.1080/10448630801975684>.
- [7] M. Takeda, M. Nakamura, Y. Shimojo, and K. Kakurai, Nuclear Instruments and Methods in Physics Research Section A: Accelerators, Spectrometers, Detectors and Associated Equipment **586**, 229 (2008).
- [8] T. Nakajima, H. Saito, N. Kobayashi, T. Kawasaki, T. Nakamura, H. Kawano-Furukawa, S. Asai, and T. Masuda, J. Phys. Soc. Jpn. **93**, 091002 (2024).
- [9] S. Mühlbauer, B. Binz, F. Jonietz, C. Pfleiderer, A. Rosch, A. Neubauer, R. Georgii, and P. Böni, Science **323**, 915 (2009).
- [10] Y. Tokura, S. Seki, and N. Nagaosa, Rep. Prog. Phys. **77**, 076501 (2014).
- [11] N. Kanazawa, A. Kitaori, J. White, V. Ukleev, H. Rønnow, A. Tsukazaki, M. Ichikawa, M. Kawasaki, and Y. Tokura, Phys. Rev. Lett. **125**, 137202 (2020).
- [12] Y. Fujishiro, N. Kanazawa, T. Nakajima, X. Z. Yu, K. Ohishi, Y. Kawamura, K. Kakurai, T. Arima, H. Mitamura, A. Miyake, K. Akiba, M. Tokunaga, A. Matsuo, K. Kindo, T. Koretsune, R. Arita, and Y. Tokura, Nat Commun **10**, 1059 (2019).
- [13] T. Kurumaji, N. Paul, S. Fang, P. M. Neves, M. Kang, J. S. White, T. Nakajima, D. Graf, L. Ye, M. K. Chan, T. Suzuki, J. Denlinger, C. Jozwiak, A. Bostwick, E. Rotenberg, Y. Zhao, J. W. Lynn, E. Kaxiras, R. Comin, L. Fu, and J. G. Checkelsky, Science Advances **11**, eadu6686 (2025).
- [14] D. Singh, Y. Fujishiro, S. Hayami, S. H. Moody, T. Nomoto, P. R. Baral, V. Ukleev, R. Cubitt, N.-J. Steinke, D. J. Gawryluk, E. Pomjakushina, Y. Ōnuki, R. Arita, Y. Tokura, N. Kanazawa, and J. S. White, Nat Commun **14**, 8050 (2023).
- [15] R. Takagi, J. S. White, S. Hayami, R. Arita, D. Honecker, H. M. Rønnow, Y. Tokura, and S. Seki, Science Advances **4**, eaau3402 (2018).
- [16] H. Thoma, W. Lubertstetter, J. Peters, and V. Hutnanu, J Appl Cryst **51**, 17 (2018).
- [17] W. T. H. Lee and T. D'Adam, Neutron News **27**, 35 (2016), eprint: <https://doi.org/10.1080/10448632.2016.1166912>.
- [18] W. Heil, K. H. Andersen, R. Cywinski, H. Humblot, C. Ritter, T. W. Roberts, and J. R. Stewart, Nuclear In-

- struments and Methods in Physics Research Section A: Accelerators, Spectrometers, Detectors and Associated Equipment **485**, 551 (2002).
- [19] C. B. Fu, T. R. Gentile, G. L. Jones, W. C. Chen, R. Erwin, S. Watson, C. Broholm, J. A. Rodriguez-Rivera, and J. Scherschligt, *Physica B: Condensed Matter Proceedings of the 8th International Workshop on Polarised Neutrons for Condensed Matter Investigation*, **406**, 2419 (2011).
- [20] Q. Ye, T. R. Gentile, J. Anderson, C. Broholm, W. C. Chen, Z. DeLand, R. W. Erwin, C. B. Fu, J. Fuller, A. Kirchhoff, J. A. Rodriguez-Rivera, V. Thampy, T. G. Walker, and S. Watson, *Physics Procedia 9th International Conference on Polarised Neutrons in Condensed Matter Investigations*, **42**, 206 (2013).
- [21] W. Chen, T. Gentile, Q. Ye, A. Kirchhoff, S. Watson, J. Rodriguez-Rivera, Y. Qiu, and C. Broholm, *Journal of Physics: Conference Series* **746**, 012016 (2016).
- [22] G. J. Nilsen, J. Kořata, M. Devonport, P. Galsworthy, R. I. Bewley, D. J. Voneshen, R. Dalglish, and J. R. Stewart, *Journal of Physics: Conference Series* **862**, 012019 (2017).
- [23] G. Cassella, J. R. Stewart, G. M. Paternò, V. García Sakai, M. Devonport, P. J. Galsworthy, R. I. Bewley, D. J. Voneshen, D. Raspino, and G. J. Nilsen, *Journal of Physics: Conference Series* **1316**, 012007 (2019).
- [24] I. A. Zaliznyak, A. T. Savici, V. Ovidiu Garlea, B. Winn, U. Filges, J. Schneeloch, J. M. Tranquada, G. Gu, A. Wang, and C. Petrovic, *Journal of Physics: Conference Series* **862**, 012030 (2017).
- [25] A. Maignan, W. Peng, A. C. Komarek, C.-Y. Kuo, C.-F. Chang, X. Wang, Z. Hu, C.-T. Chen, A. Tanaka, L. H. Tjeng, O. I. Lebedev, and C. Martin, *Chem. Mater.* **32**, 5664 (2020).
- [26] Y. Osawa, S. Takahashi, T. Nakajima, *et al.*, (In preparation).
- [27] T. Nakamura, T. Kawasaki, T. Hosoya, K. Toh, K. Oikawa, K. Sakasai, M. Ebine, A. Birumachi, K. Soyama, and M. Katagiri, *Nuclear Instruments and Methods in Physics Research Section A: Accelerators, Spectrometers, Detectors and Associated Equipment* **686**, 64 (2012).
- [28] Compact neutron diffraction system utilizing a two-dimensional scintillation detector.
- [29] M. A. Bouchiat, T. R. Carver, and C. M. Varnum, *Physical Review Letters* **5**, 373 (1960).
- [30] F. Colegrove, L. Scheerer, and G. Walters, *Physical Review* **132**, 2561 (1963).
- [31] T. Ino, M. Ohkawara, K. Ohoyama, T. Yokoo, S. Itoh, Y. Nambu, M. Fujita, H. Kira, H. Hayashida, K. Hiroi, K. Sakai, T. Oku, and K. Kakurai, *Journal of Physics: Conference Series* **862**, 012011 (2017).
- [32] T. Ino, Y. Arimoto, H. M. Shimizu, Y. Sakaguchi, K. Sakai, H. Kira, T. Shinohara, T. Oku, J.-i. Suzuki, K. Kakurai, and L.-J. Chang, *Journal of Physics: Conference Series* **340**, 012006 (2012).
- [33] E. Babcock, I. Nelson, S. Kadlecěk, B. Driehuys, L. W. Anderson, F. W. Hersman, and T. G. Walker, *Physical Review Letters* **91**, 123003 (2003).
- [34] W. C. Chen, T. R. Gentile, T. G. Walker, and E. Babcock, *Physical Review A* **75**, 013416 (2007).
- [35] E. Babcock, Z. Salhi, E. Kentzinger, S. Mattauach, and A. Ioffe, *Journal of Physics: Conference Series* **862**, 012001 (2017).
- [36] M. Blume, *Physical Review* **130**, 1670 (1963).
- [37] K. P. Coulter, T. E. Chupp, A. B. McDonald, C. D. Bowman, J. D. Bowman, J. J. Szymanski, V. Yuan, G. D. Cates, D. R. Benton, and E. D. Earle, *Nuclear Instruments and Methods in Physics Research Section A: Accelerators, Spectrometers, Detectors and Associated Equipment* **288**, 463 (1990).
- [38] L. Passell and R. I. Schermer, *Physical Review* **150**, 146 (1966).
- [39] S. Takahashi, R. Kiyanagi, T. Okudaira, S. Takada, R. Kobayashi, M. Okuizumi, T. Ino, K. Asai, Y. Tsuchikawa, K. Oikawa, M. Harada, T. Ohhara, J. Suzuki, M. Fujita, Y. Ikeda, K. Kakurai, and T. Oku, *Nuclear Instruments and Methods in Physics Research Section A: Accelerators, Spectrometers, Detectors and Associated Equipment* **1075**, 170410 (2025).
- [40] A. R. Wildes, *Review of Scientific Instruments* **70**, 4241 (1999).
- [41] A. R. Wildes, *Neutron News* **17**, 17 (2006), [_eprint: https://doi.org/10.1080/10448630600668738](https://doi.org/10.1080/10448630600668738).