

Heat Transfer Instrumentation for Human Factors and Composite Materials Characterization: Intel Collaboration


Paul Soldate

Introduction

What: An advanced thermesthesiometer has been developed to measure the heat flux, touch-force, and internal temperature profile of a simulated body part coming into contact with a warm surface. This instrument is used to characterize various materials for end-use conditions and aims to quantify potential thermal hazards in correlation with human subjective testing.

Why: Computing platforms and wearable electronics dissipate heat. It is not always possible to calculate the heat transferred to the end user since the thermal and surface properties of many electronic devices are often composed of complex composite shells or housed in materials that vary in surface texture. **How:** A suitably chosen material with thermal characteristics similar to human tissue is used for bare skin simulation and is thermally regulated using a programmable logic controller (PLC). An automated driving mechanism provides variable touch-occurrences and pressures over specially engineered test-surfaces with varying effusivities and surface roughness.

Thermal Response of Human Skin

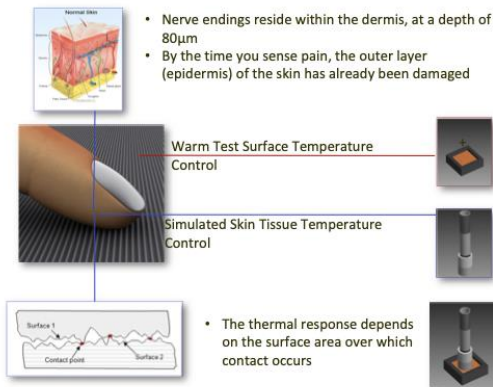

• Heat transfer between two objects is proportional to the density, heat capacity and thermal conductivity of each object, i.e. the effusivity:


$$\lambda = \sqrt{k\rho c_p}$$

• Unfortunately, fundamental heat flow is typically not sufficient for calculations involving surface roughness and complex composites


• A room temperature vulcanizing (RTV) silicone can be mixed with Aluminum Oxide (Al_2O_3) to obtain a weighted thermal inertia similar to that of human tissue, e.g. 60% Al_2O_3 + 40% RTV

Instrumentation



This instrument includes a **test chamber** to secure novel composite structures for heating, Kapton (low thermal inertia) heating elements, a **load cell** for touch force measurements, heat flux & temperature sensors for feedback control and precision, a **mechanical driving mechanism**, automation and **readout hardware/software** for repeatability and measurement, as well as a novel silicone mixture to simulate human tissue

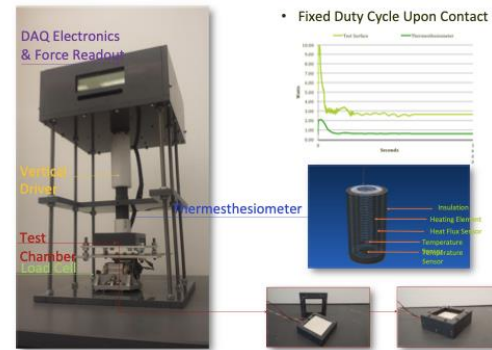


Steady-State Thermal Response



(Left) The temperature response of several test materials, initially heated to 44 °C, contacting the simulated skin, held initially at 32.5 °C. The legend describes each material, e.g. "1.5mm ABS" is a composite made of 1mm Aluminum underneath 1.5mm of ABS plastic. (Below) Similar to the temperature response parameters given (Left), the heat flux response is shown below..




Effusivity

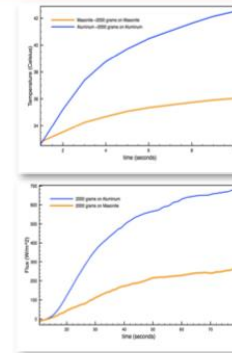

• (Top) Comparing the temperature response of the thermesthesiometer (regulated at 32.5°C) touching a 44°C sheet of Aluminum and Masonite. (Bottom) Heat flux.

Contact Resistance

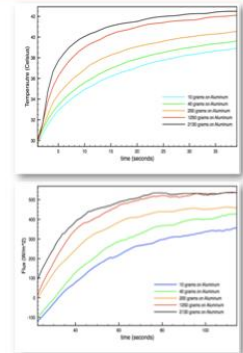

• (Top) The temperature response of the thermesthesiometer (regulated at 32.5°C) coming into contact with a 1mm sheet of 6061 Aluminum under several different contact forces. (Bottom) Heat flux.

References

1. Alberts, B., Wilson, J., and Tim, H. Molecular Biology of the Cell, New York : Garland Science, (2008).
2. ASTM Designation: C1057 – 03 Standard Practice for Determination of Skin Contact Temperature from Heated Surfaces Using a Mathematical Model and Thermesthesiometer (2010).
3. Carslaw H. S. and Jaeger, J. C. Conduction of Heat in Solids, 2nd ed. London, England: Oxford (1959).
4. Cengel, Y. Introduction to Thermodynamics and Heat Transfer, Second Edition, pp. 374, McGraw Hill Companies (2008).
5. Hattori A. P., and Halldanarson H. The Role of Contact Resistance in Skin Burns. Journal of Biomedical Engineering, 1(2), pp. 97-102 (1982).
6. Hedge, A. and Zhang, H. Warm Surfaces of Electronic Devices and Human Thermal Responses, Final Report for Intel (2016).
7. ISO 13732-1 Ergonomics of the Thermal Environment - Methods for the Assessment of Human Responses to Contact with Surfaces, Part 1: Hot Surfaces, ISO, Geneva, Switzerland (2006).
8. Marzetta, L.A. A Thermesthesiometer – An Instrument for Burn Hazard Measurement, I.E.E.E. Transactions on Biomedical Engineering, Sept. 1974, pp. 425-427 (1974).
9. Stoll, A.M., Chianta, M.A., and Piergallini, J.R. Thermal Conduction Effects in Human Skin, Aviation, Space and Environmental Medicine, Vol. 50, No. 8, Aug. 1979, pp. 778-787 (1979).
10. Ungar, E. and Stroud K. A New Approach to Defining Human Touch Temperature Standards. NASA/Johnson Space Center (<https://nasa.larc.nasa.gov/search.jsp?R=20090042589&q=1>) (2010).
11. Wu, Y.C. Materials Property Criteria for Thermal Safety, J. Materials, JMLSA, 7, 573-579 (1972).


Acknowledgements

The authors would like to thank Intel, Mark Macdonald, Mondira Pant, and Wu Yuen Shing for useful discussions. This work was supported by a grant from Intel and performed at Cornell University.

Overview

- I. Heat Transfer Instrumentation for Human Factors and Composite Materials Characterization
- II. Heat and Mass Transfer Instrumentation for Textiles and Smart Fabrics

Automated Pressure Sensitive Thermesthesiometer

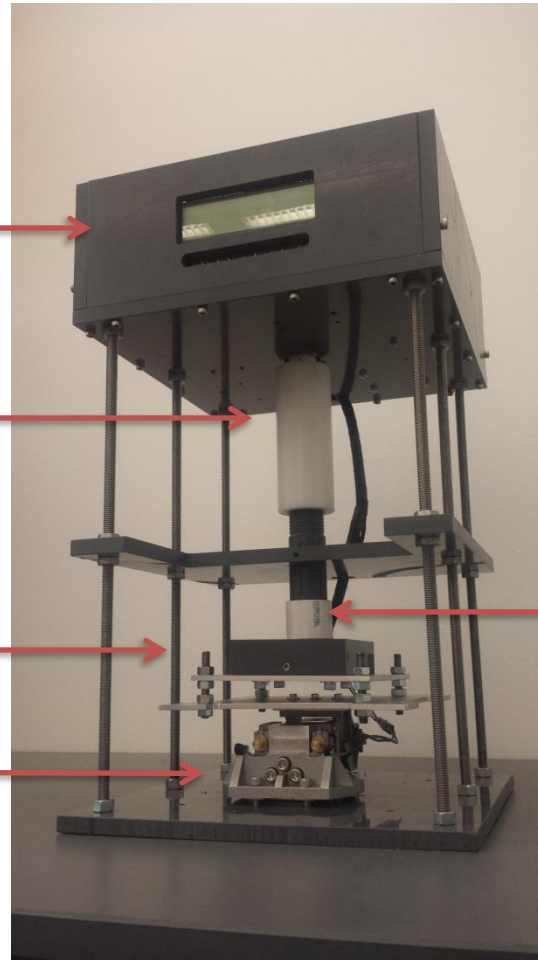

DAQ Hardware

Mechanical Driver

Heated Test Surface

Load Cell
with LCD

Thermesthesiometer


1st Tier: DAQ and Electronics

- ✓ DAQ (National Instruments)
 - Digital Out (32 Channel)
 - Analog Read (4 Channel)
- ✓ Micro-controller with Bipolar Stepper Motor
- ✓ Miniaturized heat flux sensor with $\pm 3\%$ accuracy
- ✓ Pt100 RTD with $\pm 1^\circ\text{C}$ accuracy
- ✓ MSR45 Heat Flux Data Logger
- ✓ Solid-state Relays for PID Controls
- ✓ 12V Power Supply for Stepper and Load Cell
- ✓ 5V Power Supply for Digital Out, Relays and Microcontroller
- ✓ Cooling Fan
- ✓ Kapton, resistive heating element ($21^\circ\text{C} - 200^\circ\text{C}$)
- ✓ Load Cell (0 to 6000 grams $\pm 1\text{g}$)
- ✓ Housed in a PVC shell:
 - .5" thick walls
 - Low enough conductivity $k = .19 \frac{\text{W}}{\text{mK}}$






Top and Posterior

- ✓ Breathable grating for air circulation
- ✓ USB Hub for heat flux sensor data and uploading code to the micro-controller.
- ✓ Ethernet Cable for DAQ System
- ✓ Power Outlet


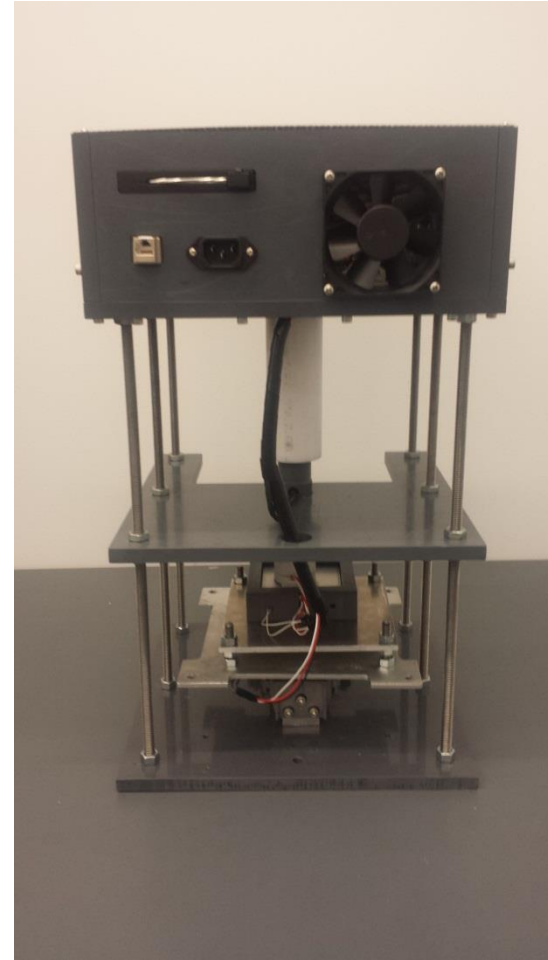


ANSYS Simulations Done to Aid in Design

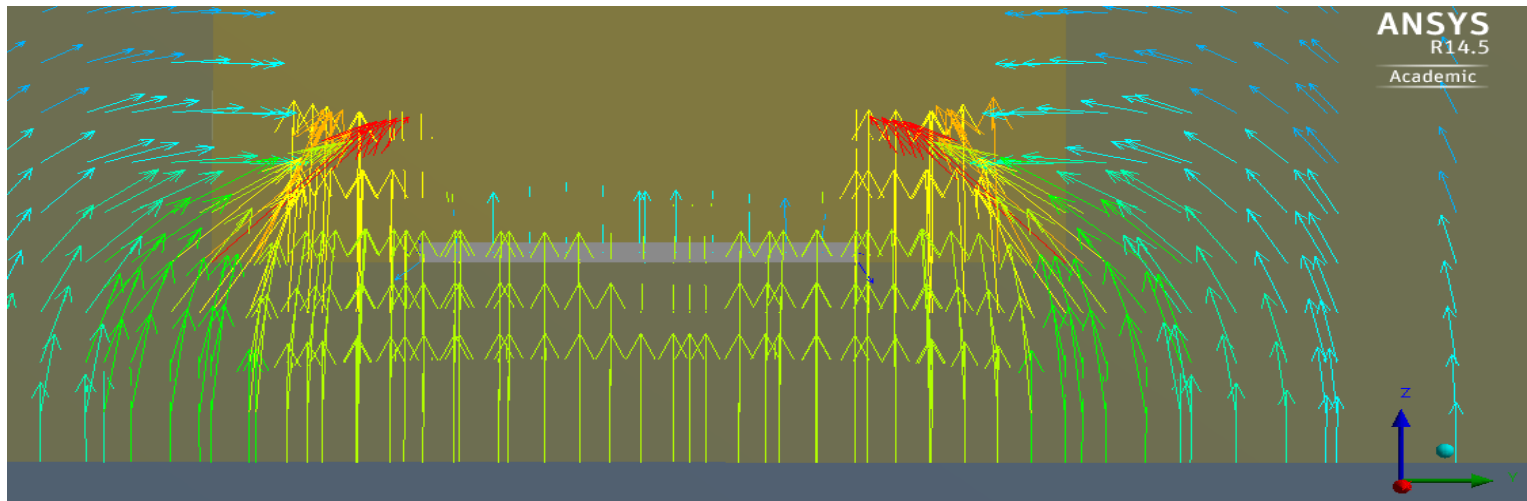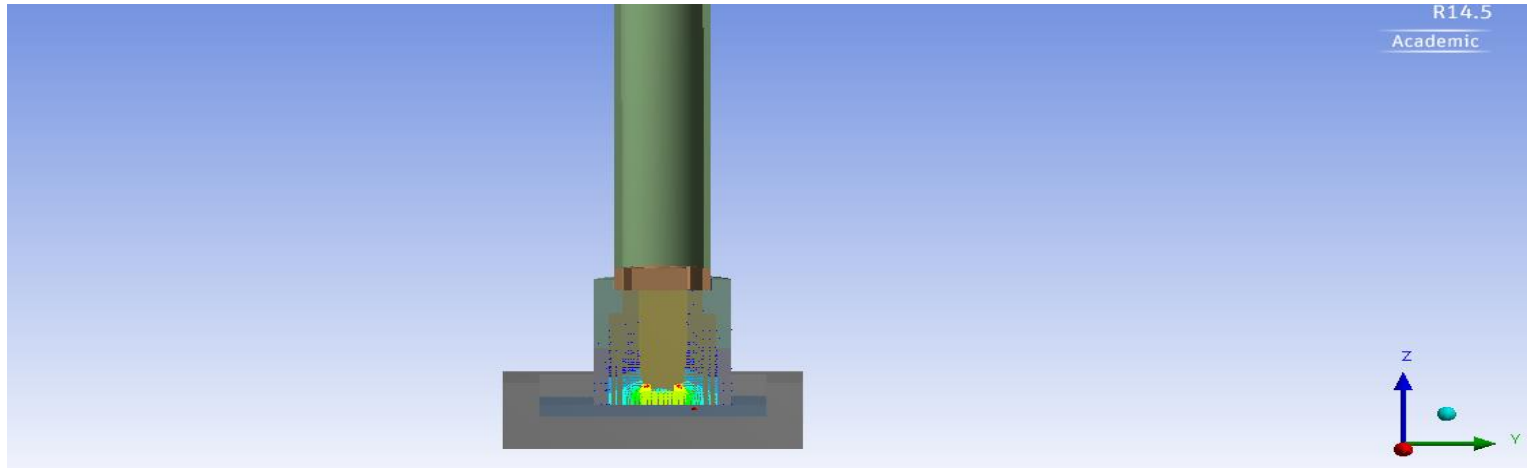

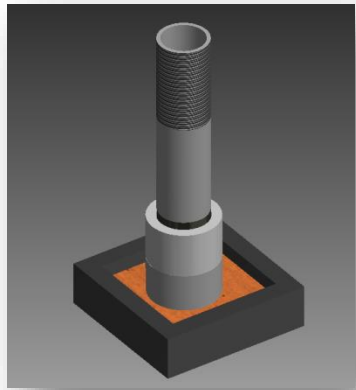



Temperature Copper + ABS 44 Surface VS 32.5 Skin

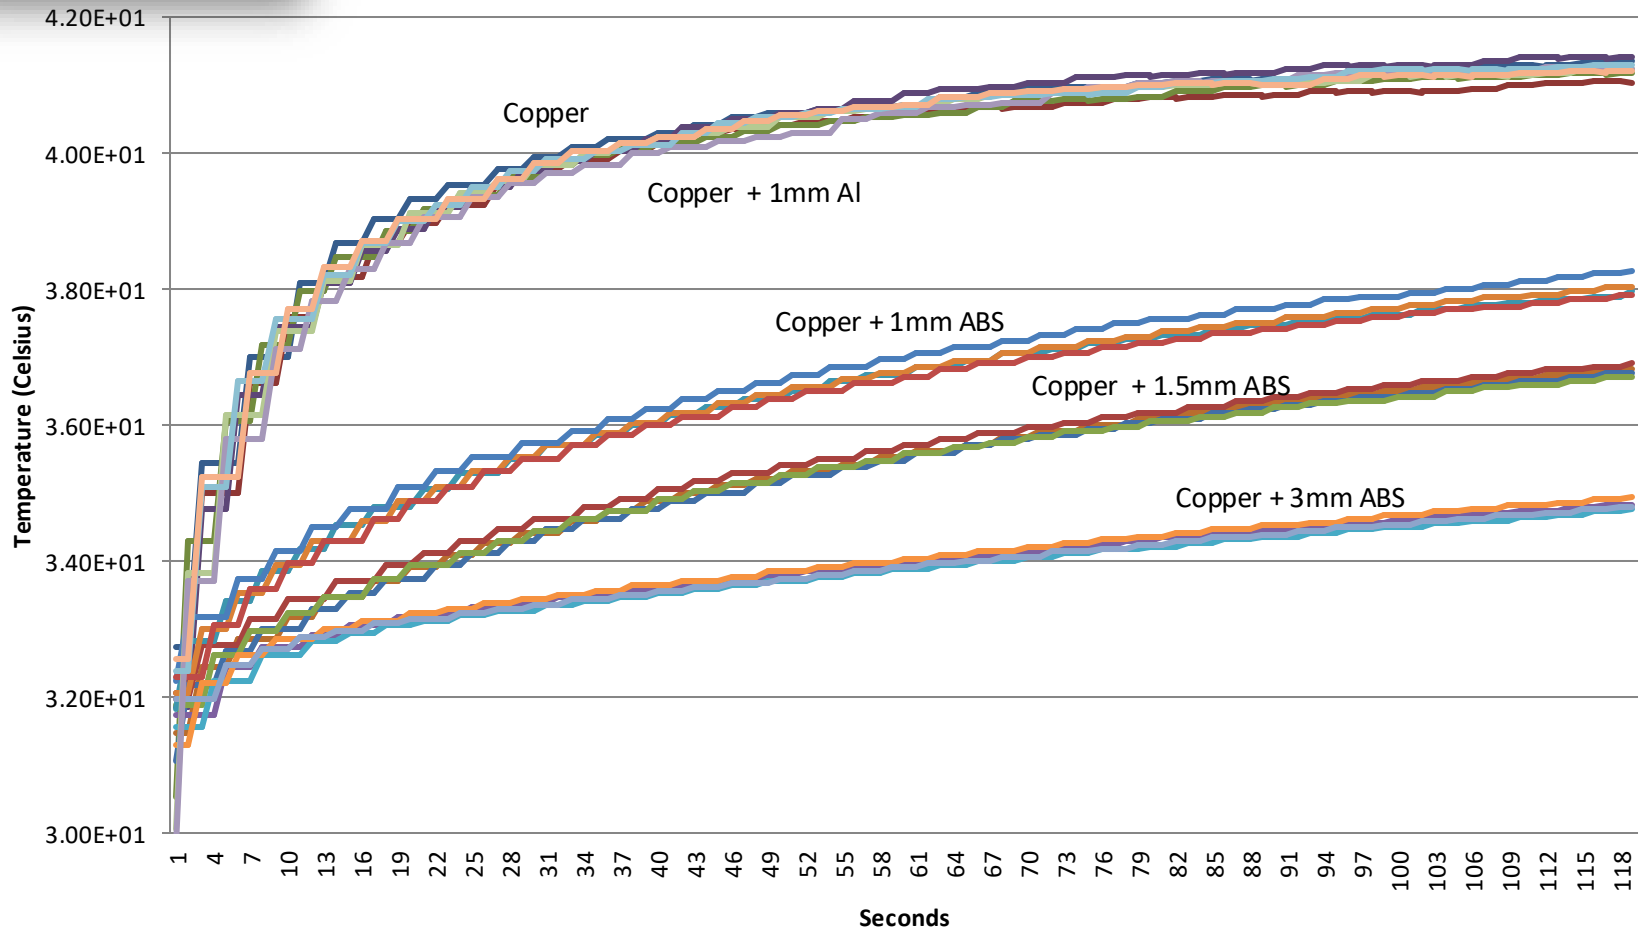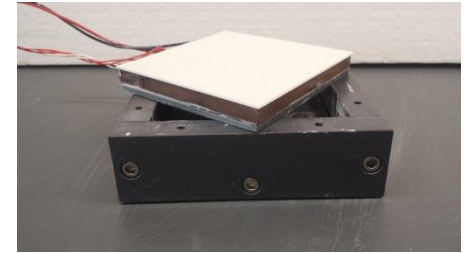

Contact Resistances and the Transient Thermal Response


- The epidermal thickness is related to the heat flux by the amount of time it takes for the heat to transfer to the dermal layer, i.e. the time it takes to feel pain

Setpoint at $T = 42^{\circ}\text{C}$

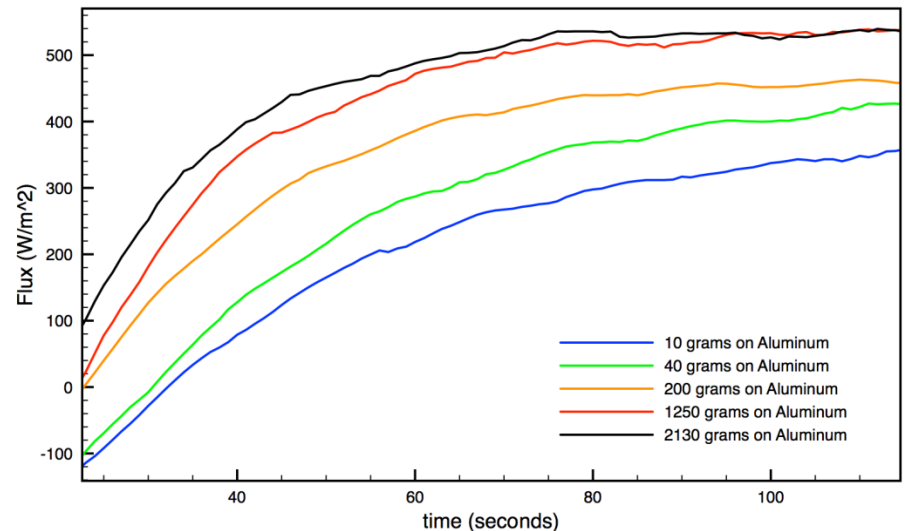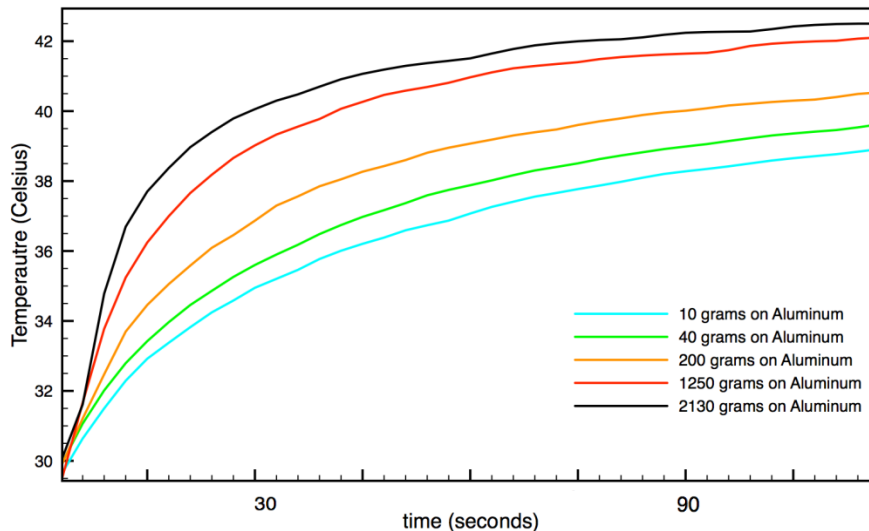

Complete System

- Heat Flux Readout

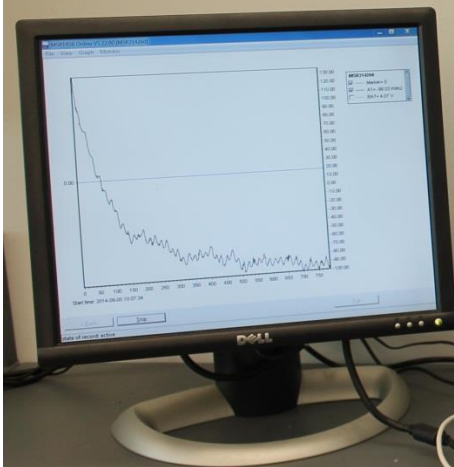

- PID Control
- Data Logging



- Automated Instrument

