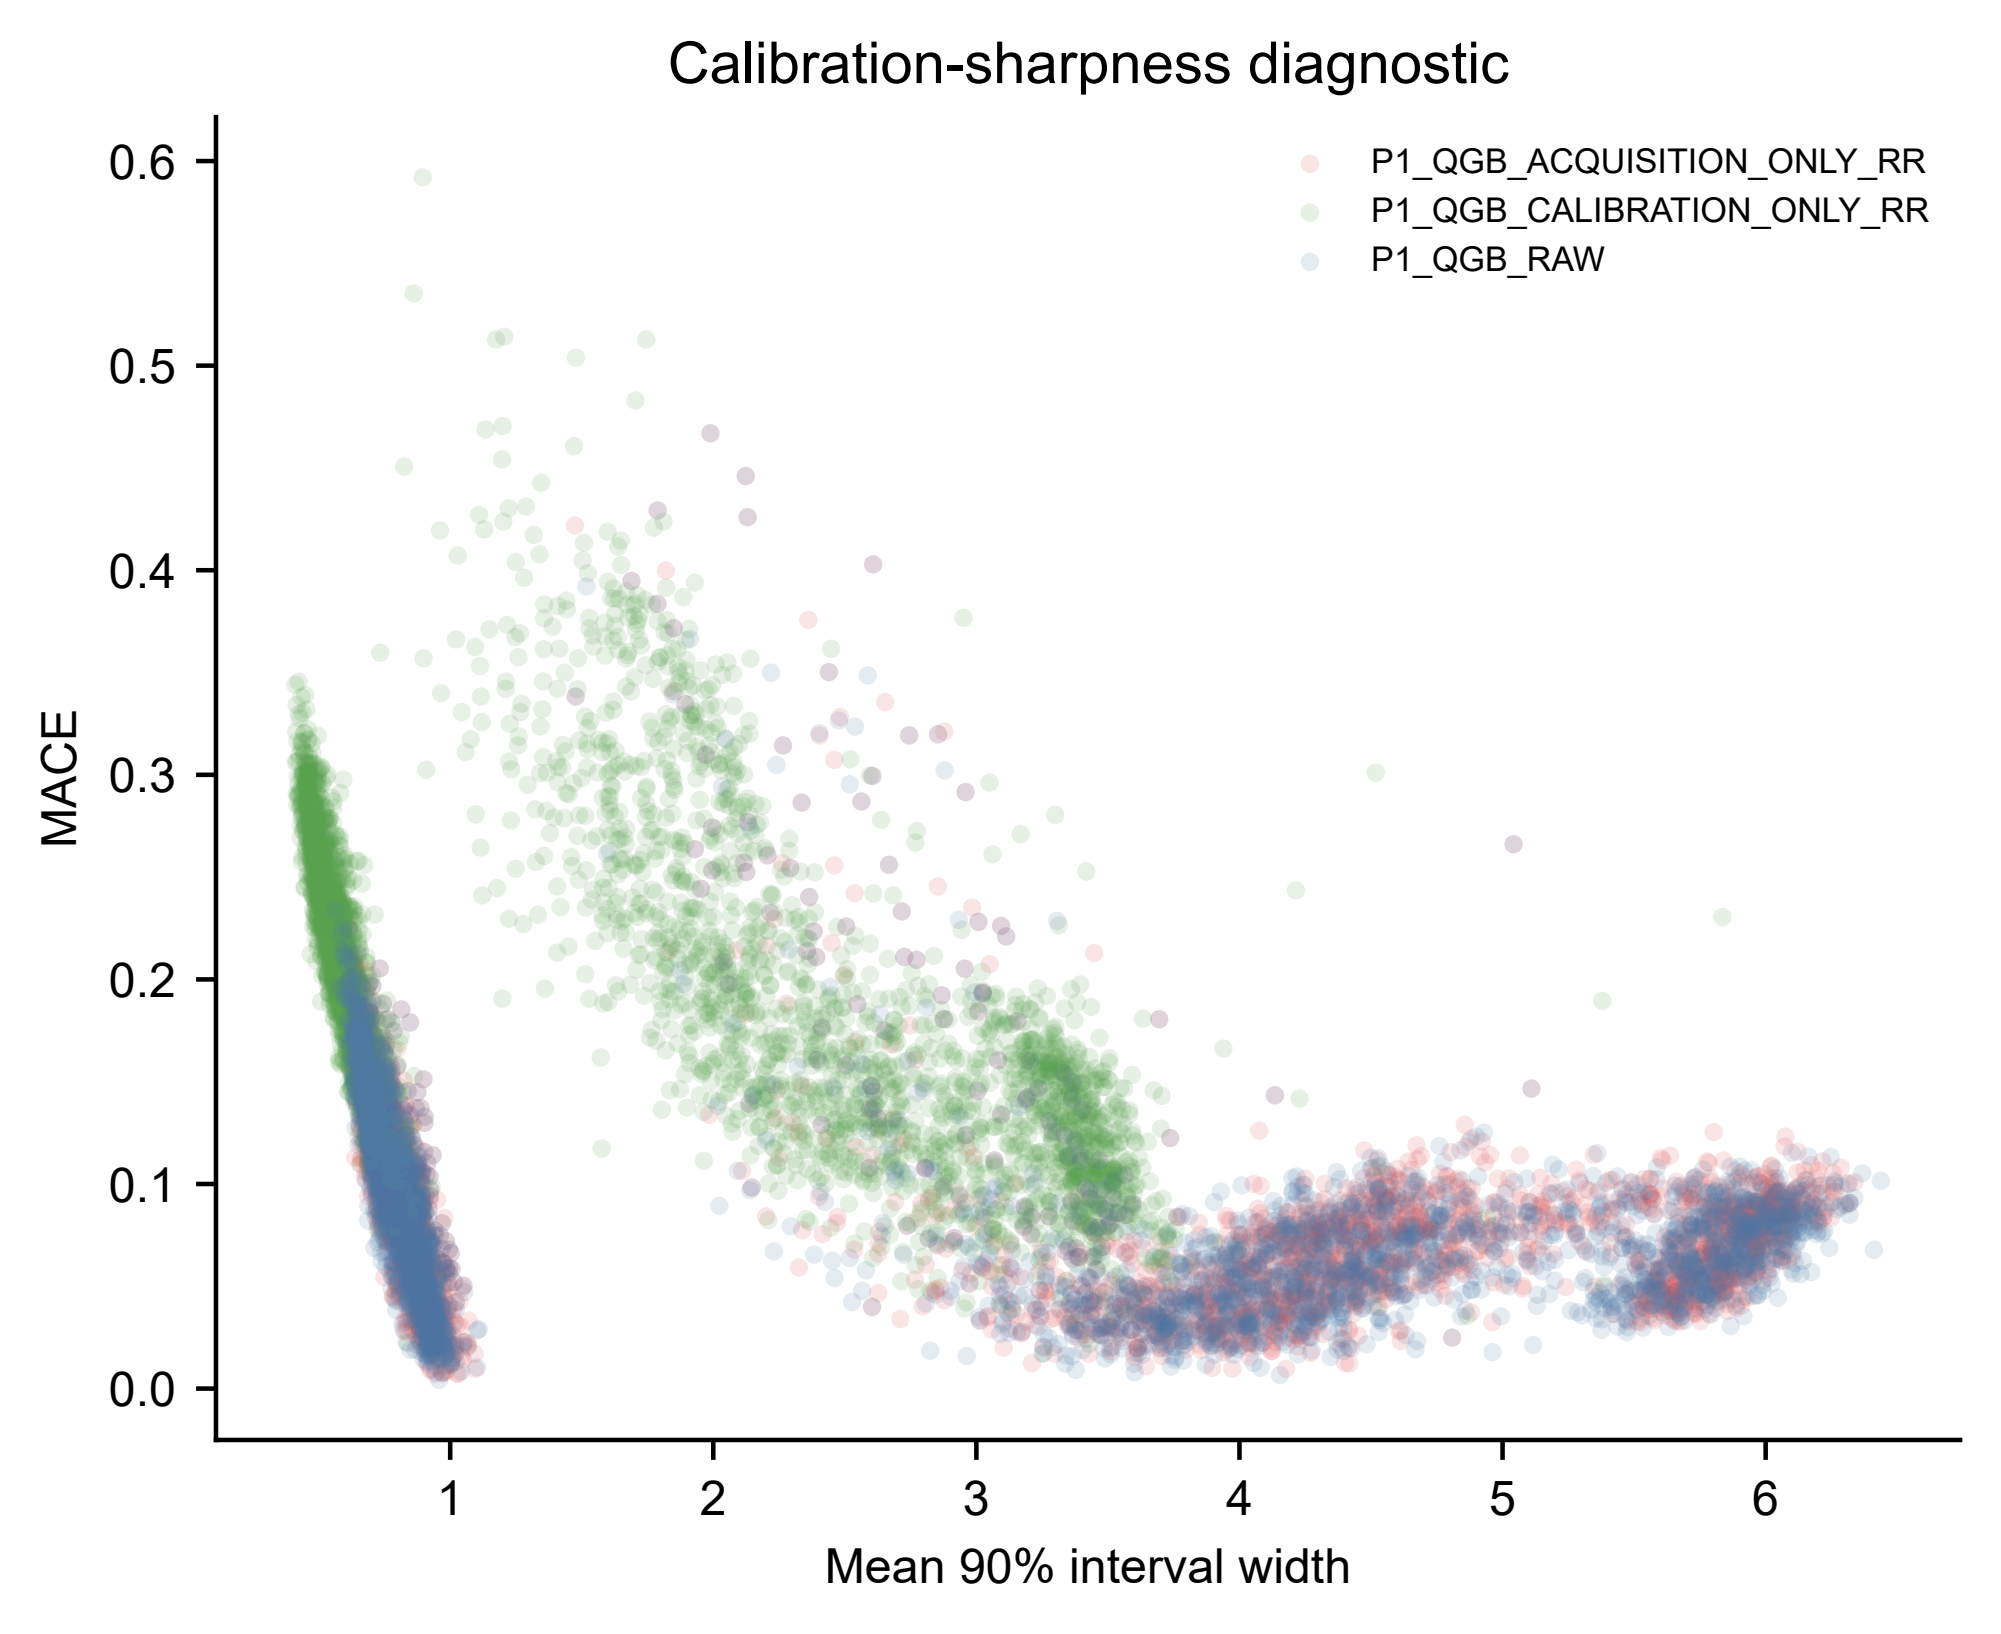

Calibration-sharpness diagnostic
P1_QGB_ACQUISITION_ONLY_RR
P1_QGB_CALIBRATION_ONLY_RR
P1_QGB_RAW
MACE
0.0
0.1
0.2
0.3
0.4
0.5
0.6
1
2
3
4
5
6
Mean 90% interval width