Spectral QC Summary Report

This QC report is for guidance only. Spectra are expected to vary somewhat by instrument and protocol; minor deviations from library references are normal.

Fluorophore	Similarity	Status
BUV395	0.9994	**PASS**
BUV615	0.987	**PASS**
BUV805	0.9918	**PASS**
BV421	0.9936	**PASS**
BV711	0.9372	**WARNING**
BB515	0.9998	**PASS**
RB613	0.9942	**PASS**
RB705	0.9944	**PASS**
RB780	0.9976	**PASS**
PE	0.9913	**PASS**
RY655	0.9918	**PASS**
RY703	0.9988	**PASS**
PE−Cy7	0.9931	**PASS**
APC	0.9847	**PASS**
APC−H7	0.9957	**PASS**
Helix NP Blue	N/A	**No Reference Available**
Live Dead Nir (876)	N/A	**No Reference Available**

BUV395

Cosine Similarity: 0.9994

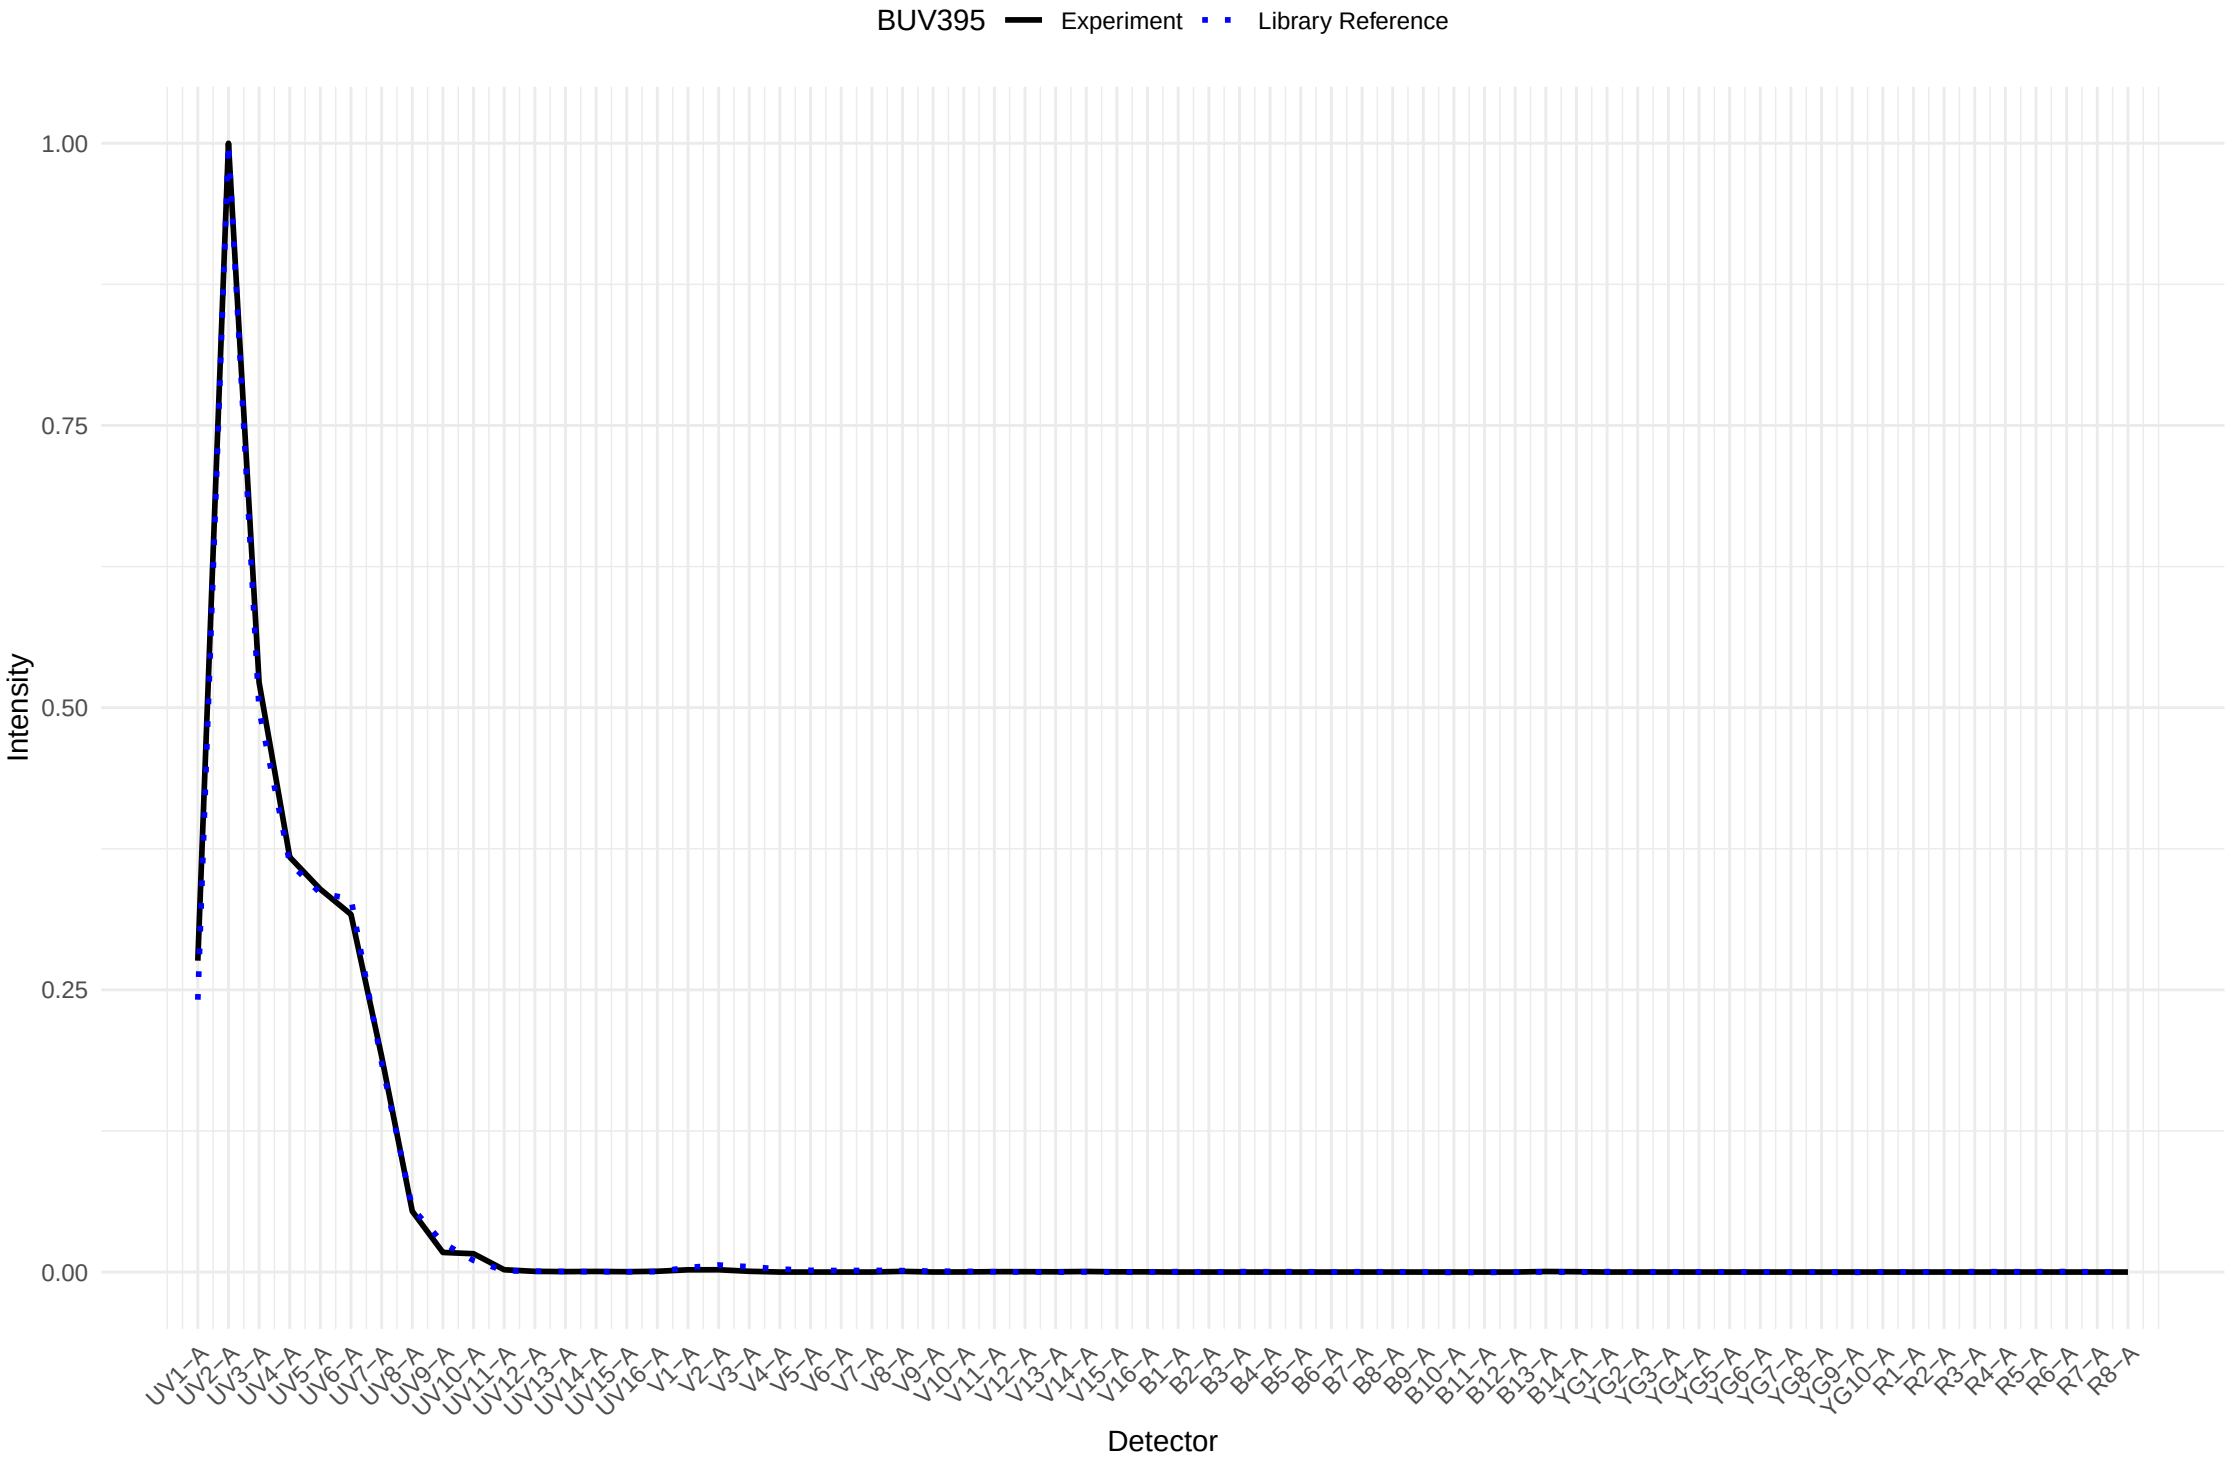

BUV615

Cosine Similarity: 0.987

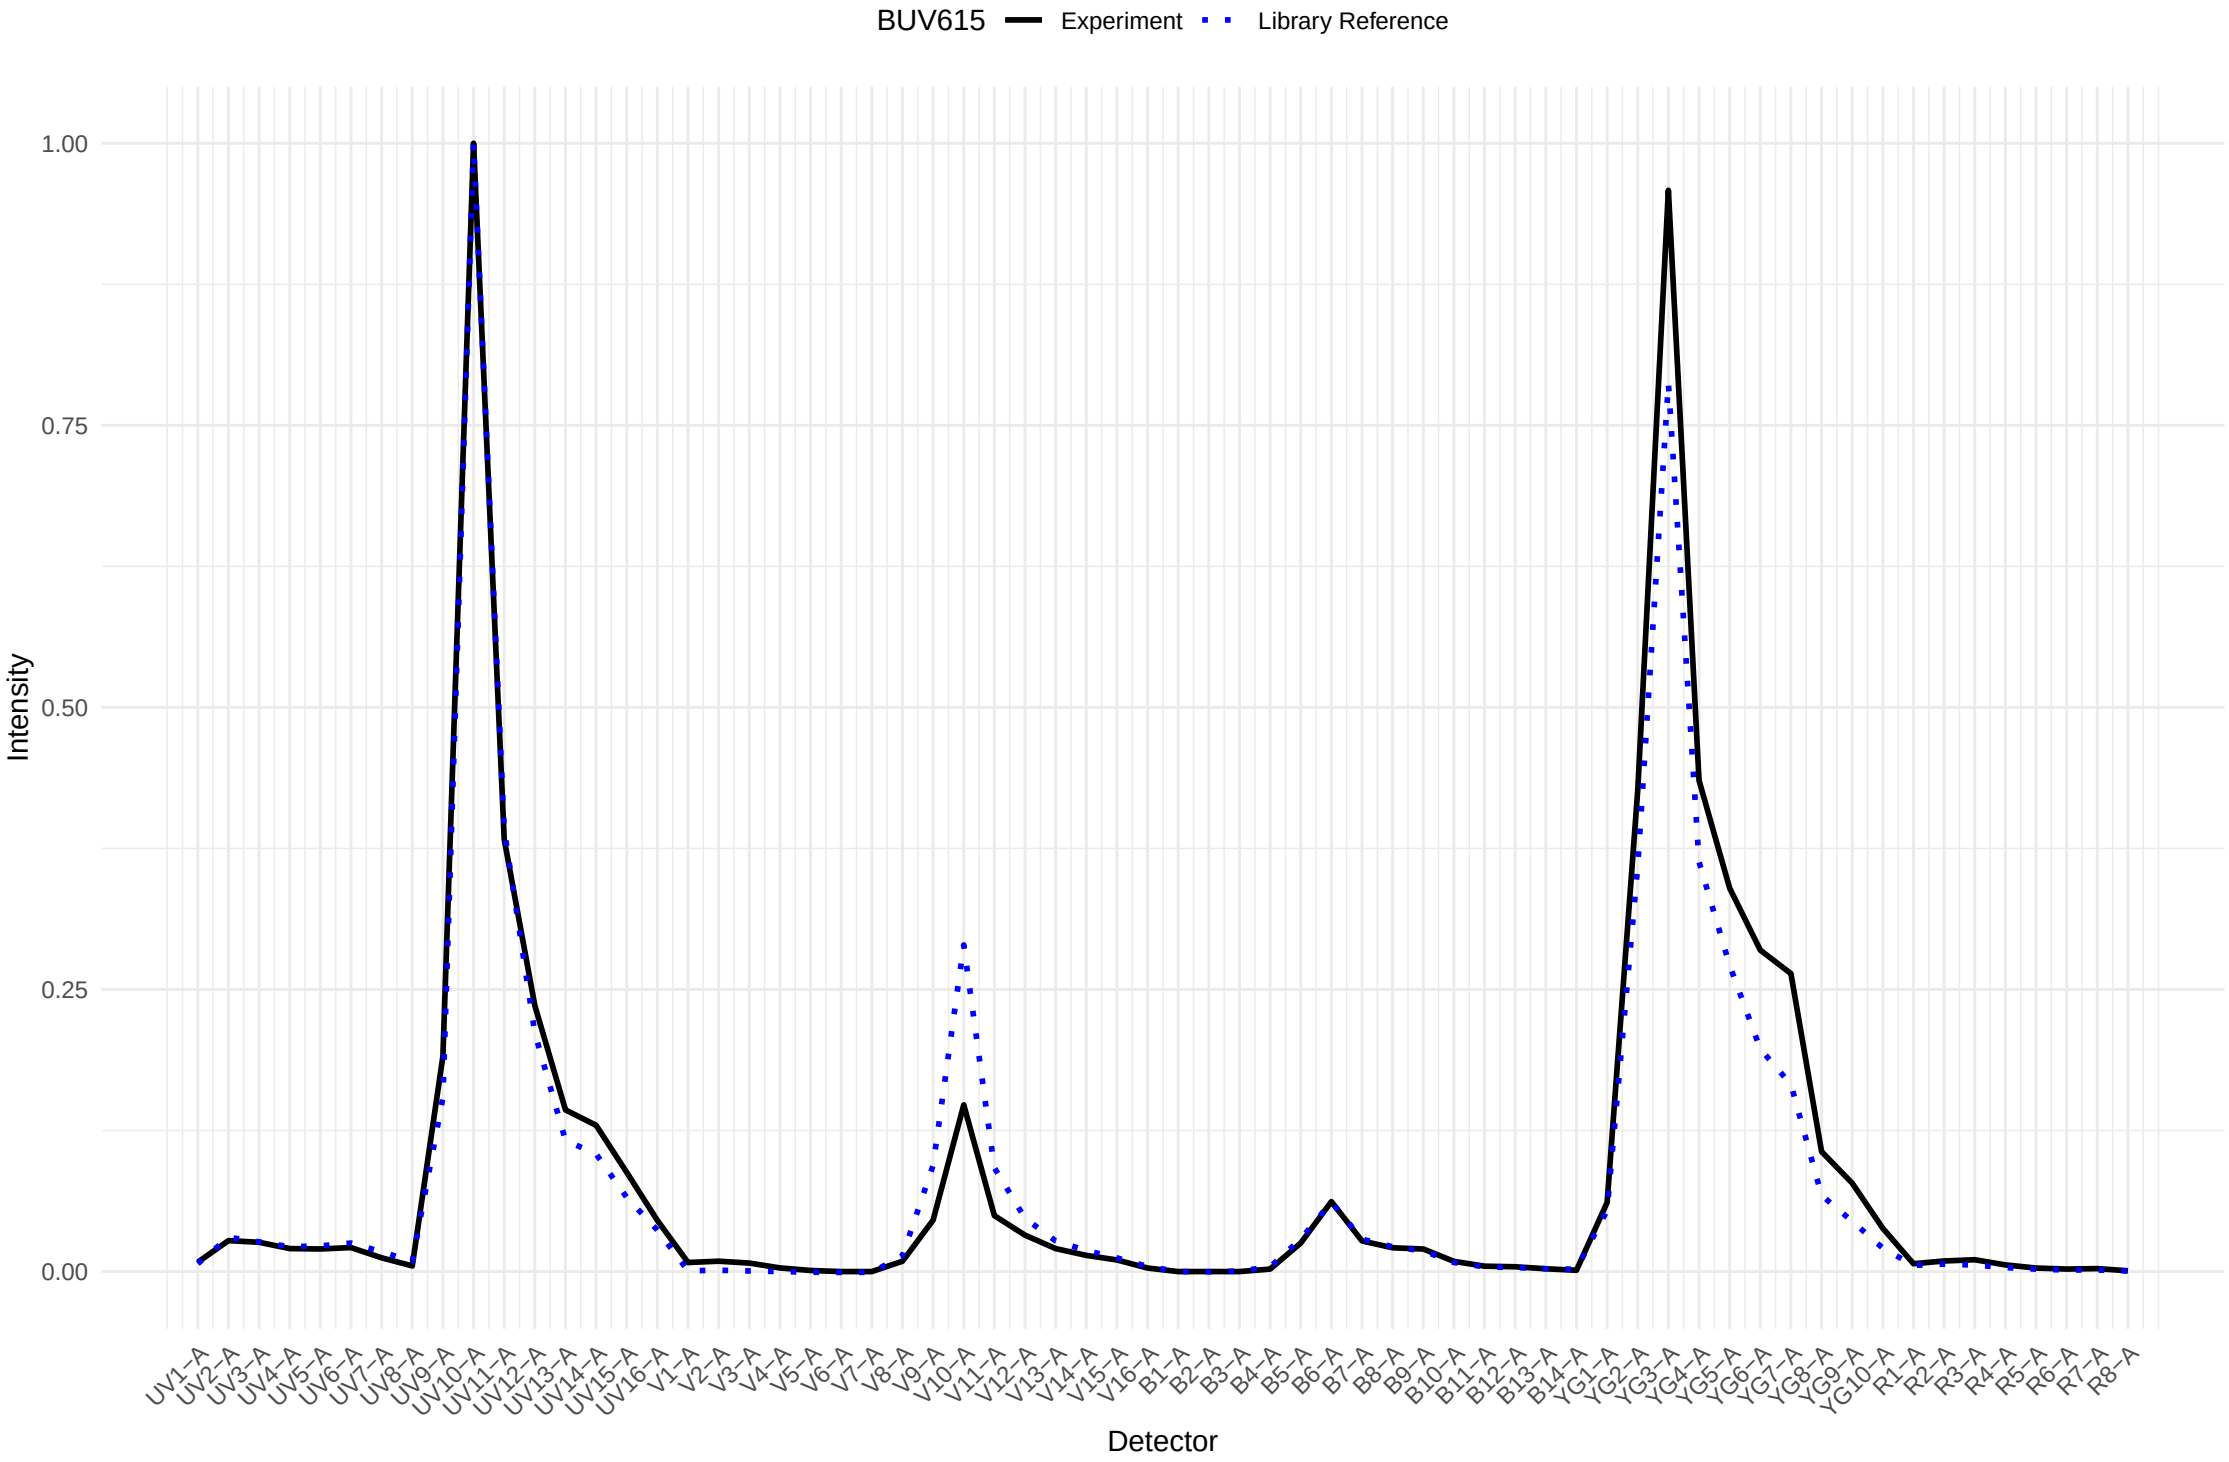

BUV805

Cosine Similarity: 0.9918

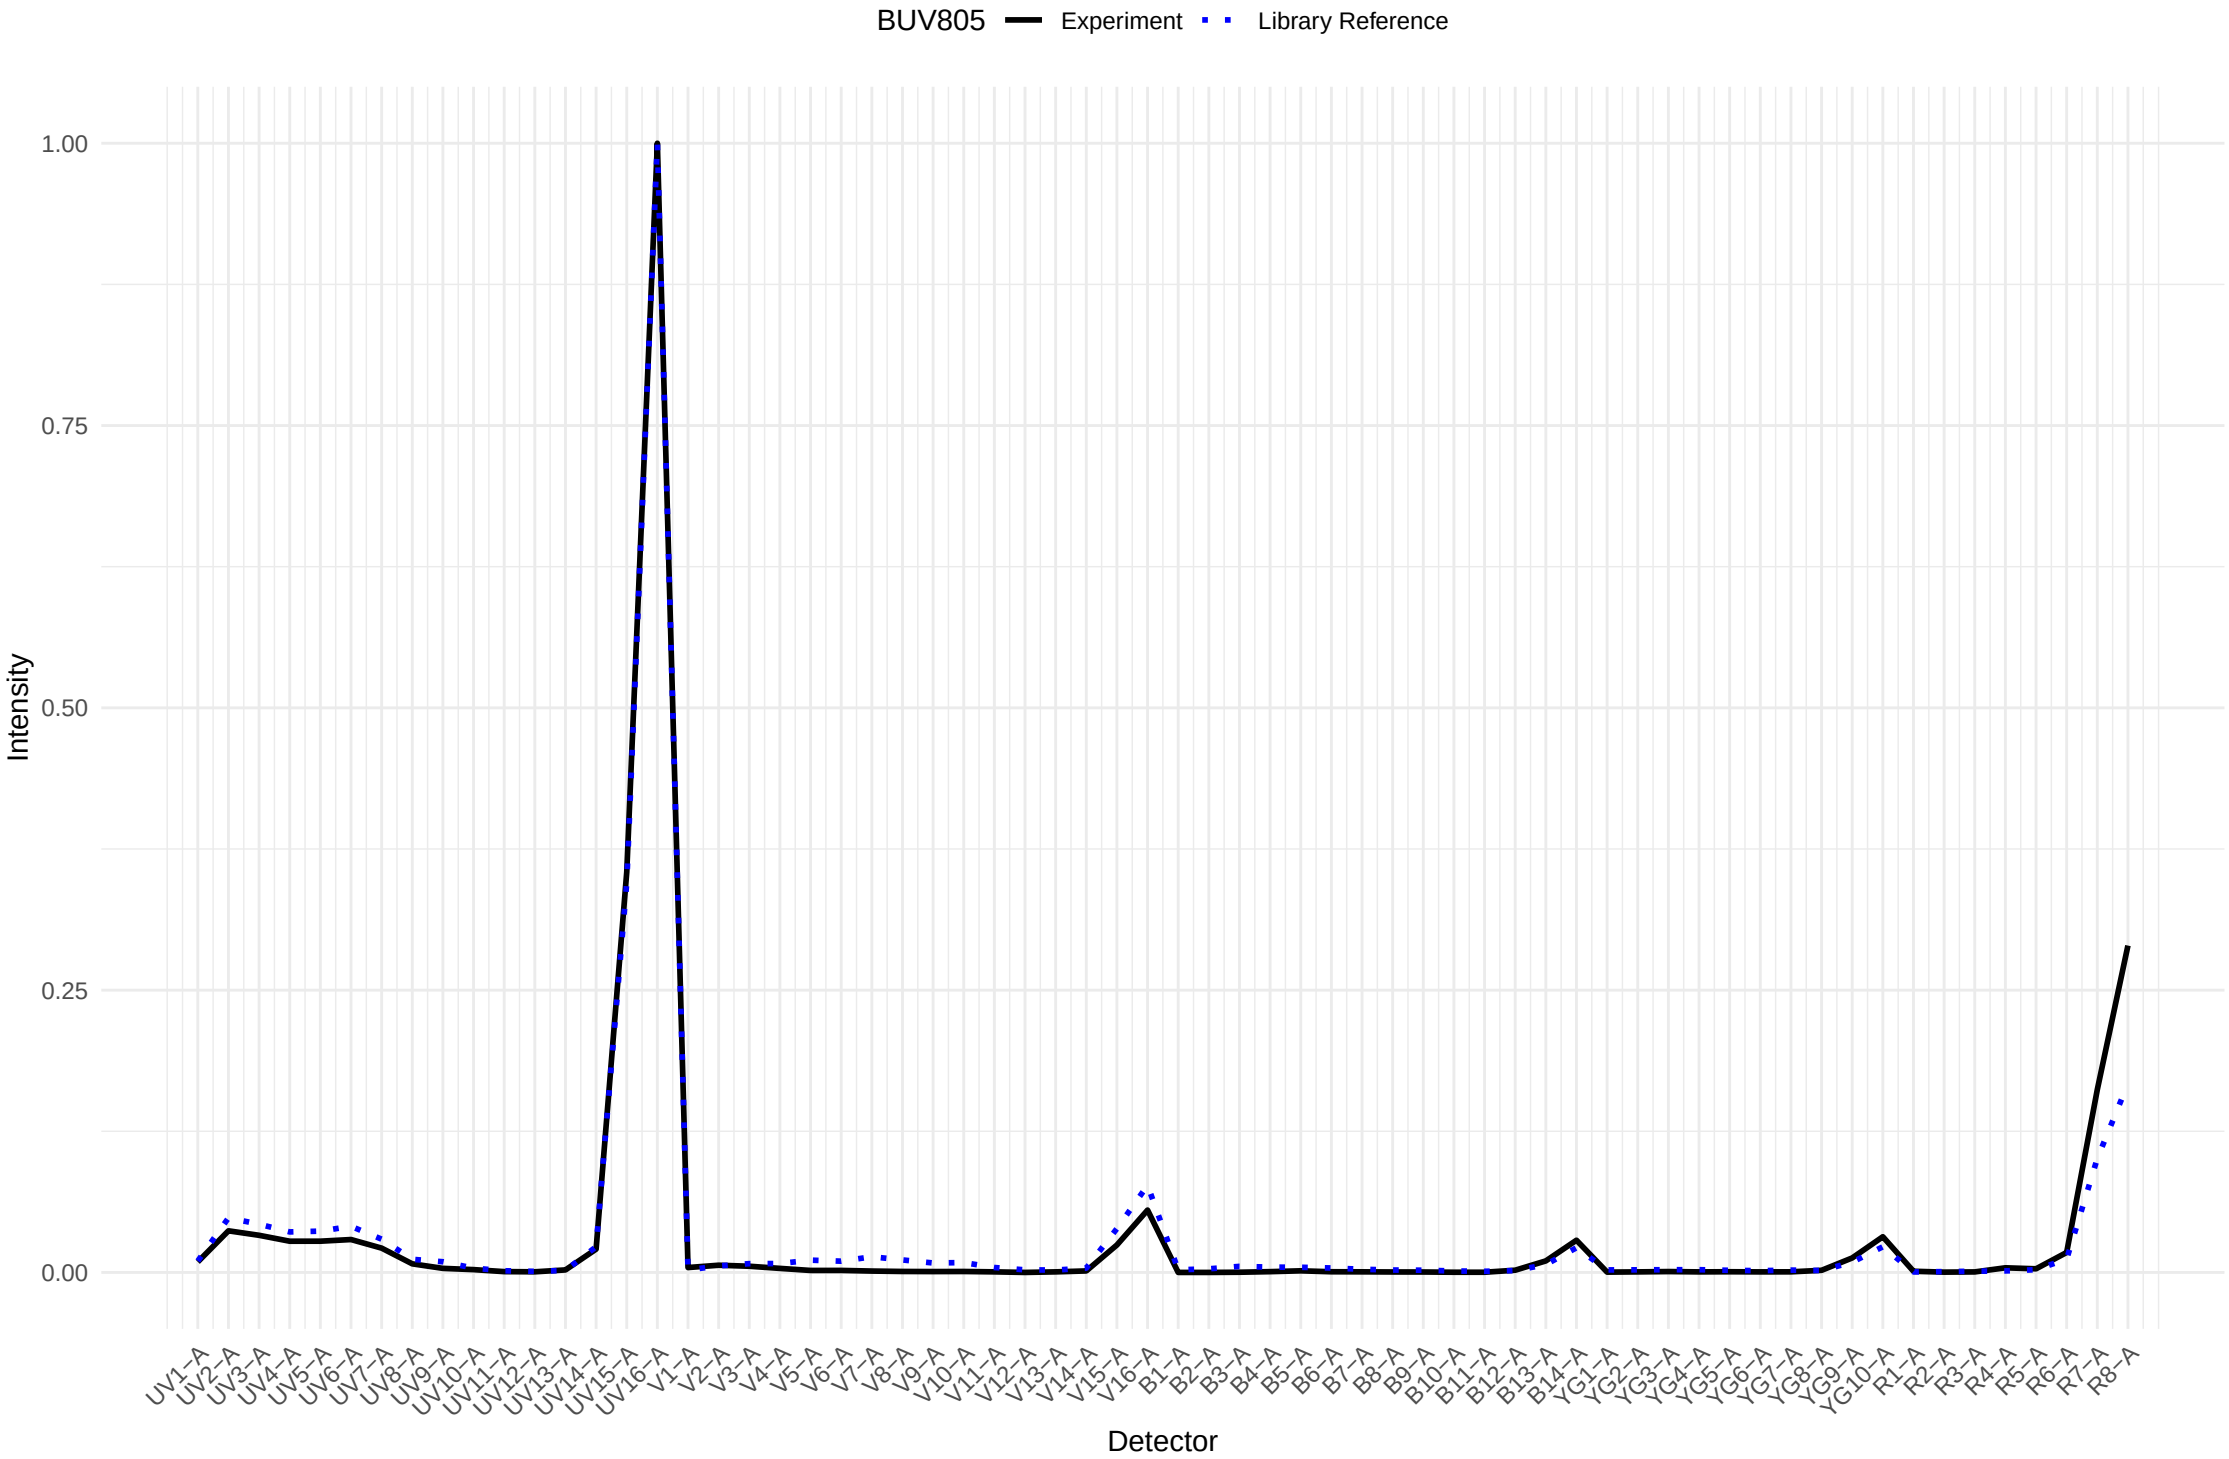

BV421

Cosine Similarity: 0.9936

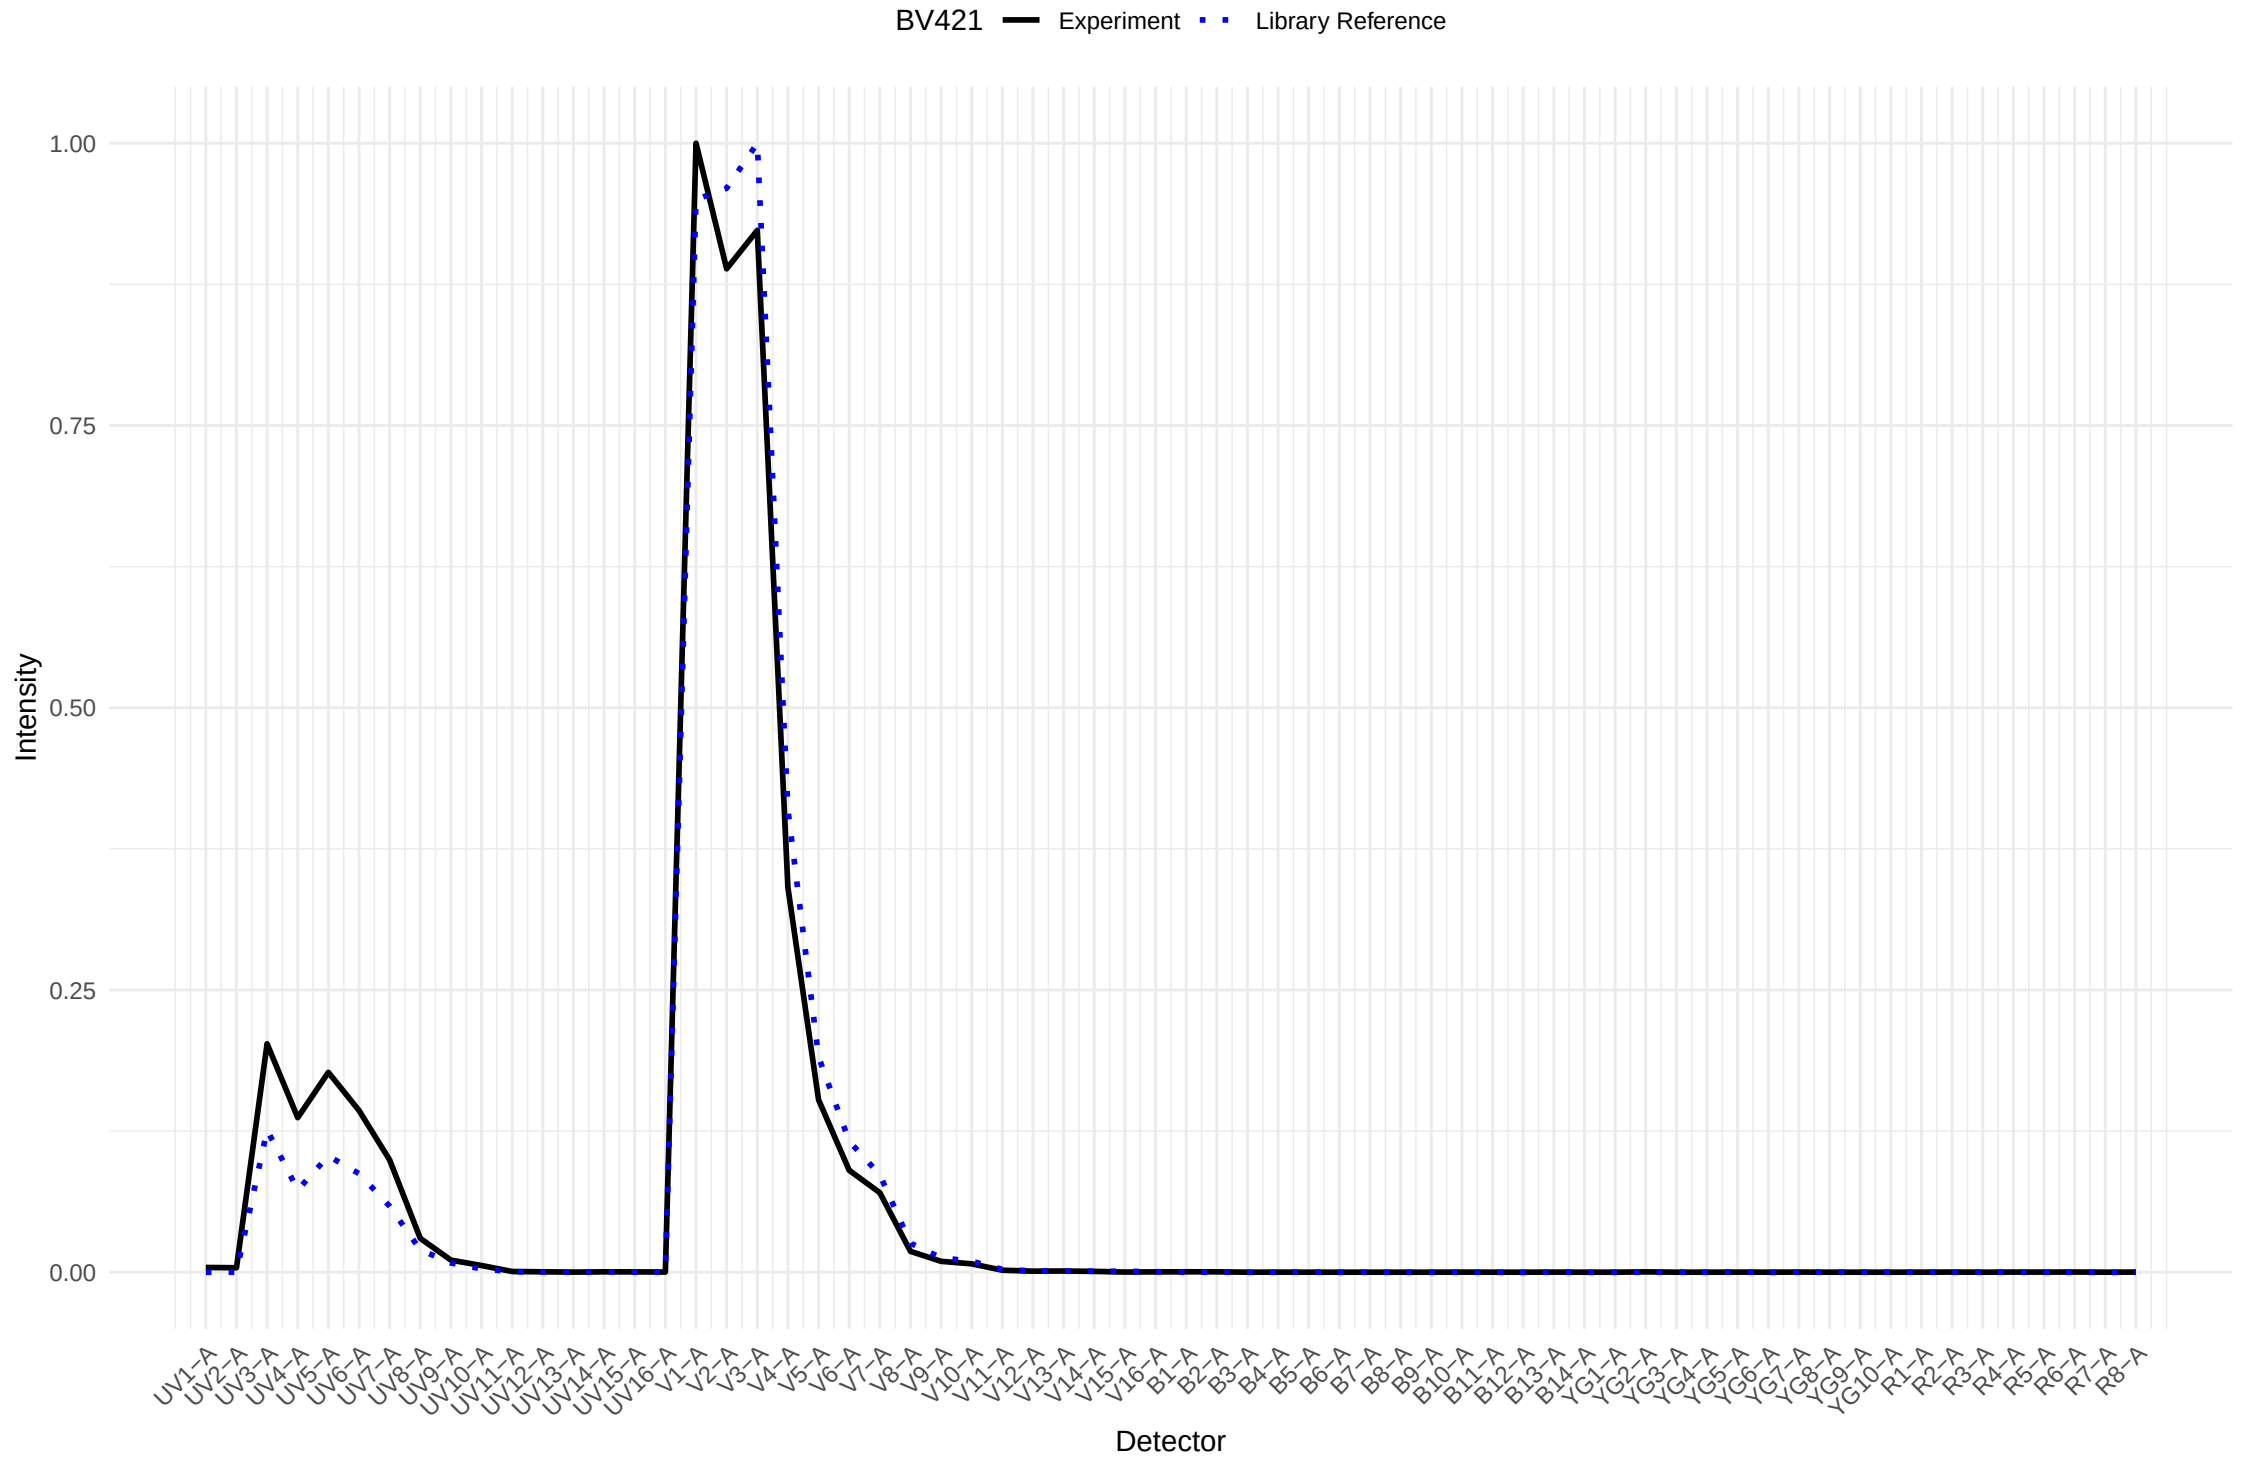

BV711

Cosine Similarity: 0.9372 [REFINED]

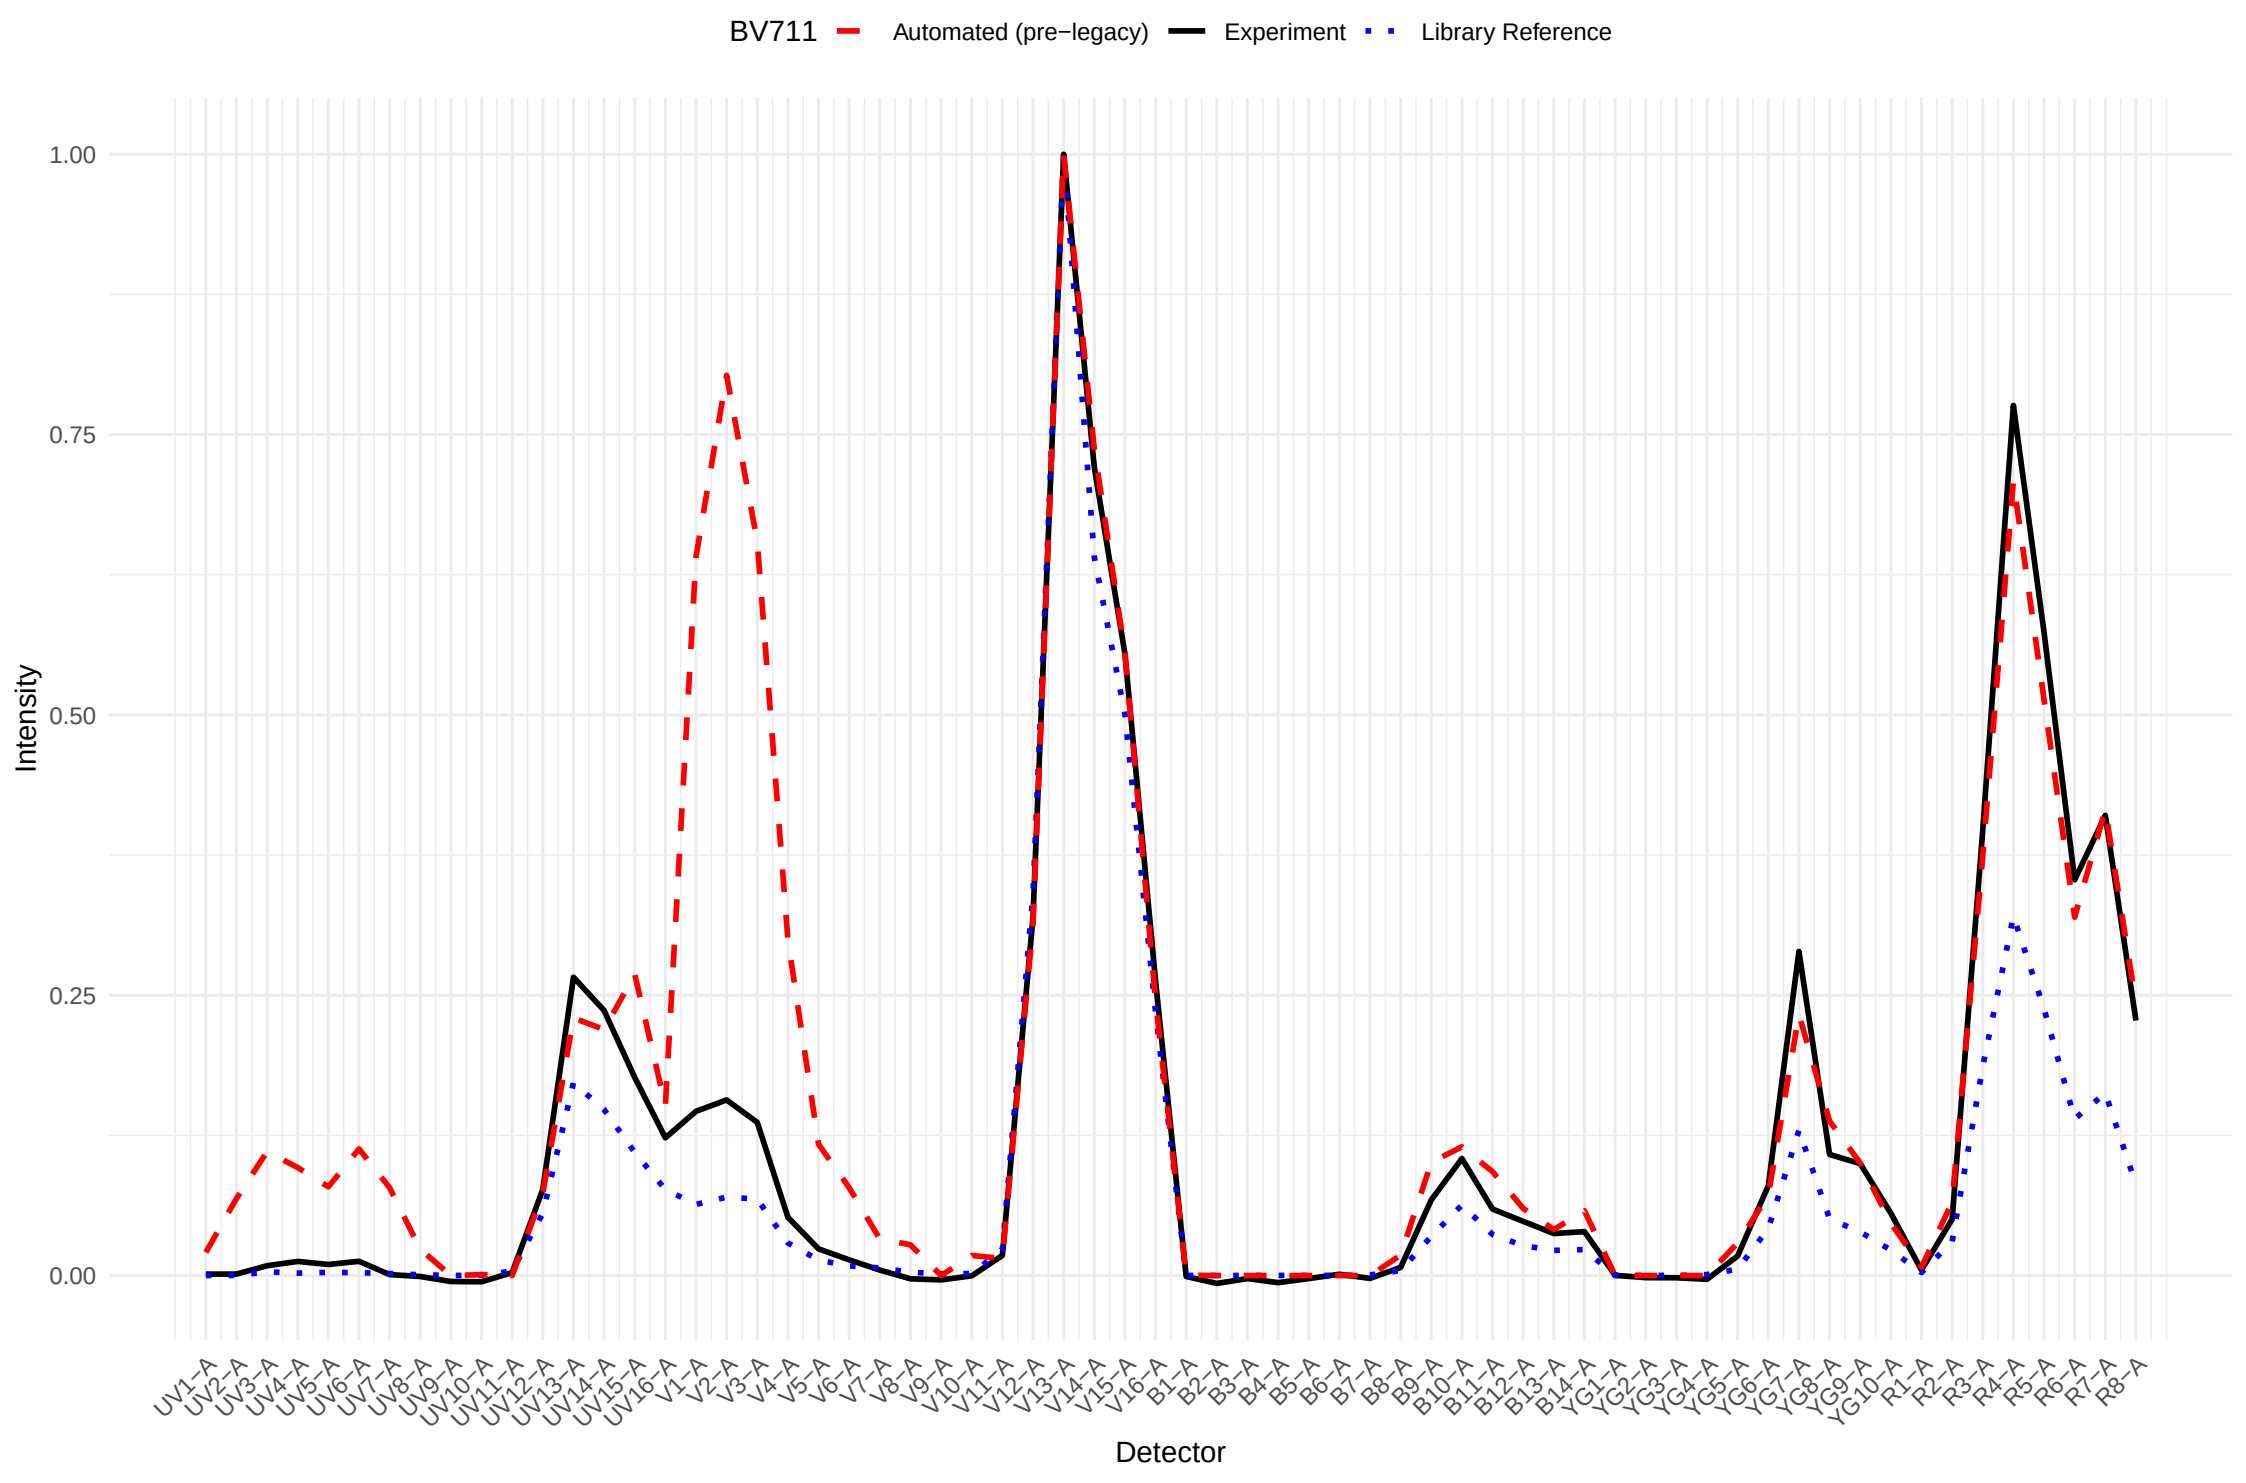

BB515

Cosine Similarity: 0.9998

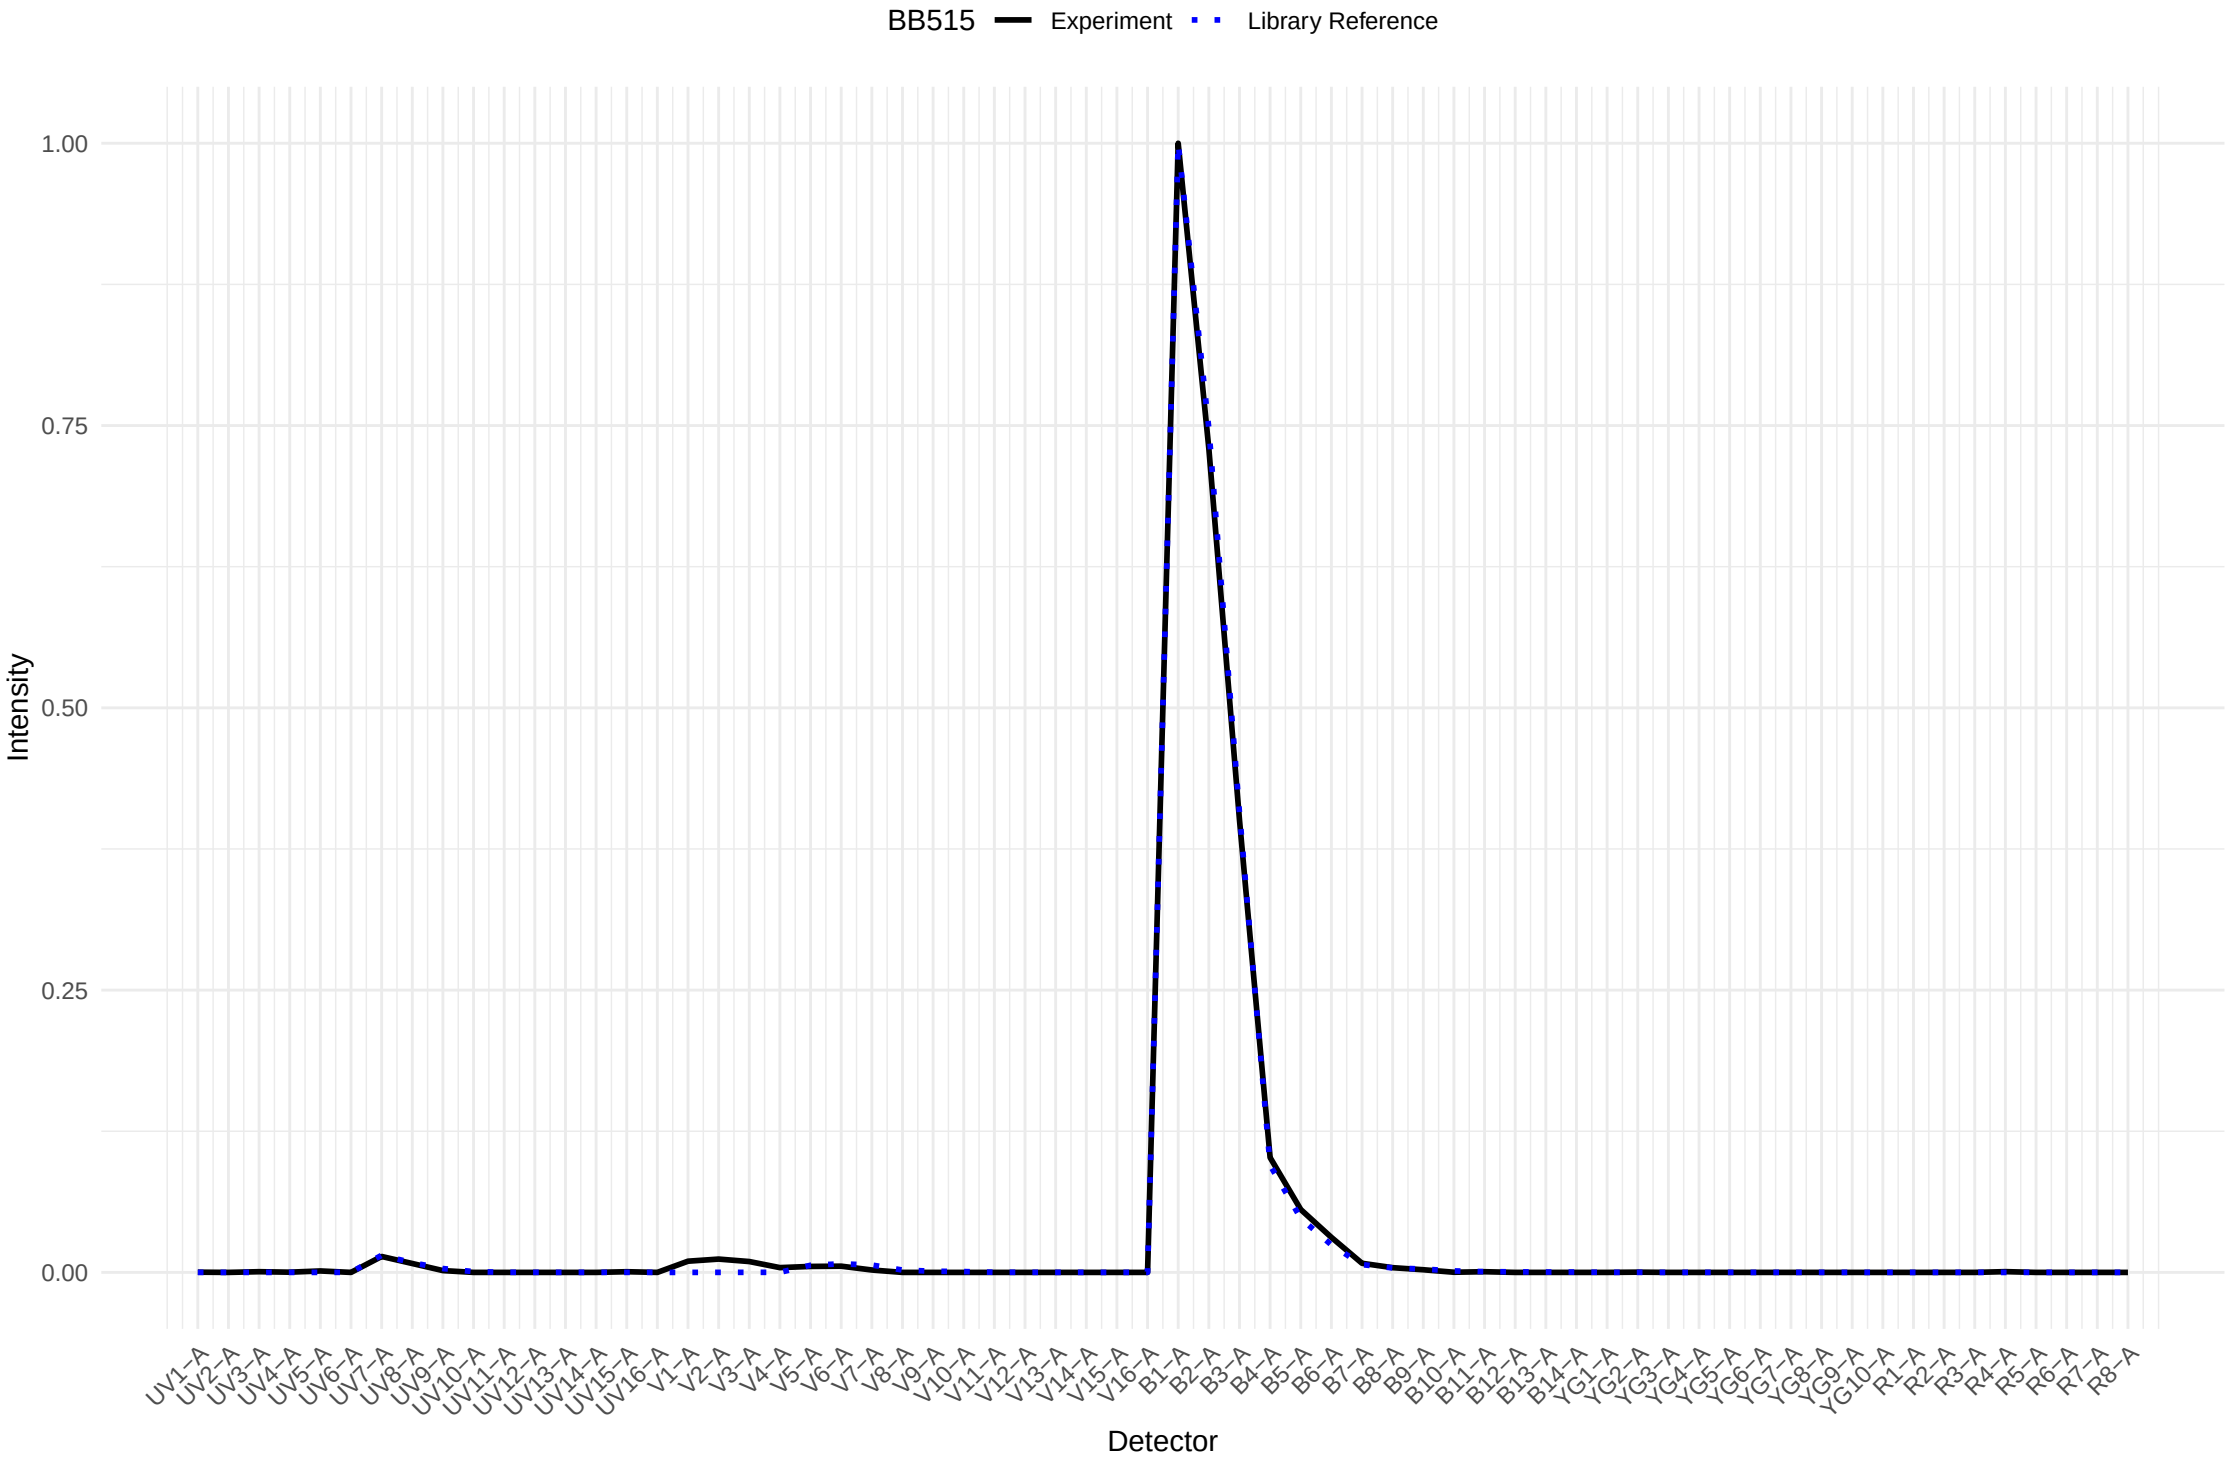

RB613

Cosine Similarity: 0.9942

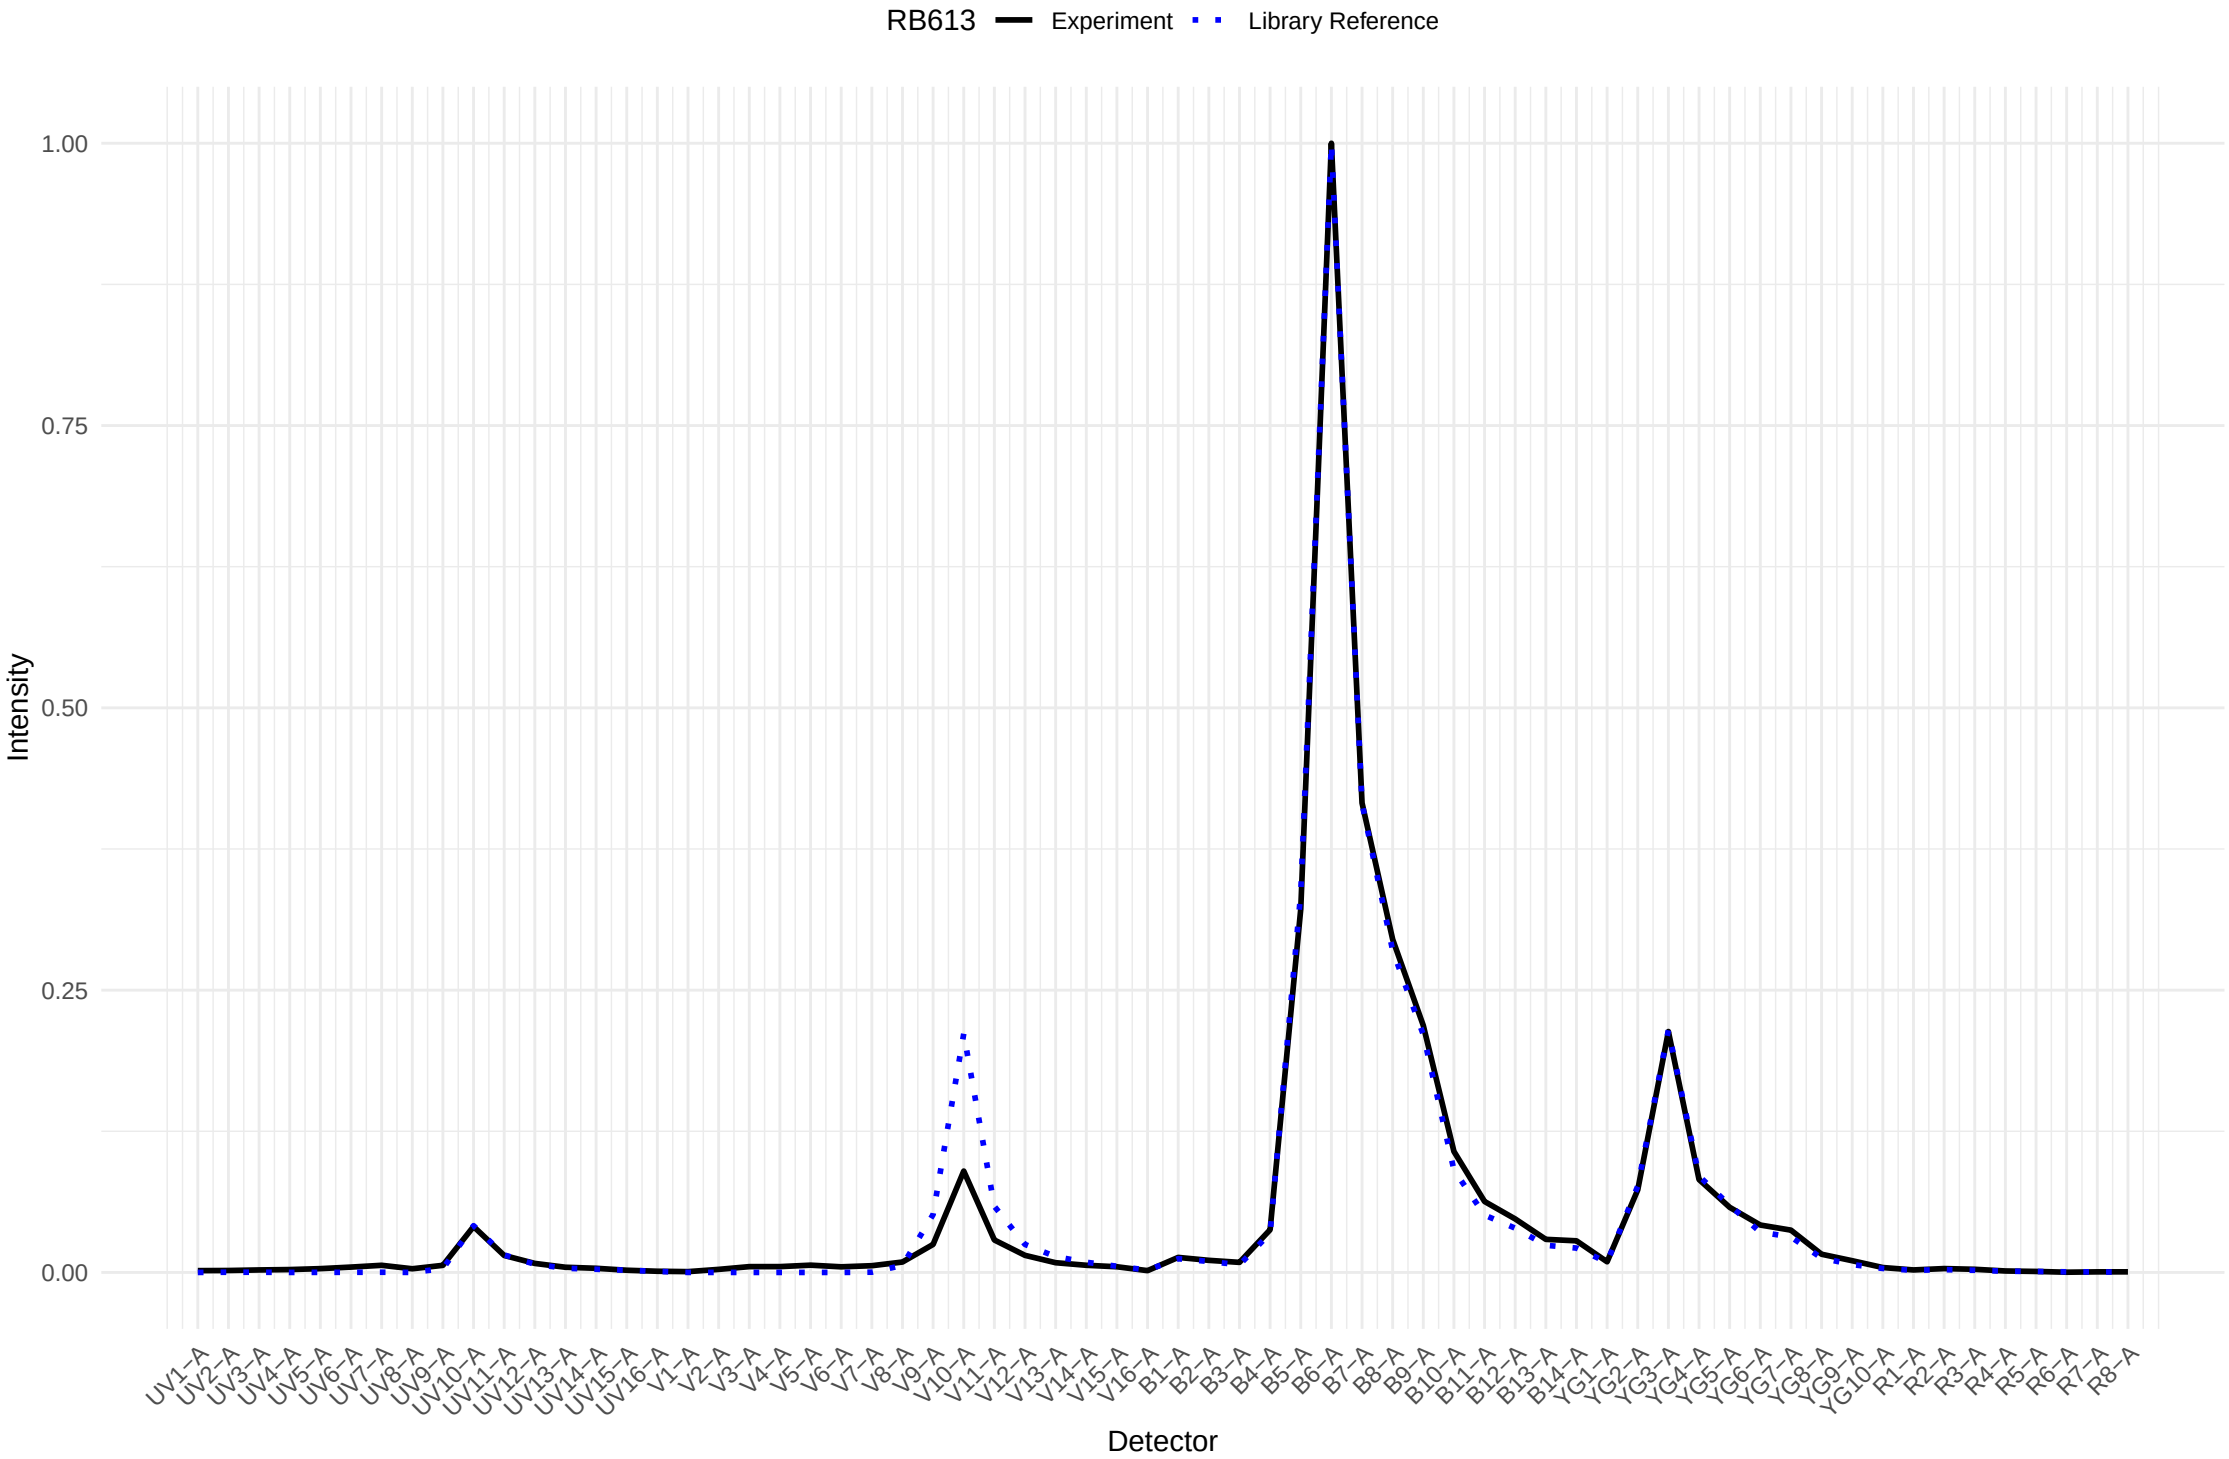

RB705

Cosine Similarity: 0.9944

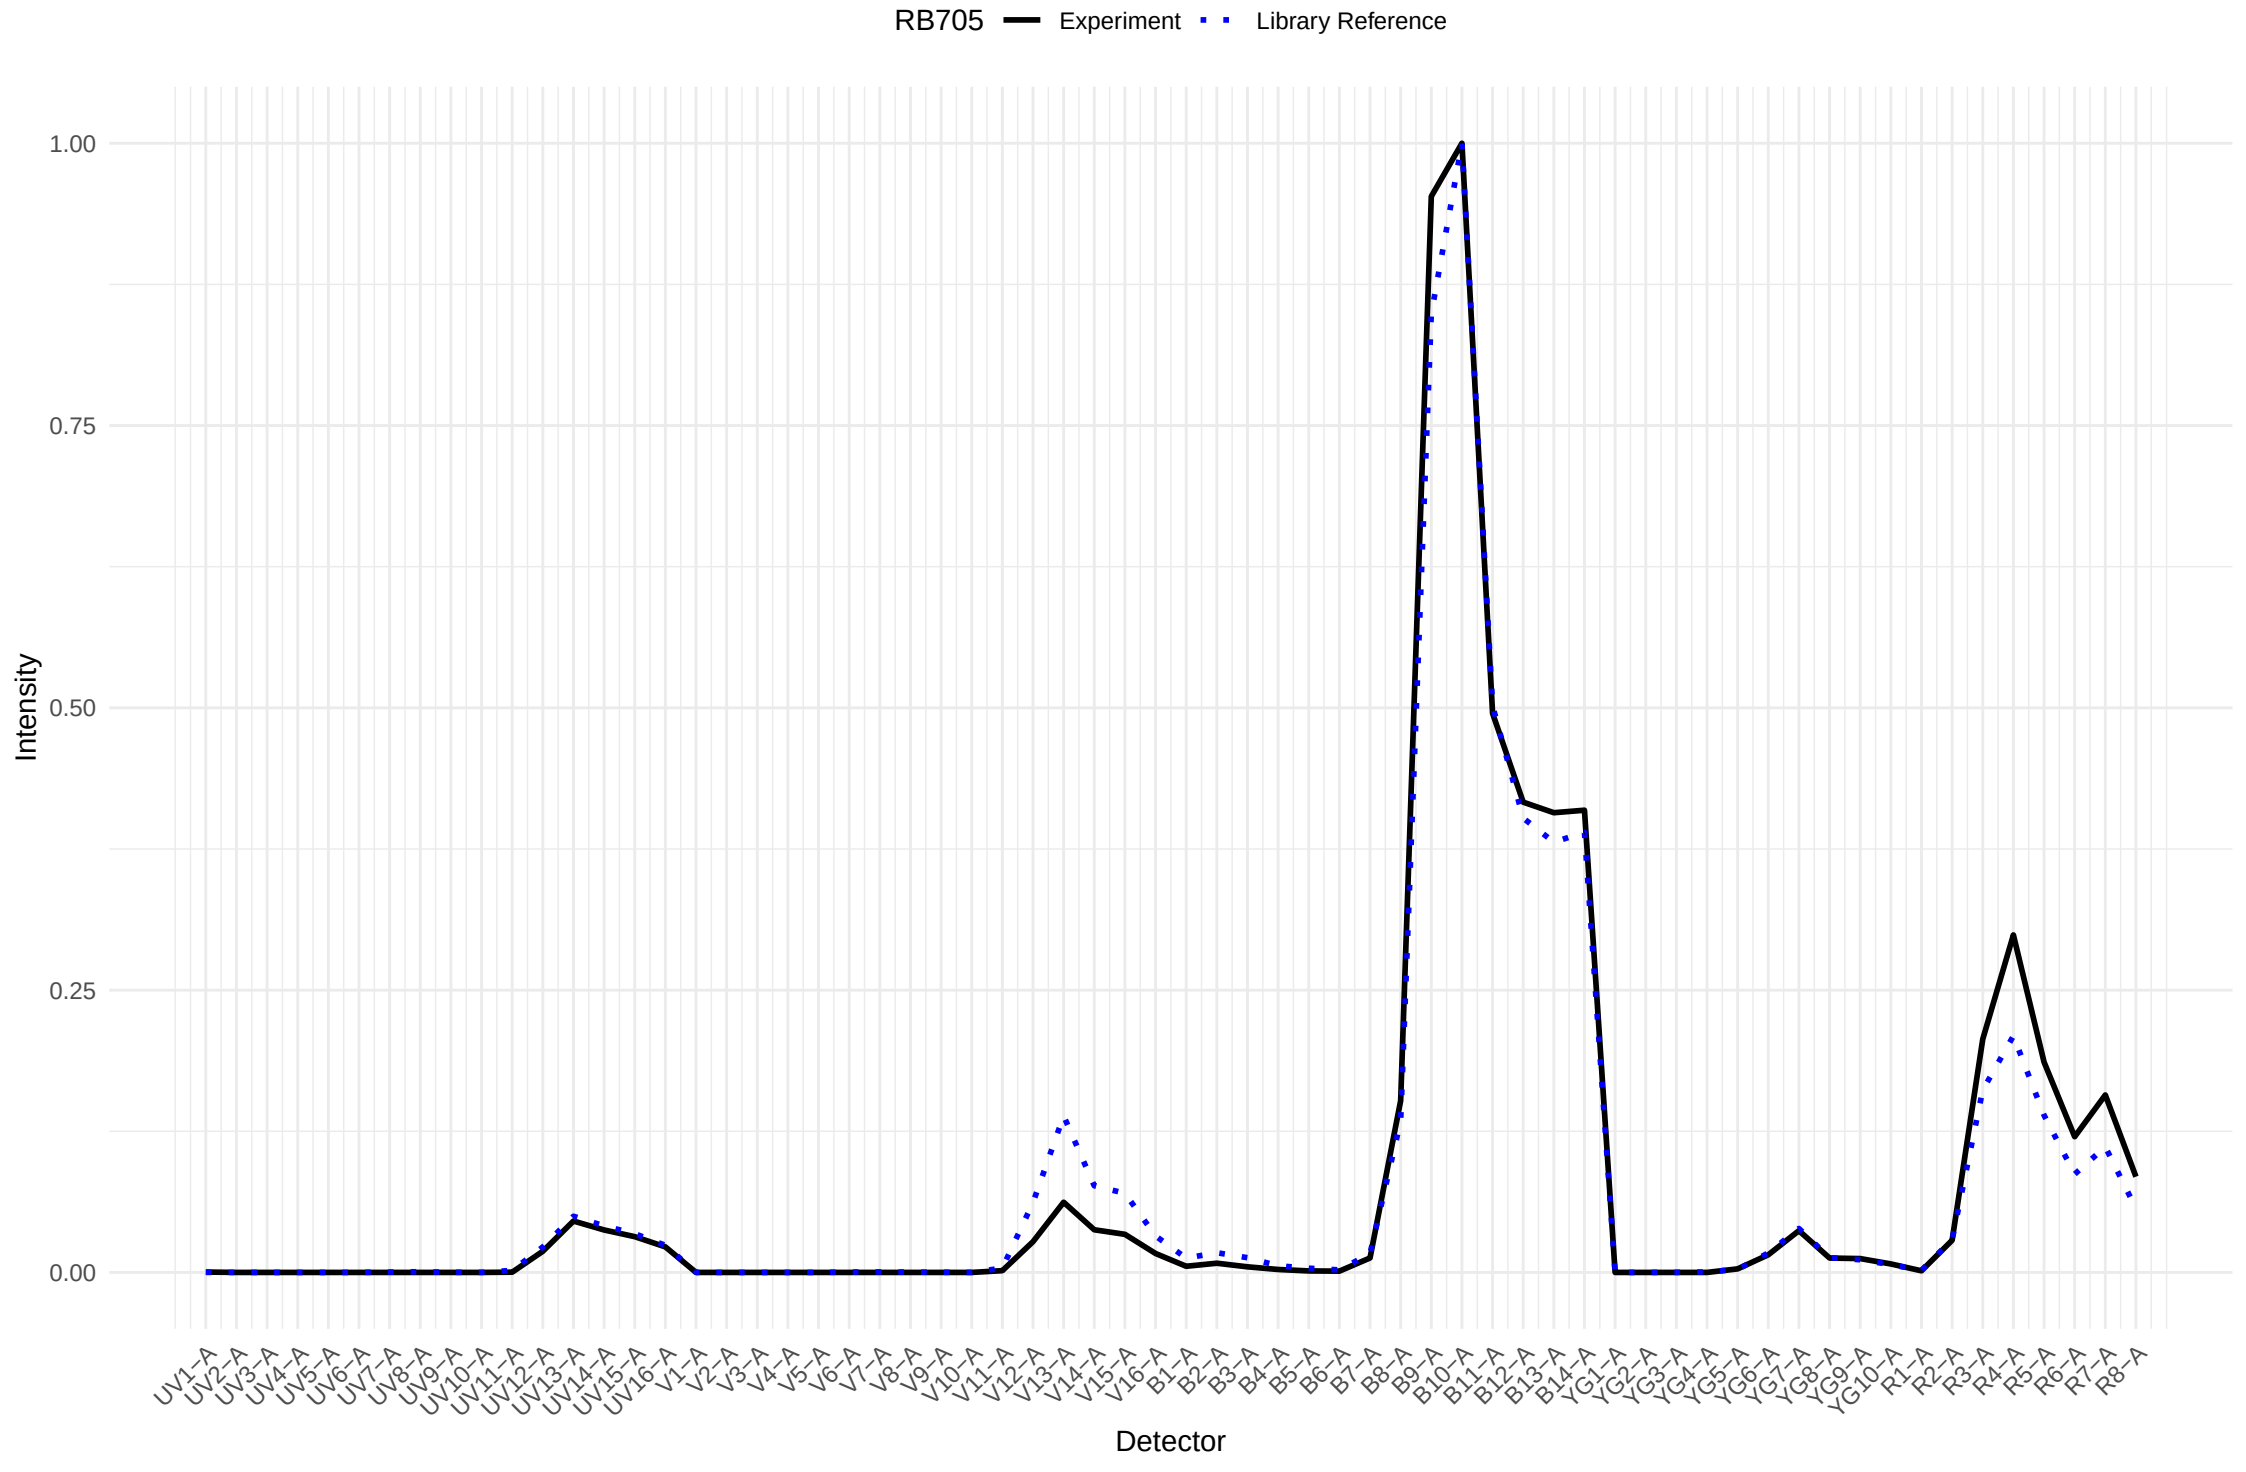

RB780

Cosine Similarity: 0.9976

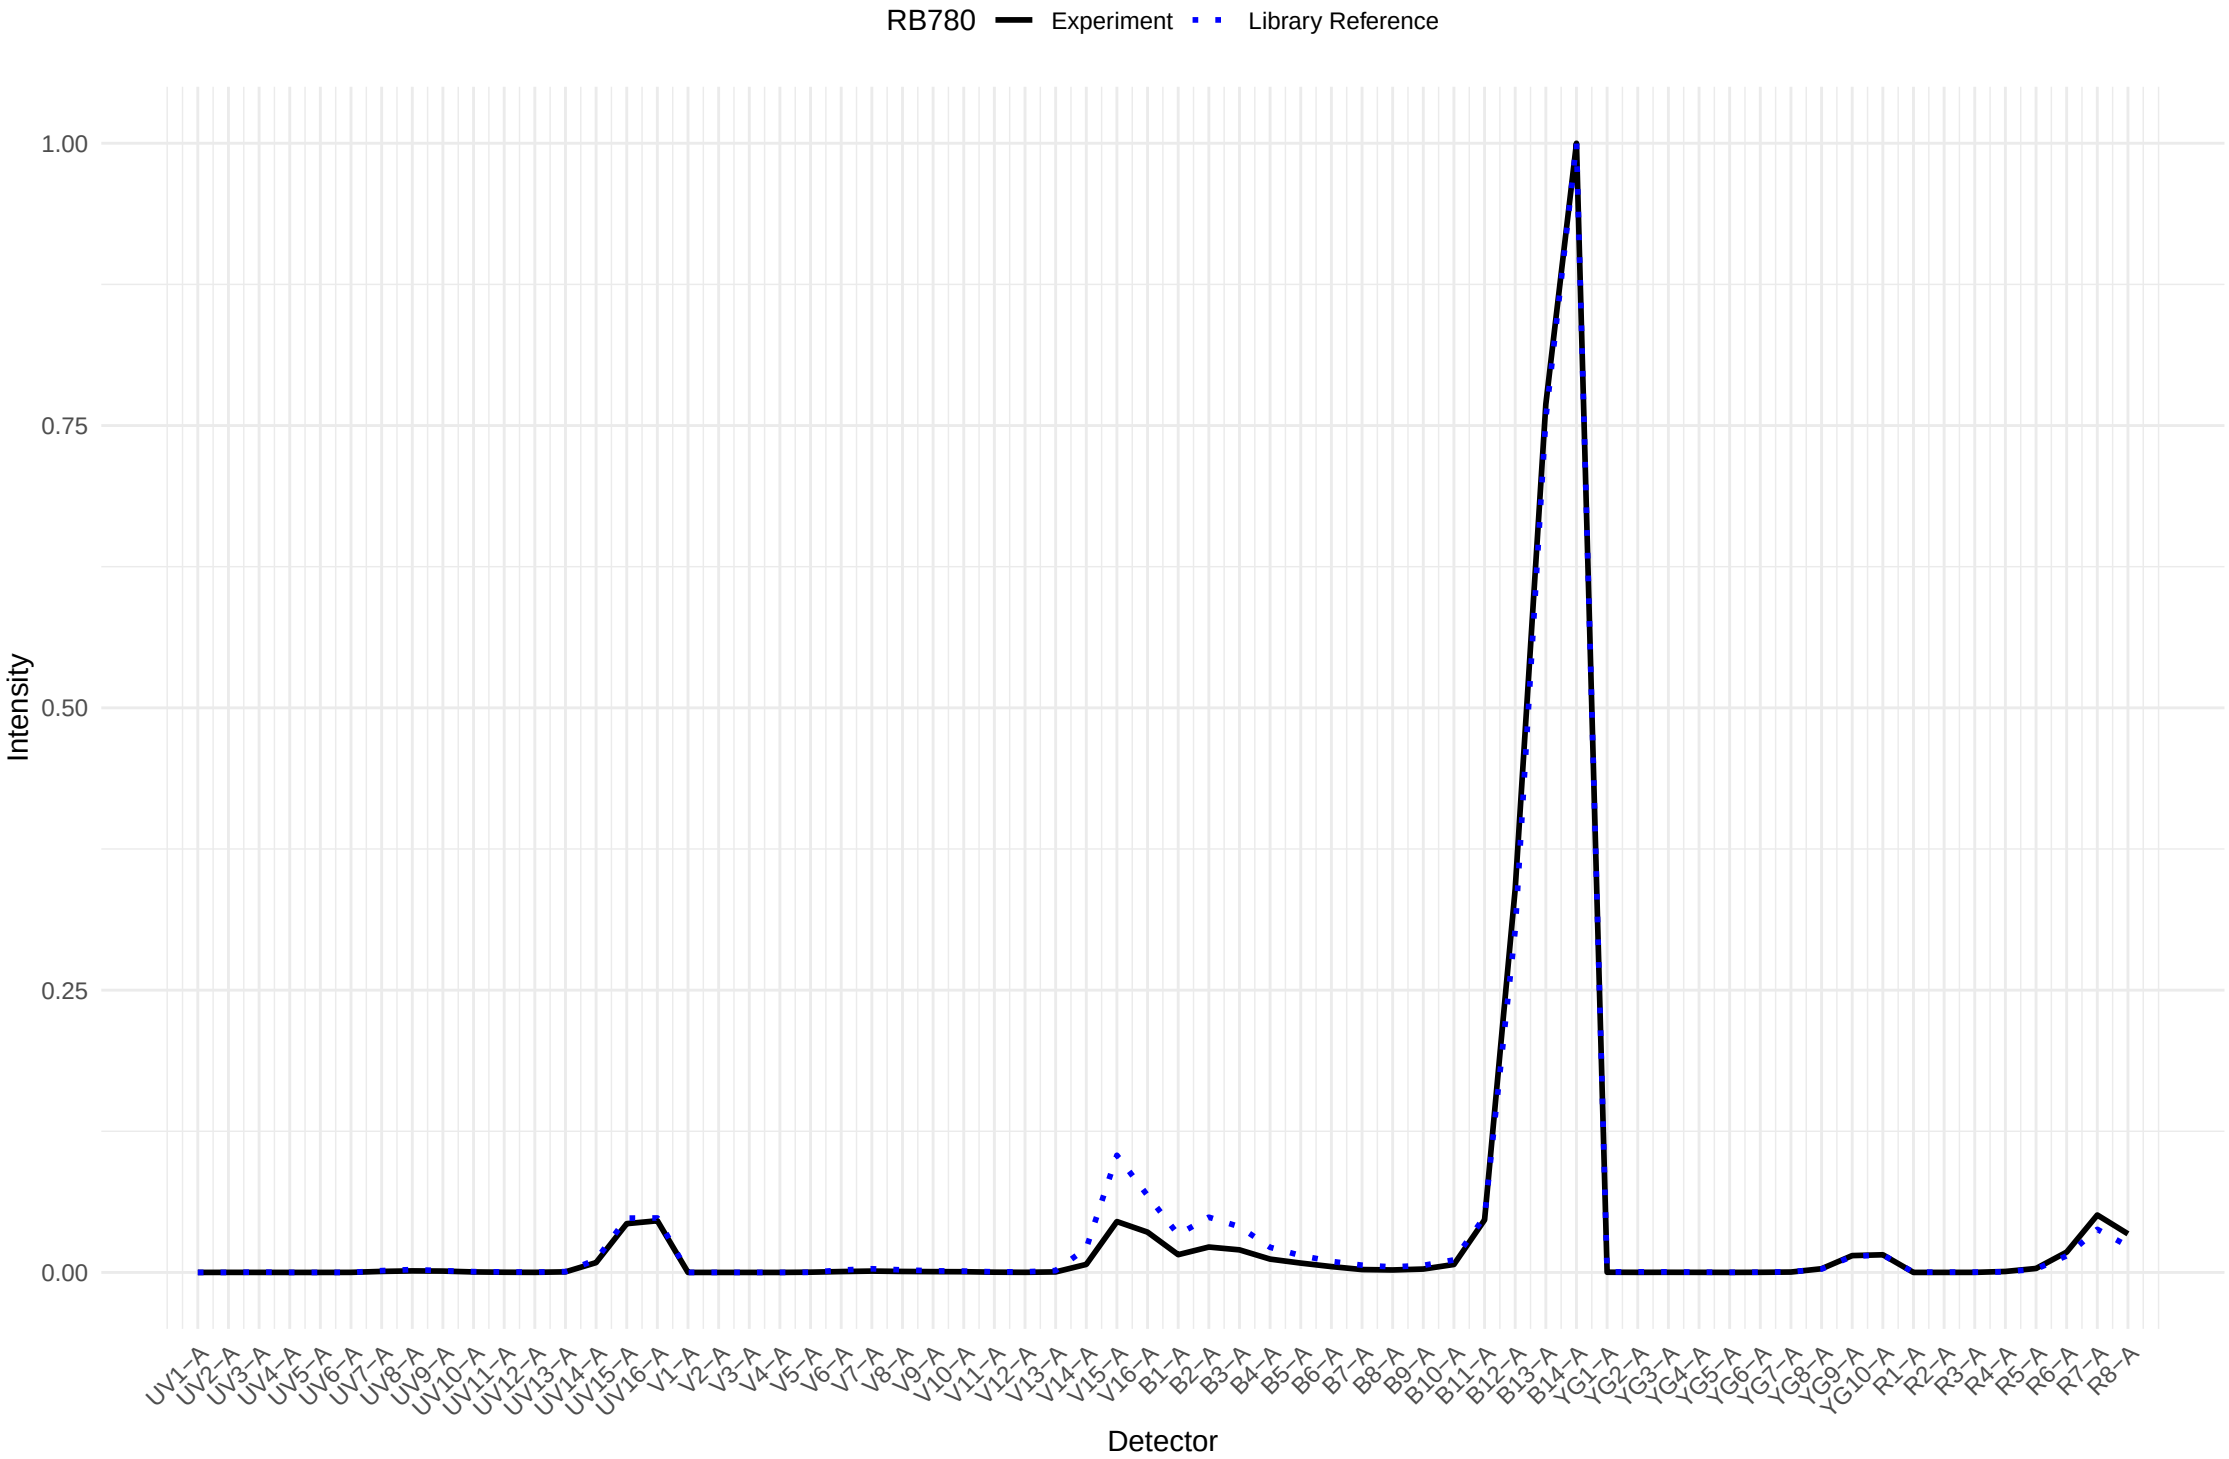

PE

Cosine Similarity: 0.9913

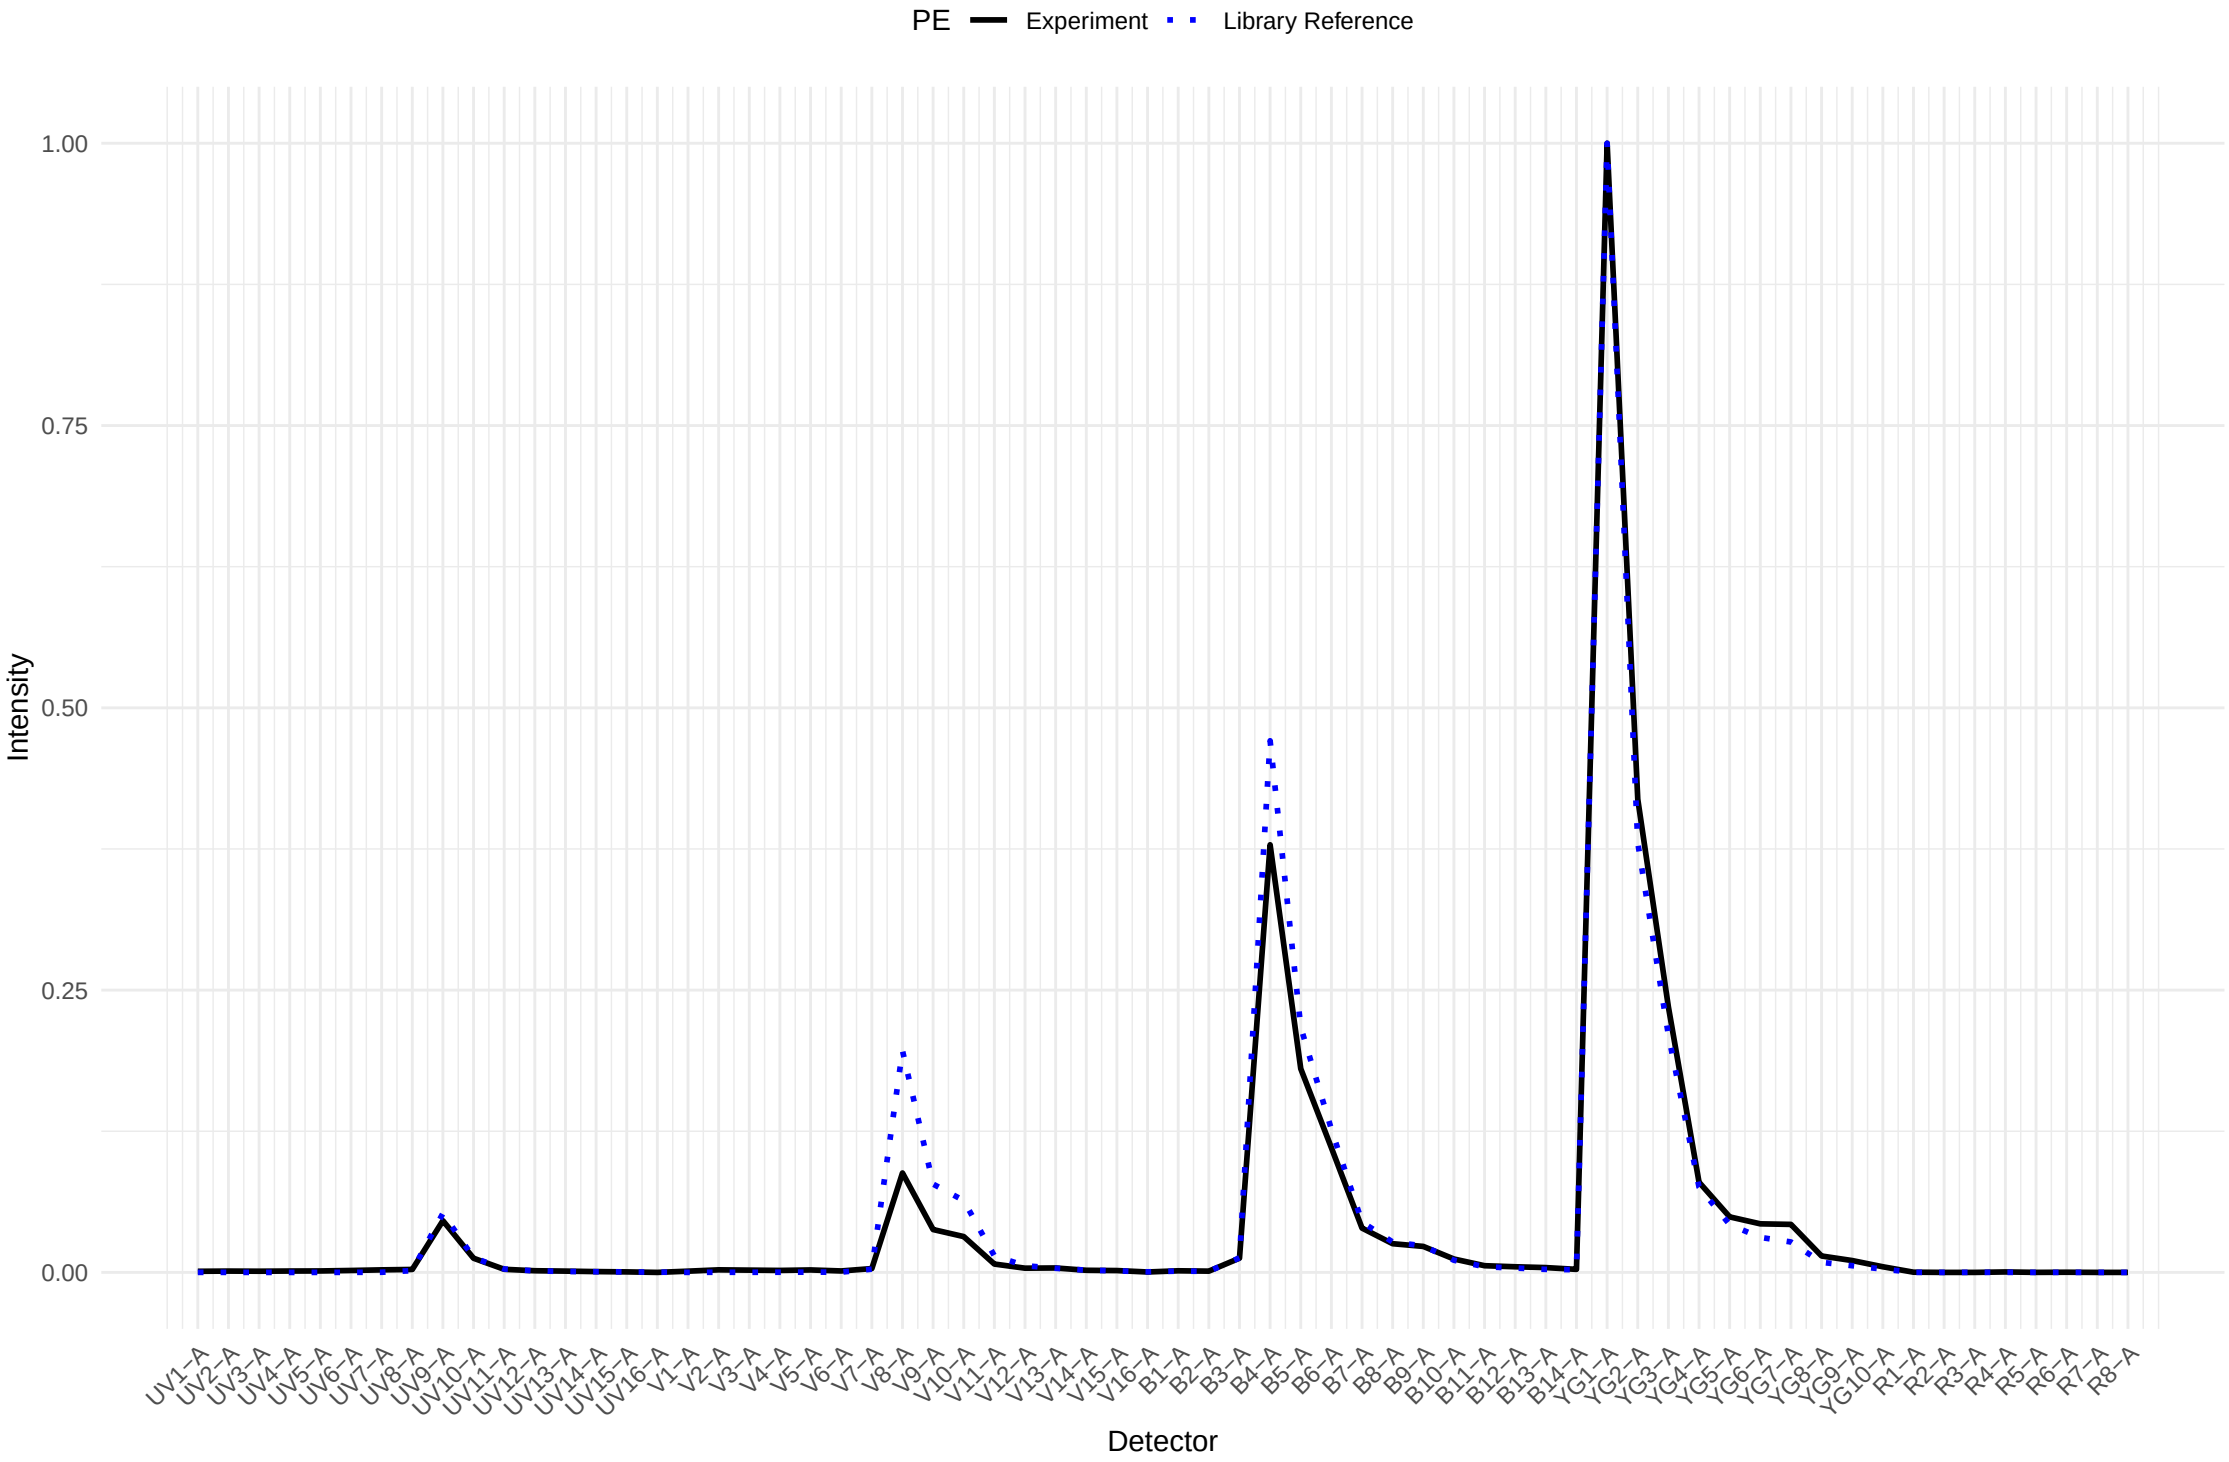

RY655

Cosine Similarity: 0.9918

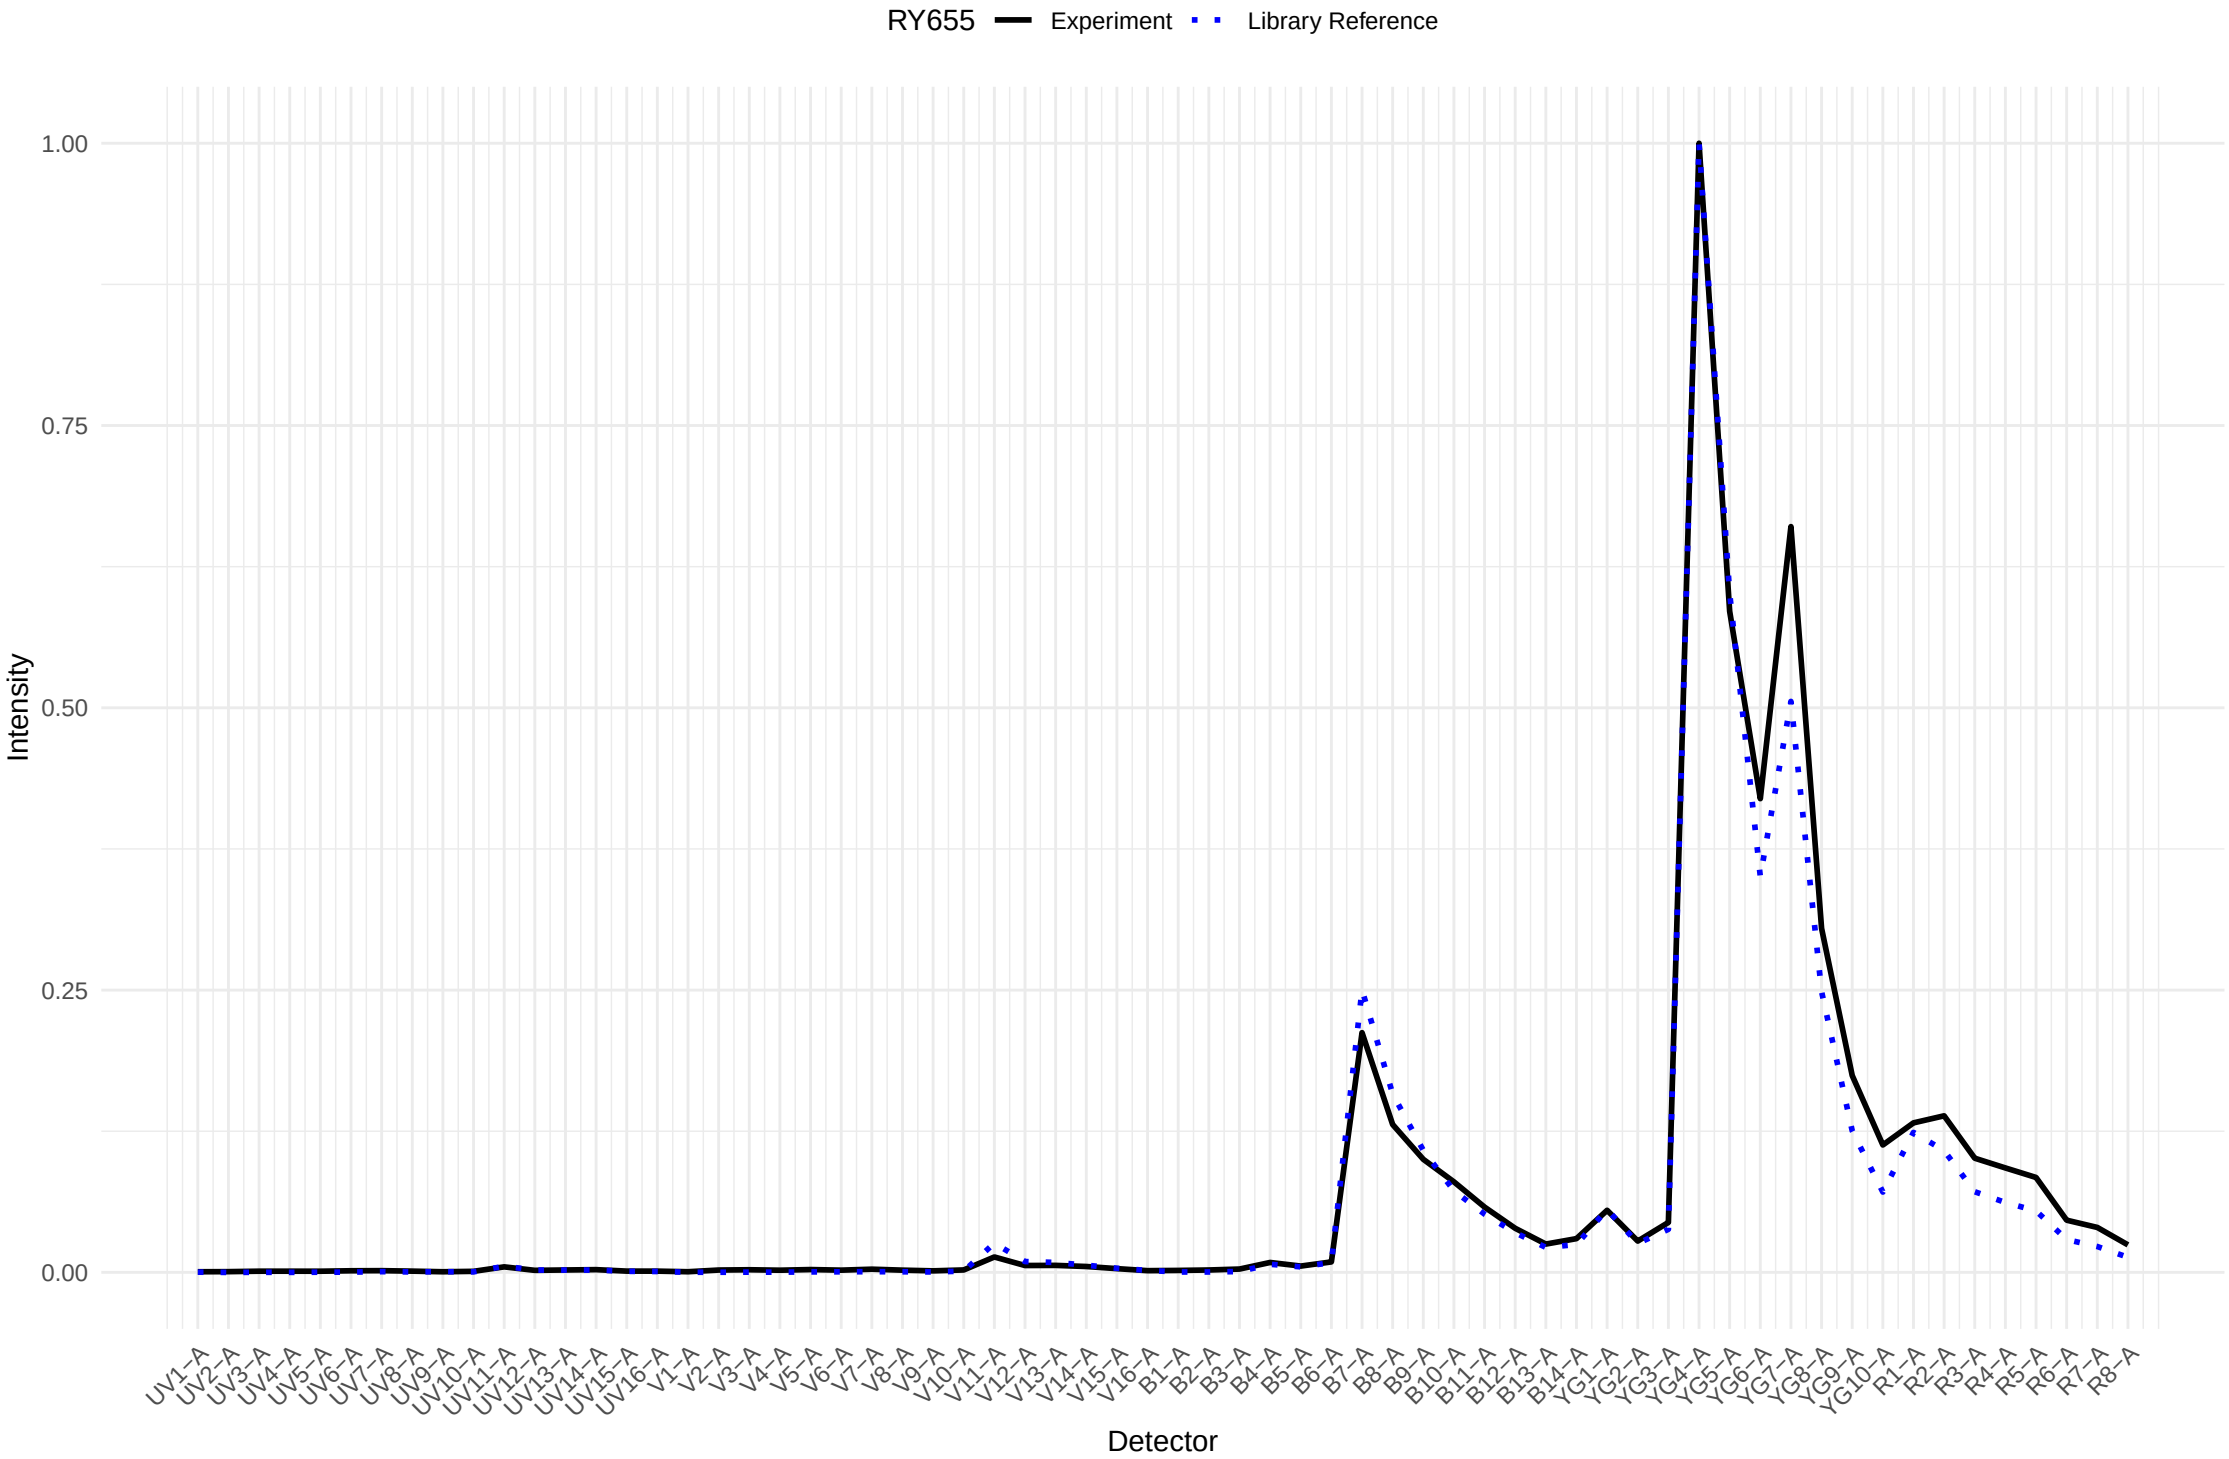

RY703

Cosine Similarity: 0.9988

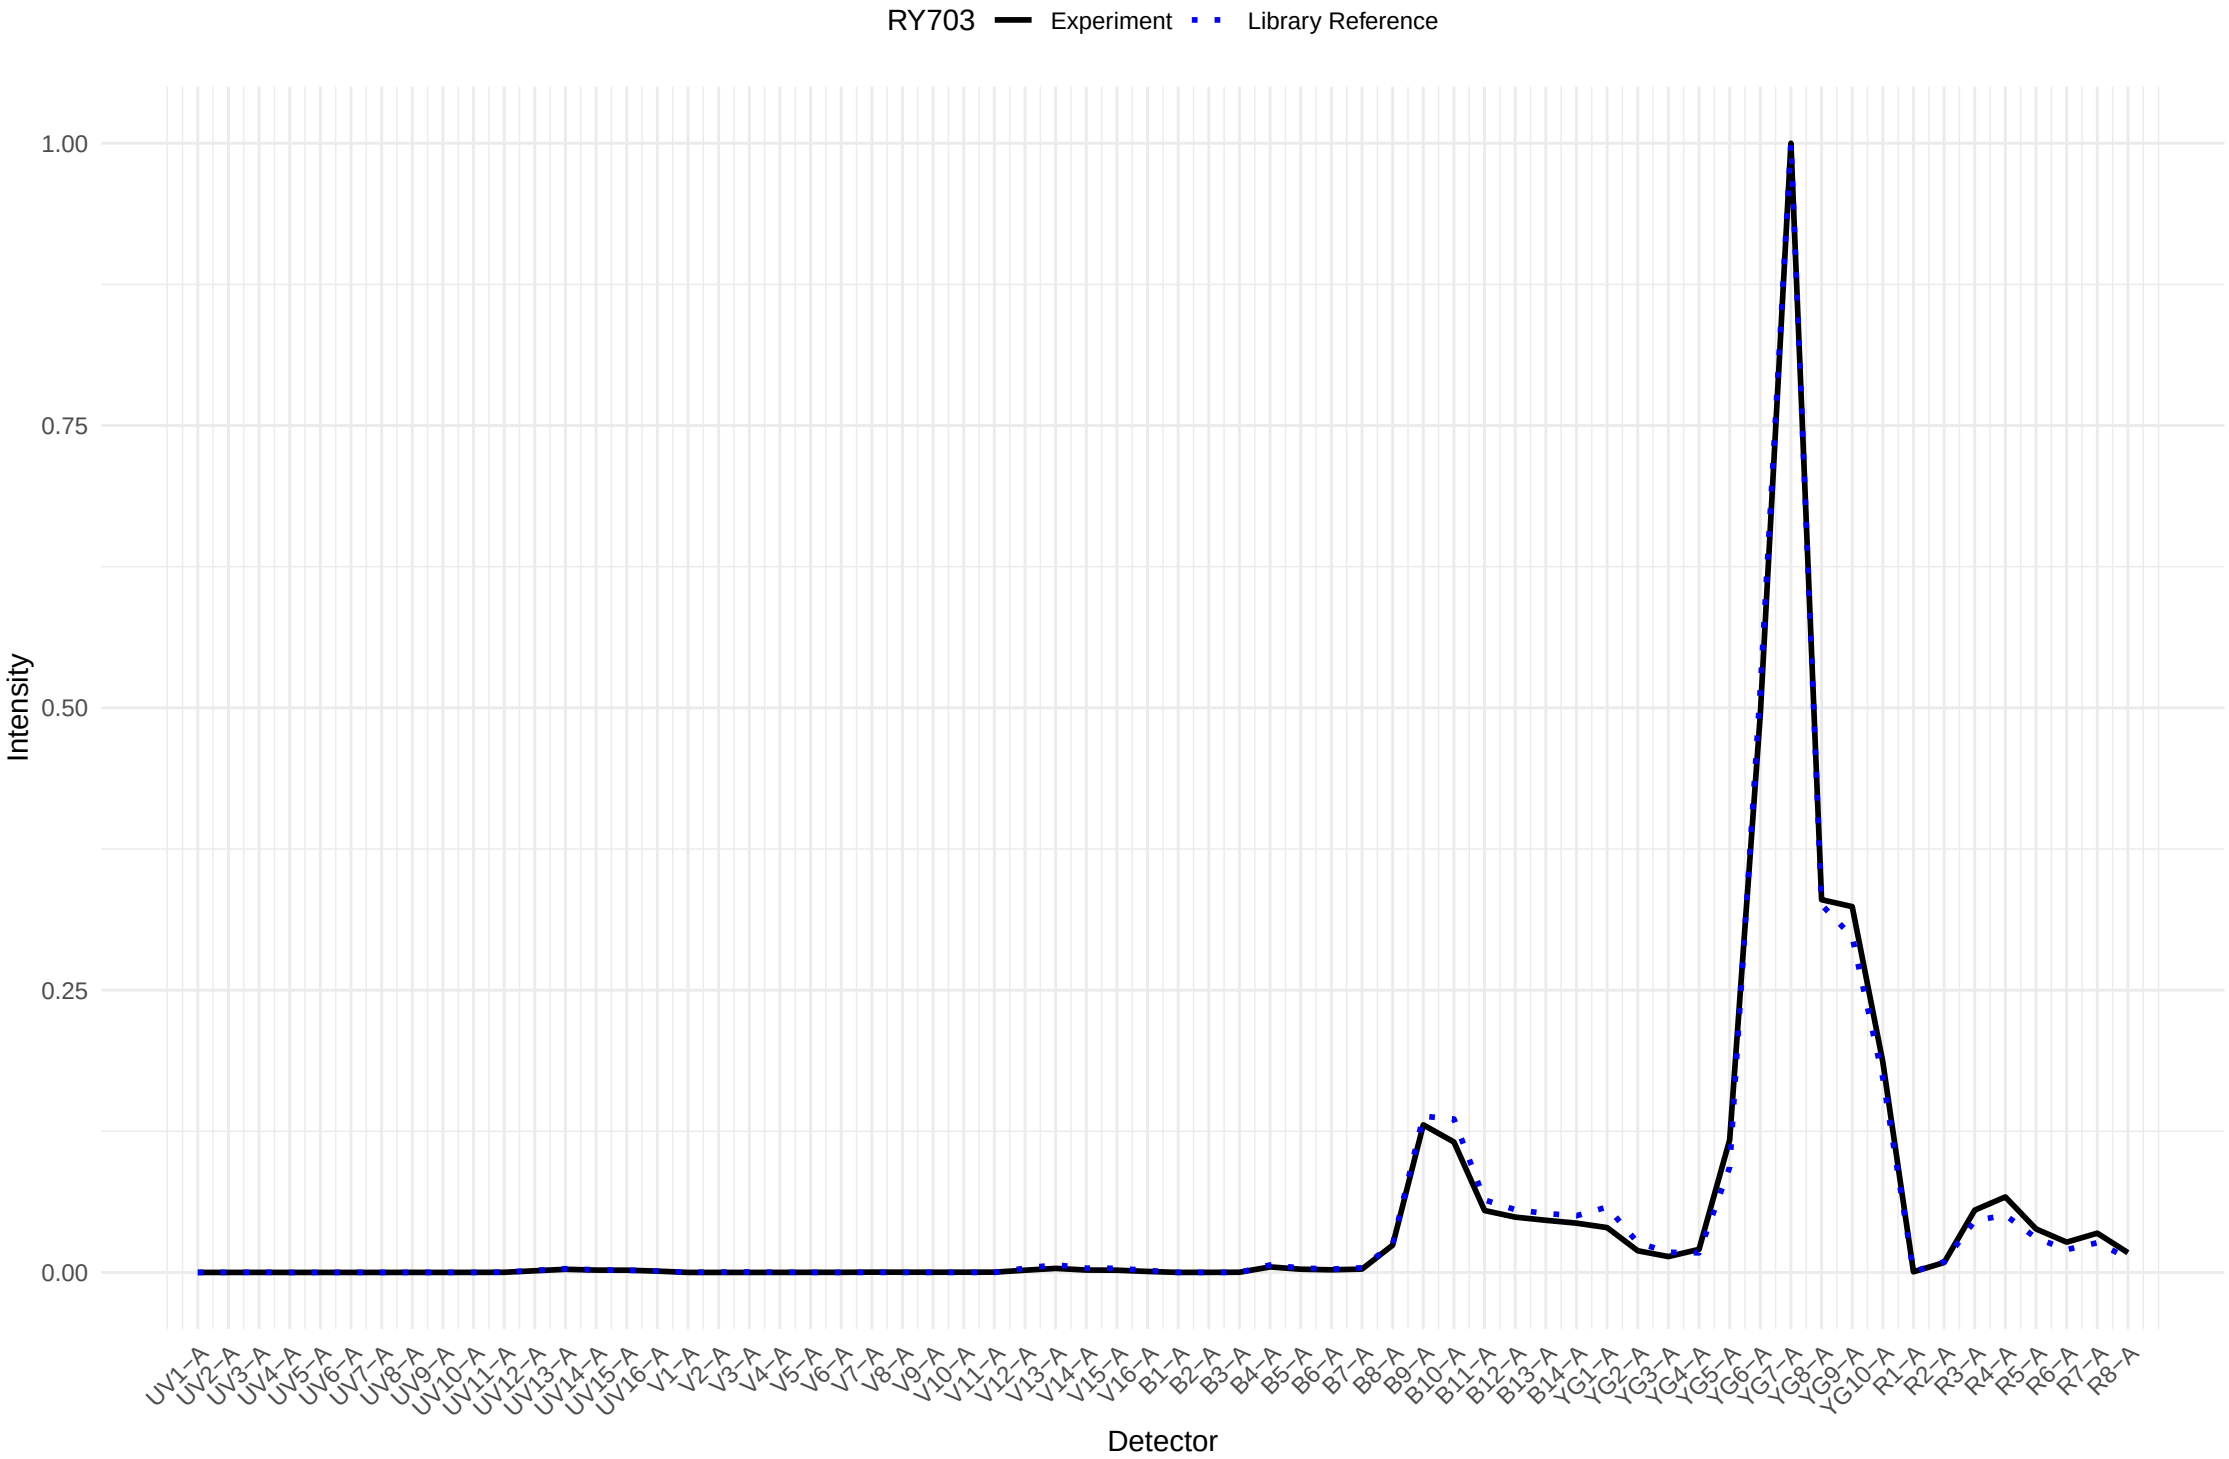

PE−Cy7

Cosine Similarity: 0.9931

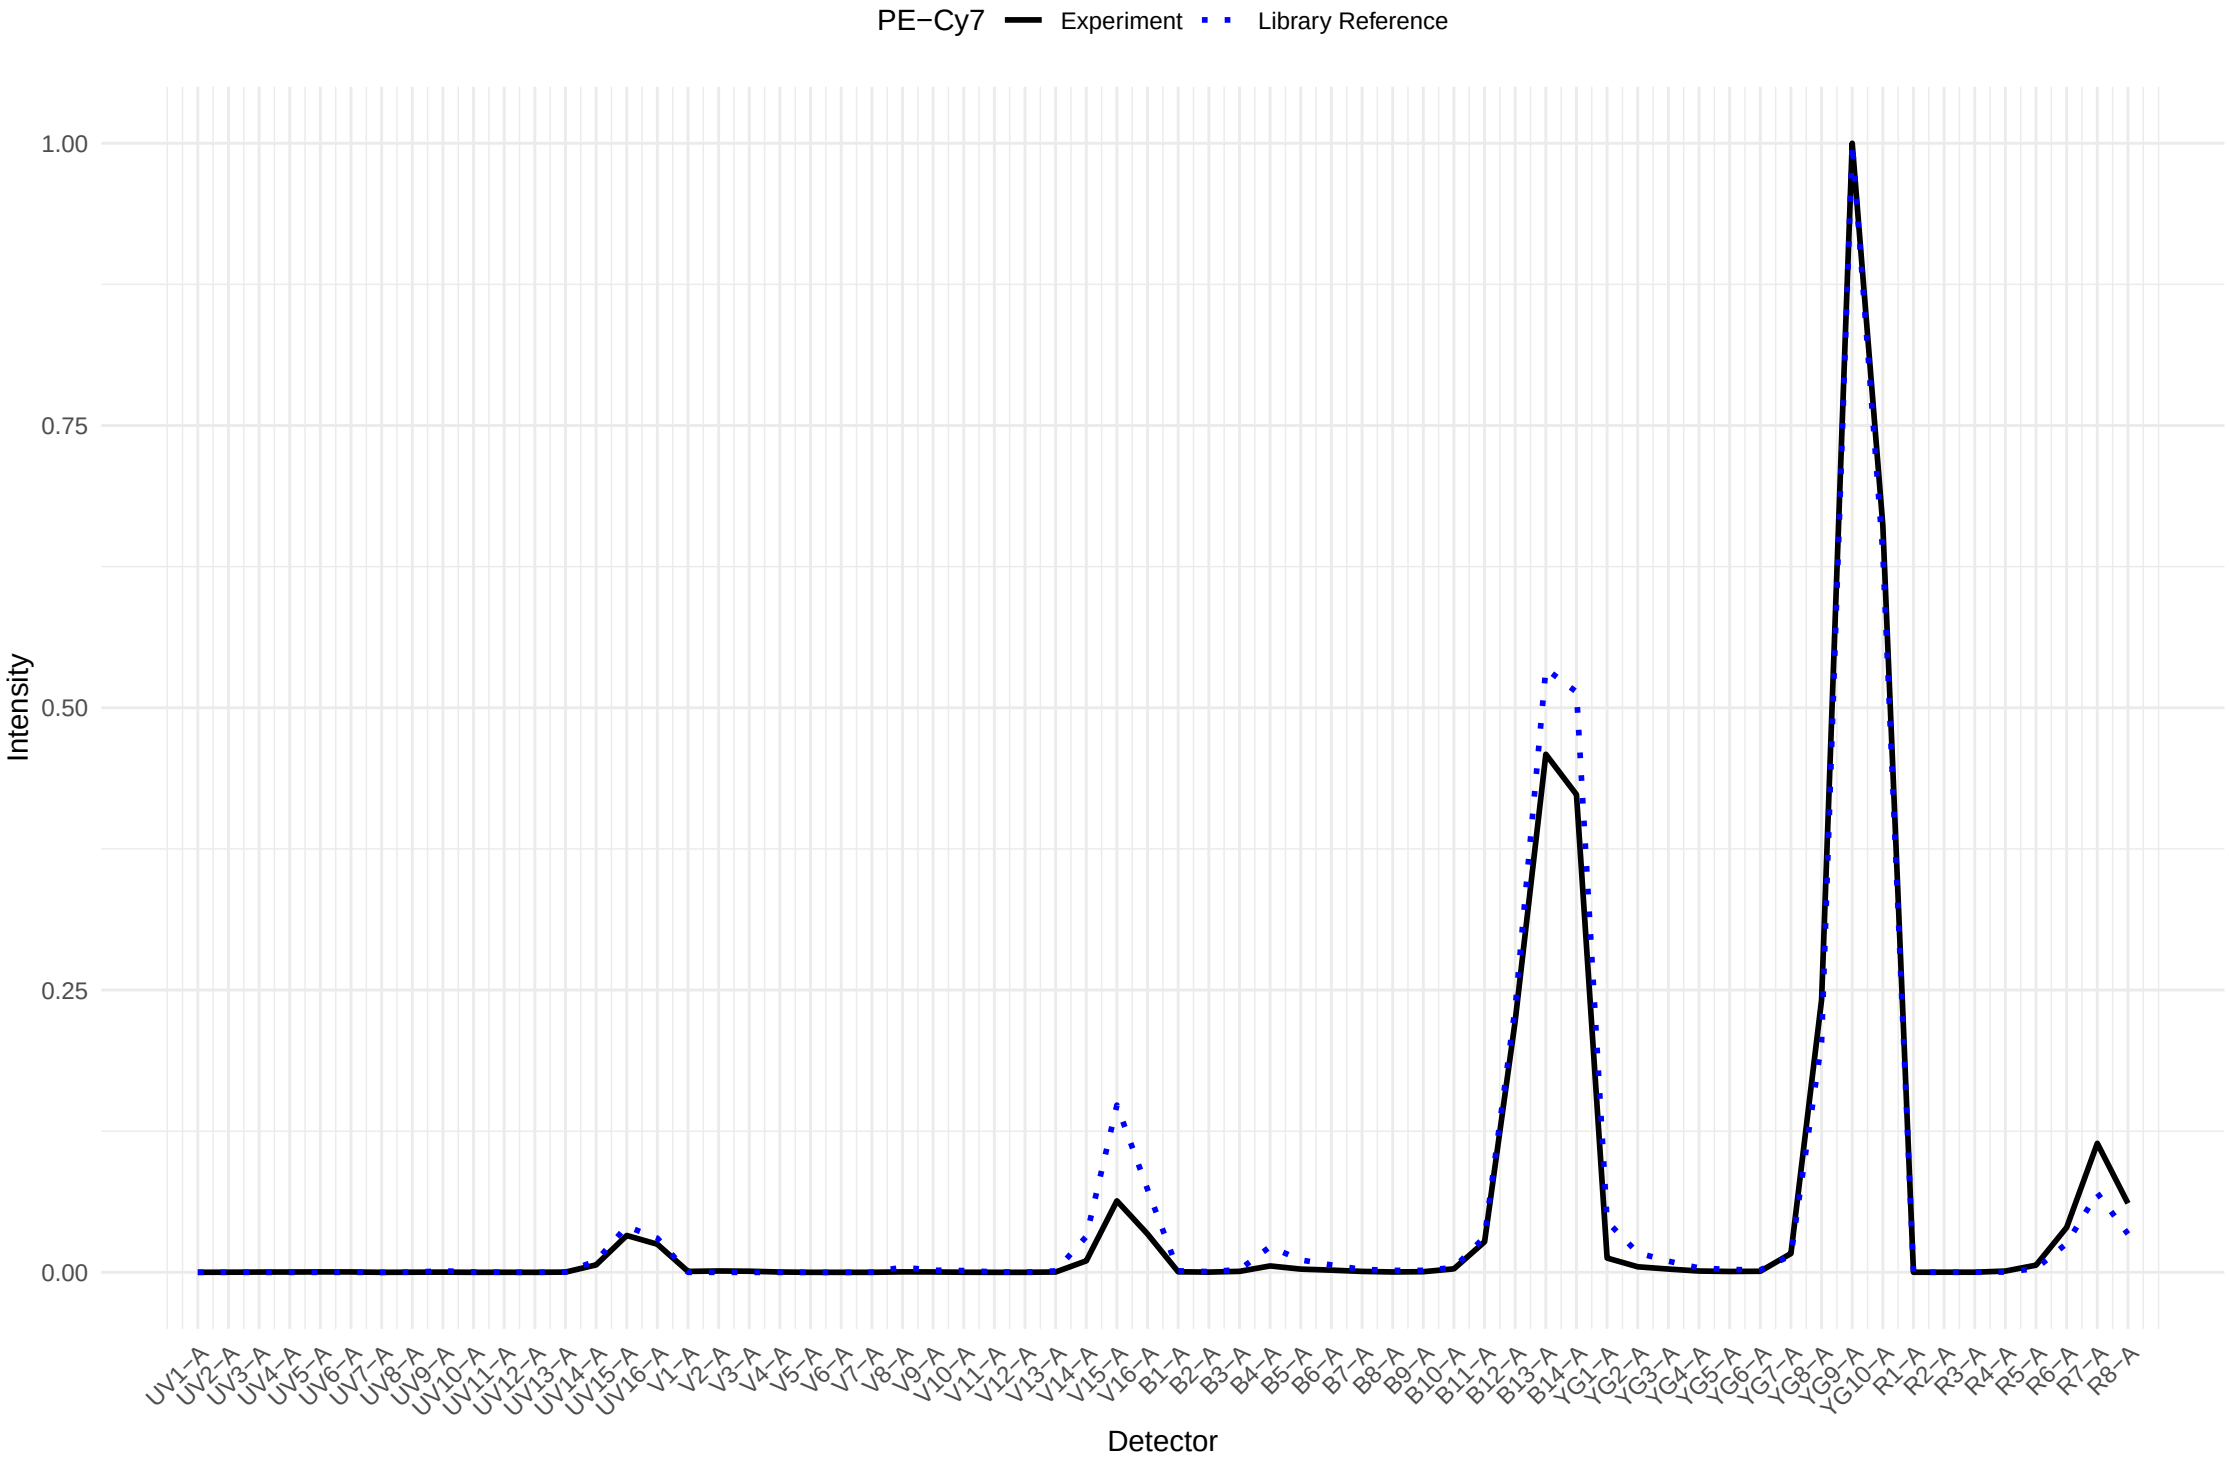

APC

Cosine Similarity: 0.9847

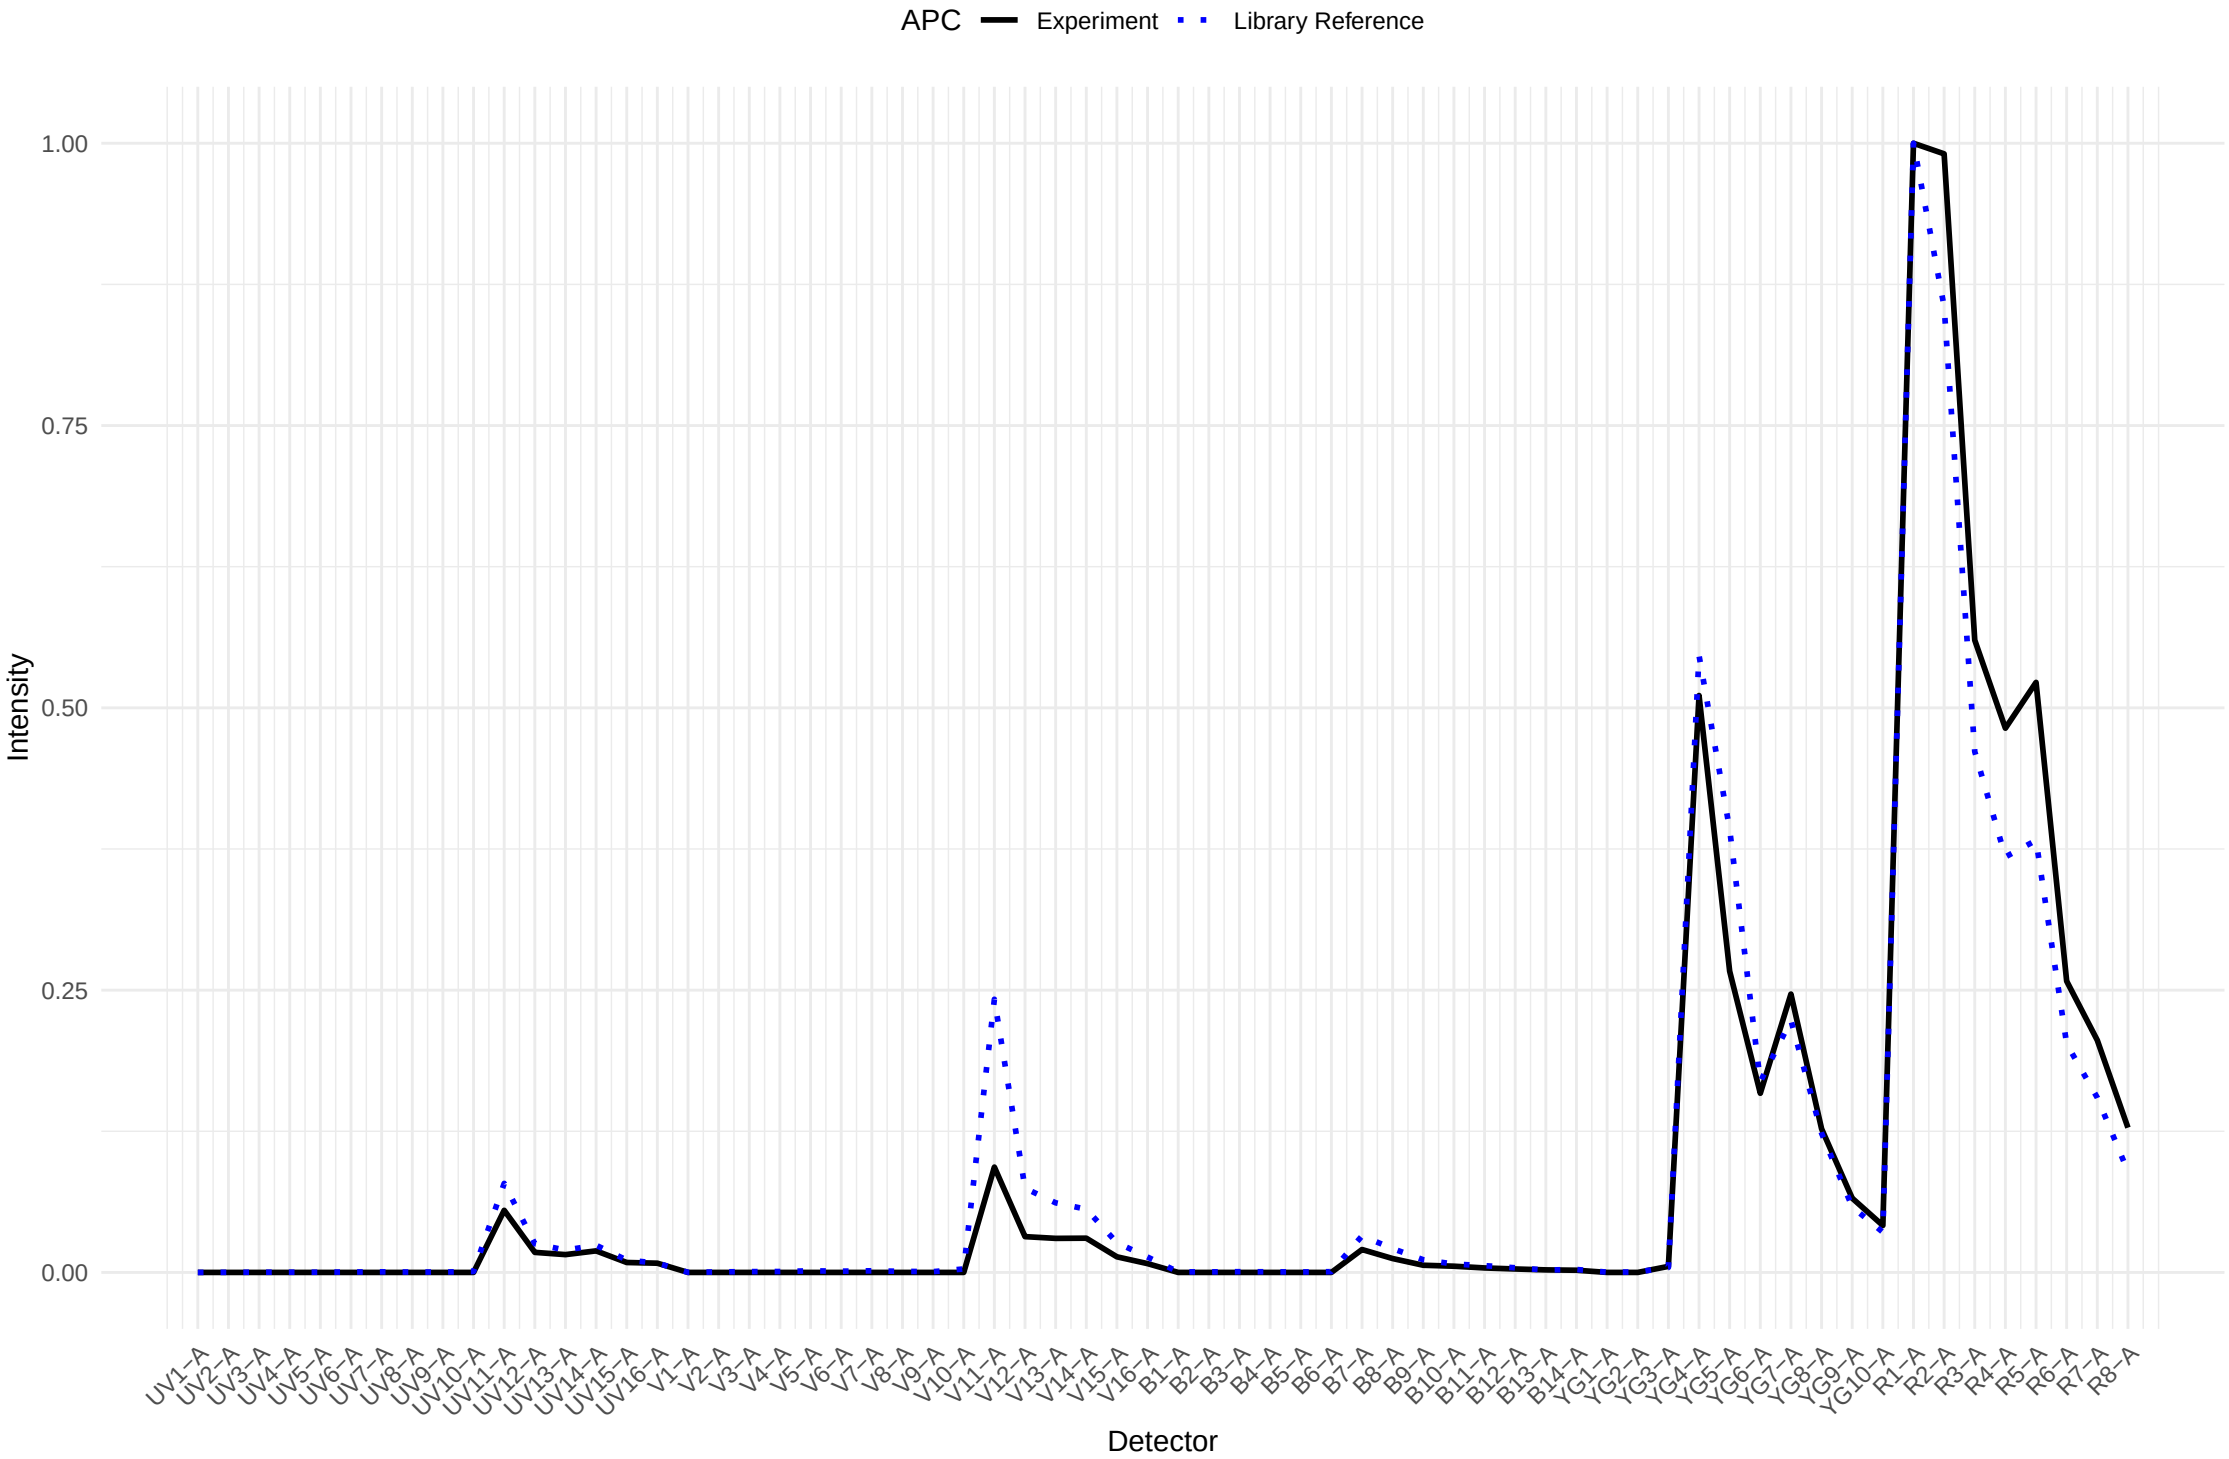

APC−H7

Cosine Similarity: 0.9957

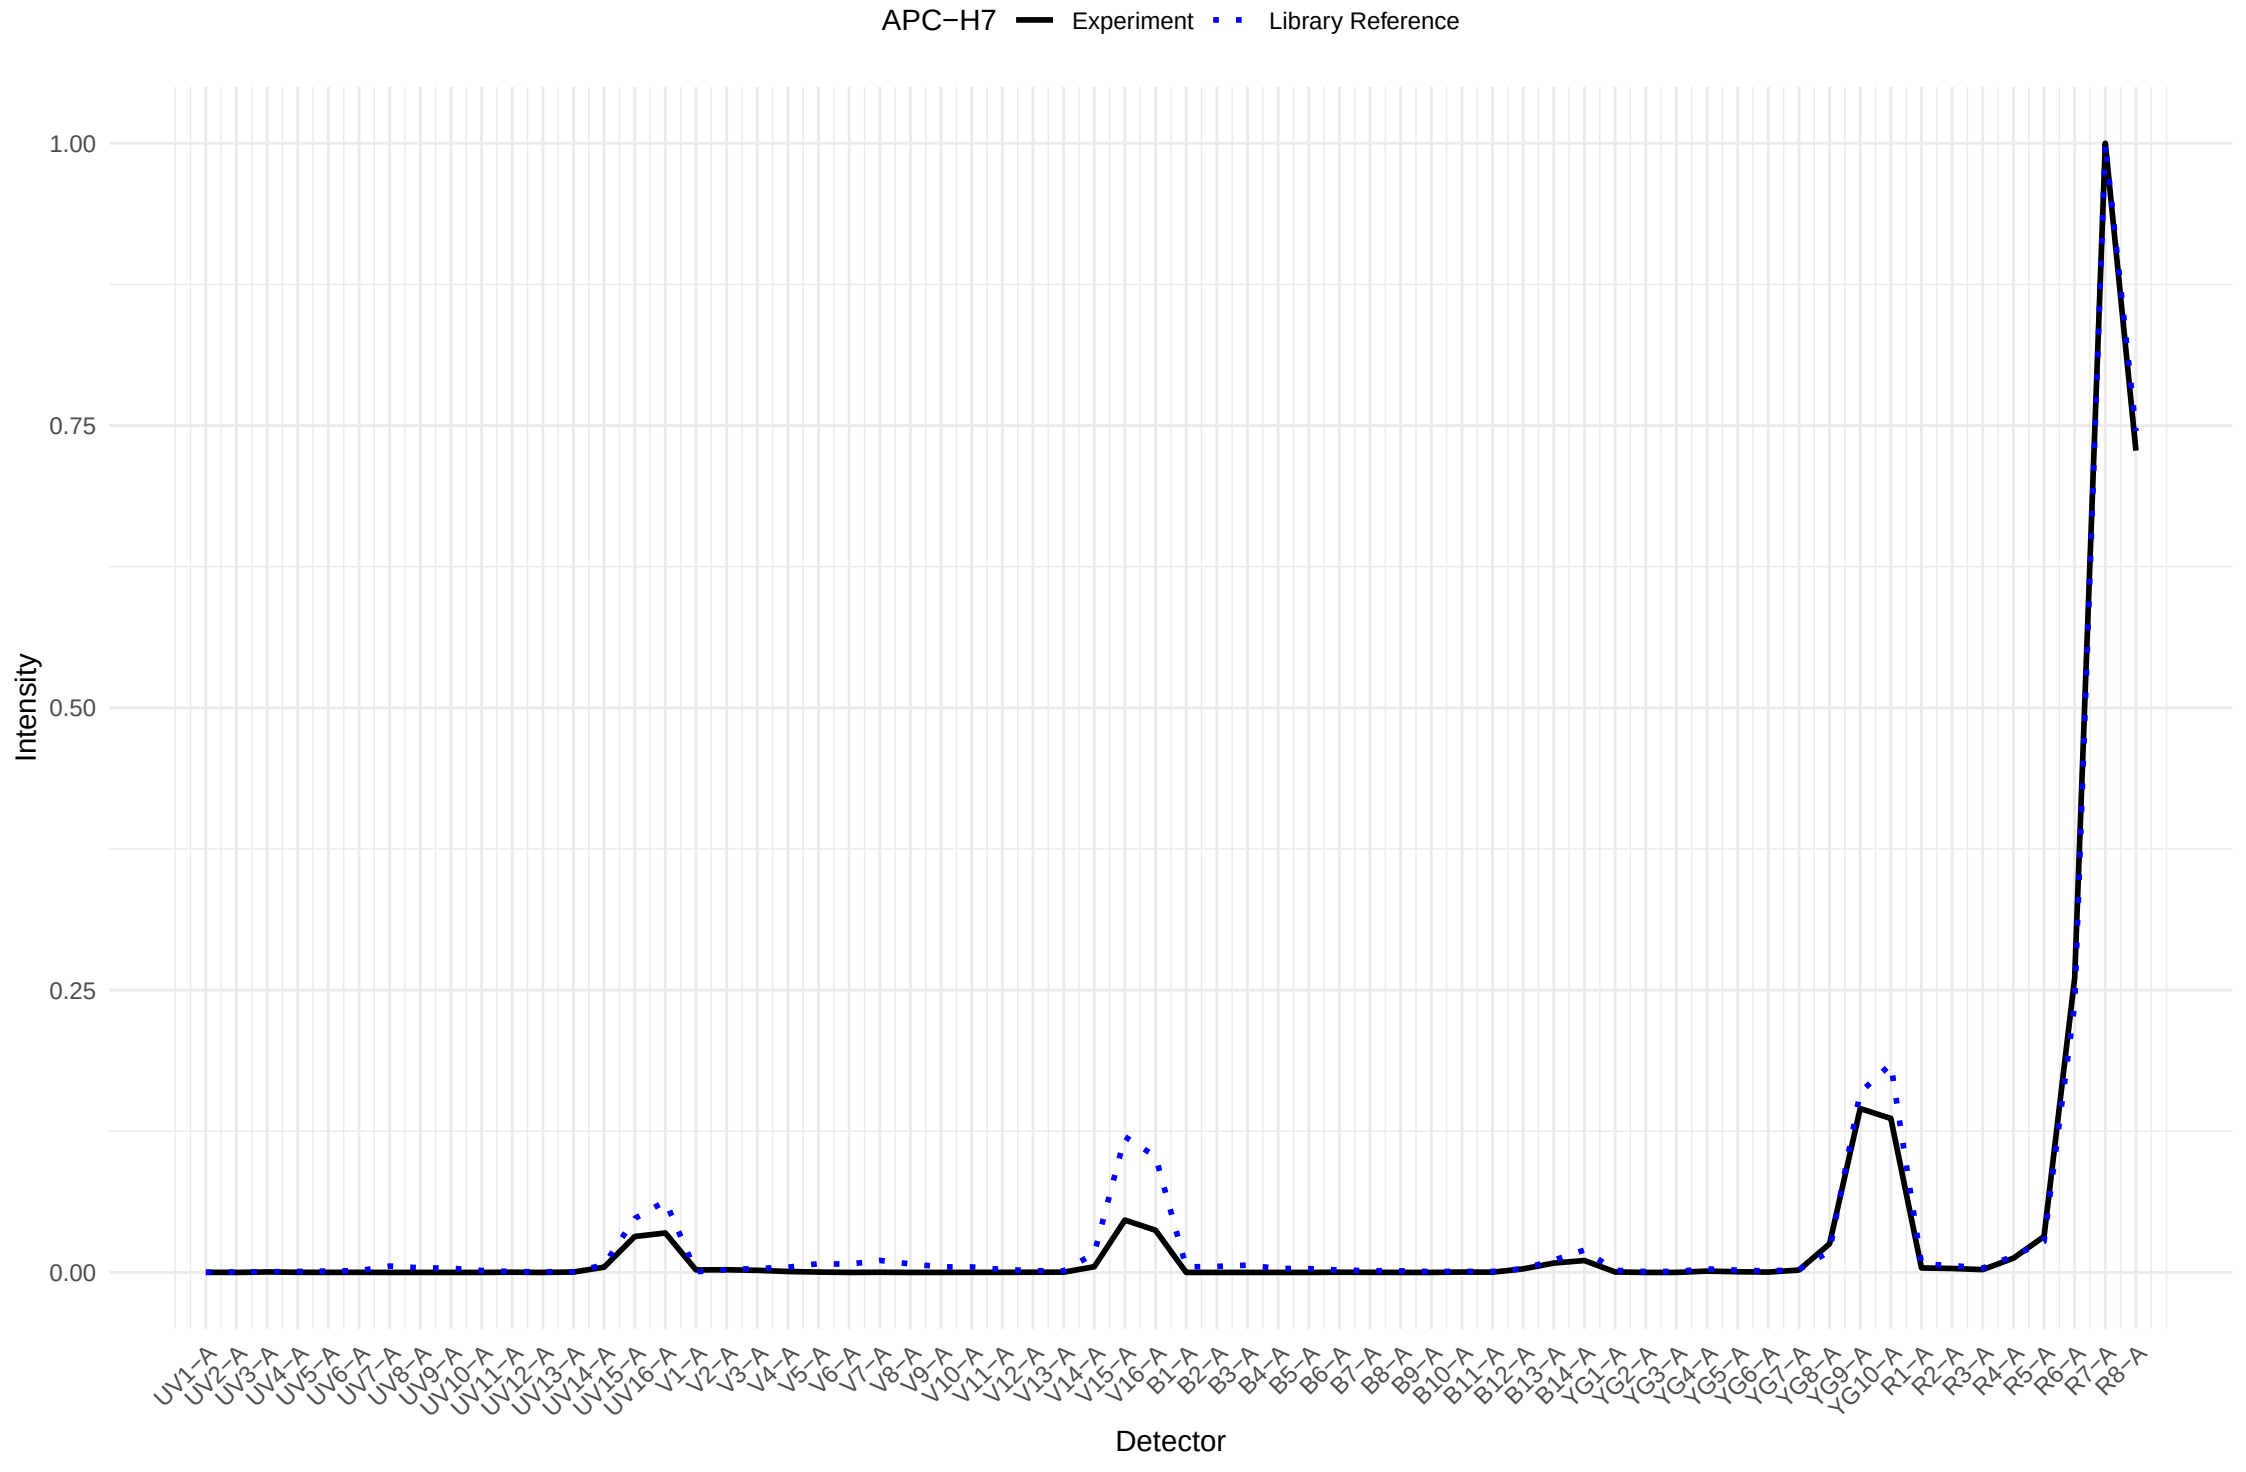

Helix NP Blue

No Reference Available

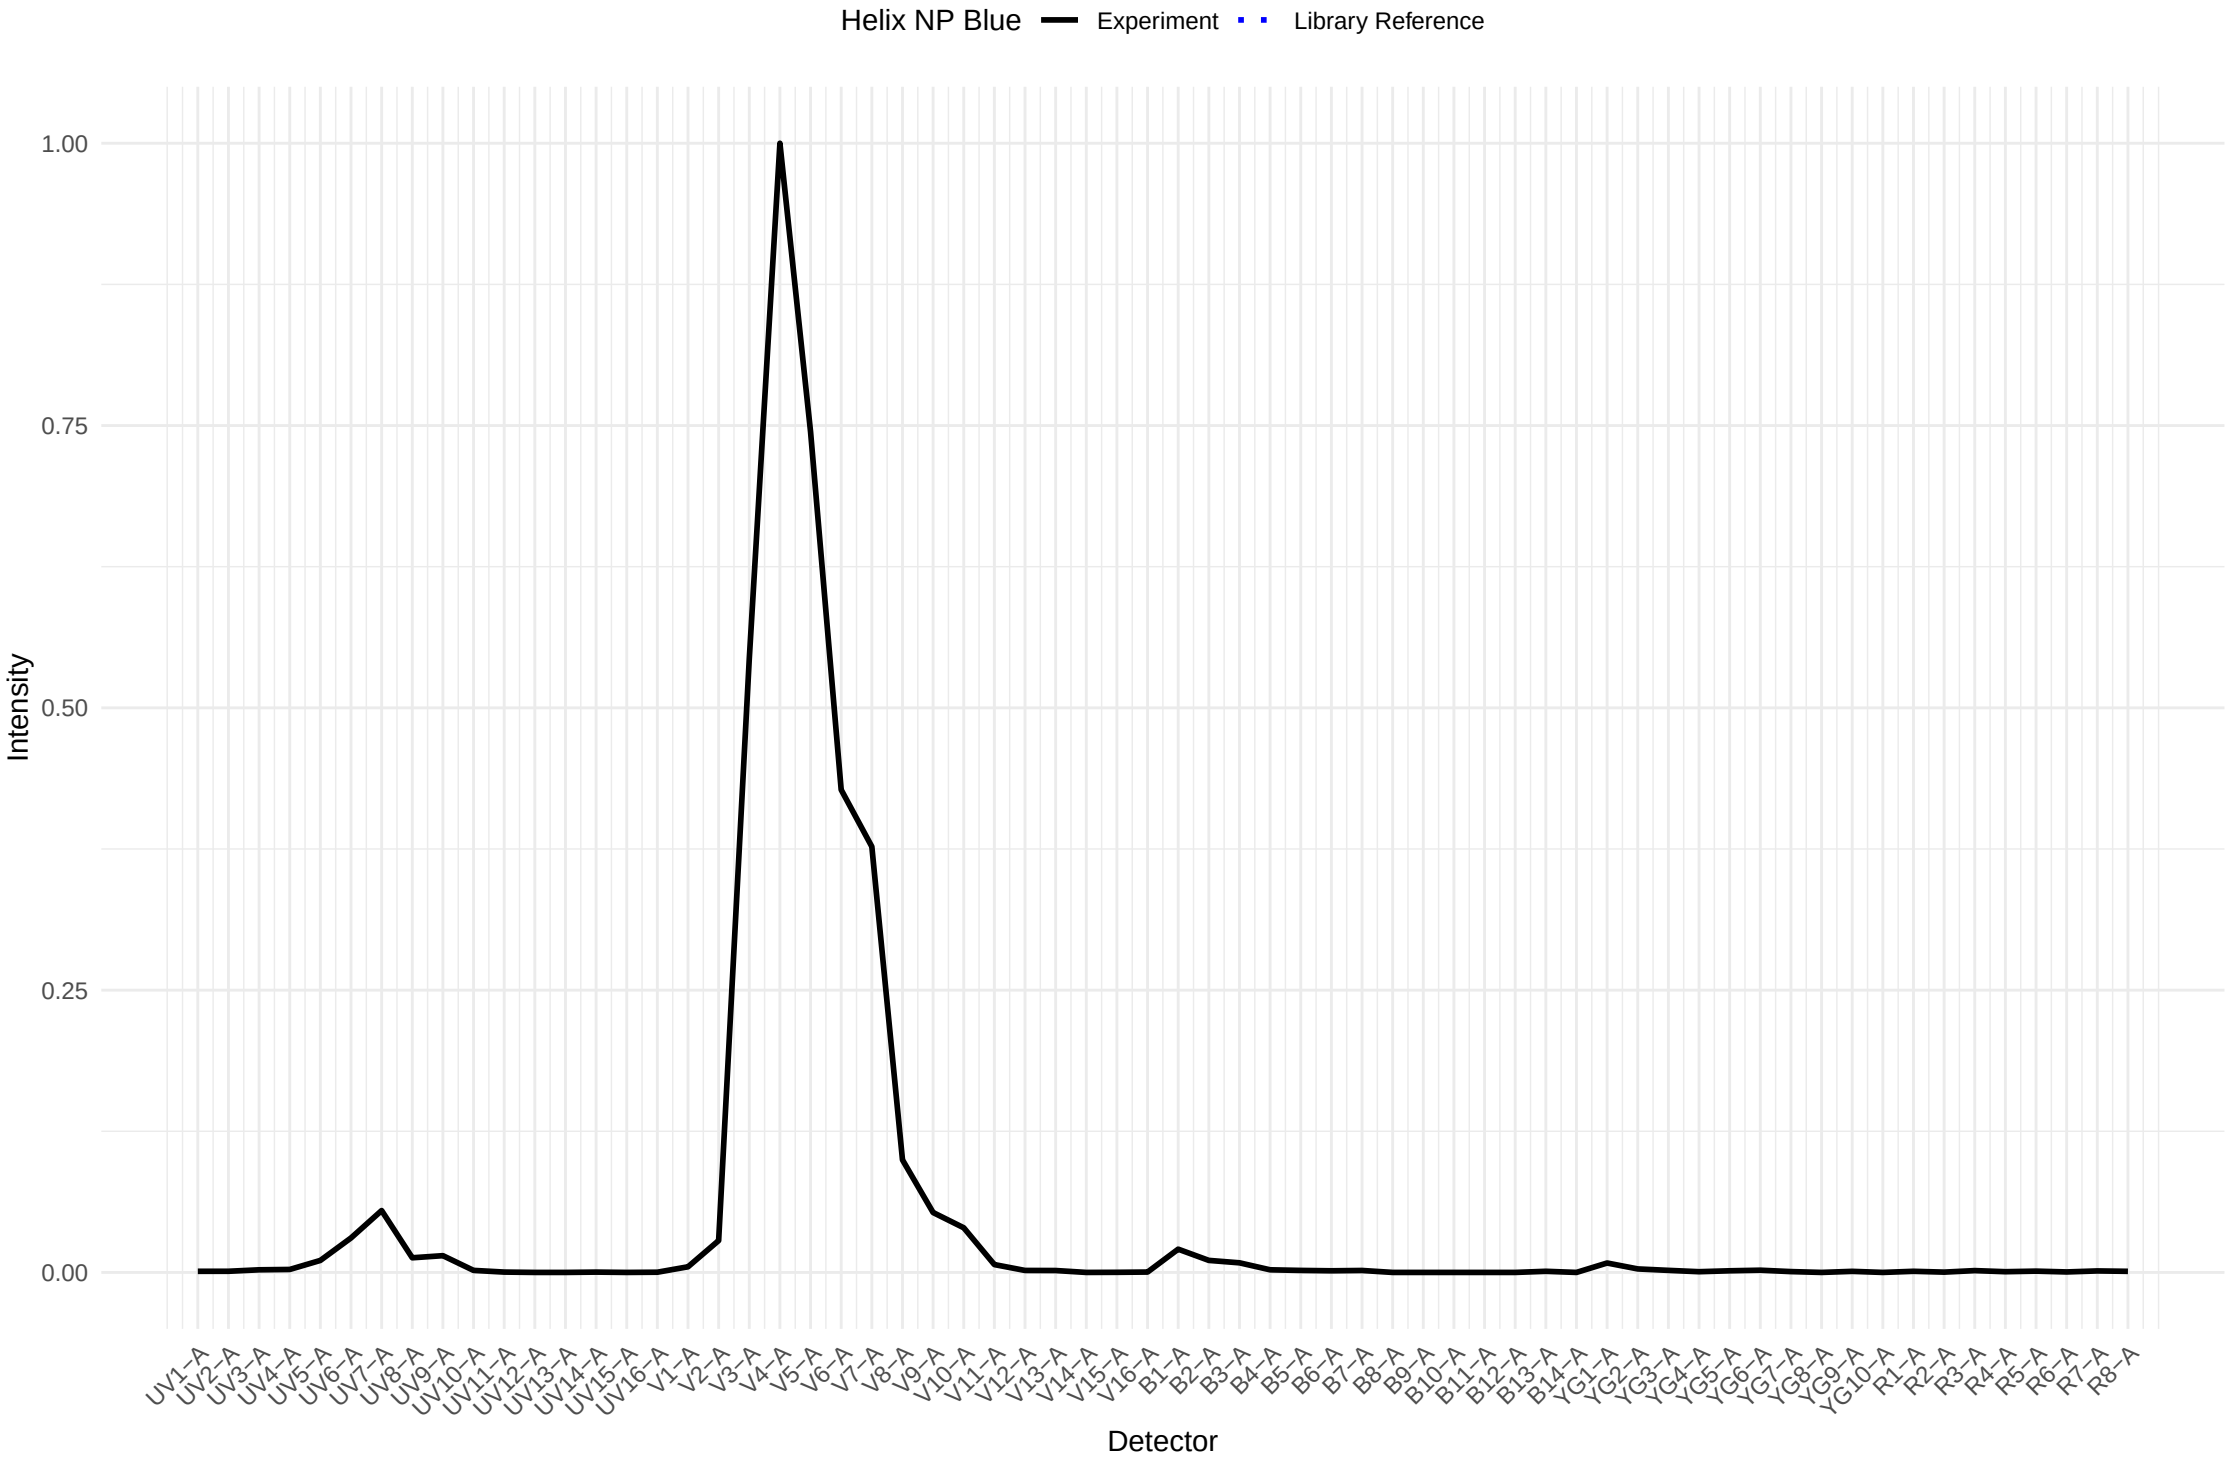

Live Dead Nir (876)
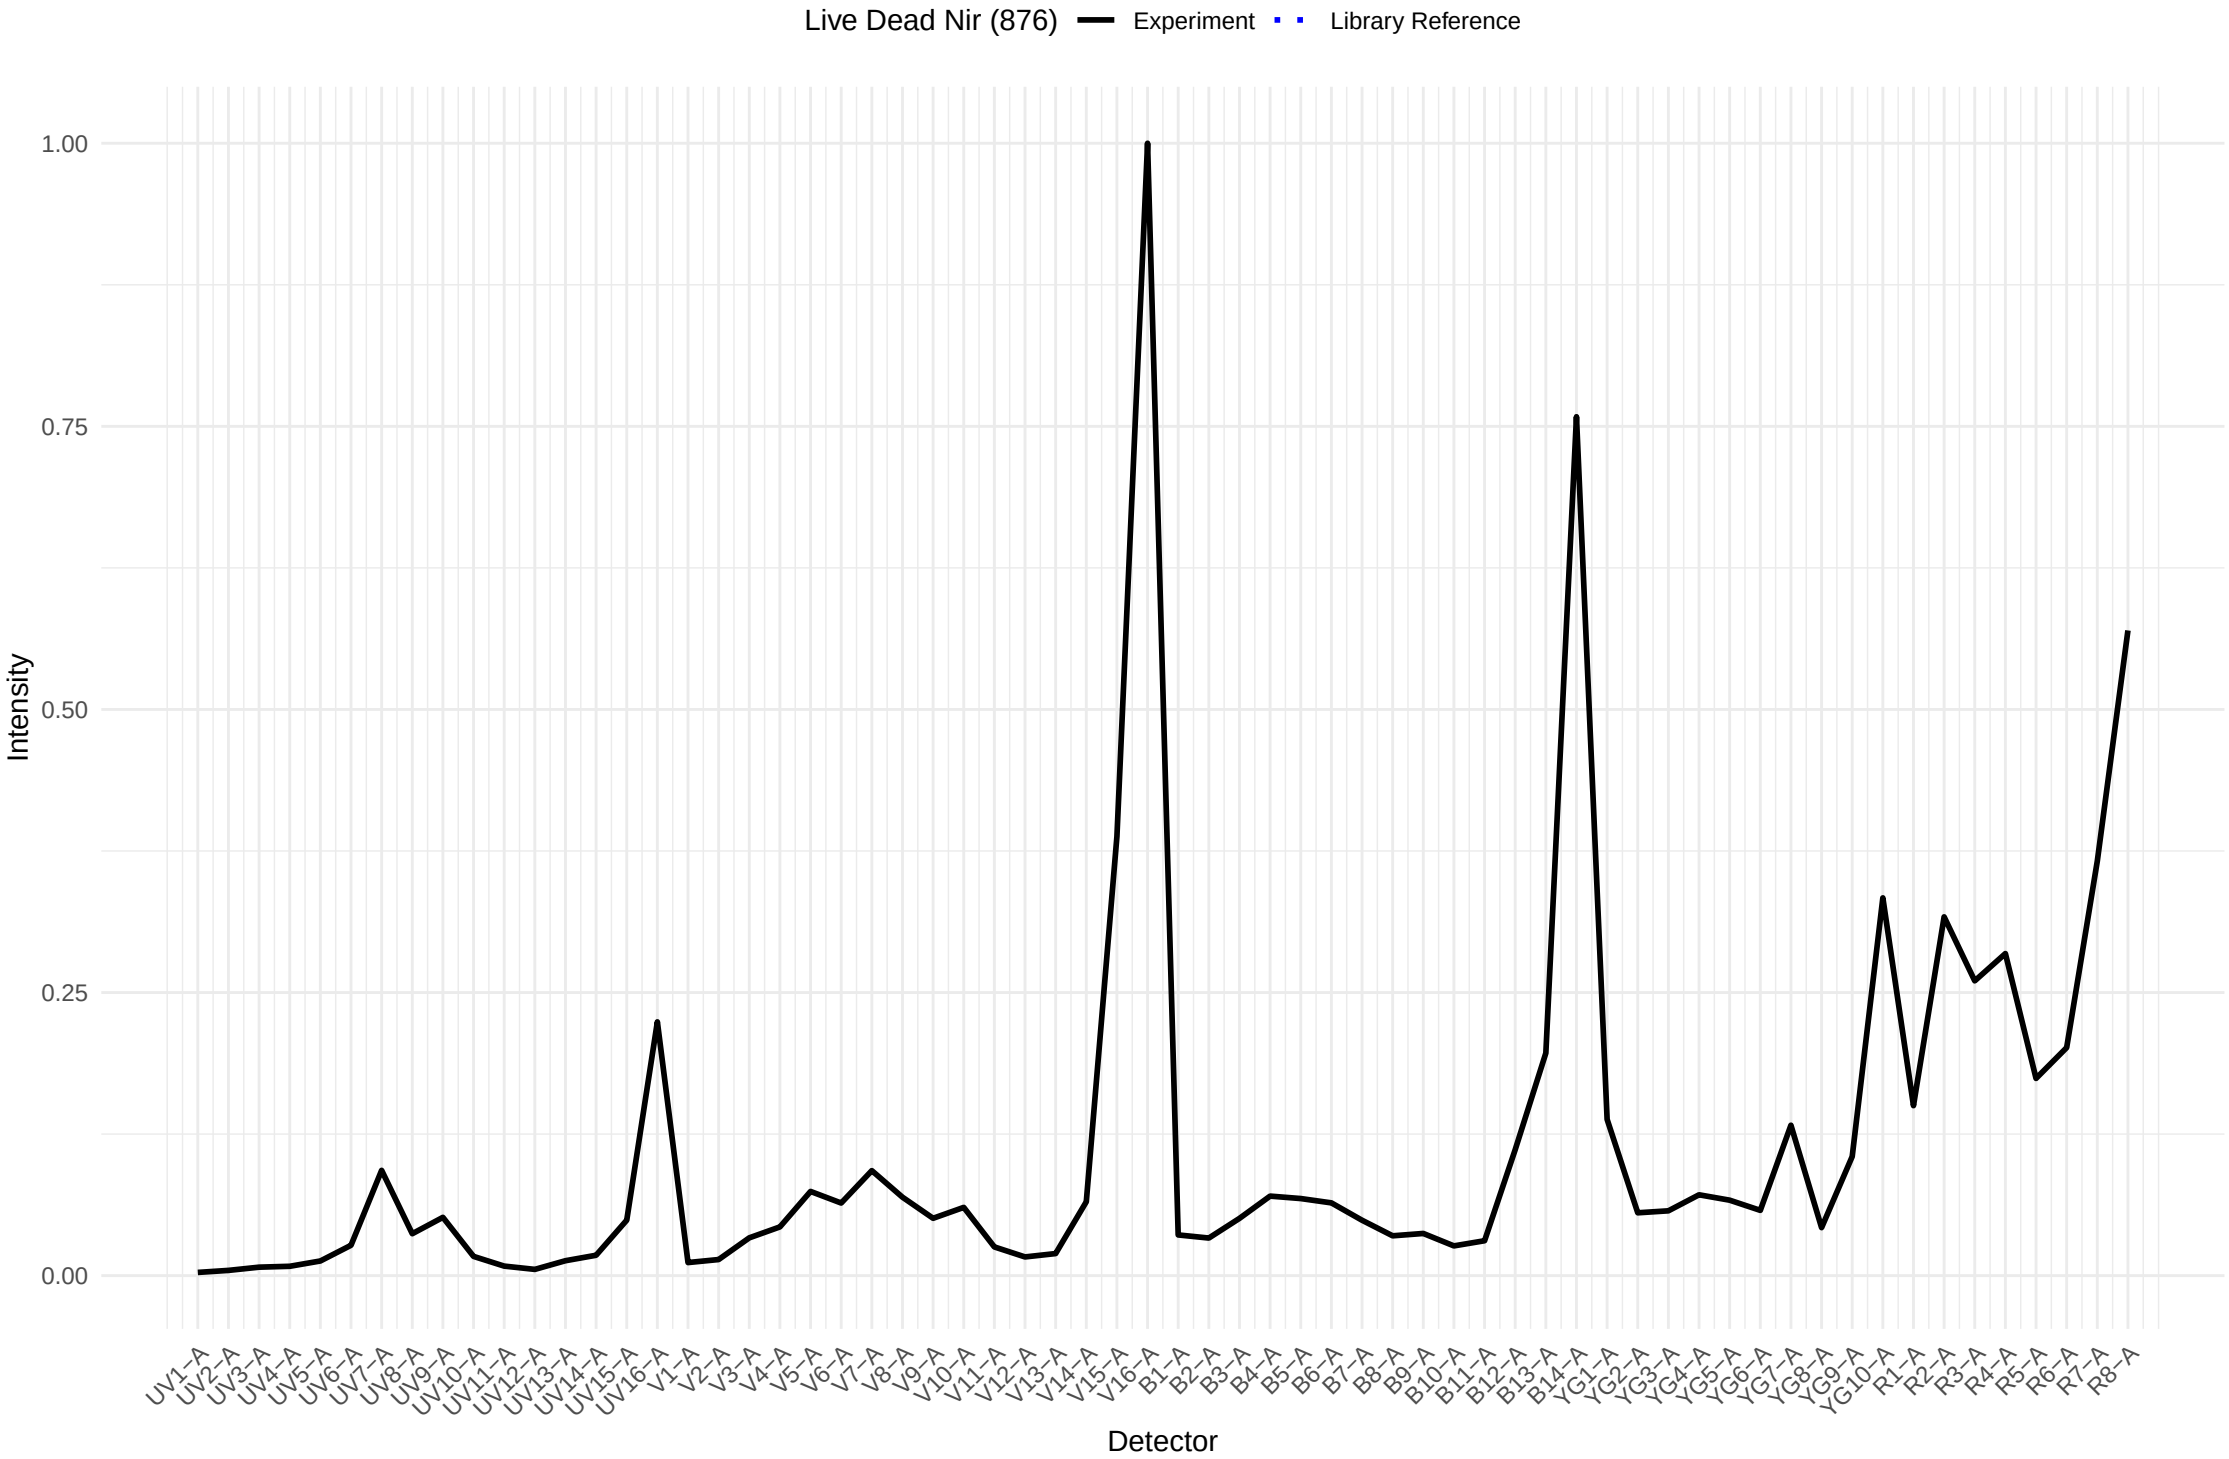
No Reference Available