Spectral QC Summary Report

This QC report is for guidance only. Spectra are expected to vary somewhat by instrument and protocol; minor deviations from library references are normal.

Fluorophore	Similarity	Status
BV711	0.9372	WARNING

BV711
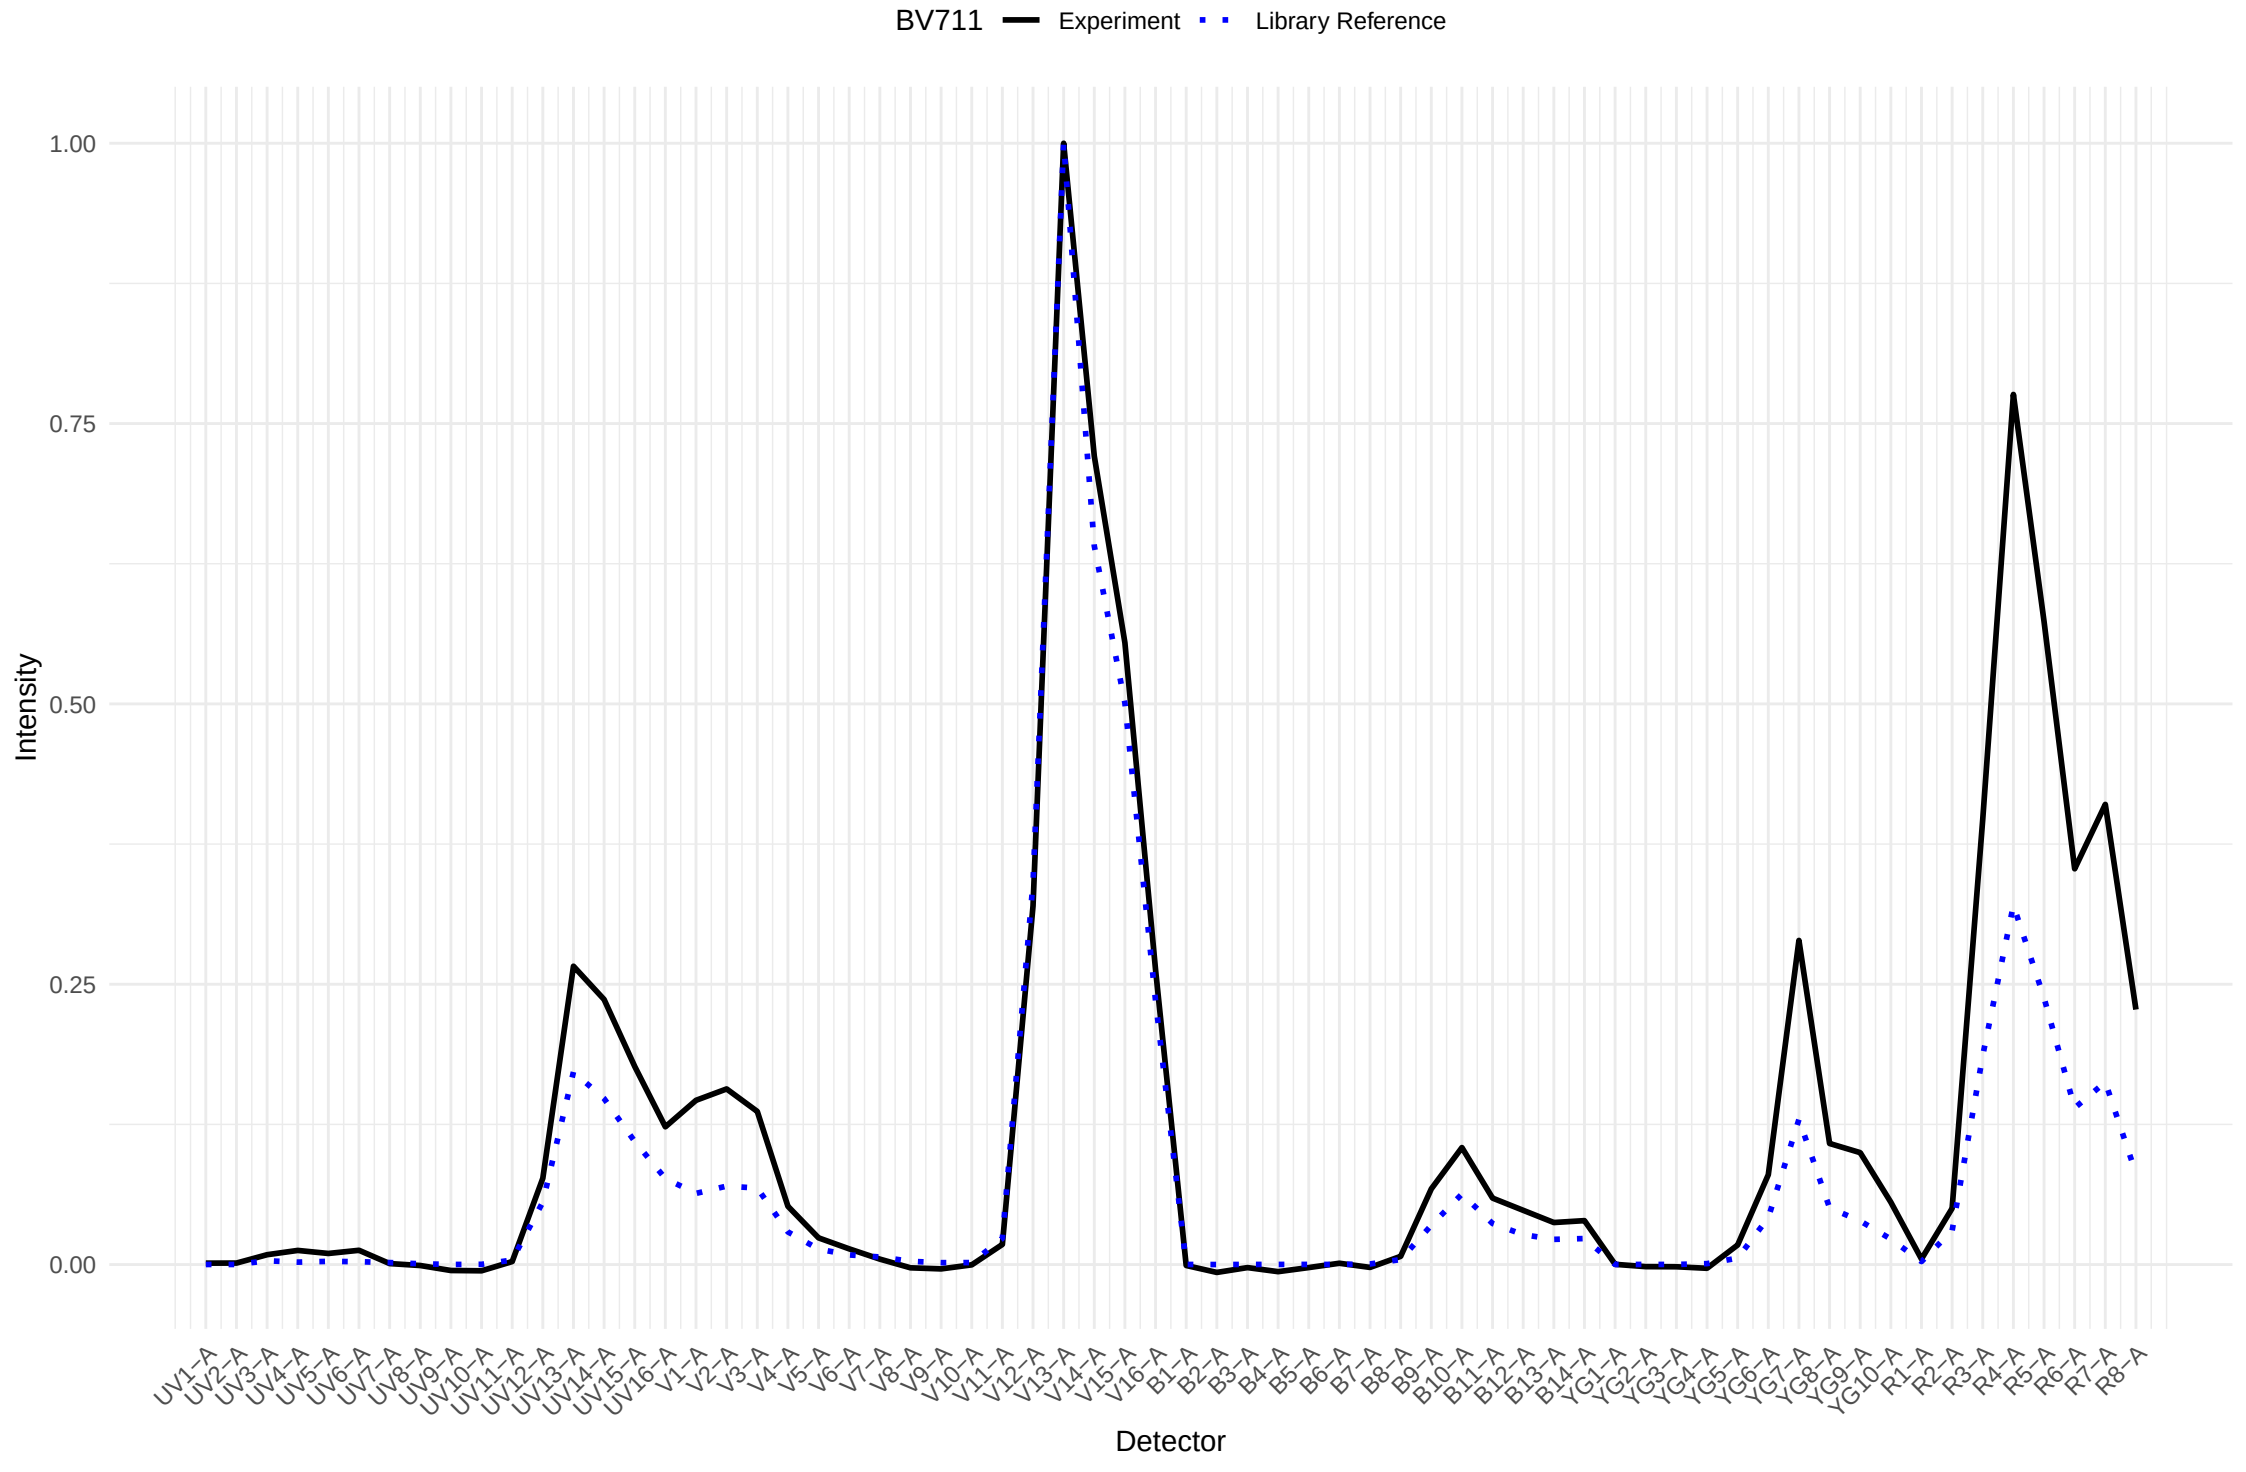
Cosine Similarity: 0.9372