



Vacuum Box Coater Model: BC-300



Hind High Vacuum Co. Pvt. Ltd.

Site No.17, Phase 1, Peenya Industrial Area. Bangalore-560 058, India

Phone.: 080 41931000 Fax.: 080-28394874

Email – info@hhv.in

website: www.hhv.in

OA. NO.: 10392..... WO. NO.: STD-312

CUSTOMER: NATIONAL INSTITUTE OF SCIENCE EDUCATION & RESEARCH

SYSTEM: VACUUM BOX COATER MODEL: BC-300

Page 1

Front View of the System




1. Chamber View Ports
2. Source Shutter Operating Knob
3. Gas Needle Valve
4. Electrical Control Console
5. High Vacuum Valve
6. Air Admittance Valve
7. LT Selector Switches
8. Combinational Valve

View of Control Console



1. Analog Penning Gauge
2. Analog Pirani Gauge
3. HT/LT Control Pot
4. Control Switches
5. HT Primary Current Meter
6. LT Secondary Current Meter
7. Mains Indication
8. HT/LT Circuit Breakers

View of Electrical Console

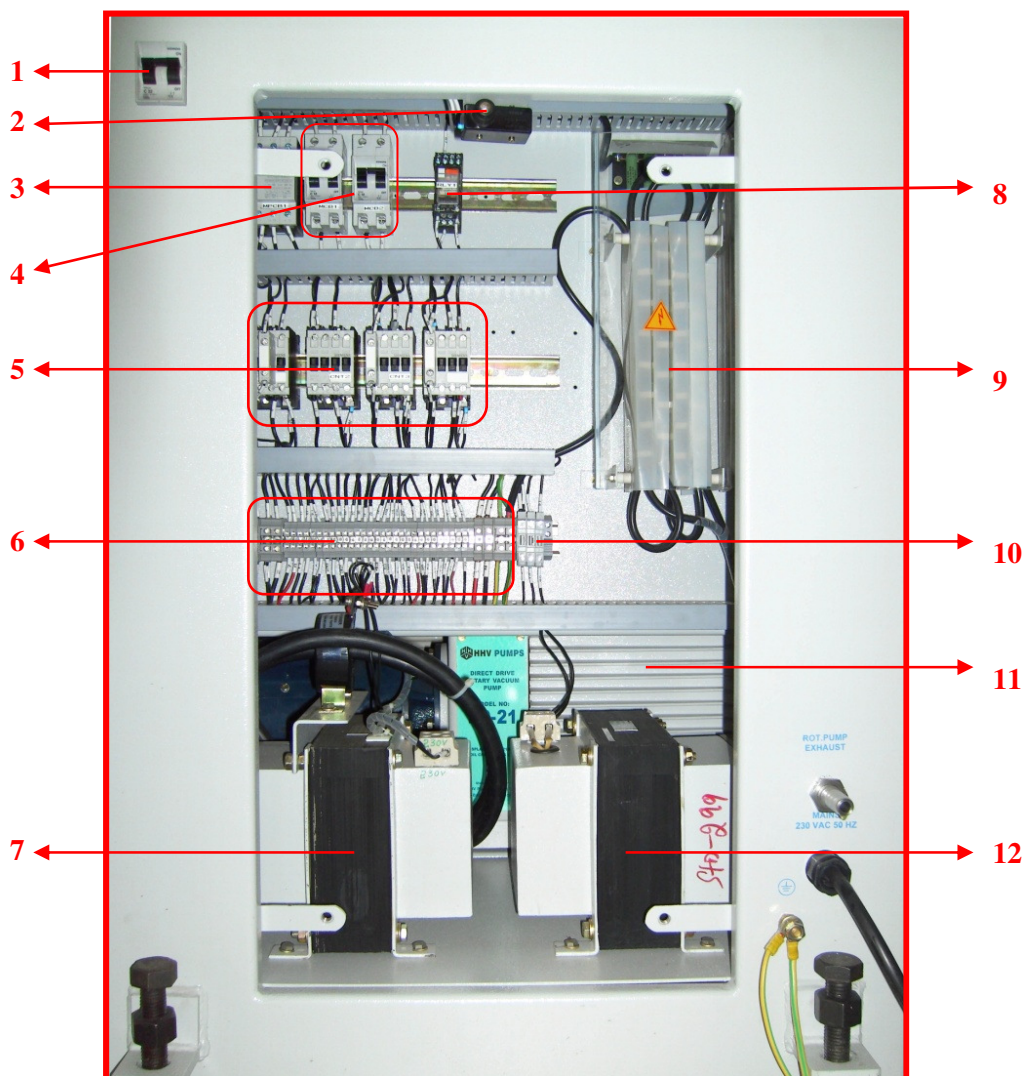


1. Mains Supply Circuit Breaker
2. Door Switch
3. MPCB For Rotary Pump
4. MCB's
5. Contactor's
6. CST's
7. LT Transformer
8. Interlock Relay
9. HT Board
10. Fuse Links
11. Rotary Vacuum Pump
12. HT Transformer

OA. NO.: 10392..... WO. NO.: STD-312

CUSTOMER: NATIONAL INSTITUTE OF SCIENCE EDUCATION & RESEARCH


SYSTEM: VACUUM BOX COATER MODEL: BC-300

Rear View of Control Console

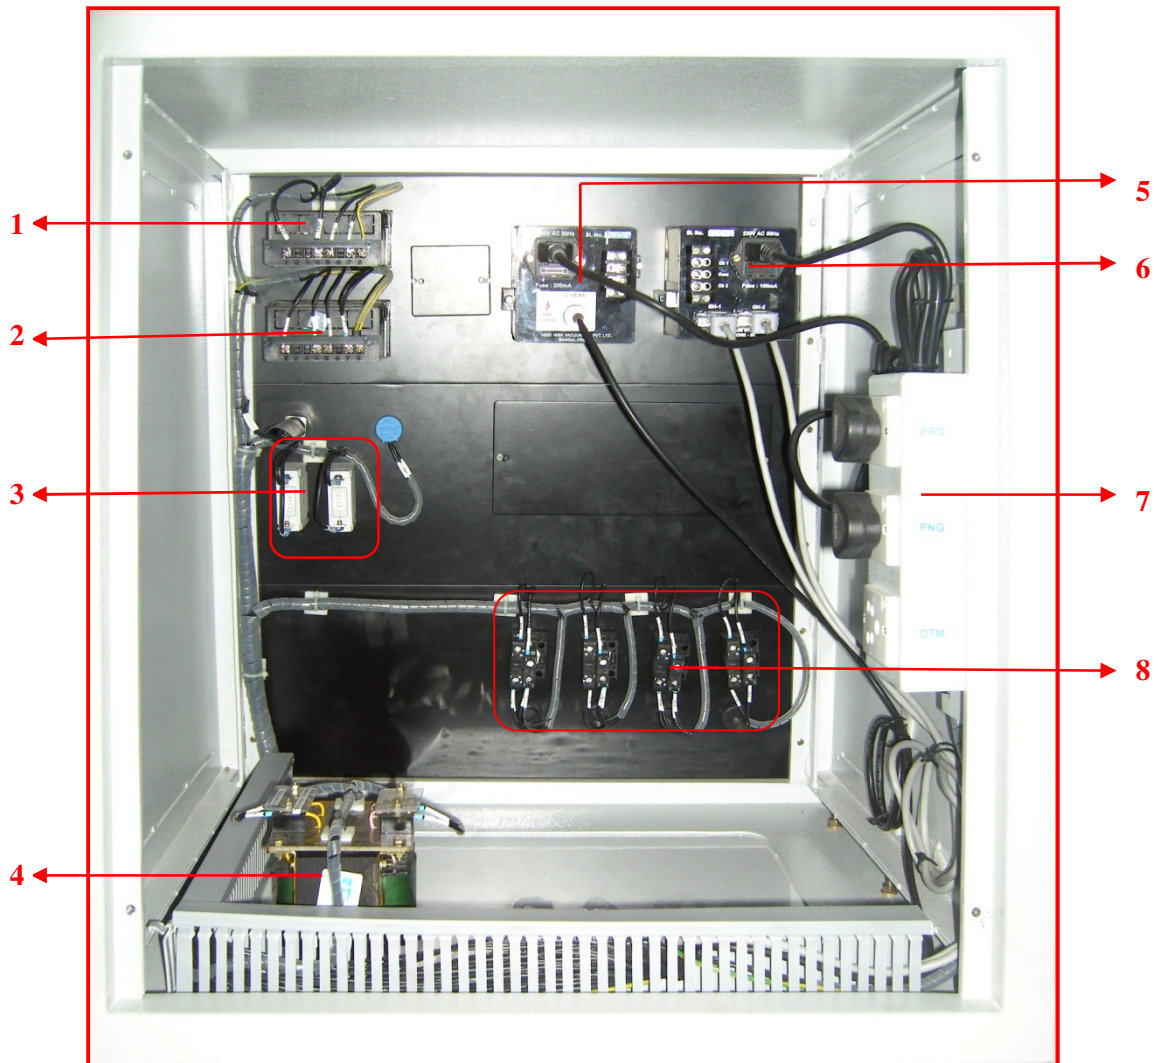

1. HT Primary Current Meter
2. LT Secondary Current Meter
3. HT/LT Circuit Breakers
4. Control Circuit Transformer
5. Analog Penning Gauge
6. Analog Pirani Gauge
7. Power Distribution Box
8. Control Switches

Rear View of Pumping System

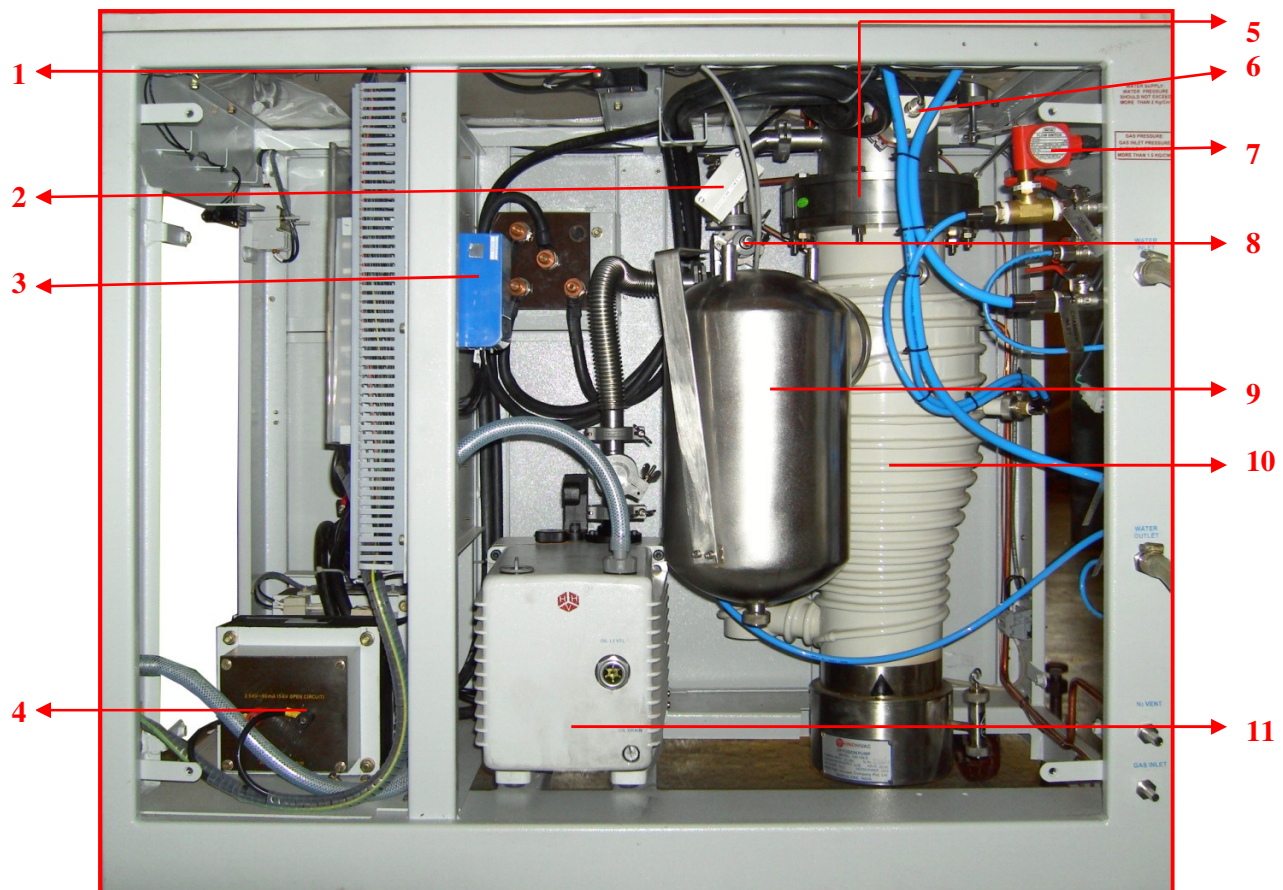

1. Door Switch
2. Vacuum Switch
3. Thyristor Controller
4. HT Transformer
5. High Vacuum Valve
6. Penning Gauge Head
7. Water Flow Switch
8. Pirani Gauge Head
9. Cryo Trap
10. Oil Diffusion Pump
11. Rotary Vacuum Pump


OA. NO.: 10392..... WO. NO.: STD-312

CUSTOMER: NATIONAL INSTITUTE OF SCIENCE EDUCATION & RESEARCH

SYSTEM: VACUUM BOX COATER MODEL: BC-300


Page 6

Side View of Pumping System

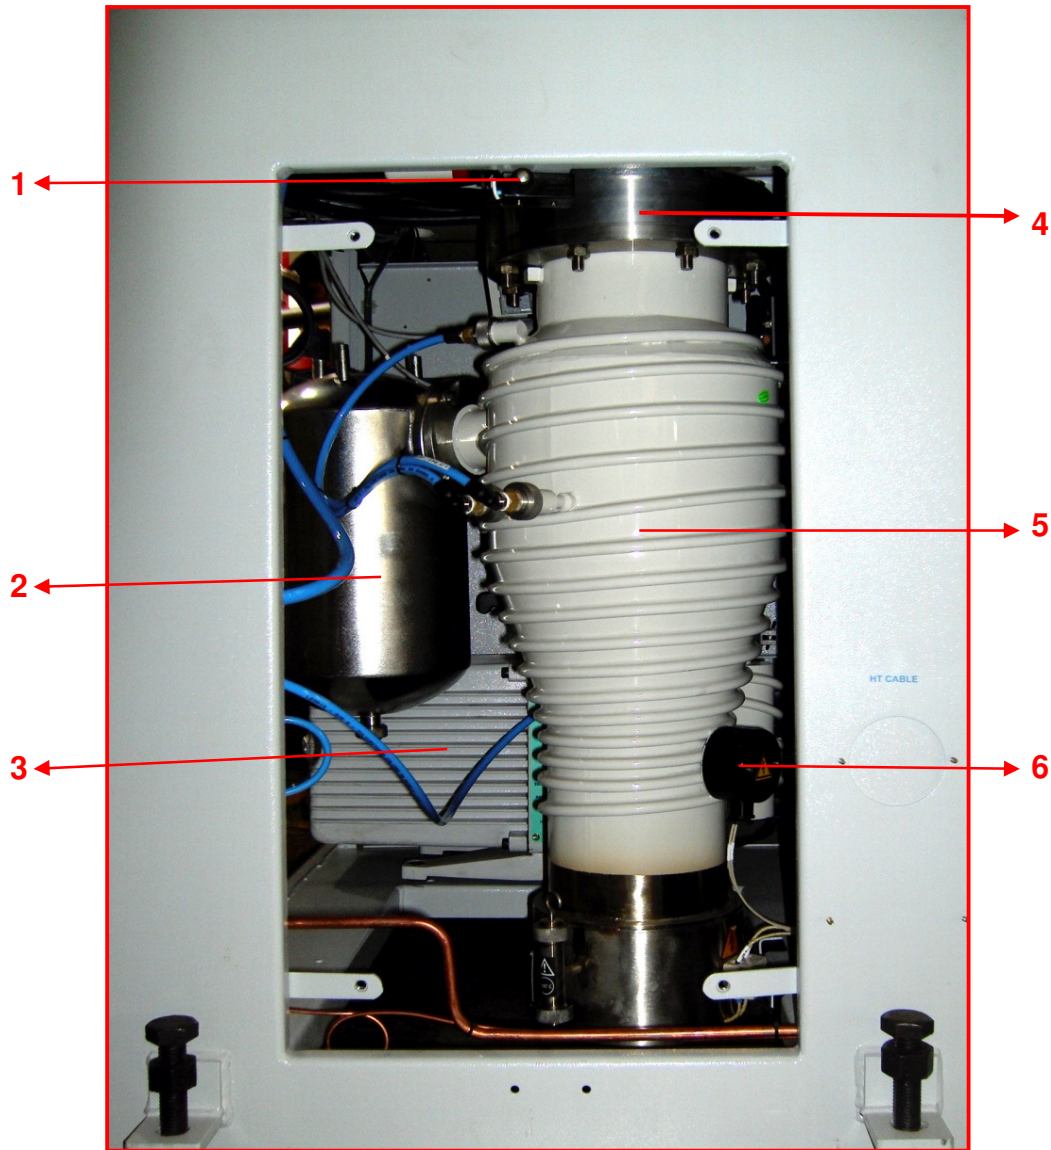

1. Door Switch
2. Cryo Trap
3. Rotary Vacuum Pump
4. High Vacuum Valve
5. Oil Diffusion Pump
6. Thermostat

Base Plate Configuration

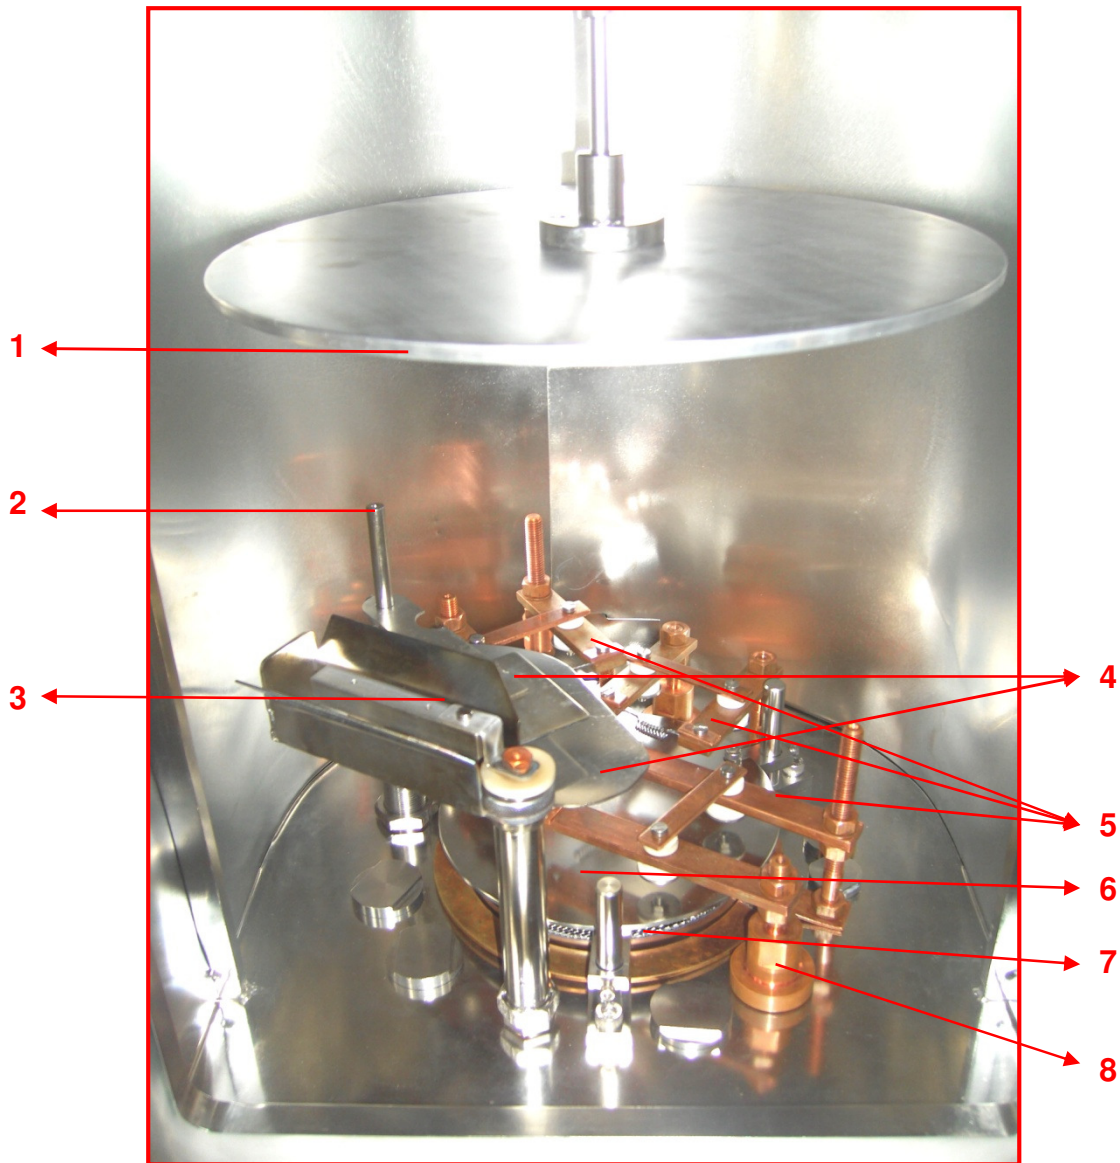

1. Circular Work Holder
2. Source Shutter Shaft Seal
3. HT Ion Bombardment Gadgetry
4. Source Shutter Plates
5. LT Filament Holders
6. Baffle Plate
7. Filter Mesh
8. LT Live Electrode

OA. NO.: 10392..... WO. NO.: STD-312

CUSTOMER: NATIONAL INSTITUTE OF SCIENCE EDUCATION & RESEARCH

SYSTEM: VACUUM BOX COATER MODEL: BC-300

Page 8