


Full-dose overshoot motivated label-free D75 selection

Prospective calibration curve



Full-dose safety did not generalize across samples

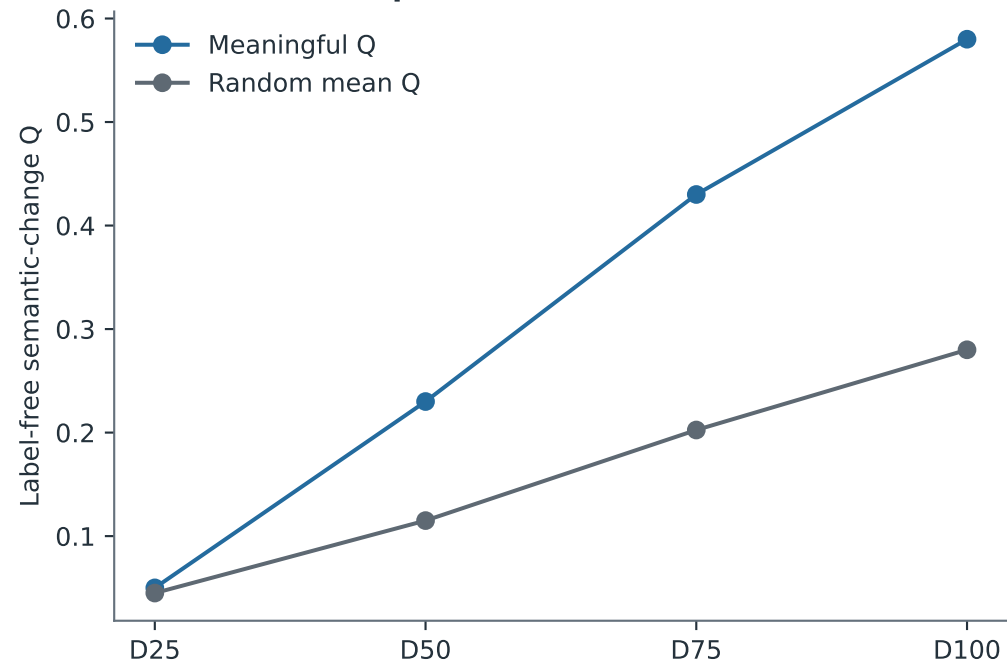