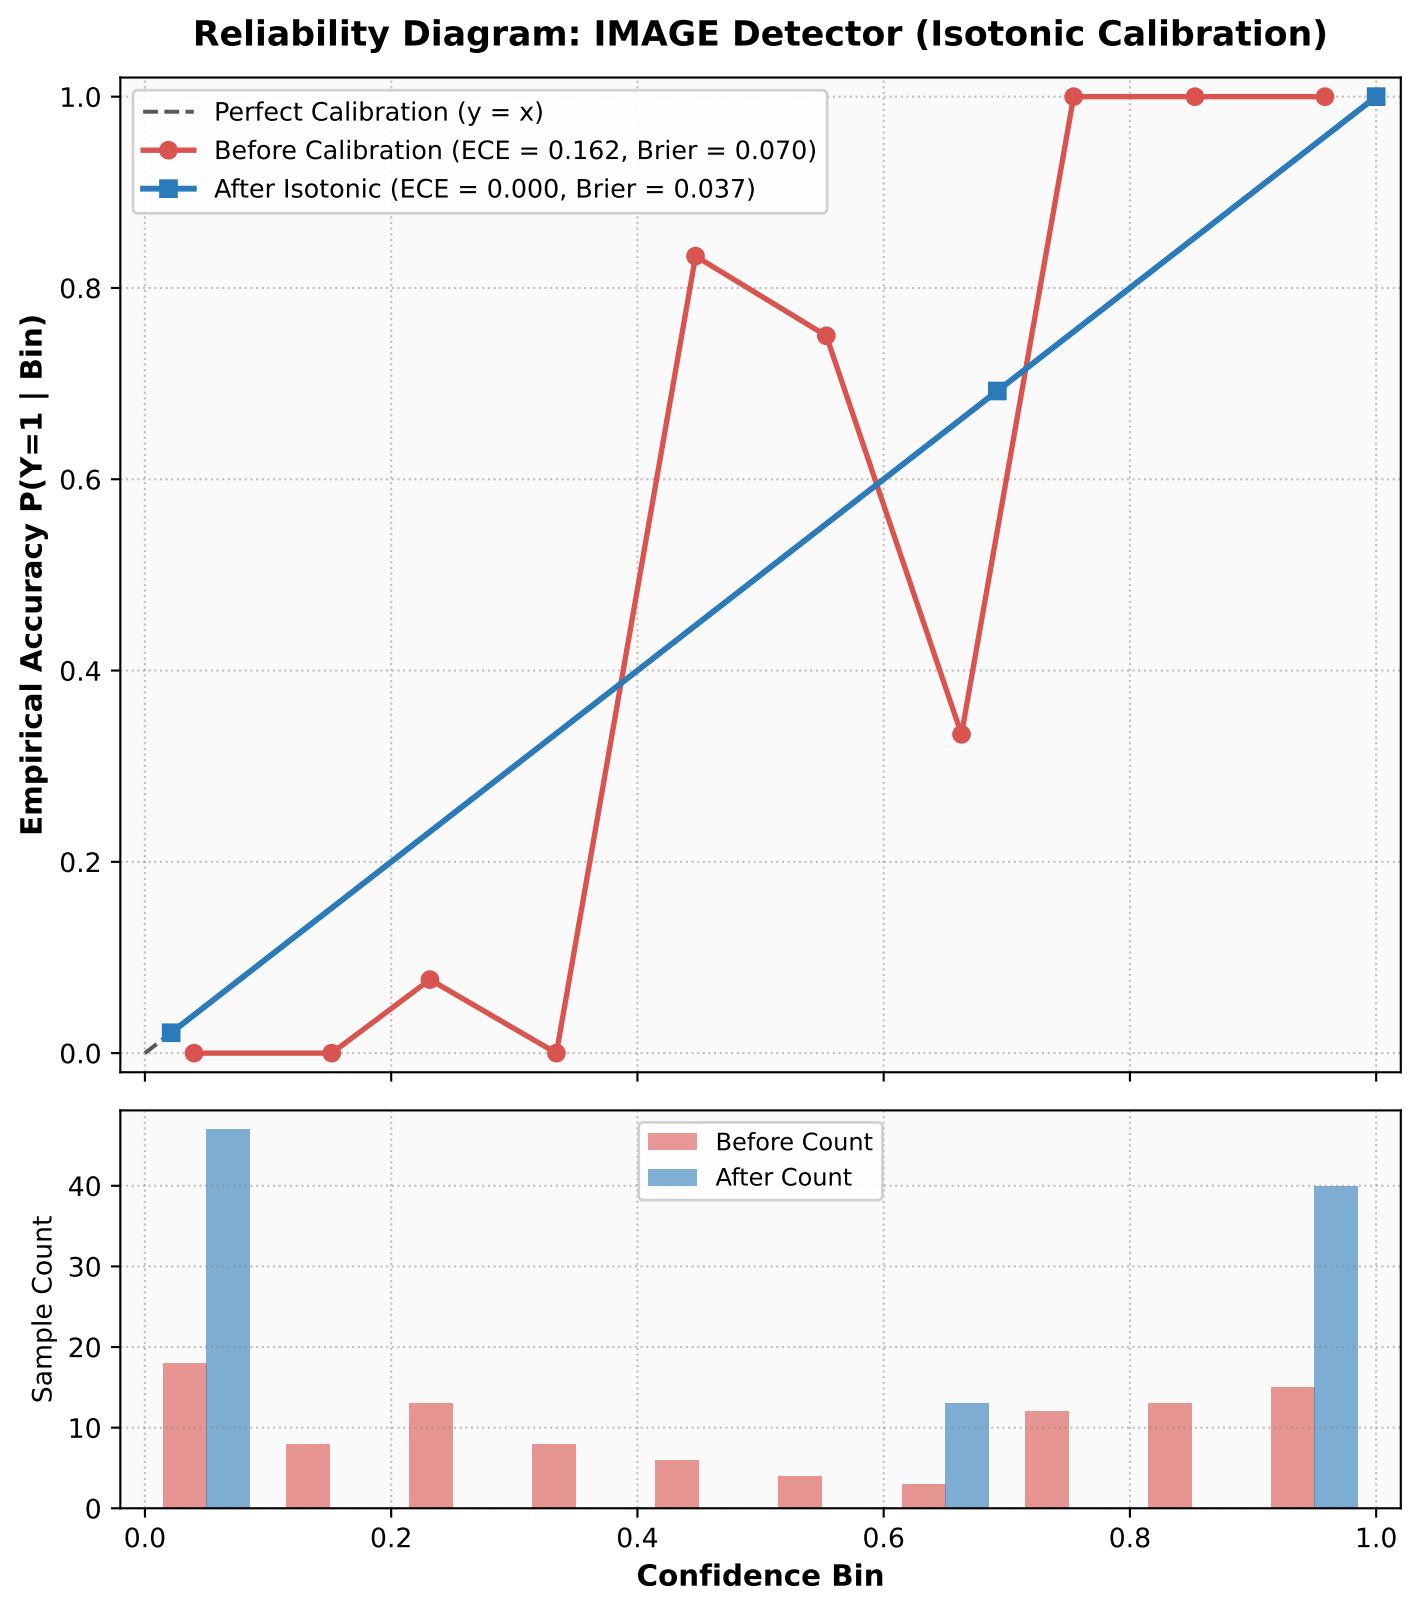
Reliability Diagram: IMAGE Detector (Isotonic Calibration)
Perfect Calibration (y = x)
Before Calibration (ECE = 0.162, Brier = 0.070)
After Isotonic (ECE = 0.000, Brier = 0.037)
Empirical Accuracy P(Y=1 | Bin)
1.0
0.8
0.6
0.4
0.2
0.0
Before Count
After Count
Sample Count
40
30
20
10
0
0.0
0.2
0.4
0.6
0.8
1.0
Confidence Bin