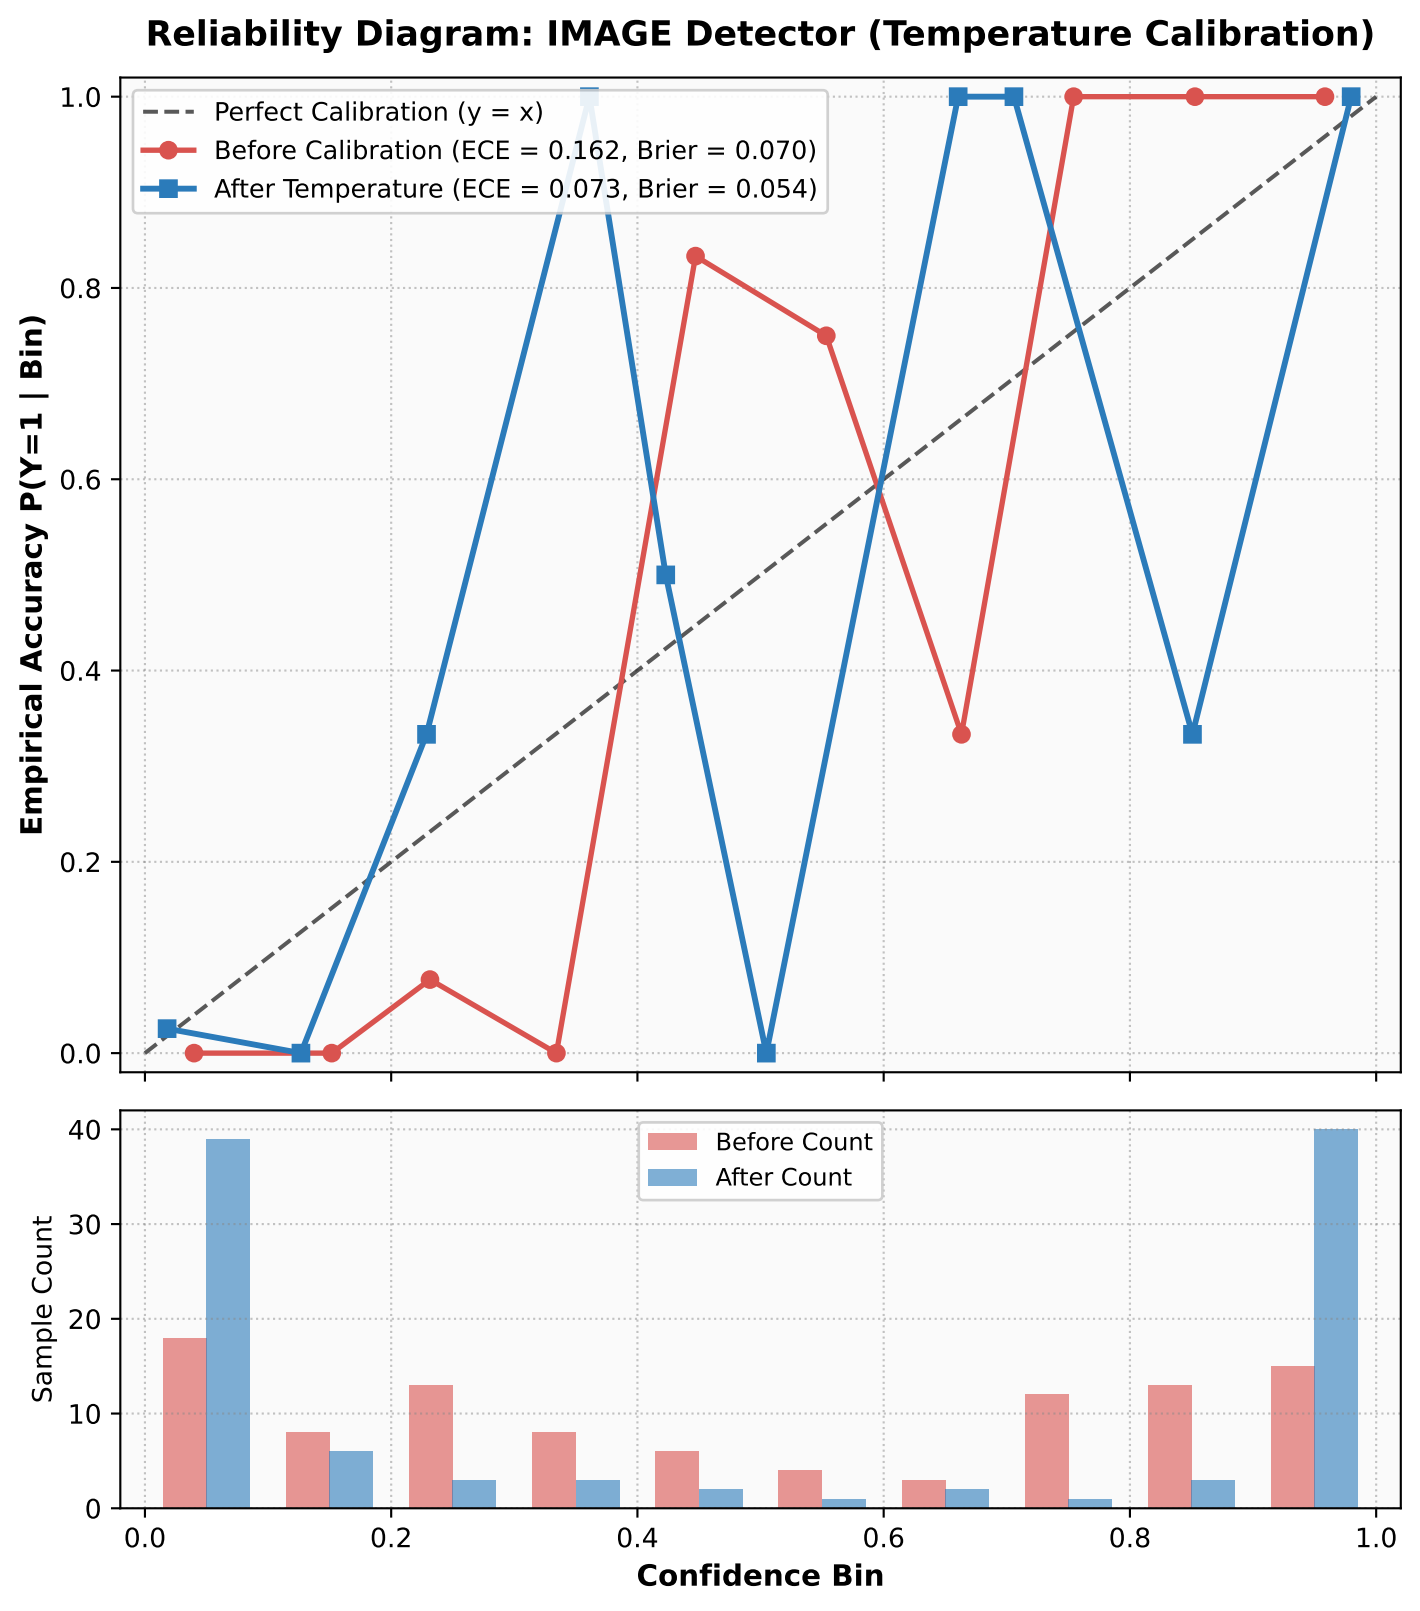
Reliability Diagram: IMAGE Detector (Temperature Calibration)
Perfect Calibration (y = x)
Before Calibration (ECE = 0.162, Brier = 0.070)
After Temperature (ECE = 0.073, Brier = 0.054)
Empirical Accuracy P(Y=1 | Bin)
0.0
0.2
0.4
0.6
0.8
1.0
Before Count
After Count
Sample Count
0
10
20
30
40
0.0
0.2
0.4
0.6
0.8
1.0
Confidence Bin