


Threshold sensitivity: conclusions are STABLE under +/-20% threshold perturbation

Every ablation conclusion holds at every threshold scale. Cell = runtime integrity score (colour + top line); undetected-risk rate (URR) below it.

30 executions = 6 configurations x 5 threshold scales; 4 stability checks evaluated at every scale.

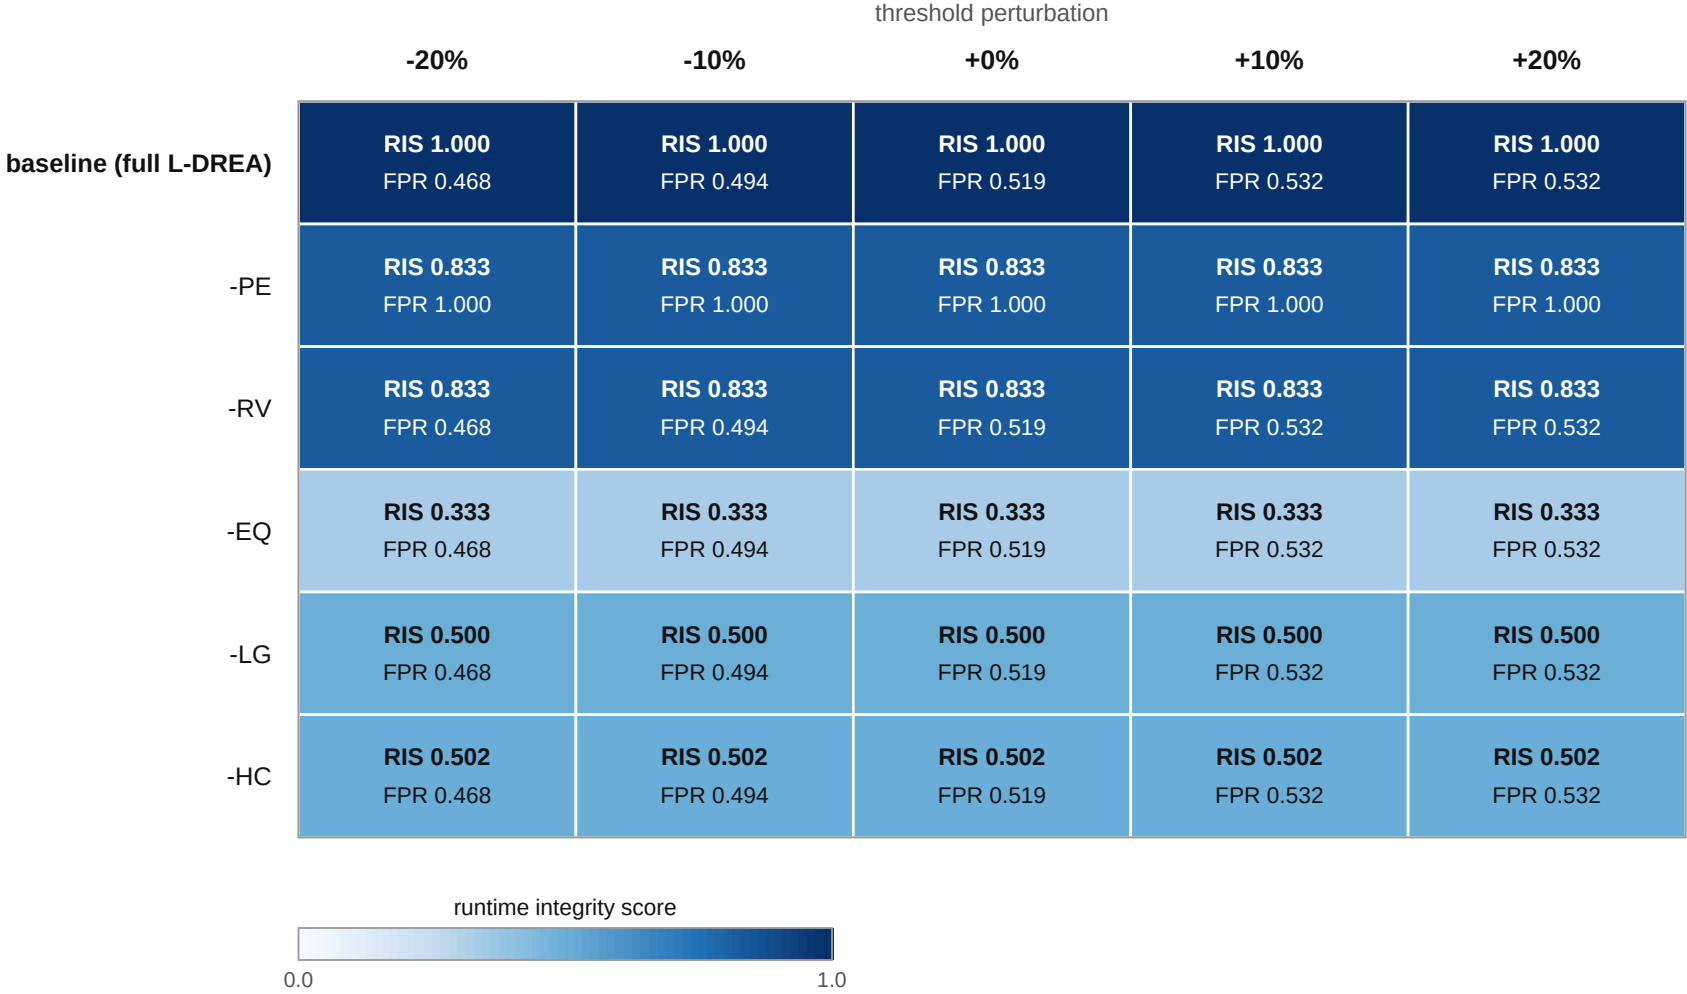

RIS is invariant to the threshold scale (every row is flat): the ablation ranking does not depend on where the decision thresholds sit. Only the undetected-risk rate (URR) moves with the threshold, and it moves for the baseline and the ablations alike.