


Training pipeline (per funnel stage)

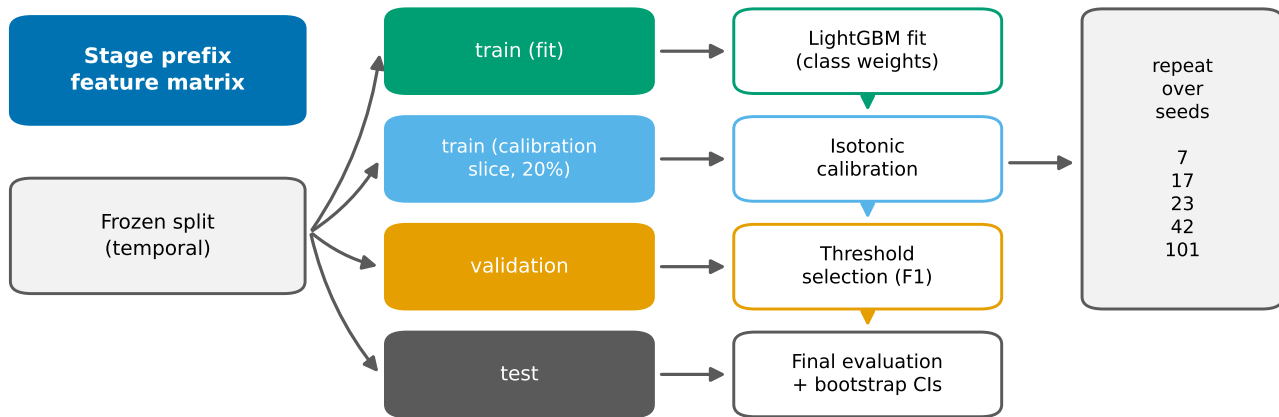

Calibration is fitted on a held-out slice of the *training* period, not on validation. Under the prior shift present in these data, calibrating on validation raises expected calibration error by roughly an order of magnitude (Figure 5); the textbook choice is the wrong one here. The test partition enters only at the final evaluation box.