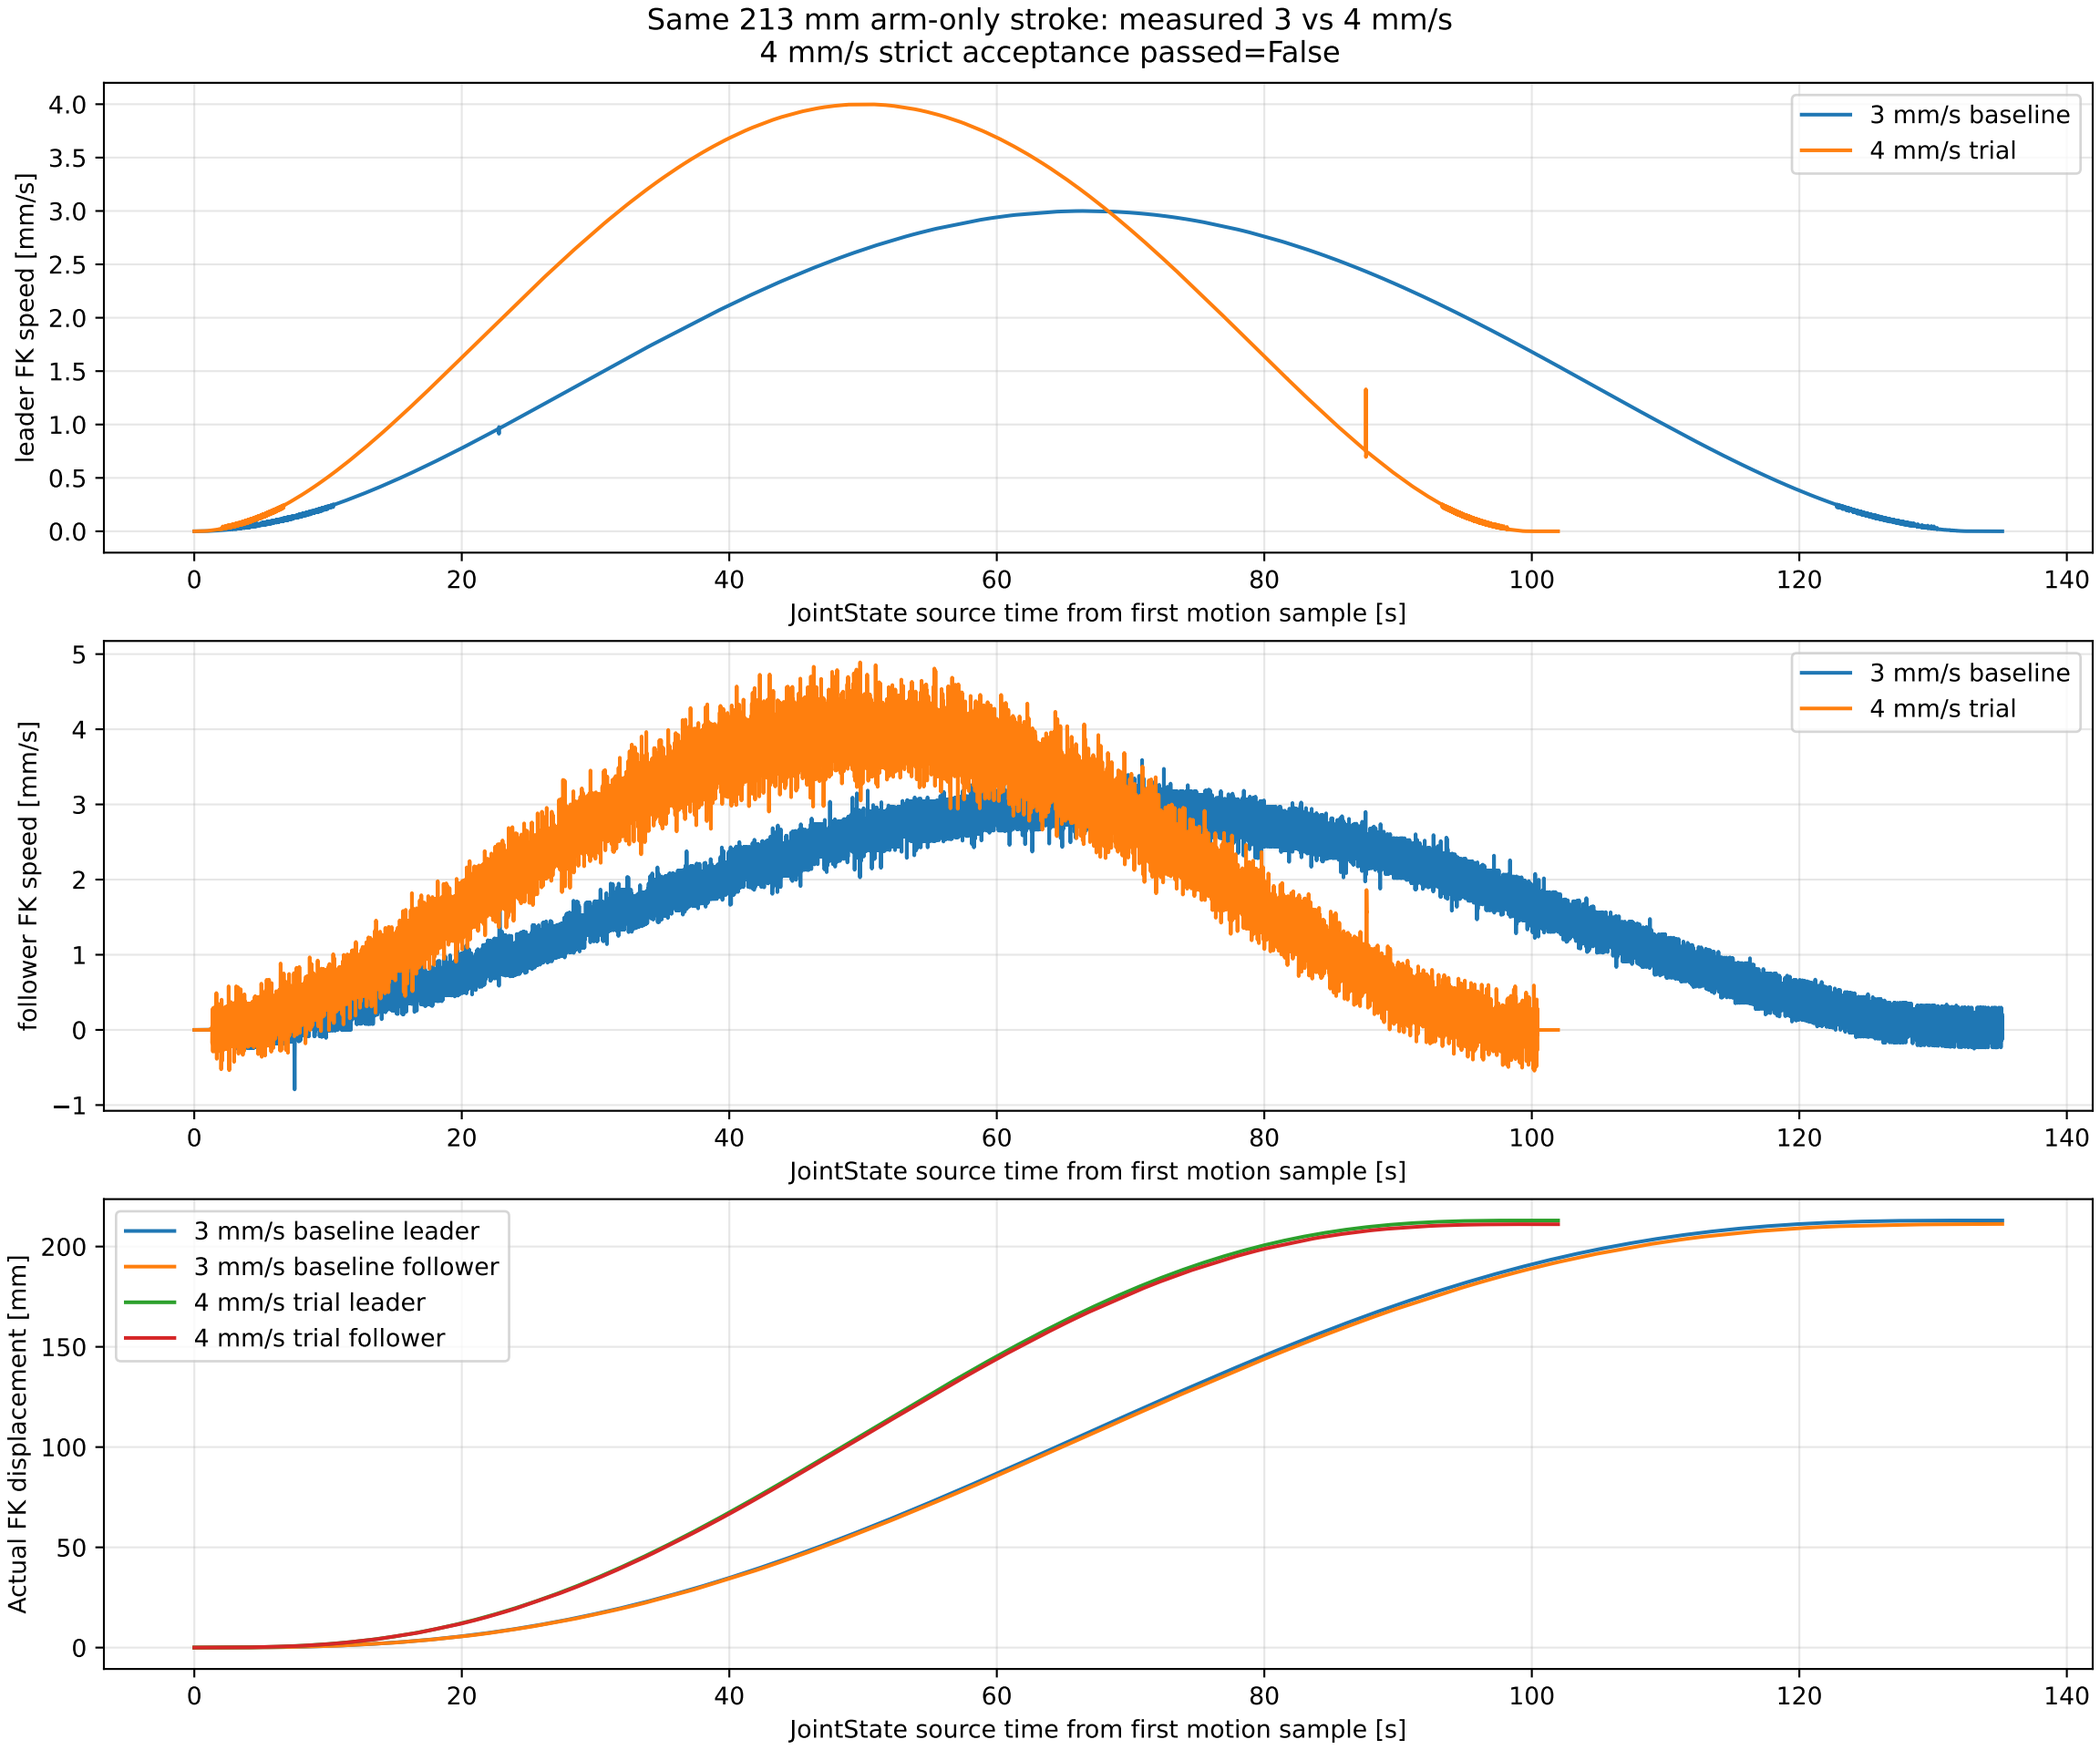

Same 213 mm arm-only stroke: measured 3 vs 4 mm/s
4 mm/s strict acceptance passed=False
leader FK speed [mm/s]
3 mm/s baseline
4 mm/s trial
JointState source time from first motion sample [s]
follower FK speed [mm/s]
3 mm/s baseline
4 mm/s trial
JointState source time from first motion sample [s]
Actual FK displacement [mm]
3 mm/s baseline leader
3 mm/s baseline follower
4 mm/s trial leader
4 mm/s trial follower
JointState source time from first motion sample [s]