



Record a new therapy
Sequence Diagram
(Use Case 6)


User presses the Finish Session button to simulate a therapy ending properly by waiting the selected time.

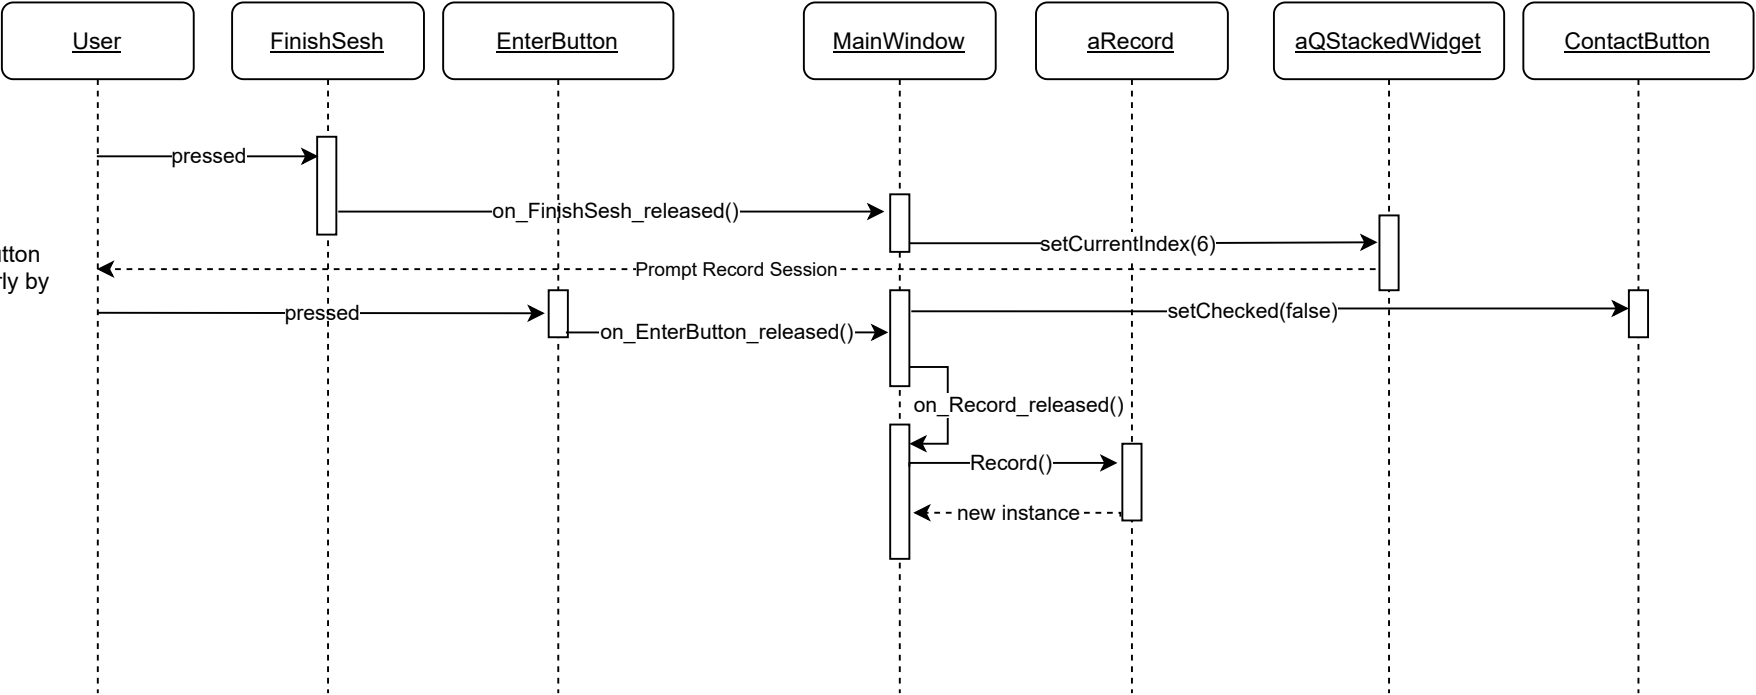

User waits for the therapy timer to reach zero and end the session properly

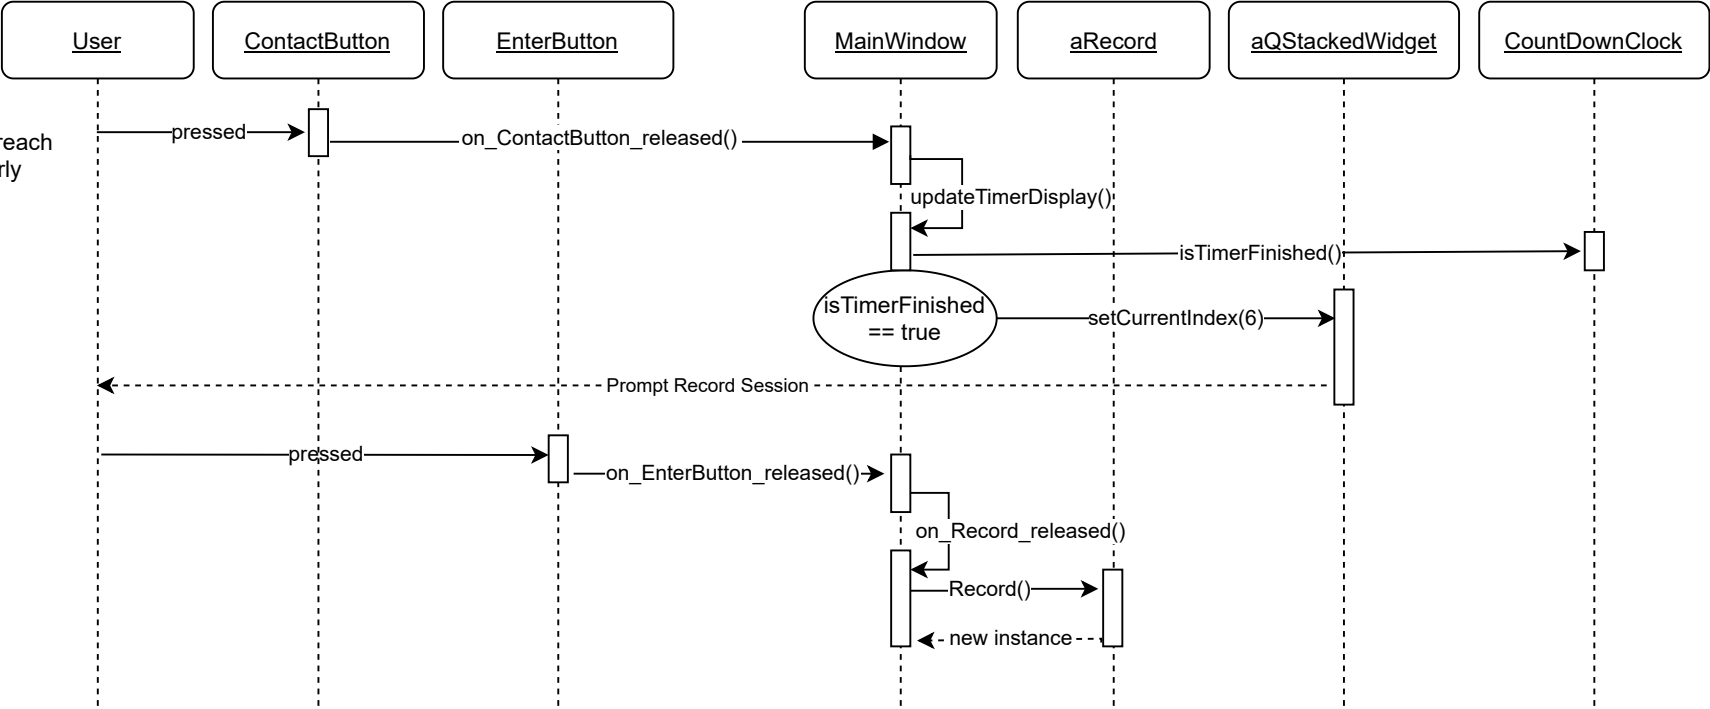

Contact is made starting the Therapy session and then removed for longer than 5 seconds ending the therapy session.

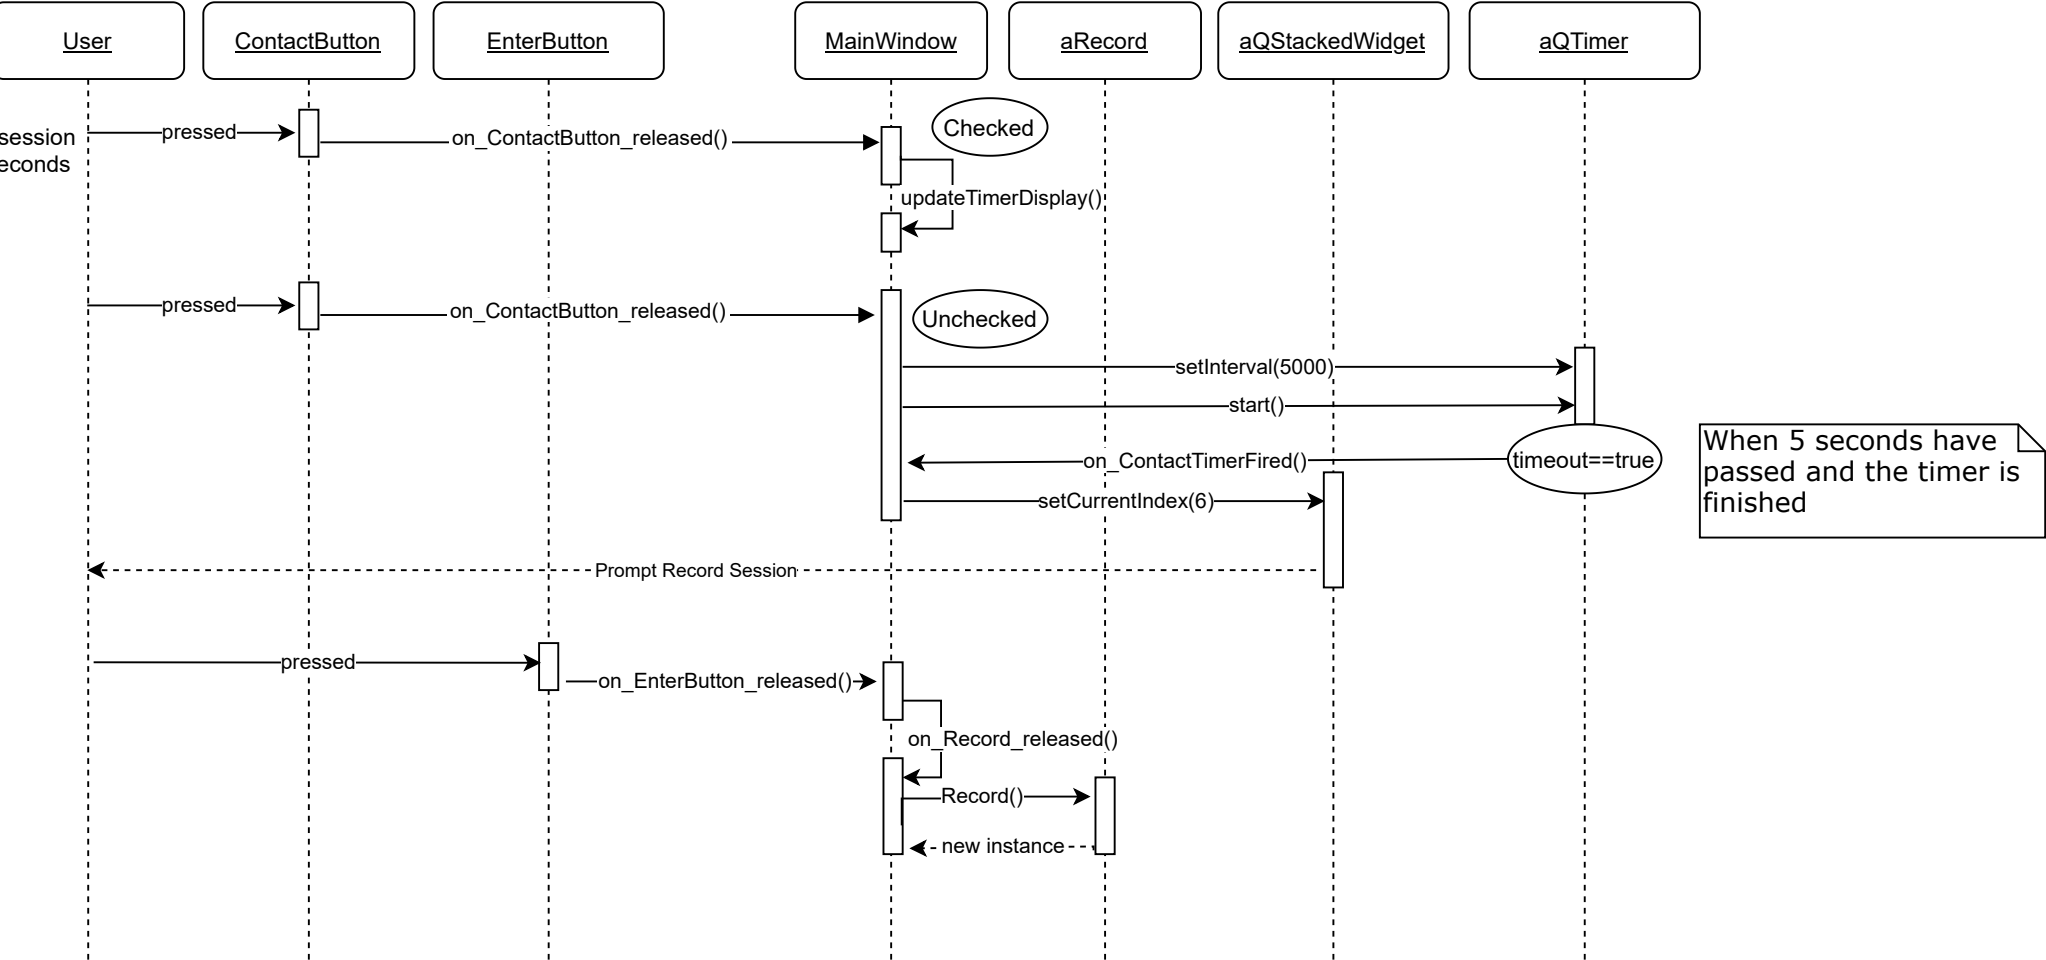

When 5 seconds have passed and the timer is finished