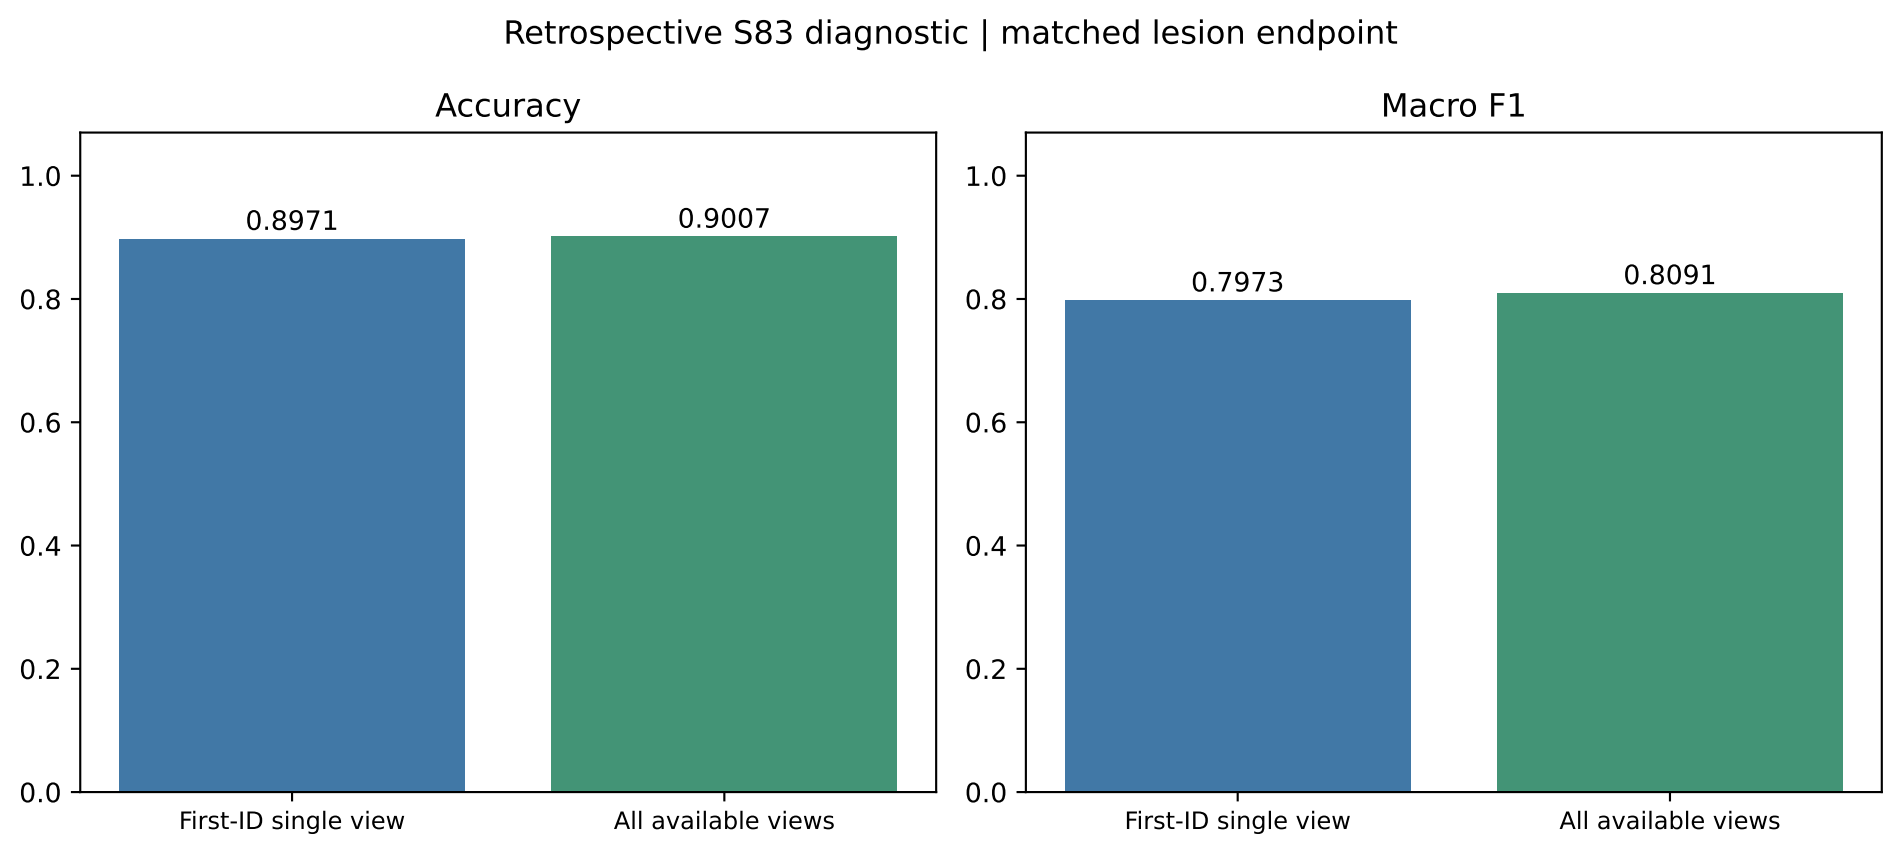
Retrospective S83 diagnostic | matched lesion endpoint
Accuracy
Macro F1
1.0
0.8
0.6
0.4
0.2
0.0
0.8971
0.9007
0.7973
0.8091
First-ID single view
All available views
First-ID single view
All available views