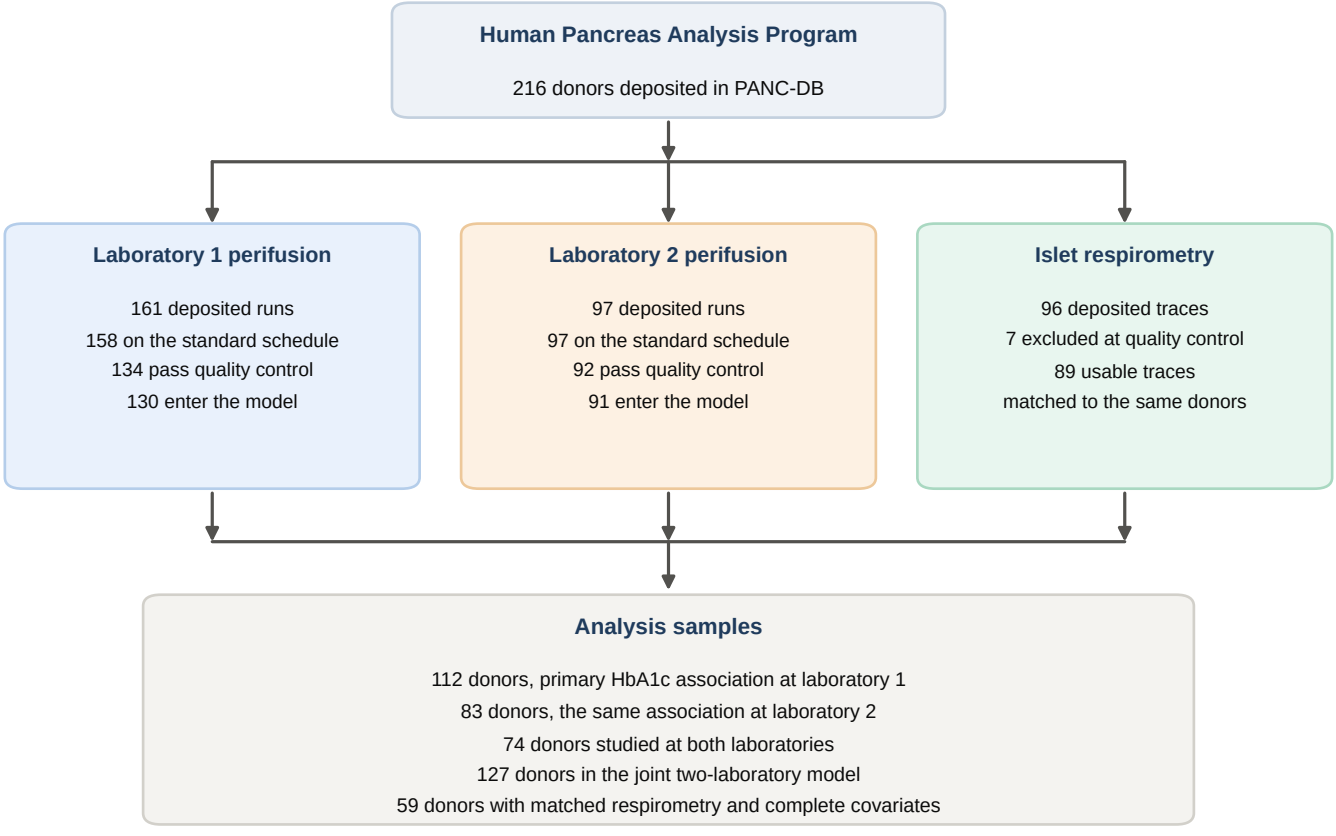
Human Pancreas Analysis Program
216 donors deposited in PANC-DB
Laboratory 1 perifusion
161 deposited runs
158 on the standard schedule
134 pass quality control
130 enter the model
Laboratory 2 perifusion
97 deposited runs
97 on the standard schedule
92 pass quality control
91 enter the model
Islet respirometry
96 deposited traces
7 excluded at quality control
89 usable traces
matched to the same donors
Analysis samples
112 donors, primary HbA1c association at laboratory 1
83 donors, the same association at laboratory 2
74 donors studied at both laboratories
127 donors in the joint two-laboratory model
59 donors with matched respirometry and complete covariates