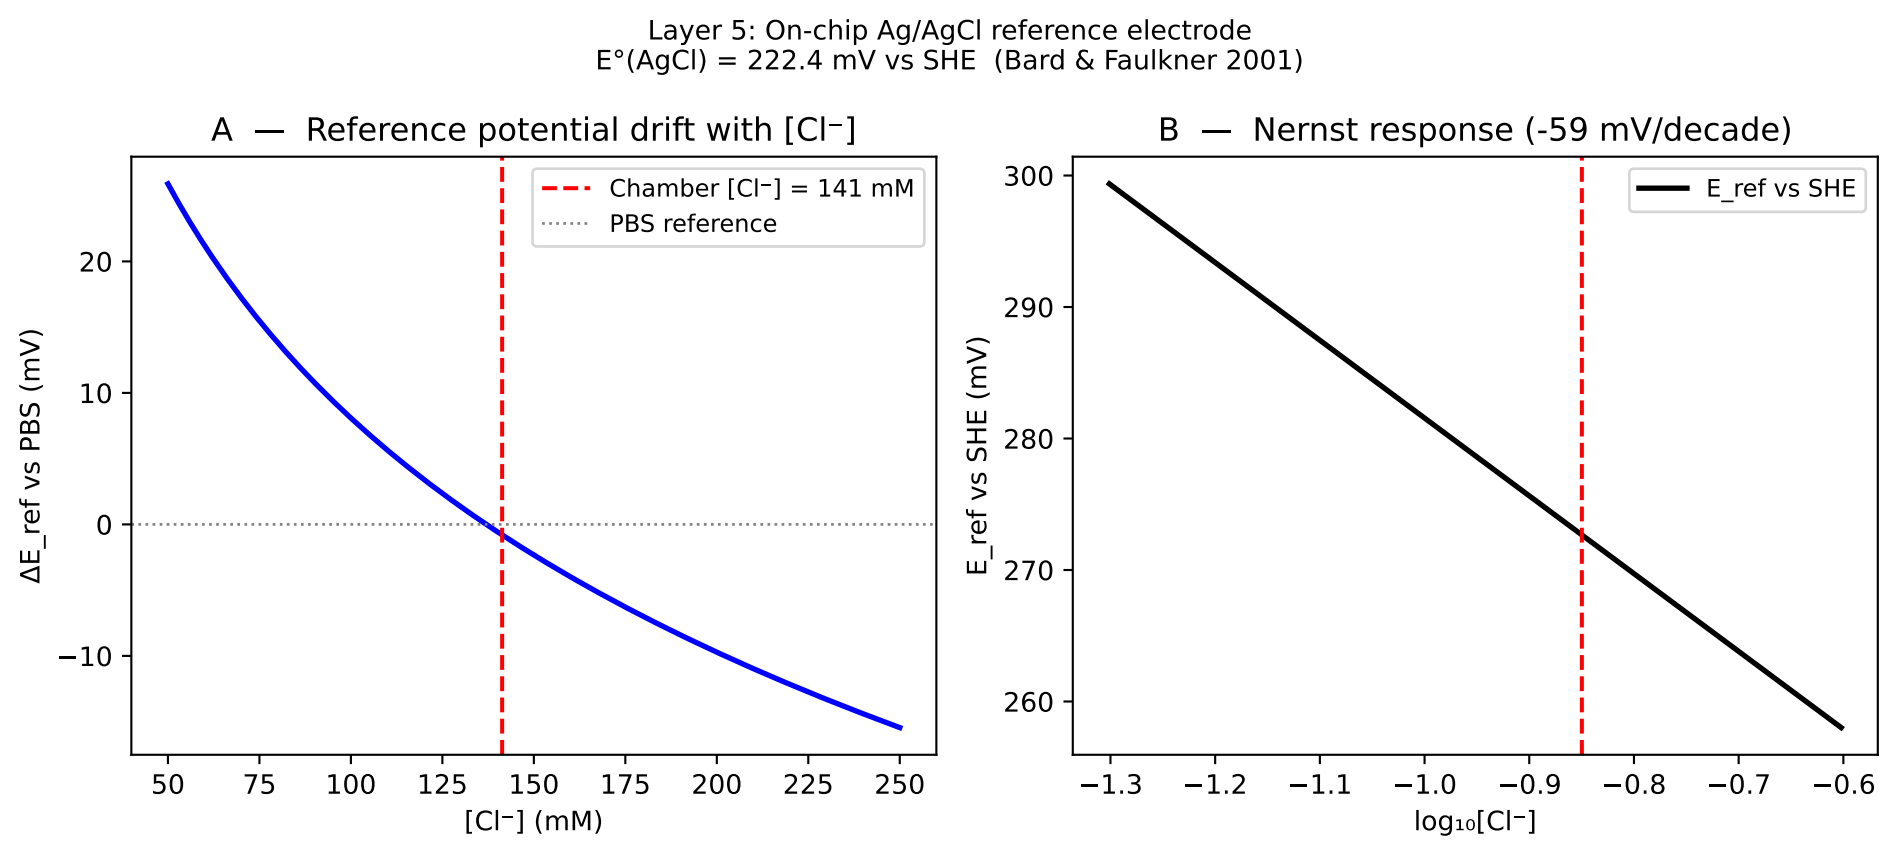
Layer 5: On-chip Ag/AgCl reference electrode
E°(AgCl) = 222.4 mV vs SHE (Bard & Faulkner 2001)
A — Reference potential drift with [Cl⁻]
Chamber [Cl⁻] = 141 mM
PBS reference
ΔE_ref vs PBS (mV)
[Cl⁻] (mM)
B — Nernst response (-59 mV/decade)
E_ref vs SHE
E_ref vs SHE (mV)
log₁₀[Cl⁻]