

GRIFOLS Diagnostic Grifols, S.A.	Reference:	REGD-0000793	Version:	3.0, CURRENT
	Status:	Effective	Effective Date:	26-May-2011
Title:	SM DG57-DG517. Power fuse status verification.			Page 2 of 5

DG-57 / DG-517 Service Manual

POWER FUSE STATUS VERIFICATION

Procedure description
This procedure describes how check the fuses related to power. <i>Note: Document REGD-0000793_v3 replaces document REGD-0000793_v2.</i>


GRIFOLS Diagnostic Grifols, S.A.	Reference:	REGD-0000793	Version:	3.0, CURRENT
	Status:	Effective	Effective Date:	26-May-2011
Title:	SM DG57-DG517. Power fuse status verification.			Page 3 of 5

EQUIPMENT

1. Multimeter.

SET UP

1. Turn instrument off
2. Open the rear panel
3. Turn instrument on




CAUTION!

Short-circuit between any powered part and ground, may damage the instrument

PROCEDURE

Process	Expected Results
Checking the 8V fuse NOTE: If led D1 is OFF when the instrument is turned on, the fuse is probably broken. 1. To check the fuse status, measure the voltage between TP1 (negative) and FUSE_IN_8V with the multimeter (see Picture 1) Picture 1	--- $7.75 \pm 0,25 \text{ V}$

GRIFOLS Diagnostic Grifols, S.A.	Reference:	REGD-0000793	Version:	3.0, CURRENT
	Status:	Effective	Effective Date:	26-May-2011
Title:	SM DG57-DG517. Power fuse status verification.			Page 4 of 5

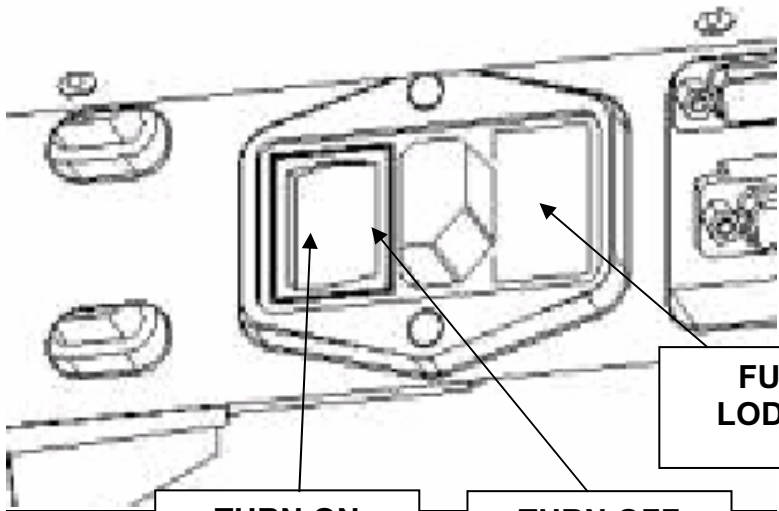Process	Expected Results
Checking the 12V supply 2.  NOTE: If led D1 is OFF when the instrument is turned on, the fuse is probably broken. 3. To check the fuse status, measure the voltage between TP1 (negative) and FUSE_IN_12V with the multimeter (see picture 1) Checking the mains fuses 4.  NOTE: If the fan of switched power supply doesn't rotate when the instrument is turned on, the mains fuses are probably broken. 5. Turn off the instrument. (See Picture 2)  Picture 2 6. Open Fuses Lodging. 7. To check fuses status, measure the conductivity of each fuse.	--- 12.15 ± 0,25 V --- --- --- ---

GRIFOLS Diagnostic Grifols, S.A.	Reference:	REGD-0000793	Version:	3.0, CURRENT
	Status:	Effective	Effective Date:	26-May-2011
Title:	SM DG57-DG517. Power fuse status verification.			Page 5 of 5

DOCUMENT CHANGE HISTORY

Document change history			
Version	Date	Change	Rationale
2.0	2005/05/09	<i>Document REGD-0000793_v2 replaces document 57021V0M000.</i>	Document reference changed.
3.0	See document header.	Added previous version 'data', 'change' and 'rationale' inside document change history section.	Update change history for previous document history modification.
3.0	See document header.	<i>Document REGD-0000793_v3 replaces document REGD-0000793_v2.</i>	Document version changed.
3.0	See document header.	Modified picture 1.	Picture available for DG-57 and DG-517.
3.0	See document header.	Document title.	-Commercial reference substituted by project reference. -Verification is related to power fuses.
3.0	See document header.	Document header.	Increase information to easy document search.