

GRIFOLS Diagnostic Grifols, S.A.	Reference:	REGD-0000817	Version:	4.0, CURRENT
	Status:	Effective	Effective Date:	08-Jul-2011
Title:	SM DG57-DG517. Pressure detector adjustment.			Page 2 of 5

DG-57 / DG-517 Service Manual

PRESSURE DETECTOR ADJUSTMENT

Procedure description
This procedure describes how to adjust the value of the potentiometer P2 of PCA Control IO57-2 in order to detect when there is enough pressure in the fluidic system. <i>Note: Document REGD-0000817_v4 replaces document REGD-0000817_v3.</i>

GRIFOLS Diagnostic Grifols, S.A.	Reference:	REGD-0000817	Version:	4.0, CURRENT
	Status:	Effective	Effective Date:	08-Jul-2011
Title:	SM DG57-DG517. Pressure detector adjustment.			Page 3 of 5

EQUIPMENT

1. Manometer + racor type CPC (1 unit code 232201 and 1 unit 231860).
2. Multimeter.
3. Calculator.



NOTE:

Ground in all measurements is TP23

SET UP

1. Turn instrument off.
2. Open the rear panel.
3. Turn instrument on.
4. Execute the ST software (Technical Service software).
5. Enter the Technical Service password (d+g_diana).
6. Pumps turned off.



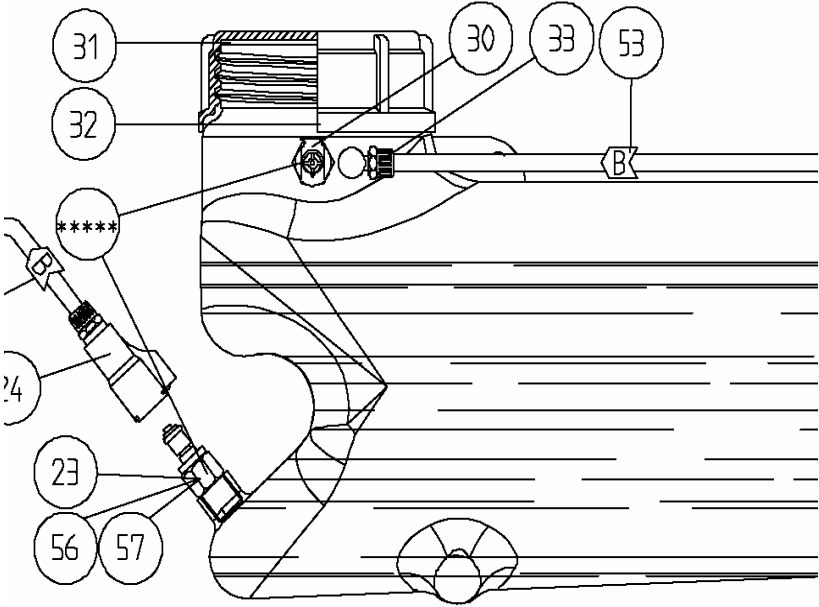
CAUTION!

Short-circuit between any powered part and ground, may damage the instrument.

PROCEDURE

Process	Expected Results
1. Measure and record the value in TP9* [mV]. See Picture 1.	TP9 P2 ... TP12 TP23
Picture 1	

GRIFOLS Diagnostic Grifols, S.A.	Reference:	REGD-0000817	Version:	4.0, CURRENT
	Status:	Effective	Effective Date:	08-Jul-2011
Title:	SM DG57-DG517. Pressure detector adjustment.			Page 4 of 5

Process	Expected Results
2. Disconnect the racor n°33 from the racor n°30 (bottle). Connect the manometer between these two racors.  Picture 2 3. Activate the pumps: Access I/O tab, click on Pumps checkbox. 4. Wait until the manometer measure is stable. 5. Record the measured pressure [mbar]. 6. Measure and record the value in TP9* [mV] again. See picture 1. 7. Calculate: $\text{Press} = \frac{\text{Value (step 6[mV])} - \text{Value (Step 1[mV])}}{\text{Value (step 5[mbar])}} \times 125 + \text{Value (step 1[mV])}$ 8. Place the multimeter in TP12. 9. Adjust potentiometer P2 until voltage measured in TP12 is the calculated one in step 7.	--- Pumps turn on 180±20mbar --- --- --- --- Press

* Note: instruments with s/n < 057-118-xxxx, be aware that corresponding value should be measured at TP11 instead of TP9.

GRIFOLS Diagnostic Grifols, S.A.	Reference:	REGD-0000817	Version:	4.0, CURRENT
	Status:	Effective	Effective Date:	08-Jul-2011
Title:	SM DG57-DG517. Pressure detector adjustment.			Page 5 of 5

DOCUMENT CHANGE HISTORY

Document change history			
Version	Date	Change	Rationale
3.0	2005/05/09	<i>Document REGD-0000817_v3 replaces document 57044V0M001.</i>	Document reference changed.
3.0	2005/09/09	Included pressure test points name I/O Board version dependence.	Update procedure.
4.0	See document header	Added `previous version `data`, `change` and `rationale` inside document change history section.	Update change history for previous document history modification.
4.0	See document header.	<i>Document REGD-0000817_v4 replaces document REGD-0000817_v3.</i>	Document version changed.
4.0	See document header.	Equipment section updated.	Added spare part codes.
4.0	See document header.	`Set up` section updated.	Document available for DG-57 and DG-517.
4.0	See document header.	Document title.	Commercial reference substituted by project reference.
4.0	See document header.	Document header.	Increase information to easy document search.