

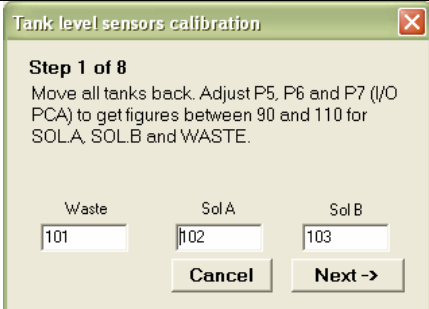
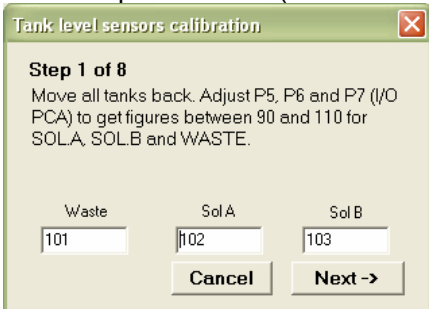
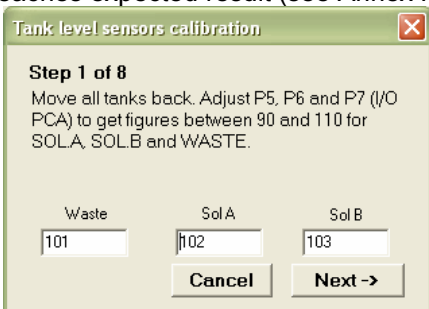
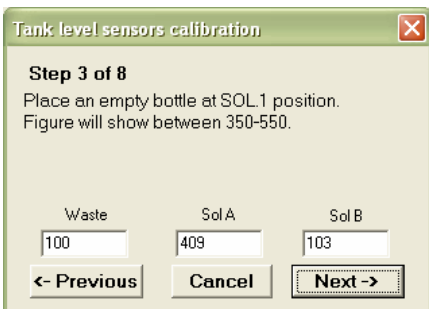
GRIFOLS Diagnostic Grifols, S.A.	Reference:	REGD-0000819	Version:	4.0, CURRENT
	Status:	Effective	Effective Date:	08-Jul-2011
Title:	SM DG57-DG517. Load cells adjustment.			Page 2 of 7

DG-57 / DG-517 Service Manual

LOAD CELLS ADJUSTMENT

Procedure description
This procedure describes how adjust the value of the potentiometer P5,P6 and P7 of PCA Cntr IO57-2 to adjust the load cells. Note: Document REGD-0000819_v4 replaces document REGD-0000819_v3.

GRIFOLS Diagnostic Grifols, S.A.	Reference:	REGD-0000819	Version:	4.0, CURRENT
	Status:	Effective	Effective Date:	08-Jul-2011
Title:	SM DG57-DG517. Load cells adjustment.			Page 4 of 7

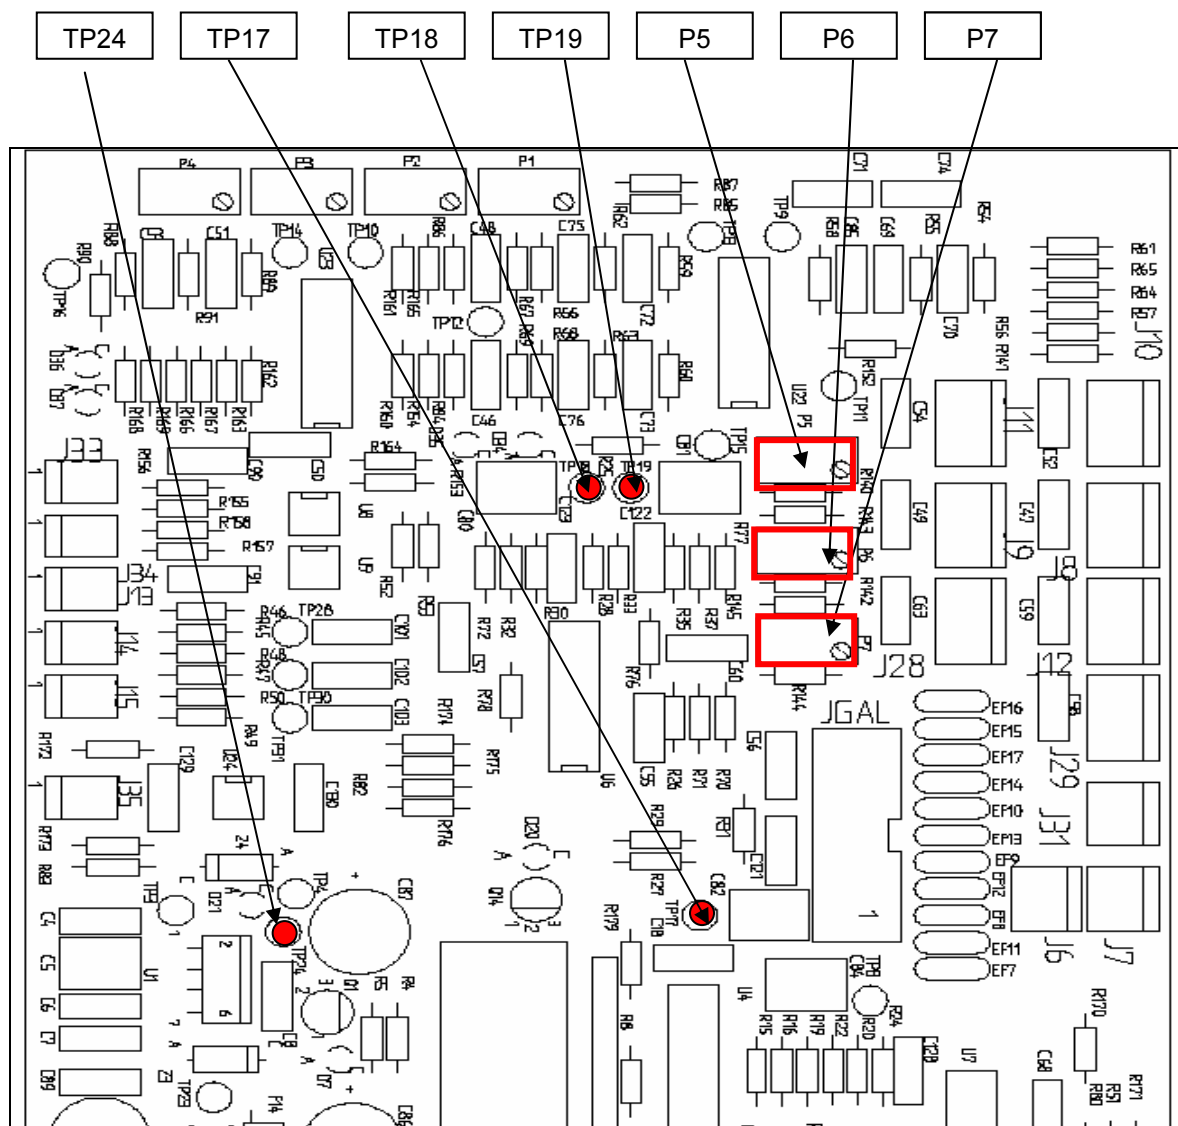
Process	Expected Results
4. Position the multimeter in TP19 (positive) and TP24 (negative). Adjust P6 until the measured value reaches expected result (see Annex PCA Layout) 	100±10 mV
5. Position the multimeter in TP18 (positive) and TP24 (negative). Adjust P7 until the measured value reaches expected result (see Annex PCA Layout) 	100±10 mV
6. Follow the instructions given on the screen.  	--

Reference:	REGD-0000819	Version:	4.0, CURRENT
Status:	Effective	Effective Date:	08-Jul-2011
Title:	SM DG57-DG517. Load cells adjustment.		Page 5 of 7

Process	Expected Results
Tank level sensors calibration Step 4 of 8 Place an empty bottle at SOL.2 position. Figure will show between 350-550. Waste Sol A Sol B 100 102 401 <- Previous Cancel Next -> Tank level sensors calibration Step 5 of 8 Place a bottle with 4 liters of water at Waste position. The value will showw between 1950 and 2650. Waste Sol A Sol B 2225 102 103 <- Previous Cancel Next -> Tank level sensors calibration Step 6 of 8 Place a bottle with 4 liters of water at SOL.1 position. The value will showw between 1950 and 2650. Waste Sol A Sol B 100 2187 102 <- Previous Cancel Next -> Tank level sensors calibration Step 7 of 8 Place a bottle with 4 liters of water at SOL.2 position. The value will showw between 1950 and 2650. Waste Sol A Sol B 100 101 2192 <- Previous Cancel Next -> Tank level sensors calibration Step 8 of 8 Threshold values to save will be: Waste: 2179 Sol.A: 631 Sol.B: 631 Waste Sol A Sol B 100 101 2191 <- Previous Cancel Finish 7. Press Finish button to accept all the steps previously carried out. --	

GRIFOLS Diagnostic Grifols, S.A.	Reference:	REGD-0000819	Version:	4.0, CURRENT
	Status:	Effective	Effective Date:	08-Jul-2011
Title:	SM DG57-DG517. Load cells adjustment.			Page 6 of 7

ANNEX PCA IO57-2 layout



GRIFOLS Diagnostic Grifols, S.A.	Reference:	REGD-0000819	Version:	4.0, CURRENT
	Status:	Effective	Effective Date:	08-Jul-2011
Title:	SM DG57-DG517. Load cells adjustment.			Page 7 of 7

DOCUMENT CHANGE HISTORY

Document change history			
Version	Date	Change	Rationale
2.0	2005/05/09	Document REGD-0000819_v2 replaces document 57046V0M000.	Uploaded document to GxPharma.
3.0	2011/04/28	Included all the pictures describing the load cells adjustment.	The document didn't have pictures about the adjustment process.
3.0	2011/04/28	Changed the expected results margins from 100±5 mV to 100±10 mV.	The expected results didn't match the real values set on the program.
3.0	2011/04/28	Updated the Document Change History: - Date format changed to YYYY/MM/DD - Dates changed to document version effective date.	Adoption of ISO 8601 date format to avoid ambiguity.
3.0	2011/04/28	ID-GELSTATION and PROVUE erased from the title.	Service manual intended for Grifols market.
4.0	See document header.	Document REGD-0000819_v4 replaces document REGD-0000819_v3.	Document version changed.
4.0	See document header.	Document title.	Commercial reference substituted by project reference.
4.0	See document header.	Document header.	Increase information to easy document search.