


Temperature Ablation: Flip Rates at temp=1.0 vs temp=0

gpt-4o-mini



gpt-4.1-mini

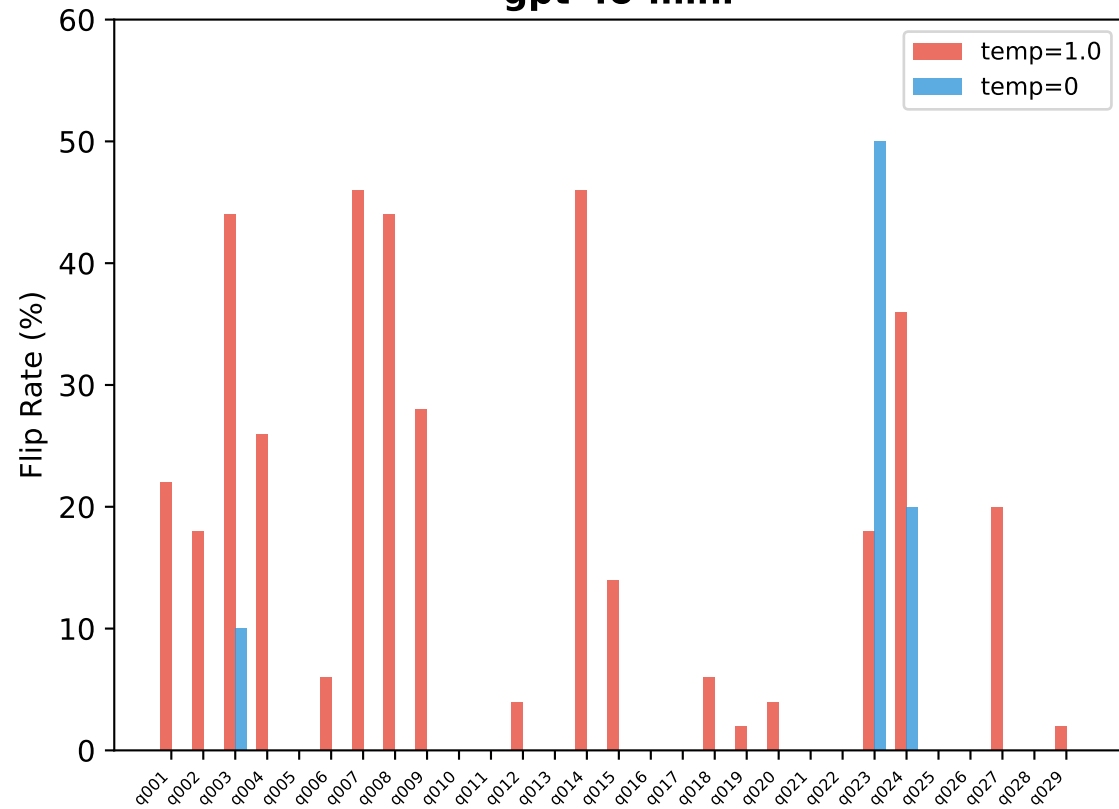