


Parameter recovery: sensor acuity

Acuity recovery $R^2 = 1.000$



Absolute recovery error per acuity level

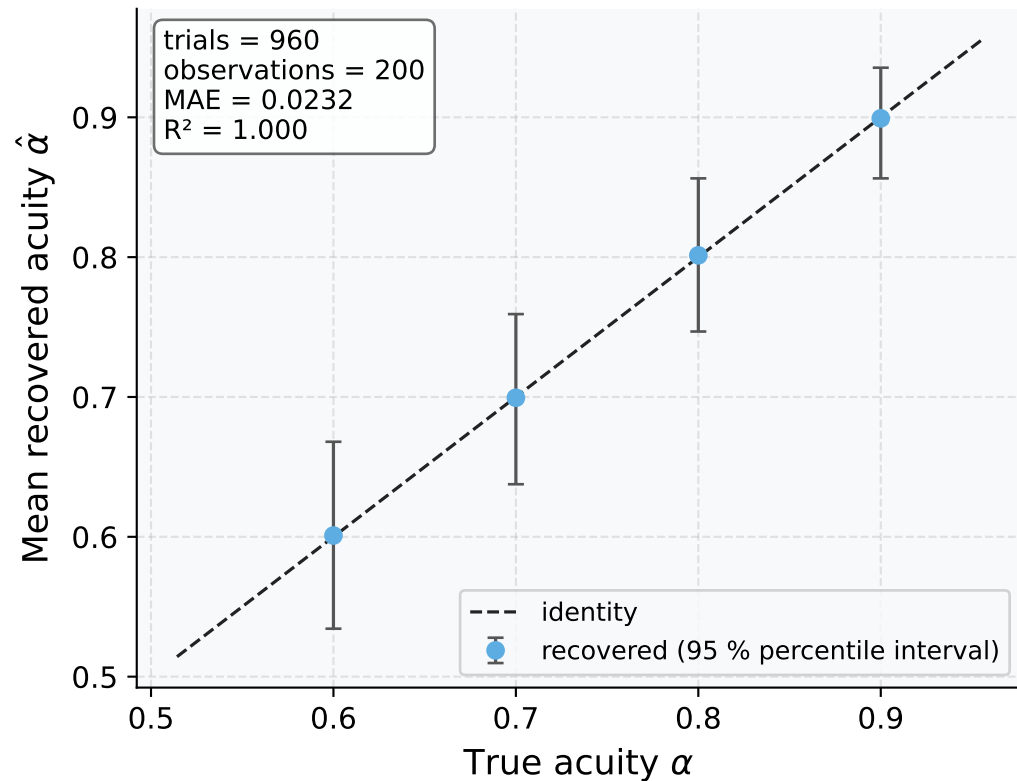