



Validation and Benchmarking of a Wearable EEG Acquisition Platform for Real-World Applications

Olivier Valentin , Mikaël Ducharme, Gabrielle Crétot-Richert, Hami Monsarrat-Chanon, Guilhem Viallet, Aidin Delnavaz, and Jérémie Voix 

Abstract—This paper presents the experimental validation of a readout circuit for the acquisition, amplification, and transmission of extremely weak biopotentials with a focus on electroencephalography (EEG) signals. The device, dubbed CochIEEG, benefits from a low-power design for long-term power autonomy and provides configurable gain and sampling rates to suit the needs of various EEG applications. CochIEEG features high sampling rates, up to 4 kHz, low-noise signal acquisitions, support for active electrodes, and a potential for Wi-Fi data transmission. Moreover, it is lightweight, pocket size, and affordable, which makes CochIEEG suitable for wearable and real-world applications. The efficiency of CochIEEG in EEG data acquisition is also investigated in this paper. Auditory steady-state responses acquisition results validate CochIEEG's capability in recording EEG with a signal quality comparable to commercial mobile or research EEG acquisition devices. Moreover, the results of an oddball paradigm experiment prove the capability of CochIEEG in recording event-related potentials and demonstrate its potential for brain-computer interface applications and electrophysiological research applications requiring higher temporal resolution.

Index Terms—Auditory steady-state response (ASSR), event-related potentials (ERP), wearable electroencephalography (EEG).

I. INTRODUCTION

RECENT advances in the manufacturing of inconspicuous body sensors and miniaturized circuits as well as considerable developments in telecommunications and data analysis techniques have opened up new possibilities for the integration of sensors into various accessories worn in daily life, such as clothing, hats and shoes. Body sensors and wearables have various applications including health and safety monitoring, home rehabilitation, and early detection of disorders, to name a few examples [1].

Electroencephalography (EEG) sensors for measuring brain electrical activity are becoming a major category of body-worn

sensors with a variety of applications in clinical studies, medical diagnosis and neurological researches. EEG signals can be measured by active or passive electrodes placed on or next to the scalp. These acquired signals must then be amplified and transmitted to a computer usually for further processing. Conventional EEG signal acquisition systems are bulky, which has impeded their integration into wearables and imposes serious limitations on EEG applications outside of a laboratory environment. Over the years, several mobile EEG signal acquisition systems have emerged. Some of these are commercialized as consumer products. For example, SMARTING (mBrainTrain, Belgrade, Serbia) is a small EEG device for real-time brain activity monitoring. ENOBIO (Neuroelectronics, Barcelona, Spain) is a wearable wireless electrophysiological signal acquisition system for EEG recording. Also, the EEG-SMT board (Olimex Ltd, Plovdiv, Bulgaria) is available as an open-source software and hardware unit for recording EEG signals. Similarly, Cyton biosensing board (OpenBCI, Brooklyn, NY, USA) can be used to record brain, muscle and heart activity on a wireless open-source platform. Moreover, Cognionics Inc. (San Diego, CA, USA) offers a wide range of mobile EEG systems for both high-density and low-density EEG recordings. Finally, Brain Products (Munich, Germany) recently released LiveAmp, a high-quality mobile wireless EEG recording solution.

Aside from the commercialized products, some research groups have developed their own mobile EEG recording systems for more specific applications. For example, EEGu2 is an embedded device for brain/body signal acquisition developed and used in the context of human-in-the-loop cyber-physical systems [2]. BioDAQ (Biological Data Acquisition) is a low-cost system that has been developed by Rahman and Nasor for real time biomedical applications [3] and a wearable multi-channel EEG recording system featuring a compression algorithm is presented by Dufort *et al.* [4].

However, most mobile EEG products on the market share common downsides. They are expensive, ranging from several hundred dollars to more than tens of thousands, which may impose a serious financial barrier on neurological research studies. It can also prevent EEG systems from being widely used in Brain-Computer Interface (BCI) devices. Furthermore, often-times some commercial products do not provide the raw EEG data to the consumers, which makes them less interesting for research applications. In addition, the limited sampling rate (often 500 Hz and less) of commercial products prevents their use for specific electrophysiological research applications that require

Manuscript received June 19, 2018; revised August 11, 2018 and September 24, 2018; accepted September 30, 2018. Date of publication October 15, 2018; date of current version January 25, 2019. This work was supported in parts by the NSERC-EERS Industrial Research Chair in In-Ear Technologies (CRITIAS) and MITACS Elevation program. This paper was recommended by associate editor M. Zaghloul. (Corresponding author: Olivier Valentin.)

The authors are with the NSERC-EERS Industrial Research Chair in In-Ear Technologies, École de technologie supérieure, Montreal QC H3C 1K3, Canada (e-mail: m.olivier.valentin@gmail.com; mikaelducharme@gmail.com; gabrielle.cretot-richert@etsmtl.ca; hami.monsarrat-CHANON@ets-mtl.ca; guilhem.viallet@etsmtl.ca; aidin.delnavaz@ens.etsmtl.ca; jeremie.voix@etsmtl.ca).

Color versions of one or more of the figures in this paper are available online at <http://ieeexplore.ieee.org>.

Digital Object Identifier 10.1109/TBCAS.2018.2876240

higher temporal resolution. Finally, many commercial EEG systems can only support a limited number of electrodes (under 5) and are not compatible with active EEG electrodes.

While these more recent portable EEG recording devices, developed by research groups and companies alike, answer innovative applications' need for less bulky equipment, they can be limiting compared to research grade equipment. Certain applications for wearable EEG devices might be impeded by these constraints. A more accessible and flexible system that could accommodate electrode technology while supporting multiple input channels as well as greater sampling frequencies and raw data output streams could be the solution for these applications.

This paper presents a wearable electronic device dubbed CochIEEG intended for the acquisition, amplification and transmission of EEG signals, designed in an attempt to overcome the previously described limitations. It provides eight channels that can connect to both passive and active EEG electrodes. Its battery-powered circuit board along with its lightweight and pocket-sized packaging, positions the CochIEEG as an ideal candidate for portable EEG. It is convenient to carry and would be easy to integrate into wearables. Moreover, it offers a very precise time resolution with sampling frequency reaching up to 4 kHz, which is required for applications such as Frequency Following Responses (FFR) among others. The objective of this research is to test and compare the EEG recording performance of CochIEEG. For that purpose, two EEG paradigms with high potential in the context of auditory research and BCI applications were chosen to evaluate the performance of CochIEEG to record EEG time series and frequency spectrums. In a first study, Auditory Steady-State Responses (ASSRs) recording performance with CochIEEG was tested and the spectral results were compared with those obtained by 1) Rotman MASTER research system (Baycrest Center, University of Toronto, Canada) as a conventional research-grade EEG research system and 2) SMARTING as a well-known, tested and proven, commercially available mobile EEG device. In a second study, Event-Related Potentials (ERP) from an auditory oddball paradigm were recorded using CochIEEG to demonstrate the capability of the proposed EEG acquisition platform for such applications in the temporal domain.

This paper is structured as follows: the equipment and experimental procedures are described in Section II. ASSRs results and ERP results are presented in Section III and discussed in Section IV. Conclusions and the future works are given in Section V.

II. METHODS

Two studies were conducted and the methodologies employed are presented in this section. The first study is a comparison study between three EEG systems presented in Table I, an ASSR paradigm was used. Previous work from Melnik *et al.* [5] developed a scientific approach to evaluate and compare EEG systems. To account for the systems different electrode count and placement, they interpolated the channel recordings over a mesh-head model. This is important because differences

TABLE I
CHARACTERISTICS OF THE THREE DIFFERENT ACQUISITION SYSTEMS

	SAMPLING FREQUENCY	RESOLUTION	INPUT NOISE (RMS)	WEIGHT	SIZE
SMARTING	250 to 500 Hz	24 bits	353 nV *	64 g	82 x 51 x 14 mm
COCHIEEG	250 to 4000 Hz		139 nV	47 g	66 x 33 x 23 mm
MASTER	1000 Hz	12 bits	N/A**	Couple kg	Table-top setup

*Data apparently taken from TI's datasheet, by Smarting manual.

**Master's input noise is tricky to measure as this system needs several equipment to be fully functional.

between systems could be attributed to electrode positions. For this study however, electrode count and placement remained the same over all systems, only the EEG amplifiers differed. Melnik *et al.*'s approach also took into consideration the different sources of variability and they found that variance across subjects was generally higher than variance across systems. Although this comparison is interesting when evaluating the importance of the difference in performance between systems, it was beyond the scope of this article. Another important comparison study between EEG systems was presented in De Vos *et al.*'s [6]. Their ERP study for a P300 speller application proposed as basis for comparison: EEG waveform, performance in spelling and information transfer rates (ITRs). These are in fact very relevant to consider when comparing systems for ERP studies. The ASSR paradigm however is a passive paradigm where the expected result is a frequency peak in the EEG spectrum.

The second study consisted of recording ERPs elicited with an active auditory oddball paradigm. This study was chosen to demonstrate CochIEEG's capability to record waveforms but was not a comparison between systems.

These studies were reviewed and approved by the *Comité d'éthique pour la recherche*, the Internal review Board at École de technologie supérieure (ÉTS) in Montreal, Canada. Informed consent was obtained from all participants before they were enrolled in the study.

A. Participants

Ten individuals (eight males, two females) aged between 22 and 34 and having hearing thresholds below 25 dB HL (pure tone audiometry between 125 to 8000 Hz) participated in the ASSR study. Ten individuals (seven males, three females) with ages ranging from 21 to 34 and also with hearing thresholds below 25 dB HL participated in the ERP study. All participants were free of past or present neurological conditions.

B. Hardware Used

1) *Hardware 1: MASTER System:* The Rotman MASTER (multiple auditory steady-state evoked response) research system is a data acquisition system designed by John & Picton [7] to assess human hearing by recording ASSRs. This LabVIEW-based environment is capable of simultaneously generating multiple amplitude-modulated and/or frequency-modulated

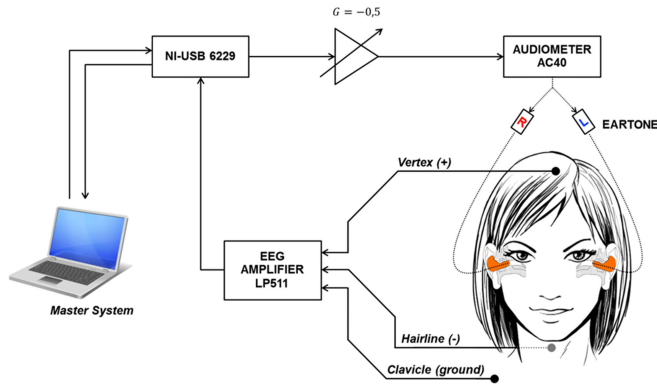


Fig. 1. Overview of a typical MASTER system setup. All components are monitored by a single PC. The stimulation signals from the analog output of the NI-USB 6229 board are attenuated by an operational amplifier with a gain of -0.5 , so that they may be delivered to the line input of the audiometer, which enables the operator to adjust the levels of stimuli delivered by the insert earphones. In parallel, ASSRs are scalp-recorded by the electrodes (placed between vertex (+) and hairline (-), with clavicle as a ground) and are then amplified by an EEG amplifier before reaching the analog input of the data acquisition board. Data are processed online through the MASTER system software.

auditory stimuli, acquiring corresponding electrophysiological responses, displaying results in the frequency-domain, and determines whether the responses are significantly larger than background physiological activity. The MASTER system data acquisition setup for ASSR recordings is schematically illustrated in Fig. 1.

ASSRs were filtered using a band-pass filter of 0.3–300 Hz (12 dB/octave) and amplified 50,000X (10,000X in GRASS Technologies LP511 AC Amplifier and 5X in National Instruments USB-6259 BNC). All data were collected using an Analog-to-digital (A/D) conversion rate of 1000 samples per second. In each recording, individual data epochs of 1024 points each were collected and connected together into sweeps (16 epochs per sweep of 16.384 seconds each). A typical ASSR recording for this study required a total of 6 sweeps over 98.304 seconds. To minimize artifacts, epochs containing signals exceeding $\pm 80 \mu\text{V}$ were rejected.

ASSR sweeps of data were averaged in the time domain and then analyzed on-line in the frequency domain using the Fast Fourier Transform (FFT).

Amplitudes are expressed in nanovolts (nV). An F-ratio statistic is used by the MASTER system to evaluate the probability that the amplitude of the ASSR is significantly different from the average amplitude of the background noise in the adjacent frequencies (within ± 60 bins of the modulation frequency). A response is considered to be present if $p < 0.05$.

2) *Hardware 2: SMARTING*: SMARTING shown in Fig. 2 is a 24-channel mobile EEG amplifier developed by mBrainTrain (Belgrade, Serbia). The system features two sampling frequencies (250 Hz or 500 Hz), a resolution of 24 bits and a bandwidth from DC to 250 Hz. The weight and size of the version used are respectively 64 grams and $82 \times 51 \times 14$ mm. The amplifier unit includes a 3D gyroscope and a power supply for several hours of use. It transmits data wirelessly with Bluetooth (v2.1) protocol to a paired laptop, which was



Fig. 2. SMARTING mobile EEG amplifier.

positioned in the audiometric booth at a distance of about two meters from the participant, well within the device's range of 10 meters. ASSRs were recorded during 98.304 seconds, which corresponds to 6 sweeps of 16.384 seconds each, with two available sampling rates (250 and 500 Hz), by using the software provided by the manufacturer (Smarting Streamer version 2.2.2.0). Event markers were generated at the beginning and at the end of each stimulation using Lab Streaming Layer (LSL), a data acquisition and control framework developed at the Swartz Center for Computational Neuroscience (available: <https://github.com/sccn/labstreaminglayer>) [8] for recording stimulations and data streams with precise synchronizing performances.

Data and event markers were written into a common file format (.xdf).

Data were analyzed offline using MATLAB and EEGLAB [9]. ASSR data were filtered using a FIR band-pass filter with an upper cut-off frequency of 0.1 Hz and lower cut-off frequency of half of the sampling rate. Sweeps of data were then extracted from the data stream using LSL markers and were averaged in the time domain before being translated in the frequency domain using FFT. The procedures of calculating amplitudes and background noise were similar to those used for the MASTER system.

3) *Hardware 3: CochIEEG*: CochIEEG, shown in Fig. 3, is a custom 8-channel portable EEG research platform using a low-noise simultaneous 24-bit sampling analog-to-digital converter (ADS1299) developed by Texas Instruments. CochIEEG benefits from the use of this integrated chip by having user-configurable variable gain amplifiers, and variable sampling rates from 250 Hz to 4000 Hz. CochIEEG's measured input-referred noise is 139 nV_{RMS} (using a linear gain of 24 and 250 Hz). It has a bipolar 2.5 V supply output for active electrodes support and a mini-USB port with 5 kV isolation for data transmission. The system is 47 grams in weight and measures $66 \times 33 \times 23$ mm, including the battery. CochIEEG can acquire EEG data for multiple hours without interruption. A block diagram of the hardware architecture is illustrated in Fig. 4.

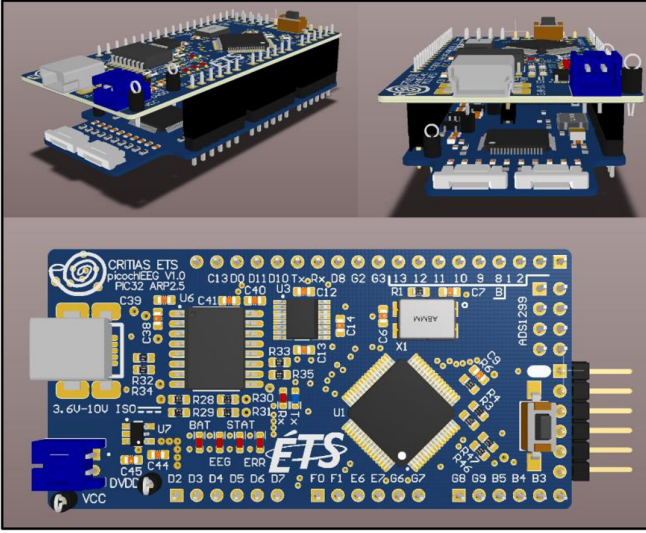


Fig. 3. 3D rendering of CochIEEG portable EEG amplifier (from [10]).

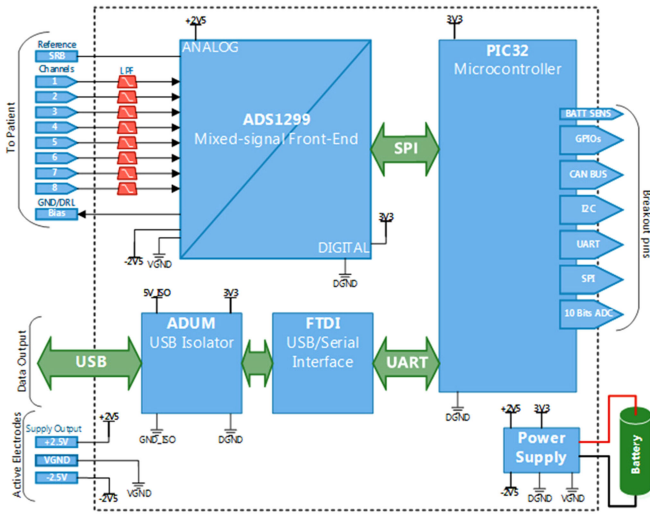


Fig. 4. CochIEEG block diagram showing the proper integration of the ADS1299 specialized chip (from [10]).

The current firmware version supports up to 4000 Hz sampling rate for 8 channels, it could support up to 16000 Hz for 8 channels pending minor hardware redesign.

CochIEEG offers highly configurable options using a custom LSL driver interface as shown in Fig. 5. Each channel is independently configurable and global system settings such as EEG reference selection, sampling rate and timestamp source can be configured. The driver acts as an LSL stream publisher. Any LSL subscriber application is then free to listen to the published streams. CochIEEG timestamps every data conversion with a microsecond precision using an internal timer on a 40 MHz bus clock to alleviate any possible data transmission timing issue. Internal timestamping of the EEG data reduces potential contamination of the signal by jitter or delay issues.

CochIEEG-recorded ASSRs were collected with sampling rates of 250, 500, 1000 and 2000 Hz. The stimulation and

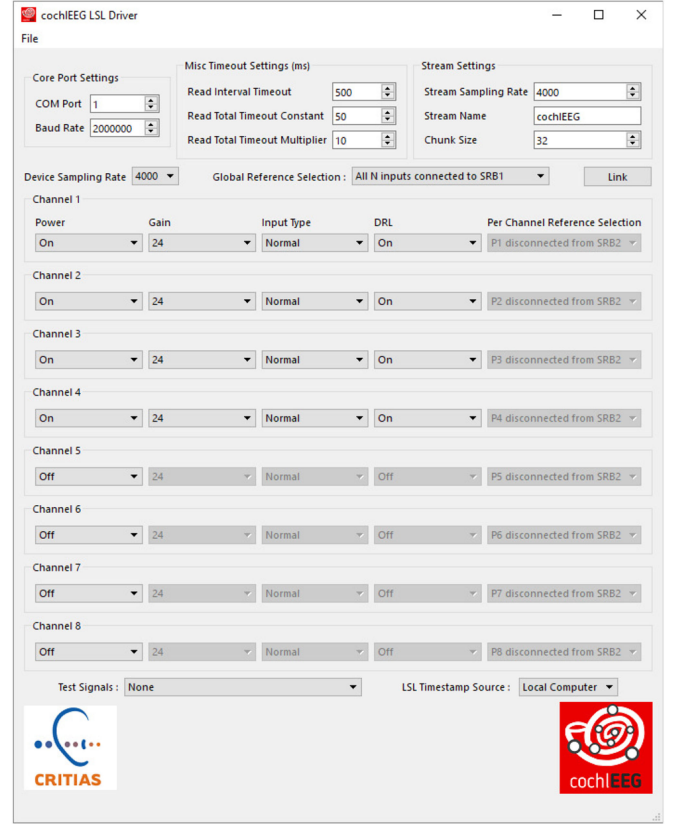


Fig. 5. Graphical User Interface (GUI) of the CochIEEG LSL driver showing the various channel configurations and streaming options.

recording were synchronized by using LSL. Data and event markers were written into a common file format (.xdf). Markers were generated in the beginning and at the end of each stimulation using LSL. Data processing was carried out offline using the same MATLAB script as for the SMARTING-recorded ASSR. Recording duration for task 3 was rigorously the same as that of tasks 1 and 2 (98.307 seconds which corresponds to 6 sweeps of 16.384 seconds each).

C. Study 1: Auditory Steady-State Responses

ASSR techniques have been largely developed to overcome the various difficulties in the assessment of hearing thresholds of very young children, older patients or those with cognitive deficits or behavioral disorders [11], [12]. ASSRs are electrophysiological responses, recorded from the human scalp, and often evoked by one or more carrier frequencies f_c that are amplitude-modulated at a specific frequency f_m . In practice, when a subject is exposed to such a stimulus, a peak in the frequency of their EEG will manifest at f_m , and may also appear at its harmonics [16].

Historically, ASSRs were first recorded at modulation frequencies near 40 Hz [13]. Since 40 Hz-ASSRs are sensitive to arousal effects, a large number of studies using ASSRs for threshold estimation have concentrated on modulation frequencies in the range of 70–110 Hz. In the case of alert/awake adults, modulation frequency at 40 Hz provides higher ASSR

TABLE II
INDIVIDUAL STIMULI CHARACTERISTICS USED TO CREATE THE FINAL STIMULI

	Stimuli parameters					
	A	f_c	θ_c	f_m	M	θ_m
#1	1	500 Hz	0	41 Hz	1	0
#2		1000 Hz				
#3		2000 Hz				
#4		4000 Hz				

amplitudes and better signal-to-noise ratios, which may enable a faster and more efficient ASSR detection [14], [15].

ASSRs have been the subject of many studies so far, however, the capability of CochIEEG to record high-quality ASSR signals is investigated in this research and the obtained results are compared with similar mobile and conventional research EEG recording systems.

1) *Stimuli*: ASSR stimuli used in this experiment consist of sinusoidal tones with the carrier frequencies of 500, 1000, 2000 and 4000 Hz that are all 100% amplitude modulated at 41 Hz. Each amplitude-modulated stimulus is created by multiplying two sine waves. The sine wave with the higher frequency is the carrier frequency f_c and the sine wave with the lower frequency forms represents the modulating envelope f_m . The full mathematical formula used to generate the stimuli $y(t)$ is given by:

$$y(t) = \frac{[A \cdot \sin(2\pi f_c t + \theta_c)] [(M \cdot \sin(2\pi f_m t + \theta_m) + 1)]}{M + 1} \quad (1)$$

Where A and M are respectively the amplitude at the carrier frequency and the amount of modulation (from 0 to 1); θ_c and θ_m are the corresponding phase angles. The final stimuli were obtained by summing the individual amplitude-modulated stimuli. Individual stimuli characteristics are listed in Table II.

Both carrier and modulation frequencies were software-adjusted automatically so that an integer number of cycles occurred within each recording section. Consequently, individual sections can be linked without acoustic artifacts and are interchangeable during artifact rejection [16]. For simplicity, the frequencies will henceforth be reported to the nearest integer value. For example, a modulation frequency of 41.016 Hz is reported as 41 Hz.

Stimuli were generated by either the MASTER system (for task 1) or MATLAB R2015b (for tasks 2 & 3) and then were amplified by an Interacoustic audiometer (model AC40) before being presented binaurally to the test-subjects using E-A-RTONE insert earphones (model 3A 410-310). Test signals were calibrated at 75 dB SPL with a Brüel & Kjaer Head and Torso Simulator (model 4128).

2) *Recordings*: All ASSR data were collected from an electrode placed at the vertex (Cz) using an electrode on the back of the neck (below the hair-line) as reference and an electrode on the clavicle as ground. Electrodes were not removed between recordings and all interelectrode impedances were below 5 k Ω at 10 Hz. Data were first recorded using the MASTER system and then SMARTING subsequently. Finally, data were collected using CochIEEG. During all these measurements, test-



Fig. 6. Subject seated in audiometric booth, wearing CochIEEG, indicated by the red circle.

subjects remained seated on a comfortable ergonomic chair inside a double-walled audiometric booth (Fig. 6).

D. Study 2: Event-Related Potentials

Event-related potentials (ERP) are electrophysiological responses that are time-locked to an event (such as the onset of a stimulus) and characterized by waveforms consisting of a series of positive and negative voltage deflections related to a set of components involved in neurocognitive processes [17].

Most of these voltage deflections are referred to by a letter indicating the polarity (N for negative and P for positive) and by a number indicating the theoretical latency in milliseconds (or the ordinal position in the waveform). For instance, the N100 (or N1) wave is the first negative deflection peaking between 80 and 120 ms after the onset of an auditory stimulus and reflects the detection of a change in the acoustic environment [18].

The P300 (or P3) wave is the largest positive deflection, peaking between 250 and 500 ms after presentation of a task-relevant stimulus and reflects processes involved in decision-making. In a classic two-stimulus oddball task, participants are asked to respond to the target stimuli with a specific action while ignoring the standard stimuli. The P300 wave is typically observed around 300 ms after the onset of a target stimulus [19]. Auditory oddball paradigms use tonal stimuli presented in random order, with the target tone occurring less frequently than the standard tone.

ERP waveforms may also be referred to with acronyms as, for instance, the mismatch negativity (MMN) which is a brain response to violations of a rule, established by a sequence of sensory stimuli (typically in the auditory domain) [20]. The MMN reflects the brain's ability to perform automatic comparisons, detecting any change in a sequence of auditory stimuli, using traces developed by the previous stimulation. In a typical

oddball task, the MMN is produced when deviant stimuli are presented in an otherwise homogeneous sequence of auditory stimuli; for instance, in a sequence of sounds “a a a a a i a a a i a a a . . .”, the deviant stimulus “i” will elicit an MMN response. Contrary to the P300, the MMN is not task-dependent and can be triggered even when the participant is passive. Both the P300 and the MMN are studied using difference waves between target and non-target stimuli, and standard and deviant stimuli respectively. This isolates the studied phenomenon or wave from the rest of the EEG activity which should be the same for each recording.

Since ERP paradigms are widely used in brain-computer interfaces (BCI) [21], the capability of CochIEEG in recording reliable ERP waves is investigated in this research to illustrate the feasibility of using the proposed EEG acquisition platform for future BCI applications. Specifically the P300 was chosen since it reflects a conscious, voluntary cognitive process.

1) *Stimuli*: Auditory oddball stimuli consist of two pure-tone sounds (1000 Hz and 2000 Hz) of 69.8 ms duration (9.9 ms rise/fall and 50 ms plateau). A total of 20 sequences of 10 tones were presented binaurally with a 2 seconds inter-stimulus interval at a participant-controlled comfortable loudness using E-A-RTONE insert earphones. The first six tones were always 1000 Hz standard tones, with a 2000 Hz target tone presented randomly at either the 7th, 8th, 9th or 10th position (standard tones were presented in the remaining non-target positions). A fixed inter-sequence interval of 4000 ms was used between recording sessions.

2) *Recordings*: Since the feasibility of using CochIEEG in ERP-based BCI applications is investigated in this study, a minimal number of electrodes was deliberately used to reproduce the limitations of acceptability of any device that is to be worn in social settings. Consequently, ERPs were recorded using the vertex (Cz) as the active electrode, the left earlobes as the reference electrode and the forehead as the ground electrode; no electrooculogram electrode was used to correct eye-blink artefacts in the EEG. All interelectrode impedances were below 5 k Ω at 10 Hz. No online filtering was applied (aside from the anti-aliasing filter implemented in the hardware) and no online rejection criteria were set. During all these measurements, test-subjects remained seated on a comfortable ergonomic chair inside a double-walled audiometric booth (see Fig. 6) and were instructed to silently count each occurrence of the target stimuli and to respond to the target stimuli by pressing a button when the target was detected.

For the analysis of the oddball data, continuous time series were band-pass filtered with a zero-phase finite impulse response filter between 0.1 Hz (−6 dB cut-off at 0.05 Hz, filter order 33000) and 20 Hz (−6 dB cutoff at 20.015 Hz, order 33000) and afterwards epoched from −200 to 700 ms and baseline corrected (−200 to 0 ms).

III. RESULTS

Fig. 7 presents the average ASSR signal-to-noise ratios (SNRs) computed on ten test-subjects for each recording

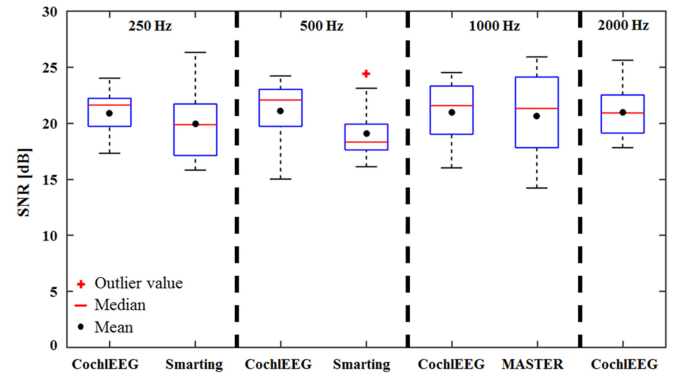


Fig. 7. Average ASSR signal-to-noise ratios, in dB, computed on ten subjects.

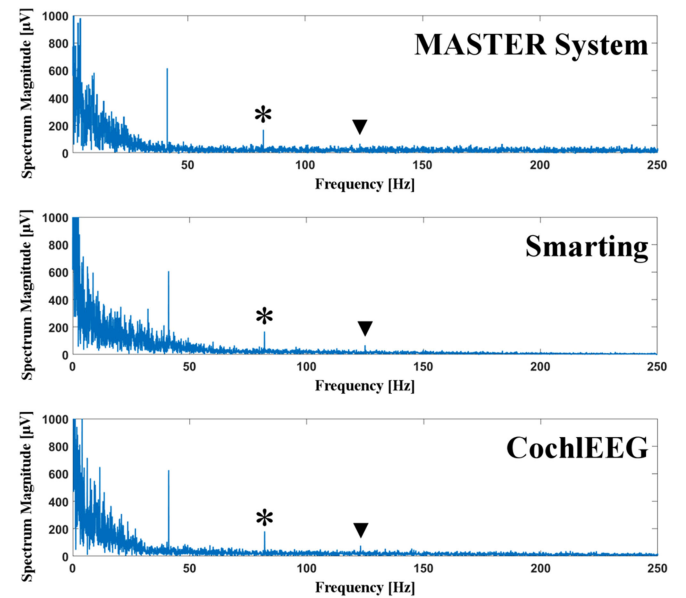


Fig. 8. Power spectrum of EEG signals recorded on subject #1 with the MASTER system (top), the SMARTING with a 500 Hz sampling frequency (middle) and CochIEEG with a 1 kHz sampling frequency (bottom). Peaks indicated with asterisks and solid triangles correspond to the second and third harmonics of the 41 Hz responses, which are particularly visible in this subject.

system. Examples of individual ASSR results recorded with the MASTER system, the SMARTING and CochIEEG are shown in Fig. 8. The grand average ERP is illustrated in Fig. 9.

The low target detection error rates for the ERP study (mean = 0.1%) demonstrates that subjects were able to easily distinguish the target stimuli from the standard stimuli during the auditory oddball experiment.

Results in Fig. 7 indicate that SNRs obtained using CochIEEG seem comparable to those obtained with the SMARTING at 250 Hz and 500 Hz. Also, SNRs obtained using CochIEEG seem comparable to those obtained with MASTER system at 1000 Hz. Furthermore, SNRs obtained using CochIEEG at 2000 Hz seem comparable to those obtained with CochIEEG at 1000 Hz, 500 Hz and 250 Hz sampling rates.

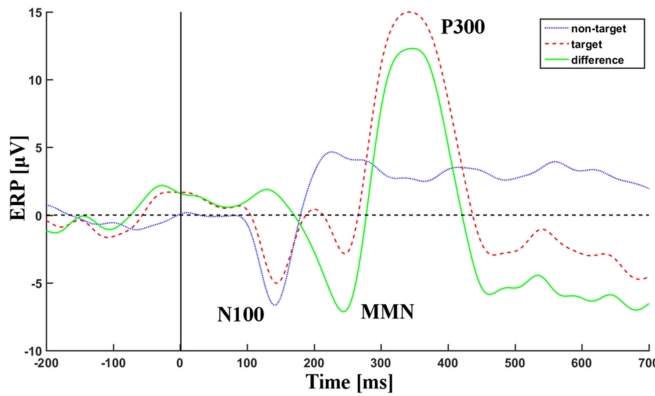


Fig. 9. Grand average ERPs ($N = 10$) observed at Cz.

These observations are confirmed by Wilcoxon tests, computed using R 3.1.0 with MASS 7.3–35 [22]. These tests fail to reject the null-hypothesis at a 5% significance level at 250 Hz for SNRs obtained using CochIEEG and SMARTING ($p = 0.241$), at 500 Hz for SNRs obtained using CochIEEG and SMARTING ($p = 0.054$) and at 1 kHz for SNRs obtained using CochIEEG and MASTER system ($p = 0.919$). The Wilcoxon tests give the same results when comparing SNRs obtained using CochIEEG at 2000 Hz and SNRs obtained using CochIEEG at 1000 Hz ($p = 0.696$), at 500 Hz ($p = 0.838$) and at 250 Hz ($p = 0.646$). A two one-sided test procedure (TOST) [23] concludes that:

- i) At 250 Hz, CochIEEG's SNRs and SMARTING's SNRs are equivalent at ± 4 dB ($p < 0.05$).
- ii) At 500 Hz, CochIEEG's SNRs and SMARTING's SNRs are equivalent at ± 5 dB ($p < 0.05$).
- iii) At 1000 Hz, CochIEEG's SNRs and MASTER system's SNRs are equivalent at ± 3 dB ($p < 0.05$).

IV. DISCUSSION

From the previous results, the fact that SNR results for CochIEEG and MASTER system are equivalent at 1000 Hz supports the idea that CochIEEG could be a suitable recording platform for ASSR. Indeed, MASTER System is a research-grade, well-established ASSR recording platform being widely used and it is accepted as accurate. Additionally, the fact that SNR results for CochIEEG and SMARTING are equivalent at 250 Hz and 500 Hz supports the idea that these two devices, based on TI's ADS1299 chip, are comparable. Furthermore, ERP results demonstrate the feasibility of using CochIEEG in ERP-based applications. As shown in Fig. 9, at Cz position, the N100 waveform is clearly identifiable and target ERPs evoked a large P300 and elicit a clear MMN response.

V. CONCLUSION AND FUTURE WORK

CochIEEG was presented in this paper as a light-weight EEG acquisition platform with the intention of enabling future innovative mobile EEG applications. The performance of CochIEEG was evaluated with a conventional ASSR recording platform (MASTER system), a mobile EEG amplifier

(SMARTING) under two electrophysiological paradigms (ERPs and ASSRs). The results prove the capability of the developed EEG data acquisition platform to reliably record good quality EEG data. CochIEEG benefits from high sampling rates (theoretically up to 16 kHz and currently tested up to 4 kHz, with an 8 kHz sampling frequency in development). These features make CochIEEG suitable for data acquisition for various applications in BCI, assistive technologies, ubiquitous healthcare and wellness, telemedicine as well as nonmedical-oriented fields such as neurogaming. Furthermore, CochIEEG's higher sampling rate (up to 4000 Hz) could lead to the development of several key applications in audiology such as objective assessment of hearing (click elicited ABR) or objective characterization of the speech processing in population with language-based learning disability (speech elicited ABR), to name a few. Nevertheless, several optimizations and improvements are required to gain access to this new realm of countless daily-life applications.

Future work should, in particular, address the following outstanding issues:

- CochIEEG is lightweight in pocket-sized packaging, easy to wear at the shoulder or clipped on a belt. However, data are currently transmitted to a computer through a USB cable. Consequently, a wireless data transmission stack should be added to CochIEEG to render it fully mobile.
- While CochIEEG has been validated with traditional wet electrodes, it has also to support the use of dry capacitive electrodes. Capacitive electrodes may have a lower sensitivity and specificity than existing wet electrodes, but they do not require the abrasion of the Stratum Corneum and the use of electrolytic gel to reduce the skin impedance, which makes them more acceptable to users in social settings [24]. Nevertheless, CochIEEG's ability to accurately and precisely record EEG signals using dry capacitive electrodes needs to be further investigated.
- Despite the recent development of a small, wireless and lightweight head-mounted EEG system [25], EEG caps are still uncomfortable to wear and not suitable for daily-life situations. Consequently, CochIEEG should be compatible and tested with the next generation of inconspicuous EEG sensors acceptable in social settings as the cEEGrid [26] or the EARtrodes [27], to name a few examples.

ACKNOWLEDGMENT

The authors would like to thank EERS Global Technologies for the technical support.

REFERENCES

- [1] S. Patel, H. Park, P. Bonato, L. Chan, and M. Rodgers, "A review of wearable sensors and systems with application in rehabilitation," *J. NeuroEng. Rehabil.*, vol. 9, no. 21, pp. 1–17, 2012.
- [2] S. Feng, M. Tang, F. Quivira, T. Dyson, F. Cuckov, and G. Schirner, "EEGu2: An embedded device for brain/body signal acquisition and processing," in *Proc. 27th Int. Symp. Rapid Syst. Prototyping, Shortening Path Specification Prototype*, 2016, pp. 19–25.
- [3] K. K. M. Rahman and M. Nasor, "Multipurpose low cost bio-daq system for real time biomedical applications," in *Proc. Int. Conf. Inf. Commun. Technol. Res.*, 2015, pp. 286–289.

- [4] G. Dufort *et al.*, "Wearable EEG via lossless compression," in *Proc. 38th Annu. Int. Conf. IEEE Eng. Med. Biol. Soc.*, 2016, pp. 1995–1998.
- [5] A. Melnik *et al.*, "Systems, subjects, sessions: To what extent do these factors influence EEG data?" *Front. Human Neurosci.*, 30 Mar. 2017. [Online]. Available: <https://doi.org/10.3389/fnhum.2017.00150>
- [6] M. De Vos, M. Kroesen, R. Emkes, and S. Debener, "P300 speller BCI with a mobile EEG system: Comparison to a traditional amplifier," *J. Neural Eng.*, vol. 11, no. 3, pp. 1–8, 2014.
- [7] M. S. John, A. Dimitrijevic, and T. W. Picton, "MASTER: A Windows program for recording multiple auditory steady state responses," *Comput. Methods Programs Biomed.*, vol. 61, pp. 125–150, 2000.
- [8] N. Bigdely-Shamlo *et al.*, "Hierarchical event descriptor (HED) tags for analysis of event-related EEG studies," in *Proc. IEEE Global Conf. Signal Inf. Process.*, 2013, pp. 1–4. [Online]. Available: <https://doi.org/10.1109/GlobalSIP.2013.6736796>
- [9] A. Delorme and S. Makeig, "EEGLAB: An open source toolbox for analysis of single-trial EEG dynamics including independent component analysis," *J. Neurosci. Methods*, vol. 15, no. 134, pp. 9–21, 2004, doi: 10.1016/j.jneumeth.2003.10.009.
- [10] M. Ducharme, "Développement d'une plateforme de recherche portable pour électroencéphalographie intra- et circum-auriculaire," Master's thesis, École de technologie supérieure - Université du Québec, Montreal, QC, Canada, 2018.
- [11] B. Cone-Wesson, R. C. Dowell, D. Tomlin, G. Rance, and W. J. Ming, "The auditory steady-state response: Comparisons with the auditory brainstem response," *J. Amer. Acad. Audiol.*, vol. 13, pp. 173–183, 2002.
- [12] T. W. Picton, M. S. John, A. Dimitrijevic, and D. Purcell, "Human auditory steady state responses," *Int. J. Audiol.*, vol. 42, pp. 177–219, 2003.
- [13] R. Galambos, A. Makeig, and P. J. Talmachoff, "A 40-Hz auditory potential recorded from the human scalp," *Proc. Nat. Acad. Sci. USA*, vol. 78, no. 4, pp. 2643–2647, 1981.
- [14] A. Dimitrijevic, M. S. John, P. van Roon, and T. W. Picton, "Human auditory steady-state responses to tones independently modulated in both frequency and amplitude," *Ear Hear*, vol. 22, pp. 100–111, 2001.
- [15] A. Van Maanen and D. R. Stapells, "Comparison of multiple auditory steady state responses (80 versus 40 Hz) and slow cortical potentials for threshold estimation in hearing-impaired adults," *Int. J. Audiol.*, vol. 44, pp. 613–624, 2005.
- [16] M. S. John, O. G. Lins, B. L. Boucher, and T. W. Picton, "Multiple auditory steady-state responses (MASTER): Stimulus and recording parameters," *Audiology*, vol. 37, pp. 59–82, 1998.
- [17] S. J. Luck and E. S. Kappenman, *The Oxford Handbook of Event-Related Potential Components*. London, U.K.: Oxford Univ. Press, 2012.
- [18] R. Näätänen and T. Picton, "The N1 wave of the human electric and magnetic response to sound: A review and an analysis of the component structure," *Psychophysiology*, vol. 24, no. 4, pp. 375–425, 1987.
- [19] E. Donchin and M. G. Coles, "Is the P300 component a manifestation of context updating?" *Behav. Brain Sci.*, vol. 11, pp. 357–427, 1988.
- [20] R. Näätänen and I. Winkler, "The concept of auditory stimulus representation in cognitive neuroscience," *Psychological Bull.*, vol. 125, pp. 826–859, 1999.
- [21] B. Graimann, B. Allison, and G. Pfurtscheller, *Brain-Computer Interfaces*. Berlin, Germany: Springer, 2010.
- [22] R Development Core Team, *R: A Language and Environment for Statistical Computing*. Vienna, Austria: R Foundation for Statistical Computing, 2014, ISBN 3-900051-07-0. [Online]. Available: <http://www.R-project.org/>
- [23] D. J. Schuurmann, "A comparison of the two one-sided tests procedure and the power approach for assessing the equivalence of average bioavailability," *J. Pharmacokinet Biopharm.*, vol. 15, pp. 657–80, 1987.
- [24] C. T. Lin, L. D. Liao, Y. H. Liu, I. J. Wang, B. S. Lin, and J. Y. Chang, "Novel dry polymer foam electrodes for long-term EEG measurement," *IEEE Trans. Biomed. Eng.*, vol. 58, no. 5, pp. 1200–1207, May 2011.
- [25] C. Kranczioch, C. Zich, I. Schierholz, and A. Sterr, "Mobile EEG and its potential to promote the theory and application of imagery-based motor rehabilitation," *Int. J. Psychophysiol.*, 2013. [Online]. Available: <http://dx.doi.org/10.1016/j.ijpsycho.2013.10.004>
- [26] S. Debener, R. Emkes, M. De Vos, and M. Bleichner, "Unobtrusive ambulatory EEG using a smartphone and flexible printed electrodes around the ear," *Sci. Rep.*, vol. 5, pp. 1–11, 2015, Art. no. 16743.
- [27] O. Valentin, G. Viallet, and J. Voix, "EARtodes: Towards a wireless in-ear custom fitted brain computer interface," *Can. Acoust.*, vol. 45, no. 3, pp. 142–143, 2017.



Olivier Valentin received the bachelor's degree in biomedical engineering from University Claude Bernard Lyon I, Villeurbanne, France, in 2007, the master's degree in biomedical engineering from École Polytech Lyon, Villeurbanne, France, in 2010, and the Ph.D. Doctorate degree in engineering from École de technologie supérieure, Montreal, QC, Canada, in 2016. In 2016, he joined the Canada-based NSERC-EERS Industrial Research Chair in In-Ear Technologies (CRITIAS) as a Postdoctoral Researcher to develop a wireless EEG-based BCI system able to both tolerate natural movement and record brain signals. He is currently a Postdoctoral Researcher with the Groupe d'Acoustique de l'Université de Sherbrooke, Sherbrooke, QC, Canada. His research interests include brain computer interfaces, EEG, and acoustics.



Mikaël Ducharme received the B.Eng. and M.Sc. degrees in electrical engineering from the École de technologie supérieure (ÉTS), Montréal, QC, Canada. He is currently a part-time Teacher with the ÉTS and a full-time Engineer with Effenco, Montreal, QC, Canada, working on transportation connectivity, electrification, and automation. His research interests include low-noise electronic design, data analysis, signal processing, biomedical instrumentation, and IoT.



Gabrielle Crétot-Richert received the bachelor's degree in biomedical engineering and the master's degree in technological project management in 2015 from the Polytechnique School of Montréal, Montreal, QC, Canada. She is currently working toward the Ph.D degree in health technologies with the Department of Mechanical Engineering, École de Technologie Supérieure, Montréal, QC, Canada. Her research interests include electroencephalography, signal acquisition and processing in biomedical devices, machine learning, and biomedical system engineering.



Hami Monsarrat-Chanon received the graduate diploma degree under the supervision of Prof. J. Voix and is currently a Research Associate with CRITIAS. He has more than 15 years of professional experience within R&D teams of small companies. He worked on various successful projects ranging from medical apparatus to utility instrumentation systems. His primary field of action is embedded software development. He is also active in the areas of electronic development as well as system engineering. He is currently working on audio and biosignal applications and hopes to learn more about how nature accomplishes its engineering tasks.



Guilhem Viallet received the Ph.D. degree from the Department of Mechanical Engineering, École de technologie supérieure (ÉTS), Montréal, QC, Canada, in 2014. He is currently a Postdoctorate Fellow with the NSERC-EERS Industrial Research Chair in In-Ear Technologies (CRITIAS), ÉTS. His research interests include acoustic modeling and instrumentation, developing in-ear device prototypes by additive manufacturing and having a better understanding of three-dimensional printed materials.



been with École polytechnique de Montréal, Montreal, QC, Canada, since 2014. His research interests are in the area of vibrations, dynamics, and microelectromechanical systems.

Aidin Delnavaz received the B.Sc., M.Sc., and Ph.D. degrees from the Sharif University of Technology, Tehran, Iran, in 2002, 2004, and 2010 respectively, all in mechanical engineering. Since 2010, he has been with the EERS-ÉTS Industrial Research Chair in In-ear Technologies, where he is currently an Associate Researcher. He is currently working on integrated in-ear sensing systems and energy harvesting devices. He is also a Lecturer with the Department of Mechanical Engineering, École de technologie supérieure (ÉTS), Montreal, QC, Canada, and has



industrial Research Chair in In-Ear Technologies (CRITIAS). Together with a team of talented and motivated researchers, he works on the development of leading-edge technology combining in-ear instrumented hardware platforms with audio signal processing and biosignal extraction algorithms to enable its industrial partner, EERS Global Technologies, Inc., to commercialize in-ear wearables for hearing protection and augmentation, two-way communication, and brain-computer interfaces for industrial, military, consumer, and medical markets.

Jérémie Voix received the master's degree in fundamental physics from the Université des Sciences et Technologies de Lille, Villeneuve-d'Ascq, France, in 1995, the master's degree in applied sciences in acoustics from the Université de Sherbrooke, Sherbrooke, QC, Canada, in 1997, and the Ph.D. Doctorate degree in engineering—awarded with great distinction—from the École de technologie supérieure (ÉTS), Montreal, QC, Canada, in 2006. Since 2010, he has been a Professor with the ÉTS and currently leads the Canada-based NSERC-EERS In-