


1. Model Overview

Run ID:	85f2af052f4d4987975279386707ad6f
Timestamp:	2026-05-13 17:25:01.779938
Owner:	Applied AI Engineer
Intended Use:	FDA Class II Medical Device Diagnostic

2. Quantitative Performance

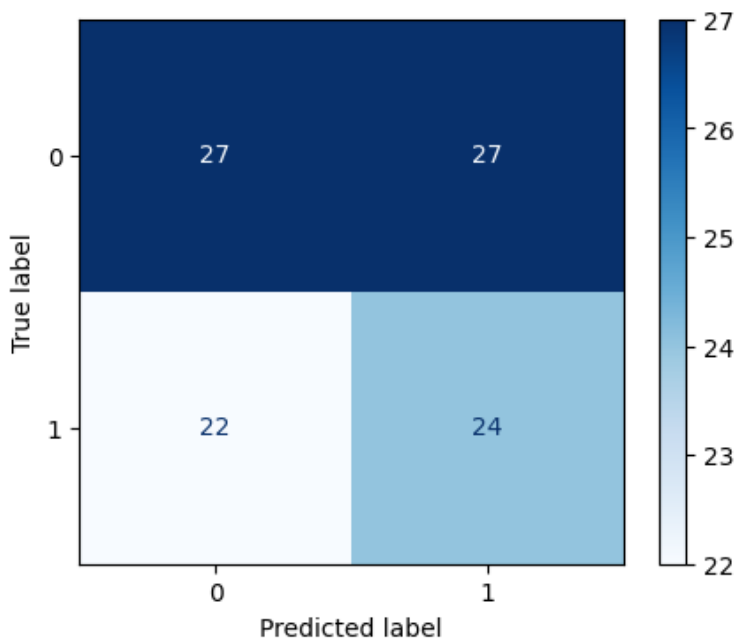

3. Slicing Analysis (Bias Check)

Group	Accuracy	Recall	Count
Age: 18-35	0.5405	0.4375	37
Age: 36-60	0.6000	0.6111	30
Age: 60+	0.3939	0.5000	33