


Native baseline absorbs gradual contact; unloading triggers the deviation guard
v5_6 NFE1/K4 · start1787396273 · seed903101

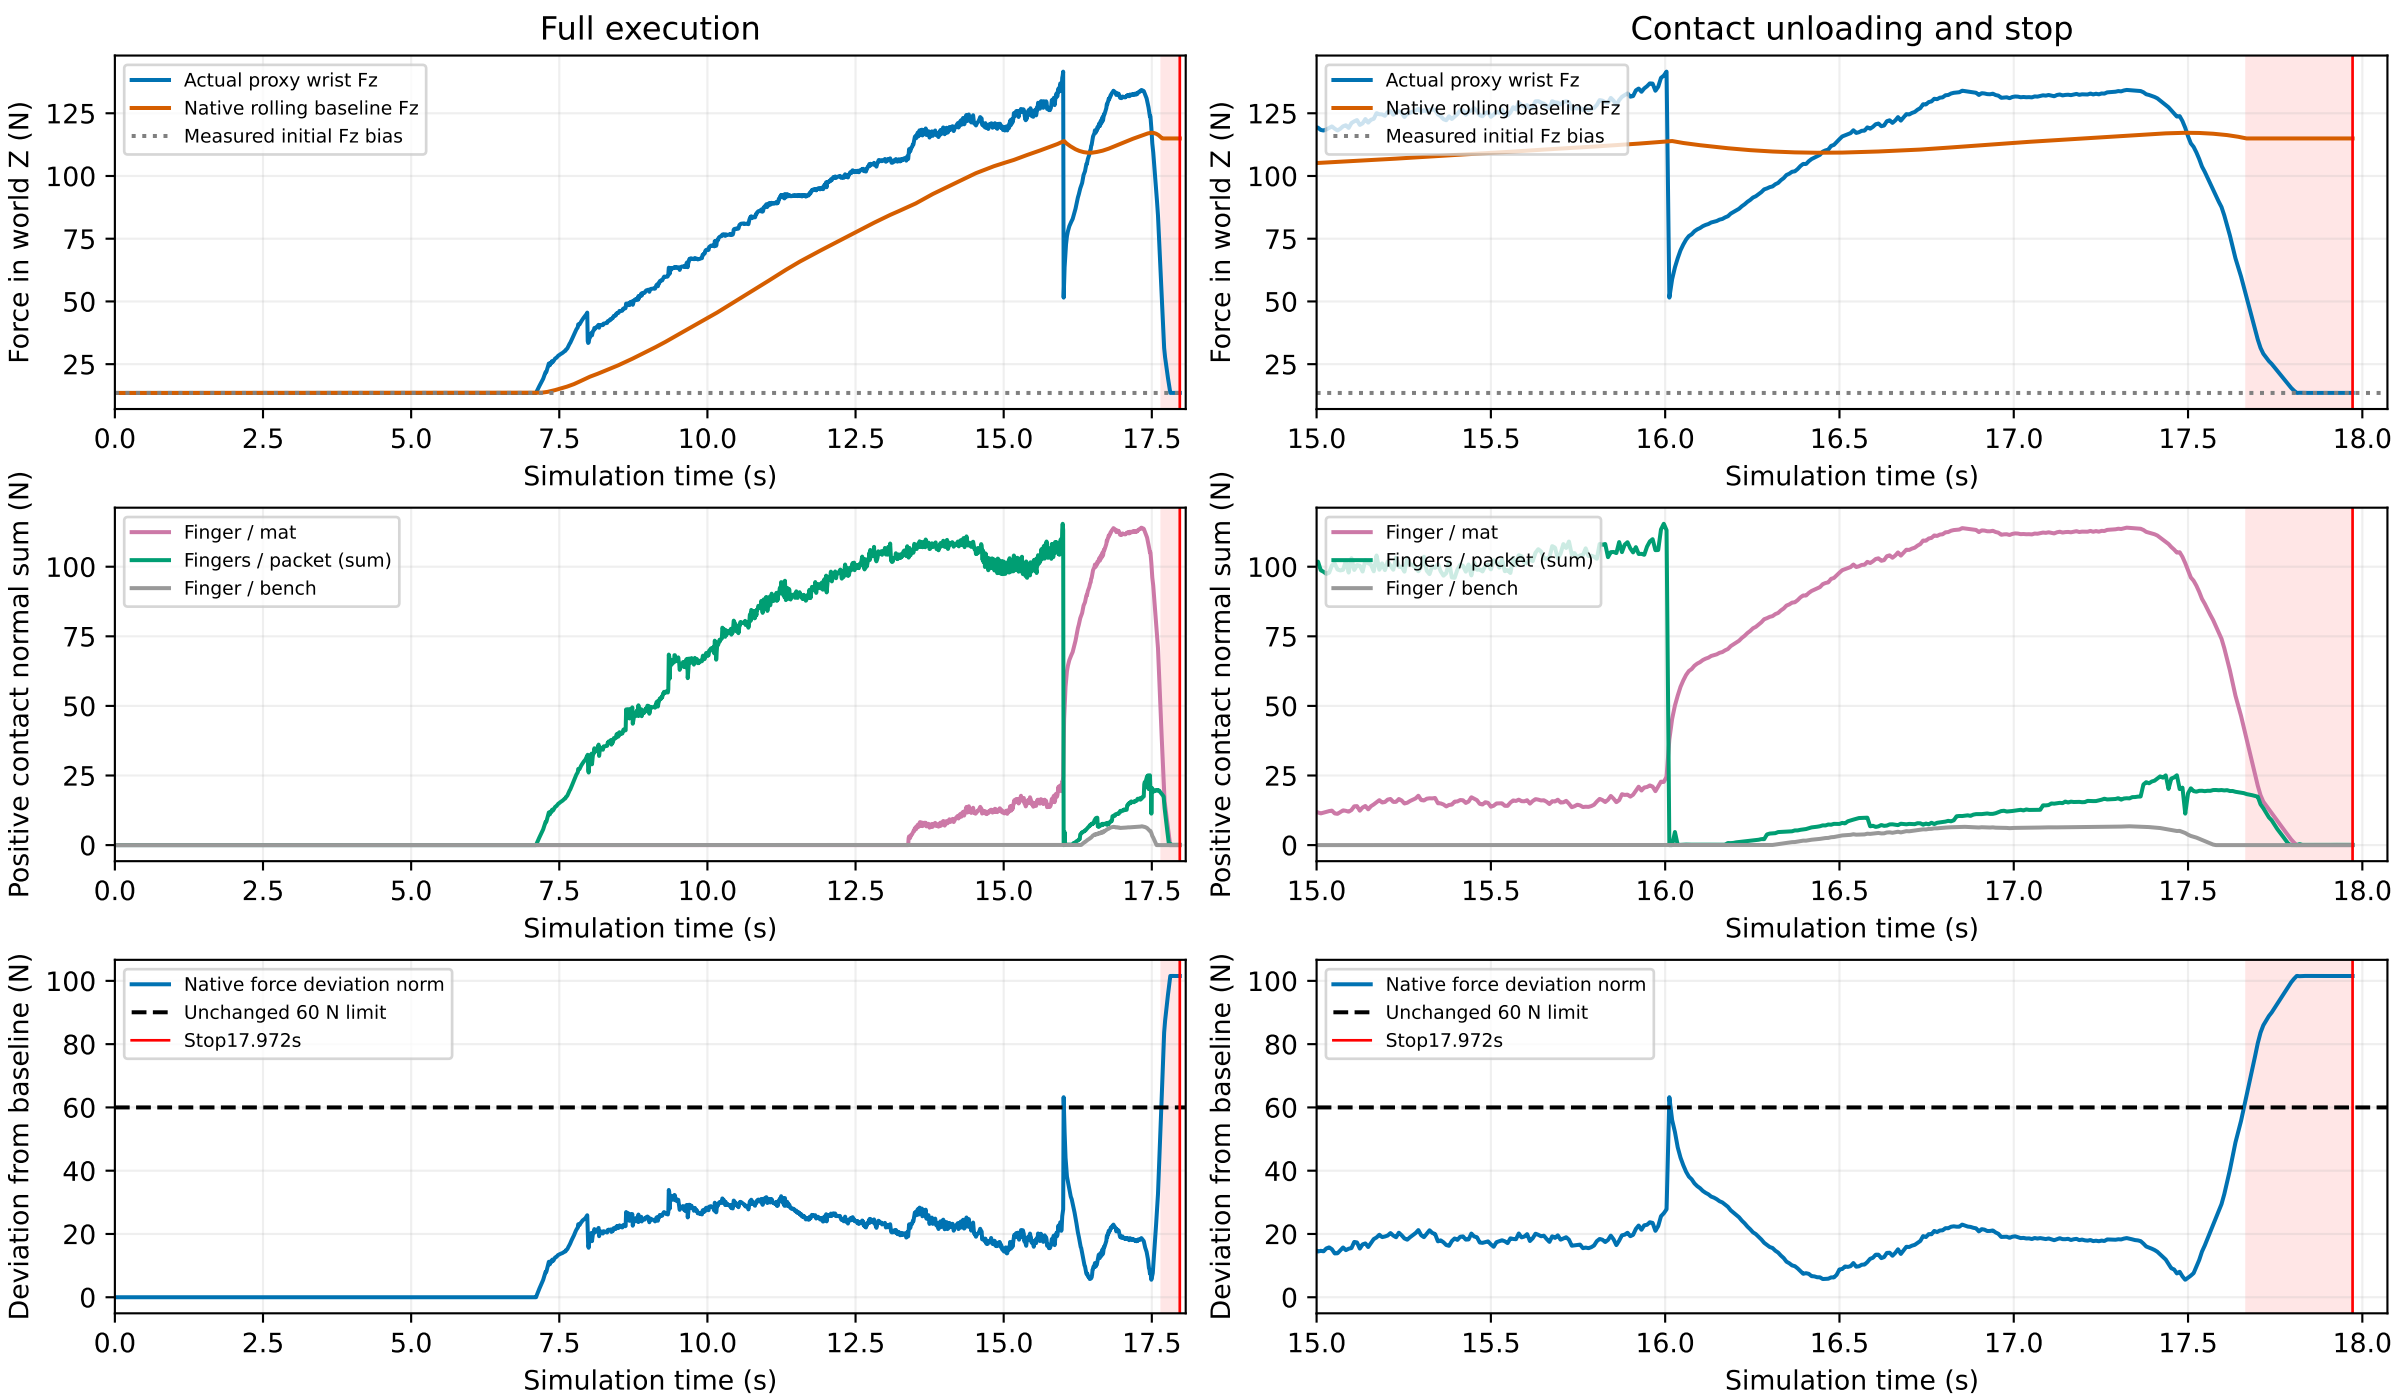

Actual frozen trial; unchanged EMA2s, 60N /15N m limits, 0.3s debounce. Contact proxy is not a calibrated UR3 wrist sensor.