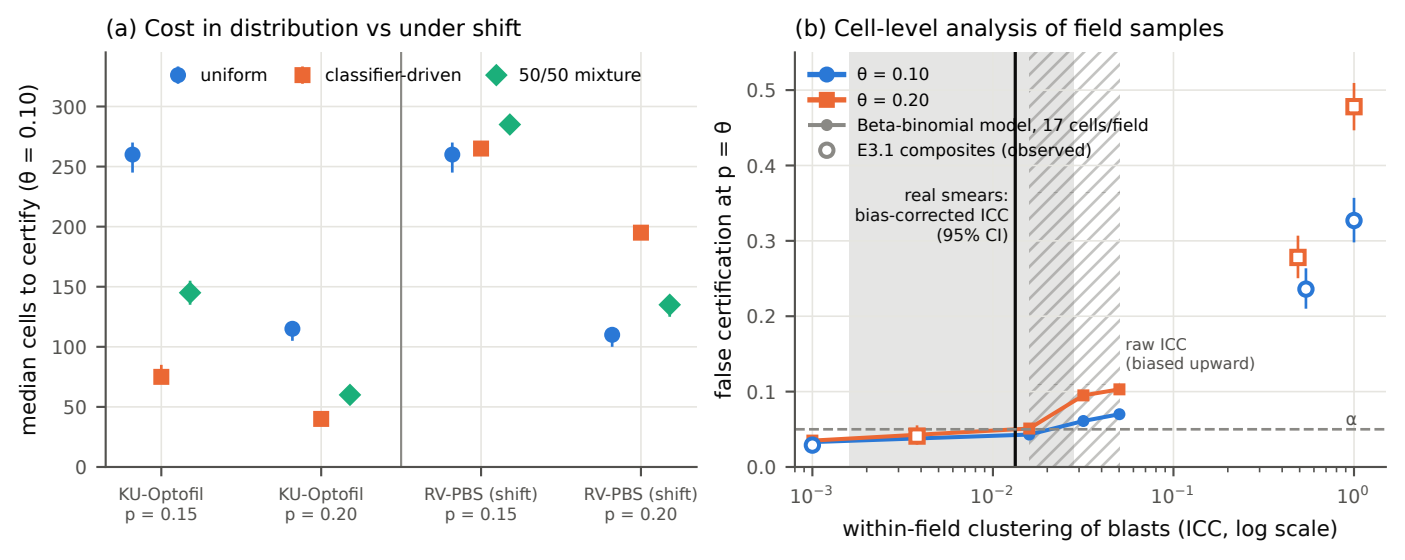
(a) Cost in distribution vs under shift
uniform
classifier-driven
50/50 mixture
median cells to certify (θ = 0.10)
300
250
200
150
100
50
0
KU-Optofil
p = 0.15
KU-Optofil
p = 0.20
RV-PBS (shift)
p = 0.15
RV-PBS (shift)
p = 0.20
(b) Cell-level analysis of field samples
θ = 0.10
θ = 0.20
Beta-binomial model, 17 cells/field
E3.1 composites (observed)
real smears:
bias-corrected ICC
(95% CI)
raw ICC
(biased upward)
α
false certification at p = θ
0.5
0.4
0.3
0.2
0.1
0.0
10⁻³
10⁻²
10⁻¹
10⁰
within-field clustering of blasts (ICC, log scale)