

A Transient sensory-current response



B Antagonist-BPA knee

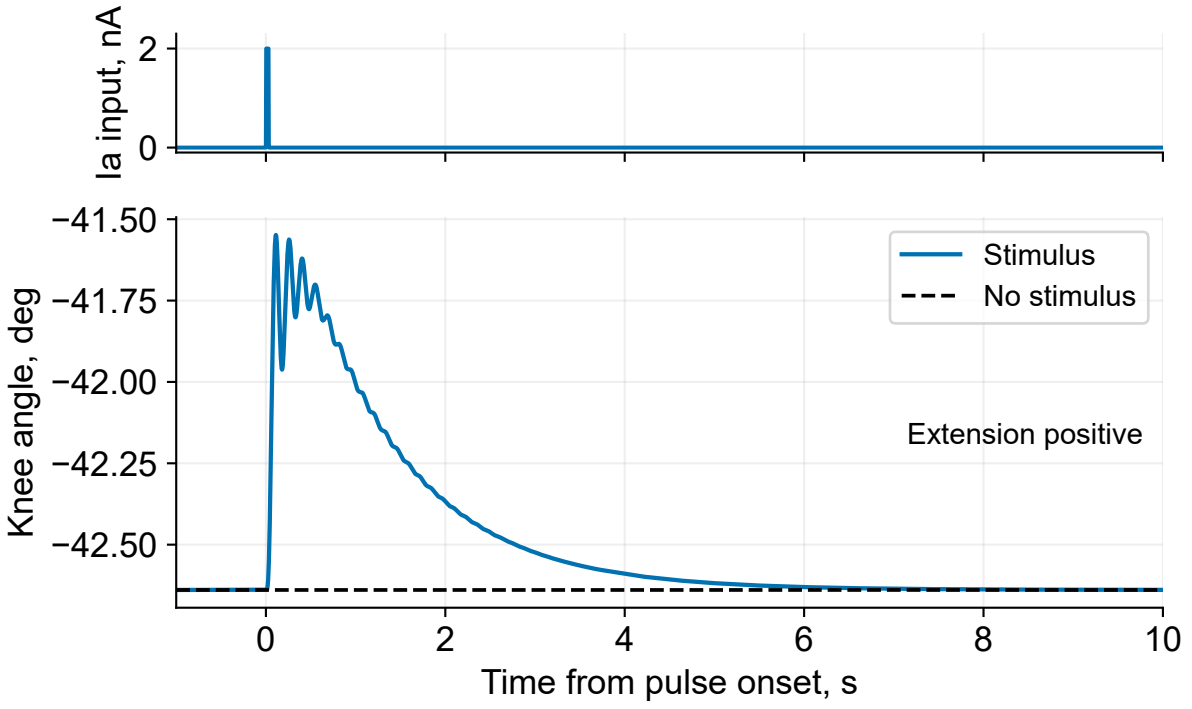

C Implemented knee feedback connections

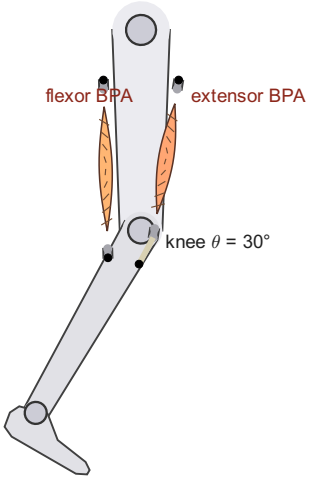