

1 Active PZW/BDE Comparison

1.1 Overview

The active PZW/BDE comparison within the HYDRA system environment is a function enabling the best possible comparison of personal BDE postings ("B" records) with the personal and calculated time intervals of PZW on a daily level. In general, the PZW posting is foremost; the personal BDE posting depends on the wage type postings of the PZW labor time calculation.



The active comparison is initially not active in a standard HYDRA system. It is only set up and activated in the HYDRA system by MPDV staff if required. The activation is described in section [Activating the Environment Variable](#).

1.2 PZW Data


The wage type postings and labor time recording provide the basis for the PZW/BDE comparison. The clock-in/clock-out data originate from recording at the terminal. Such clockings are synchronized in the course of labor time calculation according to the applicable time model of the relevant employee.

The results of labor time calculation are employee and day-related time intervals posted to wage types. The prerequisite for the PZW-BDE comparison is the error-free result of the PZW labor time calculation. A correct system result is obtained when HYDRA is able to generate a daily result on the basis of the available clock-in and clock-out data. If clocking-in or clocking-out is forgotten, the labor time calculation cannot obtain a daily result. This error is identified as requiring correction in the PZW posting list.

PZW result:

Matching clockings (not relevant for the active comparison BDE/PZW)

Date	Person	In	Out	In (evaluated)	Out (evaluated)	Duration
22-OCT	P 1	6:53	16:05	7:00	16:00	8.25 hrs

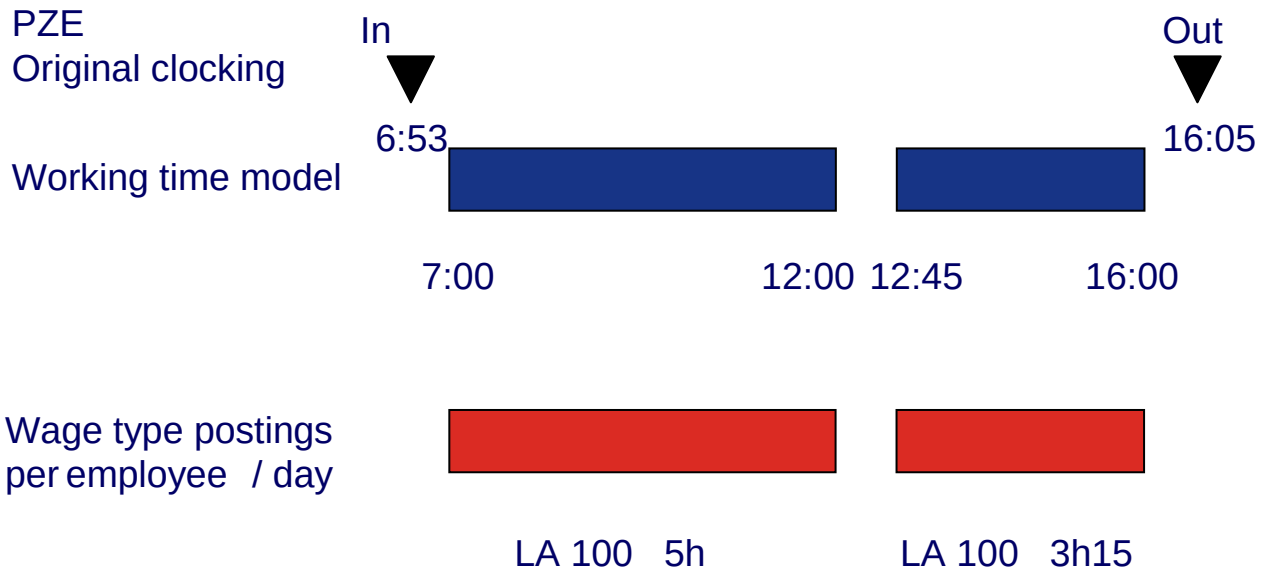

Wage type postings

Date	Person	Start	End	Duration
10/22	P1	7:00	12:00	5.00 hrs
10/22	P1	12:45	16:00	3.15 hrs

Note:

The time interval between clock-in and clock-out is transferred to two wage type postings by labor time calculation on the basis of the planned break. For comparison, the wage type postings are relevant.

The existing correct system result may nevertheless be "incorrect" in terms of the contents if the employee has clocked incorrectly.

1.3 BDE Data

Identifying the duration of a BDE posting

When the employee logs off, the BDE postings (B records) are created online. The time for the posting is calculated using the times of logon and logoff. To calculate this duration, only the time intervals are used that are defined in the shift model. Breaks and time intervals that are outside the defined shift, are not used to calculate the duration. The basic settings specify if the system uses the shift model of the workplace, which created the posting, or the BDE shift model of the person.


Resource performance accounts with reference to machine status

The personal posting depends on the machine status progress during the employee logon time. The times of individual machine statuses are balanced in the relevant resource performance accounts.

Proportionate identification of the duration with logon to several machines or operations

HYDRA takes account of multiple assignments of employees to orders as well as of multiple machine operation. With regard to any employee-related BDE posting, the so-called labor duration is allocated proportionately:

- If a person is generally only logged on to one operation, the interval of the posting is equal to the proportionate labor duration.
- If a person is logged on to more than one operation, the interval between the person's logon and logoff will exceed the proportionate labor duration, because in the case of parallel allocations of persons to several orders, HYDRA will divide the time by the number of simultaneous order allocations.
- Breaks in the BDE time model are always taken account of and excluded from the posting.

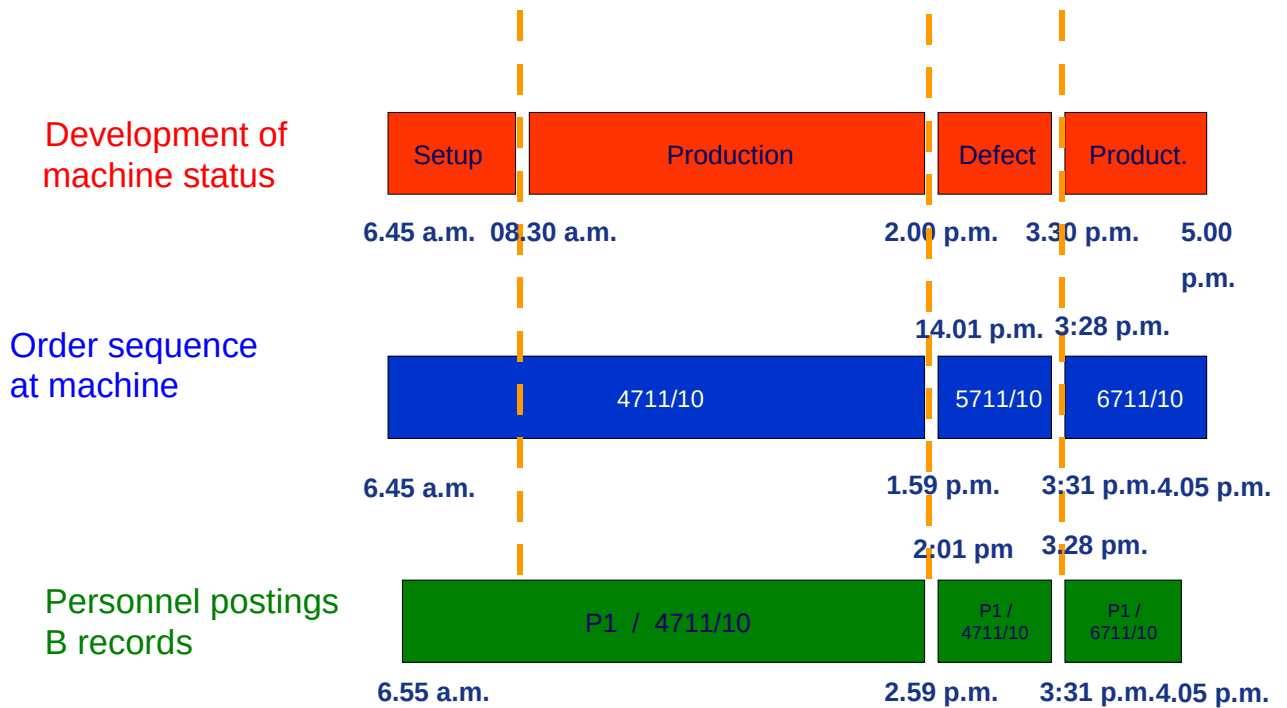

BDE result (before comparison):

Date	Person	Order	Duration	RPA	Person logon	Person logoff	Personnel time
22.10.	P 1	4711/10	7.14 h	7=1:45 h 11=5:29 h	6:55	13:59	7.04 h
22.10.	P 1	5711/10	1.27 h	2=1:27 h	14:01	15:28	1.27 h
22.10.	P 1	6711/10	1.29 h	11=1:29 h	15:31	16:05	0.34 h

1.4 Active Comparison Procedure

1.4.1 Comparison of recorded and/or maintained BDE personnel postings

The PZW-BDE comparison is started automatically after the PZW labor time calculation and processes the personal BDE postings of persons and days evaluated by the labor time calculation. The PZW-BDE comparison processes both results generated for the first time and corrected results of labor time calculation.

The PZW-BDE comparison compares the PZW wage type postings with the personal BDE postings ("B" records) of the employee and makes the following corrections.


- The start and end times of the employee's PZW posting are foremost. The PZW-BDE comparison uses any relevant wage type posting of a day (e.g. the wage type posting from before noon between 07:00 AM - 12:00 AM and the wage type posting from the afternoon between 1:00 PM and 5:00 PM) and searches for the associated personal BDE postings relating to the wage type posting period. The BDE postings may start earlier or later and end during or after the wage type posting.
- Note:
Only BDE postings are used that are made up to two hours before or after the PZW wage type postings. If a clock-out has been forgotten and to prevent these long durations from falsifying the result, the system only uses the postings made within an interval of up to 10 hours before or after the PZW wage type postings. BDE postings, which are even further outside the PZW wage type postings, must be edited manually.
- Example: the PZW wage type postings cover the time from 6:00 to 14:00.
 - A BDE posting from 15:30 to 18:00 is booked, the duration is set to 0.
 - A BDE posting from 16:10 to 18:00 is not booked because this posting starts later than two hours after 14:00. The duration is not changed.
 - A BDE posting from 15:30 to 1:00 of the next day is not booked because this posting ends more than 10 hours after 14:00. The duration is not changed.

- In HYDRA-PZW it is possible to configure whether a wage type is relevant for the active comparison. Time intervals not posted to appropriately identified wage types are excluded in the BDE postings. This is of interest, for example, for break times which are to be remunerated in PZW but excluded in BDE. If several wage types are identified as relevant, they can also overlap. Overlapping wage type postings are scaled to one single time scale during comparison.
- BDE times **not** covered by any relevant PZW wage type posting are not valid in terms of the PZW-BDE comparison and are excluded from the duration of the BDE posting. This means that the PZW-BDE comparison can always *only reduce* the personal BDE postings and will *never increase* them.
- **If no relevant PZW wage type postings are available**, the BDE times are not changed. The comparison is only made if relevant PZW wage type postings exist for the person on the specified day.
This way, the actually recorded BDE times are not set to a duration of 0 with persons who generally do not use PZW or who have no relevant wage type postings on this day because of a clocking or planning error in the PZW.
- The comparison will change the following values of the personal BDE posting (B record):
Personal resource performance account HNZ (RPA11) = synchronized proportionate labor duration
Labor duration = synchronized proportionate labor duration
Order-related resource performance account HNZ = synchronized labor duration, not proportionate
Sum total of order-related RPA = synchronized labor duration, not proportionate
The personal and order-related RPA01, RPA02, RPA03, RPA04, RPA05, RPA06, RPA07, RPA08, RPA09, RPA10, RPA12 are set to 0.
The terminal number of the posting is set to 999.
The posting is signed off, the originator is set to "PZADE".
- Start and end times are retained
The original posting times of the personal BDE posting ("B record") are retained. The correction only affects the duration and the labor duration.

- Proportionate posting of labor utilization

The proportionate labor utilization times of the personal BDE posting are again determined in relation to the existing simultaneous order processing by the PZW-BDE comparison. With regard to merged operations, too, the labor time is divided by the number of simultaneously processed operations and is equally allocated to these operations.

As with normal entries, the order-related resource performance accounts and their time total are not calculated proportionately.

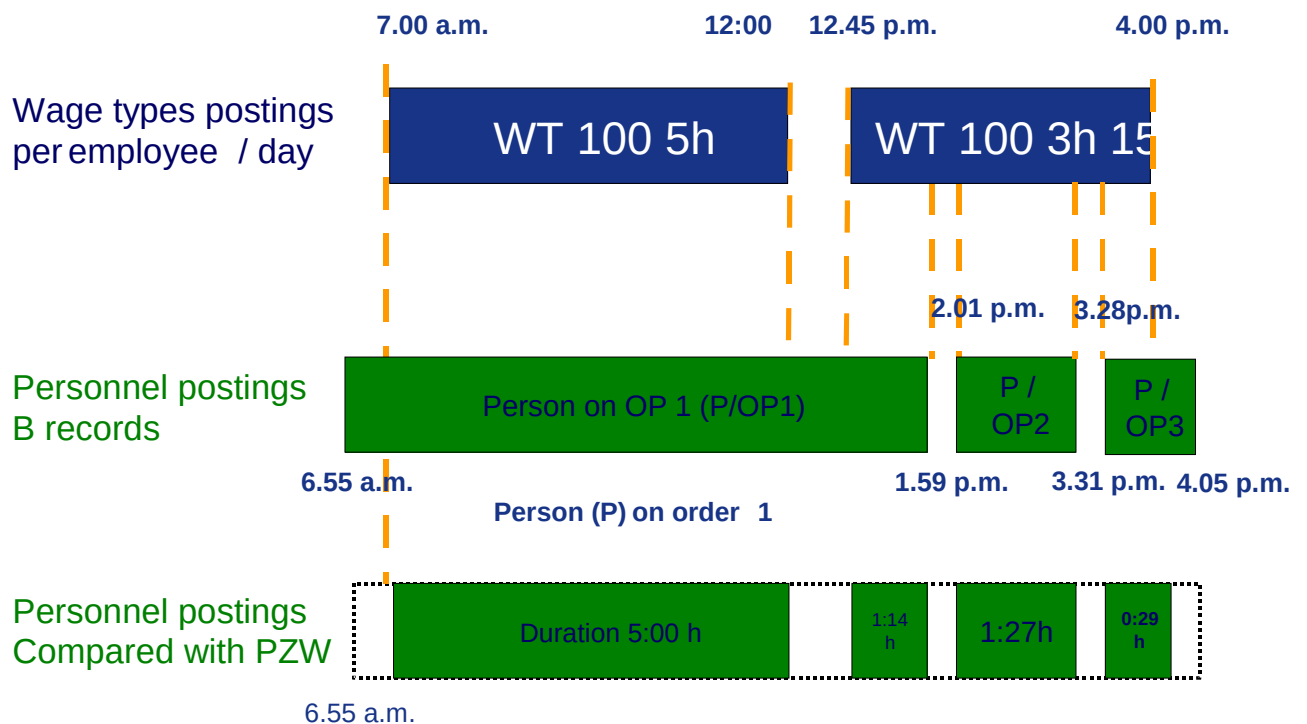

PZW-BDE Comparison Result:

The data in the table below refer exclusively to the date 10/22 and person P1.

Start	End	Order	Log person on	Log person off	Labor dur.	Start (synchronized)	End (synchronized)	Labor duration (synchronized)
7:00 AM	12:00 PM	4711/10	6:55 AM	1:59 PM	7:04 hrs	7:00 AM	12:00 PM	5:00 hrs
12:45 PM	4:00 PM	4711/10	6:55 AM	1:59 PM	7:04 hrs	12:45 PM	1:59 PM	1:14 hrs
		4711/10	6:55 AM	1:59 PM	6:14 hrs			

12:45 PM	4:00 PM	5711/10	2:01 PM	3:28 PM	1:27 hrs	2:01 PM	3:28 PM	1:27 hrs
		5711/10	2:01 PM	3:28 PM	1:27 hrs			
12:45 PM	4:00 PM	6711/10	3:31 PM	4:05 PM	0:34 hrs	3:31 PM	4:00 PM	12:29 AM hrs
		6711/10	3:31 PM	4:05 PM	0:29 hrs			

The PZW-BDE comparison result is represented by the personal BDE postings in bold type not highlighted in color. The start and end times from the original BDE posting are retained, but the labor duration is synchronized with the evaluated PZW times of the person.

Please note:

- The PZW-BDE comparison does not process the order-related BDE postings ("U records" and "E records").
- A button can be used to set whether or not manually modified BDE postings ("B records") are processed by the PZW-BDE comparison.
- With regard to the processed B records, the originator PZADE is entered in the posting. In addition, the comparison signs off the posting.
- Gaps occurring in the posting sequence between the logons and logoffs of persons can be avoided by activating the waiting period processing in the HYDRA setup.

1.4.2 Closing Gaps

Similar to BDE waiting period processing, gaps between BDE personnel postings may be filled by waiting period orders in the comparison.

The waiting period order must be entered in the HYDRA basic settings.

Gap filling by waiting period orders is activated by MPDV staff through an INI configuration.

Optionally, the gap between PZW start and the first BDE personnel posting or the last gap between the last BDE personnel posting and PZW end can each be filled by separate waiting period operations. This is also activated by MPDV staff through an INI configuration.

Rules for closing gaps

1. The persons relevant for gap filling are those who have the "PZW/BDE comparison" option activated in the HR master data ("BDE" tab, "Incentive payment data" group).
2. Days on which no BDE personnel posting is available at all will also be filled for the relevant persons.
3. The PZW times relevant for gap filling are derived from the PZW definition of wage types. In this regard, the identifier "Use wage type for BDE comparison" is decisive, as it is for comparing personnel postings. Wage types must be maintained appropriately so that, for example, absence times such as holidays are not relevant for gap filling.
4. Gap filling will not result in any BDE order postings (record types U/E). No U/E records will be created upon subsequent comparison, either.
5. Long running BDE personnel postings may occur, for example, from maintenance or posting errors. Such postings are always only assigned to a defined PZW evaluation date if HYDRA time management is used. This is the last possible date of PZW evaluation. (Same assignment as in the comparison list and the subsequent entry via the "PZW evaluation date" column.)
6. Intentional gaps in the BDE timeline are not possible if gap filling is used, since they will always be filled automatically. If gaps are specifically requested in production orders, such gaps must be filled by the employee or the person in charge by posting at the terminal or by means of manual maintenance, e.g. by inserting an overhead costs posting. Alternately, a gap may be created in the PZW times relevant for comparison by selecting an appropriate payment day type in PZW or by manually processing the wage type postings.

1.4.2.1 Closing Gaps in Mode WAITINGPERIODOP

To close gaps, you always use fixed orders specifically configured in mode WAITINGPERIODOP. Usually, the waiting period OP is used, which is stored in the HYDRA basic settings.

To close the gap between PZW start and the first BDE personal posting and to close the last gap between the last BDE personnel posting and the PZW end, separate waiting period OPs can optionally be used. An MPDV consultant can activate this option via INI configuration.

Special rules for closing gaps in mode WAITINPERIODOP

1. The personnel postings are used to close gaps, these postings include the workplace where the person has last been logged on before the gap. If no previous BDE postings of the person are found, then the waiting period posting includes the machine that follows after the gap. If no machine can be identified this way, the gap is not closed. This is recorded in a log file. This can happen with persons who are new.

The following examples describe how the "close gap" function works.

Legend:



→ PZW posting




→ entered BDE posting (B record) PO: Production order



→ Overhead cost order start (gaps between clock-in and first BDE login INI-configuration FIRSTOP)




→ Overhead cost order end (gaps between last BDE posting and clock-out INI-configuration LASTOP)




→ Overhead cost order (gaps between BDE postings Setup – Waiting period processing – Posting to OP)

Example 1

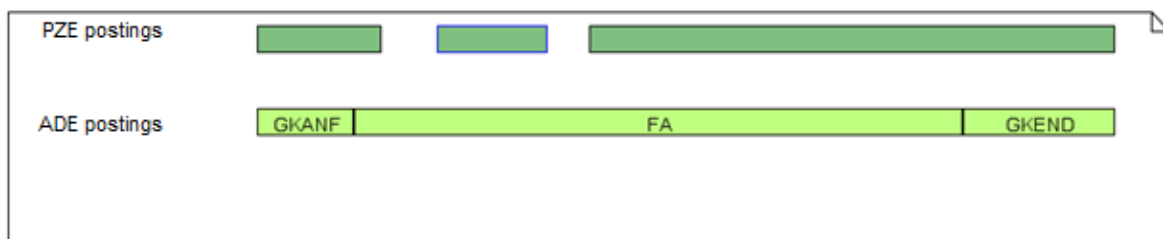


The first gap was filled with GKANF, the last with GKEND.

Example 2

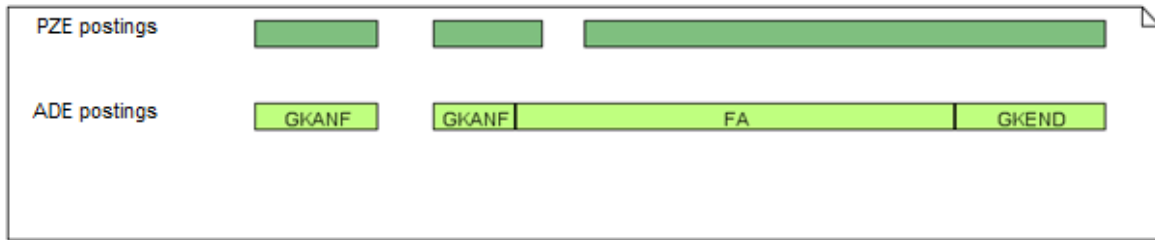


In this case, there are two PZW postings with an interruption. For this case, two waiting period postings with GKANF are generated.

Example 3

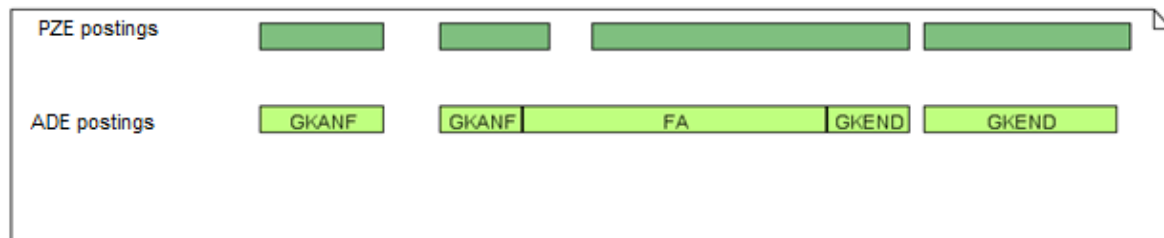


In this case, there are two PZW postings with an interruption. For this case, two waiting period postings with GKANF are generated. At the end, two waiting period postings with GKEND are generated.

Example 4

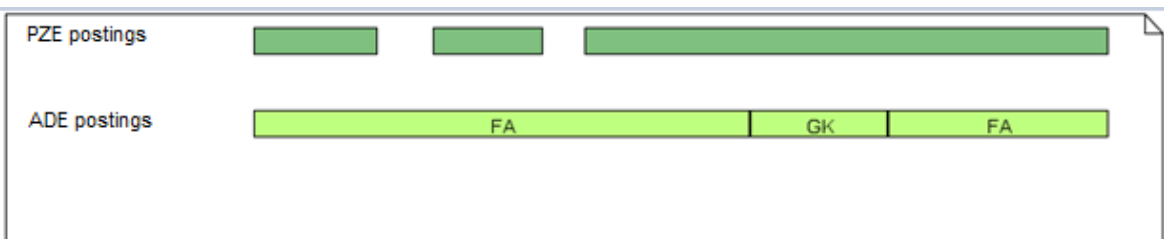


The gap between the production orders is filled with an overhead cost waiting period posting.


Example 5

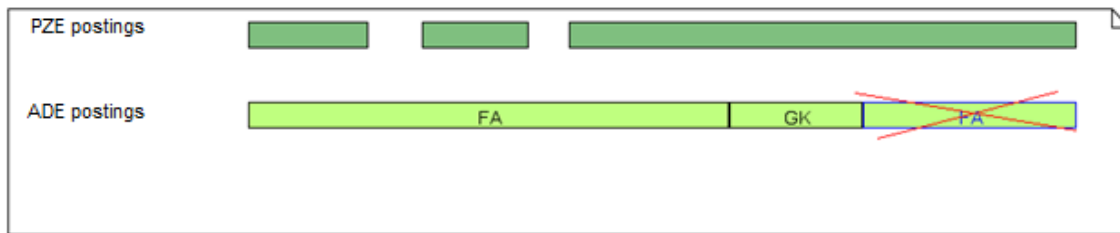

This is based on example 4. Now, the latest BDE posting (PO) is deleted manually. The following scenario is generated for the next run.

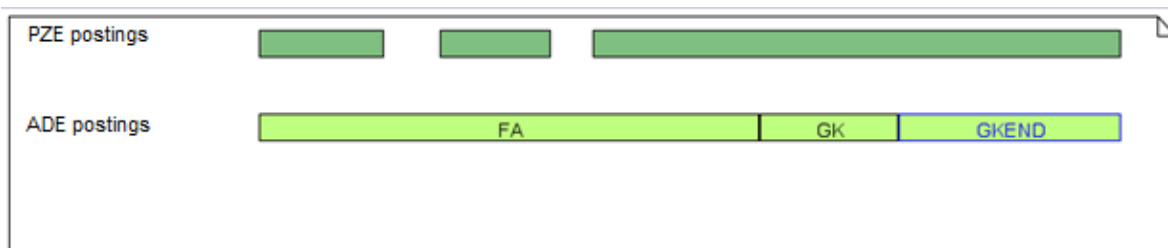

Example 6

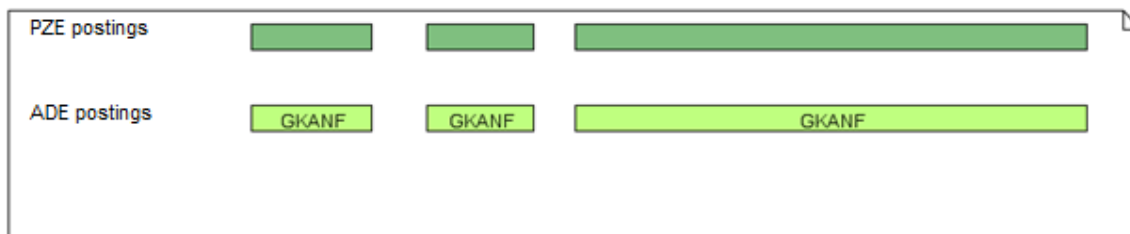

There are no BDE postings for this day. Through the comparison, three waiting period postings with GKANF are generated.

Please note: These GKANF waiting period postings are only generated if an BDE posting can be found for this person in the past 10 days. This posting from the past determines the workplace to which this posting is allocated. If no posting is found, no waiting period posting is generated, either.

Example 7



This is based on example 6. The two latest waiting period postings are deleted manually. The following scenario is again generated for the next run.



It is verified whether the previously generated BDE posting was also a waiting period posting with this order number (GKANF). If so, this GKANF waiting period posting is continued.

1.4.2.2 Closing Gaps in Mode PREDECESSOR

Special rules for closing gaps in mode PREDECESSOR


1. You start to close gaps from the "start" following the rule "The person works on their orders until other postings are available".
2. The function to close gaps is relevant for all persons with the active option *BDE/PZW comparison* in the HR master data (tab *Incentive wages*).
3. The PZW times that are relevant for the close gap function are defined in the PZW wage types. Here, the option *Use wage type for comparing with HYDRA-BDE* enables or disables the function, as it is with the comparison of personnel postings. The wage types are edited by the customer. For example, it must be specified that absence times like holidays are not used to close gaps.
4. In case of days without any BDE personnel posting, the gaps are closed for the relevant persons.
5. Multiple machine operation in a gap is **not** supported. A gap is only closed using an operation. The system uses the operation where the person has last logged off. If the

person has logged off from several operations at the same time, the operation with the largest number is used.


6. Editing or posting errors can create long lasting BDE personnel postings. These postings are always assigned to a defined day of PZW evaluation. Here, the last day of the possible days of PZW evaluation is used. (Same assignment as in application *Labor time comparison* and subsequent entry using the column *PZW evaluation day*).
7. The system still posts to finished OPs, but does not reactivate the OPs. For this reason, SAP PP can receive confirmations/postings for operations that have already been finished.
8. If no previous BDE postings of the person can be found, then the gap cannot be closed. This is recorded in a log file. This can happen with persons who are new or after very long absences of persons.

The following examples describe how the "close gap" function works.


Legend:

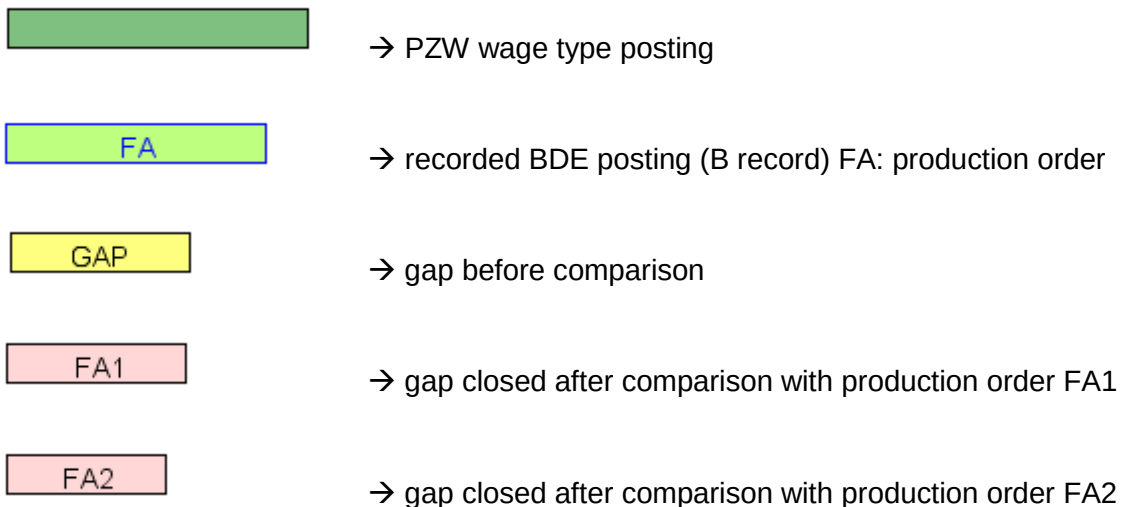


Example 1

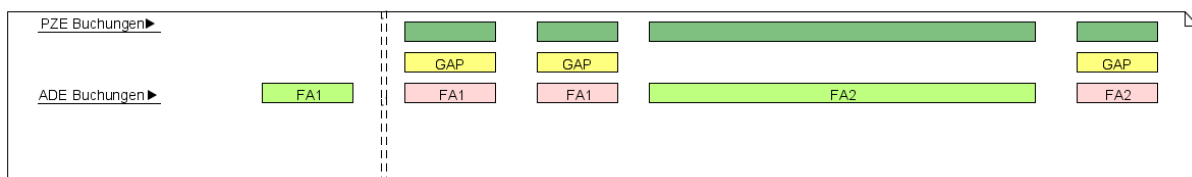


Example 2

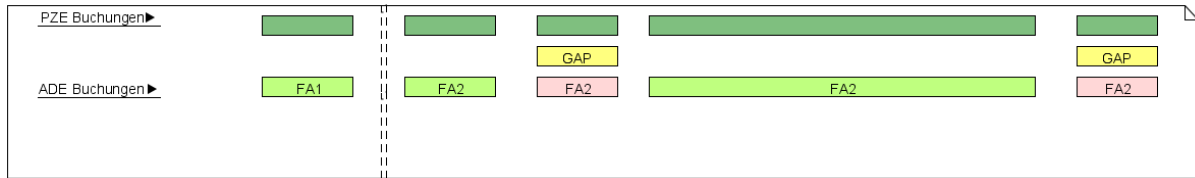


Example 3

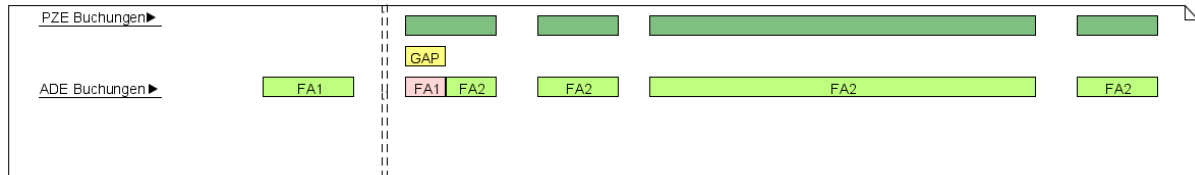

Example 4

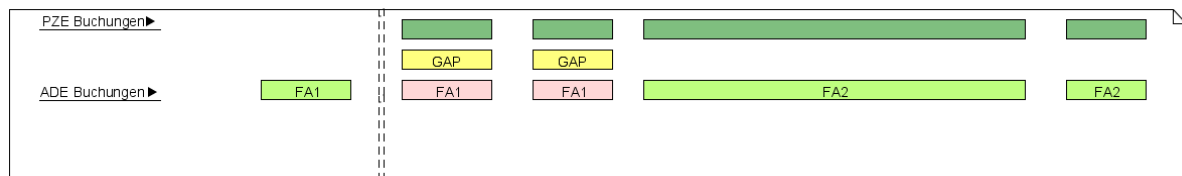


Example 5

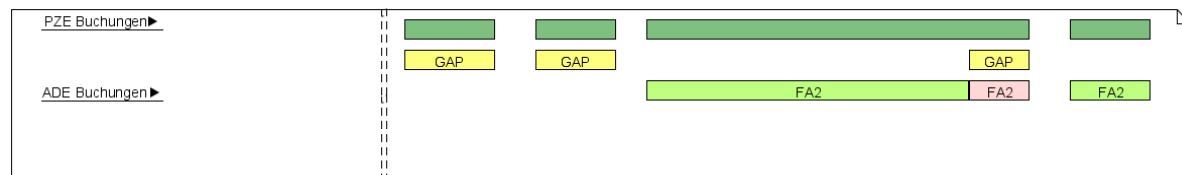

No production order is found here in the past. The first two gaps cannot be closed.

Example 6

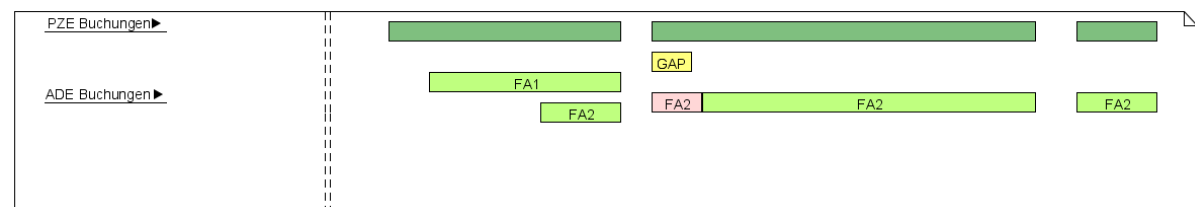

The system does **not** support to close a gap with multiple machine operation. A gap is only closed using an operation. The system uses the operation where the person has last logged off. If the person has logged off from several operations at the same time, the operation with the largest number is used.

1.5 Configurations Required

1.5.1 HR Master Data

For persons who are to be processed by the comparison, the "BDE/PZW comparison" option must be set in the HR master data, "incentive payment" tab.

1.5.2 Wage Types

In PZW, you must enable the option "Use wage type for comparing with HYDRA-BDE" for the wage types relevant for the comparison.

1.5.3 Customizing "Close Gap" function

1.5.3.1 Mode WAITINGPERIODOP

HYDRA basic settings

In the HYDRA basic settings, the waiting period operation must be entered. Here, the BDE waiting period processing should also be suitably configured, so that small gaps between BDE personnel postings are avoided in the entry already.

Activate closing gap

Closing gap is activated through an INI configuration.

Ini-Name: ADEPZECOMP
Section: FILLGAP
Key/Value: MODE=WAITINGPERIODOP

Optional: own waiting period operations for start/end

Note:

The options for special waiting period operations at the beginning and end are only available, if the close gap function is activated in mode WAITINGPERIODOP. The special waiting period OPs are only useful, if the comparison is made **for a day**. This condition is only fulfilled if you have configured daily evaluation periods for the overtime compensation in the Personnel Time Management.

Ini-Name: ADEPZECOMP
Section: FILLGAP
Key/Value: FIRSTOP=<Waiting period operation number>

Ini-Name: ADEPZECOMP
Section: FILLGAP
Key/Value: LASTOP=<Waiting period operation number>

1.5.3.2 Mode PREDECESSOR

Activate closing gaps

The function is activated via INI configuration

Ini name: ADEPZECOMP
Section: FILLGAP
Key/Value: MODE=PREDECESSOR

1.6 System Requirements

1.6.1 Restrictions

- The active PDE/PZW comparison is **only available in HYDRA with operation mode "Maintenance of postings"**.
- The comparison function books all durations in the processed BDE personnel postings (B records) to resource performance account 11 only. The RPA assignment that depends on the workplace status is discarded.

1.6.2 Activating the Environment variable

The active BDE/PZW comparison is not active by default. The comparison must be activated. The reasons for this approach are the following:

- The active BDE/PZW comparison changes the BDE data and you cannot undo these changes. Because of the restrictions and conditions, the data changed by the comparison is different to the data recorded online. Example: The active comparison function books all durations to resource performance account 11 only. The RPA assignment that depends on the workplace status is discarded.
- The active comparison is integrated in the labor time calculation of the Personnel Time Management PZW. If the active comparison is activated, this has an effect on the run time of the labor time calculation, which you must not neglect.

Follow the instructions below to activate or deactivate the active BDE/PZW comparison. If you are not sure how to proceed or which effects might result, then you can have the active comparison activated or deactivated by MPDV as service including consulting.

General

You use the system environment variable PZE_ADE_ABGL to activate the active comparison on the server. Two options are available:

PZE_ADE_ABGL=ALL	All B records (also manually changed records) are compared with the PZE (default).
PZE_ADE_ABGL=NOEDIT	Manually changed B records are not compared with the PZE.

Different activation steps must be performed for the different server operating systems. Please mind the valid standard installation instruction for HYDRA.

Windows activation

Perform the following steps for each system number where the active comparison must be activated:

1. Activate the entry for the environment variable in the file <SystemNr>\hymap.cfg
Select the relevant option ALL or NOEDIT:

```
...
# Activation of active BDE/PZW comparison
# PZE_ADE_ABGL=ALL      : All B records, even those edited manually, are
#                        synchronized by BDE/PZW comparison (default).
# PZE_ADE_ABGL=NOEDIT : Manually edited B records are not synchronized
#                        by BDE/PZW comparison.
PZE_ADE_ABGL=ALL
```

Note: It is possible that the comments in the file on your system are different.

2. Create a file <SystemNr>\hymap_pzw_ade.cfg on the server with the following contents.

Select the same value for PZE_ADE_ABGL as in the file above.

Mind the correct system number of HYSYSTEM!

```
[Default]
HYSYSTEM=1

[Environment]
PZE_ADE_ABGL=ALL
```

- Install the new file using the following command (change the system number!):

```
ntinst -if 1\hymap_pzw_ade.cfg
```

Screen output:

```
HYDRA 1
hydadm:1:D:\hydra>ntinst -if 1\hymap_pzw_ade.cfg
-----

[Default]
hysystem=1
Key SOFTWARE\MPDV\Hydra\1\Environment created.


[Environment]
Key SOFTWARE\MPDV\Hydra\1\Environment created.
Key SOFTWARE\MPDV\Hydra\1\Environment value PZE_ADE_ABGL with content ALL created.

hydadm:1:D:\hydra>
```

- Restart HYDRA on the server.

Checking the result

On the server, an entry with key PZE_ADE_ABGL in path "HKEY_LOCAL_MACHINE\SOFTWARE\MPDV\Hydra\<SystemNo>\Environment" must be available in the registry.

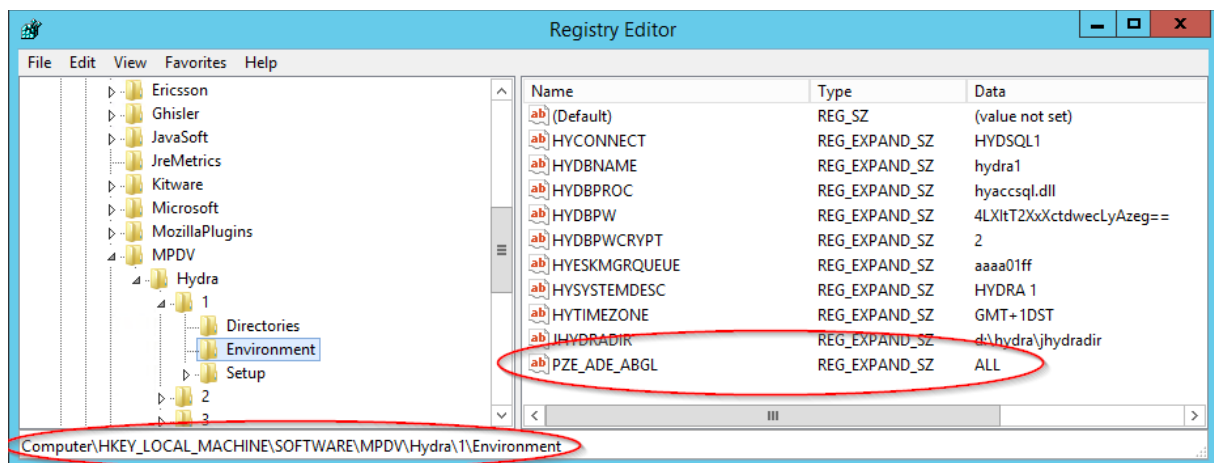

- Mind the correct system number.
- The value must be ALL or NOEDIT.

You can use the command "hygetenv" to check in the command line on the server if the environment variable of the registry is correctly evaluated in the software:

```
hydadm:F:\Hydra3>hygetenv.exe +PZE_ADE_ABGL
ALL
hydadm:F:\Hydra3>
```

The output must be ALL or NOEDIT depending on the option selected.

If the environment variable is included in the registry or if it is not shown with `hygetenv`, then you must check the activation steps and correct them, if required.

Windows deactivation

Perform the following steps for each system number where the active comparison must be deactivated: The instructions refer to the activation steps mentioned above:

1. Set the comment character in front of the activated entry in file `<SystemNo>\hymap.cfg` in front of the value `PZE_ADE_ABGL`
2. Delete the key `PZE_ADE_ABGL` from the registry.
3. Restart HYDRA on the server.

Linux activation

- 1) Activate the entry for the environment variable in the file `<SystemNo>\hy_env.scr`.

Select the relevant option ALL or NOEDIT:

```
...
#
# Activation of active BDE/PZW comparison
# PZE_ADE_ABGL=ALL      : All B records, even those edited manually, are
#                        synchronized by BDE/PZW comparison (default).
# PZE_ADE_ABGL=NOEDIT : Manually edited B records are not synchronized
#                        by BDE/PZW comparison.
export PZE_ADE_ABGL=ALL
...
```

Note: It is possible that the comments in the file on your system are different.

- 2) Restart HYDRA on the server.

Checking the result

You can use the command "hygetenv" to check in the command line on the server if the environment variable is correctly evaluated in the software:

```
server:hyadm:1:/u1/hydra1> hygetenv.out +PZE_ADE_ABGL
ALLserver:hyadm:1:/u1/hydra1>
server:hyadm:1:/u1/hydra1>
```

The output must be ALL or NOEDIT depending on the option selected.

If the environment variable is not shown with `hygetenv`, then you must check the activation steps and correct and repeat them, if required.

Linux deactivation

Perform the following steps for each system number where the active comparison must be deactivated: The instructions refer to the activation steps mentioned above:

- 1) Set the comment character in the file <SystemNr>\hy_env.scr in front of the entry for the environment variable PZE_ADE_ABGL.
- 2) Restart HYDRA on the server.

1.7 Logging

1.7.1 Log files

The active BDE/PZW comparison automatically creates log files on the server. The log files include technical information. The log files can inform about missing settings when the active BDE/PZW comparison is activated or the log files are requested by the MPDV support to analyze specific issues.

For each personnel number, an own log file is created. It is then easier to make person-related analyzes. If the files have a specific size, they are renamed and a new file is started. The log files are located in a subdirectory of the installation directory:

Schema: <InstDir>\<SystemNr>\err\pzeadeab_<PersonnelNo>.pro

Example: \\MyServer\Hydra3\3\err\pzeadeab_00906000.pro

If no log files are available after a labor time calculation, then the activation was not correct.

Example of the content:

```
07.03.19 12:00 ===== S T A R T =====
07.03.19 12:00 Start PZE/ADE comparison PNR: [906000] DATB: [02/15/2019] DATE:[03/14/2019] SCOPE: [ALL]
07.03.19 12:00 Option PZE/ADE comparison [N] is not set for person 906000, 02/15/2019 - 03/14/2019
07.03.19 12:00 No PZE bookings for person [906000] available. DATB: [02/15/2019] DATE:[03/14/2019]
07.03.19 12:00 End PZE/ADE comparison PNR: [906000]
07.03.19 12:00 ===== E N D =====
07.03.19 12:11 ===== S T A R T =====
07.03.19 12:11 Start PZE/ADE comparison PNR: [906000] DATB: [02/15/2019] DATE:[03/14/2019] SCOPE: [ALL]
07.03.19 12:11 DB pzebuchung[906000] --> PzeList.size: (0)
07.03.19 12:11 No PZE bookings for person [906000] available. DATB: [02/15/2019] DATE:[03/14/2019]
07.03.19 12:11 End PZE/ADE comparison PNR: [906000]
07.03.19 12:11 ===== E N D =====
07.03.19 12:12 ===== S T A R T =====
07.03.19 12:12 Start PZE/ADE comparison PNR: [906000] DATB: [02/15/2019] DATE:[03/14/2019] SCOPE: [ALL]
07.03.19 12:12 DB pzebuchung[906000] --> PzeList.size: (4)
ZEIB: 26.02. 05:00:00 ZEIE: 26.02. 10:15:00 PZEAUTAG(43521): 02/26/2019 00:00:00
ZEIB: 26.02. 10:45:00 ZEIE: 26.02. 13:00:00 PZEAUTAG(43521): 02/26/2019 00:00:00
ZEIB: 04.03. 14:00:00 ZEIE: 04.03. 18:15:00 PZEAUTAG(43527): 03/04/2019 00:00:00
ZEIB: 04.03. 18:45:00 ZEIE: 04.03. 22:00:00 PZEAUTAG(43527): 03/04/2019 00:00:00
07.03.19 12:12 Last B-Booking to old PNR: [906000] ZEIE: [05.11. 09:49:40] MAXABSENCE: [10]
07.03.19 12:12 No past B-Booking found for PNR: [906000] MAXABSENCE: [10]
07.03.19 12:12 HyFillGap --> m_opMap.size: (1) m_mode:(0)
AdeBookings Result (0):
07.03.19 12:12 End PZE/ADE comparison PNR: [906000]
07.03.19 12:12 ===== E N D =====
07.03.19 12:25 ===== S T A R T =====
```

```

07.03.19 12:25 Start PZE/ADE comparison PNR: [906000] DATB: [02/15/2019] DATE:[03/14/2019] SCOPE: [ALL]
07.03.19 12:25 DB pzebuchung[906000] --> PzeList.size: (4)
ZEIB: 26.02. 05:00:00 ZEIE: 26.02. 10:15:00 PZEAWTAG(43521): 02/26/2019 00:00:00
ZEIB: 26.02. 10:45:00 ZEIE: 26.02. 13:00:00 PZEAWTAG(43521): 02/26/2019 00:00:00
ZEIB: 04.03. 14:00:00 ZEIE: 04.03. 18:15:00 PZEAWTAG(43527): 03/04/2019 00:00:00
ZEIB: 04.03. 18:45:00 ZEIE: 04.03. 22:00:00 PZEAWTAG(43527): 03/04/2019 00:00:00
07.03.19 12:25 Last B-Booking to old PNR: [906000] ZEIE: [05.11. 09:49:40] MAXABSENCE: [10]
07.03.19 12:25 No past B-Booking found for PNR: [906000] MAXABSENCE: [10]
07.03.19 12:25 HyFillGap --> m_opMap.size: (1) m_mode:(0)
AdeBookings Result (1):
  @ ID: 47995 0 MNR=50500 ANR=100000020004 ZEIB=04.03. 13:37:44 ZEIE=04.03. 22:17:54 AGL= 27000 (7.50) CALC= 31210
PZEAWTAG=03/04/2019
ADEPRO.SELECT RET: [0] VERWEIS:(47995) RET.VERWEIS: [47995] UPDATE.RET:[0]
ADEPRO.SetValue ----- VERWEIS:(47995) --> changing EGR:BMK07 from "1620" to "0"
ADEPRO.UPDATE RET: [0] VERWEIS:(47995) RET.VERWEIS: [47995] UPDATE.RET:[0]
ADEPRO.SIGN RET: [0] VERWEIS:(47995) RET.VERWEIS: [47995] UPDATE.RET:[0]
07.03.19 12:25 End PZE/ADE comparison PNR: [906000]
07.03.19 12:25 ===== E N D =====

```

Option PZE/ADE comparison [N] is not set for person

For this person, the active BDE/PZW comparison is not activated. Activate the option "BDE/PZE comparison" in the HR master data. Only then a comparison can be made for this person.

No PZE bookings for person

Either the labor time calculation did not calculate the wage type postings because of an error, or you must activate the option *Use wage type for comparing with HYDRA-BDE* in the master data of wage type(s).

B-Booking to old

The last BDE posting of the person cannot be used to close the gap because it is too long in the past.

B-Booking / AdeBookings

Information on BDE personnel postings (B records).