

Manual

Process Data Management: Collection Rules PDV-VRP 8.2

Version 1.0.23049

Last changed on: 02.09.2020

Copyright

©Copyright 2020 All rights reserved.

SAP® and R/3® are registered trademarks of SAP AG.

WINDOWS® is a registered trademark of Microsoft Corporation.

MPDV® and HYDRA® are registered trademarks of MPDV Mikrolab GmbH.

ORACLE® is a registered trademark of ORACLE Corporation, California, USA.

Copying and distribution of this documentation or any part thereof, for any purpose or in any form, is prohibited without prior written permission from MPDV Mikrolab GmbH.

The information contained in this documentation is subject to change without prior notice.

Contents

1	Process Data Management: Processing Rules	4
2	Collection Rules	5
3	Collection Request	10

1 Process Data Management: Processing Rules

Overview

Purpose

The PDV-VRP function package "Processing rules for process data" provides the functions used to define collection rules and collection processes. The characteristics defined in the basic package are linked with the access paths by defining collection rules. This activates PDV data collection

Integration

This function package requires a machine interface for data collection in the HYDRA Process Communication Controller (PCC) and the basic package PDV-PDM.

Features

- Development of machine-related collection rules managed in specific versions. Consolidation of characteristics planned for this machine. Definition of limits. Specification for statistics processing.
- Development of article-related collection rules managed in specific versions. Consolidation of characteristics planned for this article. Definition of limits. Specification for statistics processing.
- Taking the specification list into account, planned values can be redefined by referring to tools, machines or articles.
- The collection rules have a version number and can be blocked or released by the user. Versions remain unchanged when rules are modified. A version of a collection rule can be activated. It is then used as the basis for collecting measured values.
- Definition of conversion factors for characteristics and the ability to calculate new characteristics from existing characteristics.
- Collection rules are converted into active collection requests by order processing (for article-related collection rules) or manual specification (machine-related collection rule). Collection requests regulate data collection and provide the ability to evaluate the history.
- When the collection request is changed, active collection processes are automatically notified and, as a result, collection specifications automatically change at runtime.


2 Collection Rules

Overview

Menu	Quality management → Process data collection → Collection rules
Transaction code	iplpd
Function authorization	iplpd

Purpose

The automatic data collection of process characteristics is based on the collection rules specified in the Process Data Collection module.

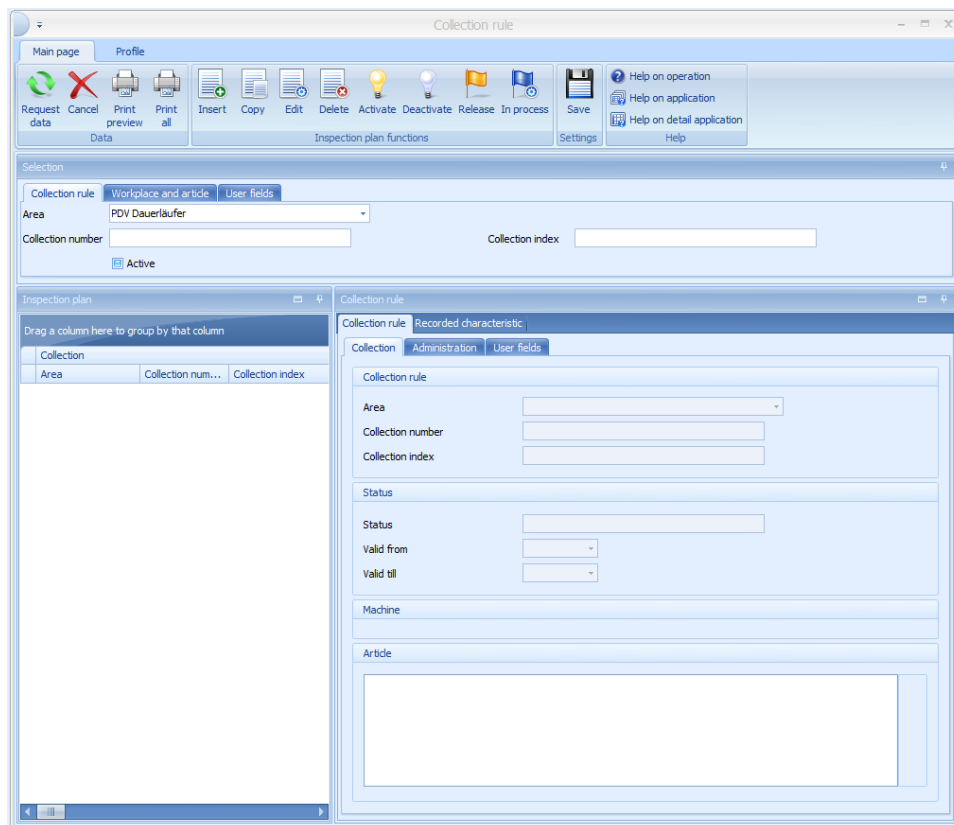

Integration

Collection rules result in collection requests. Collection requests activate the defined rules for data collection. Characteristics are the basis for collection rules. You can take the characteristics from the characteristics master data catalog. The generation of collection requests activates the actual data collection process. The data collection uses the logical channel that is defined by the process parameter of the characteristic.

Requirements

The characteristics catalog must be defined.

Selection criteria

The application provides the following selection criteria:

You can choose from three different tabs to select data. You can use the tabs "Collection rule", "Workplace and article" and "User fields".

Collection rule:

Area (drop-down list)

You can use the drop-down list to select the required area.

Collection number

Select the collection number.

Collection index

Select the collection index.

Active checkbox

Enable the checkbox to select active collection rules.

Workplace and article:

Machine

Select the required machine.

Article number

You can use a search application to search for and select an article number.

Article name/designation

You can select the article name.

User fields:

Object type

You can select an object type.


User field key

Use the drop-down list to select a user field key.

Field descriptions

The table view of the detail application offers an overview of existing entries. You can sort the displayed information using table functions. The displayed data complies with the specified selection parameters.

The table view is an integrated master-detail table, which contains not only the collection rules, but can also be expanded to show the recorded characteristics:

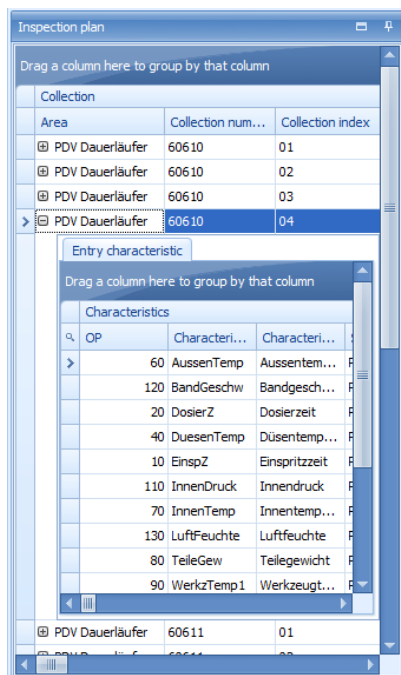

Collection		
Area	Collection num...	Collection index
PDV Dauerläufer	60610	01
PDV Dauerläufer	60610	02
PDV Dauerläufer	60610	03
PDV Dauerläufer	60610	04

Entry characteristic		
OP	Characteri...	Characteri...
60	AussenTemp	Aussentem...
120	BandGeschw	Bandgesch...
20	DosierZ	Dosierzeit
40	DuesenTemp	Düsentemp...
10	EinspZ	Einspritzzeit
110	InnenDruck	Innendruck
70	InnenTemp	Innentemp...
130	LuftFeuchte	Luftfeuchte
80	TeileGew	Teilgewicht
90	WerkzTemp1	Werkzeugt...

Depending on the selected line, the details pane shows the corresponding information. The tabs vary accordingly.

When you call up an editing function, this function affects the entry/entries selected in the table.

Toolbar

In addition to the standard buttons for creating, deleting and editing, the following, context sensitive buttons are available for the collection rules:



Activate

Function authorization: `iplpd.activate`

Click this button to enable the selected collection rule. Only one version of a collection rule can be active at a time! If you activate continuous monitoring rules, the system immediately generates a collection request. This activates data collection. If you activate article-related collection rules, the system automatically generates a collection request the next time you log on a production order for this article.



Deactivate

Function authorization: `iplpd.deactivate`

Click this button to deactivate the selected collection rule. If you deactivate continuous monitoring rules, the system terminates the collection request.



Release

Function authorization: `iplpd.release`

Click this button to release the selected collection rule. You can no longer edit released rules. You can only activate released rules.



In process

Function authorization: `iplpd.inprocess`

Click this button to cancel the release for the selected collection rule. You can now edit the rule.

Detail applications

The detail view shows the information matching the entry selected in the table view.

The detail view consists of two tabs, i.e. the collection rule and the recorded characteristic. These tabs include some additional sub-tabs.

Collection rule:

Collection: The detail view shows the data that has to do with data collection. These include the collection rule, the status, the machine and the article.

Administration: This detail view displays the data that has to do with data management. This is primarily a time stamp for the selected inspection plan.

User fields: Shows the object type and the user field key.

Recorded characteristic:

Characteristics: This detail view shows the characteristics for the current inspection plan.

Specifications: This detail view shows the samples and dimensions in detail. You need the function authorization *iriscp.interval* in order to store an interval value in the sampling scheme.



Please note that sample-related reports/evaluations are not available for process characteristics whose limit values are controlled via specification lists.

Storage: Shows the selected filter function.

Visualization: Detail view for the visualization.

Inspection - computation: Detail view for inspection and calculation.

Administration: This detail view displays the data that has to do with data management. This is primarily a time stamp for the selected inspection plan.

User fields: Shows the object type and the user field key.

3 Collection Request

Summary

Menu	Quality Management → Process Data Collection → Collection Request
Transaction code	crpd
Function authorization	crpd

The collection requests are generated according to defined rules from the collection rules. The actual collection of data is activated by the collection requests.

Usage

The collection requests are generated by

- Continuous collection rules, fully automatic when the collection rule is activated. When it is deactivated, the request is automatically closed again.
- Article related collection rules, fully automatic when production orders for the defined article are generated or logged on.

Integration

The collection requests are created from the collection rules and then transferred to the collection computer in compressed form so that it starts the collection after it receives the rule.

Normally no manual intervention into the collection requests is necessary because they are created and ended automatically. Rather, the function is used only for purposes of analysis.

Requirement

In addition to the collection rules, the collection of the logical channels must be defined so that collection can occur.

Toolbar

The toolbar contains function for controlling the activity of the collection requests such as release, complete and cancel.