AS-5216x64 DLL

Interface Package for 64 bit Windows Applications

Version 2.3.0.0

USER'S MANUAL
June 2012

Avantes B.V.

Oude Apeldoornseweg 28
NL-7333 NS Apeldoorn
The Netherlands
Tel: +31-313-670170
Fax: +31-313-670179

Web: www.avantes.com
Email: info@avantes.com

Microsoft, Visual C++, Visual Basic, Visual C# , Windows, Windows 95/98/Me, Windows NT/2000/XP and Microsoft Office are registered trademarks of the Microsoft Corporation. Windows Vista and Windows 7 are either registered trademarks or trademarks of Microsoft Corporation in the United States and/or other countries.

Delphi and C++Builder are trademarks of CodeGear, a subsidiary of Embarcadero Technologies

LabVIEW is a trademark of the National Instruments Corporation

MATLAB is a registered trademark of The MathWorks, Inc.

Qt is a trademark of Nokia Corporation in Finland and/or other countries worldwide.

Software License

THE INFORMATION AND CODE PROVIDED HEREUNDER (COLLECTIVELY REFERRED TO AS "SOFTWARE") IS PROVIDED AS IS WITHOUT WARRANTY OF ANY KIND, EITHER EXPRESS OR IMPLIED, INCLUDING BUT NOT LIMITED TO THE IMPLIED WARRANTIES OF MERCHANTABILITY AND FITNESS FOR A PARTICULAR PURPOSE. IN NO EVENT SHALL AVANTES BV OR ITS SUPPLIERS BE LIABLE FOR ANY DAMAGES WHATSOEVER INCLUDING DIRECT, INDIRECT, INCIDENTAL, CONSEQUENTIAL, LOSS OF BUSINESS PROFITS OR SPECIAL DAMAGES, EVEN IF AVANTES BV OR ITS SUPPLIERS HAVE BEEN ADVISED OF THE POSSIBILITY OF SUCH DAMAGES. SOME STATES DO NOT ALLOW THE EXCLUSION OR LIMITATION OF LIABILITY FOR CONSEQUENTIAL OR INCIDENTAL DAMAGES SO THE FOREGOING LIMITATION MAY NOT APPLY.

This Software gives you the ability to write applications to acquire and process data from Avantes equipment. You have the right to redistribute the libraries contained in the Software, subject to the following conditions:

1. You are developing applications to control Avantes equipment. If you use the code contained herein to develop applications for other purposes, you MUST obtain a separate software license .
2. You distribute only the drivers necessary to support your application.
3. You place all copyright notices and other protective disclaimers and notices contained on the Software on all copies of the Software and your software product.
4. You or your company provides technical support to the users of your application. Avantes bv will not provide software support to these customers.
5. You agree to indemnify, hold harmless, and defend Avantes bv and its suppliers from and against any claims or lawsuits, including attorneys' fees that arise or result from the use or distribution of your software product and any modifications to the Software.

0　Installation

The AS5216x64 DLL is the 64 bit version of the AS5216 driver interface. It is needed when you want the DLL to cooperate with 64 bit programs, like self-written 64 bit programs or the 64 bit versions of LabVIEW or MATLAB. Note that the 32 bit versions of LabVIEW or MATLAB can run perfectly well on 64 bit versions of Windows. You will have to determine your version, generally this is displayed in the About box of each program. The Visual Studio IDE is a 32 bit application, that can generate either 32 or 64 bit programs.

The AS5216x64 DLL package version can be installed under the following operating systems:

- XP/Vista/Windows7 x64 (64-bit O/S)

The installation program can be started by running the file "setup64.exe" from the CD-ROM.

Installation Dialogs
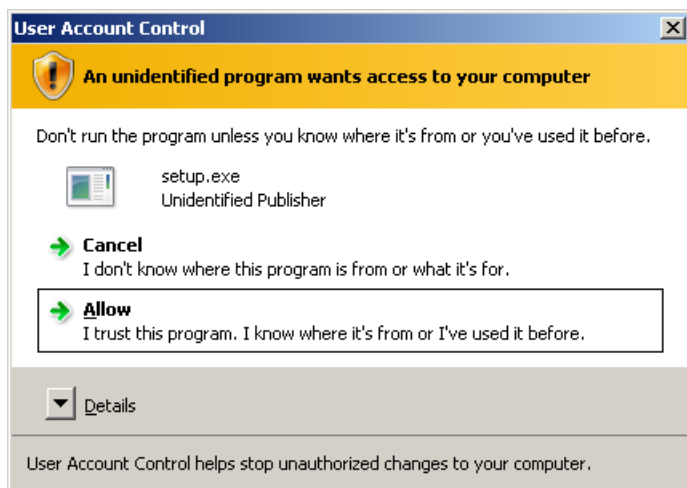
If you use Windows Vista, and the UAC setting is enabled, you will get the warning displayed to the left. Please select "Allow" to install the package.

This installation is password protected. Enter the following password to proceed with the installation:

Avantes6961LL4a

The setup program will check the system configuration of the computer. If no problems are detected, the first dialog is the "Welcome" dialog with some general information

In the next dialog, the destination directory for the AS5216x64 DLL software can be changed. The default destination directory is C:\AS5216x64-DLL_2.3. If you want to install the software to a different directory, click the Browse button, select a new directory and click OK.

If the specified directory does not exist, it will be created.
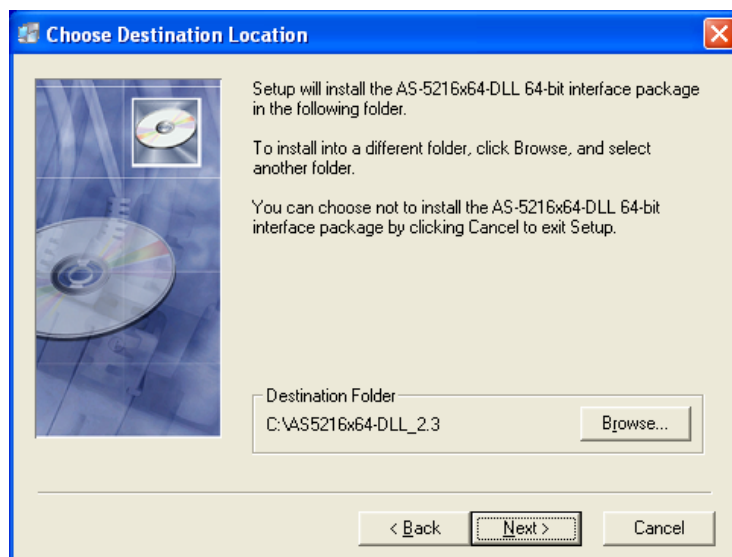
During this installation, the installation program will check if the most recent USB driver has been installed already at the PC. If no driver is found, or if the driver needs to be upgraded, the Device Driver Installation Wizard is launched automatically, click Next. Starting with version 1.6, the driver packages are signed, and should not generate a warning that the publisher of the driver software cannot be identified. If this warning appears anyway, please select "Install this driver software anyway".
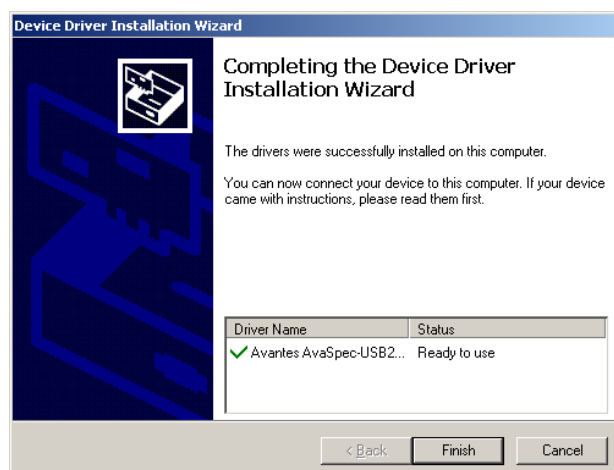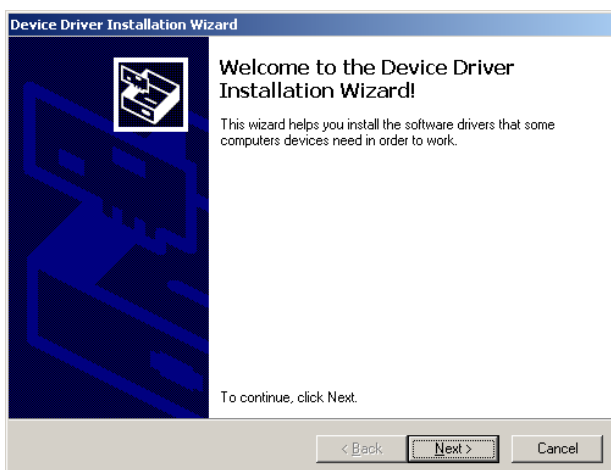
After the drivers have been installed successfully, the dialog at the right is displayed, click Finish. After all files have been installed, the "Installation Complete" dialog shows up. Click Finish.

Connecting the hardware

Connect the USB connector to a USB port on your computer with the supplied USB cable. Windows XP will display the "Found New Hardware" dialog. Select the (default) option to install the software automatically, and click next.

After the Hardware Wizard has completed, the following dialog is displayed under Windows XP:
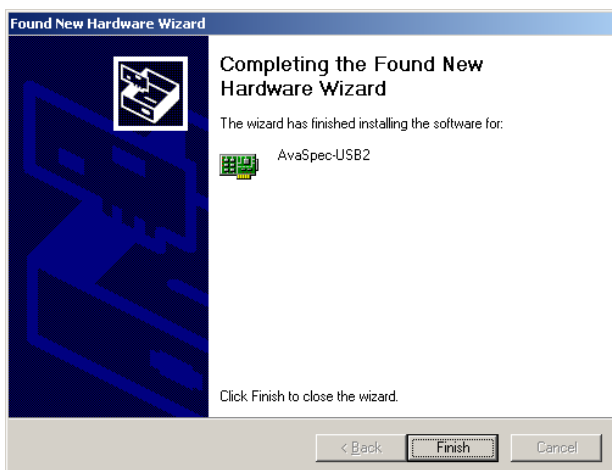
Click Finish to complete the installation.

Please note that if the spectrometer is Connected to another USB port to which it has not been connected before, the "Found New Hardware Wizard" will need to install the software for this port as well. For this reason, this Wizard will run "NrOfChannel" times for a multichannel AvaSpec-USB2 spectrometer system. This happens because inside the housing, the USB ports for each spectrometer channel are connected to a USB-Hub.

Windows Vista, or Windows 7 will install the driver silently, without displaying the "Found New Hardware Wizard" dialogs.

Launching the software
This AS5216x64 DLL manual can be started from the Windows Start Menu. The source code of the example programs can be found in the Examples folder.

1 Version History

This section will be used to describe the new features in as5216x64.dll c.q. as5216.dll, compared to the previous versions.

1.1 New in version 2.3.0.0

- A new function has been added for the NIR detectors (all AvaSpec-NIR models). The AvaSpec-NIR models can be operated in "Low Noise" or "High Sensitivity" mode. The new function AVS_SetSensitivityMode can be used to switch between these modes. See also section 2.3.37.

1.2 New in version 2.2.0.0

- Added support for the new detector in the AvaSpec-2048XL spectrometers, the Hamamatsu S11155.
- The version of the Qt libraries was updated to 4.6.3
- The AvaSpec-HS1024x58 and 1024x122 (High Sensitivity) series with Hamamatsu S7031 detector were already supported in as5216x64.dll v 2.1, but detector specific data such as minimum integration time, smoothing and triggering characteristics were missing in the AS5216x64-DLL v2.1 manual.

1.3 New in version 2.1.0.0

- Added dynamic dark support for the new detectors in the AvaSpec 2048x16 and the AvaSpec 2048x64 spectrometers. It is strongly recommended to keep dynamic dark correction enabled (default state). See also section 3.2.5.
- Minimum integration time for the AvaSpec-2048x16 changed from 0.91ms to 1.82 ms (see also section 3.2.2).
- Minimum integration time for the AvaSpec-2048x64 changed from 1.75ms to 2.40 ms (see also section 3.2.2).
- The Qt samples were extended with a full featured graph, from the open source Qwt library. A distribution file for this library is included.

1.4 New in version 2.0.0.0

- Support for 64 bit programs, for both native and managed code. The 64 bit DLL is now written in Microsoft Visual C++ 2008, combined with the Qt4 framework. The 64 bit DLL requires the Microsoft Visual C++ 2008 and Qt4 runtimes to function. The setup program installs the VC++2008 runtime, which is called 'vcredist_x64.exe'. You may need to run this file yourself on other PC's that do not have VC++2008 installed. The Qt4 runtime is called 'QtCore4.dll', and is best located in the same directory as 'as5216x64.dll'.
- As the Qt4 framework uses the WM_USER+1 message itself, the DLL now uses the WM_APP+1 windows message to signal the arrival of new data.
- Addition of two samples written in Microsoft Visual C++ 2008, combined with the Qt4 framework. These are 64 bit native code samples.
- Addition of a Matlab sample, for 64 bit Matlab R2010a.
- The LabView samples were adapted for 64 bit LabView 2009. In the large sample, the Measurement Configuration structure is now also translated to a linear array of bytes, before being transferred to the DLL. In previous versions, this was not necessary. The large LabView sample was also clarified by using an event structure for the different command buttons.
- The VB .net, VC# and VC++ samples were adapted for 64 bit Visual Studio 2008. These are all managed code samples. The marshalling code of the VB sample was extensively changed, which allows it to now directly pass structures to the DLL, without translation to a linear array of bytes.

- The 32 bit only samples (for Delphi, C++ Builder, VB6 and VC++ 6) were removed from the 64 bit DLL package.
- Addition of support for the new detectors in the AvaSpec 2048x16 and the AvaSpec 2048x64 spectrometers.

1.5 New in version 1.7.0.0

- Support of Dynamic Dark Correction for AvaSpec-NIR-2.0/2.2/2.5. The offset level for the cooled NIR detectors strongly depends on the ambient temperature. By using Dynamic Dark Correction, the offset level is measured with each new scan at a few blocked data pixels, and the measured signal is subtracted from all other data pixels. See also section 3.2.5.
- Floating Point Exceptions handling. The program environment in which the as5216.dll is written (C++Builder) uses by default another way of handling floating point exceptions than the MicroSoft (Visual Studio) programming environment in which the application software can be developed. As long as no floating point exceptions are created by the application (e.g. because of division by zero), no problems occurred in previous as5216.dll versions. However if floating point exceptions did occur in the application, or were thrown by other third party libraries, this may have resulted in a fatal crash of the application. In as5216.dll version 1.7.0.0, this rare problem has been solved by setting the FPU Control Word to the MicroSoft default. This solved the fatal crash in the few occasions that were reported in the past 5 years.
- Addition of new Delphi and C++Builder sample programs. The "old" Delphi 6.0 and C++Builder 5.0 sample programs are not fully compatible with the most recent Delphi and C++Builder versions. Since the Codegear 2009 versions, the character (char type) size is 2 bytes (Unicode), whereas in previous versions this type was only 1 byte. If 1 byte characters need to be used, the AnsiChar type should be used in the Codegear 2009 environment.
- Addition of a simple Visual Basic 6.0 sample program, which uses AVS_PollScan instead of Windows Messaging.
- Addition of a simple LabView sample program to illustrate how the StoreToRAM functionality can be implemented in combination with AVS_PollScan.
- Support of the new AvaSpec-(ULS)350F-USB2, AvaSpec-(ULS)950F-USB2, AvaSpec-(ULS)1350F-USB2 and AvaSpec-(ULS)1650F-USB2 spectrometers. The "F" in the name refers to Fast, because of the Fast minimum integration time that can be used for these spectrometers, see also section 3.2.2. For example, with the AvaSpec-(ULS)350F-USB2, 5000 full spectra (350 pixels) can be saved into onboard RAM in exactly one second (0.20 ms integration time).
- The return value of the function AVS_GetSaturatedPixels in previous as5216.dll functions was not implemented as intended. Unlike all other functions, AVS_GetSaturatedPixels returns '1' on success and '0' if it is called at a moment that no data is available (measurement pending). Because this return value has been present in all previous versions, changing this in the as5216.dll may result in an incompatibility of the application software. Therefore it was decided to make the notification in this manual, and leave the return value as implemented in the previous versions. See also section 2.3.15.

1.6 New in version 1.6.0.0

Addition of support for Windows Vista x64. The DLL now detects whether it is running on a 64 bit version of Windows, and will then use the WinUSB device driver, instead of the 32 bit Avsusb2.sys kernel mode device driver. WinUSB is Microsoft's own USB driver, that is distributed with Vista. The install package for the as5216.dll will configure WinUSB to support the AS5216 hardware. The DLL and examples are all still 32 bit programs, but they will now work on Vista x64 (in the so-called WoW64 mode).

1.7 New in version 1.5.0.0

- Addition of support for the AvaSpec-2048L-USB2, with Sony ILX-511 detector.
- Minimum integration time for the AvaSpec-2048x14-USB2 is changed from 2.24 msec to 2.17 msec.
- An additional delay of 500 msec is added when a device is activated, this proved to be necessary on recent PC's when using Windows Vista.

1.8 New in version 1.4.0.0

- Implementation of the StoreToRam function, which allows the storing of scans at high speed (as fast as 1.1 msecs per scan for the AvaSpec-2048-USB2, and 0.1 msecs per scan for the AvaSpec-102-USB2) in the spectrometer, without the overhead of USB communication. About 4MB of storage is available, which allows for 1013 full spectra with the AvaSpec-2048-USB2 and 19784 for the AvaSpec-102-USB2, or a lot more if the pixelrange is reduced by selecting the start- and stoppixel. StoreToRam requires firmware version 0.20 or later. A firmware upgrade utility can be downloaded from our website.
- Implementation of directory support for the Secure Digital Card.
- In a few occasions there have been problems with detecting and/or activating AvaSpec-USB2 spectrometers under Windows Vista. The reason for this is that, according to MicroSoft, "a USB device takes a long time to resume from selective suspend mode on a Windows Vista-based computer that uses UHCI (Universal Host Controller Interface) USB controllers. In the as5216.dll version 1.4, a workaround has been implemented to solve this problem.
- New sample programs for Visual C++ 2005, Delphi and LabView
    - o The Visual C++ 2005 sample program has been created in the Express version.
    - o A few sample programs in Delphi have been added: besides the comprehensive sample program that was already available in earlier as5216.dll versions, 3 new sample programs have been added:
        - A multichannel sample program in which up to 16 spectrometer channels can run simultaneously in SYNC mode or ASYNC mode.
        - An sdcard sample program which demonstrates how to save spectra to an onboard sdcard
        - A simple program with only a few lines of code which demonstrates the basic data acquisition for a single channel AvaSpec-USB2 spectrometer.
    - o The LabView sample programs have been updated to LabView version 8.2 (earlier versions can be obtained on request). There are 4 sample programs:
        - a comprehensive program for a single channel AvaSpec-USB2, which also includes subvi's for all functions in the as5216.dll
        - a program that illustrates the use of Windows Messaging in LabView.
        - a simple sample program that uses AVS_PollScan instead of Windows Messaging
        - a multichannel example program which illustrates how to run multiple spectrometer channels (fixed to 2 channels in the example program) in SYNC mode, as well as ASYNC mode.
- In this manual, examples have been added for using the function AVS_UseHighResAdc in combination with nonlinearity correction and/or irradiance calibration, see section 3.6.1 under "Using the nonlinearity correction polynomial in combination with the 16bit ADC Counts range" and section 3.6.3 under "How to convert ScopeData (A/D Counts) to a power distribution [μWatt/(cm^2.nm)]".

1.9 New in version 1.3.0.0

- Windows Vista support

- New Sample programs in Visual C# and Visual Basic.NET 2001. These sample programs can also be used in more recent .NET versions (2005) in which case the Visual Studio Conversion Wizard will convert the project to the new version. Note that for Visual Basic .NET, there was already a VB .NET 2005 sample program available.
- ProcessControl Structure added for standalone functionality (see section 3.6.6)
- Stability issues solved. Some spectrometer types (mainly the AvaSpec-102-USB2) have shown a lock up in continuous measurements over a long period at short integration time. Another problem that showed up very rarely, concerns multichannel spectrometers running in synchronization mode. Both problems have been solved in as5216.dll version 1.3.
- Support for the AvaSpec-2048x14 High UV-sensitivity back-thinned CCD Spectrometer. The new detector type used in this spectrometer is the HAMS9840 and is supported in as5216.dll version 1.3 and all the sample programs.
- The new function AVS_UseHighResAdc has been added to enable the full 16-bit ADC range which is available with a 16-bit ADC on the as5216 board as of revision 1D. See also section 2.3.36.
- A minor bug in the smoothing routine has been solved.
- The sample program in Visual Basic 6.0 has been modified because it crashed after running continuously for a number of hours. The cause was found to be in the VB6 "Timer" function that was used to show some statistics about the measurement speed. By eliminating the Timer function from the sample program, this problem was solved. Feedback from VB6 programmers who know how to use the Timer function (or an equivalent) without crashing the application is appreciated.

1.10   New in version 1.2.0.0

Visual Basic 6.0 developers may have noticed that the programs developed with as5216.dll v.1.1 or earlier and Visual Basic 6.0 are stable, but the Visual Basic 6.0 Integrated Development Environment (IDE) was not. Running the program from the VB6 IDE, caused the IDE to close down without saving any changes, as soon as the program was closed. To solve this problem, a special as5216.dll version (1.2.0.1) has been created which can be used in the VB6 IDE to develop and debug your programs. AS5216.dll version 1.2.0.1 will be installed in the VB6 example folder, as well as a readme.txt file with recommendations for redistributing programs developed with Visual Basic 6.0.
Furthermore, a parameter structure has been added to the EEProm to control the TEC cooling for the NIR spectrometer (AvaSpec-256-NIR2.2). More detailed information about this TEC Control structure can be found in section 3.6.5.
The last change in version 1.2 is only in this manual. For spectrometers that have been calibrated for irradiance measurements, the IrradianceType structure contains data that can be used to convert the ScopeData (A/D Counts) to an irradiance spectrum. Section 3.6.3 in this manual describes in more detail how this can be done.

1.11   New in version 1.1.0.0

The as5216.dll version 1.1 includes one new function (AVS_SetPrescanMode) which can be used for the AvaSpec-3648 spectrometer. Furthermore, a lower and upper limit has been added to the nonlinearity polynomial to avoid incorrect correction for very low and/or high counts. Finally, example programs with source in LabView (7.1), Visual C++ (6.0), Visual Basic (6.0) and Visual Basic .NET 2005 (2.0) have been added to the already existing examples in Delphi (6.0) and Borland C++ (5.0). The AVS_SetPrescanMode function for the AvaSpec-3648 is described in section 2.3.35, and detailed information about how to apply the nonlinearity correction can be found in section 3.6.1

1.12　　　New in version 1.0.0.0: as5216.dll versus as161.dll

Although there is no previous version for as5216.dll v1.0, a comparison can be made for programmers who have used the as161.dll to write application software for the USB1 platform AvaSpec spectrometers.

A number of improvements have been implemented in the as5216.dll when comparing the functions to the as161.dll. These improvements can be grouped into the following categories:

- Data acquisition
- Synchronization in multichannel systems
- Laser control and integration time delay, e.g. for Laser Induced Breakdown Spectroscopy
- USB2 platform spectrometer

These categories will be described in sections 1.12.1 to 1.12.4

1.12.1 Data acquisition

Just like with the as161.dll, a spectrum can be collected by calling the function AVS_Measure, and when a scan has been sent to the PC, it can be retrieved with the function AVS_GetScopeData. The following improvements have been realized in as5216x64.dll for the USB2 platform spectrometers:

1. **Starting a measurement**. In continuous mode, the USB1 platform spectrometers always run continuously, also if no measurement requests are posted. A call to AVS_Measure in as161.dll results in returning the first available scan (see section 2.2 of the as161.dll manual). The USB2 platform spectrometers are in idle mode if not scanning, and will start a scan if a measurement request (AVS_Measure) from the as5216x64.dll is received.
2. **Number of measurements**. The AVS_Measure function in as161.dll always results in one single scan. A spectrum is only sent to the PC if a measurement request is received. The AVS_Measure function in as5216x64.dll includes a "nrms" argument which specifies the number of measurements the spectrometer should perform after one measurement request.
3. **Stopping a measurement**. A measurement in as161.dll cannot be interrupted. After a measurement request, the application must wait for the response before changing measurement parameters or sending other commands to the spectrometer. The as5216x64.dll includes a function AVS_StopMeasure that can be called to interrupt a measurement request.
4. **Spectrometer not blocked while measurement is pending**. With the USB1 platform spectrometers, the spectrometer is blocked for receiving commands as long as a measurement is pending. A measurement is pending between the call to AVS_Measure and the DATA_READY message from the as161.dll to the application. The USB2 platform spectrometers are not blocked from receiving commands while a measurement is pending. This means that you can e.g. control the digital and analog IO ports while a measurement is pending.
5. **Measurement parameters**. There are a lot of parameters involved that determine the result of a scan such as integration time, number of averages, smoothing, pixelselection, dark correction etc... In the as161.dll, a lot of different functions are used to set these parameters: integration time and averaging are set in AVS_Measure, smoothing in AVS_SetSmoothing, Pixelselection in AVS_SetPixelSelection, etc… The as5216x64.dll uses a measurement structure which includes all measurement parameters and uses only one function (AVS_PrepareMeasure) to send these parameters to the spectrometer.
6. **External Trigger**. The only setting in the as161.dll for external trigger functionality is to switch this mode on or off by calling the function AVS_SetExternalTrigger. In external trigger mode, the USB1 platform spectrometer will start one single scan on the rising edge of the TTL pulse that is

sent to the external trigger input port of the spectrometer. In the as5216x64.dll, the USB2 platform spectrometer can be set into external trigger mode by setting the trigger mode parameter into hardware trigger mode. If the trigger type parameter is set to "EDGE", the number of measurements to perform after receiving one TTL pulse can be specified by setting the nrms parameter in the AVS_Measure function. If the trigger type parameter is set to "LEVEL", the spectrometer will keep scanning as long as the TTL input signal is HIGH, and when the signal becomes LOW, it will return the average scan over all scans that were performed during the HIGH time period.

7. **Integration time**. The integration time in the as161.dll can be set with a 1 ms resolution. In the as5216x64.dll, a 0.01 ms (10 µs) resolution is used for the integration time.

8. **Timestamp.** The AVS_GetScopeData function in as5216x64.dll includes a timestamp in 10 µs resolution ticks generated by the microcontroller, which can be used to measure the time between two consecutive (and processed) scans very accurately.

1.12.2 Synchronization in Multichannel systems

There is a major difference between the USB1 and USB2 platform multichannel systems. The USB1 platform multichannel systems always needs the same detectortype for each channel. Also, the integration time and number of averages in a measurement request is equal for all channels.

With the multiple usb support in the as161.dll (v.1.5 and later), spectrometers with different detectors and at different integration time or average can run simultaneously, but in that case there is no synchronization between these spectrometers.

With the USB2 platform multichannel systems, the advantage of the multiple USB implementation (up to 127 spectrometers, possibility of using different detectors, integration time and averaging per channel) has been combined with the advantage of the as161 multichannel systems (synchronization).

All USB2 platform spectrometers can be connected by a SYNC cable. In syncmode, one spectrometer is configured as "Master", all other ("slave") spectrometers are set into "Trigger by SYNC" mode. After a measurement request for the slave spectrometer(s), these spectrometers will wait until they receive the trigger signal on the SYNC cable. This SYNC signal will be started if a measurement request is posted for the Master spectrometer.

1.12.3 Laser control and integration time delay, e.g. for LIBS

If the AvaSpec-2048FT (USB1 platform) is set in external hardware trigger mode, an external trigger pulse results in an output signal (pulse width 15 µs) at pin2 of the DB15 connector (DO2), about 1.3 µs after the trigger pulse was received. The pulse at DO2 can be used to fire a laser in a LIBS application. The function AVS_SetIntegrationDelay can be used to specify an integration time delay, which is related to DO2.

With the AvaSpec-2048-USB2 and AvaSpec-3648-USB2, this feature has been improved at the following points:

1. **Not limited to external trigger mode**. The output signal and integration delay can be generated in external trigger mode, but also in "normal" (software trigger) mode.

2. **Multiple measurements**. The number of measurements can be set by the nrms parameter, in the AVS_Measure function.

3. **Pulse width**. The "laserpulse" width at pin 23 of the DB26 connector can be set by the user, between 0 and 1 ms (21 nanosec steps).

4. **Laser Delay**. The 1.3 µs period (for the AvaSpec-2048-USB2) between receiving a trigger (measurement request in software trigger mode or TTL pulse in hardware trigger mode) can be delayed from 1.3µs to 89 sec (21ns steps).

1.12.4 USB2 platform specific functions

The functions that have been added to as5216x64.dll to support the new hardware features in the USB2 platform spectrometers, can be grouped into the following categories:
- Analog IO
- Digital IO and Pulse Width Modulation
- SDCard support
- Eeprom IO

1. **Analog IO**. The USB2 platform spectrometers have 2 programmable analog output pins and 2 programmable analog input pins available at the DB26 connector. The functions AVS_SetAnalogOut and AVS_GetAnalogIn can be used to control these ports. Moreover, a number of onboard analog signals can be retrieved with the AVS_GetAnalogIn function. One of these onboard signals is an NTC thermistor which can be used for onboard temperature measurements.
2. **Digital IO and Pulse Width Modulation**. The USB2 platform spectrometers have 10 programmable digital output pins and 3 programmable input pins available at the DB26 connector. The function AVS_SetDigOut and AVS_GetDigIn can be used to control these ports. Moreover, 6 out of the 10 programmable ouput ports can be configured for pulse width modulation. With the AVS_SetPwmOut function, a frequency and duty cycle can be programmed for these 6 digital output ports
3. **SDCard support**. If the spectrometer was ordered with an SDxxx card, the function AVS_SaveSpectraToSDCard can be used to save spectra at the SDCard. To access the files that are saved at the SDCard, the functions AVS_GetFileSize, AVS_GetFile, AVS_GetFirstFile, AVS_GetNextFile and AVS_DeleteFile can be used.
4. **Eeprom IO**. With the USB1 platform spectrometers, it is also possible to read/write a number of parameters from/to Eeprom with the as161.dll, such as start- and stoppixel (AVS_GetStartStopPixel and AVS_SetStartStopPixel), wavelength calibration coefficients (AVS_GetWLCoef and AVS_SetWLCoef), gain (AVS_GetGain and AVS_SetGain) and offset (AVS_GetOffset and AVS_SetOffset). The Eeprom for the USB2 spectrometers has a lot more memory available to store all kind of parameters. These parameters have been defined in the DeviceConfigType structure (see section 2.4). The functions AVS_GetParameter and AVS_SetParameter in as5216x64.dll can be used to read/write the DeviceConfigType structure from/to Eeprom.

2   AS5216x64 DLL description

2.1 Interface overview

The interface from the PC to the DLL is based on a function interface. The interface allows the application to configure a spectrometer and to receive and send data from and to the spectrometer.

2.2 Usage of the AS5216x64 DLL

The DLL uses a single pair of open and close functions (AVS_Init() and AVS_Done()) that have to be called by an application. As long as the open function is not yet called or not successfully called, all other functions will return an error code.
The open function (AVS_Init()) tries to open a communication port for all connected devices.
The close function (AVS_Done()) closes the communication port(s) and releases all internal data storage.

The interface between the application and the DLL can be divided in four functional groups:
- internal data read functions, which read device configuration data from the internal DLL storage.
- blocking control functions which send a request to the device and wait till an answer is received or a time-out occurs before returning control to the application
- non-blocking data read functions, which send a request to the device and then return control to the application. After the answer from the device is received, or a timeout occurs a notification is sent to the application
- data send functions which send device configuration data to the device

After the application has initialised it should select the spectrometer(s) it wants to use. Therefore, the following steps have to be taken:
1. Call AVS_GetNrOfDevices to determine the number of attached devices
2. Allocate buffer to store identity info (RequiredSize = NrDevices * sizeof(AvsIdentityType))
3. Call AVS_GetList with the RequiredSize and obtain the list of connected spectrometers
4. Select the spectrometers you want to use with AVS_Activate
5. Register a notification window handle with AVS_Register to detect device attachment/removal.

2.3 Exported functions

2.3.1 AVS_Init

Function:	**int AVS_Init**
	(
	short a_Port
	)
Group:	Blocking control function
Description:	Opens the communication with the spectrometer and initialises internal data structures
Parameters:	a_Port: id. of port to be used:
	-1: use auto-detect of USB or COM port
	0: use USB port
	1: use COM1 port
	2: use COM2 port
	3: use COM3 port
	4: use COM4 port
	etc….
Return:	On success, number of connected devices
	On error, ERR_DEVICE_NOT_FOUND

2.3.2 AVS_Done

Function:	**int AVS_Done**
	(
	Void
	)
Group:	Blocking control function
Description:	Closes the communication and releases internal storage.
Parameters:	None
Return:	SUCCESS

2.3.3 AVS_GetNrOfDevices

Function:	**int AVS_GetNrOfDevices**
	(
	void
	)
Group:	Blocking control function
Description:	Internally checks the list of connected devices and returns the number of devices attached that have the status AVAILABLE.
Parameters:	None
Return:	> 0: number of devices in the list
	0: no devices found

2.3.4   AVS_GetList

Function: **int AVS_GetList**
                 (
                 unsigned int   a_ListSize,
                 unsigned int*   a_pRequiredSize,
                 AvsIdentityType*   a_pList
)

Group: Blocking control function
Description: Returns device information for each spectrometer connected to the ports indicated at AVS_Init.
Parameters: a_ListSize: number of bytes allocated by the caller to store the list data
              a_pRequiredSize: number of bytes needed to store information
              a_pList: pointer to allocated buffer to store identity information
Return: > 0:   number of devices in the list
              0:                   no devices found
              ERROR_INVALID_SIZE if (a_pRequiredSize > a_ListSize) then allocate larger buffer and retry operation

2.3.5   AVS_Activate

Function: **AvsHandle AVS_Activate**
                 (
                 AvsIdentityType*   a_pDeviceId
)

Group: Blocking control function
Description: Activates selected spectrometer for communication and reads device configuration data from Eeprom.
Parameters: On success: AvsHandle, handle to be used in subsequent function calls
Return: On error: INVALID_AVS_HANDLE_VALUE

2.3.6   AVS_Deactivate

Function: **bool AVS_Deactivate**
                 (
                 AvsHandle   a_hDeviceId
)

Group: Blocking control function
Description: Closes communication with selected spectrometer.
Parameters: a_hDeviceId: device identifier returned by AVS_Activate
Return: true: device successfully closed
              false: device identifier not found

2.3.7 AVS_Register

Function:	**bool AVS_Register**
	(
	HWND a_hWnd
	)
Group:	Blocking control function
Description:	Installs an application windows handle to which device attachment/removal messages have to be sent
Parameters:	a_hWnd: Application window handle
Return:	true: Registration successful
	false: registration failed or function not supported on OS

2.3.8 AVS_PrepareMeasure

Function:	**int AVS_PrepareMeasure**
	(
	AvsHandle a_hDevice,
	MeasConfigType* a_pMeasConfig
	)
Group:	Blocking data write function
Description:	Prepares measurement on the spectrometer using the specified measurement configuration.
Parameters:	a_hDevice: Device identifier returned by AVS_Activate
	a_pMeasConfig: pointer to structure containing measurement configuration
Return:	On success: ERR_SUCCESS
	On error: ERR_DEVICE_NOT_FOUND
	ERR_OPERATION_PENDING
	ERR_INVALID_DEVICE_ID
	ERR_INVALID_PARAMETER
	ERR_INVALID_PIXEL_RANGE
	ERR_INVALID_CONFIGURATION (invalid fpga type)
	ERR_TIMEOUT
	ERR_INVALID_MEASPARAM_DYNDARK

2.3.9 AVS_Measure

Function:	**int AVS_Measure**
	(
	AvsHandle a_hDevice,
	HWND a_hWnd,
	short a_Nmsr
	)
Group:	Non-Blocking data write function
Description:	Starts measurement on the spectrometer
Parameters:	a_hDevice: device identifier returned by AVS_Activate

| a_hWnd | window handle to notify application measurement result data is available. The DLL sends a message to the window with command WM_MEAS_READY, with SUCCESS, the number of scans that were saved in RAM (if StoreToRAM parameter > 0), or INVALID_MEAS_DATA as WPARM value and a_hDevice as LPARM value. |
| a_Nmsr | number of measurements to do after one single call to AVS_Measure (-1 is infinite) |

Return: On success: ERR_SUCCESS
            On error: ERR_OPERATION_PENDING
                              ERR_DEVICE_NOT_FOUND
                              ERR_INVALID_DEVICE_ID
                              ERR_INVALID_PARAMETER
                              ERR_INVALID_STATE

2.3.10 AVS_GetLambda

Function: **int AVS_GetLambda**
                (
                AvsHandle   a_hDevice,
                double*   a_pWavelength
)

Group: Internal data read function
Description: Returns the wavelength values corresponding to the pixels if available. This information is stored in the DLL during the AVS_Activate() procedure.
                The DLL does not test if a_pWaveLength is correctly allocated by the caller!
Parameters: a_hDevice: device identifier returned by AVS_Activate
                a_pWaveLength: array of double, with array size equal to number of pixels
Return: On success: ERR_SUCCESS
            On error: ERR_DEVICE_NOT_FOUND
                              ERR_INVALID_DEVICE_ID

2.3.11 AVS_GetNumPixels

Function: int AVS_GetNumPixels
                (
                AvsHandle   a_hDevice,
                unsigned short*   a_pNumPixels
)

Group: Internal data read function
Description: Returns the number of pixels of a spectrometer. This information is stored in the DLL during the AVS_Activate() procedure.
Parameters: a_hDevice: device identifier returned by AVS_Activate
                a_pNumPixels: pointer to unsigned integer to store number of pixels
Return: On success: ERR_SUCCESS
            On error: ERR_DEVICE_NOT_FOUND
                              ERR_INVALID_DEVICE_ID

2.3.12 AVS_GetParameter

Function:	**int AVS_GetParameter**	
	(	
	AvsHandle	a_hDevice,
	unsigned int	a_Size,
	unsigned int*	a_pRequiredSize,
	DeviceConfigType*	a_pData
	)	
Group:	Internal data read function.	
Description:	Returns the device information of the spectrometer. This information is stored in the DLL during the AVS_Activate() procedure.	
Parameters:	a_hDevice,	device identifier returned by AVS_Activate
	a_Size,	number of bytes allocated by caller to store DeviceConfigType
	a_pRequiredSize,	number of bytes needed to store DeviceConfigType
	a_pData	pointer to buffer that will be filled with the spectrometer configuration data
Return:	On success:	ERR_SUCCESS
	On error:	ERR_DEVICE_NOT_FOUND
		ERR_INVALID_DEVICE_ID
		ERR_INVALID_SIZE (a_Size is smaller than required size)

2.3.13 AVS_PollScan

Function:	**int AVS_PollScan**	
	(	
	AvsHandle	a_hDevice
	)	
Group:	Internal data read function	
Description:	Determines if new measurement results are available	
	The most effective way to let the application know when a new measurement is ready, is by using Windows Messaging in which case the as5216x64.dll sends a WM_MEAS_READY message to the application as soon as a measurement is ready to be imported into the application software (see also section 2.4.2). But if the programming environment does not support Windows Messaging, it is also possible to use AVS_PollScan for this purpose. After a measurement request has been posted by calling AVS_Measure, the function AVS_PollScan can be called in a loop until it returns "1". Note that it should be avoided that AVS_PollScan is called continuously without any delay. This can cause such a heavy CPU load that this can freeze the application software after a while. Adding a 1 millisecond delay (so polling every ms) already solves this problem.	
Parameters:	a_hDevice::	device identifier returned by AVS_Activate
Return:	On success:	0: no data available
		1: data available
	On error:	ERR_DEVICE_NOT_FOUND
		ERR_INVALID_DEVICE_ID

2.3.14 AVS_GetScopeData

Function: **int AVS_GetScopeData**

         (

AvsHandle	a_hDevice,
unsigned int*	a_pTimeLabel,
double*	a_pSpectrum

)

Group: Internal data read function,

Description: Returns the pixel values of the last performed measurement. Should be called by the application after the notification on AVS_Measure is triggered.
The DLL does not check the allocated buffer size!

Parameters:	a_hDevice,	device identifier returned by AVS_Activate
	a_pTimeLabel,	ticks count last pixel of spectrum is received by microcontroller ticks in 10 μS units since spectrometer started
	a_pSpectrum	array of doubles, size equal to the selected pixelrange
Return:	On success:	ERR_SUCCESS
	On error:	ERR_DEVICE_NOT_FOUND
		ERR_INVALID_DEVICE_ID
		ERR_INVALID_MEAS_DATA (no measurement data received)

2.3.15 AVS_GetSaturatedPixels

Function: **int AVS_GetSaturatedPixels**

         (

AvsHandle	a_hDevice,
unsigned char*	a_pSaturated

)

Group: Internal data read function,

Description: Returns for each pixel if that pixel was saturated (1) or not (0). Should be called by the application after the notification on AVS_Measure is triggered (e.g. after calling AVS_GetScopeData which also requires that valid data is available)

Parameters:	a_hDevice	device identifier returned by AVS_Activate
	a_pSaturated	array of chars (each char indicates if saturation occurred for corresponding pixel), size equal to the selected pixelrange
Return:	On success:	1 (valid measurement available)
	On error:	0 (no measurement data available)
		ERR_DEVICE_NOT_FOUND
		ERR_INVALID_DEVICE_ID

2.3.16 AVS_GetAnalogIn

Function: **int AVS_GetAnalogIn**

         (

AvsHandle	a_hDevice,
unsigned char	a_AnalogInId,
float*	a_pAnalogIn

)

Group: Blocking control function.
Description: Returns the status of the specified analog input
Parameters: a_hDevice: device identifier returned by AVS_Activate
                a_AnalogInId   identifier of analog input
                                  0 = thermistor on optical bench (NIR 2.0 / NIR2.2 / NIR 2.5 / TEC)
                                  1 = 1V2
                                  2 = 5VIO
                                  3 = 5VUSB
                                  4 = AI2 = pin 18 at 26-pins connector
                                  5 = AI1 = pin 9 at 26-pins connector
                                  6 = NTC1 onboard thermistor
                                  7 = Not used
                a_pAnalogIn: pointer to float for analog input value [Volts]
Return: On success: ERR_SUCCESS
                On error: ERR_DEVICE_NOT_FOUND
                                  ERR_INVALID_DEVICE_ID
                                  ERR_INVALID_PARAMETER (invalid analog input id.)
                                  ERR_TIMEOUT (error in communication)

2.3.17 AVS_GetDigIn

Function: int AVS_GetDigIn
                (
                AvsHandle   a_hDevice,

                unsigned char   a_DigInId,
                unsigned char*   a_pDigIn
)
Group: Blocking control function.
Description: Returns the status of the specified digital input
Parameters: a_hDevice: device identifier returned by AVS_Activate
                a_DigInId: identifier of digital input (1 – 3)
                                  0 = DI1 = Pin 24 at 26-pins connector
                                  1 = DI2 = Pin 7 at 26-pins connector
                                  2 = DI3 = Pin 16 at 26-pins connector

                a_pDigIn: pointer to digital input status (0 – 1)
Return: On success: ERR_SUCCESS, a_pDigIn contains valid value
                On error: ERR_DEVICE_NOT_FOUND
                                  ERR_INVALID_DEVICE_ID
                                  ERR_INVALID_PARAMETER (invalid digital input id.)
                                  ERR_TIMEOUT (error in communication)

2.3.18 AVS_GetVersionInfo

Function: int AVS_GetVersionInfo
                (
                AvsHandle   a_hDevice,

                unsigned char*   a_pFPGAVersion,
                unsigned char*   a_pFirmwareVersion,
                unsigned char*   a_pDLLVersion

)

Group:	Blocking read function	
Description:	Returns the status of the software version of the different parts. DLL does not check the size of the buffers allocated by the caller.	
Parameters:	a_hDevice,	device identifier returned by AVS_Activate
	a_pFPGAVersion,	pointer to buffer to store FPGA software version (16 char.)
	a_pFirmwareVersion	pointer to buffer to store Microcontroller software version (16 char.)
	a_pDLLVersion	pointer to buffer to store DLL software version (16 char.)
Return:	On success:	ERR_SUCCESS, buffer contains valid value
	On error:	ERR_DEVICE_NOT_FOUND
		ERR_INVALID_DEVICE_ID
		ERR_TIMEOUT (error in communication)

2.3.19 AVS_GetFileSize

Function: **int AVS_GetFileSize**

(
AvsHandle	a_hDevice,
unsigned char*	a_pName,
unsigned int*	a_pSize

)

Group:	Blocking read function	
Description:	Returns the file size in bytes if the file can be read from the SD card	
Parameters:	a_hDevice:	device identifier returned by AVS_Activate
	a_pName:	file name (14 characters including terminating zero)
	a_pSize:	pointer to buffer to store length
Return:	On success:	ERR_SUCCESS, buffer contains valid value
	On error:	ERR_DEVICE_NOT_FOUND
		ERR_INVALID_DEVICE_ID
		ERR_TIMEOUT (error in communication)
		ERR_INVALID_PARAMETER, no SD card present or file not found

2.3.20 AVS_GetFile

Function: **int AVS_GetFile**

(
AvsHandle	a_hDevice,
unsigned char*	a_pName,
unsigned char	a_pDest,
unsigned int	a_pSize

)

Group:	Blocking read function	
Description:	Returns the contents of a binary file from the SD card	
Parameters:	a_hDevice	device identifier returned by AVS_Activate
	a_pName	file name (14 characters including terminating zero)
	a_pDest	pointer to buffer to store binary file data
	a_pSize	length of buffer (expected file size, as determined with AVS_GetFileSize, max. length is 64kB)

AS-5216x64-DLL Manual.docx   Jun-12

Return: On success: ERR_SUCCESS, buffer contains valid value
On error: ERR_DEVICE_NOT_FOUND
ERR_INVALID_DEVICE_ID
ERR_TIMEOUT (error in communication)
ERR_INVALID_PARAMETER, no SD card present or file not found

2.3.21 AVS_GetFirstFile

Function:	**int AVS_GetFirstFile**	
	(	
	AvsHandle	a_hDevice,
	unsigned char*	a_pName
	)	
Group:	Blocking read function	
Description:	Returns the name of the first file in the root directory of the SD card	
Parameters:	a_hDevice,	device identifier returned by AVS_Activate
	a_pName	file name (14 characters including terminating zero)
Return:	On success:	ERR_SUCCESS, buffer contains valid value
	On error:	ERR_DEVICE_NOT_FOUND
		ERR_INVALID_DEVICE_ID
		ERR_TIMEOUT (error in communication)
		ERR_INVALID_PARAMETER, no SD card present or file not found

2.3.22 AVS_GetNextFile

Function:	**int AVS_GetNextFile**	
	(	
	AvsHandle	a_hDevice,
	unsigned char*	a_pPrevName,
	unsigned char*	a_pNextName
	)	
Group:	Blocking read function	
Description:	Returns the name of the next file in root directory after a_pPrevName	
Parameters:	a_hDevice	device identifier returned by AVS_Activate
	a_pPrevName	file name (14 characters including terminating zero), this is the name returned by AVS_GetFirstFile() or by the previous call to AVS_GetNextFile()
	a_pNextName	file name (14 characters including terminating zero)
Return:	On success:	ERR_SUCCESS, buffer contains valid value
	On error:	ERR_DEVICE_NOT_FOUND
		ERR_INVALID_DEVICE_ID
		ERR_TIMEOUT (error in communication)
		ERR_INVALID_PARAMETER, no SD card present or no more files on the SD card

2.3.23 AVS_DeleteFile

Function: **int AVS_DeleteFile**

(

AvsHandle	a_hDevice,
unsigned char*	a_pName

)

Group:	Blocking read function
Description:	Deletes a file from the SD card
Parameters:	a_hDevice	device identifier returned by AVS_Activate
	a_pName	file name (14 characters including terminating zero)
Return:	On success:	ERR_SUCCESS
	On error:	ERR_DEVICE_NOT_FOUND
		ERR_INVALID_DEVICE_ID
		ERR_TIMEOUT (error in communication)
		ERR_INVALID_PARAMETER, no SD card present or no more files on the SD card

2.3.24 AVS_GetFirstDirectory

Function: **int AVS_GetFirstDirectory**

(

AvsHandle	a_hDevice,
unsigned char*	a_pName

)

Group:	Blocking read function
Description:	Returns the name of the directory in the root directory of the SD card
Parameters:	a_hDevice	device identifier returned by AVS_Activate (-1 for first active device)
	a_pName:	directory name (14 characters including terminating zero)
Return:	On success:	ERR_SUCCESS (a_pName buffer contains valid info)
	On error:	ERR_DEVICE_NOT_FOUND (communication not open yet)
		ERR_INVALID_DEVICE_ID (device handle is not known in DLL)
		ERR_TIMEOUT (error in communication)
		ERR_INVALID_PARAMETER, no SD card present or no directory found on the SD card

2.3.25 AVS_GetNextDirectory

Function: **int AVS_GetNextDirectory**

(

AvsHandle	a_hDevice,
unsigned char*	a_pPrevName,
unsigned char*	a_pNextName

)

Group:	Blocking read function
Description:	Returns the name of the next directory in the root directory after a_pPrevName
Parameters:	a_hDevice	device identifier returned by AVS_Activate (-1 for first active device)
	a_pPrevName	directory name (14 characters including terminating zero), this is the name returned by AVS_GetFirstDirectory() or by the previous call to

		AVS_GetNextDirectory()
	a_pNextName	directory name (14 characters including terminating zero)
Return:	On success:	ERR_SUCCESS, a_pNextName contains valid value
	On error:	ERR_DEVICE_NOT_FOUND (communication not open yet)
		ERR_INVALID_DEVICE_ID (device handle is not known in DLL)
		ERR_TIMEOUT (error in communication)
		ERR_INVALID_PARAMETER, no SD card present or no more directories on the SD card

2.3.26 AVS_DeleteDirectory

Function:	**int AVS_DeleteDirectory**	
	(	
	AvsHandle	a_hDevice,
	unsigned char*	a_pName
	)	
Group:	Blocking read function	
Description:	Deletes a directory from the SD card	
Parameters:	a_hDevice	device identifier returned by AVS_Activate (-1 for first active device)
	a_pName	directory name (14 characters including terminating zero)
Return:	On success:	ERR_SUCCESS
	On error:	ERR_DEVICE_NOT_FOUND (communication not open yet)
		ERR_INVALID_DEVICE_ID (device handle is not known in DLL)
		ERR_TIMEOUT (error in communication)
		ERR_INVALID_PARAMETER, no SD card present or no more directories on the SD card

2.3.27 AVS_SetDirectory

Function:	**int AVS_SetDirectory**	
	(	
	AvsHandle	a_hDevice,
	char	a_aFileRootName[6]
	)	
Group:	Blocking data send function	
Description:	Sets current working directory. All file-functions will act on this directory.	
Parameters:	a_hDevice	device identifier returned by AVS_Activate (-1 for first active device)
	a_aFileRootName	string that sets the current working directory for all file-based functions
Return:	On success:	ERR_SUCCESS
	On error:	ERR_DEVICE_NOT_FOUND (communication not open yet)
		ERR_INVALID_DEVICE_ID (device handle is not known in DLL)
		ERR_TIMEOUT (error in communication)
		ERR_INVALID_PARAMETER, no SD card present

2.3.28   AVS_SaveSpectraToSDCard

Function:	**int AVS_SaveSpectraToSDCard**	
	(	
	AvsHandle	a_hDevice,
	bool	a_Enable,
	unsigned char	a_SpectrumType,
	char	a_aFileRootName[6],
	TimeStampType	a_TimeStamp
	)	
Group:	Blocking data send function.	
Description:	Enables/disables writing spectra to file (if disabled the other parameters are neglected)	
Parameters:	a_hDevice	device identifier returned by AVS_Activate
	a_Enable	enable/disable storage of spectra to SD card
	a_SpectrumType	0 = Dark Spectrum
		1 = Reference Spectrum
		2 = Normal Spectrum
		The spectrumtype determines the file extension (drk, ref or roh)
	a_aFileRootName[6]	string that is used as first part of the name of the stored spectra
	a_TimeStamp	file time and date that will be used when the spectra are stored
Return:	On success:	ERR_SUCCESS
	On error:	ERR_DEVICE_NOT_FOUND
		ERR_INVALID_DEVICE_ID
		ERR_TIMEOUT (error in communication)
		ERR_INVALID_PARAMETER
		ERR_OPERATION_NOT_SUPPORTED (SD Card not present)

2.3.29 AVS_SetParameter

Function:	**int AVS_SetParameter**	
	(	
	AvsHandle	a_hDevice,
	DeviceConfigType*	a_pData
	)	
Group:	Blocking data send function.	
Description:	Overwrites the device configuration data internally and in the spectrometer. The data is not checked.	
Parameters:	a_hDevice,	device identifier returned by AVS_Activate
	a_pData	pointer to a DeviceConfigType structure
Return:	On success:	ERR_SUCCESS
	On error:	ERR_DEVICE_NOT_FOUND
		ERR_INVALID_DEVICE_ID
		ERR_TIMEOUT (error in communication)
		ERR_OPERATION_PENDING
		ERR_INVALID_STATE (measurement pending)

2.3.30 AVS_SetAnalogOut

Function:	**int AVS_SetAnalogOut**	
	(	
	AvsHandle	a_hDevice,
	unsigned char	a_PortId,
	float	a_Value
	)	
Group:	Blocking data send function	
Description:	Sets the analog output value for the specified analog output	
Parameters:	a_hDevice	device identifier returned by AVS_Activate
	a_PortId,	identifier for one of the two output signals:
		0 = AO1 = pin 17 at 26-pins connector
		1 = AO2 = pin 26 at 26-pins connector
	a_Value	DAC value to be set in Volts (internally an 8-bits DAC is used) with range 0 – 5.0V
Return:	On success:	ERR_SUCCESS
	On error:	ERR_DEVICE_NOT_FOUND
		ERR_INVALID_DEVICE_ID
		ERR_TIMEOUT (error in communication)
		ERR_INVALID_PARAMETER

2.3.31 AVS_SetDigOut

Function:	**int AVS_SetDigOut**	
	(	
	AvsHandle	a_hDevice
	unsigned char	a_PortId,
	unsigned char	a_Value
	)	
Group:	Blocking data send function.	

Description: Sets the digital output value for the specified digital output
Parameters: a_hDevice   device identifier returned by AVS_Activate
              a_PortId: identifier for one of the 10 output signals:
                               0 = DO1 = pin 11 at 26-pins connector
                               1 = DO2 = pin 2 at 26-pins connector
                               2 = DO3 = pin 20 at 26-pins connector
                               3 = DO4 = pin 12 at 26-pins connector
                               4 = DO5 = pin 3 at 26-pins connector
                               5 = DO6 = pin 21 at 26-pins connector
                               6 = DO7 = pin 13 at 26-pins connector
                               7 = DO8 = pin 4 at 26-pins connector
                               8 = DO9 = pin 22 at 26-pins connector
                               9 = DO10 = pin 25 at 26-pins connector
              a_Value: value to be set (0-1)
Return: On success: ERR_SUCCESS
              On error: ERR_DEVICE_NOT_FOUND
                               ERR_INVALID_DEVICE_ID
                               ERR_TIMEOUT (error in communication)
                               ERR_INVALID_PARAMETER

2.3.32   AVS_SetPwmOut

Function: **int AVS_SetPwmOut**
                 (
                 AvsHandle   a_hDevice,
                 unsigned char   a_PortId,
                 unsigned long   a_Frequency,
                 unsigned char   a_DutyCycle
)
Group: Blocking data send function.
Description: Selects the PWM functionality for the specified digital output
Parameters: a_hDevice,   device identifier returned by AVS_Activate
              a_PortId   identifier for one of the 6 PWM output signals:
                               0 = DO1 = pin 11 at 26-pins connector
                               1 = DO2 = pin 2 at 26-pins connector
                               2 = DO3 = pin 20 at 26-pins connector
                               4 = DO5 = pin 3 at 26-pins connector
                               5 = DO6 = pin 21 at 26-pins connector
                               6 = DO7 = pin 13 at 26-pins connector
              a_Frequency   desired PWM frequency (500 – 300000) [Hz], the frequency of
                               outputs 0, 1 and 2 is the same (the last specified frequency is used),
                               also the frequency of outputs 4, 5 and 6 is the same
              a_DutyCycle   percentage high time in one cycle (0 – 100), channels 0, 1 and 2 have a
                               synchronised rising edge, the same holds for channels 4, 5 and 6
Return: On success: ERR_SUCCESS
              On error: ERR_DEVICE_NOT_FOUND
                               ERR_INVALID_DEVICE_ID
                               ERR_TIMEOUT (error in communication)
                               ERR_INVALID_PARAMETER

2.3.33 AVS_SetSyncMode

Function: **int AVS_SetSyncMode**
(
AvsHandle a_hDevice,
unsigned char a_Enable
)

Group: Internal DLL write function

Description Disables/enables support for synchronous measurement. DLL takes care of dividing Nmsr request into Nmsr number of single measurement requests.

Parameters a_hDevice master device identifier returned by AVS_Activate
     a_Enable 0 is disable sync mode, 1 is enables sync mode
Return: On success: ERR_SUCCESS
     On error: ERR_DEVICE_NOT_FOUND
          ERR_INVALID_DEVICE_ID

2.3.34 AVS_StopMeasure

Function: **int AVS_StopMeasure**
(
AvsHandle a_hDevice
)

Group: Blocking data send function

Description: Stops the measurements (needed if Nmsr = infinite), can also be used to stop a pending measurement with long integrationtime and/or high number of averages

Parameters: a_hDevice: device identifier returned by AVS_Activate
Return: On success: ERR_SUCCESS
      On error: ERR_DEVICE_NOT_FOUND
           ERR_INVALID_DEVICE_ID
           ERR_TIMEOUT (error in communication)
           ERR_INVALID_PARAMETER

2.3.35 AVS_SetPrescanMode

Function:	**int AVS_SetPrescanMode**
	(
	AvsHandle a_hDevice
	bool a_Prescan
	)
Group:	Blocking data send function
Description:	If a_Prescan is set, the first measurement result will be skipped. This function is only useful for the AvaSpec-3648 because this detector can be operated in prescan mode, or clearbuffer mode (see below)
Parameters:	a_hDevice: device identifier returned by AVS_Activate
	a_Prescan: If true, the first measurement result will be skipped (prescan mode), else the detector will be cleared before each new scan (clearbuffer mode)
Return:	On success: ERR_SUCCESS
	On error: ERR_DEVICE_NOT_FOUND
	ERR_INVALID_DEVICE_ID
	ERR_TIMEOUT (error in communication)

The Toshiba detector in the AvaSpec-3648, can be used in 2 different control modes:

The Prescan mode (default mode).

In this mode the Toshiba detector will automatically generate an additional prescan for every request from the PC, the first scan contains non-linear data and will be rejected, the 2nd scan contains linear data and will be sent to the PC. This prescan mode is default and should be used in most applications, like with averaging (only one prescan is generated for a nr of averages), with the use of an AvaLight-XE (one or more flashes per scan) and with multichannel spectrometers. The advantage of this mode is a very stable and linear spectrum. The disadvantage of this mode is that a minor (<5%) image of the previous scan (ghostspectrum) is included in the signal. This mode cannot be used if the integration time cycle needs to start within microseconds after the spectrometer is externally triggered, but since the prescan duration is exactly known at each integration time, accurate timing (21 nanoseconds precision in external trigger mode) is very well possible in prescan mode.

The Clear-Buffer mode.

In this mode the Toshiba detector buffer will be cleared, before a scan is taken. This clear-buffer mode should be used when timing is important, like with fast external triggering. The advantage of this mode is that a scan will start at the time of an external trigger, the disadvantage of this mode is that after clearing the buffer, the detector will have a minor threshold, in which small signals (<500 counts) will not appear and with different integration times the detector is not linear.

2.3.36 AVS_UseHighResAdc

Function:	**int AVS_UseHighResAdc** (AvsHandle a_hDevice bool a_Enable)
Group:	Internal DLL write function
Description:	With the as5216 electronic board revision 1D and later, a 16bit resolution AD Converter is used instead of a 14bit in earlier hardware versions. As a result, the ADC Counts scale can be set to the full 16 bit (0..65535) Counts. For compatibility reasons with previous hardware revisions, the default range is set to 14 bit (0..16383.75) ADC Counts.
Remark:	When using the 16 bit ADC in full High Resolution mode (0..65535), please note that the irradiance intensity calibration, as well as the nonlinearity calibration are based on the 14bit ADC range. Therefore, if using the nonlinearity correction or irradiance calibration in your own software using the High Resolution mode, you need to apply the additional correction with ADCFactor (= 4.0), as explained in detail in section 3.6.1 and 3.6.3

Parameters:	a_hDevice:	device identifier returned by AVS_Activate
	a_Enable:	True: use 16bit resolution, ADC Counts range 0..65535
		False: use 14bit resolution ADC Counts range 0..16383.75
Return:	On success:	ERR_SUCCESS
	On error:	ERR_OPERATION_NOT_SUPPORTED: this function is not supported by as5216 hardware version R1C or earlier

2.3.37 AVS_SetSensitivityMode

Function: **int AVS_SetSensitivityMode**
(
AvsHandle   a_hDevice

unsigned int   a_SensitivityMode

)

Group: Blocking data send function

Description: The AvaSpec-NIR models can be operated in LowNoise (a_SensitivityMode = 0) or High
Sensitivity Mode (a_SensitivityMode > 0).

Parameters: a_hDevice: device identifier returned by AVS_Activate
a_SensitivityMode: 0 = LowNoise, >0 = High Sensitivity

Return: On success: ERR_SUCCESS
On error: ERR_DEVICE_NOT_FOUND
ERR_INVALID_DEVICE_ID
ERR_TIMEOUT (error in communication)
ERR_NOT_SUPPORTED_BY_SENSOR_TYPE
ERR_NOT_SUPPORTED_BY_FW_VER
ERR_NOT_SUPPORTED_BY_FPGA_VER

Remark: AVS_SetSensitivityMode is supported by the following detector types: HAMS9201,
SU256LSB and SU512LDB. Calling this function for another detectortype will result in a
return value of -120 (ERR_NOT_SUPPORTED_BY_SENSOR_TYPE)
This function requires a firmware function x.30.x.x or later. Calling this function for a
spectrometer for which an older firmware version is loaded will result in a return value of
-121 (ERR_NOT_SUPPORTED_BY_FW_VER).
The detector specific FPGA needs to support the sensitivity selection feature as well. The
table below shows the minimum required version for the 3 detector types. Calling
AVS_SetSensitivityMode for a spectrometer for which an older FPGA version is loaded
will result in a return value of -122 (ERR_NOT_SUPPORTED_BY_FPGA_VER).
The table below also lists the Default Mode for each detector type. This is the mode in
which the detector operates if the function AVS_SetSensitivityMode is not called. The
default mode is also the mode that is used in models with older firmware and FPGA
versions. Note that irradiance calibrated systems are calibrated in the default mode.
Changing the sensitivity mode for an irradiance and/or nonlinearity calibrated system
requires a recalibration of the system.

Spectrometer	Detector Type	FPGA version	Default Mode
AvaSpec-NIR256-1.7, AvaSpec-NIR256-2.0TEC, AvaSpec-NIR256-2.5TEC	SENS_HAMS9201	x.13.x.x	Low Noise
AvaSpec-NIR256-1.7TEC, AvaSpec-NIR256-2.2TEC	SENS_SU256LSB	x.5.x.x	High Sensitivity
AvaSpec-NIR512-1.7TEC AvaSpec-NIR512-2.2TEC	SENS_SU512LDB	x.4.x.x	High Sensitivity

2.4 Data Elements

Several data-types used by the DLL and necessary for the application interface are given below.

Note: To match the structures that are used in the AS5216 firmware the structures mentioned here have to be compiled with *byte alignment*.

Table 1 API data elements

Type	Format	Value/Range	Description
bool	8 bits value	0 – 1	false - true
char	8 bits value	-128 <= x <= 127	signed character
unsigned char	8 bits value	0 <= x <= 255	unsigned character
short	16 bits value	-32768 <= x <= 32767	signed integer
unsigned short	16 bits value	0 <= x <= 65535	unsigned integer
int	32 bits value	2,147,483,648 <= x <= 2,147,483,647	signed integer
unsigned int	32 bits value	0 <= x <= 4294967295	unsigned integer
float	32 bits value		floating point number (7 digits precision)
double	64 bits value		double sized floating point number (15 digits precision)
HWND	32 bits value		Windows typedef for window identification, HWND is used for Windows API calls that require a Window handle.

AvsIdentity Type	struct
	{
	char m_aSerialId[10],
	char m_aUserFriendlyId[64],
	DeviceStatus m_Status
	}
			
			serial identification number
			user friendly name to be defined by application
			device status
			(Size = 75 bytes)

Type	Format	Value/Range	Description

ControlSettings Type	struct
	{
	
	unsigned short m_StrobeControl,
	
	unsigned int m_LaserDelay,
	unsigned int m_LaserWidth,
	
	float m_LaserWaveLength
	unsigned short m_StoreToRam,
	
	}
		0 – 0xFFFF
		
		0 – 0xFFFFFFFF
		0 – 0xFFFF
		
		0 – 0xFFFF
			number of strobe pulses during integration period (high time of pulse is 1 ms), (0 = no strobe pulses)
			laser delay since trigger, unit is internal FPGA clock cycle
			laser pulse width , unit is internal FPGA clock cycle
			        (0 = no laser pulse)
			Peak wavelength of laser (nm), used for Raman Spectroscopy
			0 = no storage to RAM
			> 0 = number of spectra to be stored
			
			(Size = 16 bytes)

DarkCorrection Type	struct
	{
	unsigned char m_Enable,
	unsigned char m_ForgetPercentage
	
	}
		0 – 1
		0 - 100
			disable – enable dynamic dark correction (sensor dependent)
			percentage of the new dark value pixels that has to be used. e.g., a percentage of 100 means only new dark values are used. A percentage of 10 means that 10 percent of the new dark values is used and 90 percent of the old values is used for drift correction
			(Size = 2 bytes)

Type	Format	Value/Range	Description

DeviceConfig Type	struct
	{
	unsigned short m_Len,
	unsigned short m_ConfigVersion,
	char m_aUserFriendlyId[64]
	DetectorType m_Detector,
	IrradianceType m_Irradiance,
	SpectrumCalibrationType m_Reflectance,
	SpectrumCorrectionType m_SpectrumCorrect,
	StandaloneTypem_StandAlone,
	TempSensorType m_Temperature[3],
	TecControlType m_TecControl
	ProcessControlType m_ProcessControl
	unsigned char m_aReserved[13832]
	}
		0 – 0xFFFF	Configuration data structure:
			
			size of this structure in bytes
			version of this structure
			user friendly identification string
			sensor/detector related parameters
			intensity calibration parameters
			reflectance calibration parameters
			correction parameters
			stand-alone related parameters (e.g. measure mode, control)
			calibration parameters of three temperature sensors
			TecControl parameters
			ProcessControl parameters
			makes structure size equal to 63484 bytes
			(Size = 63484)

DeviceStatus	enum
	{
	UNKNOWN,
	AVAILABLE,
	IN_USE_BY_APPLICATION,
	IN_USE_BY_OTHER
	}
		
		0
		1
		2
		3
			
			initial state
			device is connected to PC and not in use
			device is connected to PC and in use by caller
			device is connected to PC and in use by other application

Type	Format	Value/Range	Description

DetectorType	struct
	{
	
	SensorType m_SensorType,
	unsigned short m_NrPixels,
	float m_aFit[5],
	bool m_NLEnable,
	double m_aNLCorrect[8],
	double m_aLowNLCounts,
	double m_aHighNLCounts,
	float m_Gain[2],
	
	float m_Reserved,
	float m_Offset[2],
	
	float m_ExtOffset,
	unsigned short m_DefectivePixels[30],
	}
		
		0 – 4096
		
		1 – 5.7
		
		-0.350 - +0.350
		
		0.0 – 2.0
			Sensor configuration structure:
			
			sensor identification
			number of pixels of sensor
			polynomial coefficients needed to determine wavelength
			enable/disable nonlinearity correction
			polynomial coefficients needed for non linearity correction
			lower counts limit for nonlinearity correction
			higher counts limit for nonlinearity correction
			gain correction for spectrometer ADC (range is divided in 64 steps)
			not used
			offset correction for spectrometer ADC in Volt (range is divided in 512 steps)
			offset to match the detector output range with the ADC range
			defective pixel numbers
			
			(Size = 188 bytes)

IrradianceType	struct
	{
	
	SpectrumCalibrationType m_IntensityCalib,
	unsigned char m_CalibrationType,
	unsigned int m_FiberDiameter,
	}
			
			Setting during intensity calibration
			Bare fiber, diffusor, integrating sphere, ….
			Fiber diameter during intensity calibration
			(Size = 16391+1+4 = 16396 bytes)

Type	Format	Value/Range	Description

MeasConfig Type	struct
	{
	unsigned short m_StartPixel,
	unsigned short m_StopPixel,
	float m_IntegrationTime,
	unsigned int m_IntegrationDelay,
	
	unsigned int m_NrAverages,
	DarkCorrectionType m_CorDynDark,
	SmoothingType m_Smoothing,
	unsigned char m_SaturationDetection,
	
	TriggerType m_Trigger,
	ControlSettingsType m_Control,
	}
		0-4095
		0 – 4095
		0.002 – 600000
		0 – 0xFFFFFFFF
		
		1 – 0xFFFFFFFF
		
		0 – 2
			first pixel to be sent to PC
			last pixel to be sent to PC
			integration time in ms
			integration delay, unit is internal FPGA clock cycle
			      (0 = one unit before laser start)
			number of averages in a single measurement
			 dynamic dark correction parameters
			smoothing parameters
			 0 = disabled,
			 1 = enabled, determines during each measurement if pixels are saturated (ADC value = $2^{16} -1$)
			 2 = enabled, and also corrects inverted pixels (only ILX554)
			trigger parameters
			control parameters
			(Size = 41 bytes)

ProcessControl Type	struct
	{
	float m_AnalogLow[2]
	float m_AnalogHigh[2]
	float m_DigitalLow[10]
	float m_DigitalHigh[10]
	}
			Settings that can be used for the 2 analog and 10 digital output signals at the DB26 connector. The analog settings can be used to define a function output range that should correspond to the 0-5V range of the analog output signals.
			The digital output settings can be used as lower- and upper thresholds.
			(Size 96 bytes)

SDCardType	Struct
	{
	bool m_Enable,
	unsigned char m_SpectrumType,
	char m_aFileRootName[6],
	TimeStampType m_TimeStamp
	}
			Settings for SD Card, needed in stand-alone operation
			
			(Size = 12 bytes)

Type	Format	Value/Range	Description
SensorType	unsigned char	0 – 0x12	0x00 = Reserved 0x01 = Hams8378-256 0x02 = Hams8378-1024 0x03 = ILX554 0x04 = Hams9201 0x05 = Toshiba TCD1304 0x06 = TSL1301 0x07 = TSL1401 0x08 = Hams8378-512 0x09 = Hams9840 0x0A = ILX511 0x0B = Hams10420-2048x64 0x0C = Hams11071-2048x64 0x0D = Hams7031-1024x122 0x0E = Hams7031-1024x58 0x0F = Hams11071-2048x16 0x10 = Hams11155 0x11 = SU256LSB 0x12 = SU512LDB

Smoothing Type	struct
	{
	unsigned short m_SmoothPix,
	
	unsigned char m_SmoothModel
	}
		
		0 – 2048
		
		0
			
			number of neighbour pixels used for smoothing, max. has to be smaller than half the selected pixel range because both the pixels on the left and on the right are used
			Only one model defined so far
			(Size = 3 bytes)

Spectrum Calibration Type	struct
	{
	SmoothingType m_Smoothing,
	float m_CalInttime,
	float m_aCalibConvers[4096]
	}
		
		0.002 – 600000
			
			smoothing parameter during calibration
			integration time during calibration (ms)
			Conversion table from Scopedata to calibrated data
			(Size = 16391 bytes)

Type	Format	Value/Range	Description

Spectrum Correction Type	struct
	{
	float m_aSpectrumCorrect[4096]
	}
			Correct pixel values, e.g. for PRNU
			
			(Size = 16384 bytes)

Standalone Type	struct
	{
	bool m_Enable,
	MeasConfigType m_Meas,
	signed short m_Nmsr,
	SDCardType m_SDCard
	}
			
			(Size = 56 bytes)

TecControl Type	struct
	{
	bool m_Enable,
	float m_Setpoint,
	float m_aFit[2]
	}
			Tec Control parameters for AvaSpec-256-NIR2.2
			
			Set to True if device supports TE Cooling
			SetPoint for detector temperature in degr. Celsius
			DAC polynomial
			(Size = 13 bytes)

TempSensor Type	struct
	{
	float m_aFit[5]
	}
			Calibration coefficients temperature sensor
			
			(Size = 20 bytes)

TimeStamp Type	struct
	{
	unsigned short m_Date,
	
	unsigned short m_Time
	
	}
			
			bit 0..4 (day, 0 – 31)
			bit 5..8 (month, 1 – 12)
			bit 9..15 (years since 1980, 0 – 119)
			bit 0..4 (2-second unit, 0 - 30)
			bit 5..10 (minutes, 0 - 59)
			bit 11..15(hours, 0 – 23)

Type	Format	Value/Range	Description

TriggerType	struct
	{
	unsigned char m_Mode,
	unsigned char m_Source,
	unsigned char m_SourceType
	}
		
		0 – 1
		0 – 1
		0 – 1
			Trigger parameters
			
			mode, (0 = Software, 1 = Hardware)
			trigger source, (0 = external trigger, 1 = sync input)
			source type, (0 = edge trigger, 1 = level trigger)
			(Size = 3 bytes)

2.4.1 Return value constants

The following table gives an overview of possible integer return codes:

Return code	Value	Description
ERR_SUCCESS	0	Operation succeeded
ERR_INVALID_PARAMETER	-1	Function called with invalid parameter value.
ERR_OPERATION_NOT_SUPPORTED	-2	e.g. Function called to use 16bit ADC mode, with 14bit ADC hardware
ERR_DEVICE_NOT_FOUND	-3	Opening communication failed or time-out during communication occurred.
ERR_INVALID_DEVICE_ID	-4	AvsHandle is unknown in the DLL
ERR_OPERATION_PENDING	-5	Function is called while result of previous call to AVS_Measure is not received yet.
ERR_TIMEOUT	-6	No answer received from device
Reserved	-7	
ERR_INVALID_MEAS_DATA	-8	No measurement data is received at the point AVS_GetScopeData is called
ERR_INVALID_SIZE	-9	Allocated buffer size too small
ERR_INVALID_PIXEL_RANGE	-10	Measurement preparation failed because pixel range is invalid
ERR_INVALID_INT_TIME	-11	Measurement preparation failed because integration time is invalid (for selected sensor)
ERR_INVALID_COMBINATION	-12	Measurement preparation failed because of an invalid combination of parameters, e.g. integration time of (600000) and (Navg > 5000)
Reserved	-13	
ERR_NO_MEAS_BUFFER_AVAIL	-14	Measurement preparation failed because no measurement buffers available
ERR_UNKNOWN	-15	Unknown error reason received from spectrometer
ERR_COMMUNICATION	-16	Error in communication occured
ERR_NO_SPECTRA_IN_RAM	-17	No more spectra available in RAM, all read or measurement not started yet.
ERR_INVALID_DLL_VERSION	-18	DLL version information can not be retrieved
ERR_NO_MEMORY	-19	Memory allocation error in the DLL
ERR_DLL_INITIALISATION	-20	Function called before AVS_Init() is called
ERR_INVALID_STATE	-21	Function failed because AS5216 is in wrong state (e.g AVS_Measure without calling AVS_PrepareMeasurement first)
ERR_INVALID_PARAMETER_NR_PIXEL	-100	NrOfPixel in Device data incorrect
ERR_INVALID_PARAMETER_ADC_GAIN	-101	Gain Setting Out of Range
ERR_INVALID_PARAMETER_ADC_OFFSET	-102	OffSet Setting Out of Range
ERR_INVALID_MEASPARAM_AVG_SAT2	-110	Use of Saturation Detection Level 2 is not

Return code	Value	Description
		compatible with the Averaging function
ERR_INVALID_MEASPARAM_AVG_RAM	-111	Use of Averaging is not compatible with the StoreToRam function
ERR_INVALID_MEASPARAM_SYNC_RAM	-112	Use of the Synchronize setting is not compatible with the StoreToRam function
ERR_INVALID_MEASPARAM_LEVEL_RAM	-113	Use of Level Triggering is not compatible with the StoreToRam function
ERR_INVALID_MEASPARAM_SAT2_RAM	-114	Use of Saturation Detection Level 2 Parameter is not compatible with the StoreToRam function
ERR_INVALID_MEASPARAM_FWVER_RAM	-115	The StoreToRam function is only supported with firmware version 0.20.0.0 or later.
ERR_INVALID_MEASPARAM_DYNDARK	-116	Dynamic Dark Correction not supported
ERR_NOT_SUPPORTED_BY_SENSOR_TYPE	-120	Use of AVS_SetSensitivityMode not supported by detector type
ERR_NOT_SUPPORTED_BY_FW_VER	-121	Use of AVS_SetSensitivityMode not supported by firmware version
ERR_NOT_SUPPORTED_BY_FPGA_VER	-122	Use of AVS_SetSensitivityMode not supported by FPGA version

2.4.2 Windows messages

The following table gives an overview of window messages.

Windows message identifier	WPARM	LPARM	Description
WM_MEAS_READY	0 (on success) < 0 (one of the above error reasons) > 0 (in StoreToRAM mode)	device handle	After measurement data is available the DLL sends this message to the application. The command value used is WM_MEAS_READY which is defined as (WM_APP + 1) for the 64 bit version of the DLL (as5216x64.dll)
WM_DEVICECHANGE	DBT_DEVNODES_CHANGED(7)	0	After device attachment/removal Windows sends this message to the application.

3 Example source code

Example source code can be found in the directory tree of the driver.
Sample programs (including header files and link libraries, where appropriate) are provided for the
following programming environments:

- Microsoft Visual C++ 2008 combined with the Qt4 framework (native code)
- LabVIEW 2009, 64 bit version (native code)
- MATLAB R2010a, 64 bit version (native code)
- Microsoft Visual Basic 2008, managed code (for .net version 3.5)
- Microsoft Visual C# 2008, managed code (for .net version 3.5)
- Microsoft Visual C++ 2008, managed code (for .net version 3.5)

For VC++2008/Qt4, both a comprehensive and a simple sample are provided.

For LabView, four sample programs are available:
- A comprehensive program for a single channel AvaSpec-USB2, which also includes subvi's
  for all functions in the as5216x64.dll (LabViewSingleChan folder)
- A simple sample program that uses AVS_PollScan instead of Windows Messaging (polling
  folder)
- A multichannel example program which illustrates how to run multiple spectrometer channels
  (fixed to 2 channels in the example program) in SYNC mode, as well as ASYNC mode
  (polling_mc folder)
- A simple sample program that illustrates how the StoreToRam functionality can be
  implemented in combination with AVS_PollScan (polling_StoreToRAM folder)

3.1 Initialization and Activation of a spectrometer

After starting the full QtDemo program, located in the 'Qtdemo_full_demo' folder, the main window
will be displayed. By clicking the "Open Communication" button, the AVS_Init function is called and
if successful, the serial number and status for the connected spectrometer(s) is collected
(AVS_GetNrOfDevices and AVS_GetList). The result is displayed in the list at the top left of the
window, as shown in the figure below.

After selecting a spectrometer from the list, clicking the "Activate" button results in a call to the AVS_Activate function. This function returns a DeviceHandle which needs to be used in further communication between the dll and this device. After a successful call to AVS_Activate, the status for the selected device will change from "AVAILABLE" to "IN_USE_BY_APPLICATION".

The sample program uses one DeviceHandle, so if you want to run multiple devices simultaneously, you need to allocate storage space for multiple devicehandles (see the main sample program in the 'Qtdemo_full_demo' subfolder).

For the activated device, the Device information is collected (AVS_GetVersionInfo, AVS_GetNumPixels, AVS_GetParameter, AVS_GetLambda), and displayed in the main window.

Thanks to the Windows API OnDeviceChange function, attachment and removal of spectrometers can be detected by the application (see the OnDeviceChange function in the source code).

Note: To match the structures that are used in the AS5216 firmware the structures used in the as5216x64.dll should be compiled with *byte alignment*

3.2 Starting a measurement

Measurements can be started by clicking the "Start Measurement" button. The Nr of Scans field displays how many scans will be performed after one measurement request. Before a call to AVS_Measure is done, the AVS_PrepareMeasurement function is called with the parameters in the MeasConfigType structure. The "Prepare Measurement Settings" group in the figure below shows all the parameters in this MeasConfigType structure:

```
unsigned short        m_StartPixel
unsigned short        m_StopPixel
float                 m_IntegrationTime
unsigned int          m_IntegrationDelay
unsigned int          m_NrAverages
DarkCorrectionType    m_CorDynDark
SmoothingType         m_Smoothing
unsigned char         m_SaturationDetection
TriggerType           m_Trigger
ControlSettingsType   m_Control
```

The parameters in the measurement structure have been briefly described in section 2.4. In this section a more detailed description will be given.

3.2.1   Measurement structure: Start- and Stoppixel

The start- and stoppixel are the first and last pixel to be sent to the PC. The full range for a spectrometer is between startpixel 0 and stoppixel "NrOfPixels-1", where NrOfPixels specifies the total pixels available for the detectortype used in the spectrometer (see also AVS_GetNumPixels). If the wavelength range of a spectrometer exceeds 1100nm (1160nm for the AvaSpec-2048x14) and the detectortype is different from "HAMS9201" (AvaSpec-NIR), the stoppixel can be set to the pixelnumber that corresponds to a wavelength of 1100 (1160) nm, because the sensitivity is almost zero at this wavelength range. Reducing the range increases the data transfer speed and allows you to transfer only the data that is relevant to the application.

Note that if m_StartPixel is not equal to zero, then a_pSpectrum[n] (see AVS_GetScopeData), represents the measured data at pixel number m_StartPixel +n. Also, pSaturated[n] (see AVS_GetSaturatedPixels) represents pixel number m_StartPixel +n. For example, if m_StartPixel = 10, then a_pSpectrum[0] represents the measured data at pixel number 10.

3.2.2   Measurement structure: Integration Time

The integration time is the exposure time during one scan. The longer the integration time, the more light is exposed to the detector during a single scan, and therefore the higher the signal. The unit is milliseconds [ms], and the resolution 0.001 ms steps. The minimum integration time is detector dependent. The table below shows the values for the different detector types

Spectrometer	Detector Type	Min. Integration time [ms]
AvaSpec-256-USB2	SENS_HAMS8378_256	0.56
AvaSpec-1024-USB2	SENS_HAMS8378_1024	2.20
AvaSpec-2048-USB2	SENS_ILX554	1.05
AvaSpec-2048L-USB2	SENS_ILX511	1.05
AvaSpec-NIR256-1.7, AvaSpec-NIR256-2.0TEC, AvaSpec-NIR256-2.5TEC	SENS_HAMS9201	0.01*
AvaSpec-NIR256-1.7TEC, AvaSpec-NIR256-2.2TEC**	SENS_SU256LSB	0.02
AvaSpec-NIR512-1.7TEC AvaSpec-NIR512-2.2TEC	SENS_SU512LDB	0.02

AvaSpec-3648-USB2	SENS_TCD1304	0.01
AvaSpec-102-USB2	SENS_TSL1301	0.06
AvaSpec-128-USB2	SENS_TSL1401	0.07
AvaSpec-2048x14-USB2	SENS_HAMS9840	2.17
AvaSpec-350F-USB2	SENS_ILX554	0.20
AvaSpec-950F-USB2	SENS_ILX554	0.50
AvaSpec-1350F-USB2	SENS_ILX554	0.70
AvaSpec-1650F-USB2	SENS_ILX554	0.85
AvaSpec-2048x16-USB2	SENS_HAMS11071_2048X16	1.82***
AvaSpec-2048x64-USB2	SENS_HAMS11071_2048X64	2.40****
AvaSpec-HS1024x58-USB2	SENS_HAMS7031_1024X58	5.22
AvaSpec-HS1024x122-USB2	SENS_HAMS7031_1024X122	6.24
AvaSpec-2048XL-USB2	SENS_HAMS11155	0.002

*   = 0.01ms for SENS_HAMS9201 in Firmware v. 000.025.000.000 and later, else 0.52ms
**   = AvaSpec-NIR256-2.2TEC with SENS_SU256LSB detector released in 2011, and is the successor of the   NIR2.2 with SENS_HAMS9201 detector
***   = 1.82 ms for SENS_HAMS11071_2048X16 in FPGA 006.003.000.000 or later, else 0.91ms
****   = 2.40 ms for SENS_HAMS11071_2048X64 in FPGA 006.003.000.000 or later, else 1.75ms

The longest integration time is 10 minutes (600000 ms).

3.2.3   Measurement structure: Integration Delay

The integration delay parameter can be used to start the integration time not immediately after the measurement request (or on an external hardware trigger), but after a specified delay. The unit for this delay is FPGA clock cycles. The FPGA clock runs at 48 MHz, so the integration delay can be set with 20.83 nanoseconds steps. See also section 3.2.9 about using the integration delay in combination with the control settings: laser delay and pulse width. Integration delay has been implemented and tested for the detectors that support fast triggering. These Fast Triggering detectors (Sony ILX554, Sony ILX511 and Hamamatsu S11155 in the AvaSpec-2048-USB2, AvaSpec-2048L-USB2 and AvaSpec-2048XL) can be reset in respectively 1.3, 3.3 and 0.3 microseconds and start a new integration time immediately after this reset. The Toshiba TCD1304 in the AvaSpec-3648-USB2 also supports fast triggering in clearbuffermode (see also section 2.3.35), but because of the nonlinear behavior of the detector and the "missing" lower Counts in clearbuffer mode, this detector is less suitable for the fast triggering than the Sony detectors and the Hamamatsu S11155.
For the other detector types, it is recommended to set the integration delay parameter to 0 FPGA cycles.

3.2.4   Measurement structure: Number of Averages

The signal to noise ratio of the scope data is improved by the square root of NrOfAverage. Averaging is done by the microcontroller at the as5216 board, therefore, no time is lost by sending the individual scans from the spectrometer to the PC.

3.2.5   Measurement structure: Dynamic Dark Correction

The pixels of the CCD detector are thermally sensitive, which causes a small dark current, even without exposure to light. To get an approximation of this dark current, the signal of some optical black pixels of the detector can be taken and subtracted from the raw scope data. This will happen if the "Correct for Dynamic Dark" option is enabled. Some detector types (AvaSpec-2048/2048L/3648) include dedicated optical black pixels. At these optical plack pixels, the intensity and thermal behaviour is the same as the active data pixels, if no light falls on the detector. Enabling dynamic dark

correction will therefore result in a baseline fluctuating round zero, and measurement data will be less sensitive for temperature changes than with dynamic dark correction off.

The back illuminated detectors in the AvaSpec-2048x14, 2048x16, 2048x64, 1024x122 and 1024x58 don't include optical black pixels, but a few elements in the shift register can also be used for correcting the raw data. The intensity at these elements may be different from the intensity of the (2048) data pixels in the dark, so the baseline may not fluctuate round zero, but the correction will result in a much more linear behavior of the data pixels when exposed to light. Therefore, it is strongly recommended to leave the (default) Dynamic Dark Correction state "Enabled".

The 2048XL uses 18 dummy pixels for correcting the raw data. Since these 18 pixels are located at positions 2050 to 2067, the stoppixel in the measurement structure should be set to 2067. Setting the stoppixel to a lower value for pixel reduction will have no effect with dynamic dark correction enabled, because these last 18 pixels are needed for the correction algorithm.

Some NIR detector types (NIR256-2.0TEC, NIR256-2.5TEC) also support dynamic dark, because a few datapixels are blackened during fabrication of the optical bench. These blackened pixels can then be used for dynamic dark correction.. If the spectrometer does not include blackened datapixels, nor dedicated optical black pixels, enabling the dynamic dark correction results in a return value of -116 when calling AVS_PrepareMeasure. This error can be neglected by the application (measurements can be proceeded), but dynamic dark correction is not possible in that case.

The Dark Correction Type structure includes an m_enable and m_ForgetPercentage field (see also section 2.4). Measurements have shown that taking into account the historical dark scans, does not make much difference. The recommended value for m_ForgetPercentage is therefore 100.

3.2.6   Measurement structure: Smoothing

The smoothing type structure includes a smoothpix and a smoothmodel field. In the current version of the as5216x64.dll there is just one smoothing model available (0), in which the spectral data is averaged over a number of pixels on the detector array. For example, if the smoothpix parameter is set to 2, the spectral data for all pixels x_n on the detector array will be averaged with their neighbor pixels x_{n-2}, x_{n-1}, x_{n+1} and x_{n+2}.

The optimal smoothpix parameter depends on the distance between the pixels at the detector array and the light beam that enters the spectrometer. For the AvaSpec-2048, the distance between the pixels on the CCD-array is 14 micron.
With a 200 micron fiber (no slit installed) connected, the optical pixel resolution is about 14.3 CCD-pixels. With a smoothing parameter set to 7, each pixel will be averaged with 7 left and 7 right neighbor pixels. Averaging over 15 pixels with a pitch distance between the CCD pixels of 14 micron will cover 15*14 = 210 micron at the CCD array. Using a fiber diameter of 200 micron means that we will lose resolution when setting the smoothing parameter to 7. Theoretically the optimal smoothing parameter is therefore 6. The formula is ((slit size/pixel size) – 1)/2
In the table below, the recommended smoothing values for the AvaSpec spectrometer are listed as function of the light beam that enters the spectrometer. This light beam is the fiber core diameter, or if a smaller slit has been installed in the spectrometer, the slit width. Note that this table shows the optimal smoothing without losing resolution. If resolution is not an important issue, a higher smoothing parameter can be set to decrease noise at the price of less resolution.

Slit or Fiber	AvaSpec-128	AvaSpec-256 1024	AvaSpec-HS 1024x58 1024x122	AvaSpec-2048, 2048L, 2048x14, 2048x16, 2048x64, 2048XL	AvaSpec-3648	AvaSpec-NIR256	AvaSpec-NIR512
	Pixel 63.5 μm	Pixel 25 μm	Pixel 24 μm	Pixel 14 μm	Pixel 8 μm	Pixel 50 μm	Pixel 25 μm
10μm	n.a.	n.a.	0	0	0	n.a.	n.a.
25μm	n.a.	0	0	0-1	1	n.a.	0
50μm	0	0-1	0-1	1-2	2-3	0	0-1
100μm	0-1	1-2	1-2	3	5-6	0-1	1-2
200μm	1	3-4	3-4	6-7	12	1-2	3-4
400μm	2-3	7-8	7-8	13-14	24-25	3-4	7-8
500μm	3-4	9-10	9-10	17	31	4-5	9-10
600μm	4	11-12	11-12	21	37	5-6	11-12

3.2.7 Measurement structure: Saturation Detection

The 16-bit A/D converter in the AvaSpec results in raw Scope pixel values between 0 and 65535 counts. If the value of 65535 counts is measured at one or more pixels, then these pixels are called to be saturated or overexposed. Saturation detection can be set off (m_SaturationDetection=0) or on (m_SaturationDetection=1). Saturation detection is done by the as5216x64.dll, after a measurement result has been sent to the PC. If a measurement is the result of a number of averages, the as5216x64.dll can only detect saturation if all NrOfAverage scans in a measurement were saturated for one or more pixels.

Only for AvaSpec-2048 spectrometers, the third level is available (m_SaturationDetection=2, autocorrect inverted pixels). The reason for this is that if the detector type in the AvaSpec-2048 (Sony-ILX554) is heavily saturated (at a light intensity of approximately 5 times the intensity at which saturation starts), it will return values <65535 counts. The other detector types in the AvaSpec-102, 128, 256, 1024, 2048L, 2048x14 and 3648 and AvaSpec-NIR do not show this effect, so no correction is needed. Normally, you don't need to use this third level for the AvaSpec-2048, but when measuring a peaky spectrum with some heavily saturated peaks, the autocorrect can be used. A limitation to this level is that it can be used only if no averaging is used (m_NrAverages=1).
The AvaSpec-USB2 spectrometers with an as5216 board Rev C and earlier were equipped with a 14-bit AD converter (range 0..16383). In this case the detector is saturated at 16383 counts.

3.2.8 Measurement structure: Trigger Type

The trigger type structure includes settings for Trigger Mode (Hardware, Software), Trigger Source (External, Synchronized) and Trigger type (Edge, Level).

Setting the Trigger Source to Synchronized is relevant if multiple spectrometers need to run synchronised (all spectrometers start a measurement at the same time). This option will be described below under "Running multiple spectrometers Synchronized".
Single channel spectrometers, or multiple spectrometers in ASYNC mode can operate in one of the three following Trigger settings (Trigger Source should be set to "External"):

Trigger Mode = Software
This Trigger setting is used when one or more (nrms) measurements should start after a measurement request in the software (AVS_Measure call). The Edge/Level is irrelevant because this only applies to an external hardware trigger.

Trigger Mode = Hardware, Edge triggered
This trigger setting is used when one or more (nrms) measurements should start after an external hardware trigger pulse has been received at pin 6 of the DB26 connector. First a measurement request is posted in the software (AVS_Measure call). Then the spectrometer waits until a rising edge of the TTL-input pulse is detected at pin 6 of the DB26 connector before nrms scans are started.
The delay between the rising edge of the TTL pulse and the start of the integration time cycle depends on the spectrometer type, as shown in the table below.

Spectrometer Type	Minimum Delay [μs]	Maximum Delay [μs]
AvaSpec-128-USB2	9	60
AvaSpec-256-USB2	0.80	0.84
AvaSpec-1024-USB2	0.80	0.84
AvaSpec-2048-USB2*	1.28	1.30
AvaSpec-2048L-USB2	3.28	3.30
AvaSpec-3648-USB2 (clearbuffer mode)**	0.28	0.30
AvaSpec-NIR256-1.7, AvaSpec-NIR256-2.0TEC, AvaSpec-NIR256-2.5TEC	0	600
AvaSpec-NIR256-1.7TEC, AvaSpec-NIR256-2.2TEC	4.92***	5.75***

AvaSpec-NIR512-1.7TEC, AvaSpec-NIR512-2.2TEC	4.92****	5.75****
AvaSpec-2048x14-USB2	-2170	0
AvaSpec-2048x16-USB2	-1820	0
AvaSpec-2048x64-USB2	-2400	0
AvaSpec-HS1024x58-USB2	-5220	0
AvaSpec-HS1024x122-USB2	-6240	0
AvaSpec-2048XL-USB2	0.28	0.30

*   The AvaSpec-350F-USB2, AvaSpec-950F-USB2, AvaSpec-1350F-USB2 and
       AvaSpec-1650F-USB2 use the same detector as the AvaSpec-2048-USB2 and will
       therefore have the same trigger response characteristics as the AvaSpec-2048-USB2

**   The delay for the AvaSpec-3648-USB2 in prescan mode strongly depends on the integration
       time setting, but can be calculated within 0.02 µs precision by the following equations:

       Scanspassed = floor((Inttime-0.002+3.6961)/(Inttime-0.002))
       min_delay = 0.00183 + Scanspassed*(Inttime-0.002) [ms]
       max_delay = 0.00185 + Scanspassed*(Inttime-0.002) [ms]
       Inttime = Integration time setting in milliseconds in the preparemeasurement structure

       Example1: Inttime = 0.1ms
       Scanspassed = floor(38.72) = 38
       min_delay = 0.00183 + 38*0.098 = 3.72583 ms
       max_delay = 3.72585 ms

       Example2: Inttime = 0.01ms
       Scanspassed = floor(463.01) = 463
       min_delay = 0.00183 + 463*0.008 = 3.70583ms
       max_delay = 3.70585 ms

       So if the application allows that the AvaSpec-3648-USB2 in prescan mode is triggered a
       couple of milliseconds before the event that needs to be measured, this event can be shifted
       with high precision into the integration time cycle of the spectrometer. Moreover, the
       integration delay parameter (section 3.2.3) can be used to add additional delay in steps of 21
       nanoseconds to the min_delay calculated above.

***   4.92 – 5.75 µs with FPGA version 6.4 and later, 137.5 – 138.3 µs with FPGA version 6.3

**** 4.92 – 5.75 µs with FPGA version 6.4 and later, 251.1 – 252.8 µs with FPGA version 6.3

Trigger Mode = Hardware, Level triggered
This trigger setting is used when scans should be performed as long as the external trigger at pin 6 of
the DB26 connector is HIGH. The spectrometer will start to accumulate data (take scans at the
selected integration time) at the rising edge of the TTL pulse and will continue to do so as long as the
TTL signal remains high. When the signal becomes low, the average of the accumulated data (except
for the last scan) will be sent. This mode is especially useful for conveying belt applications, when a
product needs to be scanned, independent of the transport speed.

Running multiple spectrometers Synchronized

All USB2 platform spectrometers can be connected by a SYNC cable. In syncmode, one spectrometer is configured as "Master" by calling the AVS_SetSyncMode function for this channel with the a_Enable flag set to 1. The trigger source for the Master channel should **not** be set to Synchronized, but to External. The trigger mode for the Master can be set to Software (if a measurement should start after a measurement request in the software), or to Hardware (if a measurement should start after an external hardware trigger pulse at pin 6 of the Master DB26 connector. All other ("slave") spectrometers are set into "Synchronized" mode by setting the Trigger Source to "Synchronized" and the Trigger Mode to "Hardware".

A synchronized measurement is started by calling AVS_Measure first for all slave channels. As a result, these channels start listening to their SYNC input port. Secondly a measurement request (call to AVS_Measure) needs to be posted for the Master channel. If the trigger mode for the Master is "software", this result in nrms measurements for all channels. If the trigger mode for the Master is "hardware", the nrms measurements for all channels are started after an external trigger has been received at at pin 6 of the Master DB26 connector. The nrms parameter in the AVS_Measure function should be set to the same value for all activated channels.

Source code for the sample programs that support synchronization of multichannel systems can be found in the following folders:
..\examples\ Borland Delphi 6\ multichannel\
..\examples\ Codegear Delphi 2009\ multichannel\
..\examples\LabView\polling_mc\

Synchronization is done at a measurement level. A measurement can include a number of scans to average. This "number of average" scans is only synchronized for the first scan. For example, if the number of measurements, integration time and number of average for two channels are set to:
Channel A: nrms=2, integration time 100ms, average 3
Channel B: nrms=2, integration time 65ms, average 2,
then the data acquisition timing and response in synchronized mode will look like:
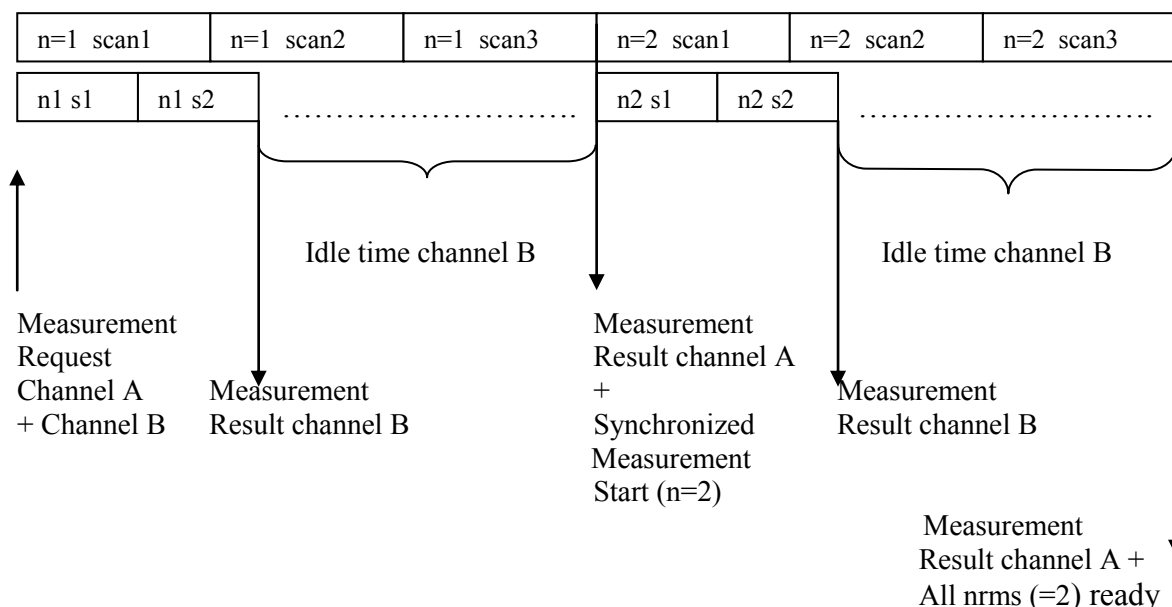
Note that in the example above, the number of averages for channel B can be set to 4 without losing time because the extra two scans will be taken in the idle time for channel B.

AS-5216x64-DLL Manual.docx   Jun-12

3.2.9   Measurement structure: Control Settings

The Control Settings include parameters to control
- A pulsed lightsource   (m_StrobeControl)
- A laser pulse   (m_LaserDelay and m_LaserWidth)
- The Number of Spectra that will be stored to onboard RAM (m_StoreToRam)

Pulsed lightsource control
A pulsed light source like the AvaLight-XE needs to be synchronized with the integration time cycle. The m_StrobeControl parameter determines the number of pulses the spectrometer sends out at pin 5 at the DB26 connector during one integration time cycle. The maximum frequency at which the AvaLight-XE operates is 100 Hz. This means that the minimum integration time for 1 pulse per scan is 10 ms. When setting the number of pulses e.g. to 3, the minimum integration time should be 30 ms. The as5216x64.dll does not check for this limitation because other light sources may operate at higher frequencies, and should also be controllable by the AvaSpec and as5216x64.dll.

Laser pulse control
For the fast trigger detectors ILX554 and ILX511 in the AvaSpec-2048 and AvaSpec2048L, pin 23 at the DB26 connector can be used to send out a TTL signal which is related to the start of the integration time cycle. In the figure below, a measurement is started at the rising edge of the Trig signal. This can be a hardware or software trigger, see also section 3.2.8. The TTL signal at pin 23 (Laser) is set after the laserdelay (T1) expires. The pulsewidth for the laser pulse (T3) is set by the m_LaserWidth parameter. The integration time cycle starts after the integration delay parameter (see section 3.2.3) expires.
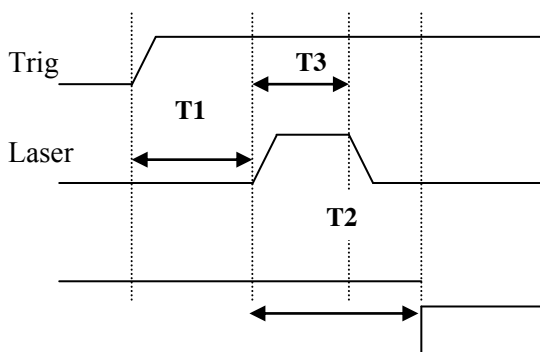
Integration

The unit for T1, T2 and T3 is FPGA clock cycles. The FPGA clock runs at 48 MHz, so delays and pulse width can be set with 20.83 nanoseconds steps. If the integration delay T2 is set to 0 FPGA

cycles, the rising edge of the integration signal will start one clock cycle (20.83ns) before the rising edge of the laser pulse. This will ensure that with this setting, the flash of the source that is triggered by the laser pulse entirely falls in the integration time cycle.

Laser Induced Breakdown Spectroscopy (LIBS) is an application where the integration delay is used in combination with a TTL-out at the DB-26 connector to fire a laser. After a measurement request (or on an external hardware trigger), the laser is fired by the TTL-out. The integration time period should not include the laser light, so the start of the integration time needs to be delayed. A typical integration delay in LIBS applications is about 1μs (ILX554 detector in AvaSpec-2048-USB2, see also section 3.2.3).

Laser wavelength
The Laser wavelength (m_LaserWaveLength) control setting is not used in the current version of the as5216. A value can be entered, but the as5216 firmware does not use this information.

StoreToRam
As of firmware version 0.20.0.0 the StoreToRam function has been implemented. To use this function, you must set the requested number of scans in the m_StoreToRam control setting, and start measuring with a call to AVS_Measure using 1 as the number of measurements (a_Nmsr).
There is an amount of 4MB available for scans, corresponding with 1013 scans of 2048 pixels. Scanning less pixels will yield a larger capacity in scans. The AVS_Measure message signaling the arrival of data will have a WParam value equal to the number of scans stored in RAM. In regular measurements, this value only signals success (with value ERR_SUCCESS) or failure (with a negative error message).
Alternatively, when using AVS_PollScan instead of a message driven interface, the AVS_PollScan function will return 1 when the StoreToRam scans are available, and 0 as long as they are not.

The scans can subsequently be read with a corresponding number of calls to AVS_GetScopeData. If you request more scans than will fit in memory, scanning will continue until the memory is fully used, therefore you should always request the number of scans that is returned in Wparam (when using Windows Messaging.

If using StoreToRAM in combination with AVS_PollScan, the number of scans that can be processed by subsequently calling AVS_GetScopeData will normally be equal to the requested number of scans in the StoreToRAM parameter. If more scans are requested than can be stored (e.g. 1500 scans of 2048 pixels), it can happen that AVS_GetScopeData will be called too many times. In case of the example, only the first 1013 calls to AVS_GetScopeData will return SUCCESS. The next call will return the error code ERR_NO_SPECTRA_IN_RAM, which can be used by the application software as an additional stop condition for reading spectra from RAM. However, reading beyond the number of scans that can be stored in RAM is a time consuming event, so it is not recommended to request   more scans than the maximum that can be stored.

The StoreToRam functionality has been implemented in most sample programs that come with the as5216x64-dll interface package. To illustrate how to use StoreToRAM in combination with AVS_PollScan, a simple LabView sample program has been added since as5216.dll version 1.7.0.0.

3.3 Measurement result

If a measurement is ready, the windows message WM_MEAS_READY is sent to the application. The Wparam value of the message should be:
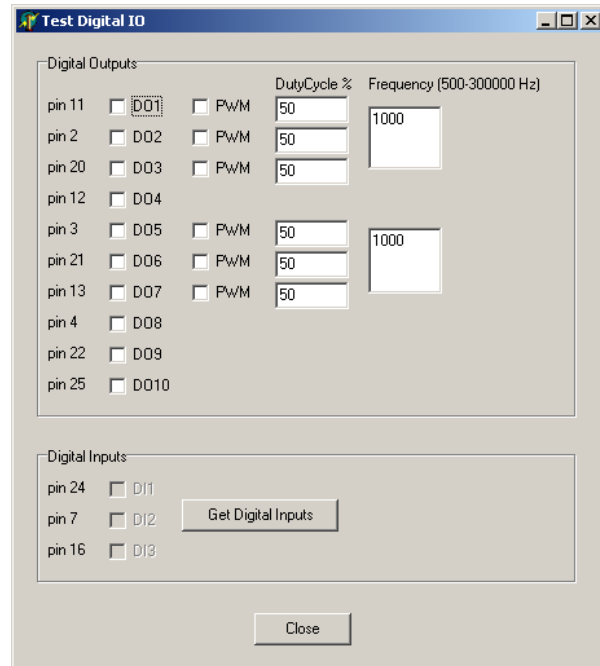
- - 0 in regular measurements (where the StoreToRam parameter is zero) to indicate SUCCESS
- - > 0 in StoreToRam mode, Wparam holds the number of spectra that were actually saved in RAM
- - < 0 in case an error occurred (see section section 2.4.1).

The Lparam value of the message contains the devicehandle for the spectrometer for which the data is ready.

LabVIEW cannot easily respond to the incoming Windows message that signals the arrival of new data. AVS_Pollscan allows the application program to poll the arrival of data, i.e. to actively get the status of this data, instead of letting a message handler react to the Windows message from the dll. By calling the function AVS_GetScopeData, the spectral data is stored in the application for further processing.

3.4 Digital IO

The USB2 platform spectrometers have 10 programmable digital output pins and 3 programmable input pins available at the DB26 connector. The function AVS_SetDigOut and AVS_GetDigIn can be used to control these ports. Moreover, 6 out of the 10 programmable output ports can be configured for pulse width modulation. With the AVS_SetPwmOut function, a frequency and duty cycle can be programmed for these 6 digital output ports.

The PWM functionality can be used e.g. in controlling the intensity (dutycycle) of an AvaLight-LED light source, which receives input from DO1 (pin 11 of the DB26 connector).

3.5 Analog IO

The USB2 platform spectrometers have 2 programmable analog output pins and 2 programmable analog input pins available at the DB26 connector. The functions AVS_SetAnalogOut and AVS_GetAnalogIn can be used to control these ports. For the Analog Out signals, an 8-bit DAC is used. The Analog In signals are converted by the internal 10-bit ADC's.

A number of onboard analog signals can be retrieved as well with the AVS_GetAnalogIn function. One of these onboard signals is the NTC1 X8 thermistor which can be used for onboard temperature measurements. The polynomial for converting the voltage (U) to degrees Celsius for NTC1 is:

$$\text{Temp } [^{o}C] = 118.69 - 70.361*U + 21.02*U^2 - 3.6443*U^3 + 0.1993*U^4$$

The thermistor X11 is the signal received from a TE cooled detector and can be used to monitor the detector temperature. NTC2 X9 is not mounted.

The 1V2, 5VIO and 5VUSB are used internally to test the power supply

3.6 EEProm

The EEProm parameters in the DeviceConfigType structure have been briefly described in section 2.4. In this section a more detailed description will be given. The main sample program display most of the parameters in the structure. The Structure Length (m_Len), Structure Version (m_ConfigVersion) and InfoString (m_aUserFriendlyId[64]) are shown on top of the tabs that correspond to the structures that are used to group the parameters into the following categories:

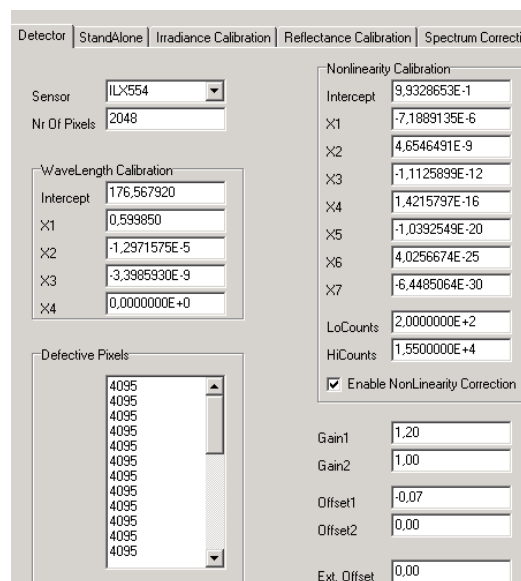|	
DetectorType	m_Detector,
IrradianceType	m_Irradiance,
SpectrumCalibrationType	m_Reflectance,
SpectrumCorrectionType	m_SpectrumCorrect,
StandaloneType	m_StandAlone,
TempSensorType	m_Temperature[3]
TecControlType	m_TecControl
ProcessControlType	m_ProcessControl (not displayed in sample program)

The structure version is used internally to maintain compatible between different versions of the dll and firmware. The Information character string can be used e.g. to write a user friendly name for the spectrometer.

3.6.1   EEProm structure: Detector Parameters

The detector parameters are defined in the DetectorType structure, which includes the following elements:

```
SensorType          m_SensorType
unsigned short      m_NrPixels
float               m_aFit[5]
bool                m_NLEnable
double              m_aNLCorrect[8]
double              m_aLowNLCounts
double              m_aHighNLCounts
float               m_Gain[2]
float               m_Reserved
float               m_Offset[2]
float               m_ExtOffset
unsigned short      m_DefectivePixels[30]
```

SensorType and Number of Pixels

The as5216 board supports many different detectors which are used in the AvaSpec spectrometers as shown in the table below:

Spectrometer	DetectorType	Number of Pixels
AvaSpec-102-USB2	SENS_TSL1301	102
AvaSpec-128-USB2	SENS_TSL1401	128
AvaSpec-256-USB2	SENS_HAMS8378_256	256
AvaSpec-1024-USB2	SENS_HAMS8378_1024	1024
AvaSpec-2048x14-USB2	SENS_HAMS9840	2048
AvaSpec-2048x16-USB2	SENS_HAMS11071_2048X16	2048
AvaSpec-2048x64-USB2	SENS_HAMS11071_2048X64	2048
AvaSpec-NIR256-1.7, AvaSpec-NIR256-2.0TEC, AvaSpec-NIR256-2.5TEC	SENS_HAMS9201	256
AvaSpec-NIR256-1.7TEC, AvaSpec-NIR256-2.2TEC*	SENS_SU256LSB	256
AvaSpec-NIR512-1.7TEC, AvaSpec-NIR512-2.2TEC	SENS_SU512LDB	512
AvaSpec-2048-USB2	SENS_ILX554	2048
AvaSpec-350F-USB2	SENS_ILX554	350
AvaSpec-950F-USB2	SENS_ILX554	950
AvaSpec-1350F-USB2	SENS_ILX554	1350
AvaSpec-1650F-USB2	SENS_ILX554	1650
AvaSpec-2048L-USB2	SENS_ILX511	2048
AvaSpec-3648-USB2	SENS_TCD1304	3648
AvaSpec-HS1024x58-USB2	SENS_HAMS7031_1024X58	1024
AvaSpec-HS1024x122-USB2	SENS_HAMS7031_1024X122	1024
AvaSpec-2048XL-USB2	SENS_HAMS11155	2068

* = AvaSpec-NIR256-2.2TEC with SENS_SU256LSB detector released in 2011, and is the successor of the NIR2.2 with SENS_HAMS9201 detector

For each detector, different FPGA firmware is needed. The SensorType parameter should therefore not be changed unless new FPGA firmware for another detectortype has been loaded.
The number of pixels is determined by the detectortype and should therefore not be changed, unless another detectortype has been connected and the right FPGA code has been loaded.
Also for the Fast Series (350F, 950F, 1350F, 1650F), the number of pixels is fixed and should not be changed.

Wavelength Calibration

The polynomial coefficients in m_aFit[5] describe the relation between the pixelnumber of the detector array (0..m_NrPixels-1) and the corresponding wavelength in nanometer at this pixelnumber:

$$\lambda = m\_aFit[0] + m\_aFit[1] *pixnr + m\_aFit[2] *pixnr^2 + m\_aFit[3] *pixnr^3 + m\_aFit[4] *pixnr^4$$

In the function AVS_GetLambda, the m_aFit coefficients are used internally to store the wavelength numbers into an array.

Nonlinearity Calibration and Correction

A polynomial can be used to correct for nonlinear behavior of the detector. The polynomial coefficients can be stored in the EEProm and used by the application software to correct the raw AD Counts.

The nonlinearity calibration service (determination of the polynomial coefficients) is included in the IRRAD-CAL irradiance calibration service, but can also be ordered separately (NL-Calibration). The m_aLowNLCounts and m_aHighNLCounts parameters have been added since as5216.dll version 1.1, to be able to limit the range (in counts) for which the correction polynomial should be applied. The correction that needs to be implemented in the application software can be illustrated by using an example:
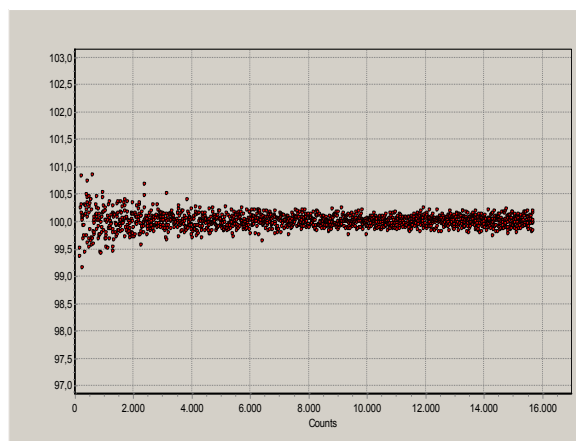
Suppose the following nonlinearity polynomial has been calculated:

```
m_aNLCorrect[0]   =  9.93286529334744E-001
m_aNLCorrect[1]   = -7.18891352982627E-006
m_aNLCorrect[2]   =  4.65464905353804E-009
m_aNLCorrect[3]   = -1.11258994803382E-012
m_aNLCorrect[4]   =  1.42157972847117E-016
m_aNLCorrect[5]   = -1.03925487491128E-020
m_aNLCorrect[6]   =  4.02566735990250E-025
m_aNLCorrect[7]   = -6.44850644473040E-030
m_aLowNLCounts    =  200.0
m_aHighNLCounts   =  15500.0
```

The polynomial is calculated by measuring the AD Counts for a number of pixels (10) over different integration times to get the pixel data over a wide range from (in this example) 200 to 15500 counts. The measured AD Counts are corrected for the offset value by subtracting the dark spectrum. For each of the 10 pixels in the measurement the counts per second is calculated and normalized to its maximum value, which is set to 100%. In the left figure below the normalized counts per second are displayed against the measured AD Counts (corrected for dark). The polynomial is the best fit through these measured points. The right figure below has been created by applying the polynomial to the measured points, and recalculating the normalized counts per second. It is important to realize that the polynomial should be applied to the AD Counts that have been corrected for the dark counts.
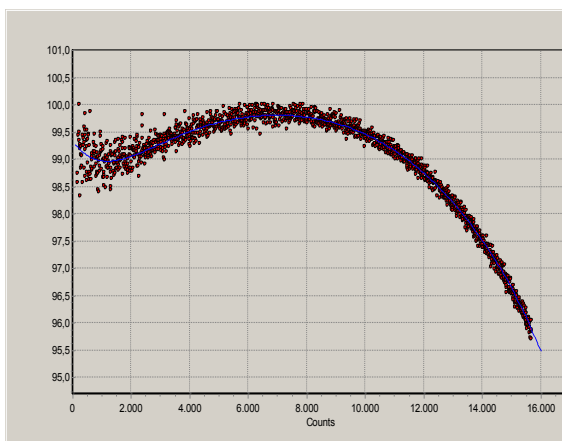
Before linearization   After linearization

In the application software, a dark spectrum needs to be saved first and subtracted from the measured AD Counts before the correction is applied. For example, suppose the measured AD Counts in the dark for a pixel is a value of 300 Counts. At a certain light intensity, the measured AD Counts for this pixel becomes a value of 14000 Counts. The AD Counts corrected for dark therefore becomes 13700. The Normalized Counts Per Second can be calculated from the polynomial:

$$
\begin{aligned}
\text{NCPS}= \text{m\_aNLCorrect}\,[0] +& \\
\text{m\_aNLCorrect}\,[1]\,*13700 +& \\
\text{m\_aNLCorrect}\,[2]\,*13700^2 +& \\
\text{m\_aNLCorrect}\,[3]\,*13700^3 +& \\
\text{m\_aNLCorrect}\,[4]\,*13700^4 +& \\
\text{m\_aNLCorrect}\,[5]\,*13700^5 +& \\
\text{m\_aNLCorrect}\,[6]\,*13700^6 +& \\
\text{m\_aNLCorrect}\,[7]\,*13700^7 = 0.97741&
\end{aligned}
$$

The AD Counts value corrected for linearity and dark becomes 13700/0.97741 = 14017 Counts. The AD Counts value corrected for linearity only (not for dark) becomes 14017+300 = 14317 Counts.

Note that the AvaSpec-2048, -2048L, -2048x14 and -3648 include a "Correct for Dynamic Dark" option (see section 3.2.5). If this correction is applied, the measured dark AD Counts value (without subtracting measured dark counts) is already fluctuating around zero. The polynomial can therefore be applied directly to the measured counts.

The m_aLowNLCounts and m_aHighNLCounts parameters can be used to limit the range for the correction (in counts) for which the polynomial should be applied. The use of polynomials beyond the range of measured data points can give erratic corrections. In AvaSoft, Avantes uses the same correction factor (NCPS) for measured counts (corrected for dark) that are lower than m_aLowNLCounts as is used for m_aLowNLCounts, and for counts higher than m_aHighNLCounts the same NCPS as is used for m_aHighNLCounts. In the example above, NCPS[200] = 0.99203 and all counts <= 200 will be corrected in AvaSoft by dividing through 0.99203. Likewise NCPS[15500] = 0.96099 and all counts >= 15500 will be corrected in AvaSoft by dividing through 0.96099. All counts: 200<counts<15500 will be corrected by the NCPS calculated by the polynomial.

Using the nonlinearity correction polynomial in combination with the 16bit ADC Counts range (see also section 2.3.36, function AVS_UseHighResAdc) does require a small modification in your application software, since the polynomial was recorded in 14bit mode, and therefore should be applied to a 14bit range when calculating the NCPS. This will be illustrated by introducing the variable "ADCFactor" to the equations that are used in the correction (same example as above, same polynomial). The value of "ADCFactor" becomes 0.25 when running in 16bit ADC mode and 1.0 when running in 14bit ADC mode.

In 16bit ADC mode, the measured counts will be a factor 4 higher than in 14bit mode, or with a 14 bit ADC. Therefore, the same pixel of the same spectrometer in this example returns 4*300 = 1200 Counts for darkdata and 4*14000 = 56000 Counts at a certain light intensity. The AD Counts corrected for dark therefore becomes 54800. The Normalized Counts Per Second can be calculated from the polynomial:

NCPS= $\texttt{m\_aNLCorrect}$ [0] +

$\quad\quad$ $\texttt{m\_aNLCorrect}$ [1] * (ADCFactor * 54800) +

$\quad\quad$ $\texttt{m\_aNLCorrect}$ [2] * (ADCFactor * 54800)^2 +

$\quad\quad$ $\texttt{m\_aNLCorrect}$ [3] * (ADCFactor * 54800)^3 +

$\quad\quad$ $\texttt{m\_aNLCorrect}$ [4] * (ADCFactor * 54800)^4 +

$\quad\quad$ $\texttt{m\_aNLCorrect}$ [5] * (ADCFactor * 54800)^5 +

$\quad\quad$ $\texttt{m\_aNLCorrect}$ [6] * (ADCFactor * 54800)^6 +

$\quad\quad$ $\texttt{m\_aNLCorrect}$ [7] * (ADCFactor * 54800)^7 = 0.97741

The AD Counts value corrected for linearity and dark becomes 54800/0.97741 = 56067 Counts. The AD Counts value corrected for linearity only (not for dark) becomes 56067+1200 = 57267 Counts.

Using the m_aLowNLCounts and m_aHighNLCounts parameters in 16bit mode also requires to include the ADCFactor when comparing the measured Counts to these parameters:
m_aLowNLCounts = 200, therefore:
if ADCFactor*(measured counts (corrected for Dark))<200, use NCPS[200] = 0.99203
else if ADCFactor*(measured counts (corrected for Dark))>15500, use NCPS[15500] = 0.96099
else, calculate NCPS as shown above.

In the example above, all counts (corrected for dark) <= 800 will be corrected in AvaSoft by dividing through 0.99203. Likewise, all counts (corrected for dark) >= 62000 will be corrected in AvaSoft by dividing through 0.96099. All counts (corrected for dark): 800<counts<62000 will be corrected by the NCPS calculated by the polynomial.

Gain and Offset
These parameters have been optimized by Avantes, and there should be no need to change these values. The m_Gain and m_Offset parameters are used to optimize the Gain and Offset of the AD Converter. Most detector types use only the m_Gain[0] and m_Offset[0]. The parameters m_Gain[1] and m_Offset[1] are only used by the SENS_SU512LDB detectors (512 pixel NIRs). The m_ExtOffset parameter is used to be able to match the detector output range with the ADC range.
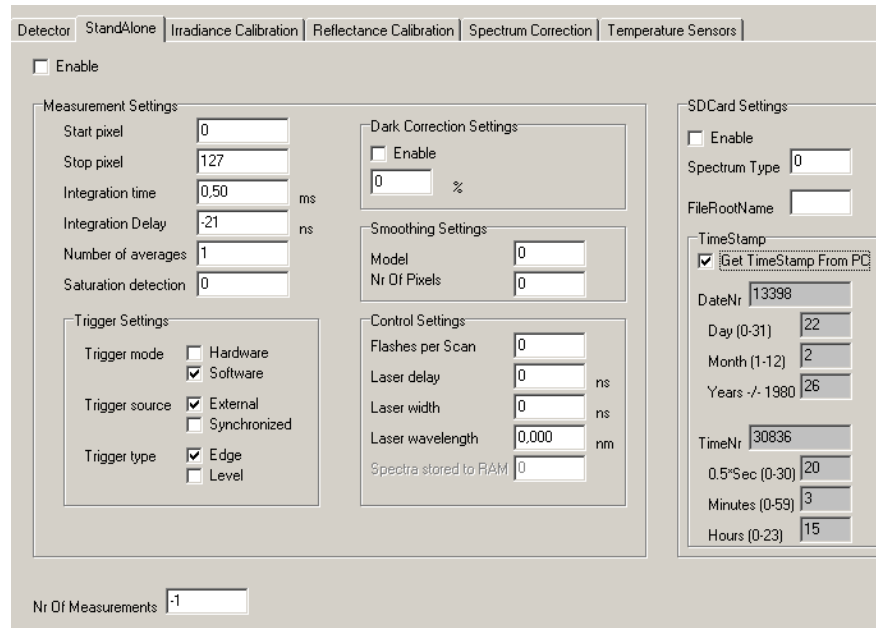
Defective Pixels
The m_DefectivePixels[30] array can be used to store the pixelnumbers that should be eliminated from the data transfer. The as5216x64.dll will calculate the data for a defective pixel by interpolating the data of the neigbor pixels. A defective pixel can be specified in the range from 0 to "NrOfPixels-1", where NrOfPixels specifies the total pixels available for the detectortype used in the spectrometer (see also AVS_GetNumPixels).
The as5216x64.dll evaluates the array $\texttt{m\_DefectivePixels[i]}$ in an increasing order until a pixel is specified which is equal or larger than the number of pixels in the detector.

Jun-12 $\quad\quad\quad\quad\quad\quad\quad\quad\quad\quad\quad\quad$ AS-5216x64-DLL Manual.docx $\quad\quad\quad\quad\quad\quad\quad\quad\quad\quad\quad\quad$ 63

Avantes $\quad\quad\quad\quad\quad\quad\quad\quad\quad$ website: http://www.avantes.com $\quad\quad\quad\quad\quad\quad\quad$ email: Info@avantes.com

3.6.2   EEProm structure: Standalone Parameters

The StandaloneType structure includes a boolean (**m_Enable**) which is not used in the standard version, but which can be used for user specific standalone functionality. The Measurement parameters are also included in this structure, as well as the Number of Measurements parameter (m_Nmsr). Finally, the SDCardType structure has been added, to have storage space available to store dark and reference and scopemode spectra.

The Measurement parameter structure (**MeasConfigType**) has been described in detail in section 3.2, as well as the **Number of Measurements** parameter (m_Nmsr).

The **SDCardType** structure includes the following parameters:

bool   m_Enable
unsigned char   m_SpectrumType
char   m_aFileRootName[6]
TimeStampType   m_TimeStamp

These are the same parameters that have been defined in the function AVS_SaveSpectraToSDCard. The boolean **m_Enable** is not used but has been added for possible future standalone functionality to start saving spectra to the SDCard if m_Enable becomes true;

The **m_SpectrumType** can be set to 0, 1 or 2 to indicate that a dark (*.drk), reference (*.ref) or scope (*.roh) spectrum should be saved. The **m_aFileRootName[6]** parameter is a character string that is used as first part of the name of the stored spectra. A sequence number (00 to 99 if the rootname is six characters long, 000 to 999 if the rootname is five characters long etc…) and the file extension (*.drk), reference (*.ref) or scope (*.roh) completes the filename on SDCard.

The **m_TimeStamp** parameter has been added to be able to add a date/time to the files saved on SDCard.

3.6.3   EEProm structure: Irradiance, Reflectance Calibration and Spectrum Correction

The m_Irradiance, m_Reflectance and m_SpectrumCorrect parameters occupy together over 99% of the defined memory in the EEProm structure (Sizeof(DeviceParamType) with the m_aReserved block excluded). This is because each of these three parameters include an array of 4096 (MAX_NR_PIXELS) float numbers which can hold pixel specific calibration data.

The Irradiance Calibration structure (IrradianceType) has been defined to store the results of an irradiance intensity calibration in EEProm, as well as the settings during this calibration (integration time, smoothing, measurement setup, fiberdiameter). By reading these data from EEProm, it will be possible to convert a spectrum with raw scopedata into an irradiance spectrum.

How to convert ScopeData (A/D Counts) to a power distribution [µWatt/(cm^2.nm)]

In the application software, the smoothpix value in the preparemeasurement structure should be set to the same value as the smoothpix during the intensity calibration. This value can be found in m_Irradiance.m_IntensityCalib.m_Smoothing.m_SmoothPix.

Also, before the irradiance intensity for a pixel i can be calculated, a dark spectrum (= A/D Counts with no light exposed to spectrometer) should be saved (once) at the integration time that will be used in the measurements. The dark spectrum for each pixel i can be called e.g. darkdata(i).

The irradiance intensity at a certain pixel i (i = 0 ..totalpixels-1) can then
be calculated from:

ScopeData(i)   = Measured A/D Counts at pixel i (AVS_GetScopeData)
DarkData(i)   = Dark data at pixel i, saved in application software
IntensityCal(i)   = m_Irradiance.m_IntensityCalib.m_aCalibConvers[i]
CalInttime   = m_Irradiance.m_IntensityCalib.m_CalInttime
CurInttime   = Integration time in measurement (used in the PrepareMeasurement structure)

The equation for irradiance intensity at pixel i then becomes:

Inttimefactor = (CalInttime/CurInttime)
Irradiance Intensity = Inttimefactor* ((ScopeData(i) -DarkData(i))/IntensityCal(i))

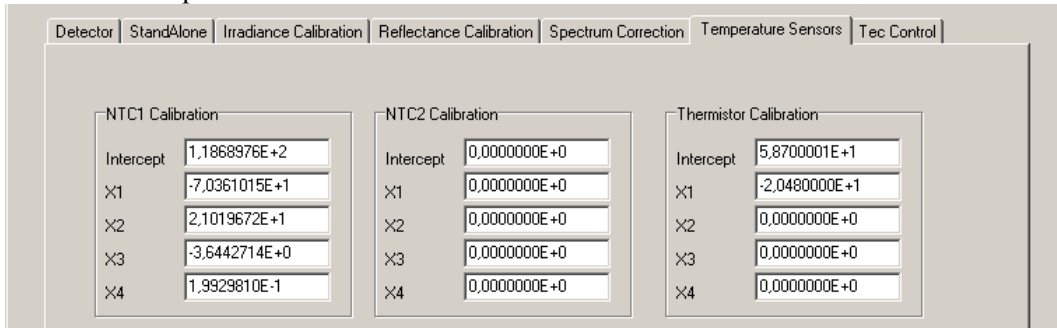**If Scopedata(i) and Darkdata(i) are taken with the 16bit ADC Counts range** (see also section 2.3.36, function AVS_UseHighResAdc), an additional "ADCFactor" needs to be added to the equation above, because the intensity calibration (if performed by Avantes, or by using AvaSoft application software) is always recorded in 14bit mode. The value of "ADCFactor" becomes 0.25 when running in 16bit ADC mode and 1.0 when running in 14bit ADC mode. The equation becomes:
Irradiance Intensity = ADCFactor * Inttimefactor * ((ScopeData(i) -DarkData(i))/IntensityCal(i))

The Reflectance Calibration data can be used to convert the scopedata into a Reflectance or Absorbance spectrum. The Spectrum Correction data can be used to correct the spectral data, e.g. for Pixel Response Non Uniformity (PRNU), or for temperature effects. The Reflectance and Correction arrays are not yet used for calibration purposes by Avantes.

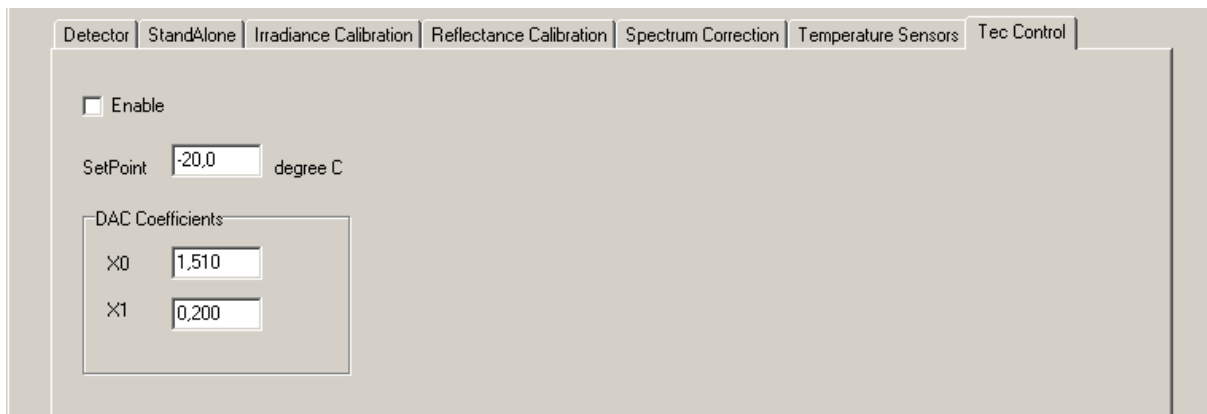### 3.6.4   EEProm structure: Temperature Sensors

The as5216 boards are prepared for using up to three thermistors. NTC1 is mounted on the board, NTC2 is not mounted, and the third thermistor is in the detector. The voltage level of the thermistors can be retrieved by calling the AVS_GetAnalogIn function (see also section 2.3.16 and 3.5).
The structure TempSensorType can hold the coefficients for a polynomial that converts the voltage level into a temperature.

| Detector | StandAlone | Irradiance Calibration | Reflectance Calibration | Spectrum Correction | Temperature Sensors | Tec Control |

NTC1 Calibration		NTC2 Calibration		Thermistor Calibration	
Intercept	1,1868976E+2	Intercept	0,0000000E+0	Intercept	5,8700001E+1
X1	-7,0361015E+1	X1	0,0000000E+0	X1	-2,0480000E+1
X2	2,1019672E+1	X2	0,0000000E+0	X2	0,0000000E+0
X3	-3,6442714E+0	X3	0,0000000E+0	X3	0,0000000E+0
X4	1,9929810E-1	X4	0,0000000E+0	X4	0,0000000E+0

3.6.5   EEProm structure: Tec Control

| Detector | StandAlone | Irradiance Calibration | Reflectance Calibration | Spectrum Correction | Temperature Sensors | Tec Control |

□ Enable

SetPoint   -20,0   degree C

DAC Coefficients

X0   1,510

X1   0,200

The TecControl parameters are used to control the cooling of the detector in the AvaSpec-256-NIR 2.0/2.2/2.5, the AvaSpec-2048TEC-USB2 and AvaSpec-3648TEC-USB2
For these spectrometer types, the m_Enable flag will be set to true.
The default setpoint in degrees Celsius is –20 °C for the AvaSpec-256-NIR (two-stage cooling) and +5°C for the 2048TEC and 3648TEC (one-stage cooling), but it can be changed if needed.

It is not recommended to change the DAC polynomial (m_aFit) which has been optimized for the detector type. For recent models (AvaSpec-ULS2048-TEC and for the ASM5216 boards), the X0 and X1 coefficients in the m_aFit polynomial are 0.0, because the PID control has been entirely implemented in the firmware.

To monitor the detector temperature, use the AVS_GetAnalogIn function, with a_AnalogInId set to 0 (see also section 2.3.16 and 3.5). The polynomial coefficients for converting the measured voltage (U) to degrees Celsius can be found in the table below:

Spectrometer	DetectorType	m_aTemperature[2]. m_aFit[0]	m_aTemperature[2]. m_aFit[1]
AvaSpec-NIR-2.0/2.5TEC	SENS_HAMS9201	58.70	-20.48
AvaSpec-NIR256-1.7/2.2TEC	SENS_SU256LSB	56.60	-18.58
AvaSpec-NIR512-1.7/2.2TEC	SENS_SU512LDB	56.60	-18.58
AvaSpec-2048TEC	SENS_ILX554	51.4	-16.38
AvaSpec-3648TEC	SENS_TCD1304	51.4	-16.38
AvaSpec-HS1024x58	SENS_HAMS11155	82.15	-22.43
AvaSpec-HS1024x122	SENS_HAMS11155	82.15	-22.43

These coefficients are stored in the TempSensorType structure in the eeprom as described in section 3.6.4.

3.6.6   EEProm structure: ProcessControl

The settings in the ProcessControl structure can be used for the 2 analog and 10 digital output signals at the DB26 connector.

The analog settings can be used to store a function output range that should correspond to the 0-5V range of the analog output signals. For example, if the measured function output is expected to be in a range between 1000 and 2000, these values can be stored in the m_AnalogLow[0] and m_AnalogHigh[0] parameters. The function output can then be converted to a 0-5V analog output at pin 17 by using the range stored in eeprom.

The digital output settings can be used as lower- and upper thresholds, to set the corresponding pins to 0 or 5V if these thresholds are exceeded.

The Process Control structure has been successfully used in applications, in which the spectrometer runs completely standalone, without a connection to a PC. Data processing is in that case done onboard by dedicated firmware and the analog and digital outputs are used to signal the function output.