

Sheet1

kalibrace	sigma y (mm)	0.005	
k	y (mm)	delta y (mm)	
	0	15	0
	50	15.07	0.07
	100	15.14	0.14
	150	15.21	0.21
	200	15.28	0.28
	250	15.345	0.345
	300	15.41	0.41
	350	15.48	0.48
	400	15.55	0.55
	450	15.62	0.62
	500	15.69	0.69

$$\text{delta y} = 0.0013779 * k$$

$$p = \lambda / (2 * A)$$

$$\lambda \text{ (nm)} = 546.075$$

$$A \text{ (mm)} = 0.0013779$$

$$p = 0.1981548008$$

$$5.0465595385$$

He-Ne laser			
k	y (mm)	delta y (mm)	
	0	15	0
	50	15.08	0.08
	100	15.17	0.17
	150	15.245	0.245
	200	15.325	0.325
	250	15.41	0.41
	300	15.49	0.49
	350	15.57	0.57
	400	15.65	0.65
	450	15.73	0.73
	500	15.81	0.81

$$\text{delta y} = 0.0016262 * k$$

$$B \text{ (mm)} = 0.0016262$$

$$\lambda \text{ HeNe } 644.47867407$$

$$\lambda \text{ tab } 632.8 \text{ nm}$$

Kalibrace 2			
k	y (mm)	delta y (mm)	
	0	15	0
	50	15.07	0.07
	100	15.14	0.14
	150	15.21	0.21
	200	15.28	0.28
	250	15.35	0.35
	300	15.415	0.415
	350	15.485	0.485
	400	15.55	0.55
	450	15.62	0.62
	500	15.695	0.695

$$C \text{ (mm)} = 0.0013852$$

$$p2 = 0.1971105256$$

$$\text{He-Ne } 2 = 641.08227332$$

Fabry-Perot	sodíkový dublet		
k (splynutí)	y (mm)	delta y (mm)	
	0	3.79	0
	0.5	3.92	0.13
	1	4.06	0.27
	1.5	4.18	0.39
	2	4.36	0.57
	2.5	4.5	0.71
	3	4.65	0.86
	3.5	4.8	1.01
	4	4.94	1.15
	4.5	5.08	1.29
	5	5.2	1.41


$$\lambda \text{ Na } = 589.3$$

$$D \text{ (mm)} = 0.28472$$


$$\text{delta } \lambda = 0.6098526447$$

$$\text{delta tab } 0.6 \text{ nm}$$


Kalibrace

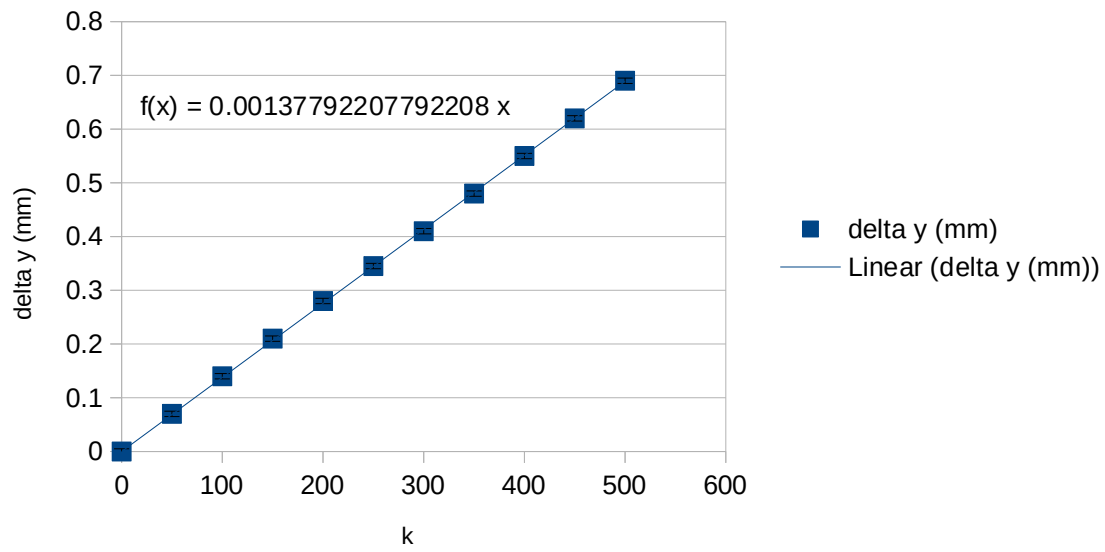

Michelson He-Ne laser

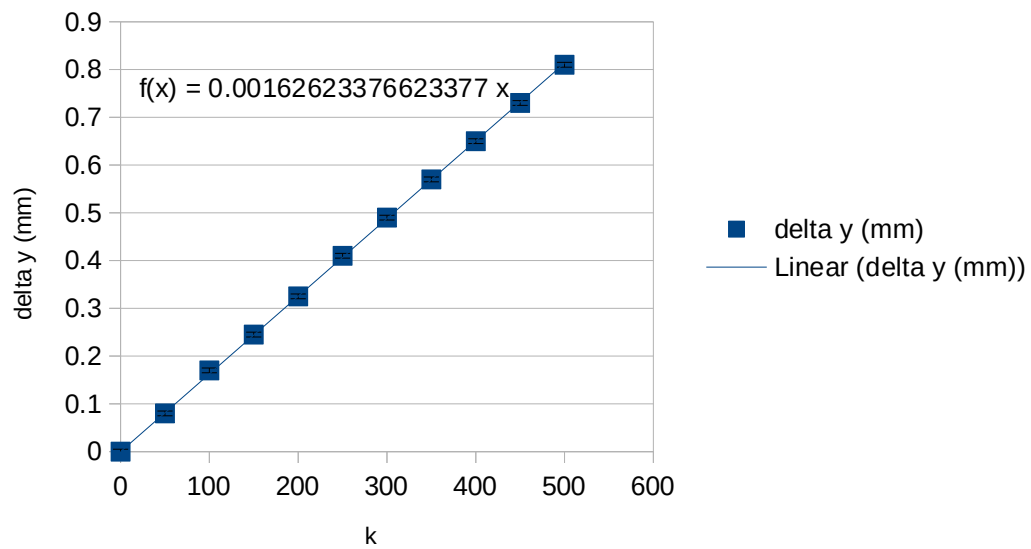

Kalibrace 2

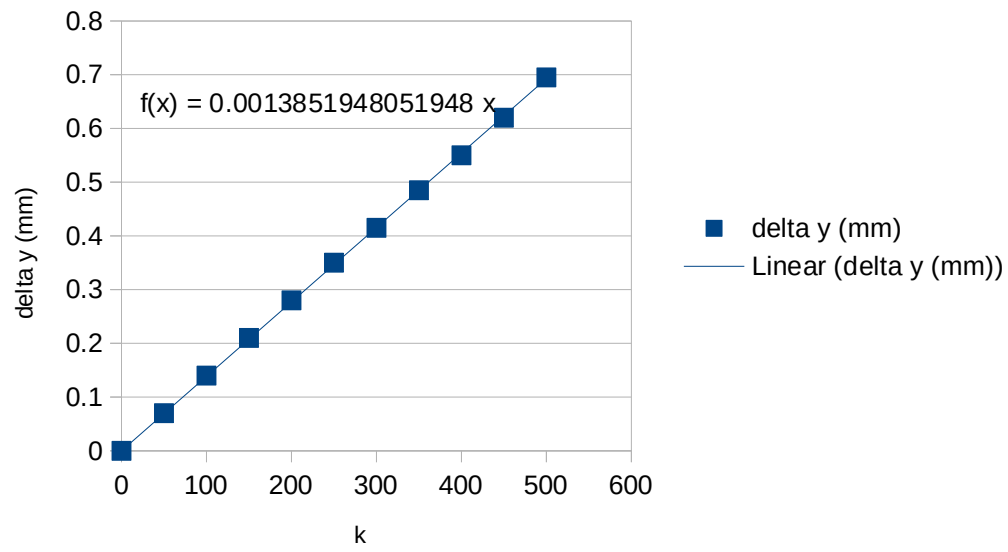

Fabry-Perot Na dublet

