
MODBUS RTU memory Map 2023. 1. 20 (Linetech) / Firmware Ver 7.3					
Slave ID	**BYTE**	**ADDRESS**	**Variable name**	**R/W**	**Description**
1~32	4	40001	Read unit flow -> high	R	**Read unit flow**
		40002	Read unit flow -> low		
	4	40003	Read percent flow -> high	R	**Read Percent flow**
		40004	Read percent flow -> low		
	1	40005	Read flow unit	R	**Read flow unit (SCCM : 0x01 / SLPM : 0x02 ~) / Unit list Refence**
	4	40006	Read Max flowrate ->high	R	**Read Max flowrate**
		40007	Read Max flowrate ->low		
	1	40008	Read MFC mode	R	**Read MFC Mode (MFC : 0x00 /MFM : 0x01)**
	1	40009	Read v & c select	R	**Read Analog Input & Output Signal (Volt : 0x00 / Current : 0x01)**
	1	40010	Select Set-Point Source	R/W	**Analog and digital setting mode(Analog : 0x00 / Digital : 0x01)**
	1	40011	Flow on/off	R/W	**flow control with digital signal (flow off : 0x00 / flow on : 0x01)**
	1	40012	Ingegration Star/stop/Reset	R/W	**Start or stop or Reset integration (integration stop : 0x00 / integration start : 0x01 / integration Reset : 0x02)**
	4	40013	Unit Flow setpoint -> high	R/W	**flow setting command**
		40014	Unit Flow setpoint -> low		
	1	40015	Baud rate Selecttion	R/W	**Baudrate(0x00:9600bps ,0x01:19200bps, 0x02:38400bps, 0x03:57600bps, 0x04:115200bps)**
	4	40016	Data(high byte)/Hour(low byte)	R	**integration : Data(1byte) / Hour(1byte) / Min(1byte) / Sec(1byte)**
		40017	Min(high byte)/Sec(low byte)		
	4	40018	Read integration unit flow -> high	R	**Read integration unit flow**
		40019	Read integration unit flow -> low		
	1	40020	Spare		

read

write

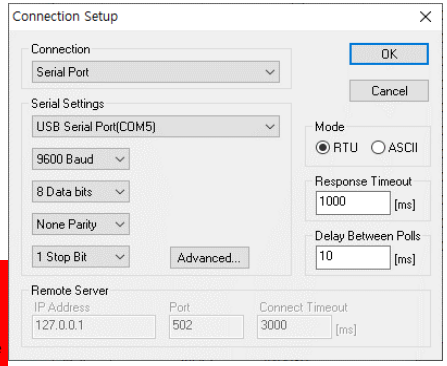

Function Code	Name
03	**Read Holding Registers**
06	**Preset Single Resgisters**
16	**Preset Multiple Resgisters**

Unit list		
No	Units	Abbr.
0	Not yet defined. (default)	
1	Standard Cubic Centimeter per Min	SCCM
2	Standard Liter per Min	SLPM
03~09	Reserved	
10	Liters per second	LPS
11	Liter per minute	LPM
12	Liter per hour	LPH
13	Cubic meter per second	
14	Cubic meter per minute	
15	Cubic meter per hour	
16	Milliliters per second	
17	Milliliters per minute	
18	Milliliters per hour	
19	Reserved	
20	Grams per second	
21	Grams per minute	
22	Grams per hour	
23	Kilograms per second	
24	Kilograms per minute	
25	Kilograms per hour	
26	Pounds per second	
27	Pounds per minute	
28	Pounds per hour	
29~31	Reserved	

Ex) ID2 : 40021~ 40040 / ID3 : 40041~ 40060

Modbuspoll Read/Write Definition

