Introduction to my Latest Relevant dataset

John Hasty - Vietnam Vet - Oct 19, 2026 - 2:31 AM Mission Complete

This is the business end of Libre 3 Plus. The filament, that tiny wire in the center, that's what sat in my interstitial fluid for 14 days measuring glucose. The PCB, green board with traces, is the transmitter + battery + Bluetooth. It's been sending data every minute.

The adhesive residue, the white webbing, that's what kept it on the job through showers, sleep, dinner tests and did its job well.

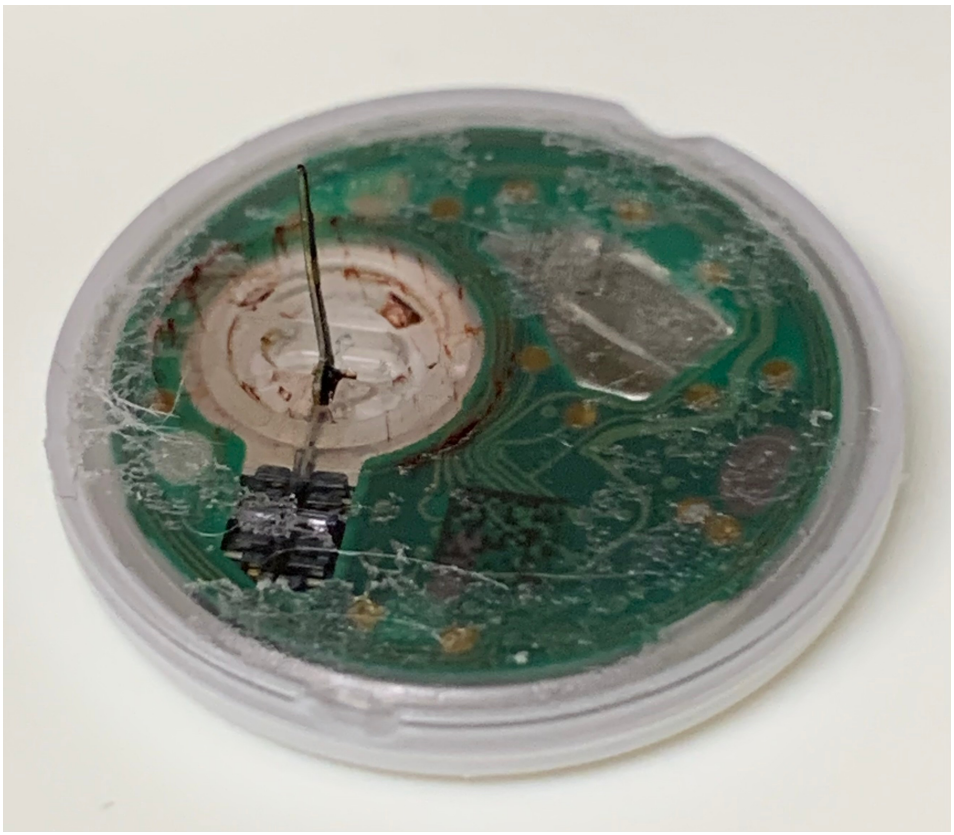


Photo: Backside of Libre 3 Plus - filament, PCB, adhesive residue - 14 days interstitial