


=====

Acq. Operator	: EDSON	Seq. Line	: 11
Acq. Instrument	: Instrument 1	Location	: Vial 11
Injection Date	: 4/25/2025 12:58:02 PM	Inj	: 1
		Inj Volume	: 10.0 µl
Acq. Method	: C:\CHEM32\1\DATA\TESTE B6-290 2025-04-23 12-55-35\B6 TESTE 290.M		
Last changed	: 4/23/2025 8:27:30 AM by EDSON		
Analysis Method	: C:\CHEM32\1\METHODS\B6.M		
Last changed	: 4/25/2025 9:51:12 AM by EDSON		

=====

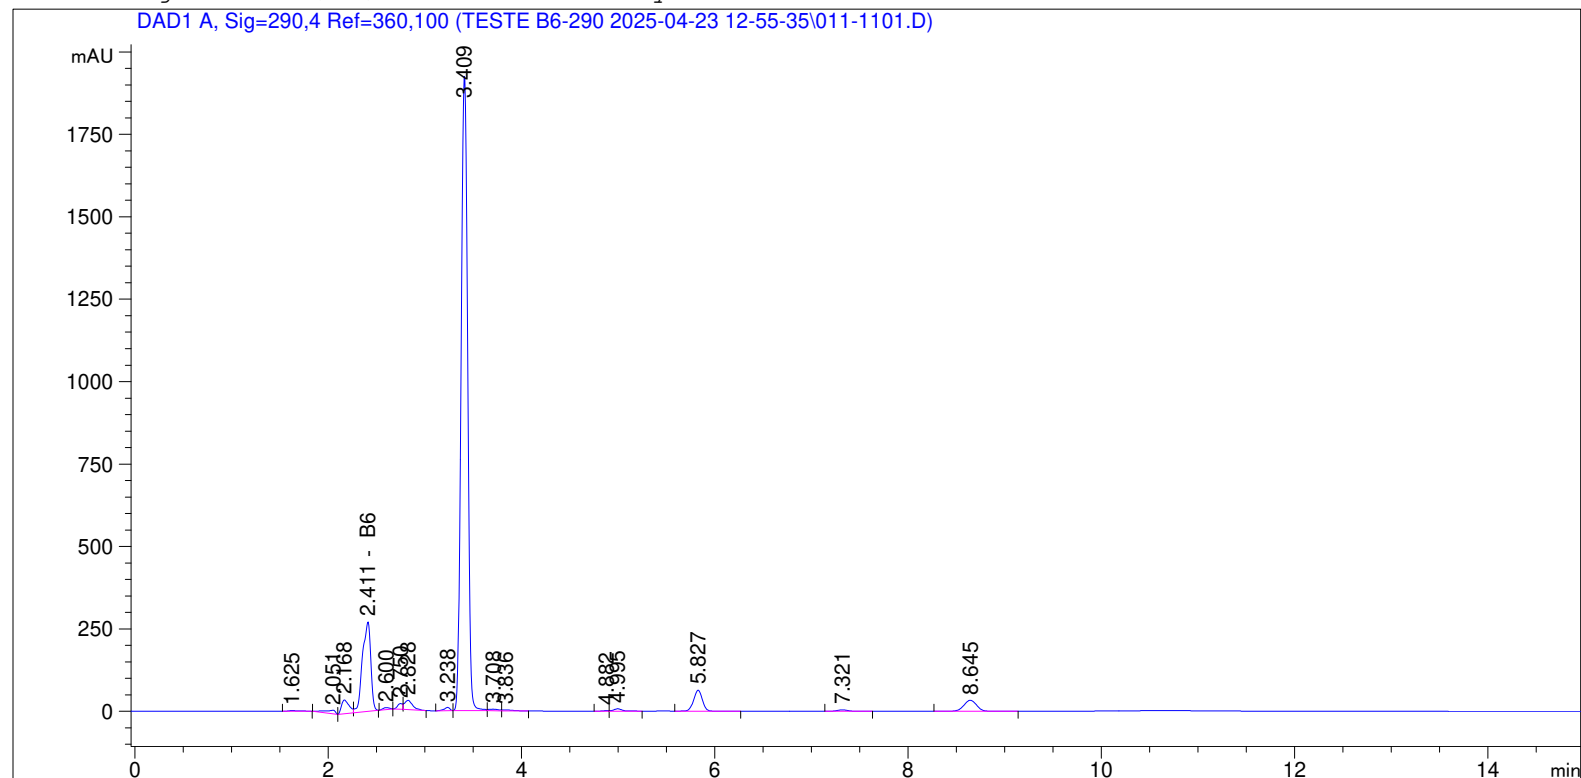

=====

External Standard Report

=====

Sorted By : Signal
Calib. Data Modified : Thursday, April 24, 2025 6:00:25 PM
Multiplier: : 1.0000
Dilution: : 1.0000
Use Multiplier & Dilution Factor with ISTDs

Signal 1: DAD1 A, Sig=290,4 Ref=360,100

RetTime [min]	Type	Area [mAU*s]	Amt/Area	Amount [ug/ml]	Grp	Name
2.411	VB	1593.10315	3.95797e-2	63.05461	B6	

Totals : 63.05461

=====

*** End of Report ***