


```
=====
Acq. Operator   : EDSON                      Seq. Line :   10
Acq. Instrument : Instrument 1                Location  : Vial 10
Injection Date  : 4/25/2025 12:41:38 PM      Inj       :    1
                                           Inj Volume: 10.0 µl

Acq. Method     : C:\CHEM32\1\DATA\TESTE B6-290 2025-04-23 12-55-35\B6 TESTE 290.M
Last changed    : 4/23/2025 8:27:30 AM by EDSON
Analysis Method : C:\CHEM32\1\METHODS\B6.M
Last changed    : 4/25/2025 9:51:12 AM by EDSON
=====
```

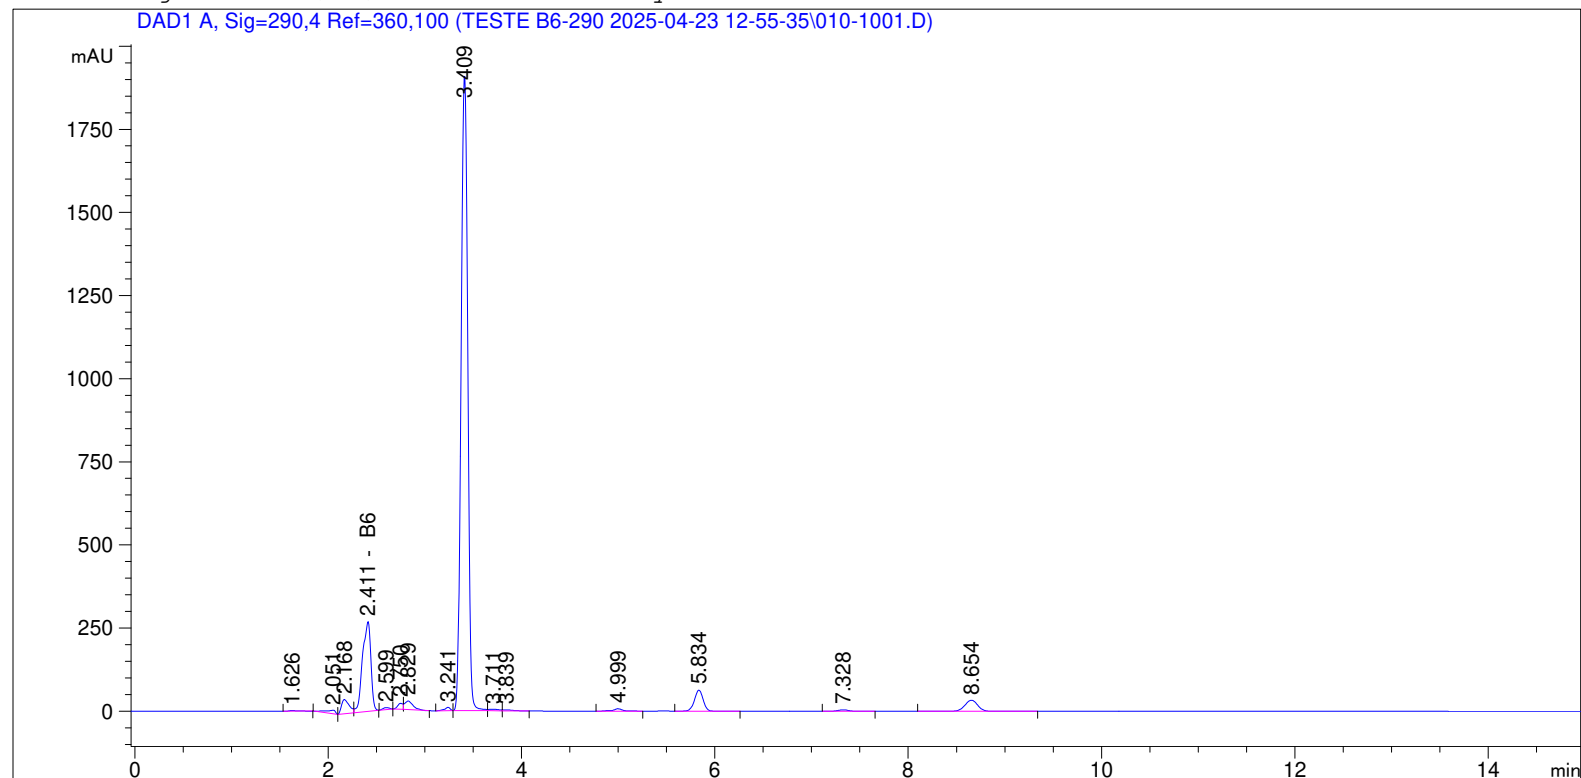

```
=====
                        External Standard Report
=====
```

```
Sorted By           :      Signal
Calib. Data Modified :      Thursday, April 24, 2025 6:00:25 PM
Multiplier:         :      1.0000
Dilution:           :      1.0000
Use Multiplier & Dilution Factor with ISTDs
```

Signal 1: DAD1 A, Sig=290,4 Ref=360,100

RetTime [min]	Type	Area [mAU*s]	Amt/Area	Amount [ug/ml]	Grp	Name
2.411	VB	1591.66736	3.95794e-2	62.99726	B6	

Totals : 62.99726

```
=====
*** End of Report ***
```