


Analysis Report

<Sample Information>

Sample Name	: Amostra_4		
Sample ID	: 010		
Data Filename	: Cafeina_MEOH_H2O_29042025_010.lcd		
Method Filename	: Cafeina_28042025.lcm		
Batch Filename	: Cafeina_MEOH_H2O.lcb		
Vial #	: 1-10	Sample Type	: Unknown
Injection Volume	: 10 uL		
Date Acquired	: 29/04/2025 15:48:44	Acquired by	: System Administrator
Date Processed	: 30/04/2025 10:40:59	Processed by	: System Administrator

<Chromatogram>

mV

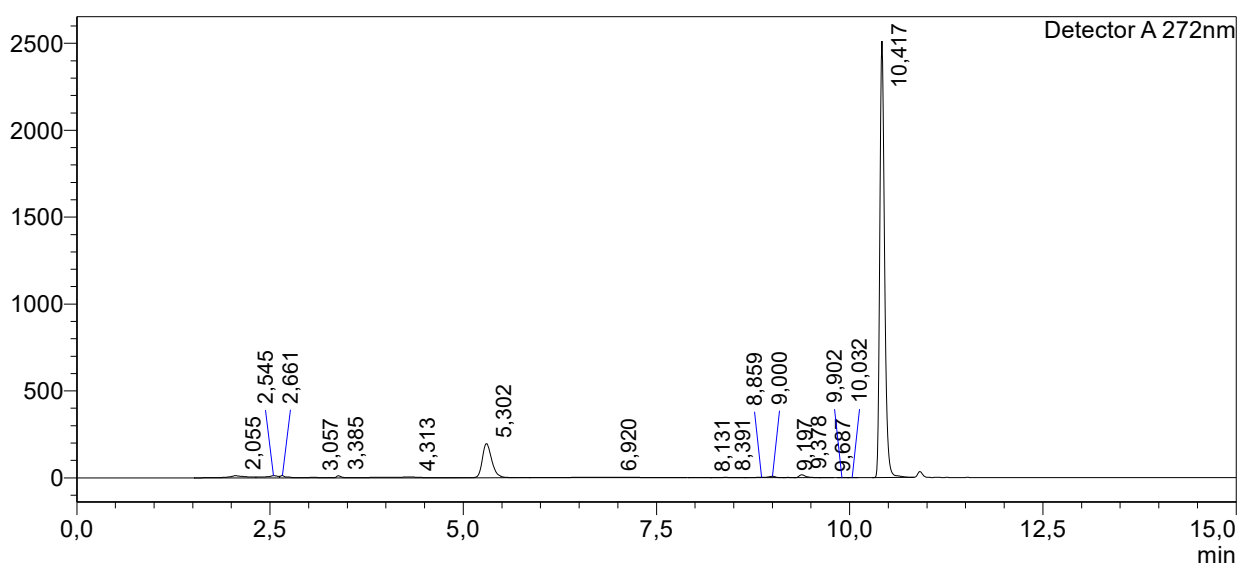

<Peak Table>

Detector A 272nm

Peak#	Ret. Time	Area	Height	Conc.	Unit	Mark	Name
1	2,055	196336	12104	0,000			
2	2,545	139571	11716	0,000		V	
3	2,661	78231	13179	0,000		V	
4	3,057	30677	3509	0,000		V	
5	3,385	53649	11880	0,000		V	
6	4,313	163774	4127	0,000		V	
7	5,302	1704735	197094	0,000		V	
8	6,920	182023	2590	0,000		V	
9	8,131	2883	376	0,000			
10	8,391	19086	2545	0,000		V	
11	8,859	16800	2046	0,000		V	
12	9,000	54694	8367	0,000		V	
13	9,197	7171	1558	0,000		V	
14	9,378	105957	16641	0,000		V	
15	9,687	4607	555	0,000		V	
16	9,902	2394	510	0,000		V	
17	10,032	1006	266	0,000		V	
18	10,417	10885303	2511825	0,382	mg/L		Cafeina
Total		13648896	2800889				