


Analysis Report

<Sample Information>

Sample Name	: Amostra_2	Sample Type	: Unknown
Sample ID	: 008		
Data Filename	: Cafeina_MEOH_H2O_29042025_008.lcd		
Method Filename	: Cafeina_28042025.lcm		
Batch Filename	: Cafeina_MEOH_H2O.lcb		
Vial #	: 1-8		
Injection Volume	: 10 uL		
Date Acquired	: 29/04/2025 15:17:46	Acquired by	: System Administrator
Date Processed	: 30/04/2025 10:35:36	Processed by	: System Administrator

<Chromatogram>

mV

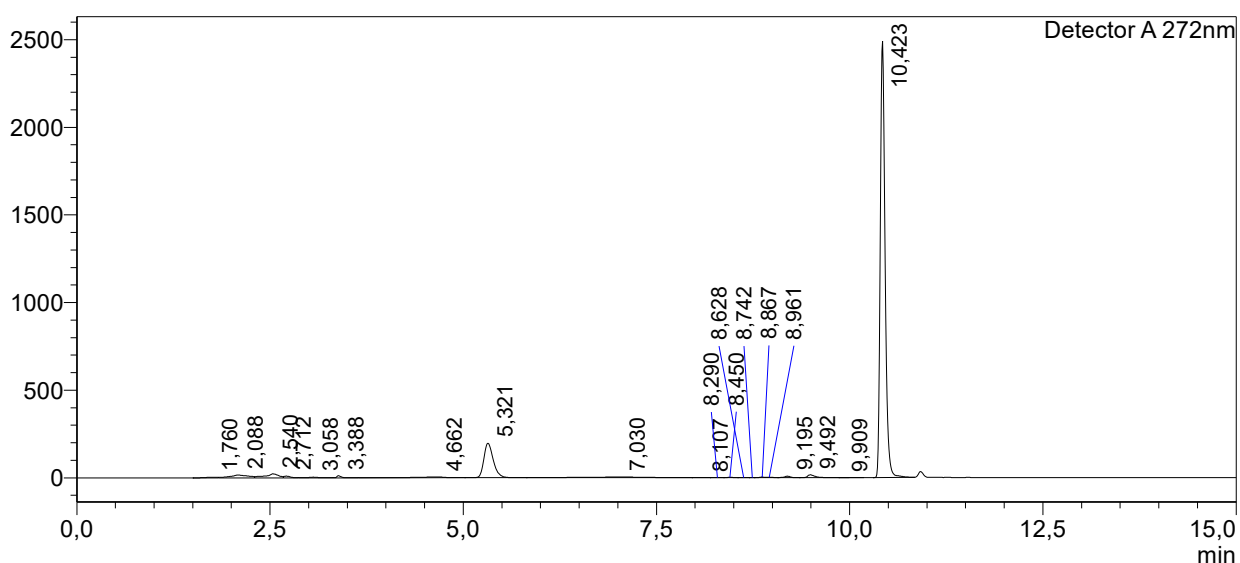

<Peak Table>

Detector A 272nm

Peak#	Ret. Time	Area	Height	Conc.	Unit	Mark	Name
1	1,760	37108	3581	0,000			
2	2,088	260215	16033	0,000		V	
3	2,540	274639	22405	0,000		V	
4	2,712	53124	9632	0,000		V	
5	3,058	41306	3871	0,000		V	
6	3,388	46585	11133	0,000		V	
7	4,662	133945	4562	0,000		V	
8	5,321	1681334	197117	0,000		V	
9	7,030	239186	3725	0,000		V	
10	8,107	2687	350	0,000		V	
11	8,290	3225	458	0,000		V	
12	8,450	12501	2734	0,000		V	
13	8,628	3326	604	0,000		V	
14	8,742	1001	267	0,000		V	
15	8,867	14314	3302	0,000		V	
16	8,961	12678	2270	0,000		V	
17	9,195	48284	8541	0,000		V	
18	9,492	112560	16160	0,000		SV	
19	9,909	1152	338	0,000		T	
20	10,423	10882265	2490554	0,381	mg/L		Cafeina
Total		13861436	2797638				