


Analysis Report

<Sample Information>

Sample Name	: Amostra_1		
Sample ID	: 007		
Data Filename	: Cafeina_MEOH_H2O_29042025_007.lcd		
Method Filename	: Cafeina_28042025.lcm		
Batch Filename	: Cafeina_MEOH_H2O.lcb		
Vial #	: 1-7	Sample Type	: Unknown
Injection Volume	: 10 uL		
Date Acquired	: 29/04/2025 15:02:18	Acquired by	: System Administrator
Date Processed	: 30/04/2025 10:35:30	Processed by	: System Administrator

<Chromatogram>

mV

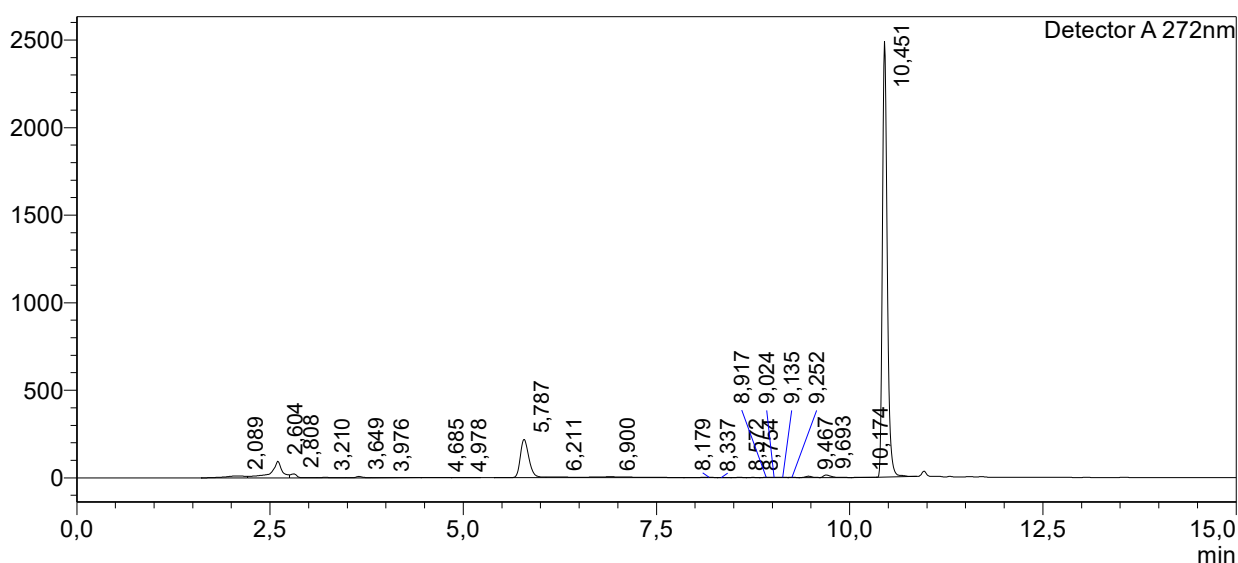

<Peak Table>

Detector A 272nm

Peak#	Ret. Time	Area	Height	Conc.	Unit	Mark	Name
1	2,089	193449	10743	0,000			
2	2,604	927200	93575	0,000		V	
3	2,808	130887	22408	0,000		V	
4	3,210	24052	3105	0,000		V	
5	3,649	48079	7407	0,000		V	
6	3,976	27014	1245	0,000		V	
7	4,685	5069	271	0,000		V	
8	4,978	3090	238	0,000		V	
9	5,787	1713952	219000	0,000			
10	6,211	80447	4095	0,000		V	
11	6,900	230311	5075	0,000		V	
12	8,179	23967	2151	0,000		V	
13	8,337	3323	602	0,000		V	
14	8,572	10635	2659	0,000			
15	8,754	5936	1036	0,000		V	
16	8,917	11115	2676	0,000		V	
17	9,024	9993	1904	0,000		V	
18	9,135	4847	880	0,000		V	
19	9,252	7643	1697	0,000		V	
20	9,467	44577	7939	0,000		V	
21	9,693	101515	14606	0,000		V	
22	10,174	6811	749	0,000			

Peak#	Ret. Time	Area	Height	Conc.	Unit	Mark	Name
23	10,451	10891578	2490623	0,382	mg/L		Cafeina
Total		14505489	2894683				