# **SPECTRO** Series

# SPECTRO-1-20-UVC-DIL

- Measuring range typ. 10 mm ... 40 mm
- Reflection-based measurement method
- UVC LED and UV filter (AC-/DC-operation or OFF for luminous objects can be switched) High scan frequency
- Gray scale detection (12-bit resolution)
- Insensitive to outside light (in AC-operation)
- Brightness correction can be activated (STAT/DYN)
- Averaging can be activated (from 1 up to over 32000 values)
- TEACH via PC or PLC
- Switching state indication by means of 2 yellow LEDs
- RS232 interface (USB or ETHERNET converter available)
- Parameterizable via Windows® software, scope function
- Temperature compensated (from 0°C to 60°C)
- Automatic threshold correction can be activated
- Switching threshold can be parameterized relative or absolute
- 2 digital inputs (0V/+Ub)
- 2 digital outputs (max. 60 kHz switching frequency)
- 1 analog output (0V...+10V or 4...20mA), selectable via software
- Various switching threshold functions (window, upper/lower threshold)
- Integrated cooling device for protection against overheating of the sensor





# Design

SPECTRO-1-20-UVC-DIL-OFL


Accessories: (p. 8)

(Spacer/offline unit)

# **Product name:**

### SPECTRO-1-20-UVC-DIL (incl. Windows® PC software SPECTRO1-Scope)

The transmitter is located in the UVC range (265 nm), the detection range is also in the UV range (typically 230 nm to 400 nm).

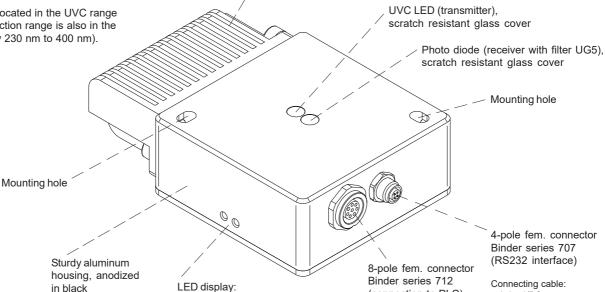

Cooling device

Binder series 707 (RS232 interface)

(connection to PLC)

Connecting cable:

cab-las8/SPS

Connecting cable: cab-las4/PC or cab-4/USB or cab-4/FTH



Switching state indication

by means of 2 yellow LEDs

in black






# **Technical Data**


Model	SPECTRO-1-20-UVC-DIL	
Voltage supply	+24VDC (± 10%), reverse polarity protected, overcurrent protected	
Current consumption	< 220 mA	
Max. switching current	100 mA, short circuit proof	
Switching state indication	2 yellow LED visualize the physical state of the outputs OUT0 and OUT1	
Digital inputs (2x)	IN0 and IN1 (Pin 3 and 4): digital (0V/+24V)	
Digital outputs (2x)	OUT0 and OUT1 (Pin 5 and 6): digital (0V/+24V), npn-/pnp-able (bright-/dark-switching, can be switched)	
Analog output (1x)	ANALOG (Pin 8): voltage 0 +10V or current 4 20mA, adjustable via PC software	
Interface	RS232	
Pulse lengthening	0 100 ms, adjustable via PC software	
Averaging	max. 32768 values, adjustable via PC software	
Scan frequency (LED mode AC, DC or OFF, can be switched via PC software)	LED mode AC (depends on parameterization): Frequency [Hz] Digital outputs Analog output Max. 50 000 Off Off Max. 48 000 On Off Max. 42 000 Off On Max. 41 000 On On Measurements were made with the smallest gain at the receiver (AMP1). At the highest gain (AMP8), rthe frequency is reduced by a factor of 10.	LED mode DC / OFF (depends on parameterization): Frequency [Hz] Digital outputs Analog output Max. 175 000 Off Off Max. 135 000 On Off Max. 100 000 Off On Max. 85 000 On On The frequency is independent of the gain set at the receiver.
Switching frequency	max. 60 kHz	
Analog band width	max. 90 kHz (-3 dB)	
Transmitter (light source)	UVC LED, 265 nm	
Transmitter control	can be switched via PC software: AC operation (LED MODE-AC), DC operation (LED MODE-DC), OFF operation (LED MODE-OFF)	
Measuring range	typ. 10 mm 40 mm	
Receiver	photo diode incl. short pass filter UG5	
Receiver gain setting	8 steps (AMP1 AMP8), adjustable via PC software	
Ambient light	max. 5000 Lux	
Detection range (half intensity width)	typ. 10 mm at a distance of 15 mm typ. 20 mm at a distance of 40 mm	
Reproducibility	2 digits at 12-bit A/D conversion	
Housing dimensions	LxWxH approx. 95 mm x 65 mm x 28 mm (without connectors)	
Housing material	aluminum, anodized in black (optics holding device: aluminum, anodized)	
Enclosure rating	IP67 (optics), IP64 (electronics)	
Connecting cables	to PLC: cab-las8/SPS or cab-las8/SPS-w to PC/RS232 interface: cab-las4/PC or cab-las4/PC-w to PC/USB interface: cab-4/USB or cab-4/USB-w to PC/Ethernet interface: cab-4/ETH	
Type of connector	connection to PLC: 8-pole fem. connector (Binder 712) connection to PC: 4-pole fem. connector (Binder 707)	
Operating temp. range	-20°C +55°C	
Storage temperature range	-20°C +85°C	
EMC test acc. to	DIN EN 60947-5-2 <b>( €</b>	





# **Dimensions**

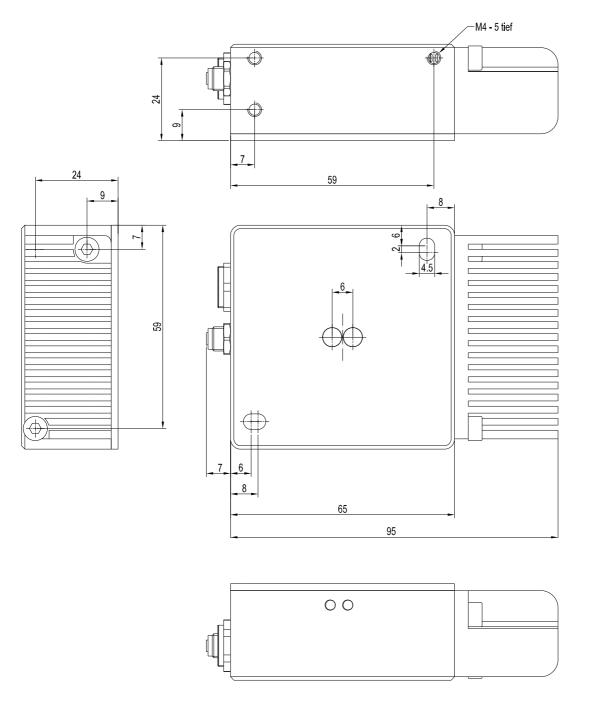



All dimensions in mm





# **Connector Assignment**

#### Connection to PLC:

### 8-pole fem. connector Binder series 712

Pin: Assignment: Color: white GND (0V) +24VDC (±10%) 2 brown 3 green IN0 (Digital 0: 0 ... 1V, Digital 1: +Ub - 10%) IN1 (Digital 0: 0 ... 1V, Digital 1: +Ub - 10%) yellow 4

grey 5 OUT0 (Digital 0: Type 0 ... 1V, Digital 1: Type +Ub - 10%) 6 OUT1 (Digital 0: Type 0 ... 1V, Digital 1: Type +Ub - 10%) pink

blue not connected

ANALOG (voltage 0...+10V or current 4...20mA) red

Connecting cable: cab-las8/SPS-(length) cab-las8/SPS-w-(length) (standard length 2m)

## **Connection to PC:** 4-pole fem. connector Binder Series 707

Assignment:

+24VDC (+Ub, OUT)

2 GND (0V) 3 RxD TxD

#### Connection via RS232 interface at the PC:

Connecting cable: cab-las4/PC-(length) cab-las4/PC-w-(length) (angle type 90°) (standard length 2m)

#### alternative:

#### Connection via USB interface at the PC:


USB converter (incl. driver software): cab-4/USB-(length) cab-4/USB-w-(length) (angle type 90°) (standard length 2m)

## alternative:

#### Connection to local network via Ethernet bus:

Ethernet converter (incl. software "SensorFinder"): cab-4/ETH-500 (standard length 0.5m)


Optional: External CAT5 cable. e.g. cab-eth/M12D-RJ45-flx-(length)



for connection of an external CAT5 cable, e.g. cab-eth/M12D-RJ45-flx-(length) cab-las8/SPS-...


(max. length 25m, outer jacket: PUR)

cab-las8/SPS-w-... (max. length 25m, outer jacket: PUR)

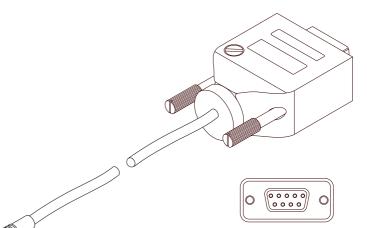


cab-las4/PC-... (max. length 10m, outer jacket: PUR) or cab-las4/PC-w-... (no picture)

(max. length 5m, outer jacket: PUR)



cab-4/USB-... or cab-4/USB-w-... (no picture) (each max. length 5m, outer jacket: PUR)



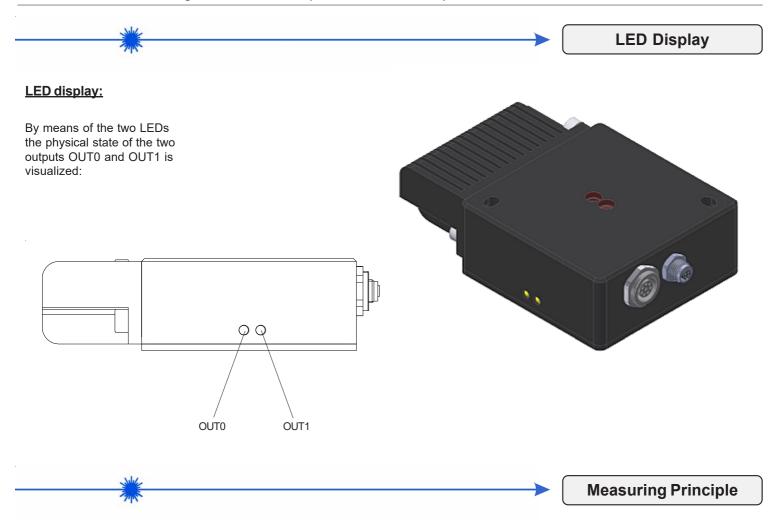

#### Measuring principle of the sensors of SPECTRO-1 series:

The sensors of the SPECTRO-1 series are of single-channel design, i.e. they acquire the analog signal that comes from a receiver and evaluate this signal. Various light sources such as white light, UV light, IR light, or a laser can be used as a transmitter. The receiver is correspondingly matched to the transmitter. The acquired analog signal is provided through a voltage output and a current output.

The software can be used to select various evaluation modes for the analog signal. The status of the analog signal is provided through 2 digital outputs in accordance with the selected evaluation mode. A digital input allows external "teaching" of the sensor. An additional input allows the "freezing" of the analog output signal upon a positive input edge.

The SPECTRO-1 sensor allows highly flexible signal acquisition. The sensor, for example, can be operated in alternating-light mode (AC mode), which means the sensor is not influenced by external light, or in constant-light mode (DC mode), which provides outstanding high-speed sensor operation. An OFF function deactivates the sensor's integrated light source and changes to DC mode, which allows the sensor to detect so-called "self-luminous objects". With the stepless adjustment of the integrated light source, the selectable gain of the receiver signal, and an INTEGRAL function the sensor can be adjusted to almost any surface or any "self-luminous object".

A micro-controller performs 12-bit analog/digital conversion of the analog signal, which allows recording and evaluation of the signal. Furthermore the SPECTRO-1 sensor offers various options for intelligent signal processing such as e.g. dirt accumulation compensation.

Parameters and measurement values can be exchanged between PC and sensor either through RS232 or Ethernet (using an Ethernet converter). Through the interface all the parameters can be stored in the non-volatile EEPROM of the sensor.

The PC software facilitates the parameterisation, diagnostics, and adjustment of the sensor system (oscilloscope function). The software furthermore provides a data recorder function that automatically records data and stores them on the hard disk of the PC.

SPECTRO-1 sensors are temperature-compensated over a range of 0°C to 80°C.






### **Parameterization**

#### Windows® user interface:

(The current software version is available for download on our website.)

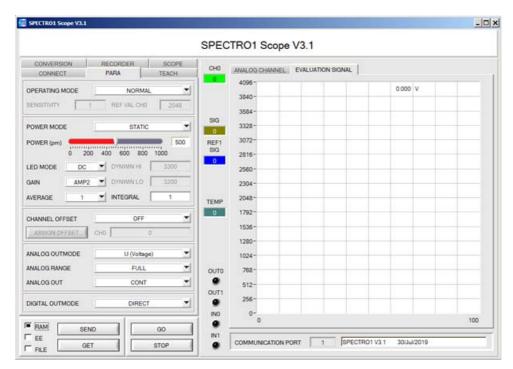

The PC software SPECTRO1-Scope facilitates the parameterization, the diagnosis, and the adjustment of the sensor system (oscilloscope function). Moreover, the software features a data recorder function that allows the automatic recording of recorded data and the saving of those at the hard disk of the PC.

Parameters and measurement values can be exchanged between PC and sensor either through RS232 or Ethernet (using an Ethernet converter). Through the interface all the parameters can be stored in the non-volatile EEPROM of the sensor.




The SCOPE tab visualises an oscilloscope.



## **Firmware Update**

### Firmware update by means of the software "FirmwareLoader":

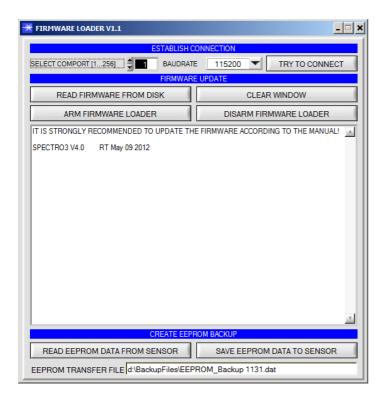


The software "Firmware Loader" allows the user to perform an automatic firmware update. The update will be carried out through the RS232 interface.


An initialisation file (xxx.ini) and a firmware file (xxx.elf.S) are required for performing a firmware update. These files can be obtained from your supplier. In some cases an additional firmware file for the program memory (xxx.elf.p.S) is also needed, and this file will be automatically provided together with the other two files






**Spacer** 







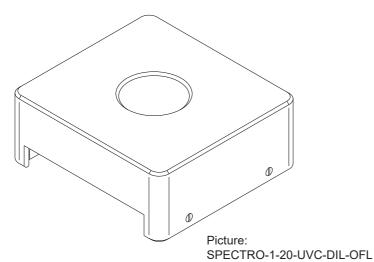






Picture: SPECTRO-1-20-UVC-DIL with SPECTRO-1-20-UVC-DIL-OFL



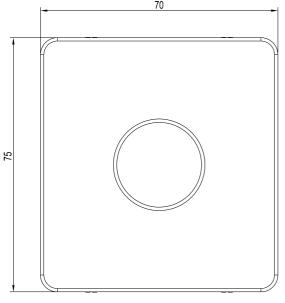



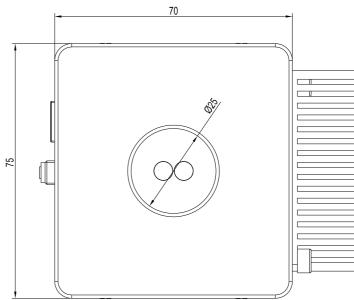

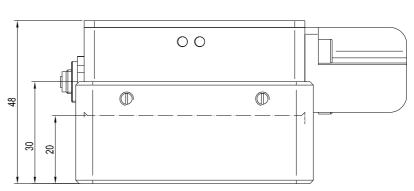

Alle Abmessungen in mm

